

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031431.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 19:17
 Operator : DD\AJ
 Sample : L4820-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TT-023-IDWGW-20201118

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 00:58:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.793	4.068	902232	873610	22.147	20.896
2)	SA Decachlor...	10.666	9.374	456265	522473	14.855	15.603
Target Compounds							
8)	L2 AR-1221-1	5.032	0.000	113015	0	240.736	N.D. #
9)	L2 AR-1221-2	0.000	4.421	0	11315	N.D.	32.042 #
31)	L7 AR-1260-1	0.000	6.950f	0	2912	N.D.	1.743 #
32)	L7 AR-1260-2	0.000	7.144f	0	3928	N.D.	1.930 #
35)	L7 AR-1260-5	0.000	7.997	0	5758	N.D.	1.457 #
37)	L8 AR-1262-2	0.000	7.997	0	5758	N.D.	1.400 #
38)	L8 AR-1262-3	0.000	8.275	0	42465	N.D.	26.643 #
41)	L9 AR-1268-1	0.000	8.275	0	42465	N.D.	8.628 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031431.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 19:17
Operator : DD\AJ
Sample : L4820-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TT-023-IDWGW-20201118

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 00:58:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

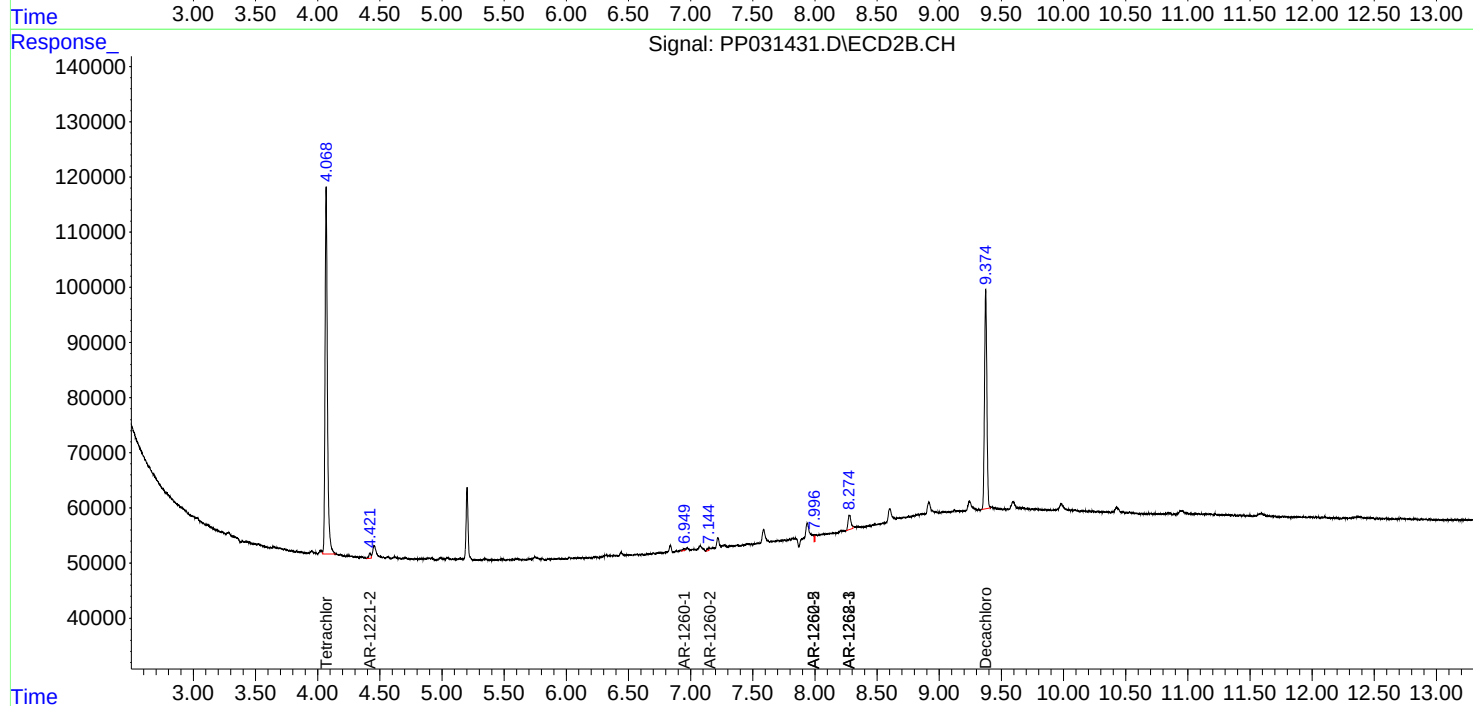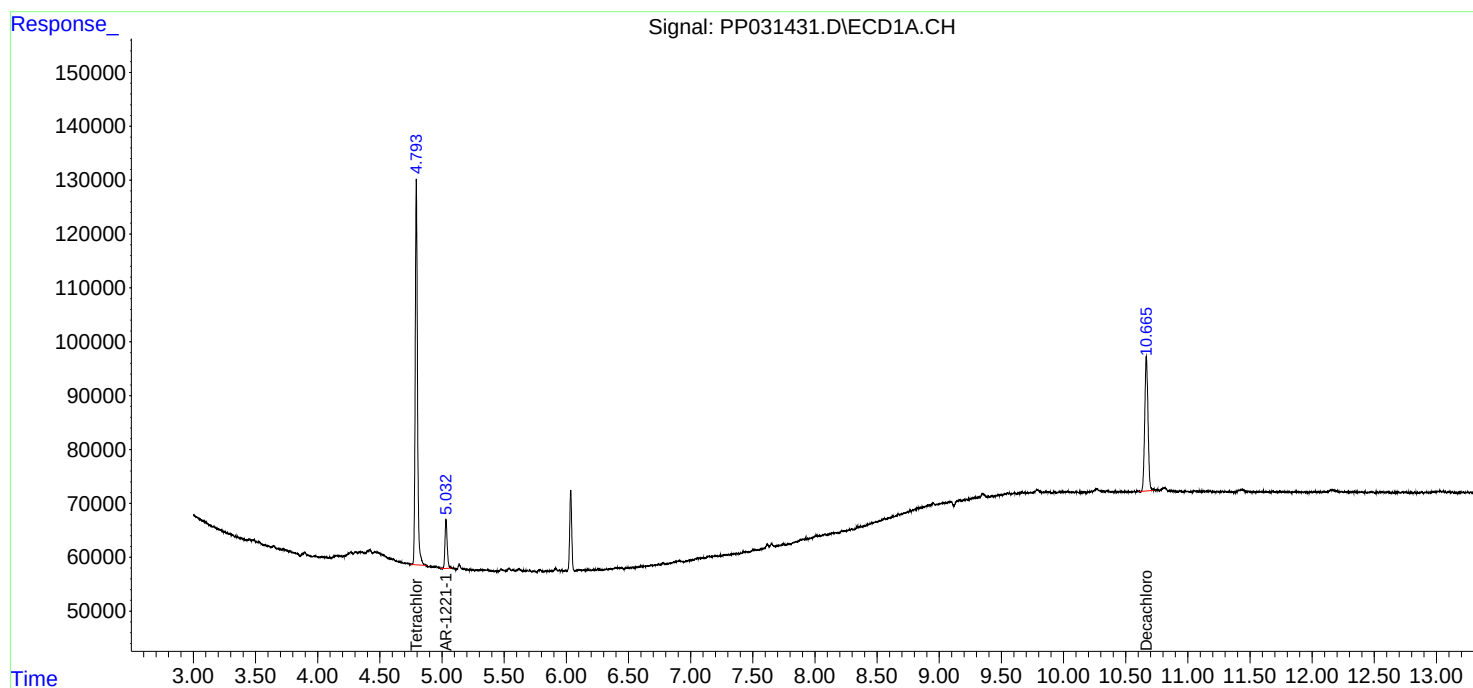


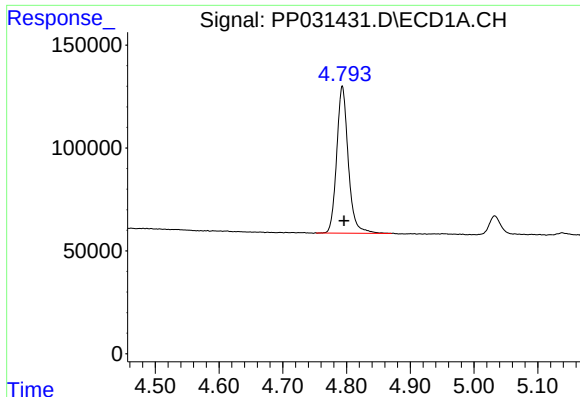

#1 Tetrachloro-m-xylene


R.T.: 4.793 min
Delta R.T.: -0.003 min
Response: 902232
Conc: 22.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-023-IDWGW-20201118

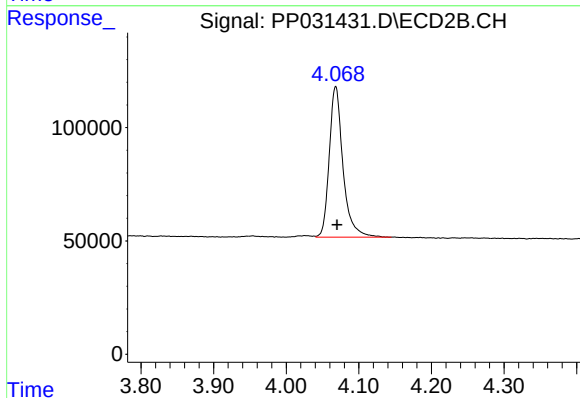


#1 Tetrachloro-m-xylene

R.T.: 4.068 min
Delta R.T.: -0.002 min
Response: 873610
Conc: 20.90 ng/ml

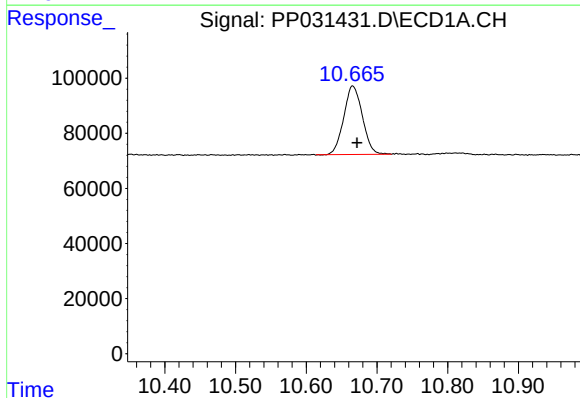


#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.006 min
Response: 456265
Conc: 14.86 ng/ml

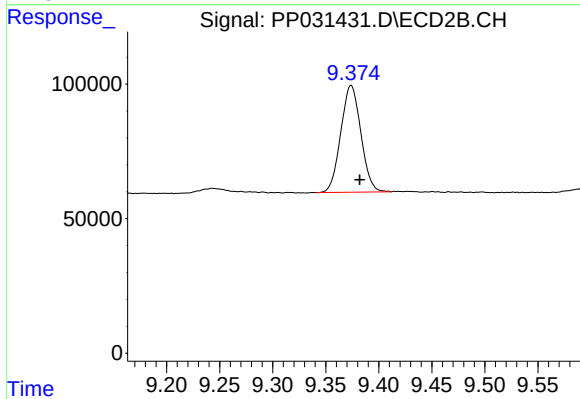

#2 Decachlorobiphenyl


R.T.: 9.374 min
Delta R.T.: -0.008 min
Response: 522473
Conc: 15.60 ng/ml

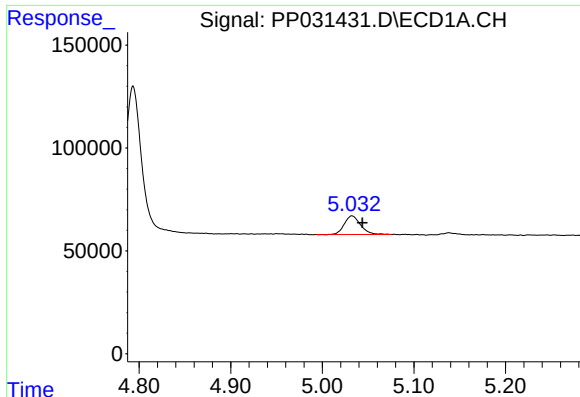

#8 AR-1221-1


R.T.: 5.032 min
Delta R.T.: -0.011 min
Response: 113015
Conc: 240.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-023-IDWGW-20201118

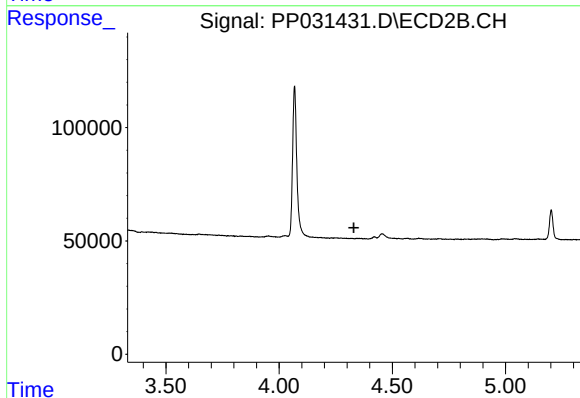


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.330 min
Response: 0
Conc: N.D.

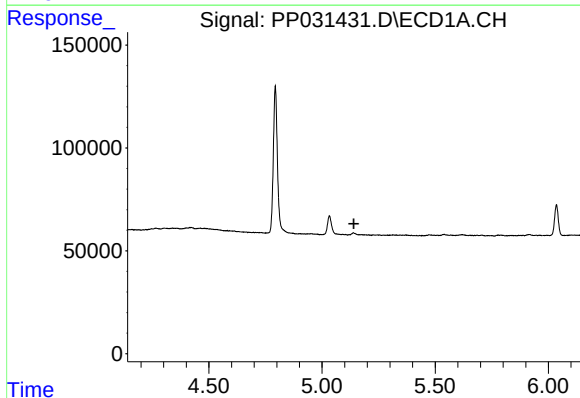


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.141 min
Response: 0
Conc: N.D.

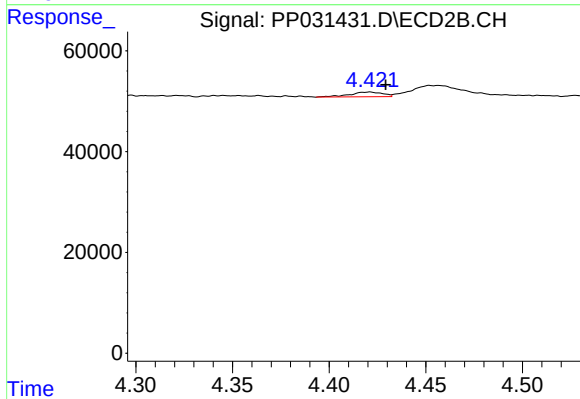

#9 AR-1221-2


R.T.: 4.421 min
Delta R.T.: -0.008 min
Response: 11315
Conc: 32.04 ng/ml

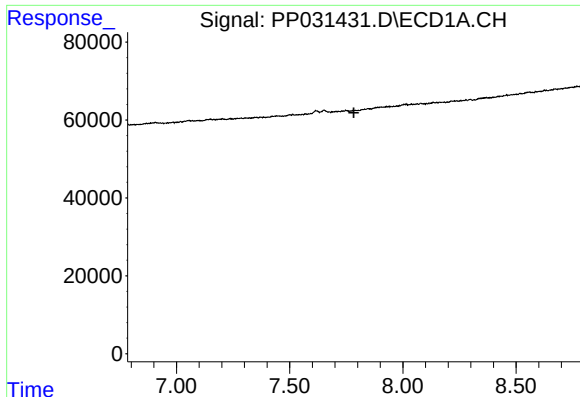

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.783 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TT-023-IDW/GW-20201118

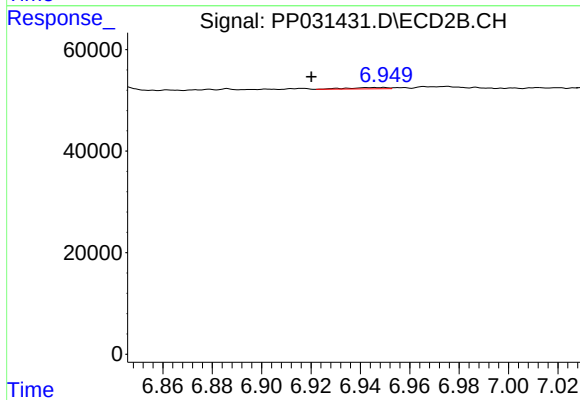


#31 AR-1260-1

R.T.: 6.950 min
Delta R.T.: 0.030 min
Response: 2912
Conc: 1.74 ng/ml

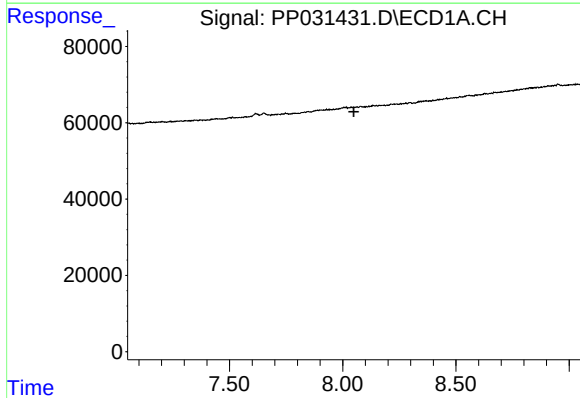


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.049 min
Response: 0
Conc: N.D.

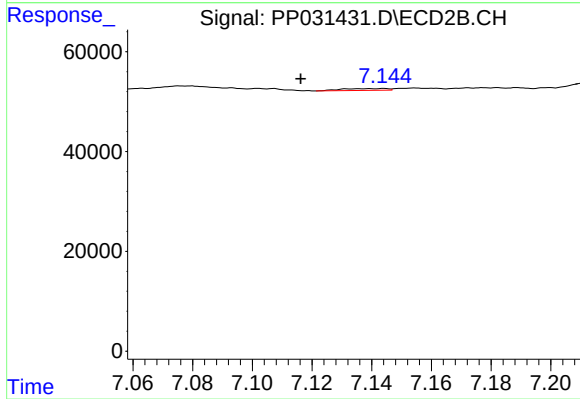

#32 AR-1260-2


R.T.: 7.144 min
Delta R.T.: 0.028 min
Response: 3928
Conc: 1.93 ng/ml

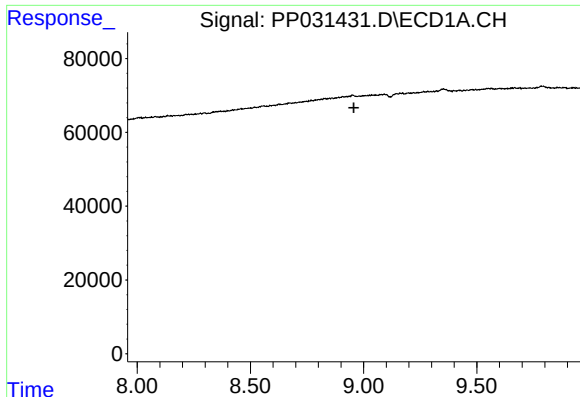

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TT-023-IDW/GW-20201118

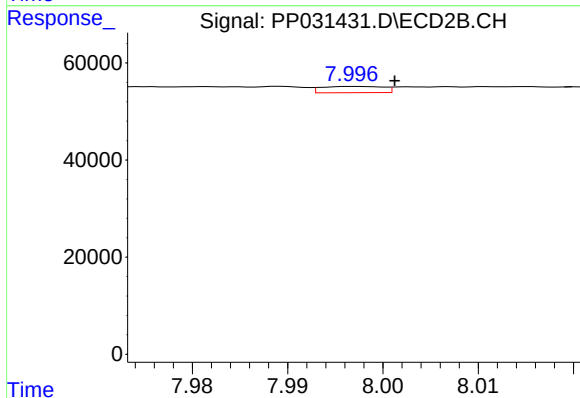


#35 AR-1260-5

R.T.: 7.997 min
Delta R.T.: -0.004 min
Response: 5758
Conc: 1.46 ng/ml

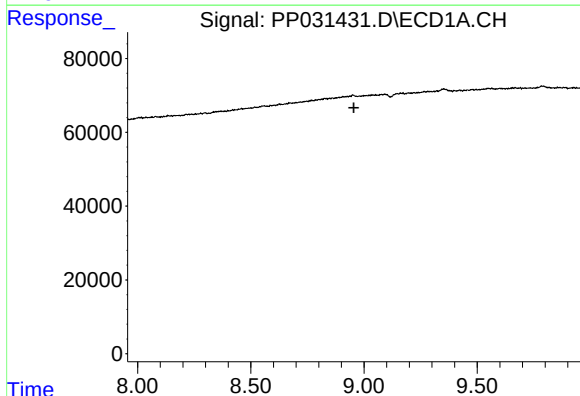


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.956 min
Response: 0
Conc: N.D.

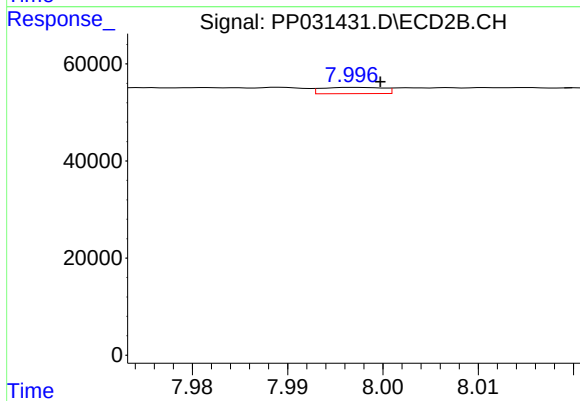

#37 AR-1262-2


R.T.: 7.997 min
Delta R.T.: -0.003 min
Response: 5758
Conc: 1.40 ng/ml

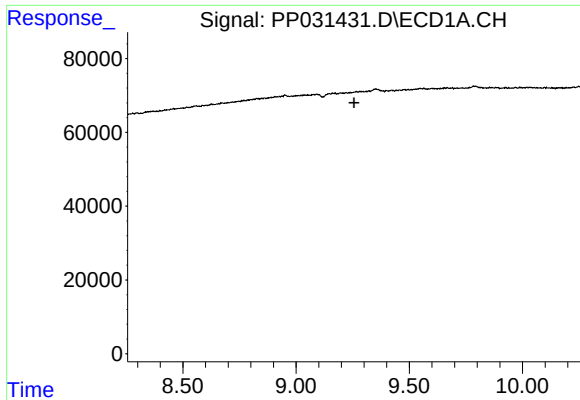

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TT-023-IDW/GW-20201118

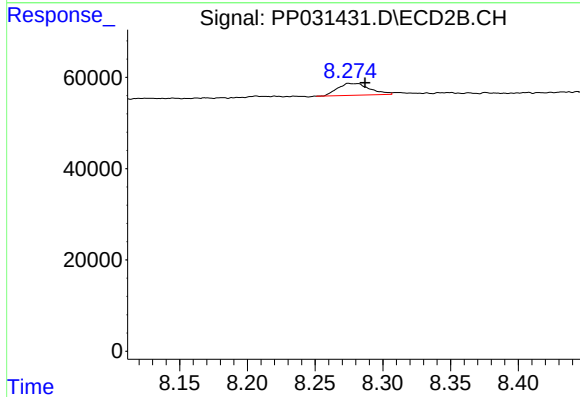


#38 AR-1262-3

R.T.: 8.275 min
Delta R.T.: -0.012 min
Response: 42465
Conc: 26.64 ng/ml

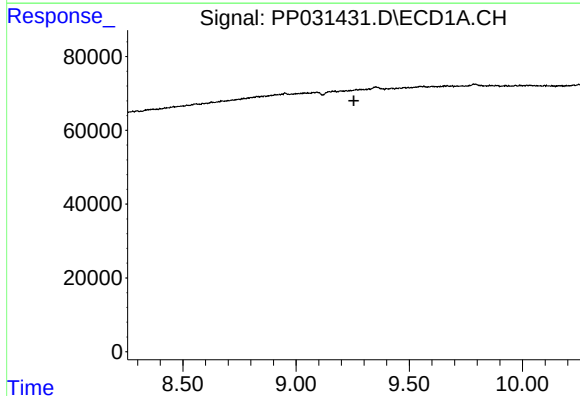

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.255 min
Response: 0
Conc: N.D.

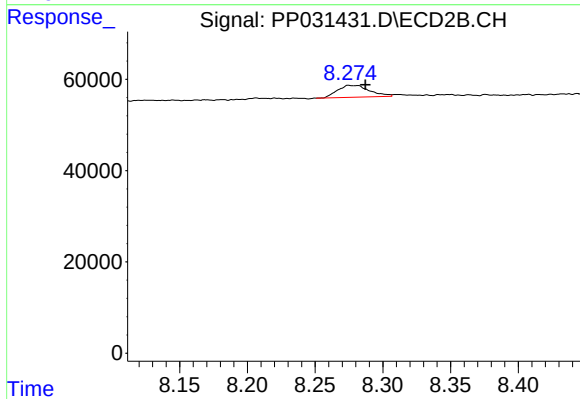

#41 AR-1268-1

R.T.: 8.275 min
Delta R.T.: -0.013 min
Response: 42465
Conc: 8.63 ng/ml