

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031402.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 9:46
 Operator : DD\AJ
 Sample : L4741-03RE 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 11-13-C

Manual Integrations
 APPROVED

mohammad
 11/20/2020 1:53:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 14:11:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.795	4.069	465322	606819	11.422	14.514m#
2) SA Decachlor...	10.666	9.369	113285	381700	3.688m	11.399m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031402.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 9:46
Operator : DD\AJ
Sample : L4741-03RE 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
11-13-C


Manual Integrations
APPROVED

mohammad
11/20/2020 1:53:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 14:11:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

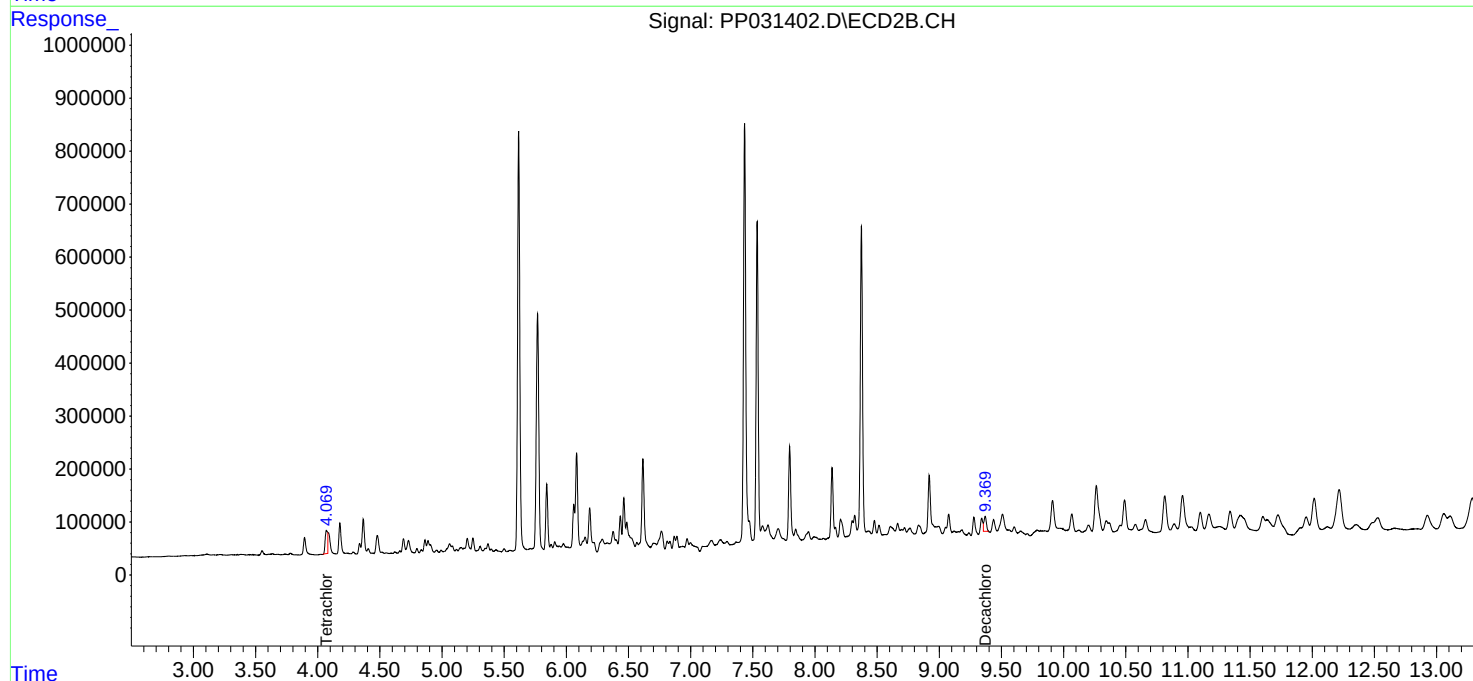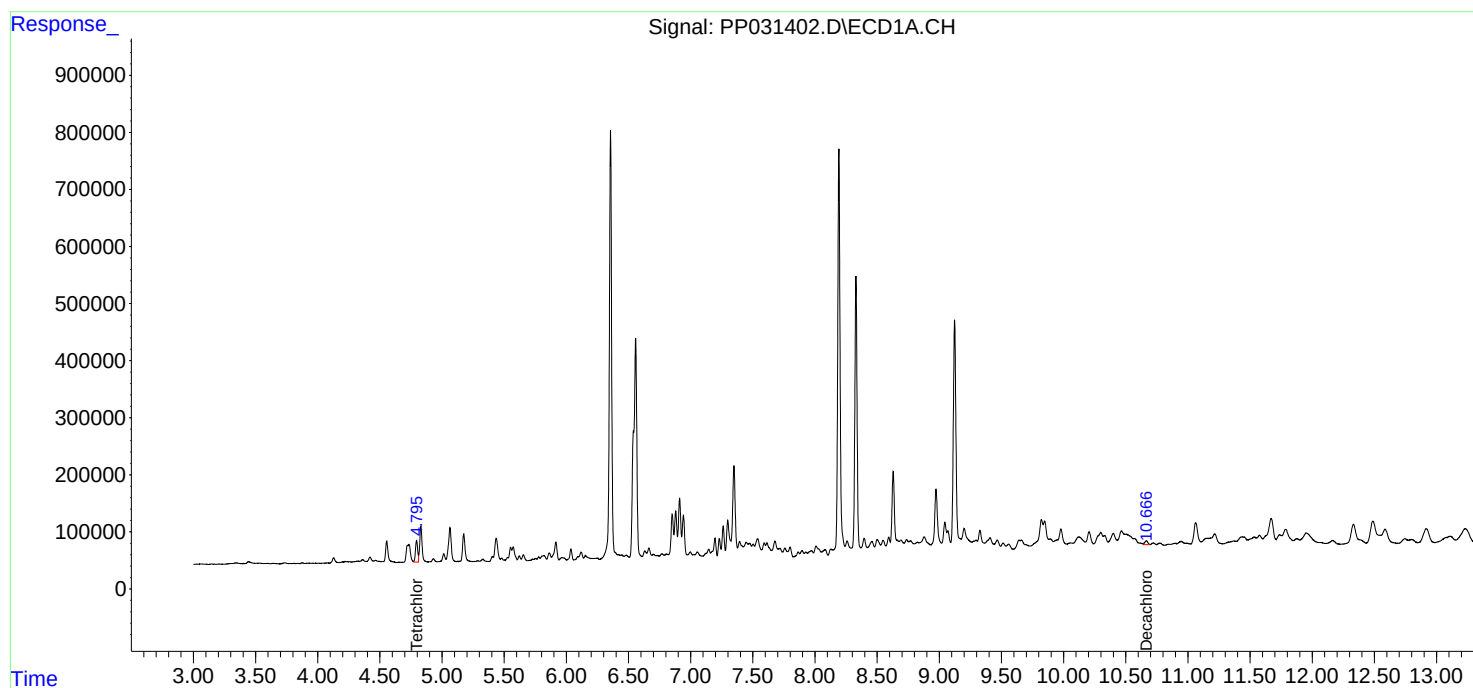

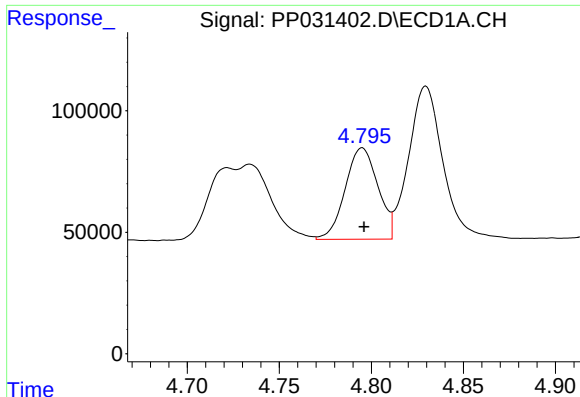


#1 Tetrachloro-m-xylene

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 465322
Conc: 11.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
11-13-C


Manual Integrations
APPROVED

mohammad
11/20/2020 1:53:20 PM

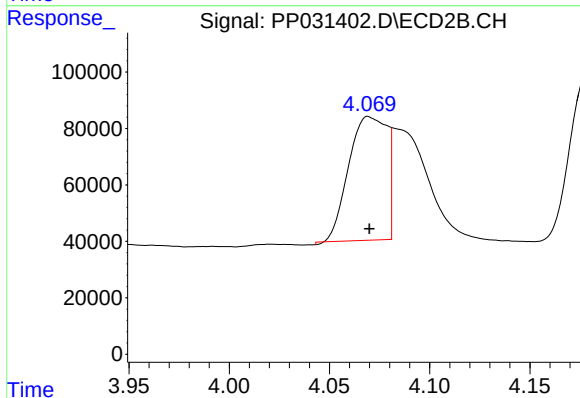


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.001 min
Response: 606819
Conc: 14.51 ng/ml m

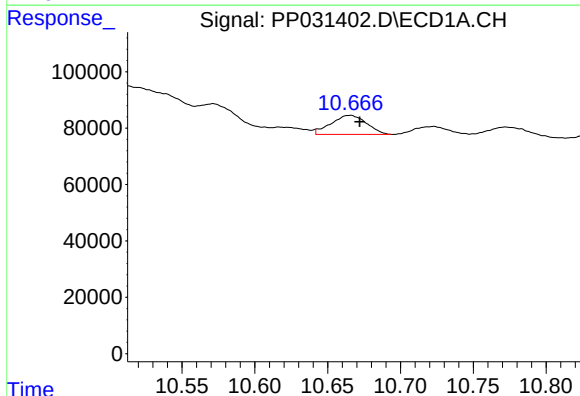

#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.006 min
Response: 113285
Conc: 3.69 ng/ml m

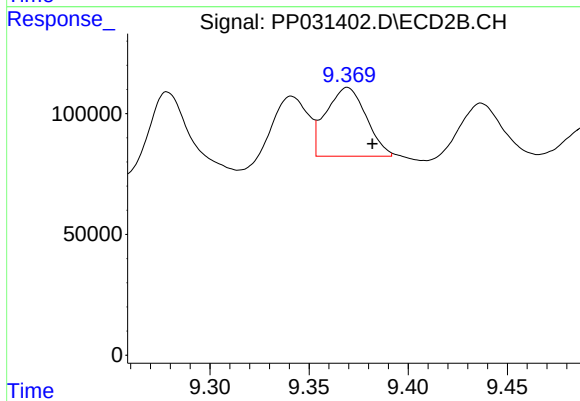

#2 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.013 min
Response: 381700
Conc: 11.40 ng/ml m