

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031405.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 10:36
 Operator : DD\AJ
 Sample : L4779-13RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-1654-1658RE

Manual Integrations
 APPROVED

mohammad
 11/20/2020 1:53:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 14:13:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.795	4.071	379040	412141	9.304m	9.858
2) SA Decachlor...	10.668	9.374	111881	128835	3.643	3.848

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 10:36
Operator : DD\AJ
Sample : L4779-13RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-1654-1658RE


Manual Integrations
APPROVED

mohammad
11/20/2020 1:53:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 14:13:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

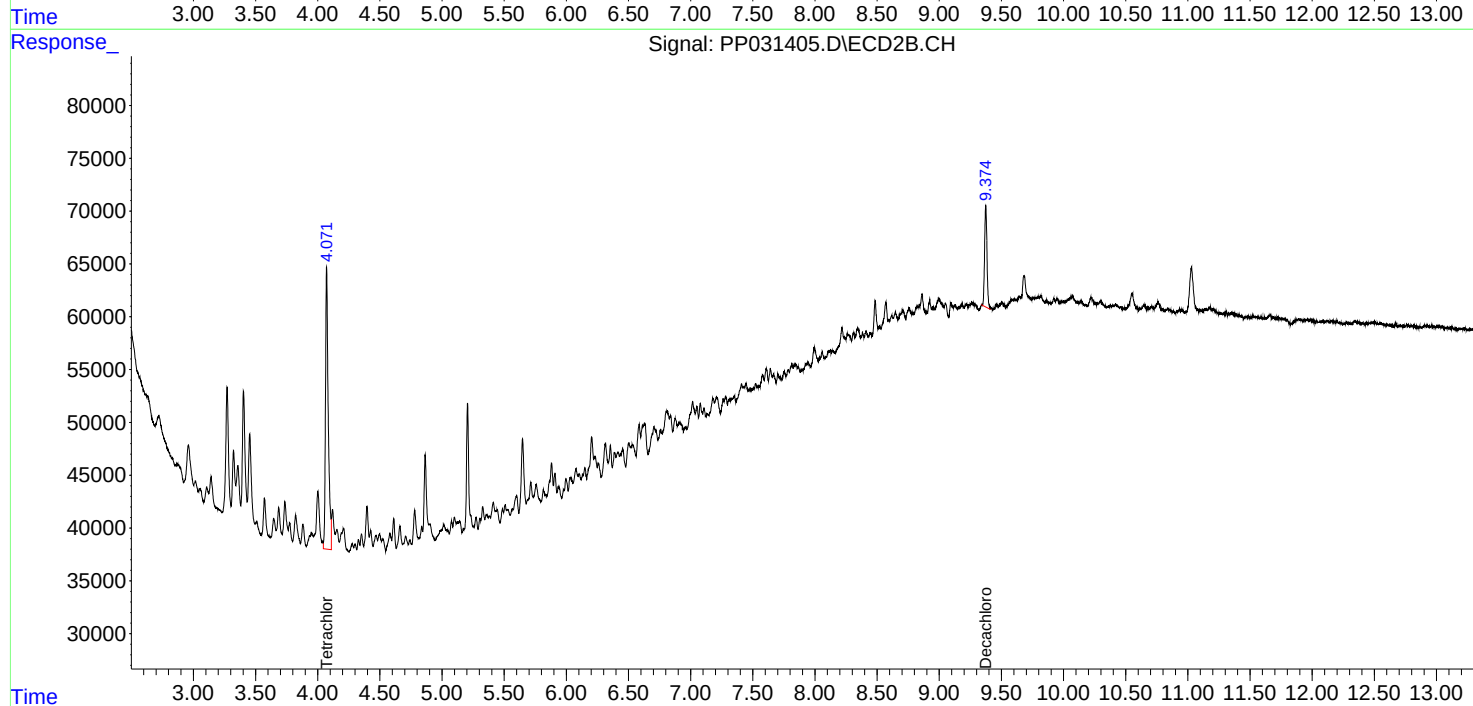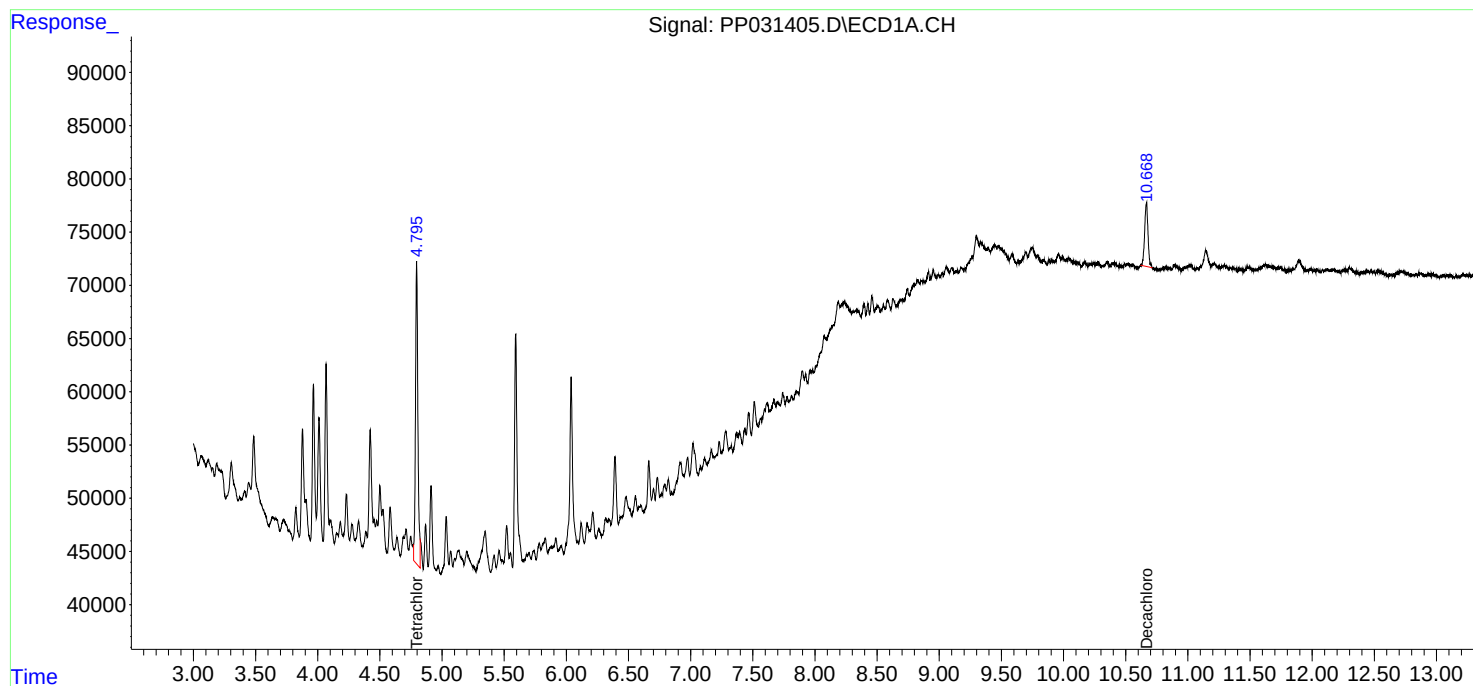

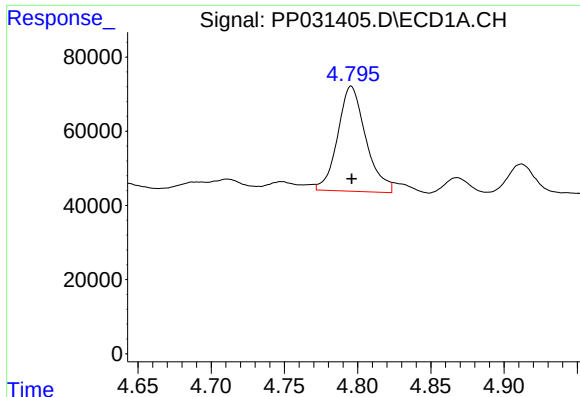


#1 Tetrachloro-m-xylene

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 379040
Conc: 9.30 ng/ml m

Instrument :
ECD_P
ClientSampleId :
COMP-1654-1658RE


Manual Integrations
APPROVED

mohammad
11/20/2020 1:53:25 PM

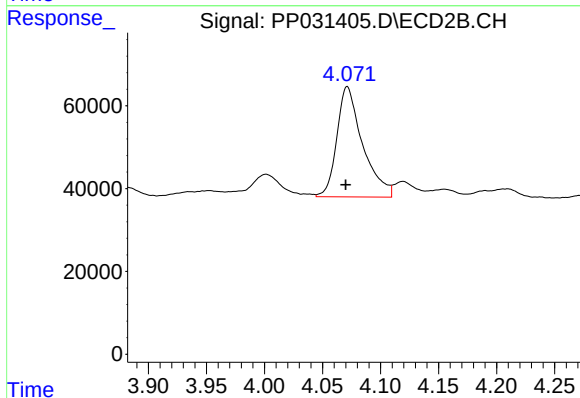


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.001 min
Response: 412141
Conc: 9.86 ng/ml

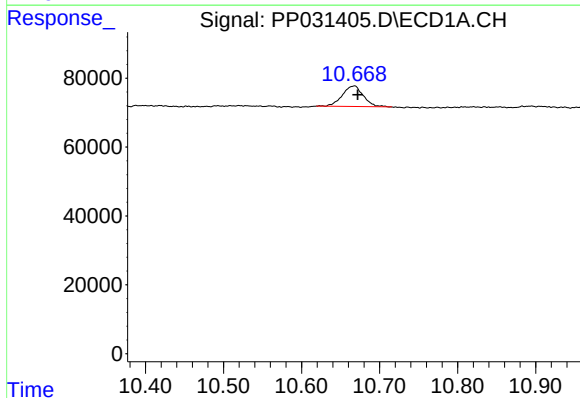

#2 Decachlorobiphenyl

R.T.: 10.668 min
Delta R.T.: -0.004 min
Response: 111881
Conc: 3.64 ng/ml

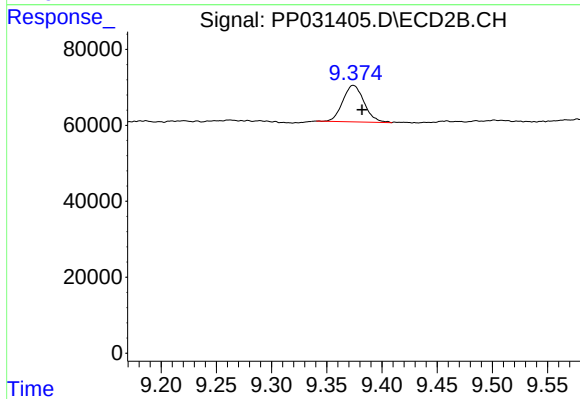

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: -0.008 min
Response: 128835
Conc: 3.85 ng/ml