

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031419.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 15:22
 Operator : DD\AJ
 Sample : L4803-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-01-C5-D5-C5A-D5A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 17:37:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.792	4.066	980553	943556	24.069	22.569
2) SA Decachlor...	10.665	9.374	659670	759845	21.478	22.692

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031419.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 15:22
Operator : DD\AJ
Sample : L4803-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 17:37:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

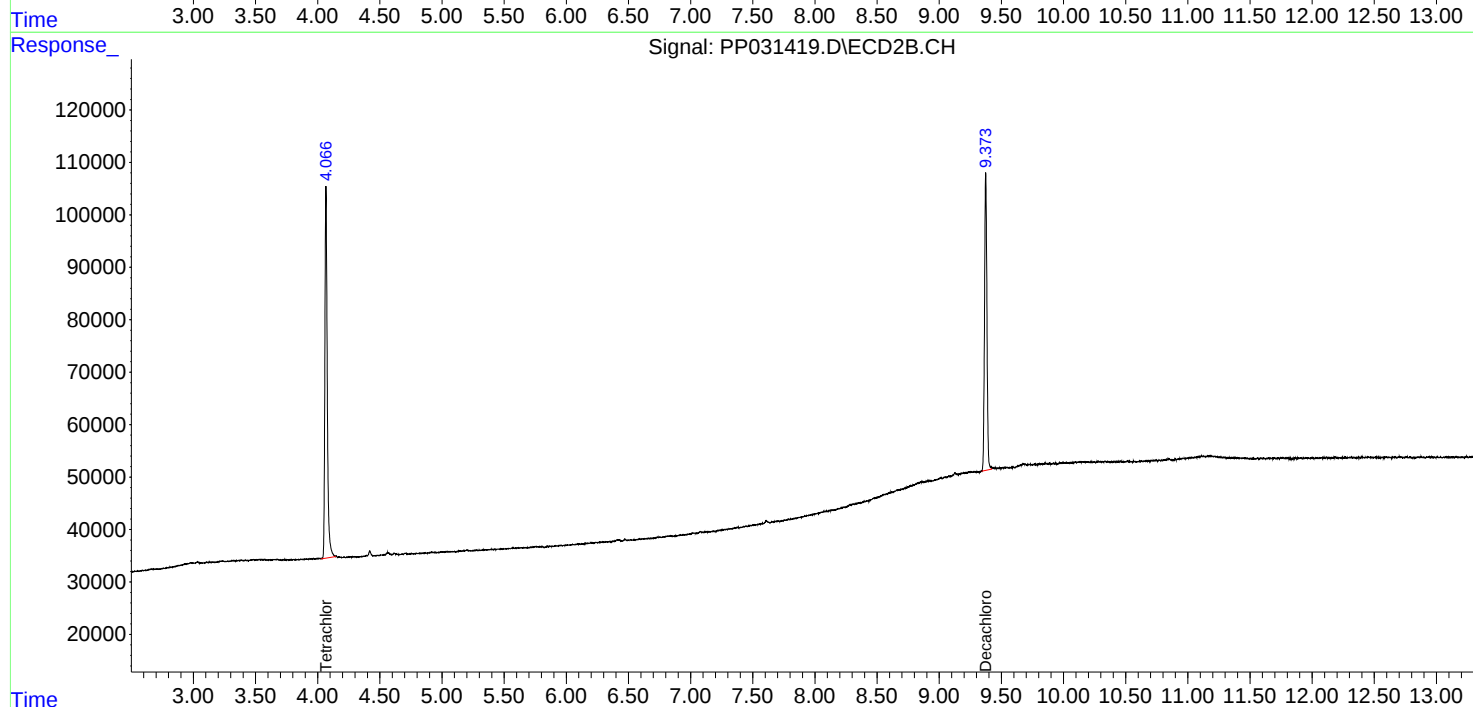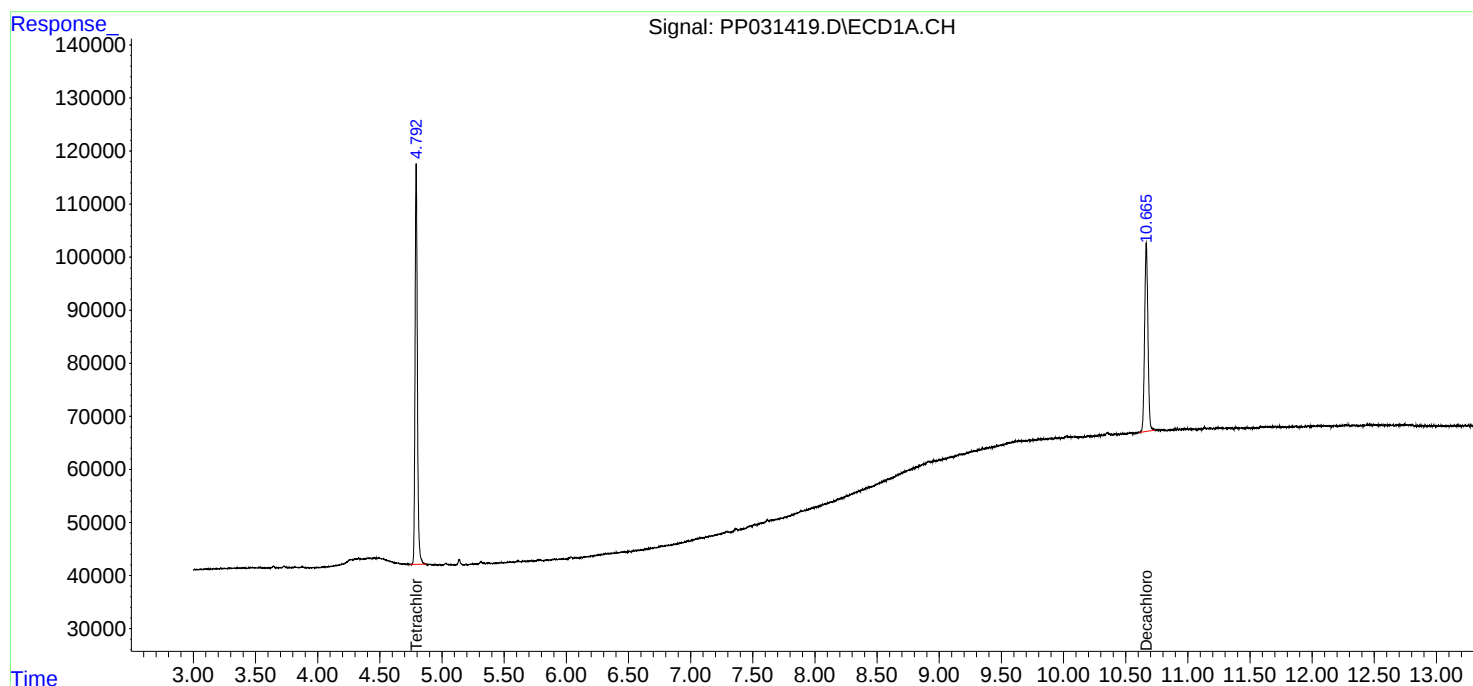


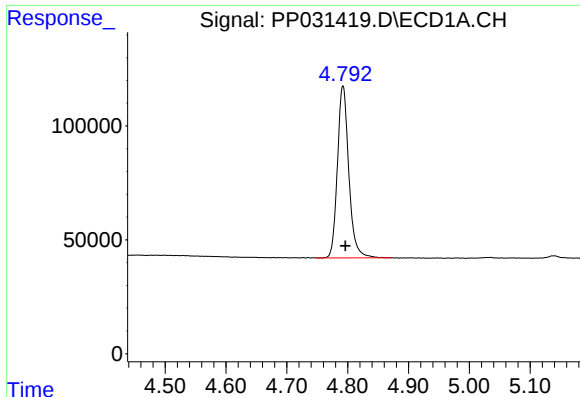

#1 Tetrachloro-m-xylene


R.T.: 4.792 min
Delta R.T.: -0.004 min
Response: 980553
Conc: 24.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

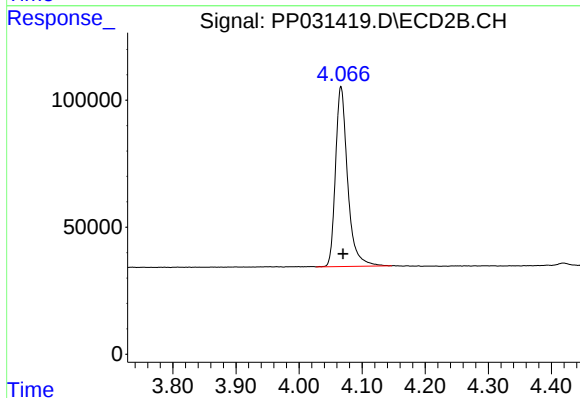


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: -0.004 min
Response: 943556
Conc: 22.57 ng/ml

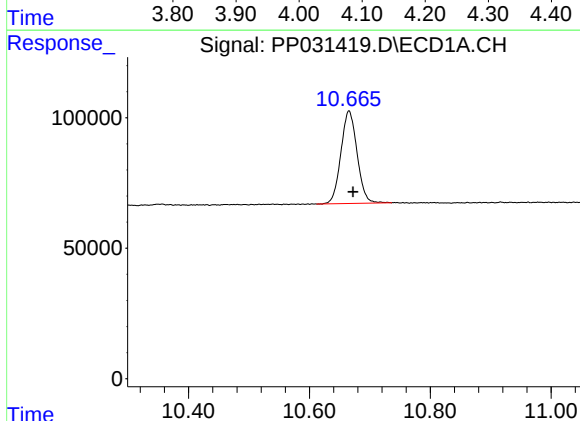

#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: -0.007 min
Response: 659670
Conc: 21.48 ng/ml

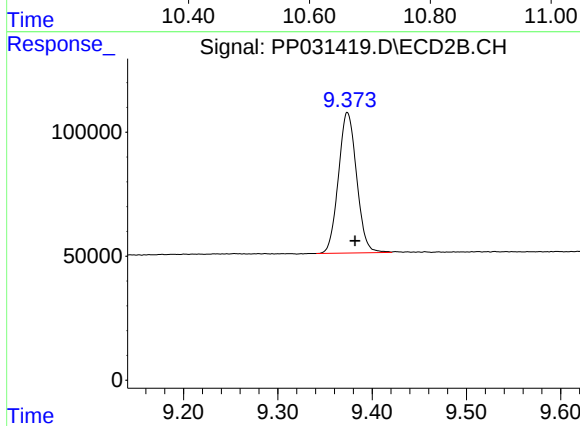

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: -0.008 min
Response: 759845
Conc: 22.69 ng/ml