

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031427.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 18:10
 Operator : DD\AJ
 Sample : L4791-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2020-11-16-EB

Manual Integrations
 APPROVED

mohammad
 11/20/2020 1:53:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 00:58:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.794	4.069	1081089	1019771	26.537	24.392m
2) SA Decachlor...	10.667	9.374	706542	813937	23.004	24.308

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031427.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 18:10
Operator : DD\AJ
Sample : L4791-20
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
2020-11-16-EB


Manual Integrations
APPROVED

mohammad
11/20/2020 1:53:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 00:58:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

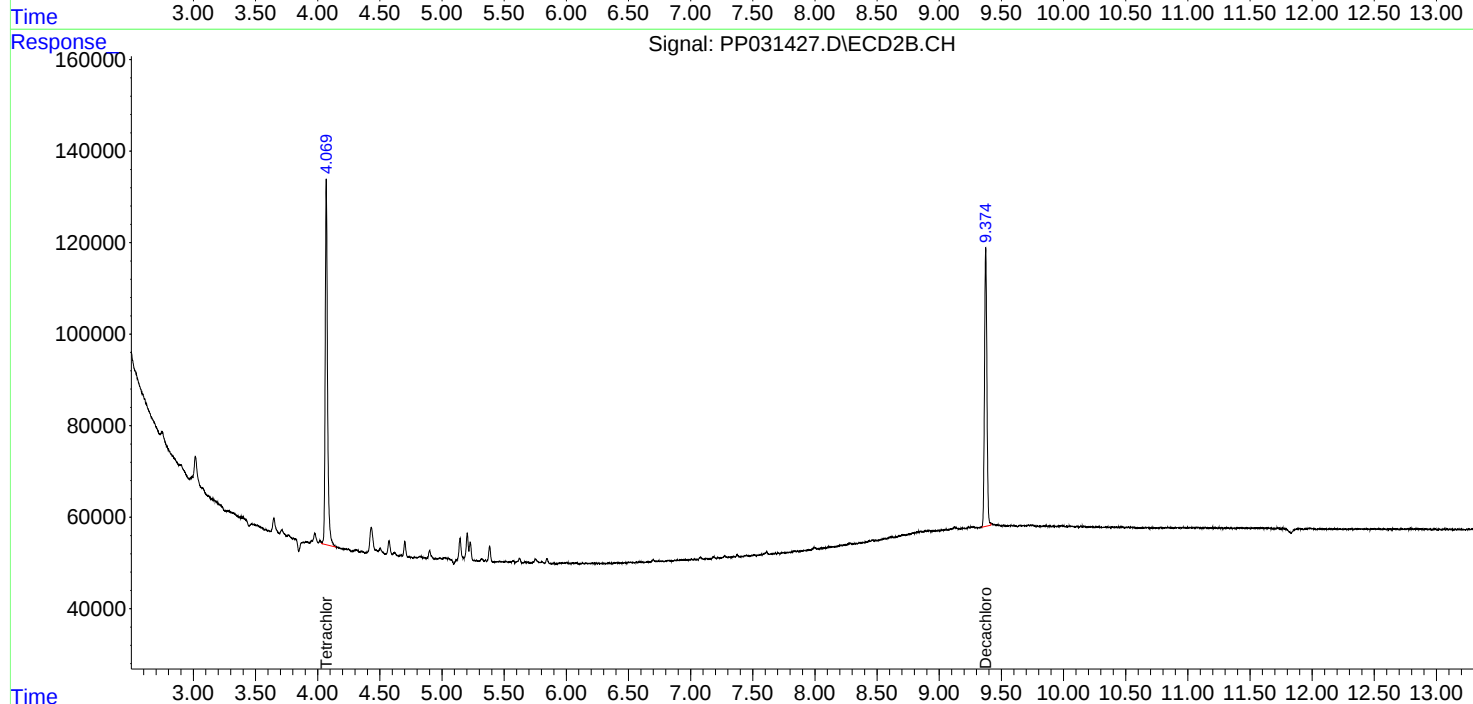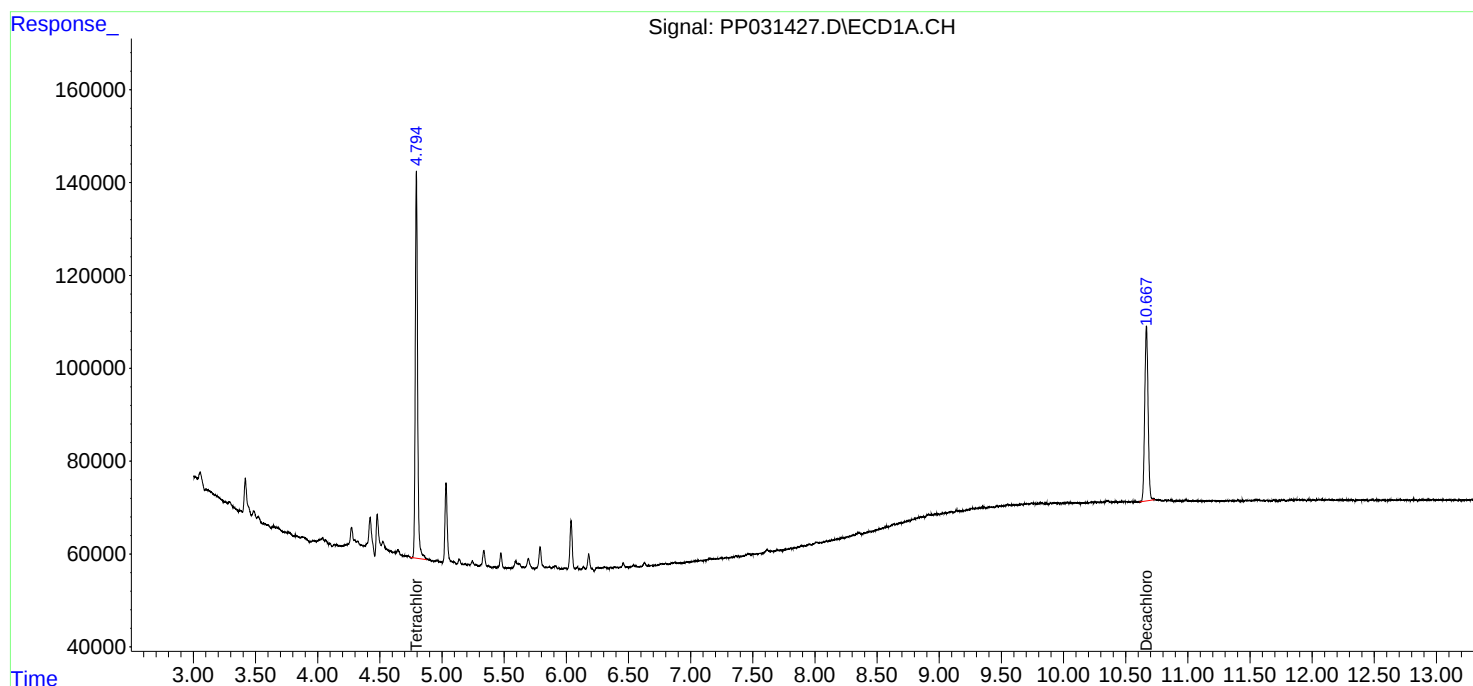

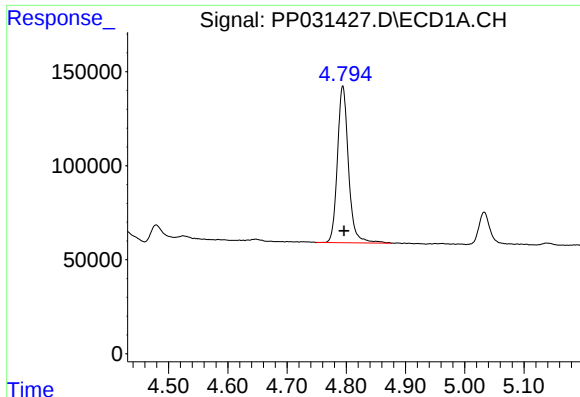


#1 Tetrachloro-m-xylene

R.T.: 4.794 min
Delta R.T.: -0.002 min
Response: 1081089
Conc: 26.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
2020-11-16-EB


Manual Integrations
APPROVED

mohammad
11/20/2020 1:53:49 PM

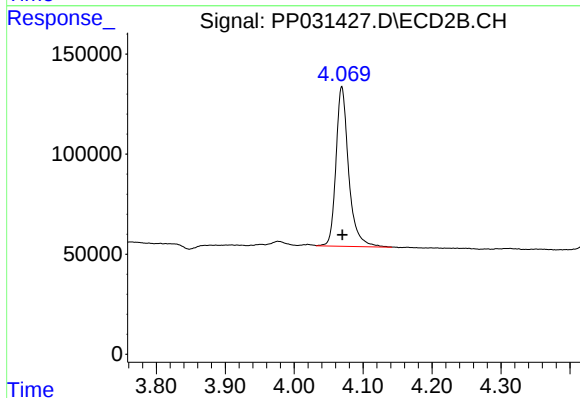


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.001 min
Response: 1019771
Conc: 24.39 ng/ml m

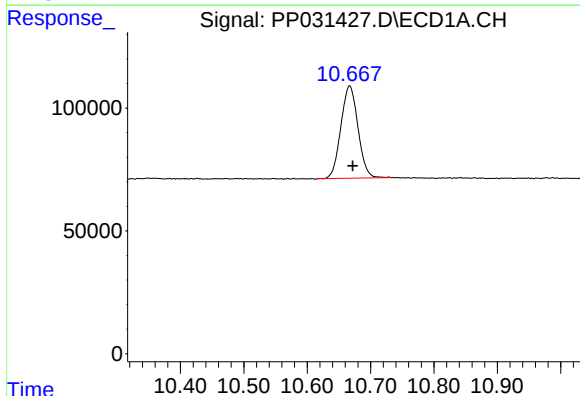

#2 Decachlorobiphenyl

R.T.: 10.667 min
Delta R.T.: -0.005 min
Response: 706542
Conc: 23.00 ng/ml

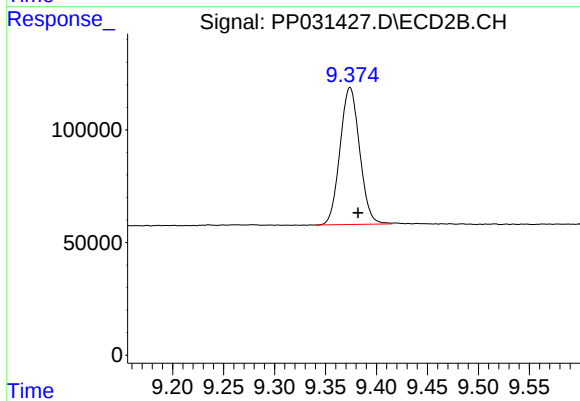

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: -0.008 min
Response: 813937
Conc: 24.31 ng/ml