

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041149.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 2:06
 Operator : AJ\MA
 Sample : M4758-31
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:29:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	3.760	434214	631793	20.590	22.734
2) SA Decachlor...	10.650	9.018	378190	251246	17.313	17.526
Target Compounds						
9) L2 AR-1221-2	0.000	4.108	0	8926	N.D.	35.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 2:06
Operator : AJ\MA
Sample : M4758-31
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:29:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

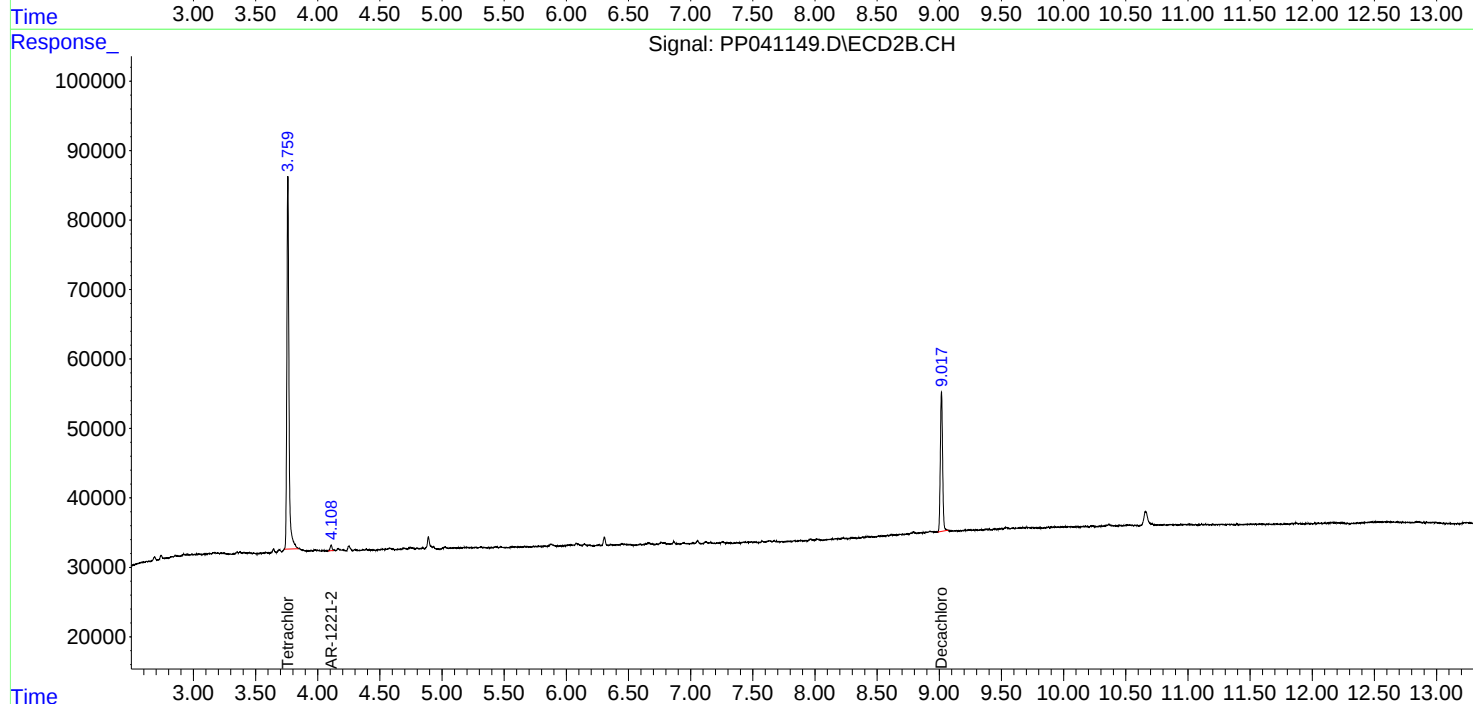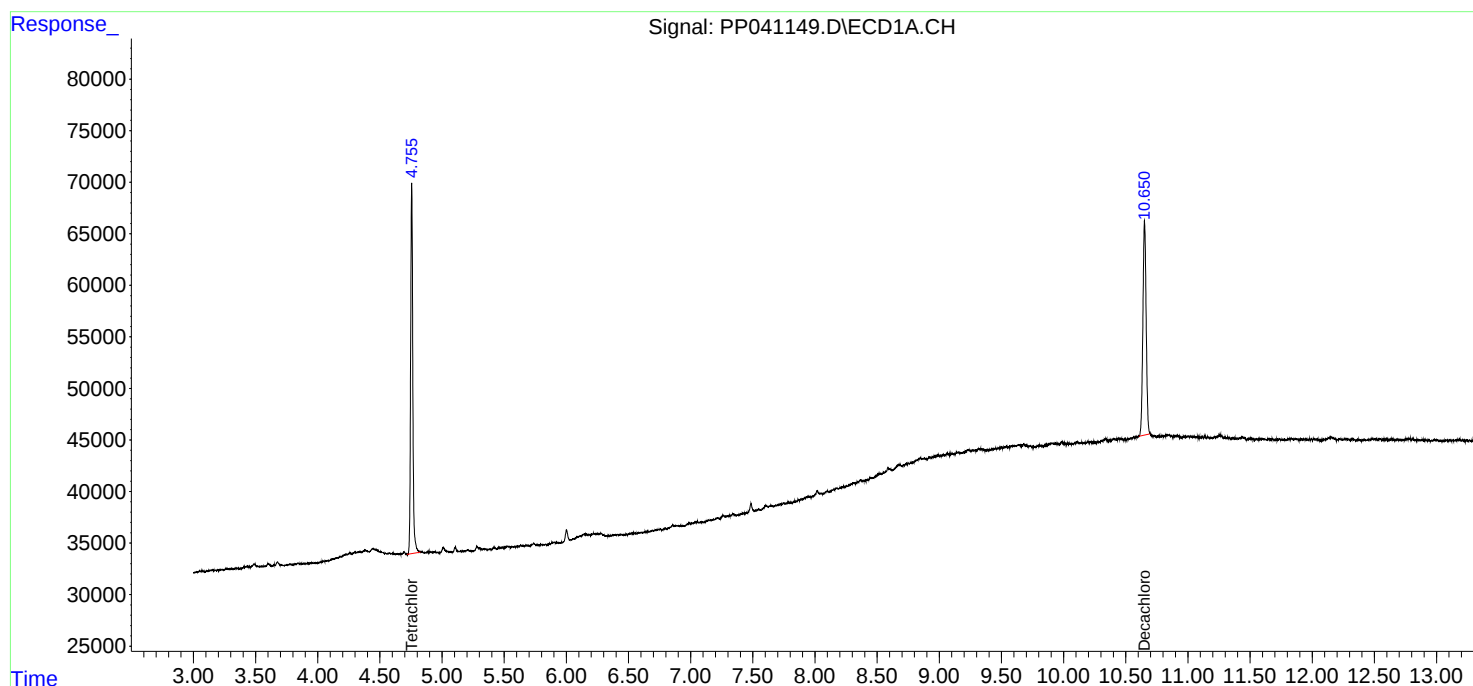


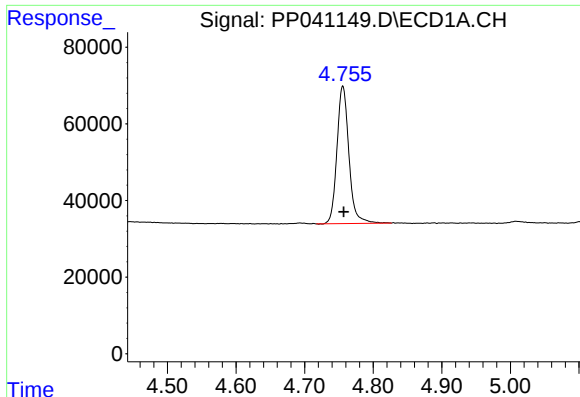

#1 Tetrachloro-m-xylene


R.T.: 4.756 min
Delta R.T.: -0.001 min
Response: 434214
Conc: 20.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP16

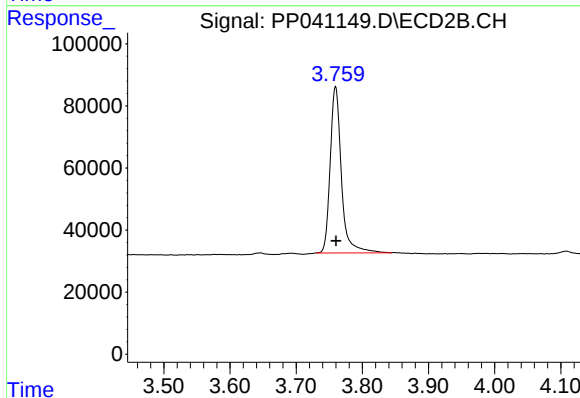


#1 Tetrachloro-m-xylene

R.T.: 3.760 min
Delta R.T.: 0.000 min
Response: 631793
Conc: 22.73 ng/ml

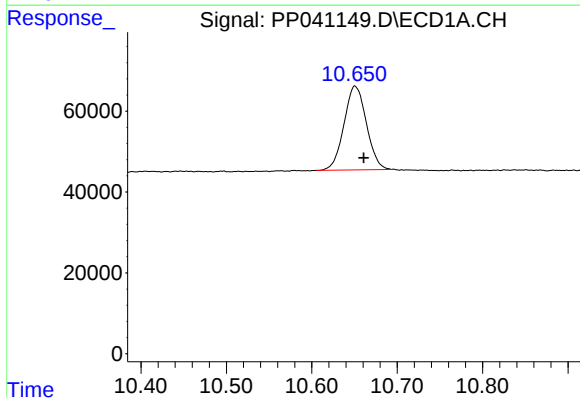


#2 Decachlorobiphenyl

R.T.: 10.650 min
Delta R.T.: -0.010 min
Response: 378190
Conc: 17.31 ng/ml

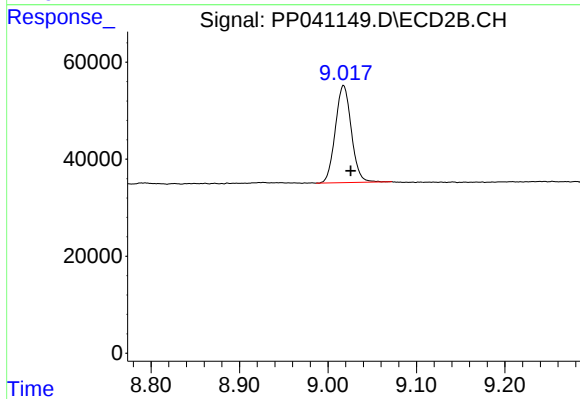

#2 Decachlorobiphenyl


R.T.: 9.018 min
Delta R.T.: -0.008 min
Response: 251246
Conc: 17.53 ng/ml

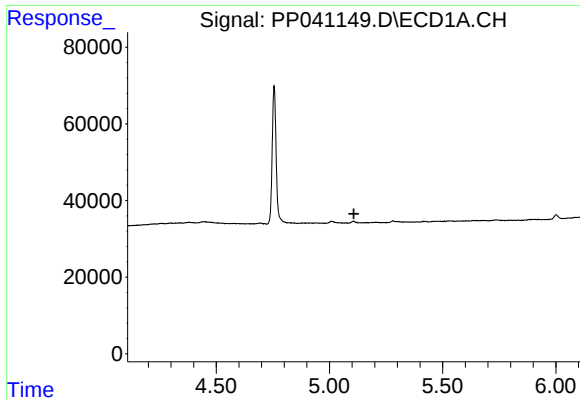

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP16

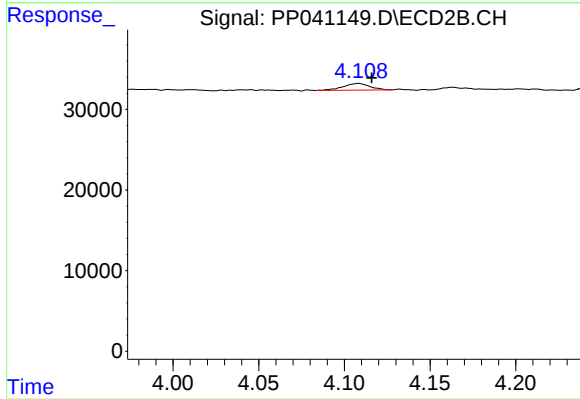

#9 AR-1221-2

R.T.: 4.108 min
Delta R.T.: -0.008 min
Response: 8926
Conc: 35.20 ng/ml