

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041174.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 10:16
 Operator : AJ\MA
 Sample : M4728-01 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2021-4A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:37:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.754	3.757	30451	56136	1.444	2.020 #
2)	SA Decachlor...	10.649	9.014	55723	34393	2.551	2.399
Target Compounds							
20)	L4 AR-1242-5	7.040	5.897f	2580	47633	5.772	88.224 #
24)	L5 AR-1248-4	7.026	0.000	2633	0	3.529	N.D. #
25)	L5 AR-1248-5	7.040	5.897f	2580	47633	3.412	65.795 #
26)	L6 AR-1254-1	6.984	5.897f	41725	47633	54.029	41.830
28)	L6 AR-1254-3	7.604	0.000	25478	0	19.027	N.D. #
29)	L6 AR-1254-4	7.873	6.710	2505	20140	2.625	24.280 #
31)	L7 AR-1260-1	0.000	6.586	0	11068	N.D.	11.561 #
32)	L7 AR-1260-2	8.031	0.000	23116	0	19.560	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041174.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 10:16
Operator : AJ\MA
Sample : M4728-01 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:37:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

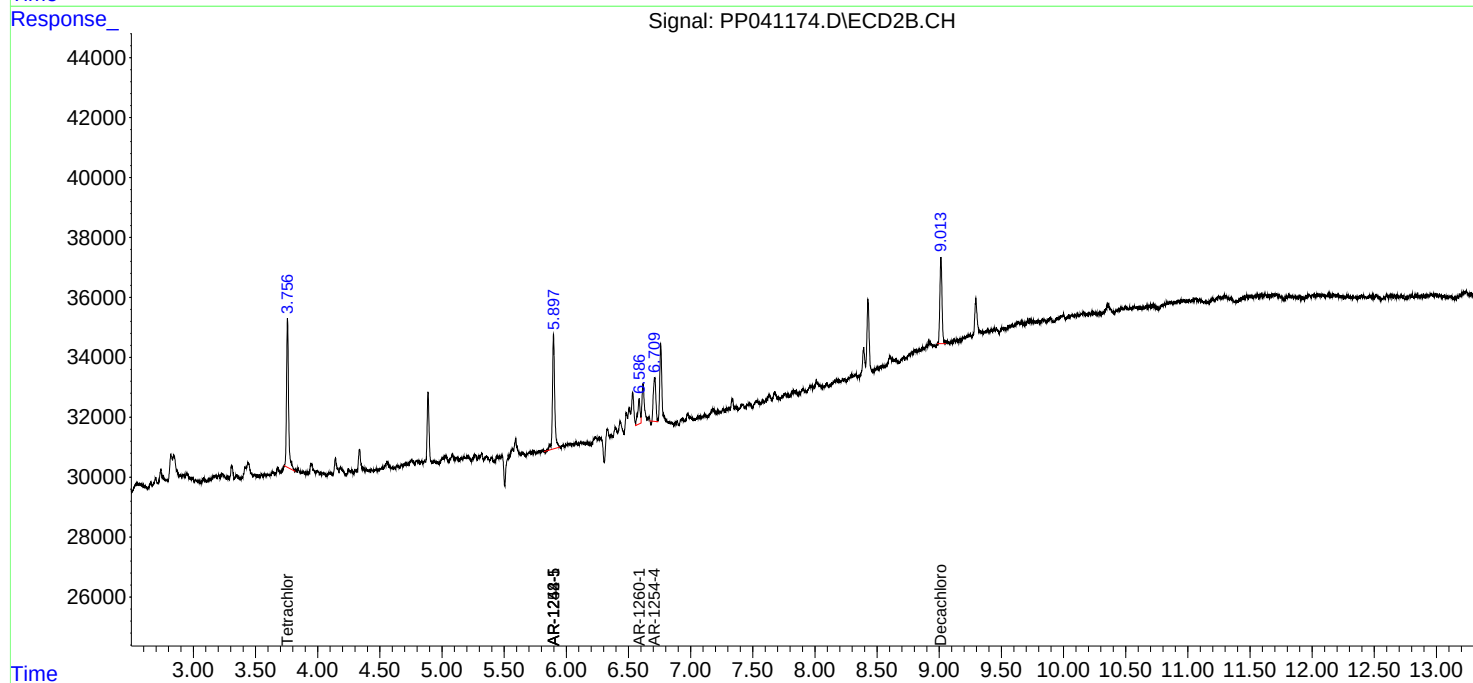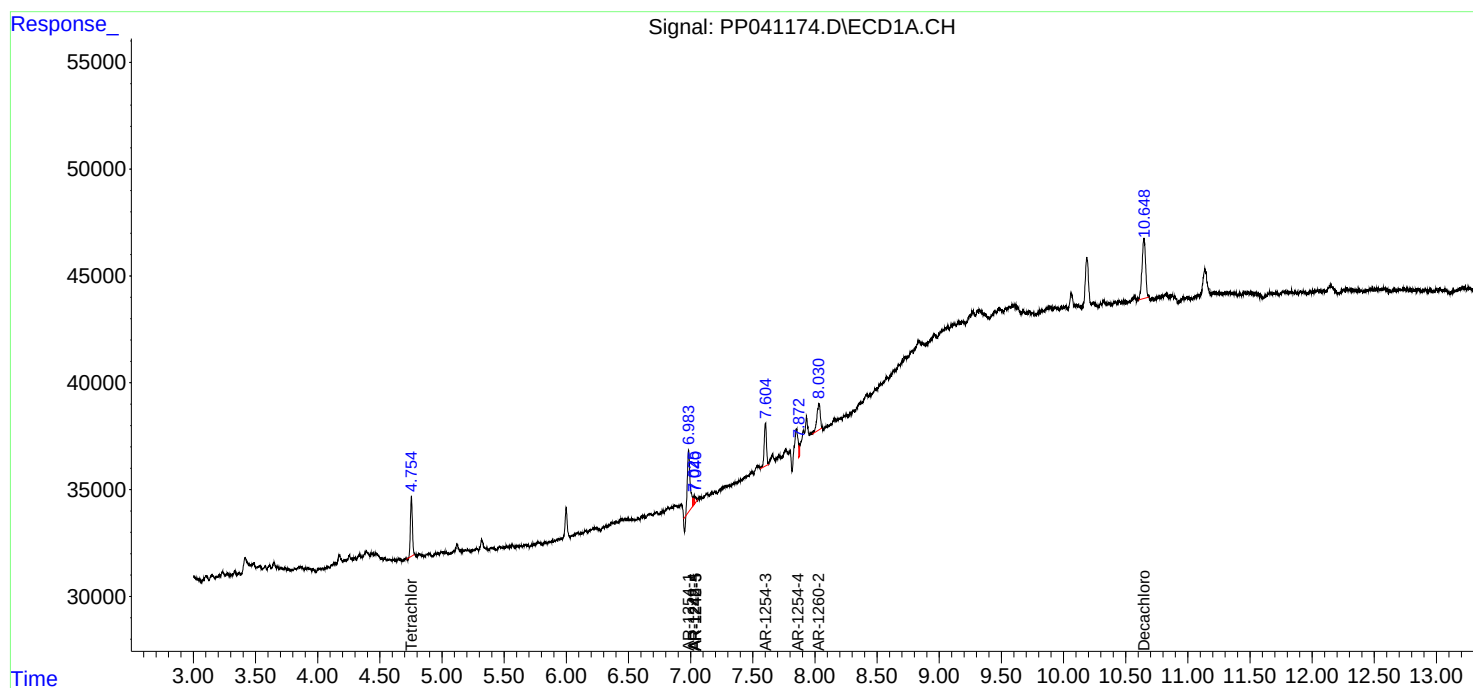


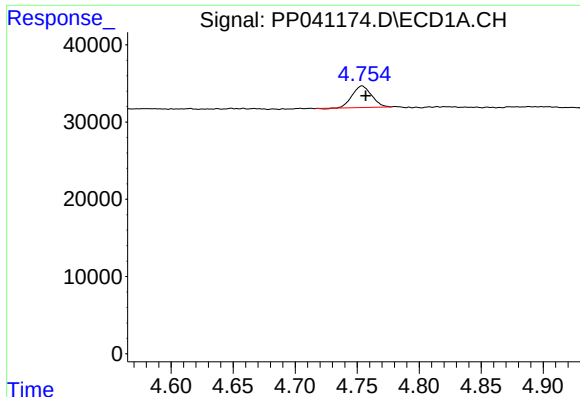

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 30451
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4A

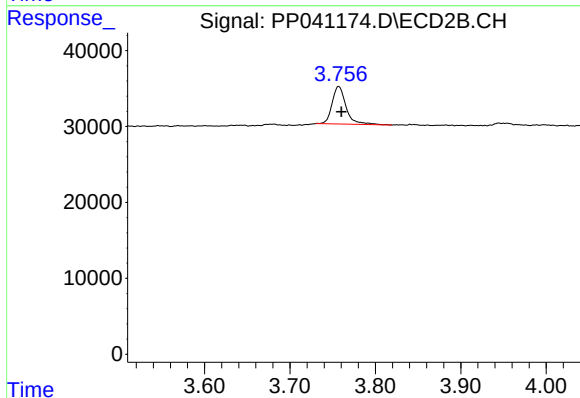


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 56136
Conc: 2.02 ng/ml

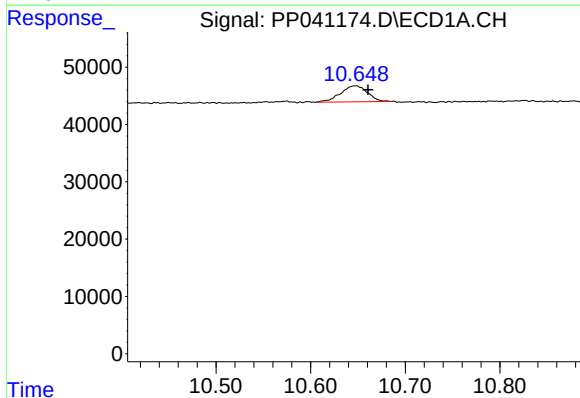


#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.012 min
Response: 55723
Conc: 2.55 ng/ml

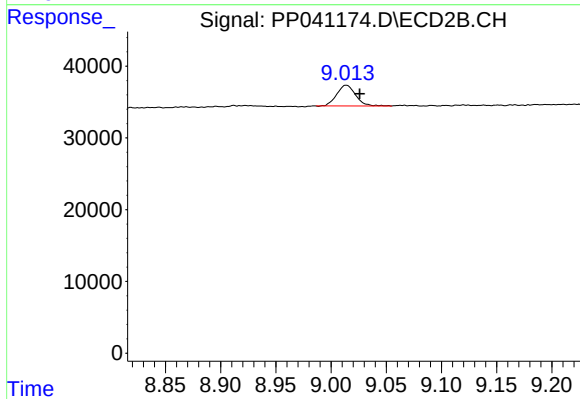

#2 Decachlorobiphenyl


R.T.: 9.014 min
Delta R.T.: -0.012 min
Response: 34393
Conc: 2.40 ng/ml

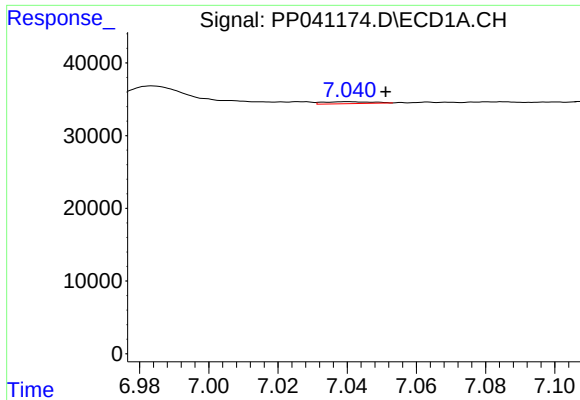

#20 AR-1242-5


R.T.: 7.040 min
Delta R.T.: -0.011 min
Response: 2580
Conc: 5.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4A

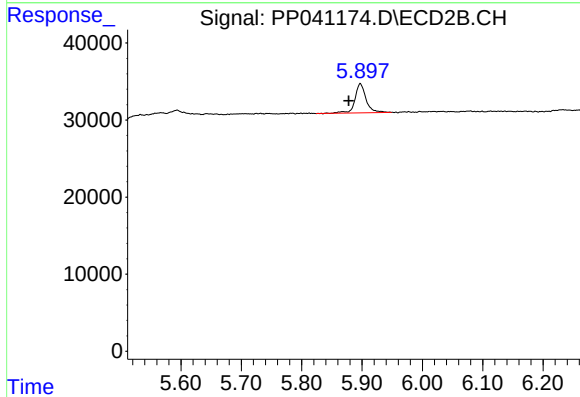


#20 AR-1242-5

R.T.: 5.897 min
Delta R.T.: 0.019 min
Response: 47633
Conc: 88.22 ng/ml

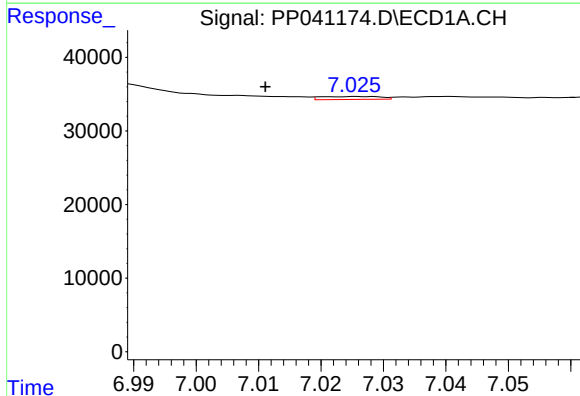


#24 AR-1248-4

R.T.: 7.026 min
Delta R.T.: 0.015 min
Response: 2633
Conc: 3.53 ng/ml

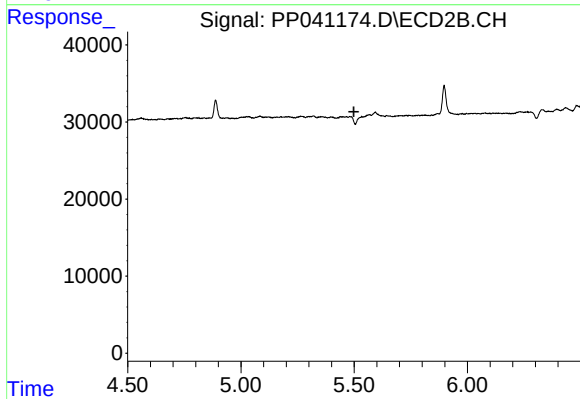

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.498 min
Response: 0
Conc: N.D.

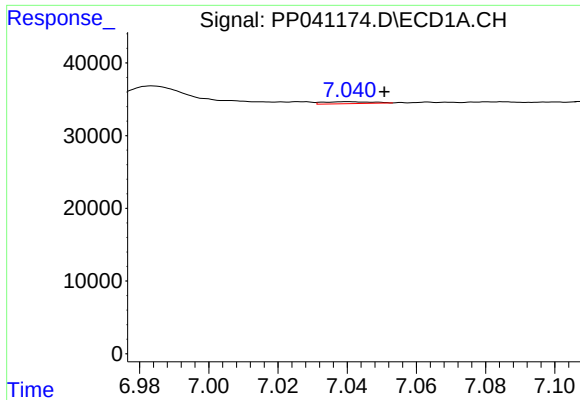

#25 AR-1248-5


R.T.: 7.040 min
Delta R.T.: -0.010 min
Response: 2580
Conc: 3.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4A

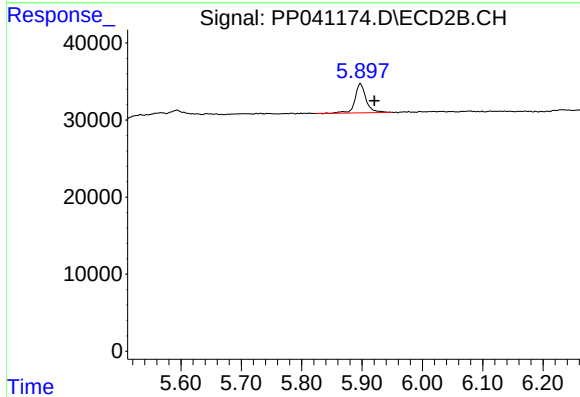


#25 AR-1248-5

R.T.: 5.897 min
Delta R.T.: -0.023 min
Response: 47633
Conc: 65.79 ng/ml

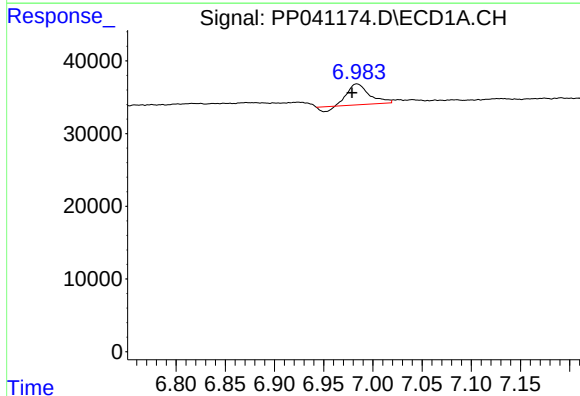


#26 AR-1254-1

R.T.: 6.984 min
Delta R.T.: 0.005 min
Response: 41725
Conc: 54.03 ng/ml

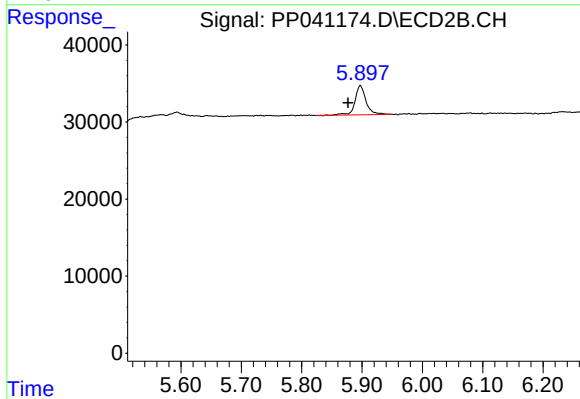

#26 AR-1254-1


R.T.: 5.897 min
Delta R.T.: 0.020 min
Response: 47633
Conc: 41.83 ng/ml

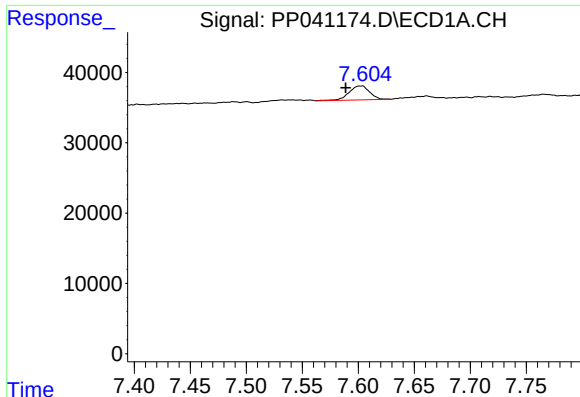

#28 AR-1254-3


R.T.: 7.604 min
Delta R.T.: 0.015 min
Response: 25478
Conc: 19.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4A

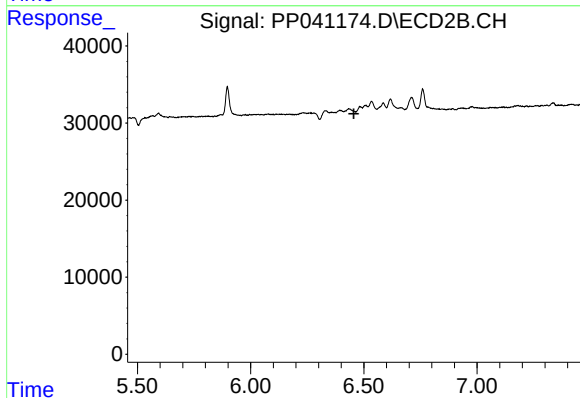


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

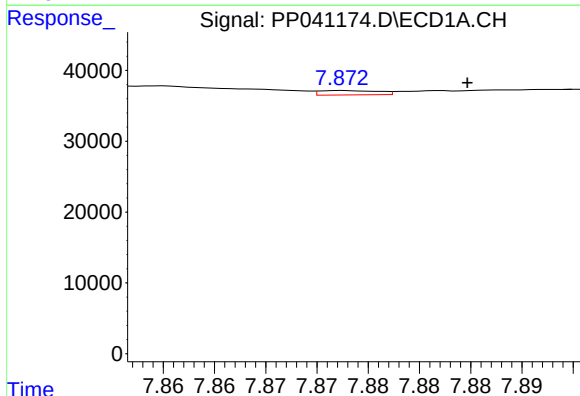


#29 AR-1254-4

R.T.: 7.873 min
Delta R.T.: -0.012 min
Response: 2505
Conc: 2.63 ng/ml

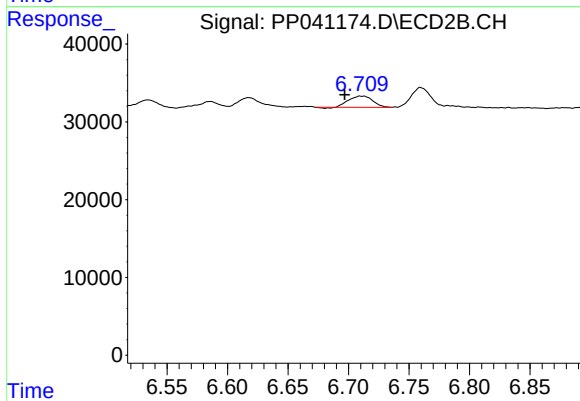

#29 AR-1254-4


R.T.: 6.710 min
Delta R.T.: 0.014 min
Response: 20140
Conc: 24.28 ng/ml

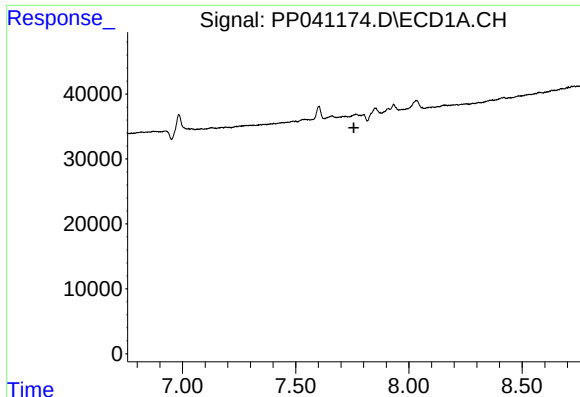

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4A

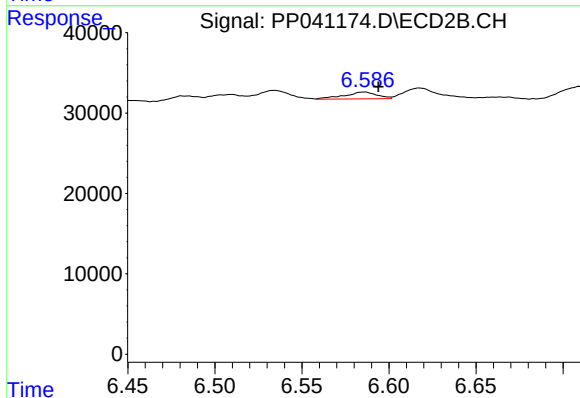


#31 AR-1260-1

R.T.: 6.586 min
Delta R.T.: -0.008 min
Response: 11068
Conc: 11.56 ng/ml

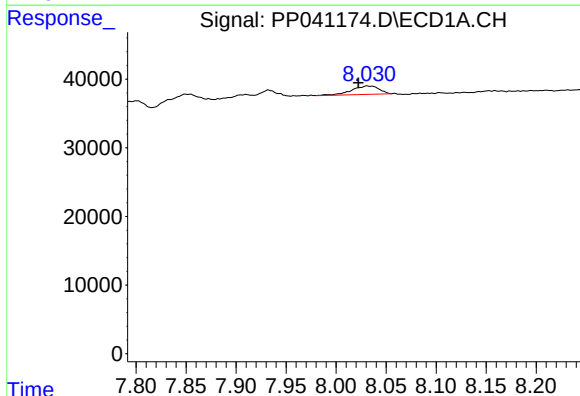

#32 AR-1260-2

R.T.: 8.031 min
Delta R.T.: 0.009 min
Response: 23116
Conc: 19.56 ng/ml

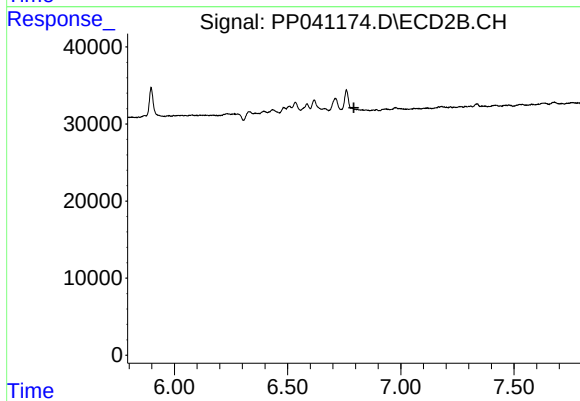

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.793 min
Response: 0
Conc: N.D.