

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041175.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 10:33
 Operator : AJ\MA
 Sample : M4728-02 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2021-4B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:37:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.753	3.756	33748	53744	1.600	1.934
2) SA Decachlor...	10.649	9.014	57758	37654	2.644	2.627
Target Compounds						
20) L4 AR-1242-5	7.045	5.897f	1266	77571	2.833	143.675 #
24) L5 AR-1248-4	7.026f	0.000	2645	0	3.545	N.D. #
25) L5 AR-1248-5	7.045	5.897f	1266	77571	1.675	107.148 #
26) L6 AR-1254-1	6.983	5.897f	97507	77571	126.261	68.122 #
28) L6 AR-1254-3	7.601	6.484f	44743	9170	33.414	6.340 #
29) L6 AR-1254-4	7.910f	6.711	34714	25297	36.375	30.497
31) L7 AR-1260-1	0.000	6.586	0	12824	N.D.	13.395 #
32) L7 AR-1260-2	8.036	0.000	48318	0	40.885	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041175.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 10:33
Operator : AJ\MA
Sample : M4728-02 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:37:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

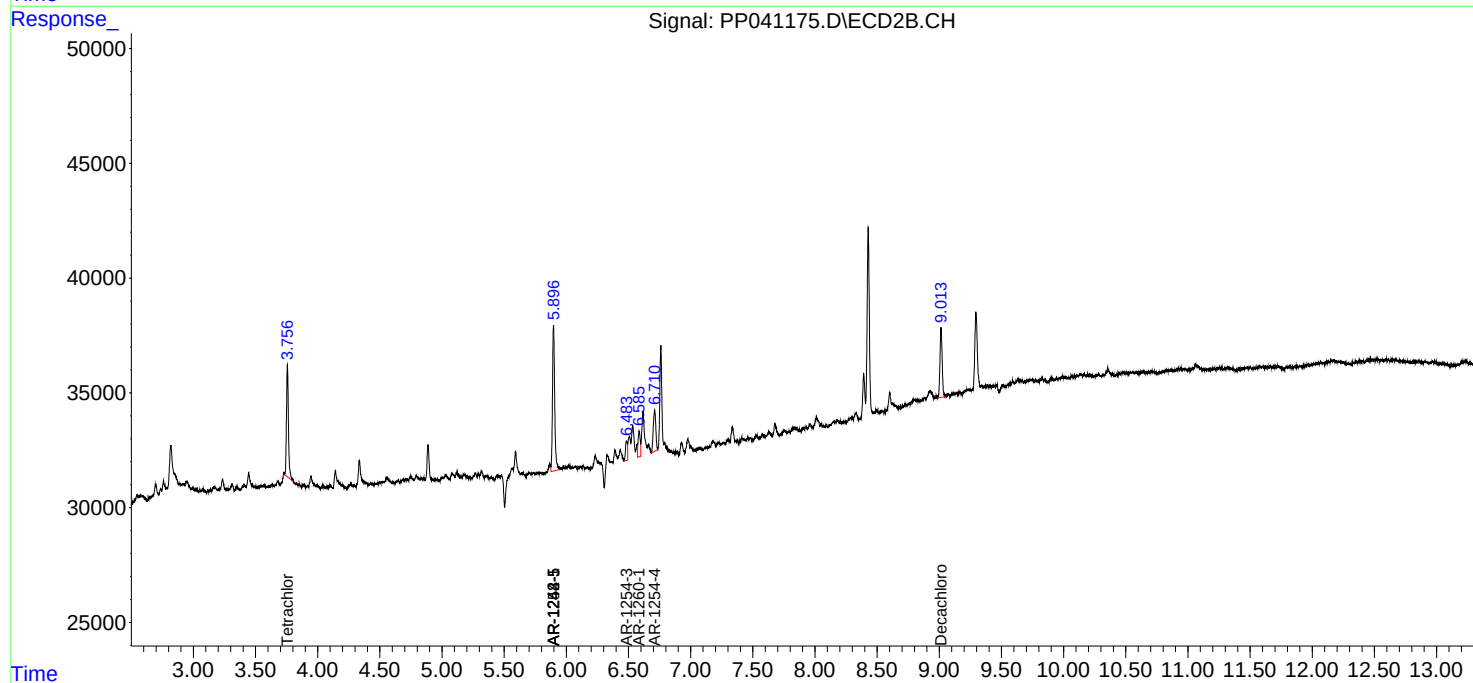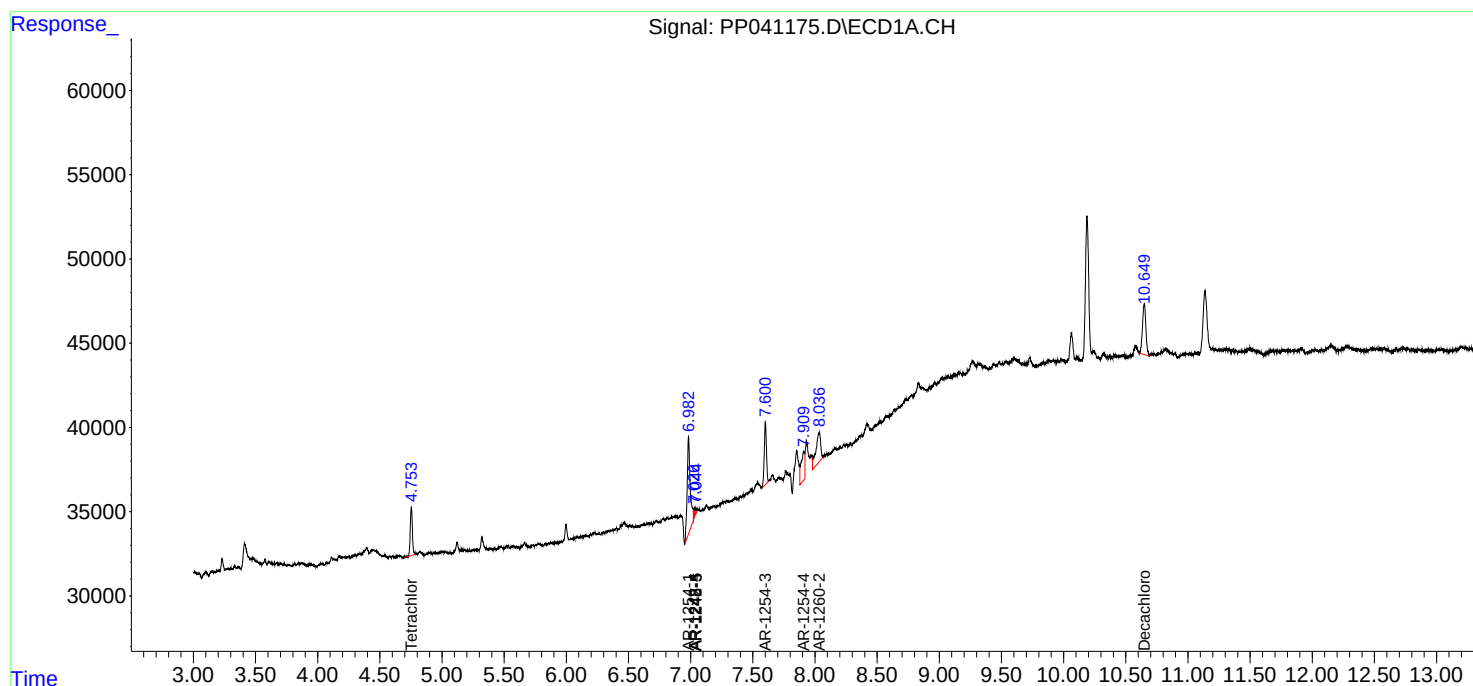


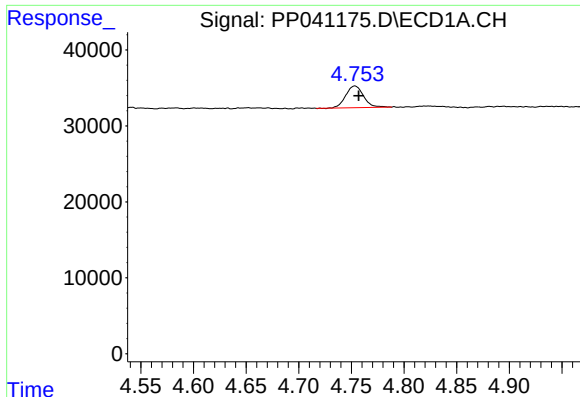

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.004 min
Response: 33748
Conc: 1.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4B

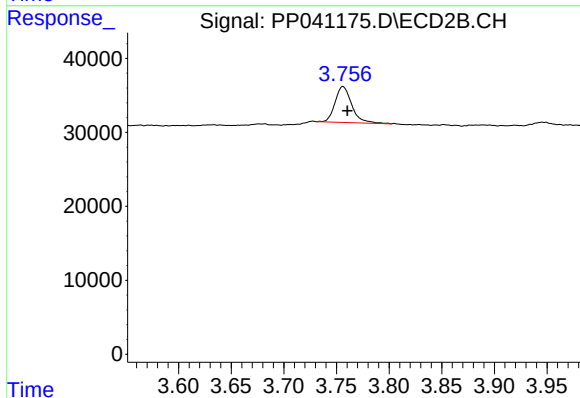


#1 Tetrachloro-m-xylene

R.T.: 3.756 min
Delta R.T.: -0.004 min
Response: 53744
Conc: 1.93 ng/ml

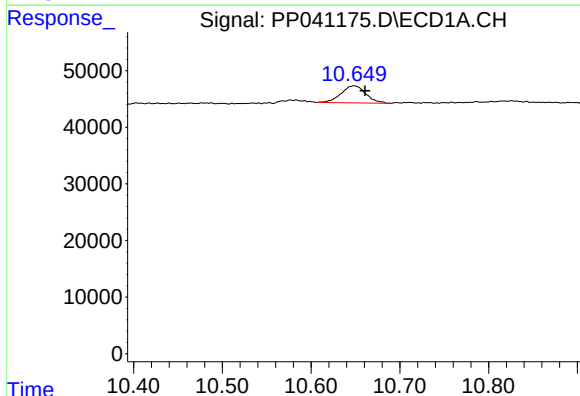


#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.012 min
Response: 57758
Conc: 2.64 ng/ml

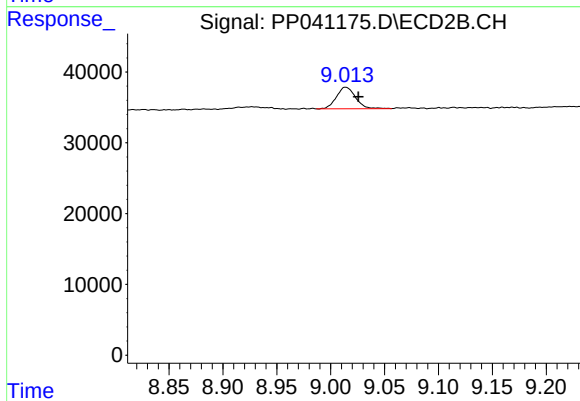

#2 Decachlorobiphenyl


R.T.: 9.014 min
Delta R.T.: -0.012 min
Response: 37654
Conc: 2.63 ng/ml

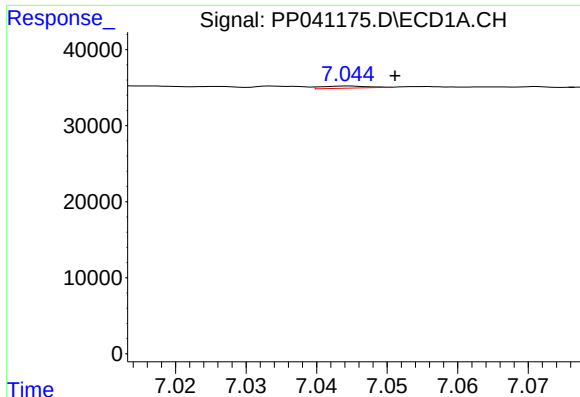

#20 AR-1242-5


R.T.: 7.045 min
Delta R.T.: -0.007 min
Response: 1266
Conc: 2.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4B

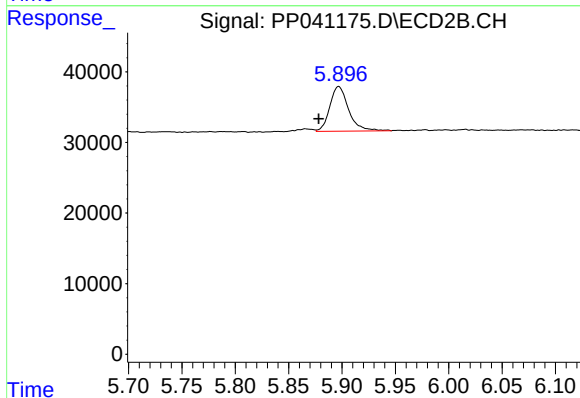


#20 AR-1242-5

R.T.: 5.897 min
Delta R.T.: 0.019 min
Response: 77571
Conc: 143.67 ng/ml

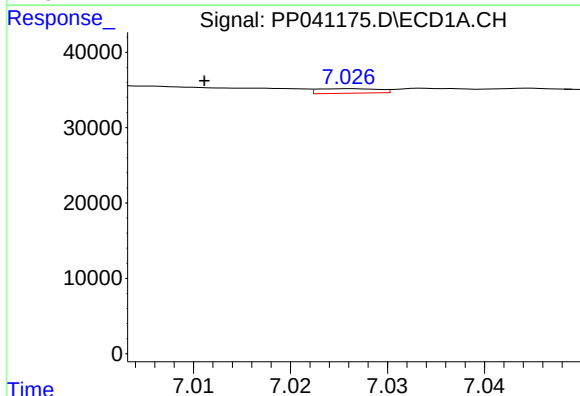


#24 AR-1248-4

R.T.: 7.026 min
Delta R.T.: 0.015 min
Response: 2645
Conc: 3.54 ng/ml

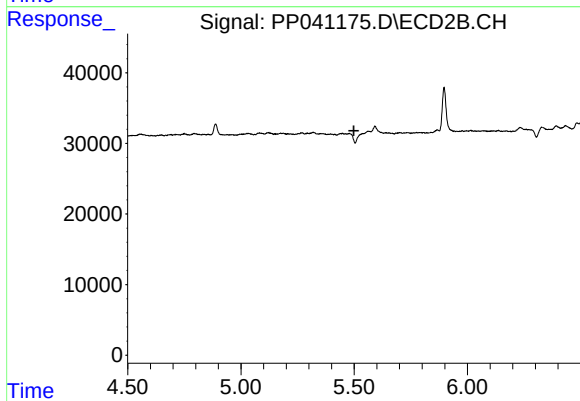

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.498 min
Response: 0
Conc: N.D.

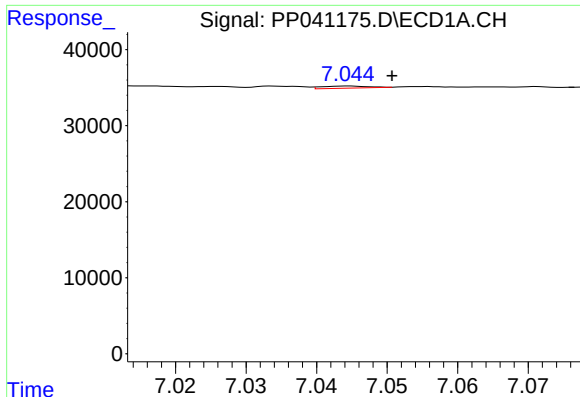

#25 AR-1248-5


R.T.: 7.045 min
Delta R.T.: -0.006 min
Response: 1266
Conc: 1.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4B

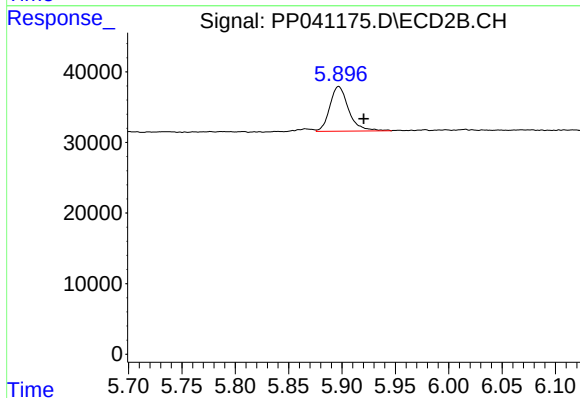


#25 AR-1248-5

R.T.: 5.897 min
Delta R.T.: -0.024 min
Response: 77571
Conc: 107.15 ng/ml

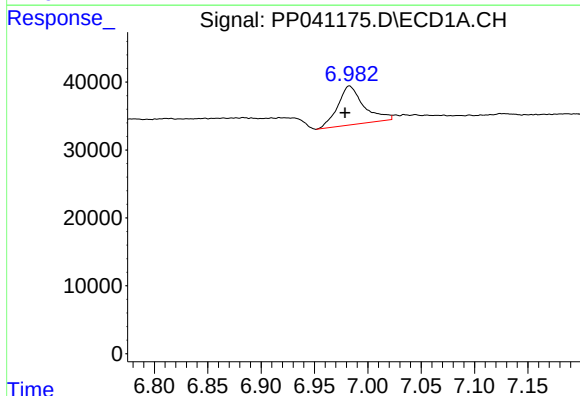


#26 AR-1254-1

R.T.: 6.983 min
Delta R.T.: 0.004 min
Response: 97507
Conc: 126.26 ng/ml

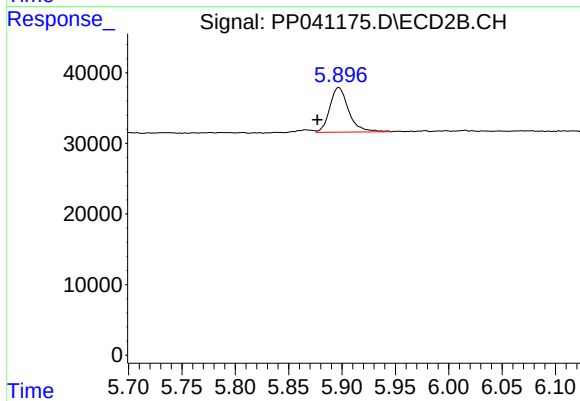

#26 AR-1254-1


R.T.: 5.897 min
Delta R.T.: 0.020 min
Response: 77571
Conc: 68.12 ng/ml

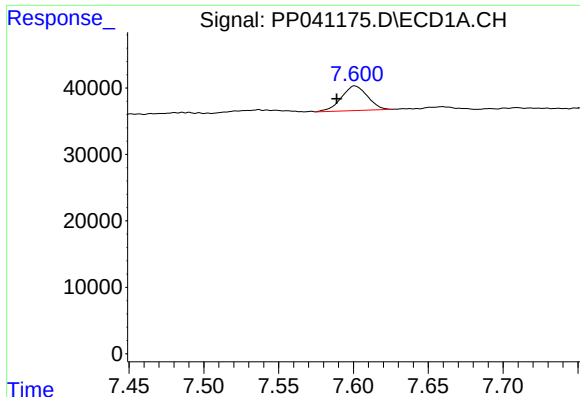

#28 AR-1254-3


R.T.: 7.601 min
Delta R.T.: 0.012 min
Response: 44743
Conc: 33.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4B

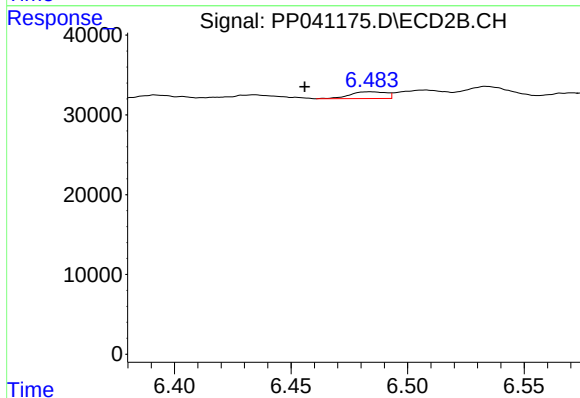


#28 AR-1254-3

R.T.: 6.484 min
Delta R.T.: 0.028 min
Response: 9170
Conc: 6.34 ng/ml

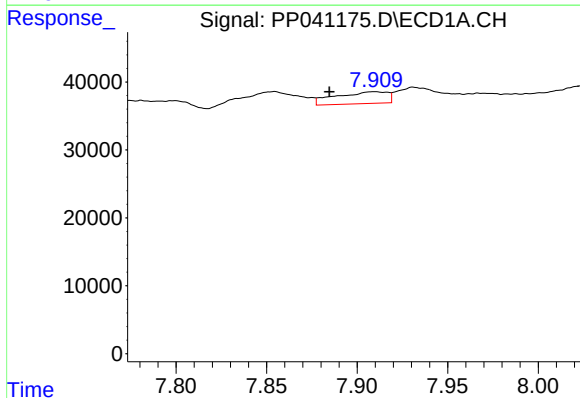


#29 AR-1254-4

R.T.: 7.910 min
Delta R.T.: 0.025 min
Response: 34714
Conc: 36.38 ng/ml

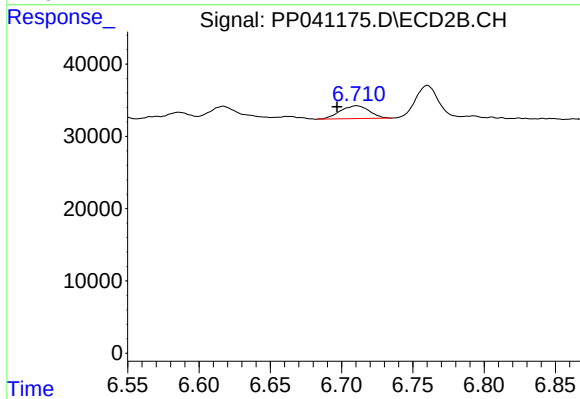

#29 AR-1254-4


R.T.: 6.711 min
Delta R.T.: 0.014 min
Response: 25297
Conc: 30.50 ng/ml

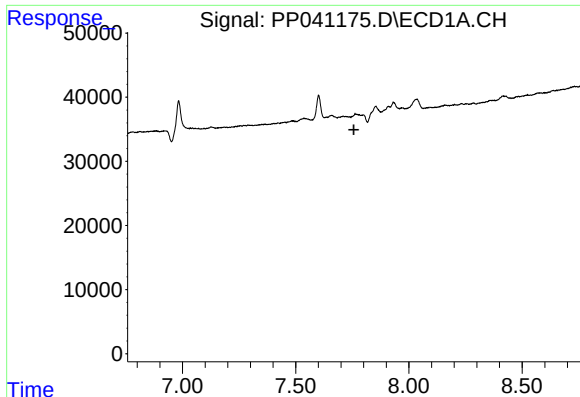

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LAW-2021-4B

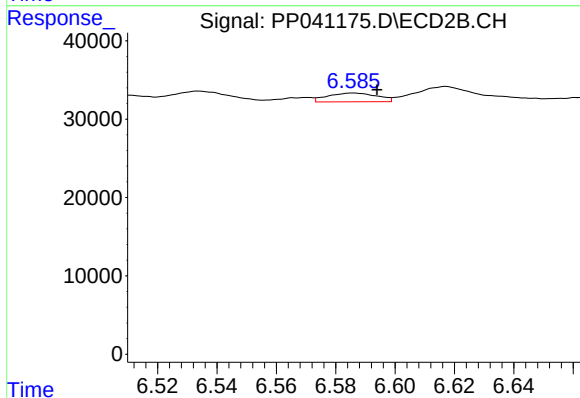


#31 AR-1260-1

R.T.: 6.586 min
Delta R.T.: -0.008 min
Response: 12824
Conc: 13.39 ng/ml

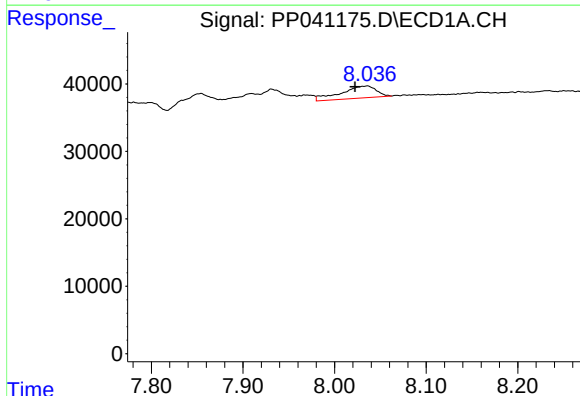

#32 AR-1260-2

R.T.: 8.036 min
Delta R.T.: 0.014 min
Response: 48318
Conc: 40.89 ng/ml

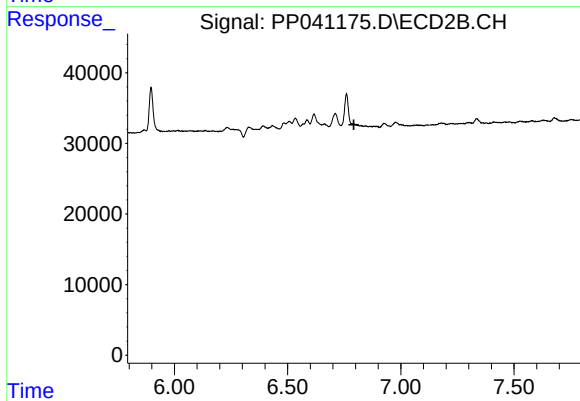

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.793 min
Response: 0
Conc: N.D.