

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041176.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 10:49
 Operator : AJ\MA
 Sample : M4728-03 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2021-5A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:38:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.753	3.757	31891	50027	1.512	1.800
2)	SA Decachlor...	10.647	9.014	55744	33757	2.552	2.355
Target Compounds							
20)	L4 AR-1242-5	7.034f	5.897f	2028	67898	4.537	125.758 #
24)	L5 AR-1248-4	7.026f	0.000	1874	0	2.512	N.D. #
25)	L5 AR-1248-5	7.034f	5.897f	2028	67898	2.682	93.786 #
26)	L6 AR-1254-1	6.984	5.897f	76890	67898	99.563	59.626 #
28)	L6 AR-1254-3	7.602	0.000	30855	0	23.042	N.D. #
29)	L6 AR-1254-4	7.910f	0.000	22944	0	24.042	N.D. #
32)	L7 AR-1260-2	7.993f	0.000	3500	0	2.961	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 10:49
Operator : AJ\MA
Sample : M4728-03 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:38:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

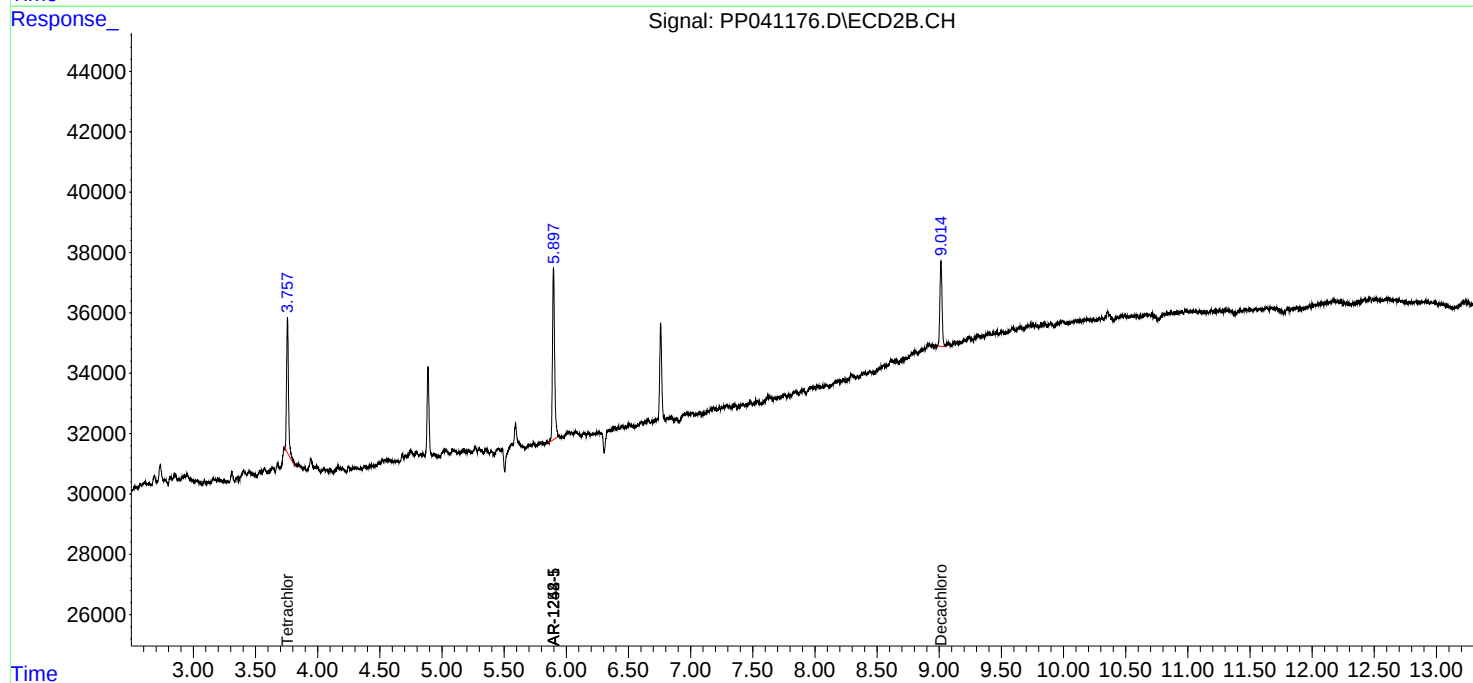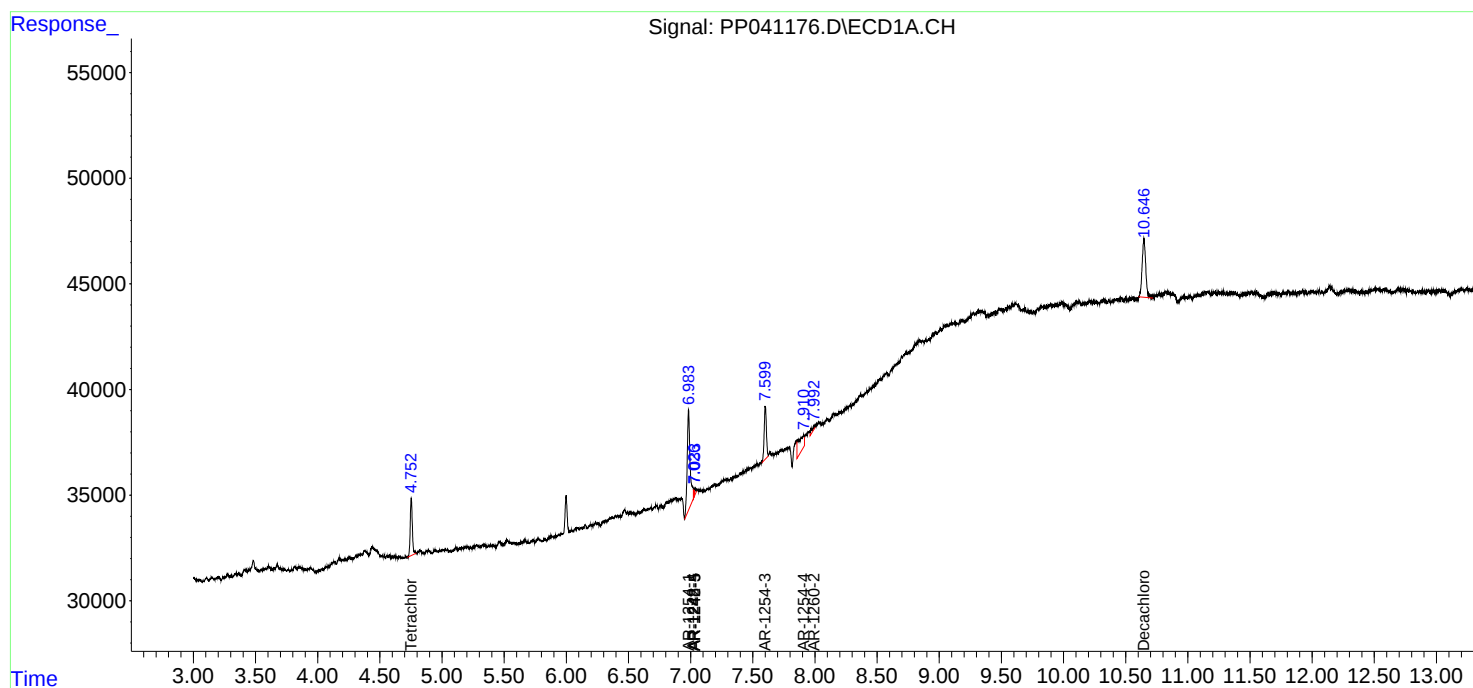


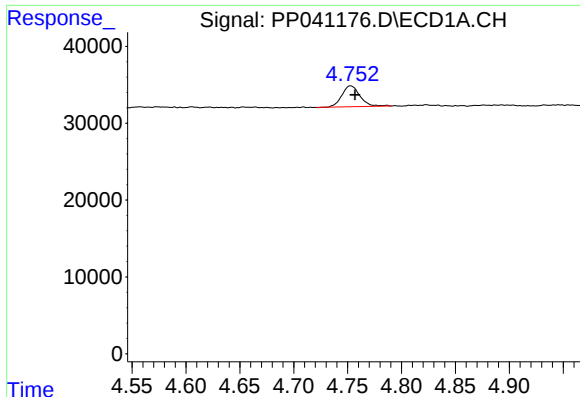

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.004 min
Response: 31891
Conc: 1.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5A

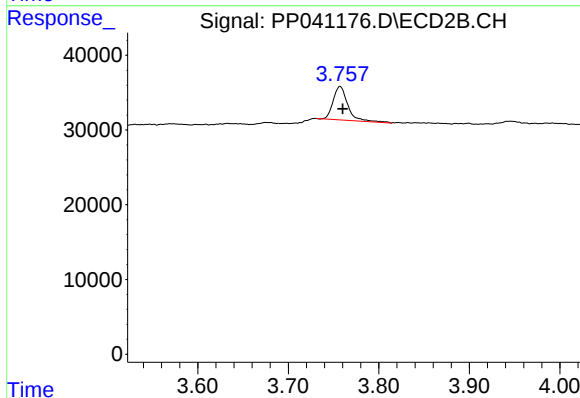


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 50027
Conc: 1.80 ng/ml

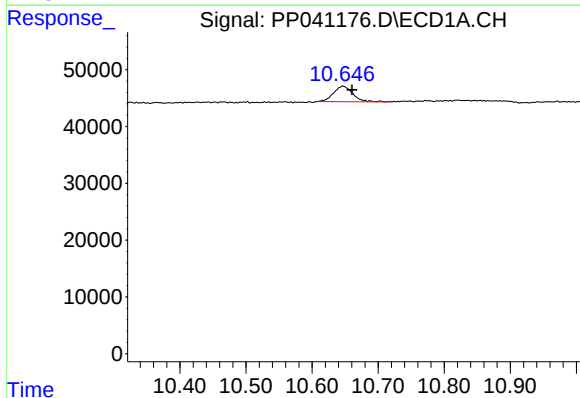


#2 Decachlorobiphenyl

R.T.: 10.647 min
Delta R.T.: -0.014 min
Response: 55744
Conc: 2.55 ng/ml

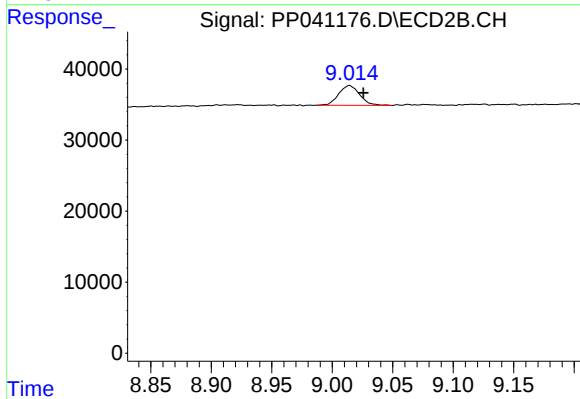

#2 Decachlorobiphenyl


R.T.: 9.014 min
Delta R.T.: -0.012 min
Response: 33757
Conc: 2.35 ng/ml

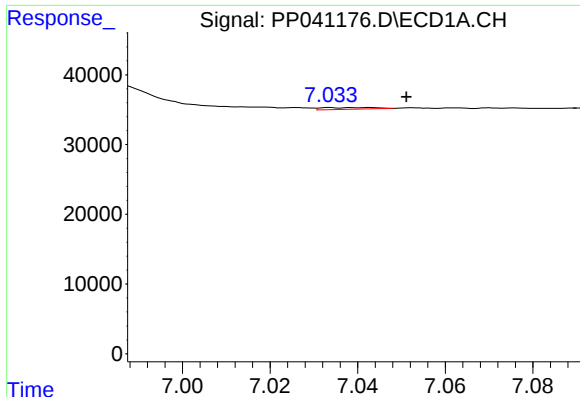

#20 AR-1242-5


R.T.: 7.034 min
Delta R.T.: -0.017 min
Response: 2028
Conc: 4.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5A

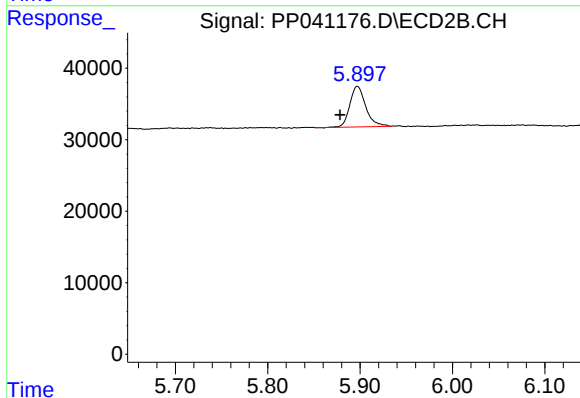


#20 AR-1242-5

R.T.: 5.897 min
Delta R.T.: 0.019 min
Response: 67898
Conc: 125.76 ng/ml

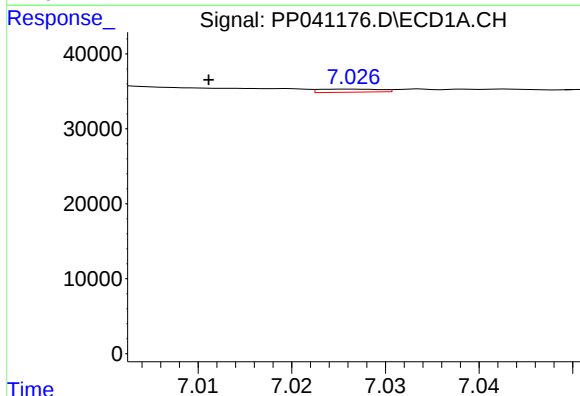


#24 AR-1248-4

R.T.: 7.026 min
Delta R.T.: 0.015 min
Response: 1874
Conc: 2.51 ng/ml

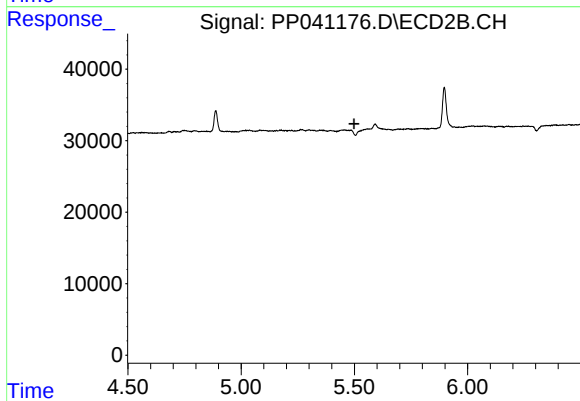

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.498 min
Response: 0
Conc: N.D.

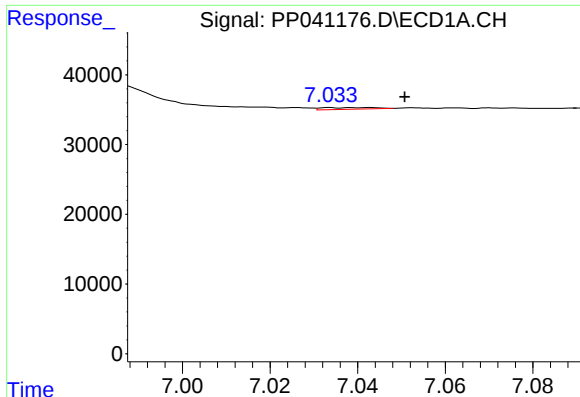

#25 AR-1248-5


R.T.: 7.034 min
Delta R.T.: -0.017 min
Response: 2028
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5A

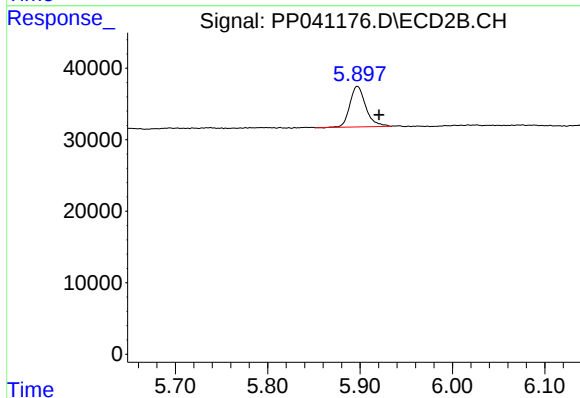


#25 AR-1248-5

R.T.: 5.897 min
Delta R.T.: -0.023 min
Response: 67898
Conc: 93.79 ng/ml

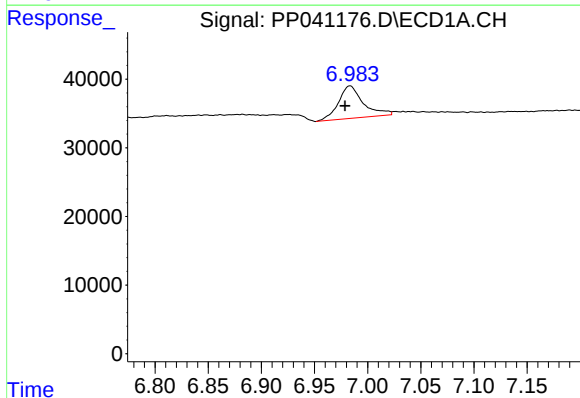


#26 AR-1254-1

R.T.: 6.984 min
Delta R.T.: 0.005 min
Response: 76890
Conc: 99.56 ng/ml

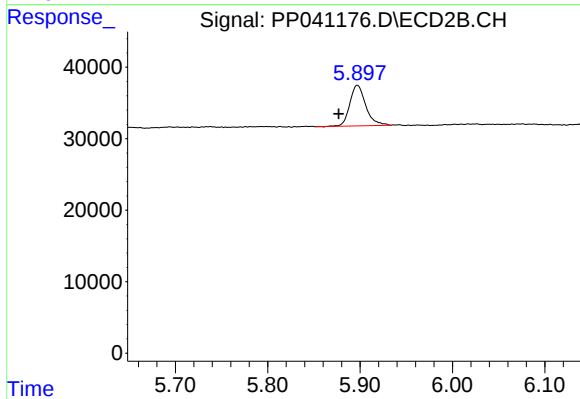

#26 AR-1254-1


R.T.: 5.897 min
Delta R.T.: 0.020 min
Response: 67898
Conc: 59.63 ng/ml

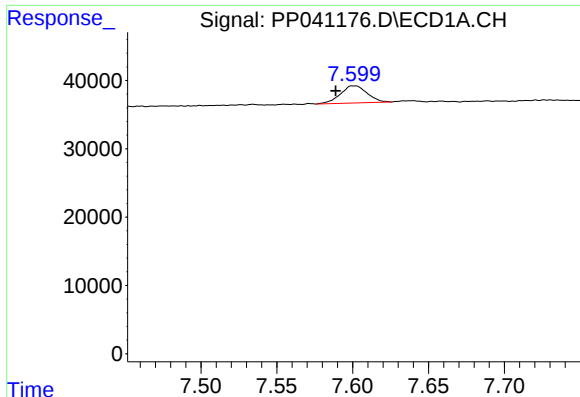

#28 AR-1254-3


R.T.: 7.602 min
Delta R.T.: 0.013 min
Response: 30855
Conc: 23.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5A

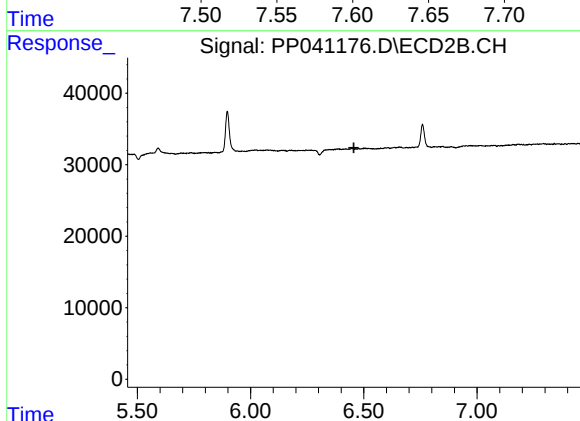


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

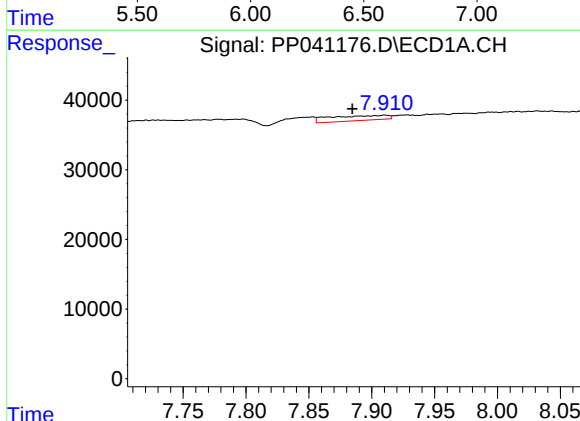


#29 AR-1254-4

R.T.: 7.910 min
Delta R.T.: 0.026 min
Response: 22944
Conc: 24.04 ng/ml

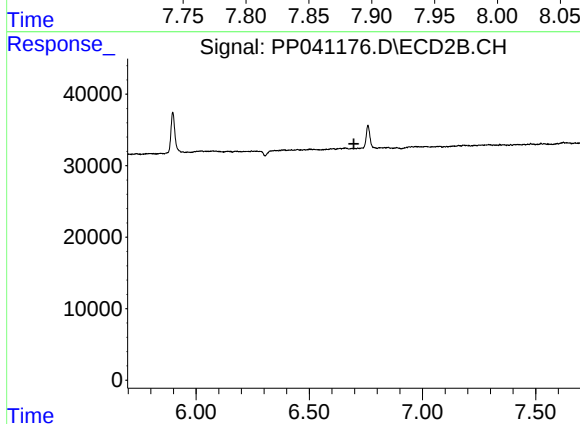

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.697 min
Response: 0
Conc: N.D.

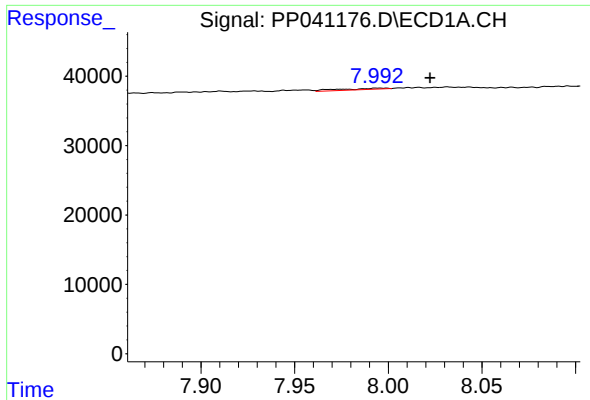

#32 AR-1260-2

R.T.: 7.993 min
Delta R.T.: -0.029 min
Response: 3500
Conc: 2.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5A

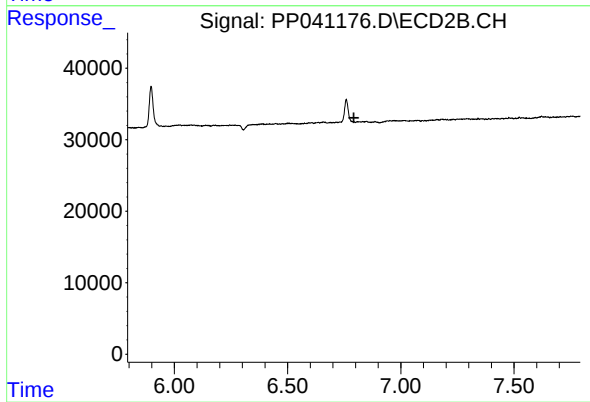

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.793 min
Response: 0
Conc: N.D.