

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041177.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 11:06
 Operator : AJ\MA
 Sample : M4728-04 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2021-5B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:38:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	3.757	37430	58578	1.775	2.108
2) SA Decachlor...	10.646	9.015	65046	38275	2.978	2.670
Target Compounds						
20) L4 AR-1242-5	7.021f	5.897f	1317	60973	2.946	112.932 #
24) L5 AR-1248-4	7.021	0.000	1317	0	1.765	N.D. #
25) L5 AR-1248-5	7.021f	5.897f	1317	60973	1.742	84.222 #
26) L6 AR-1254-1	6.983	5.897f	61083	60973	79.096	53.546 #
28) L6 AR-1254-3	7.601	0.000	25833	0	19.292	N.D. #
29) L6 AR-1254-4	7.856f	0.000	4578	0	4.797	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041177.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 11:06
Operator : AJ\MA
Sample : M4728-04 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:38:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

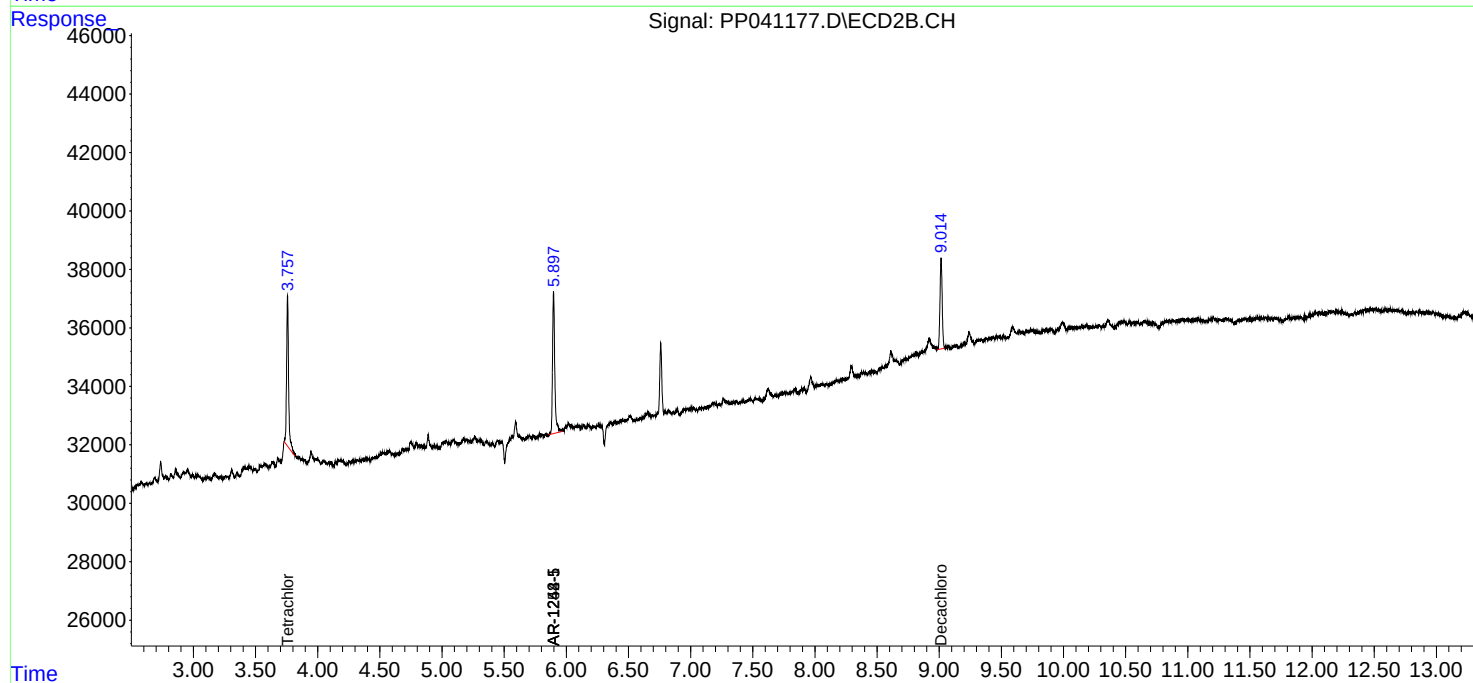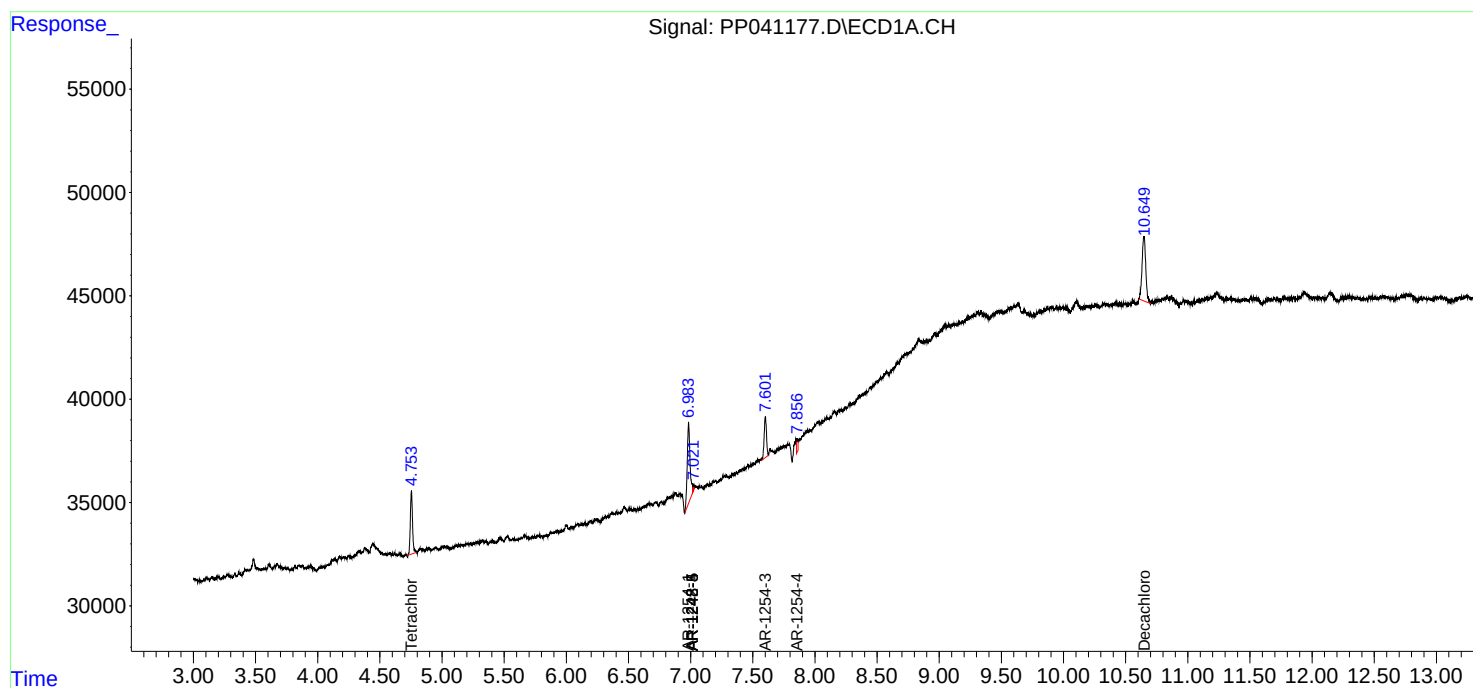


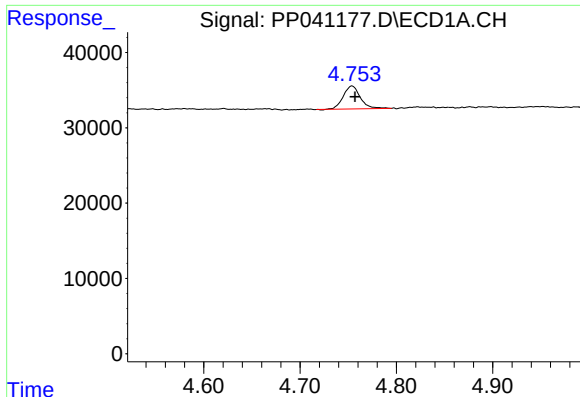

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 37430
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B

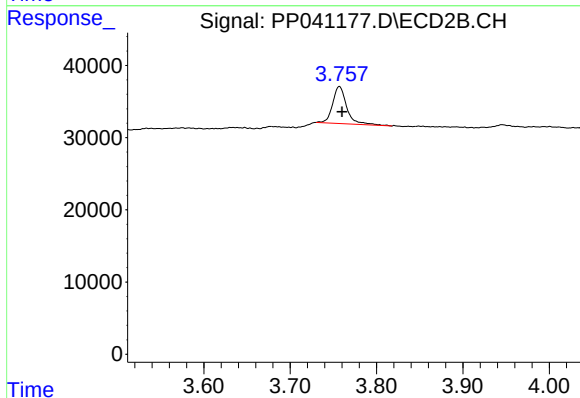


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 58578
Conc: 2.11 ng/ml

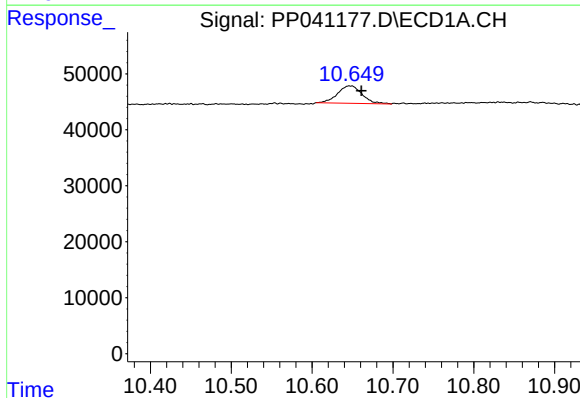


#2 Decachlorobiphenyl

R.T.: 10.646 min
Delta R.T.: -0.015 min
Response: 65046
Conc: 2.98 ng/ml

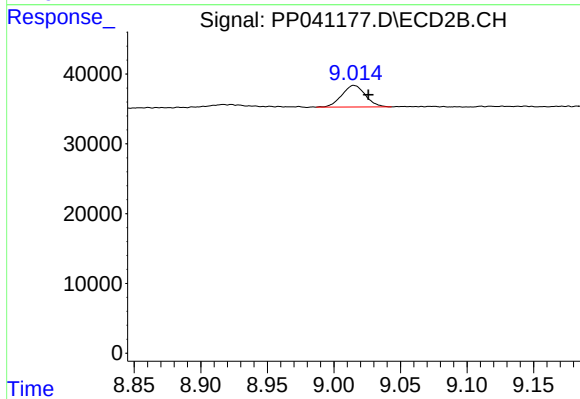

#2 Decachlorobiphenyl


R.T.: 9.015 min
Delta R.T.: -0.011 min
Response: 38275
Conc: 2.67 ng/ml

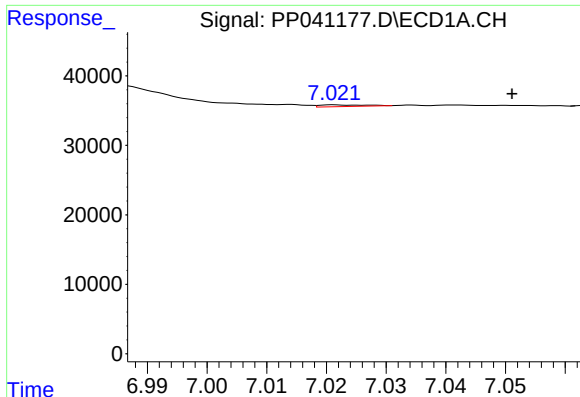

#20 AR-1242-5


R.T.: 7.021 min
Delta R.T.: -0.030 min
Response: 1317
Conc: 2.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B

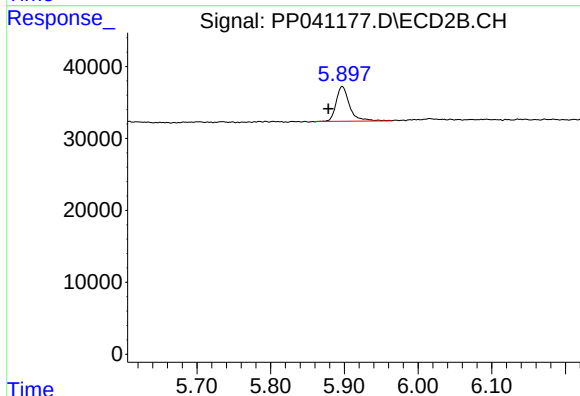


#20 AR-1242-5

R.T.: 5.897 min
Delta R.T.: 0.019 min
Response: 60973
Conc: 112.93 ng/ml

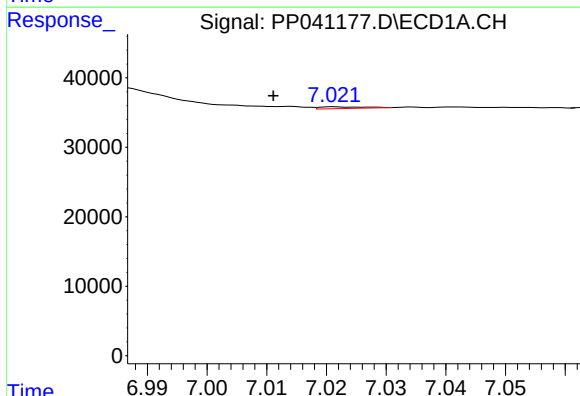


#24 AR-1248-4

R.T.: 7.021 min
Delta R.T.: 0.010 min
Response: 1317
Conc: 1.77 ng/ml

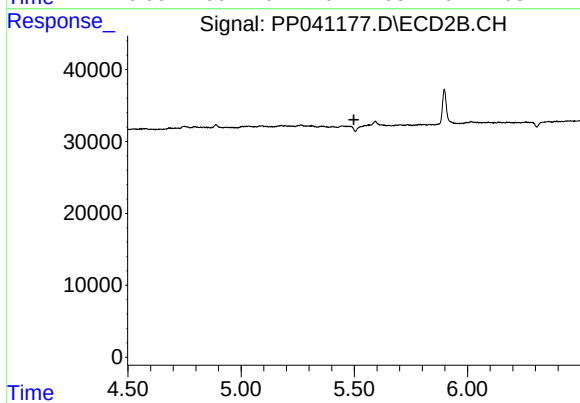

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.498 min
Response: 0
Conc: N.D.

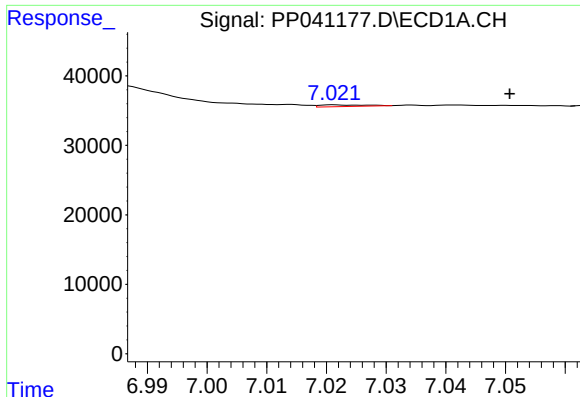

#25 AR-1248-5


R.T.: 7.021 min
Delta R.T.: -0.029 min
Response: 1317
Conc: 1.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B

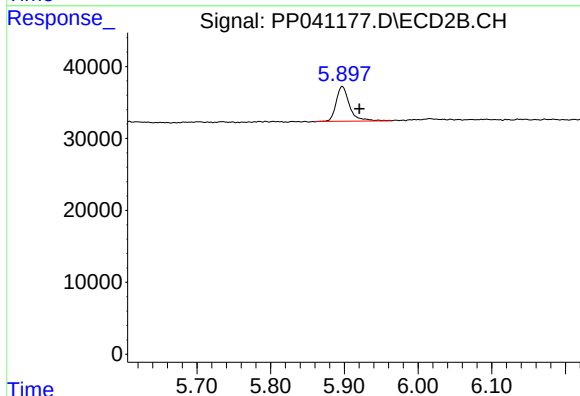


#25 AR-1248-5

R.T.: 5.897 min
Delta R.T.: -0.023 min
Response: 60973
Conc: 84.22 ng/ml

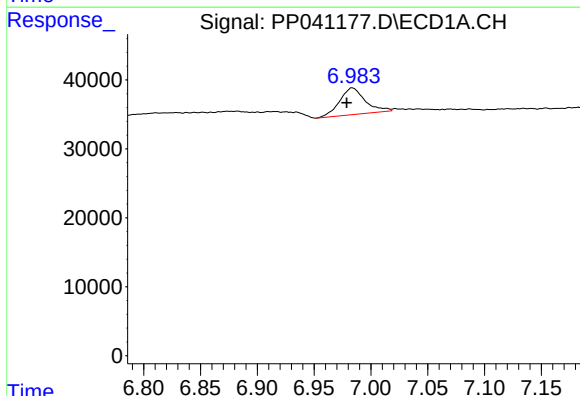


#26 AR-1254-1

R.T.: 6.983 min
Delta R.T.: 0.005 min
Response: 61083
Conc: 79.10 ng/ml

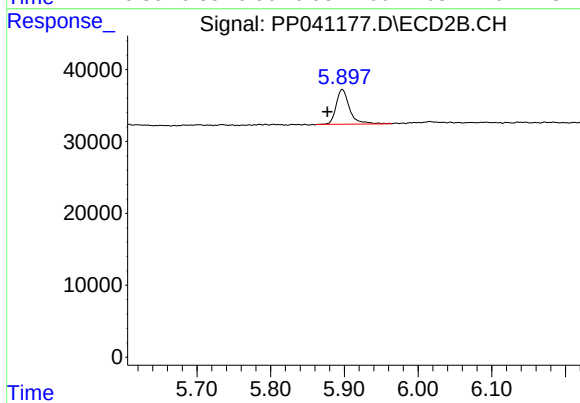

#26 AR-1254-1


R.T.: 5.897 min
Delta R.T.: 0.020 min
Response: 60973
Conc: 53.55 ng/ml

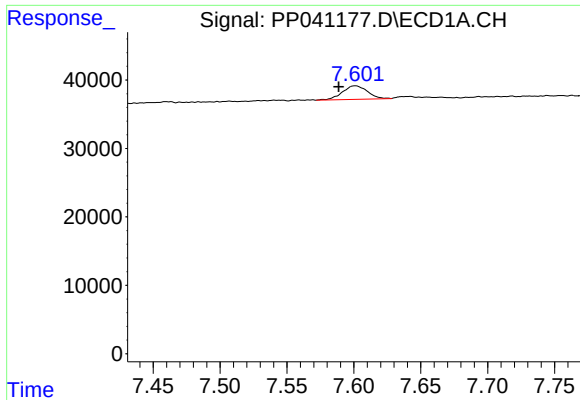

#28 AR-1254-3


R.T.: 7.601 min
Delta R.T.: 0.012 min
Response: 25833
Conc: 19.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B

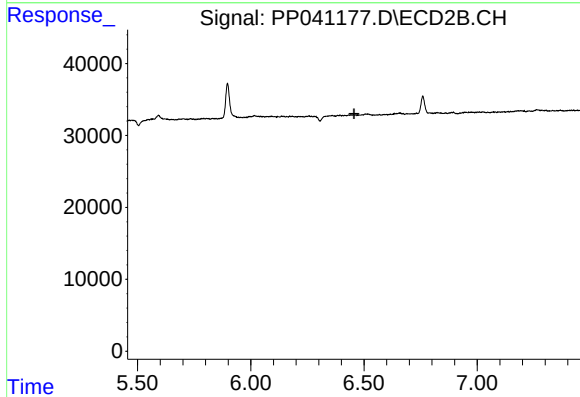


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

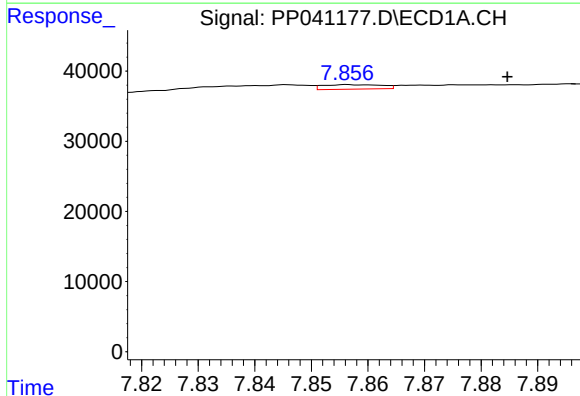

#29 AR-1254-4

R.T.: 7.856 min
Delta R.T.: -0.028 min
Response: 4578
Conc: 4.80 ng/ml

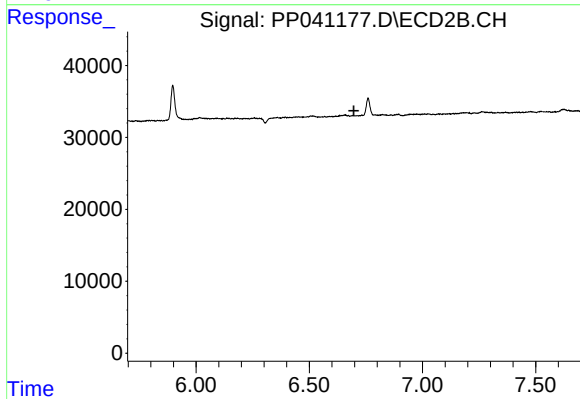

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.697 min
Response: 0
Conc: N.D.