

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041178.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 11:23
 Operator : AJ\MA
 Sample : M4728-05 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2021-5C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:38:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.754	3.757	33658	50915	1.596	1.832
2)	SA Decachlor...	10.649	9.014	49459	36210	2.264	2.526
Target Compounds							
20)	L4 AR-1242-5	7.030f	5.898f	1443	59690	3.228	110.555 #
24)	L5 AR-1248-4	7.018	0.000	1585	0	2.124	N.D. #
25)	L5 AR-1248-5	7.030f	5.898f	1443	59690	1.909	82.449 #
26)	L6 AR-1254-1	6.983	5.898f	64755	59690	83.851	52.418 #
28)	L6 AR-1254-3	7.601	0.000	34039	0	25.420	N.D. #
29)	L6 AR-1254-4	7.880	6.712	2697	14982	2.826	18.061 #
31)	L7 AR-1260-1	0.000	6.617f	0	15894	N.D.	16.603 #
32)	L7 AR-1260-2	8.037	0.000	19178	0	16.228	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041178.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 11:23
Operator : AJ\MA
Sample : M4728-05 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:38:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

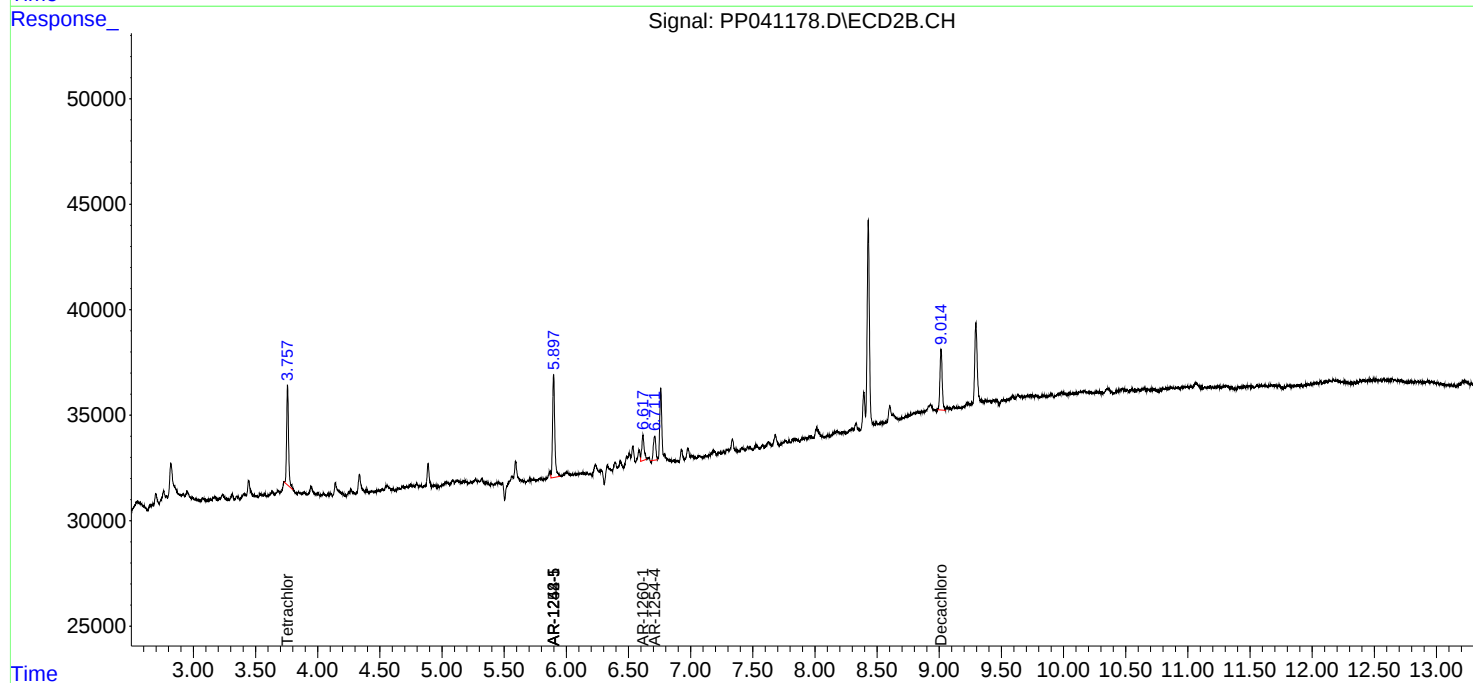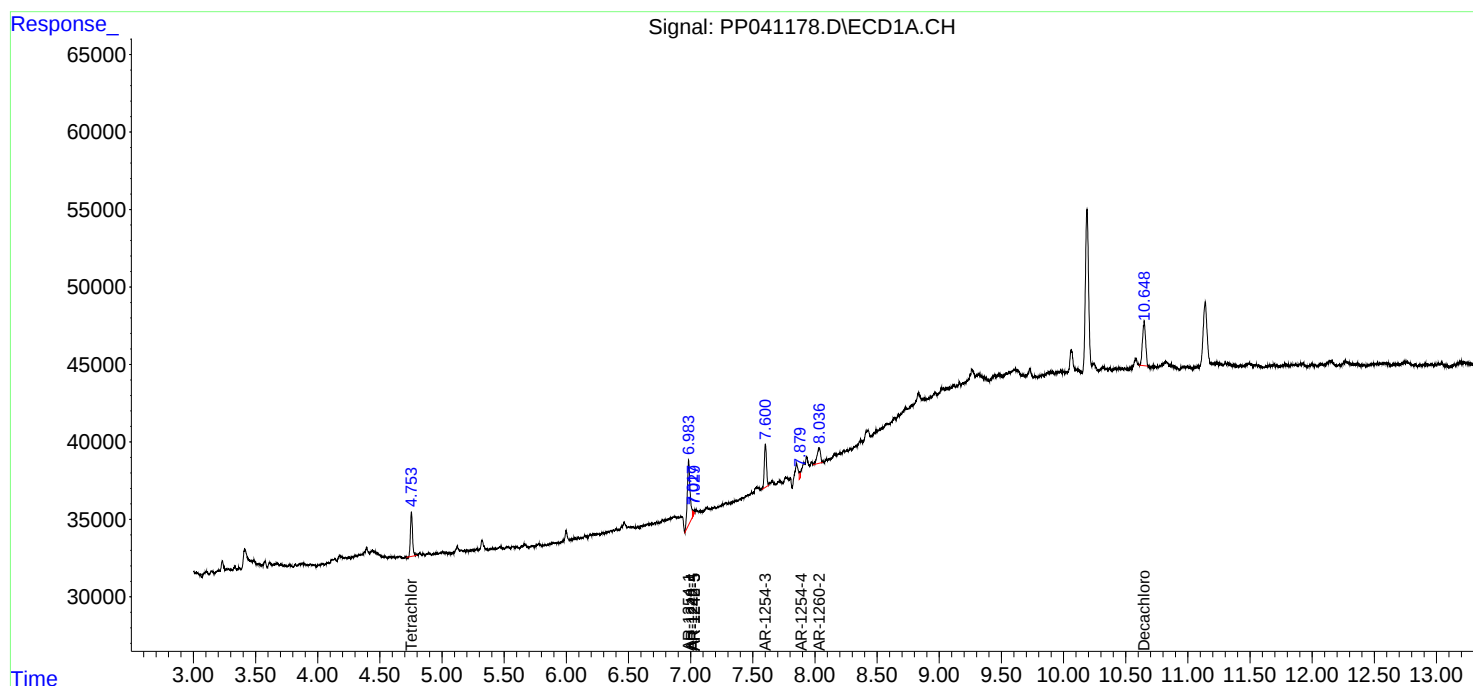


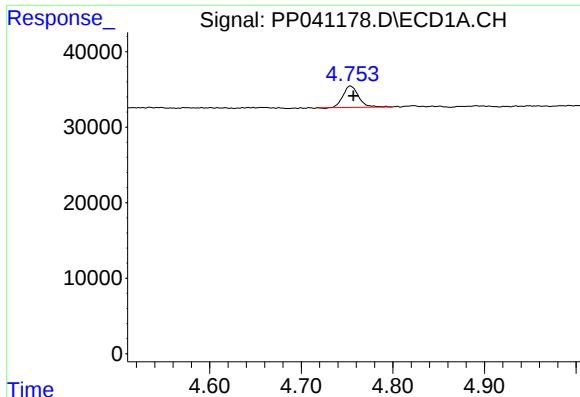

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 33658
Conc: 1.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5C

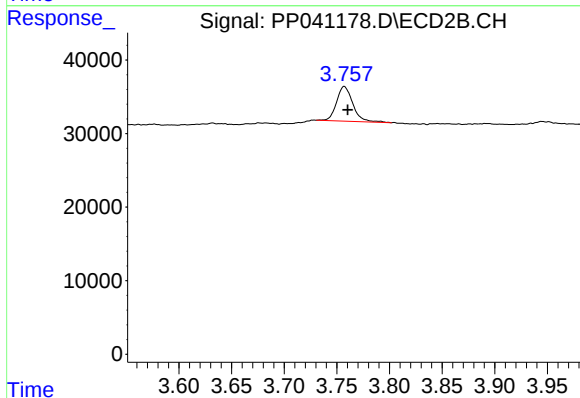


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 50915
Conc: 1.83 ng/ml

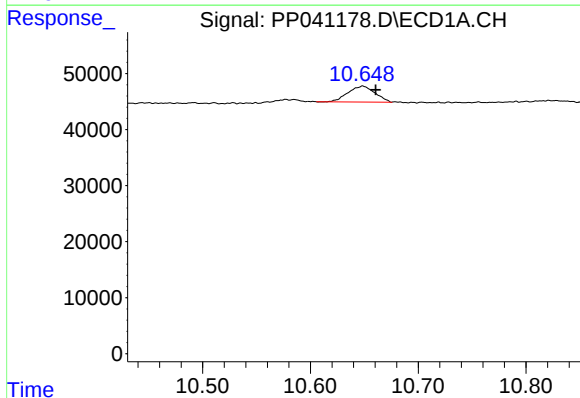


#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.012 min
Response: 49459
Conc: 2.26 ng/ml

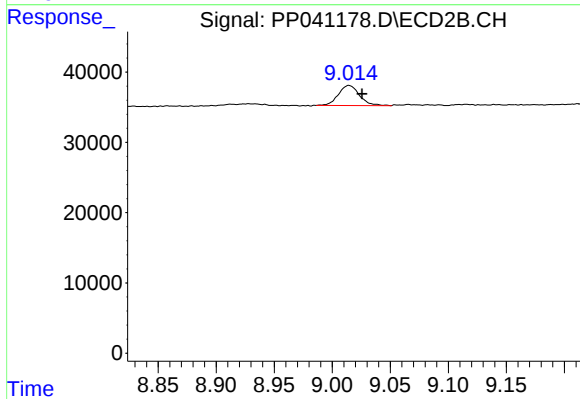

#2 Decachlorobiphenyl


R.T.: 9.014 min
Delta R.T.: -0.011 min
Response: 36210
Conc: 2.53 ng/ml

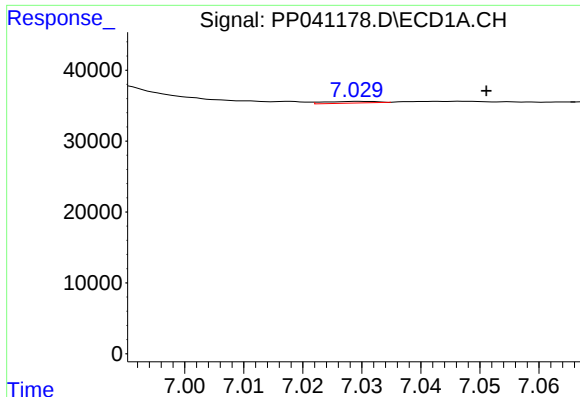

#20 AR-1242-5


R.T.: 7.030 min
Delta R.T.: -0.022 min
Response: 1443
Conc: 3.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5C

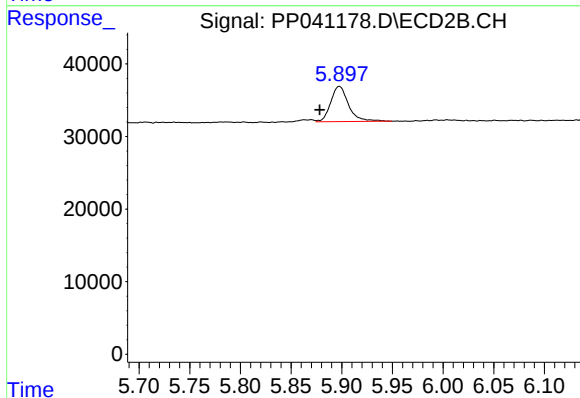


#20 AR-1242-5

R.T.: 5.898 min
Delta R.T.: 0.020 min
Response: 59690
Conc: 110.56 ng/ml

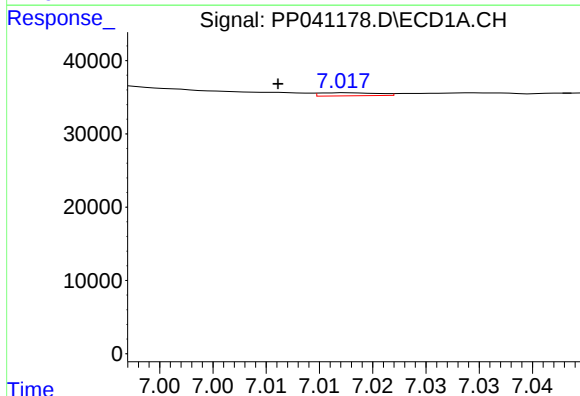


#24 AR-1248-4

R.T.: 7.018 min
Delta R.T.: 0.007 min
Response: 1585
Conc: 2.12 ng/ml

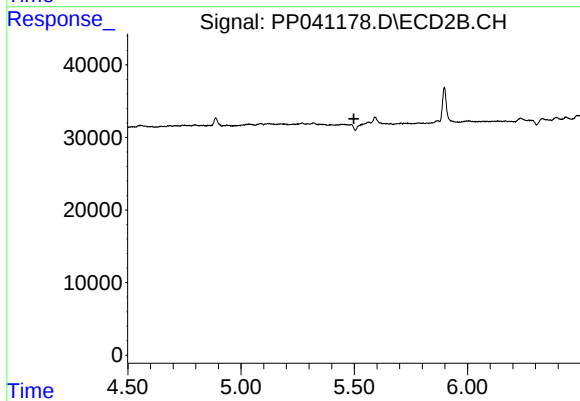

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.498 min
Response: 0
Conc: N.D.

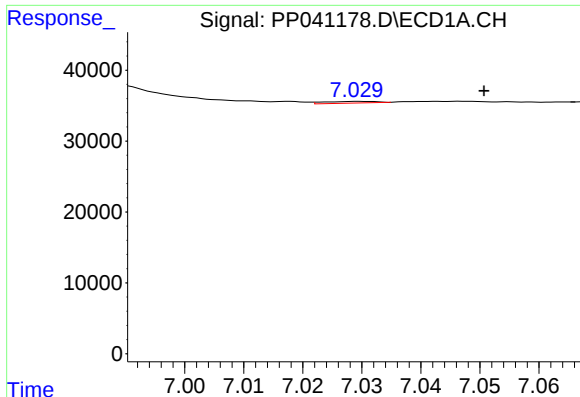

#25 AR-1248-5


R.T.: 7.030 min
Delta R.T.: -0.021 min
Response: 1443
Conc: 1.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5C

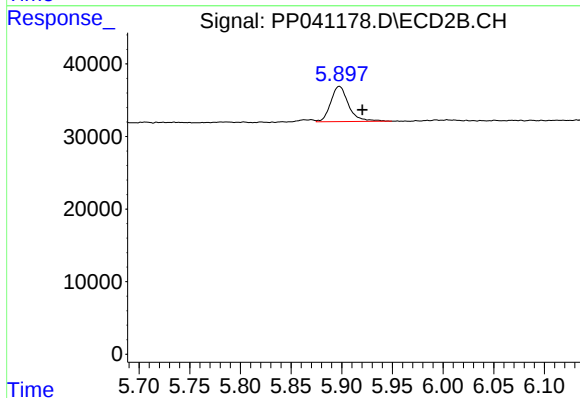


#25 AR-1248-5

R.T.: 5.898 min
Delta R.T.: -0.023 min
Response: 59690
Conc: 82.45 ng/ml

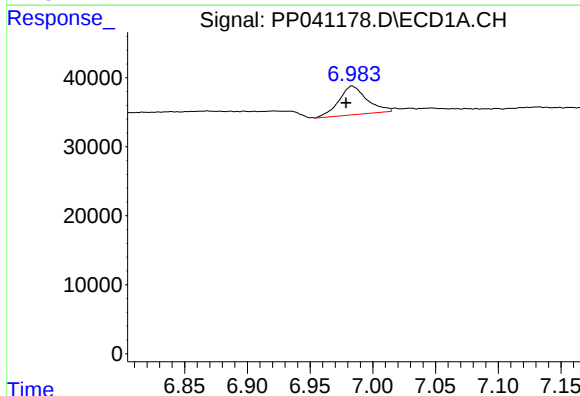


#26 AR-1254-1

R.T.: 6.983 min
Delta R.T.: 0.005 min
Response: 64755
Conc: 83.85 ng/ml

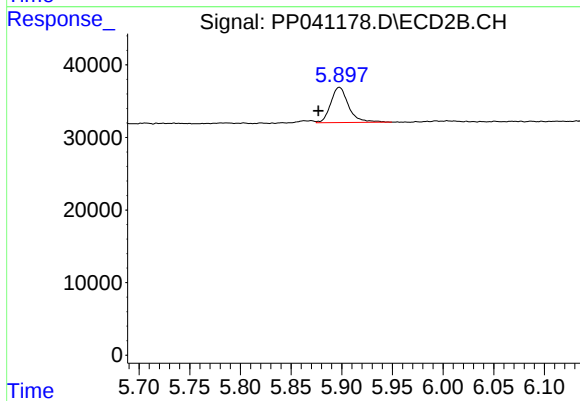

#26 AR-1254-1


R.T.: 5.898 min
Delta R.T.: 0.021 min
Response: 59690
Conc: 52.42 ng/ml

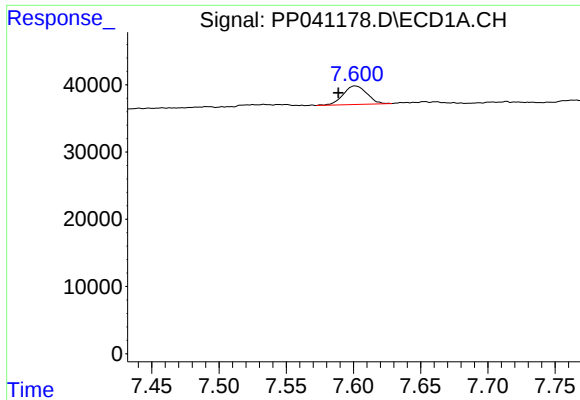

#28 AR-1254-3


R.T.: 7.601 min
Delta R.T.: 0.012 min
Response: 34039
Conc: 25.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5C

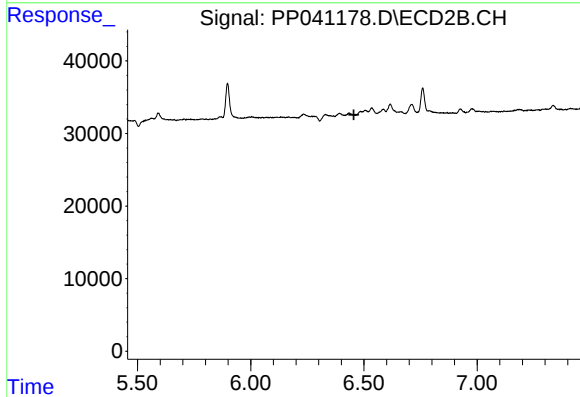


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

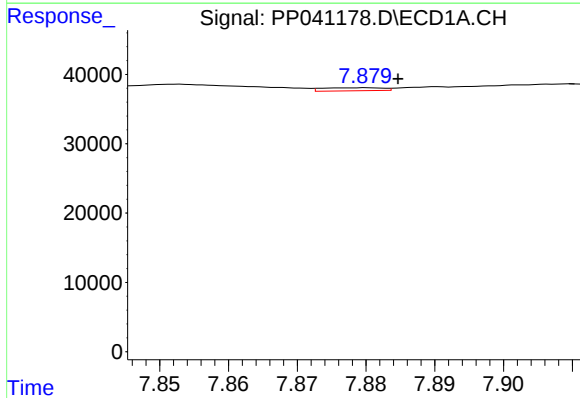


#29 AR-1254-4

R.T.: 7.880 min
Delta R.T.: -0.004 min
Response: 2697
Conc: 2.83 ng/ml

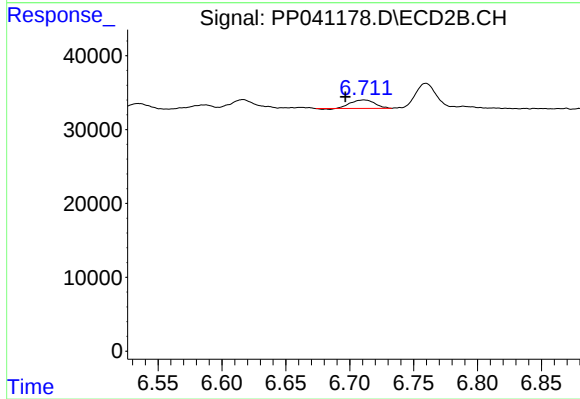

#29 AR-1254-4


R.T.: 6.712 min
Delta R.T.: 0.015 min
Response: 14982
Conc: 18.06 ng/ml

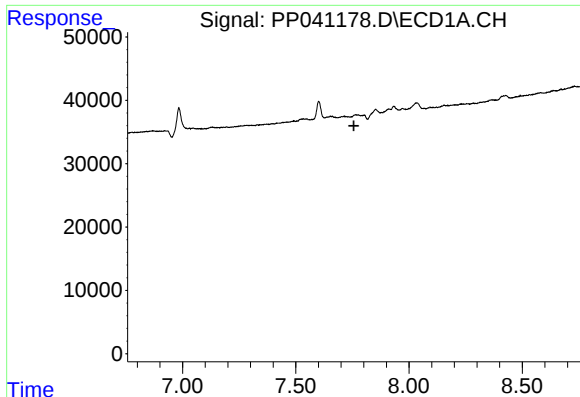

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5C

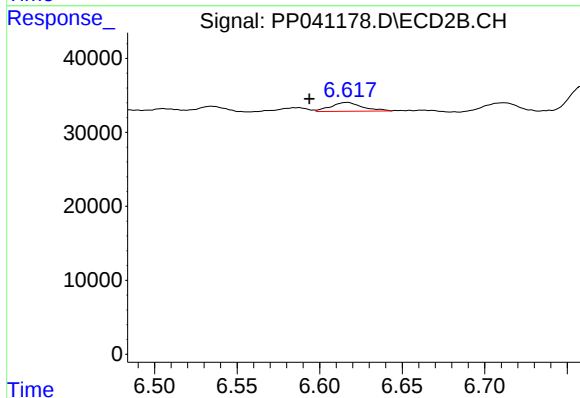


#31 AR-1260-1

R.T.: 6.617 min
Delta R.T.: 0.023 min
Response: 15894
Conc: 16.60 ng/ml

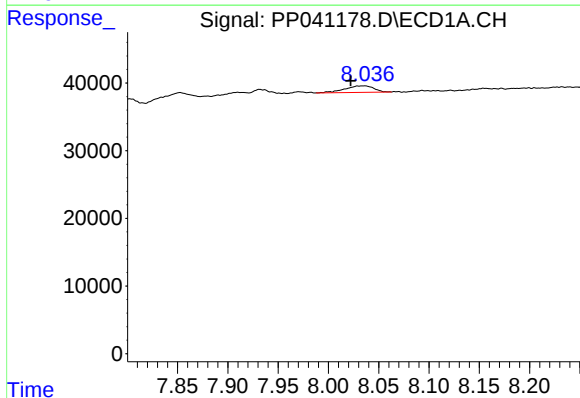

#32 AR-1260-2

R.T.: 8.037 min
Delta R.T.: 0.014 min
Response: 19178
Conc: 16.23 ng/ml

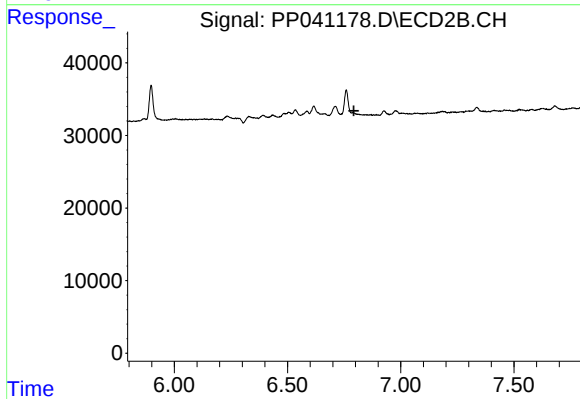

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.793 min
Response: 0
Conc: N.D.