

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041118.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2021 16:28
 Operator : AJ\MA
 Sample : M4765-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:20:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.755	3.758	421452	752675	19.985m	27.084 #
2) SA Decachlor...	10.651	9.018	436407	269630	19.978	18.809

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041118.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2021 16:28
Operator : AJ\MA
Sample : M4765-02
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
WC-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:20:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

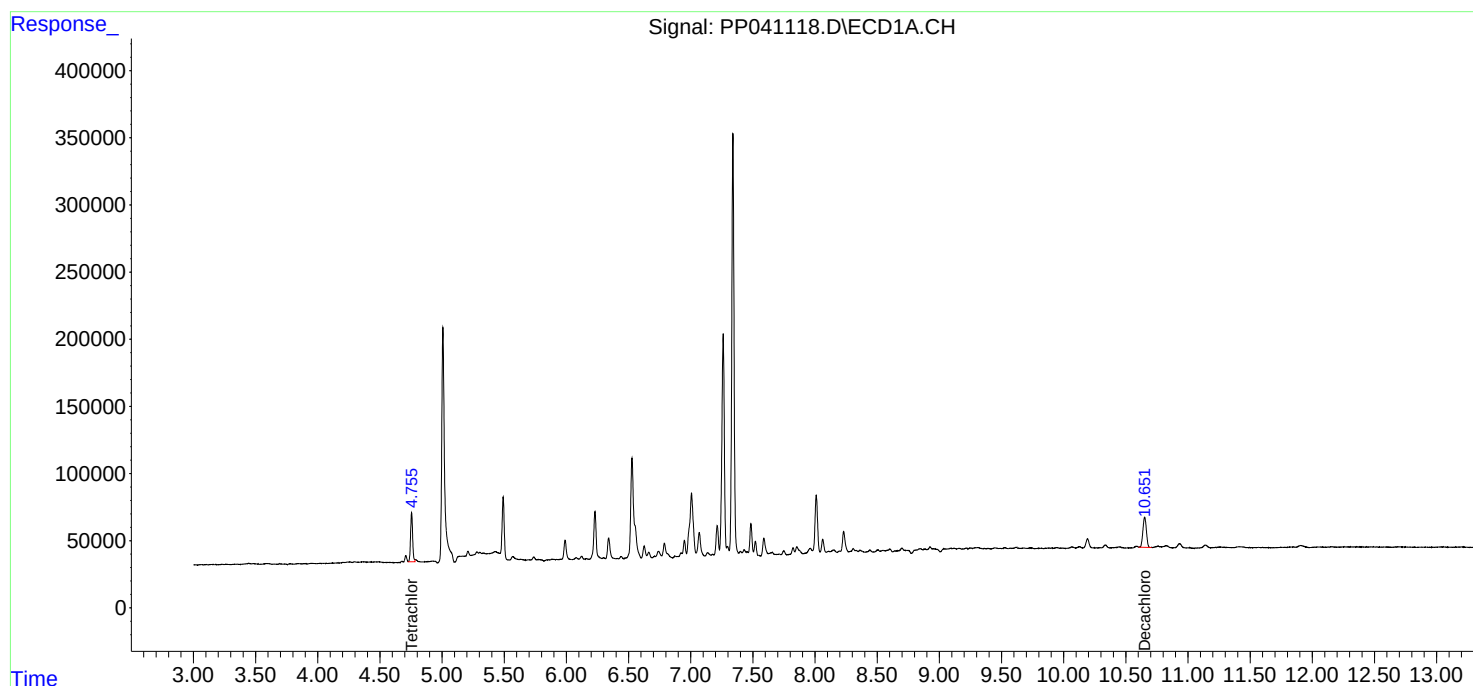

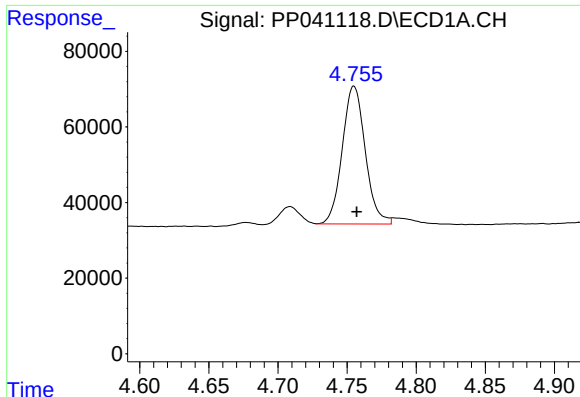


#1 Tetrachloro-m-xylene

R.T.: 4.755 min
Delta R.T.: -0.002 min
Response: 421452
Conc: 19.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

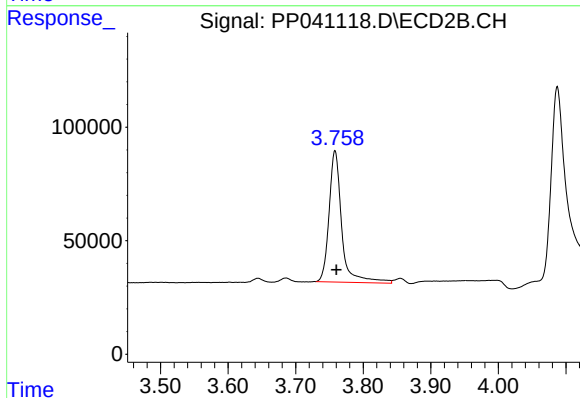


#1 Tetrachloro-m-xylene

R.T.: 3.758 min
Delta R.T.: -0.002 min
Response: 752675
Conc: 27.08 ng/ml

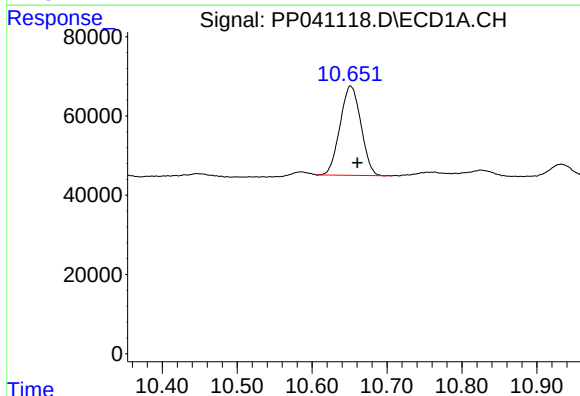

#2 Decachlorobiphenyl

R.T.: 10.651 min
Delta R.T.: -0.009 min
Response: 436407
Conc: 19.98 ng/ml

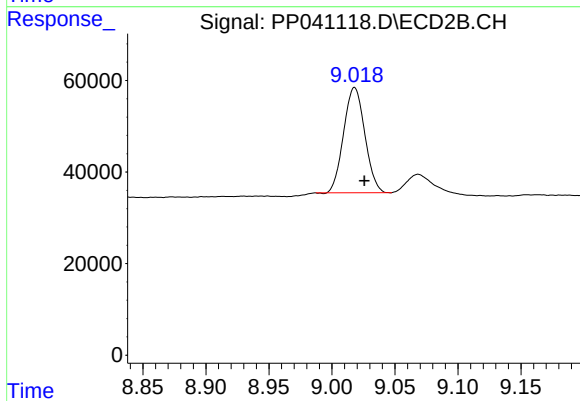

#2 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: -0.008 min
Response: 269630
Conc: 18.81 ng/ml