

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2021 17:18
 Operator : AJ\MA
 Sample : M4766-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-27106

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:21:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	3.761	319825	474326	15.166	17.068
2) SA Decachlor...	10.651	9.019	523590	339689	23.969	23.696
Target Compounds						
26) L6 AR-1254-1	6.977	5.875	23206	36652	30.049m	32.187
27) L6 AR-1254-2	7.206	6.035	40272	35296	32.582	35.997
28) L6 AR-1254-3	7.586	6.451	55502	88163	41.449	60.951 #
29) L6 AR-1254-4	7.881	6.692	27821	23351	29.152	28.151
30) L6 AR-1254-5	8.308	7.120	53442	77086	50.278m	66.131 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2021 17:18
Operator : AJ\MA
Sample : M4766-05
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CHRT-27106


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:21:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

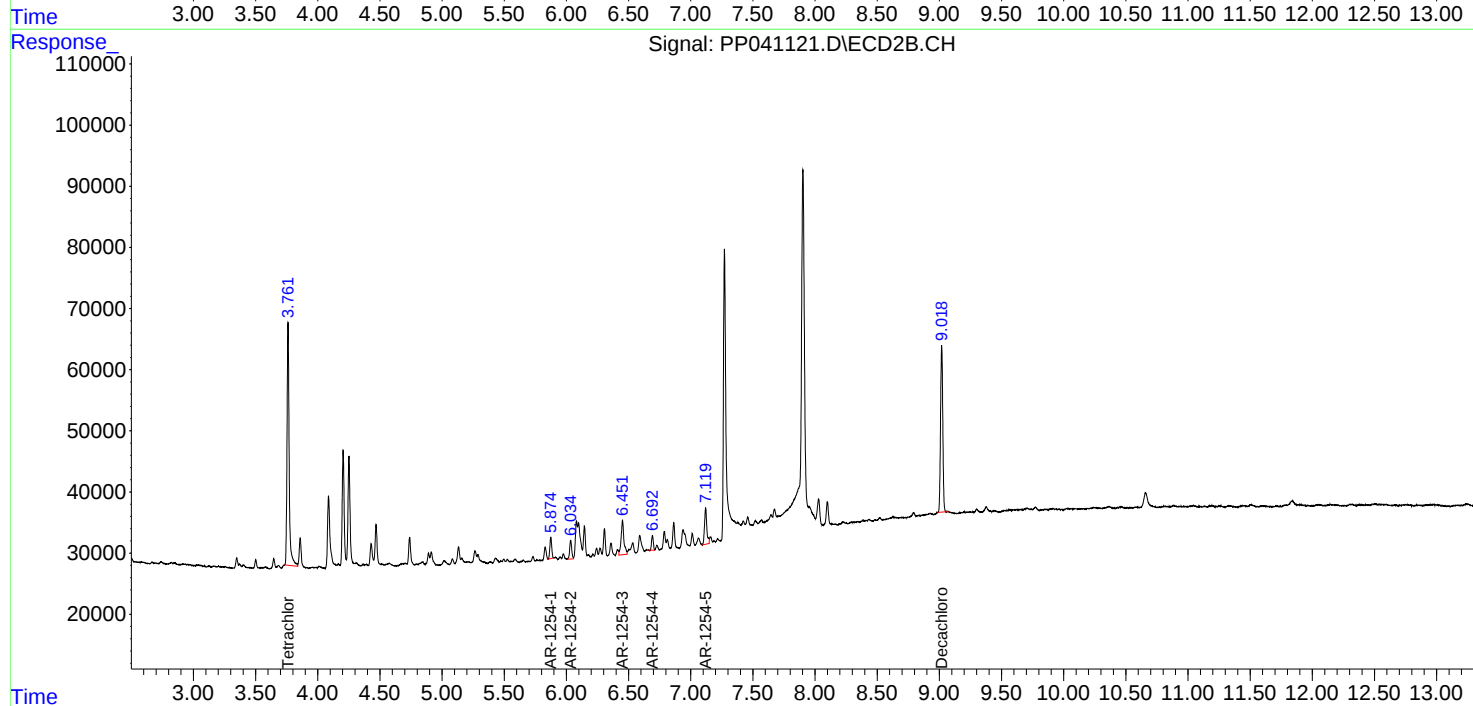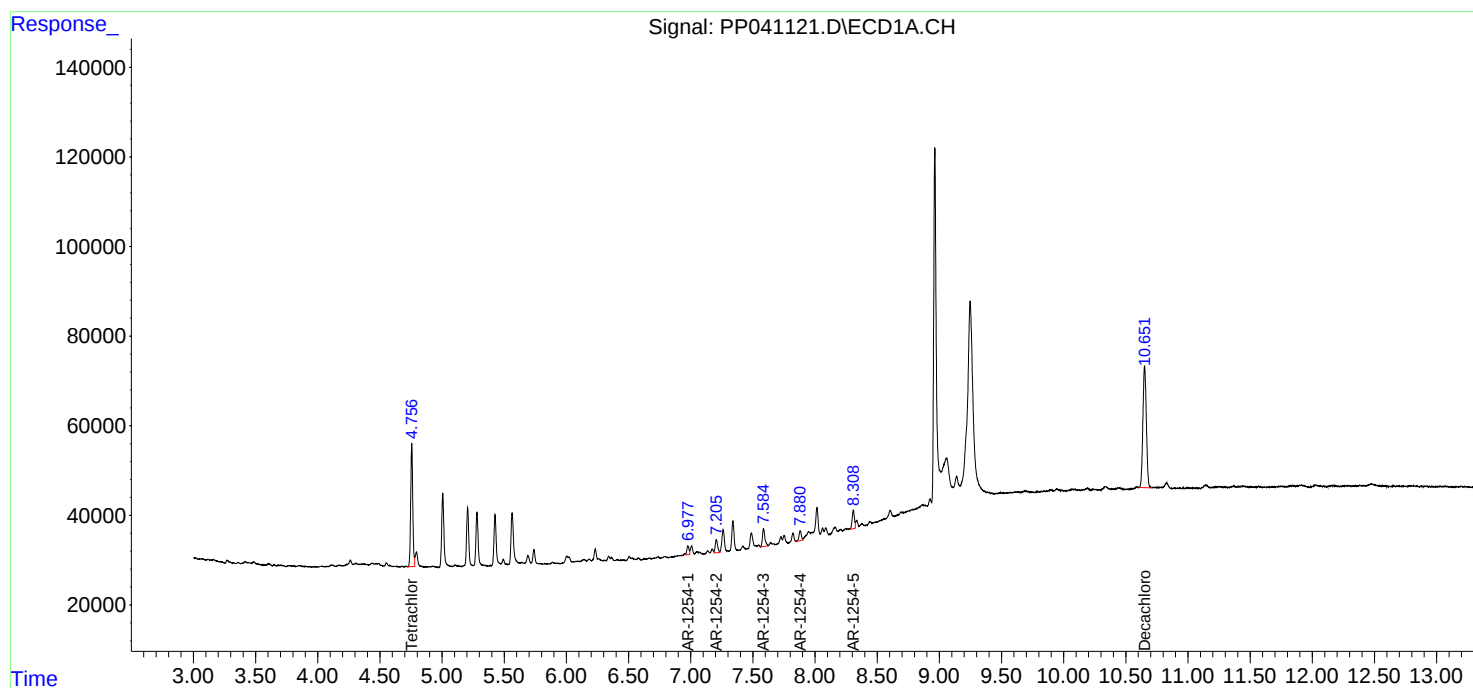

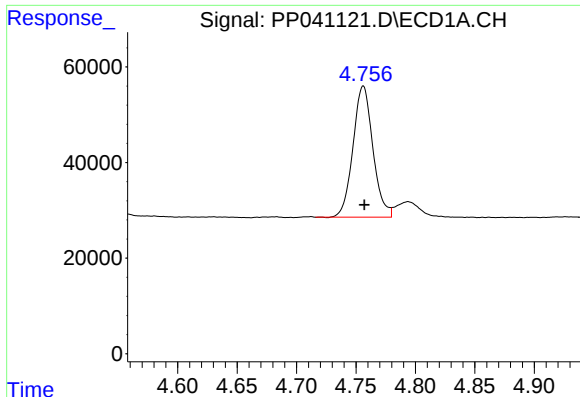


#1 Tetrachloro-m-xylene

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 319825
Conc: 15.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-27106


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

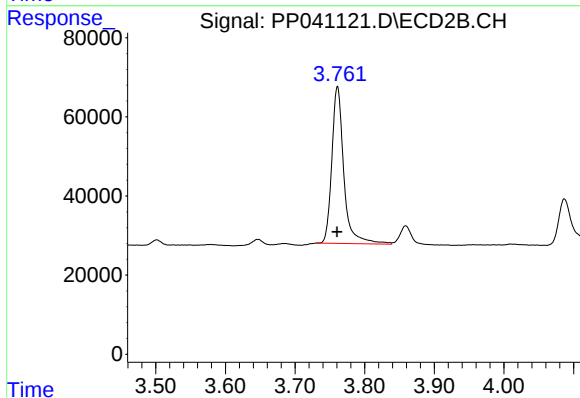


#1 Tetrachloro-m-xylene

R.T.: 3.761 min
Delta R.T.: 0.000 min
Response: 474326
Conc: 17.07 ng/ml

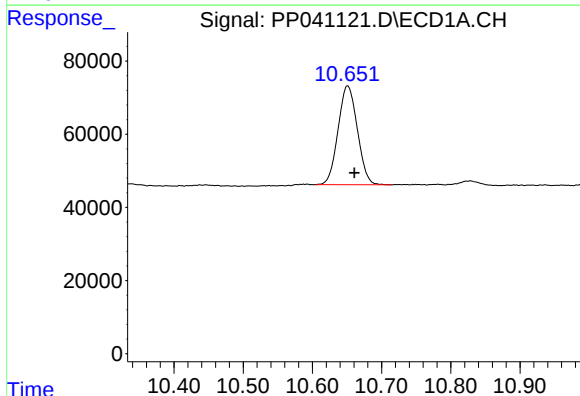


#2 Decachlorobiphenyl

R.T.: 10.651 min
Delta R.T.: -0.010 min
Response: 523590
Conc: 23.97 ng/ml

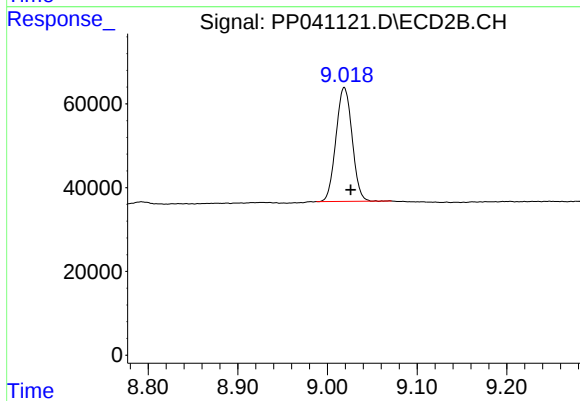

#2 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: -0.007 min
Response: 339689
Conc: 23.70 ng/ml

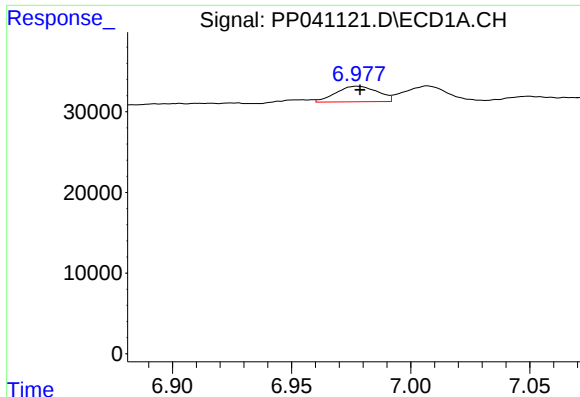


#26 AR-1254-1

R.T.: 6.977 min
Delta R.T.: -0.002 min
Response: 23206
Conc: 30.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-27106


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

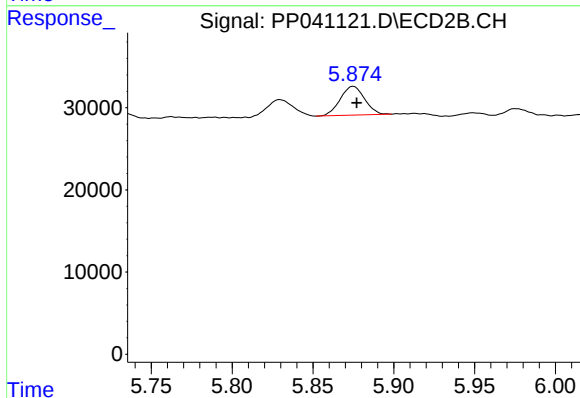


#26 AR-1254-1

R.T.: 5.875 min
Delta R.T.: -0.002 min
Response: 36652
Conc: 32.19 ng/ml

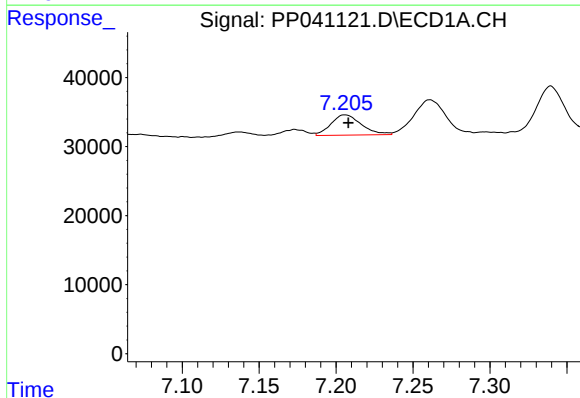


#27 AR-1254-2

R.T.: 7.206 min
Delta R.T.: -0.002 min
Response: 40272
Conc: 32.58 ng/ml

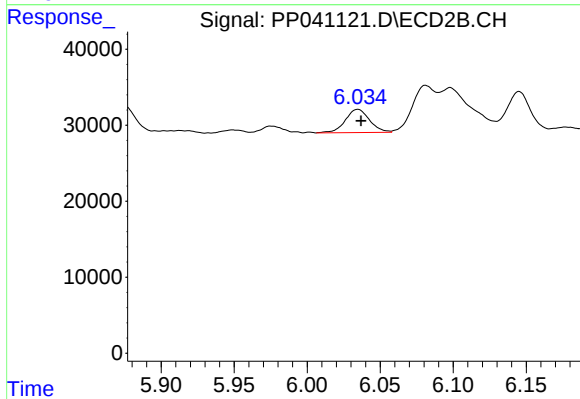

#27 AR-1254-2

R.T.: 6.035 min
Delta R.T.: -0.002 min
Response: 35296
Conc: 36.00 ng/ml

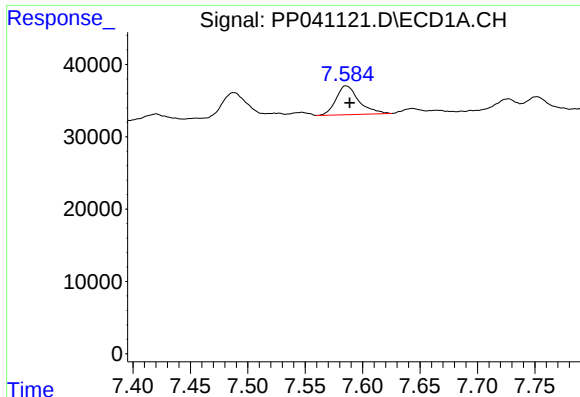


#28 AR-1254-3

R.T.: 7.586 min
Delta R.T.: -0.003 min
Response: 55502
Conc: 41.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-27106


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

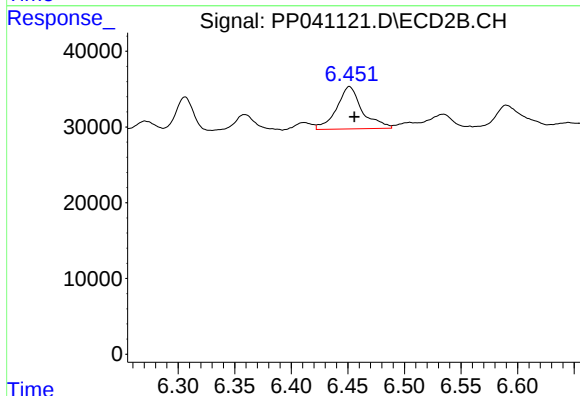


#28 AR-1254-3

R.T.: 6.451 min
Delta R.T.: -0.004 min
Response: 88163
Conc: 60.95 ng/ml

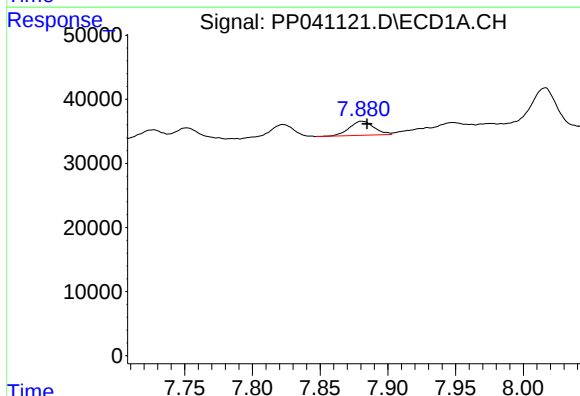


#29 AR-1254-4

R.T.: 7.881 min
Delta R.T.: -0.004 min
Response: 27821
Conc: 29.15 ng/ml

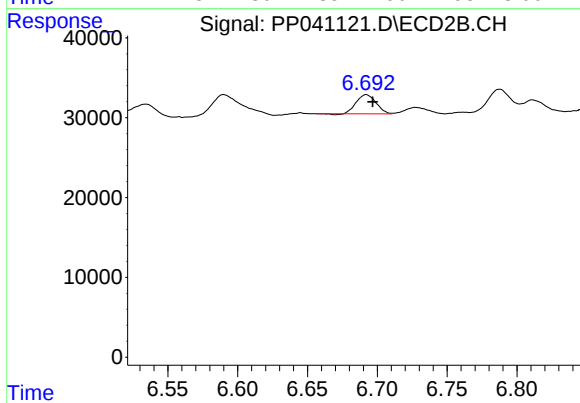

#29 AR-1254-4

R.T.: 6.692 min
Delta R.T.: -0.005 min
Response: 23351
Conc: 28.15 ng/ml

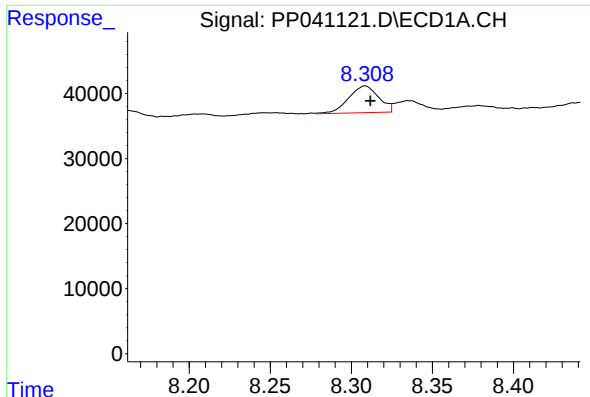


#30 AR-1254-5

R.T.: 8.308 min
Delta R.T.: -0.004 min
Response: 53442
Conc: 50.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-27106

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

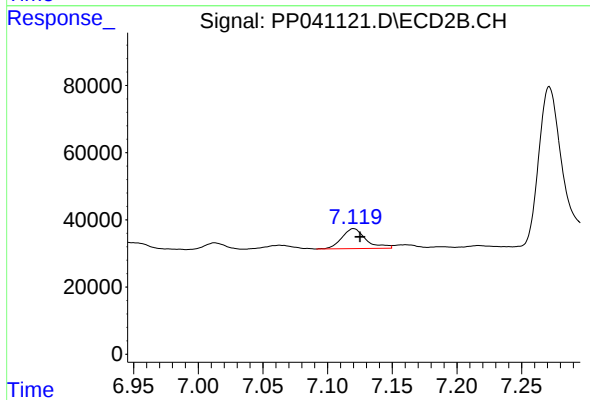

#30 AR-1254-5

R.T.: 7.120 min
Delta R.T.: -0.005 min
Response: 77086
Conc: 66.13 ng/ml