

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041133.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2021 21:08
Operator : AJ\MA
Sample : M4758-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:25:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	3.757	529009	764910	25.085	27.524
2) SA Decachlor...	10.650	9.017	532960	355674	24.398	24.811

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041133.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2021 21:08
Operator : AJ\MA
Sample : M4758-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:25:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

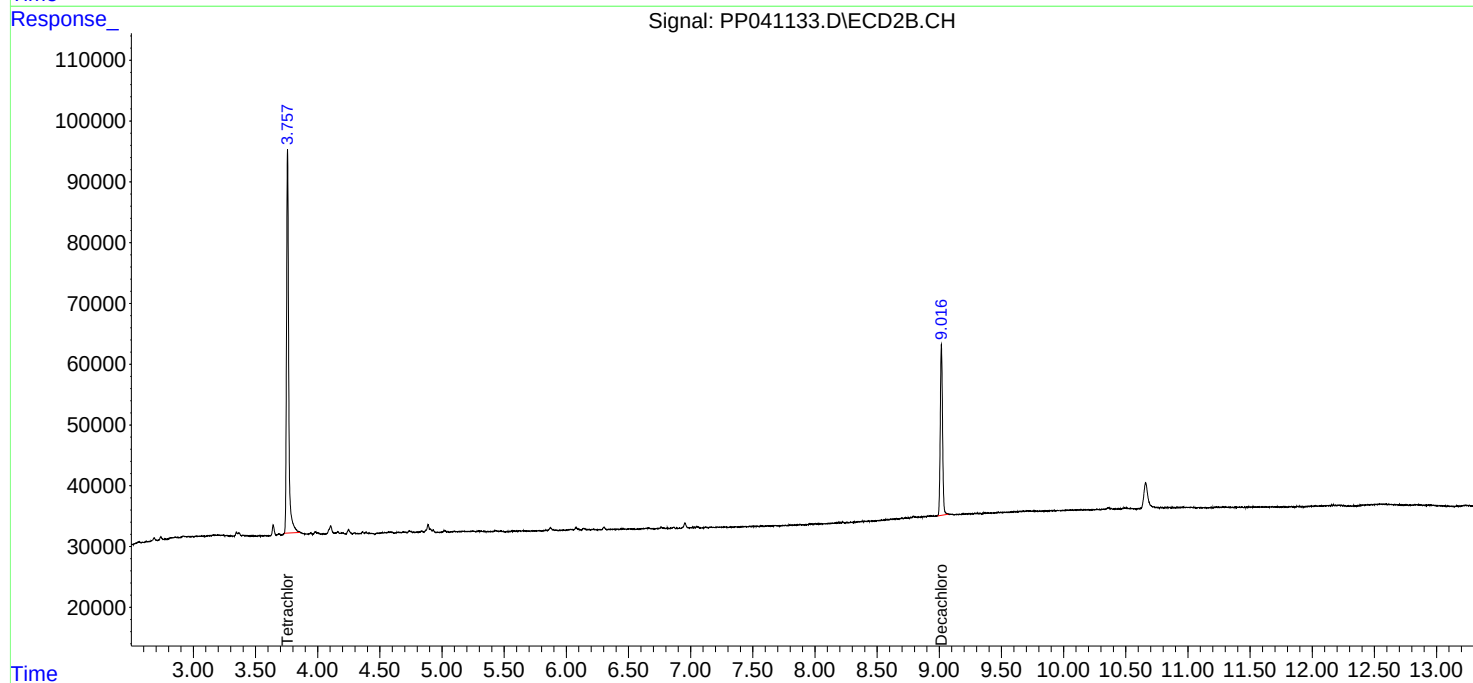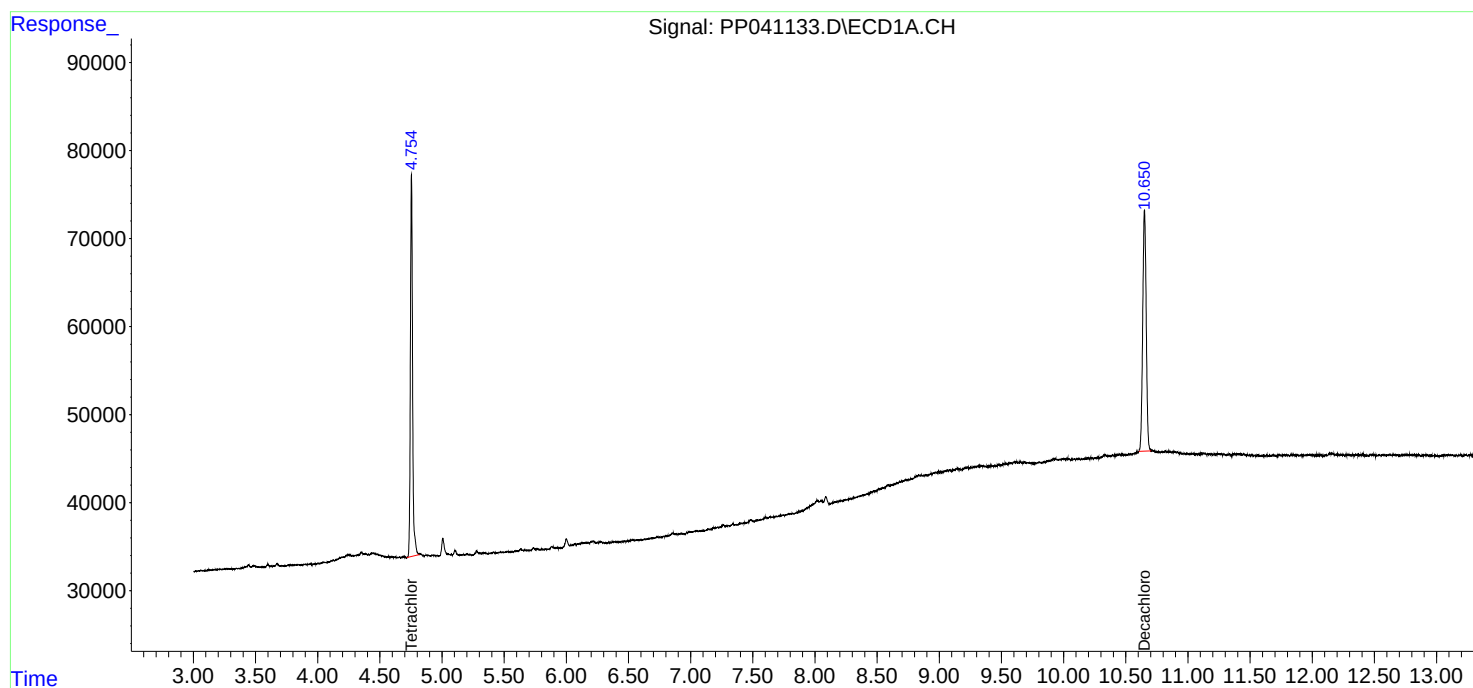


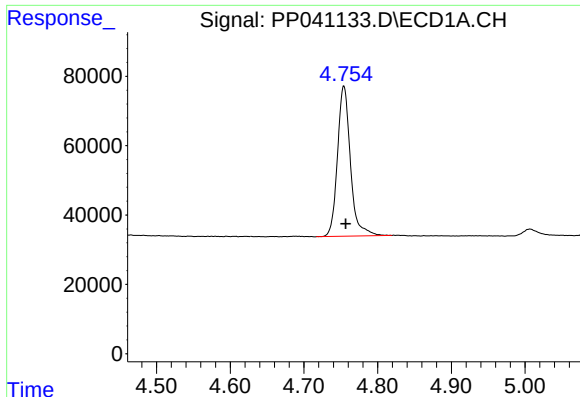

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 529009
Conc: 25.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP5

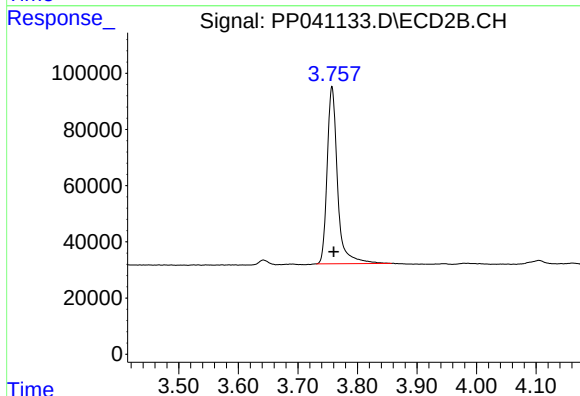


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 764910
Conc: 27.52 ng/ml

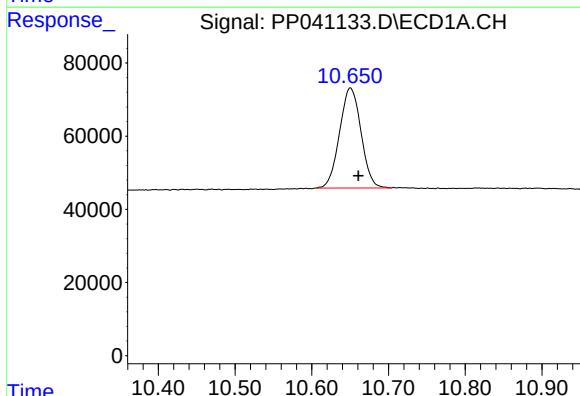

#2 Decachlorobiphenyl

R.T.: 10.650 min
Delta R.T.: -0.011 min
Response: 532960
Conc: 24.40 ng/ml

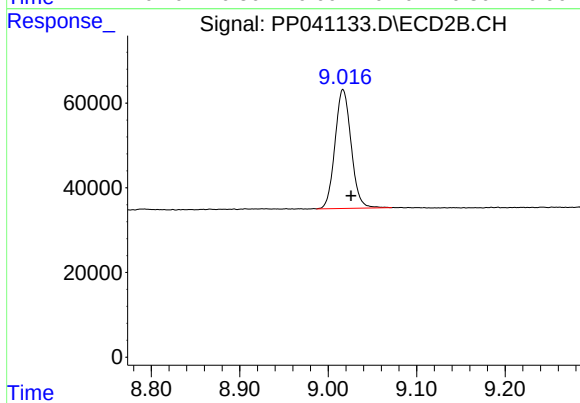

#2 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.009 min
Response: 355674
Conc: 24.81 ng/ml