

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041177.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 11:06
 Operator : AJ\MA
 Sample : M4728-04 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2021-5B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:38:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	3.757	37430	50483	1.775	1.817m
2) SA Decachlor...	10.645f	9.015	71917	38275	3.292m	2.670

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
Data File : PP041177.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2021 11:06
Operator : AJ\MA
Sample : M4728-04 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:38:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

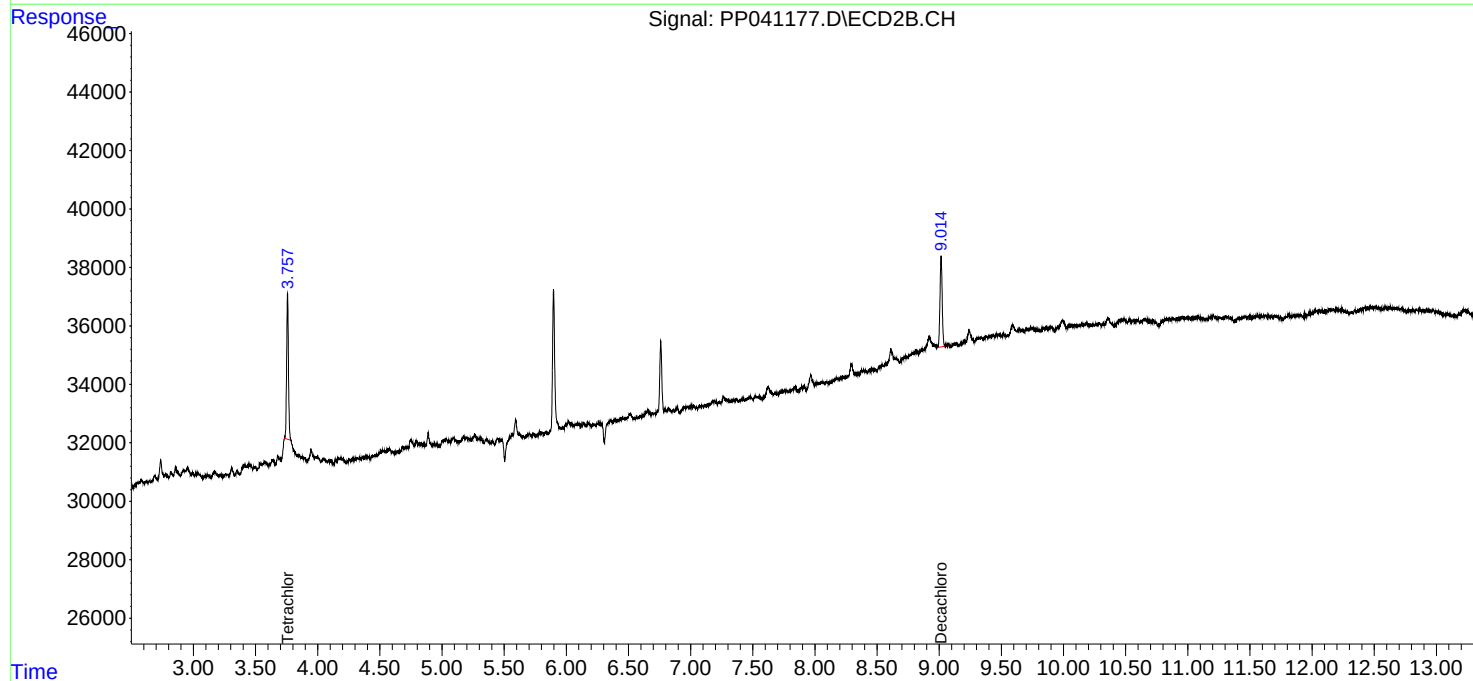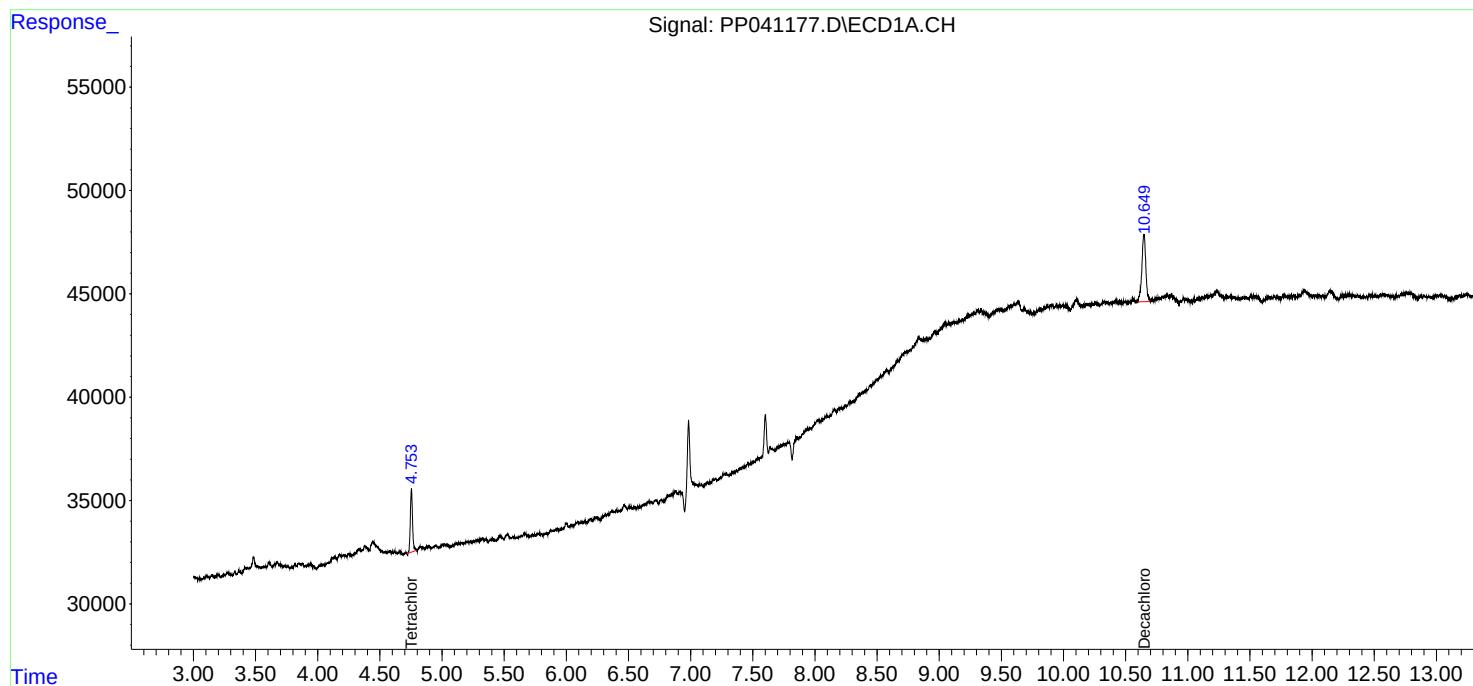

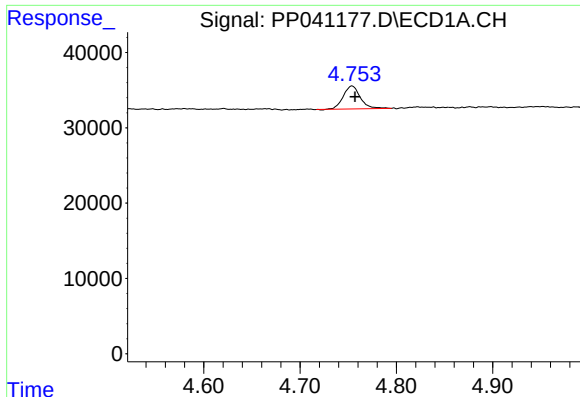


#1 Tetrachloro-m-xylene

R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 37430
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2021-5B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/22/2021
Supervised By :Sohil Jodhani 11/22/2021

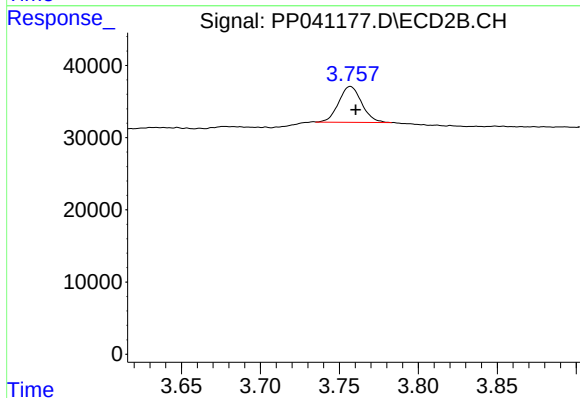


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.004 min
Response: 50483
Conc: 1.82 ng/ml m

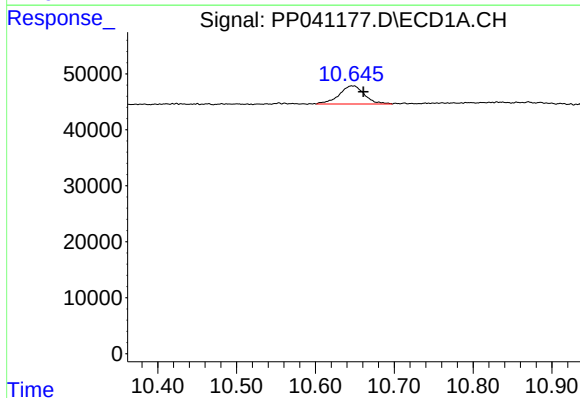

#2 Decachlorobiphenyl

R.T.: 10.645 min
Delta R.T.: -0.015 min
Response: 71917
Conc: 3.29 ng/ml m

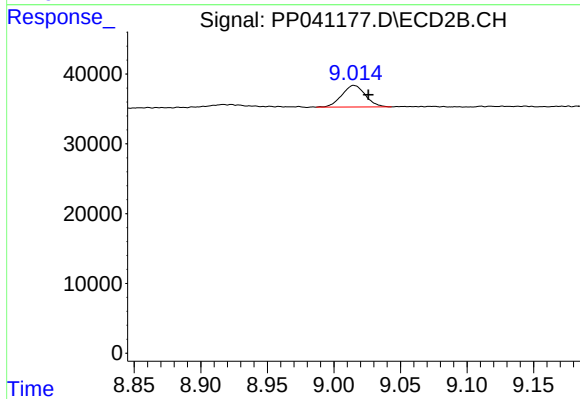

#2 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: -0.011 min
Response: 38275
Conc: 2.67 ng/ml