

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041180.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 11:56
 Operator : AJ\MA
 Sample : M4758-37
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:39:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	3.758	475233	661771	22.535	23.813
2) SA Decachlor...	10.649	9.016	410853	268724	18.808	18.746

Target Compounds



 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111921\
 Data File : PP041180.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2021 11:56
 Operator : AJ\MA
 Sample : M4758-37
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:39:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

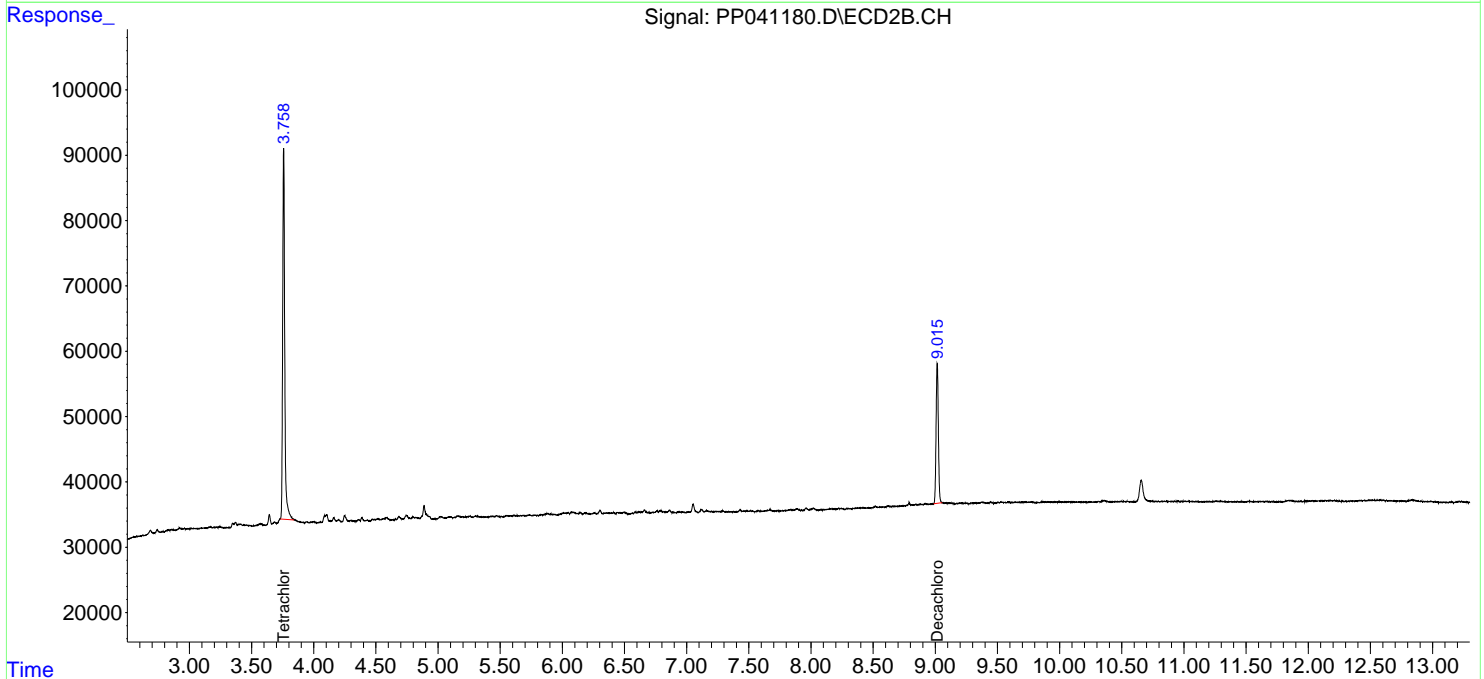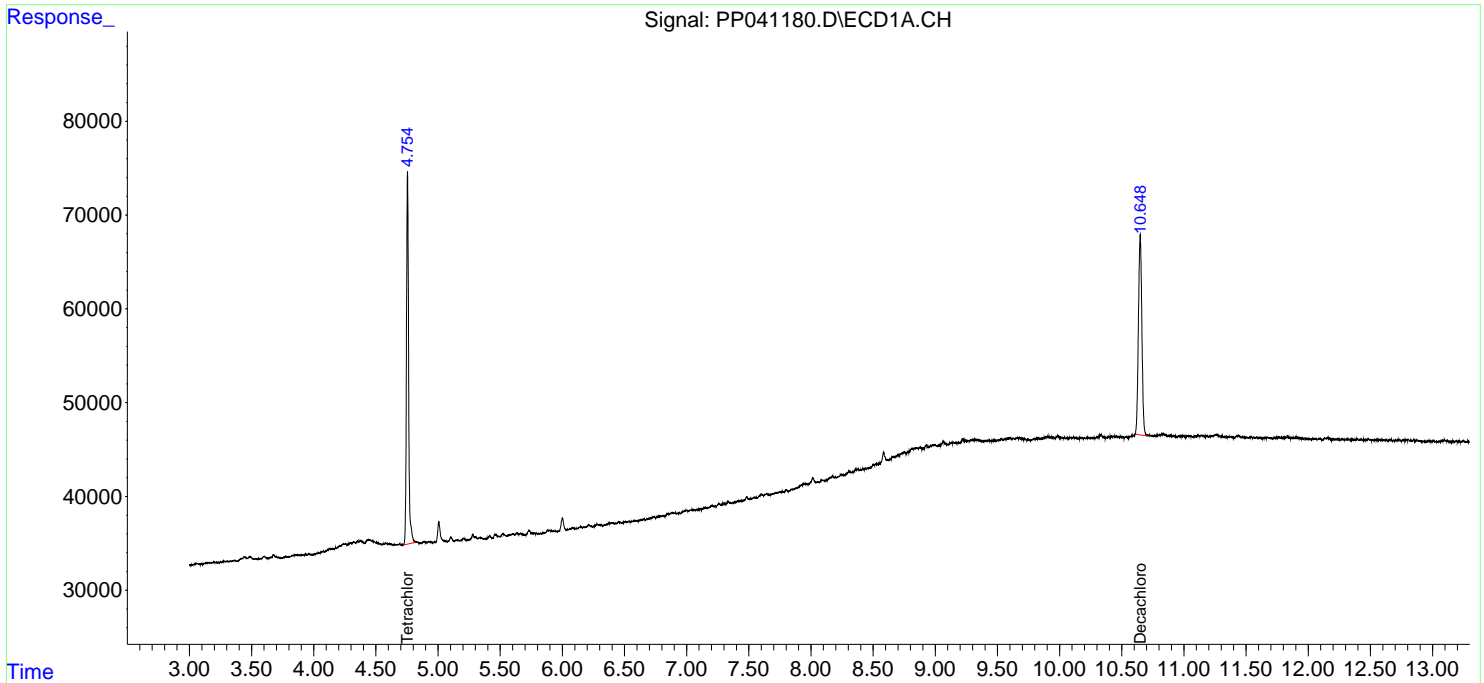

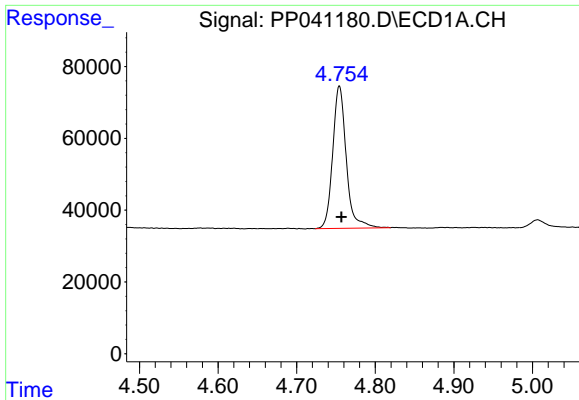


#1 Tetrachloro-m-xylene
 R.T.: 4.754 min
 Delta R.T.: -0.003 min
 Response: 475233
 Conc: 22.53 ng/ml


Instrument :
 ECD_P
 ClientSampleId :
 TP19

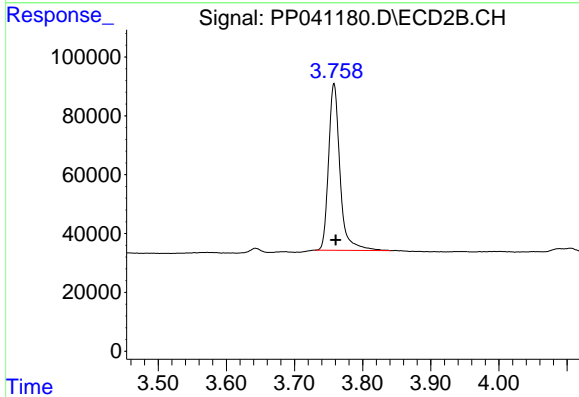

#1 Tetrachloro-m-xylene
 R.T.: 3.758 min
 Delta R.T.: -0.002 min
 Response: 661771
 Conc: 23.81 ng/ml

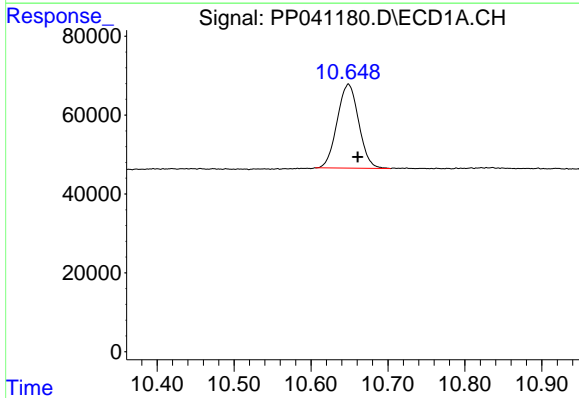

#2 Decachlorobiphenyl
 R.T.: 10.649 min
 Delta R.T.: -0.012 min
 Response: 410853
 Conc: 18.81 ng/ml

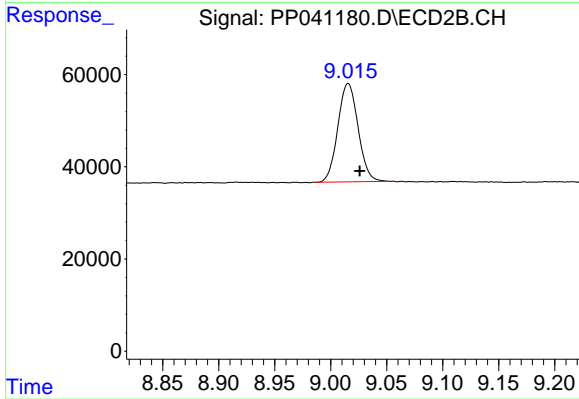

#2 Decachlorobiphenyl
 R.T.: 9.016 min
 Delta R.T.: -0.010 min
 Response: 268724
 Conc: 18.75 ng/ml