

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112020\
 Data File : PP031460.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2020 15:55
 Operator : DD\AJ
 Sample : L4809-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-CON-A

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:05:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:25:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.793	4.066	1106590	1053828	27.163	25.206
2)	SA Decachlor...	10.669	9.375	760120	865935	24.748	25.860
Target Compounds							
26)	L6 AR-1254-1	7.001	6.195	37214	59241	28.972m	31.130
27)	L6 AR-1254-2	7.231	6.352	99806	78057	51.699	47.687
28)	L6 AR-1254-3	7.609	6.774	208102	244615	95.998	89.598
29)	L6 AR-1254-4	7.904	7.013	224680	233892	148.806	150.509
30)	L6 AR-1254-5	8.331	7.442	319525	482419	195.457	199.529

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112020\
Data File : PP031460.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2020 15:55
Operator : DD\AJ
Sample : L4809-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:25:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

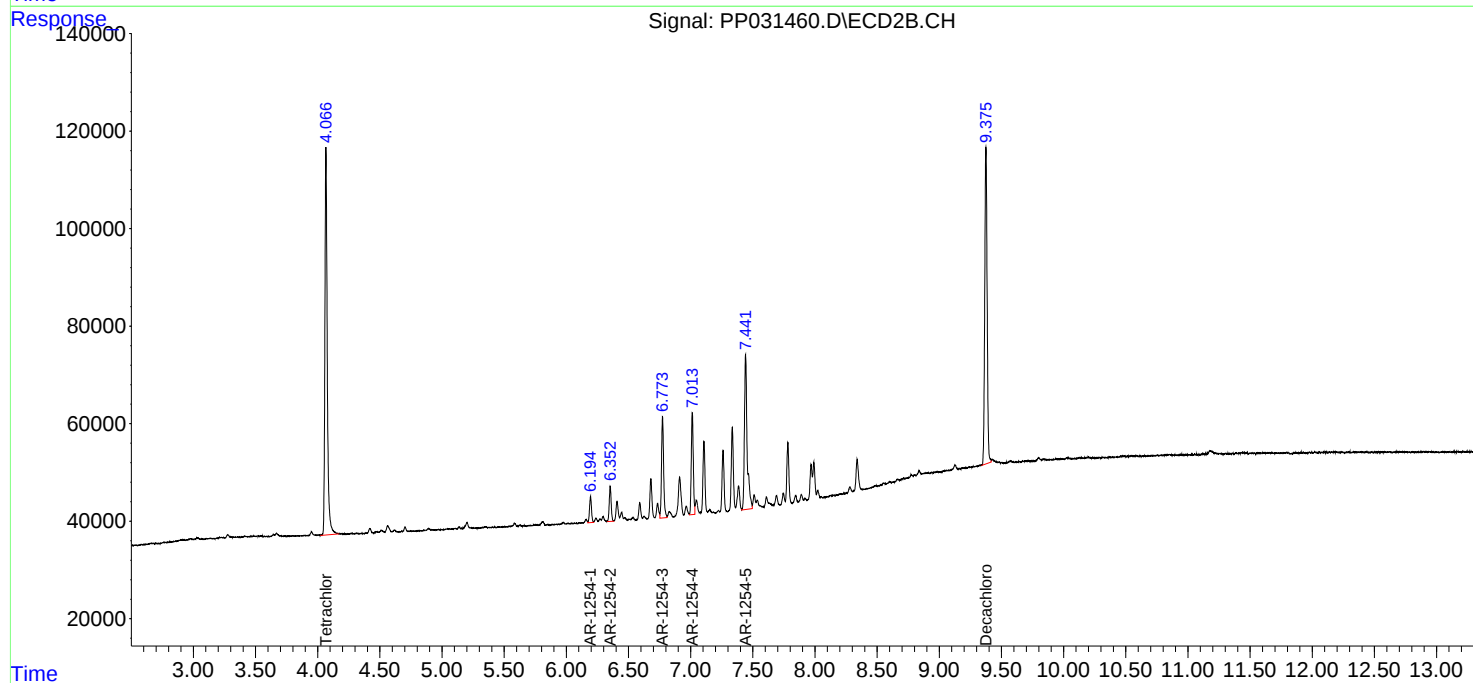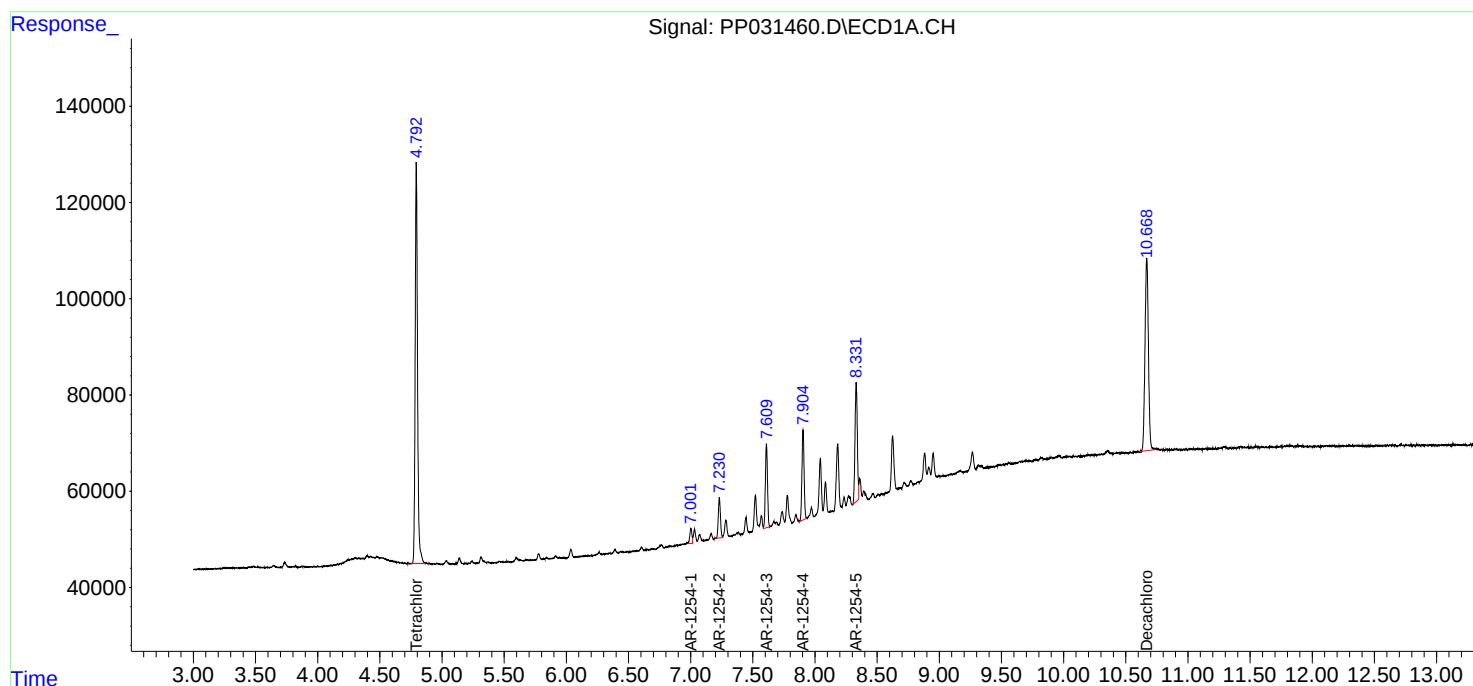

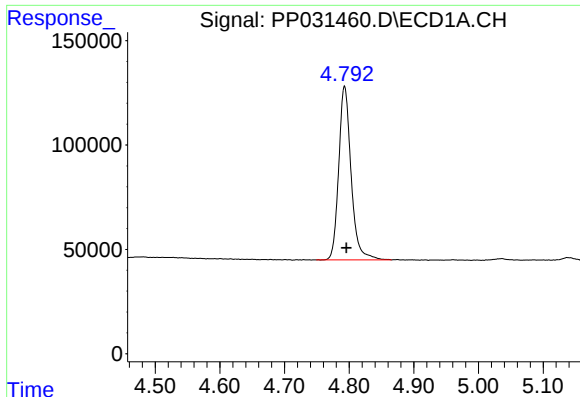


#1 Tetrachloro-m-xylene

R.T.: 4.793 min
Delta R.T.: -0.003 min
Response: 1106590
Conc: 27.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:08 PM

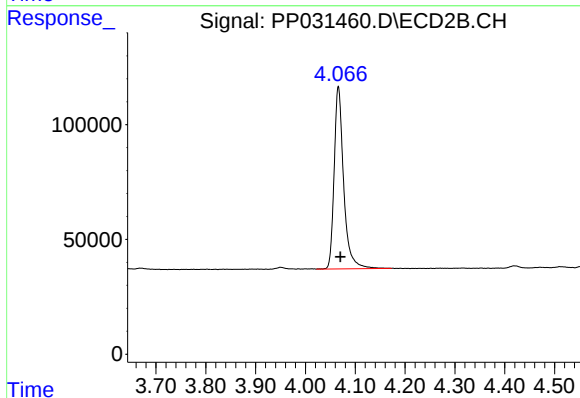


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: -0.004 min
Response: 1053828
Conc: 25.21 ng/ml

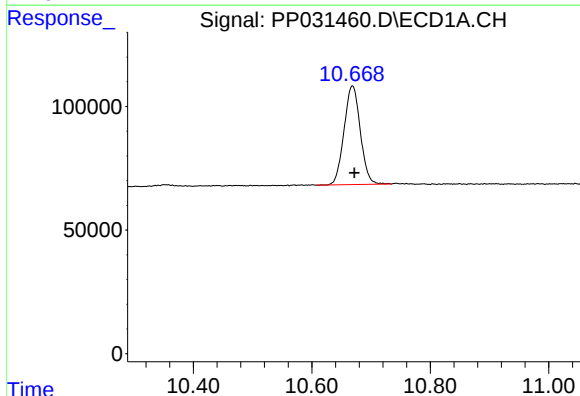


#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.003 min
Response: 760120
Conc: 24.75 ng/ml

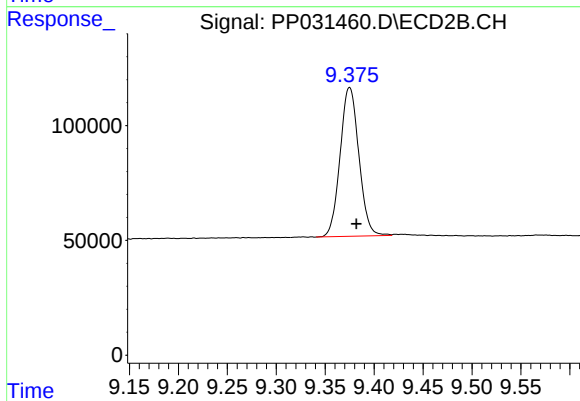

#2 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: -0.007 min
Response: 865935
Conc: 25.86 ng/ml

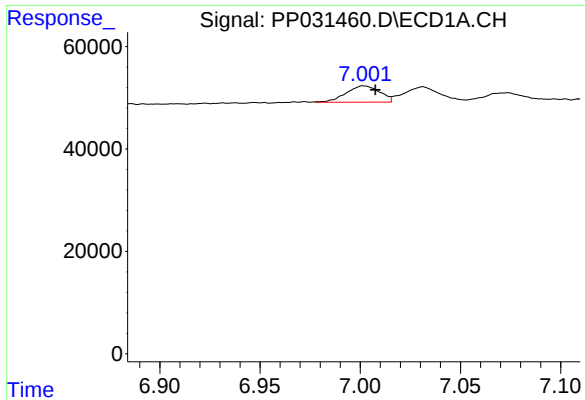


#26 AR-1254-1

R.T.: 7.001 min
Delta R.T.: -0.006 min
Response: 37214
Conc: 28.97 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:08 PM

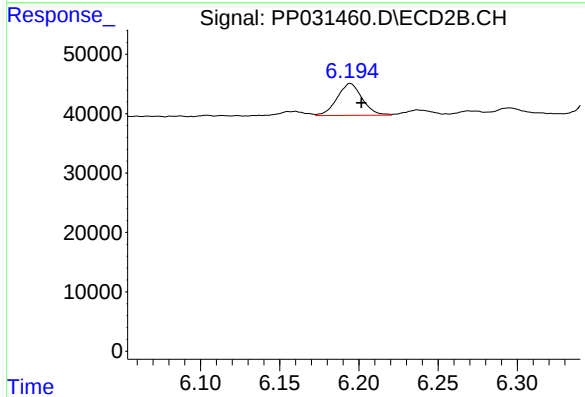


#26 AR-1254-1

R.T.: 6.195 min
Delta R.T.: -0.007 min
Response: 59241
Conc: 31.13 ng/ml

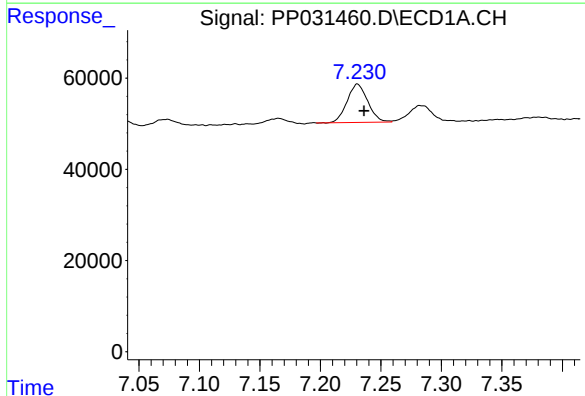


#27 AR-1254-2

R.T.: 7.231 min
Delta R.T.: -0.005 min
Response: 99806
Conc: 51.70 ng/ml

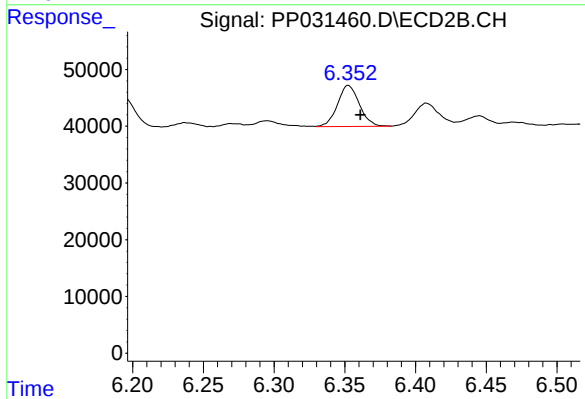

#27 AR-1254-2

R.T.: 6.352 min
Delta R.T.: -0.008 min
Response: 78057
Conc: 47.69 ng/ml

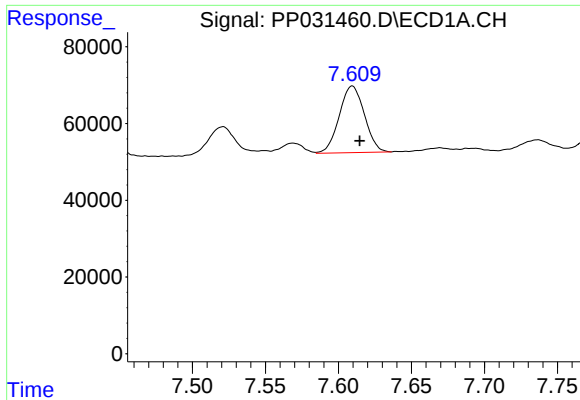


#28 AR-1254-3

R.T.: 7.609 min
Delta R.T.: -0.005 min
Response: 208102
Conc: 96.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:08 PM

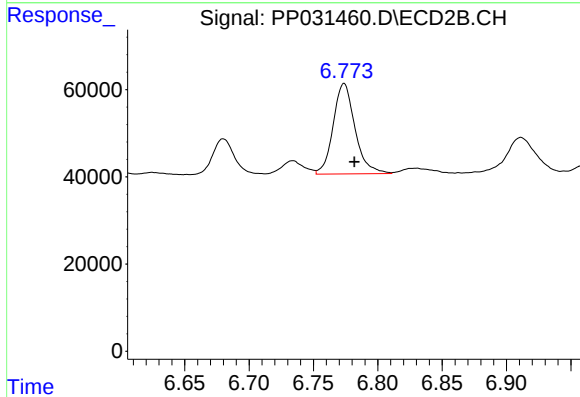


#28 AR-1254-3

R.T.: 6.774 min
Delta R.T.: -0.008 min
Response: 244615
Conc: 89.60 ng/ml

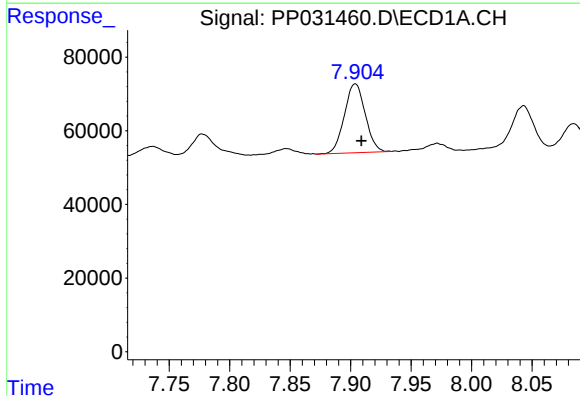


#29 AR-1254-4

R.T.: 7.904 min
Delta R.T.: -0.005 min
Response: 224680
Conc: 148.81 ng/ml

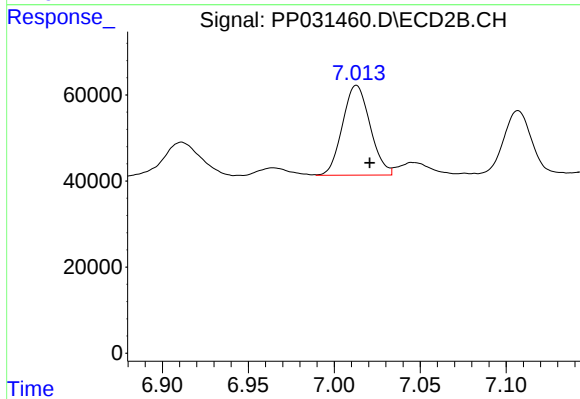

#29 AR-1254-4

R.T.: 7.013 min
Delta R.T.: -0.008 min
Response: 233892
Conc: 150.51 ng/ml

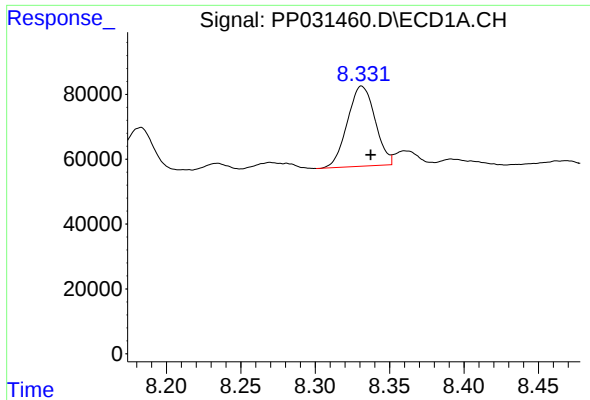


#30 AR-1254-5

R.T.: 8.331 min
Delta R.T.: -0.006 min
Response: 319525
Conc: 195.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-A

Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:08 PM

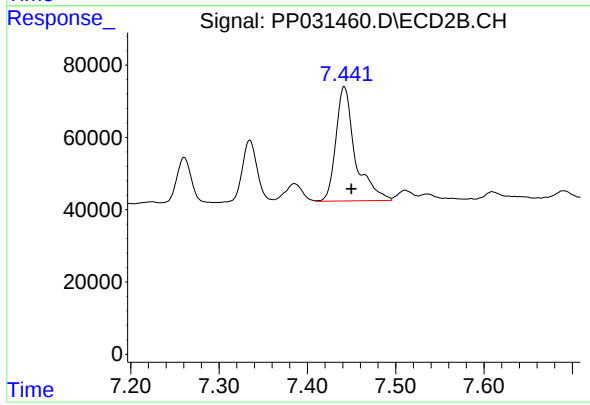

#30 AR-1254-5

R.T.: 7.442 min
Delta R.T.: -0.008 min
Response: 482419
Conc: 199.53 ng/ml