

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112020\
 Data File : PP031472.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2020 19:31
 Operator : DD\AJ
 Sample : PB133160BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB133160BL

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:05:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:30:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.793	4.067	1001700	941868	24.588	22.528
2) SA Decachlor...	10.667	9.373	733714	834150	23.889	24.911m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112020\
Data File : PP031472.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2020 19:31
Operator : DD\AJ
Sample : PB133160BL
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB133160BL


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:30:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

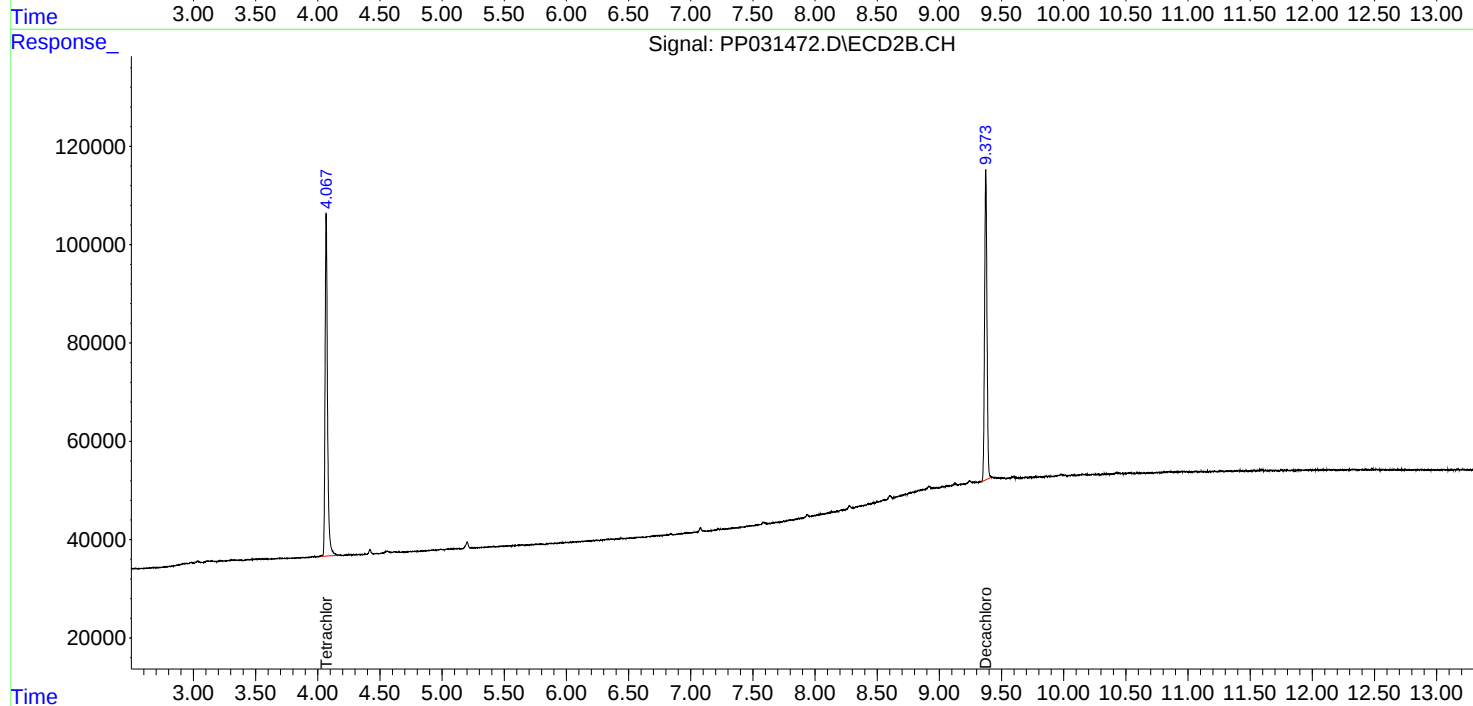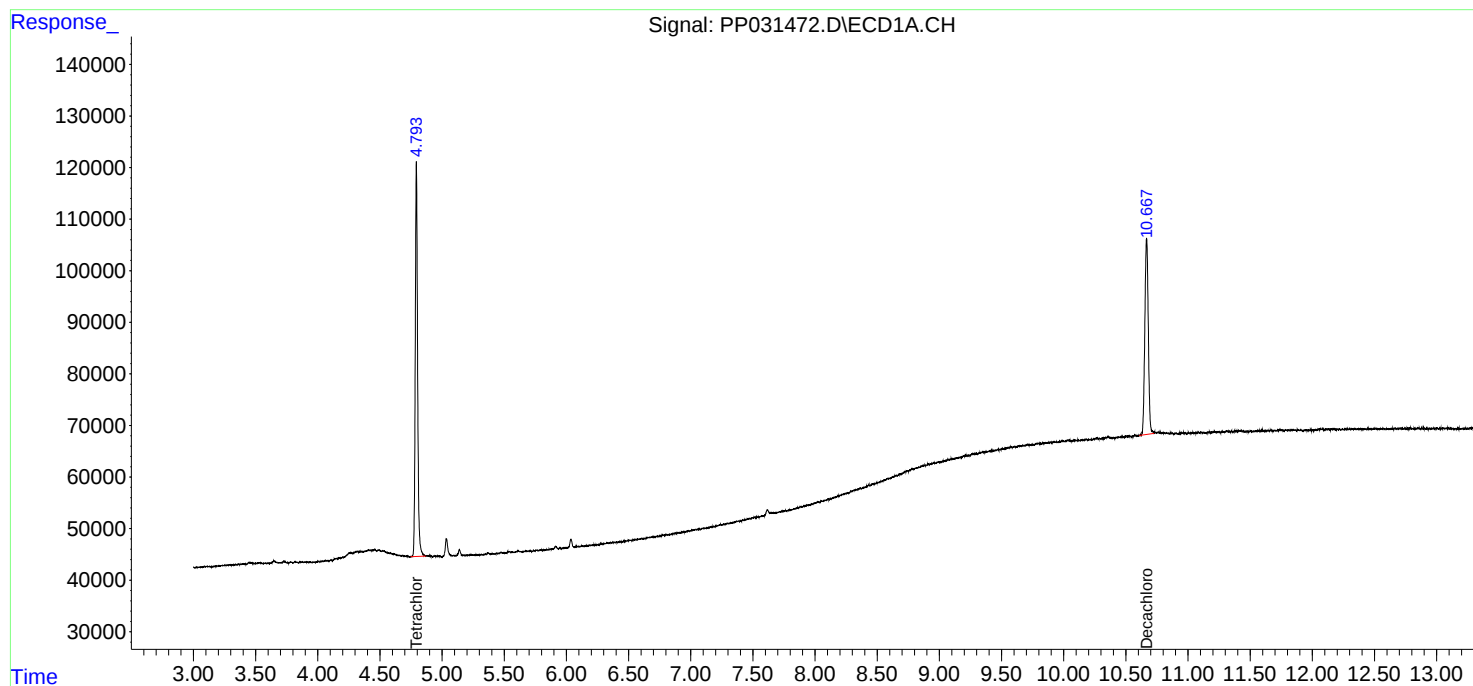

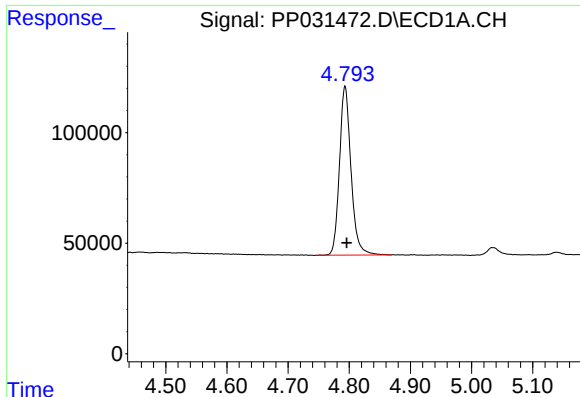


#1 Tetrachloro-m-xylene

R.T.: 4.793 min
Delta R.T.: -0.003 min
Response: 1001700
Conc: 24.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB133160BL


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:23 PM

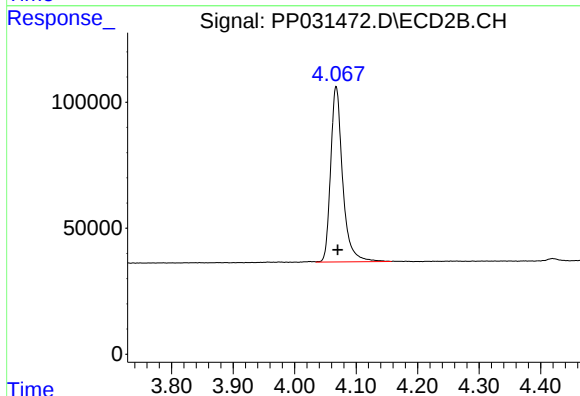


#1 Tetrachloro-m-xylene

R.T.: 4.067 min
Delta R.T.: -0.003 min
Response: 941868
Conc: 22.53 ng/ml

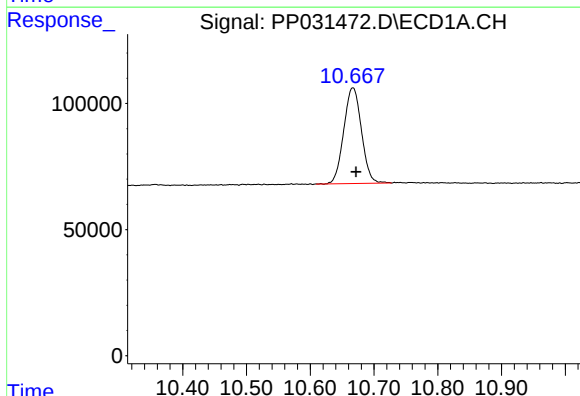

#2 Decachlorobiphenyl

R.T.: 10.667 min
Delta R.T.: -0.005 min
Response: 733714
Conc: 23.89 ng/ml

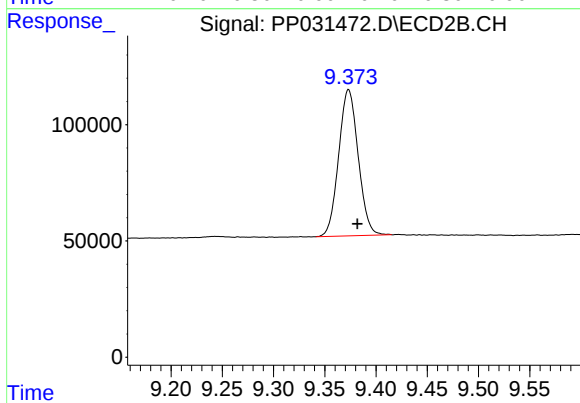

#2 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: -0.009 min
Response: 834150
Conc: 24.91 ng/ml m