

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112020\
 Data File : PP031483.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2020 22:35
 Operator : DD\AJ
 Sample : L4863-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S4-06-B

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:05:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:34:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.792	4.066	1230713	1147125	30.210	27.438
2) SA Decachlor...	10.664	9.372	791124	881007	25.758m	26.311

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112020\
Data File : PP031483.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2020 22:35
Operator : DD\AJ
Sample : L4863-08
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S4-06-B


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:34:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

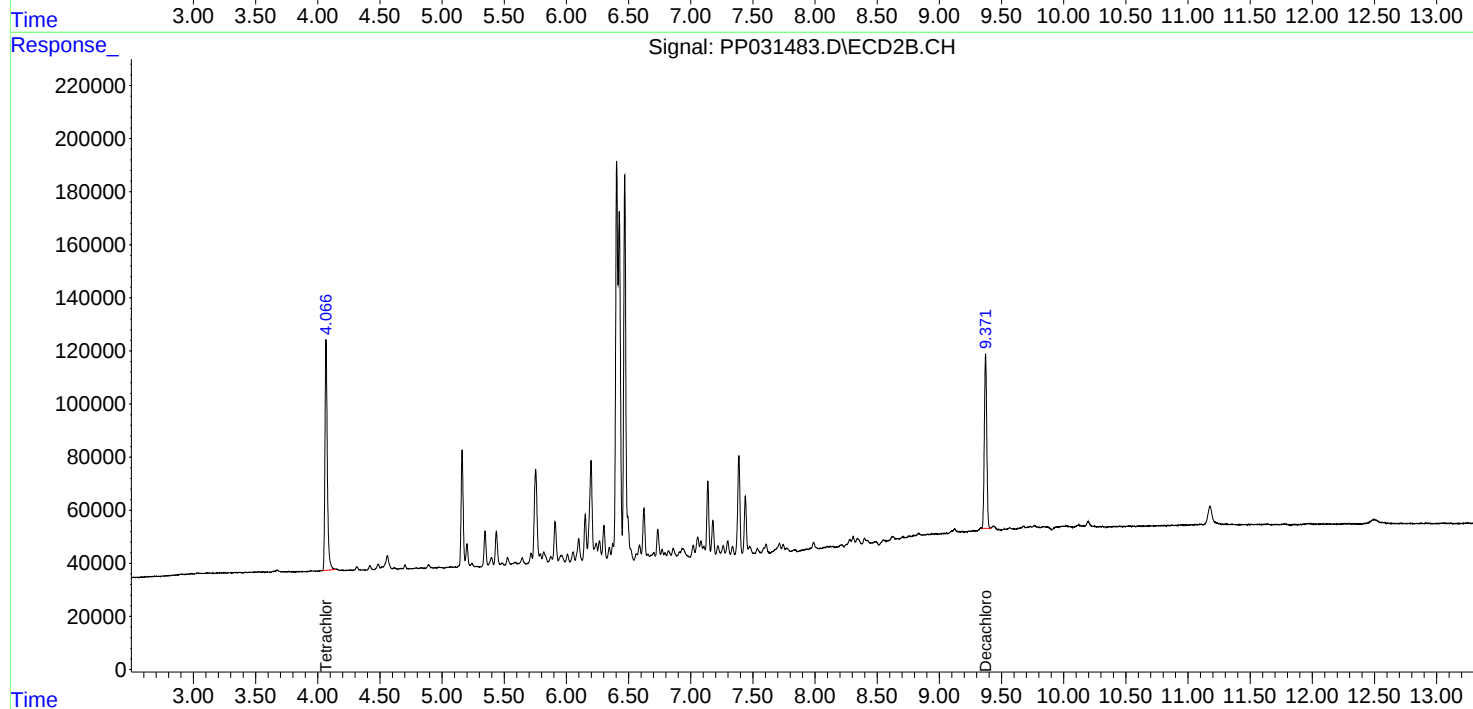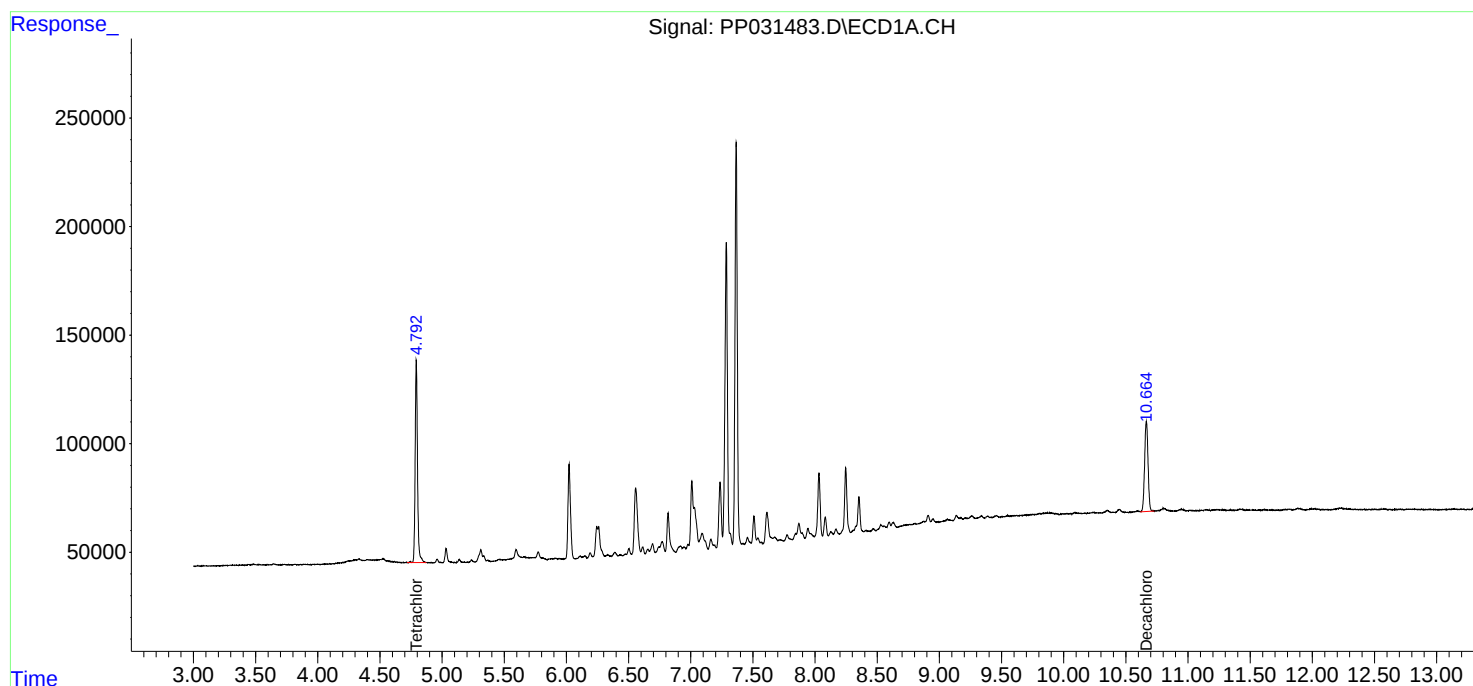

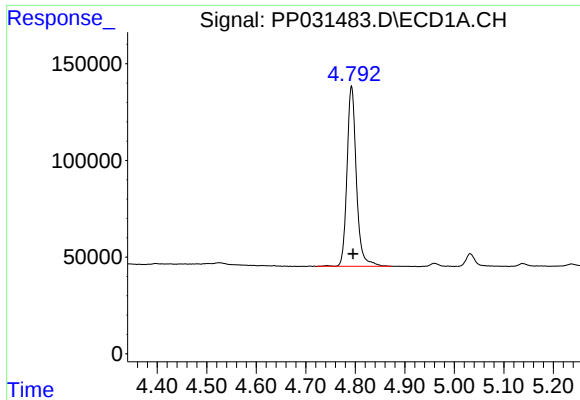


#1 Tetrachloro-m-xylene

R.T.: 4.792 min
Delta R.T.: -0.004 min
Response: 1230713
Conc: 30.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4-06-B


Manual Integrations
APPROVED

mohammad
11/23/2020 12:05:41 PM

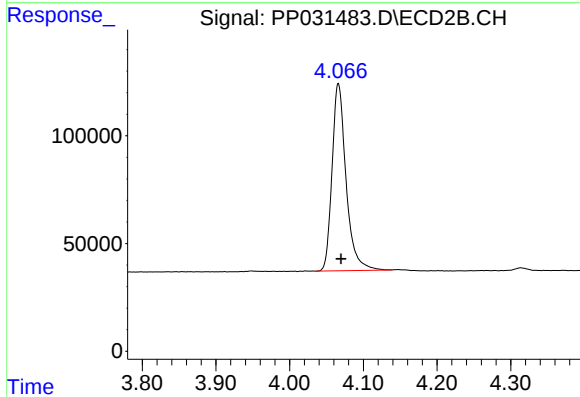


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: -0.004 min
Response: 1147125
Conc: 27.44 ng/ml

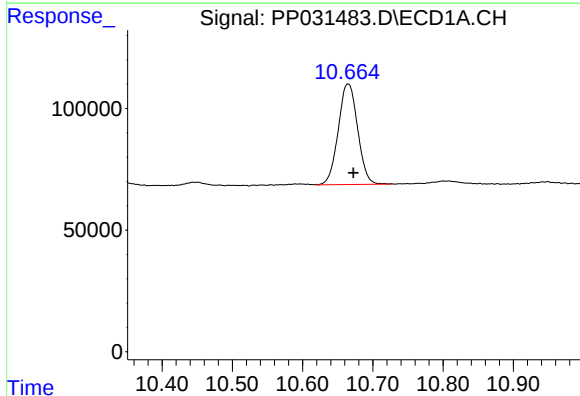

#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.008 min
Response: 791124
Conc: 25.76 ng/ml m

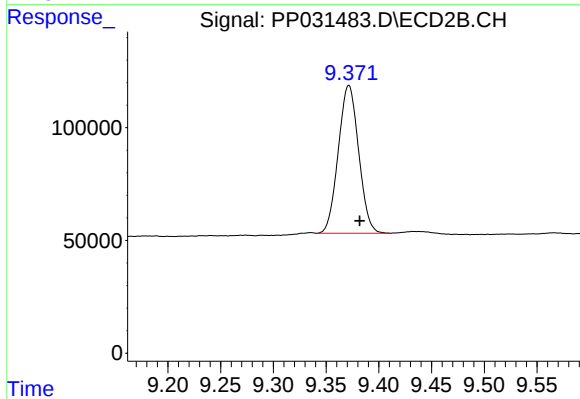

#2 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.010 min
Response: 881007
Conc: 26.31 ng/ml