

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112023\
 Data File : PP061784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 18:50
 Operator : YP\AJ
 Sample : 05471-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SP-D-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:25:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 16 04:03:35 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.726	31282178	43320303	23.738	20.591
2) SA Decachlor...	10.238	8.852	26394625	42210907	26.145m	25.862m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112023\
Data File : PP061784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 18:50
Operator : YP\AJ
Sample : 05471-02
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SP-D-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:25:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111523.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 16 04:03:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

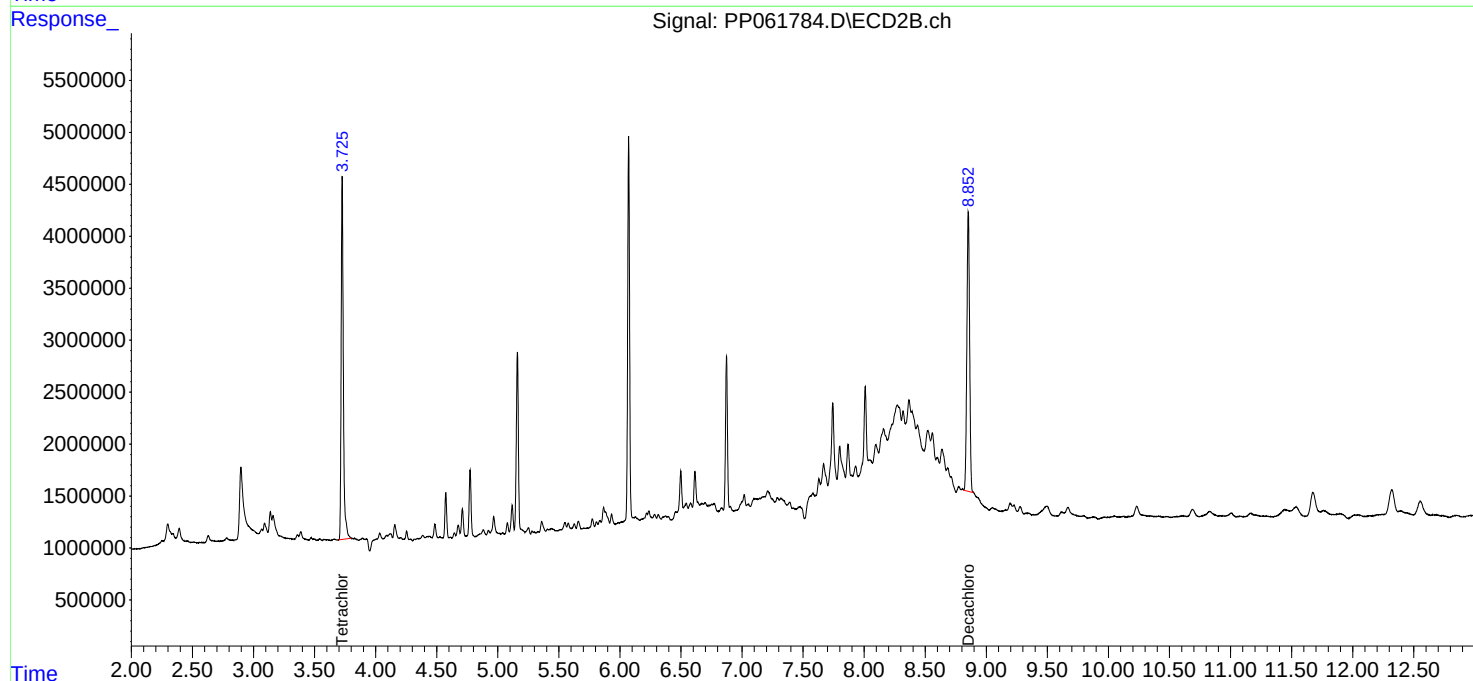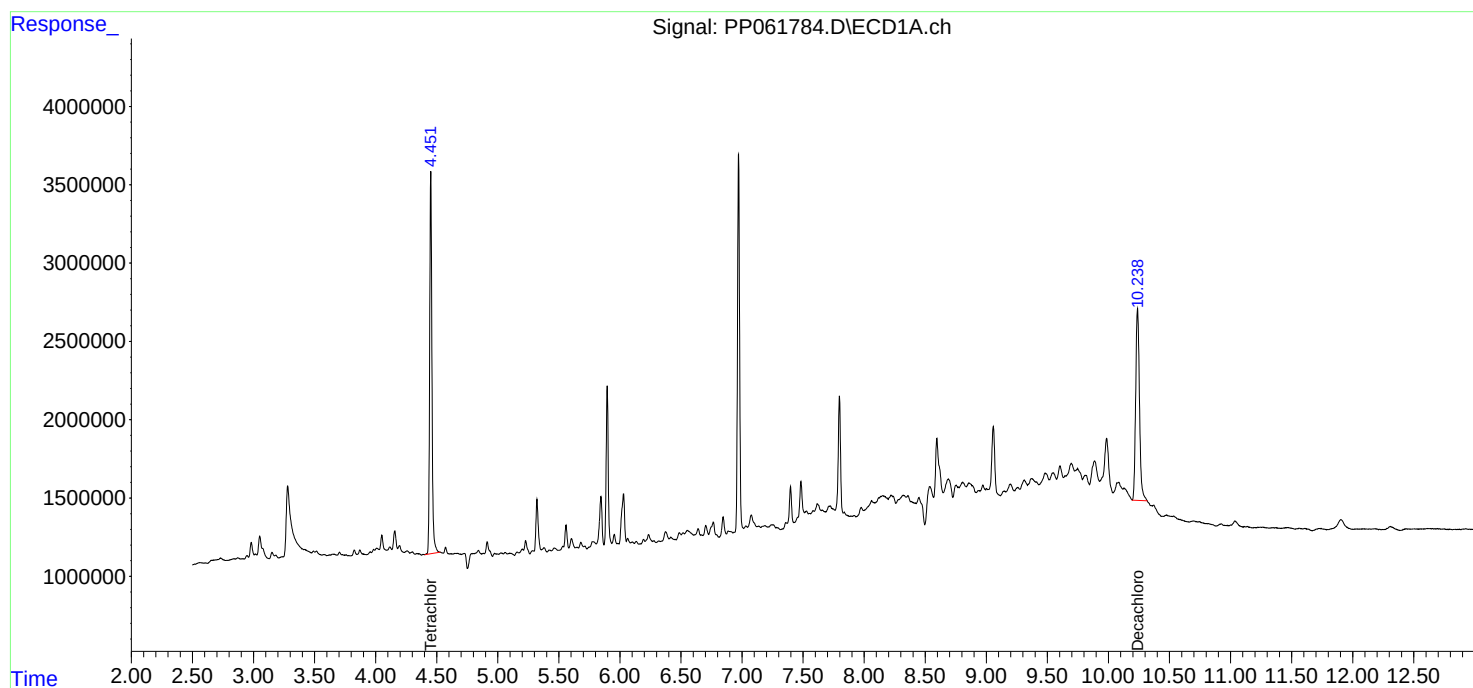

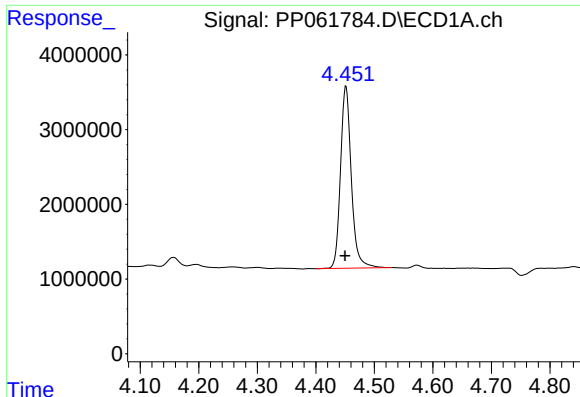


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: 0.002 min
Response: 31282178
Conc: 23.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-D-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

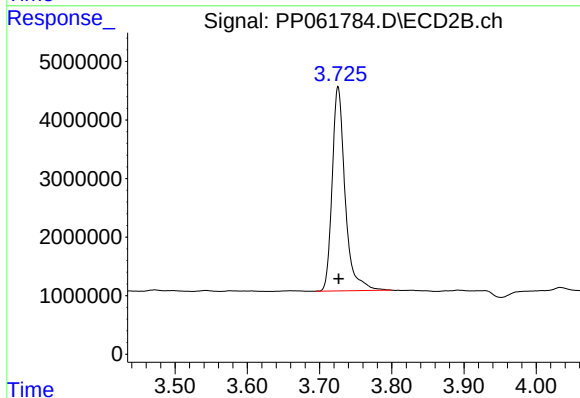


#1 Tetrachloro-m-xylene

R.T.: 3.726 min
Delta R.T.: -0.001 min
Response: 43320303
Conc: 20.59 ng/ml

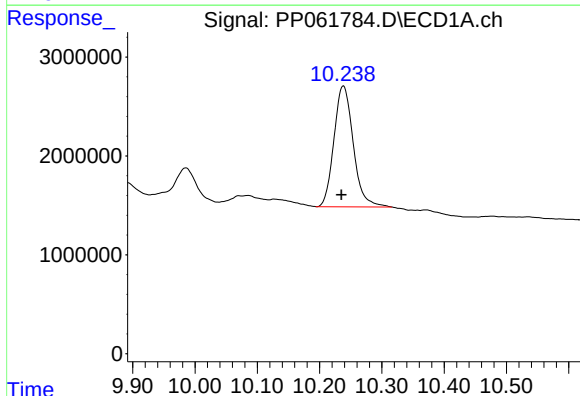

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: 0.003 min
Response: 26394625
Conc: 26.14 ng/ml m

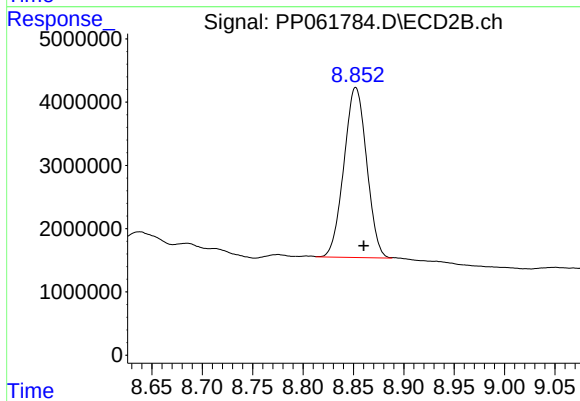

#2 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: -0.009 min
Response: 42210907
Conc: 25.86 ng/ml m