

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112024\
 Data File : PP068625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 14:15
 Operator : YP\AJ
 Sample : P4918-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ROOF-1-2A-2B-2C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2024
 Supervised By :Ankita Jodhani 11/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 02:45:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	4.051	48225265	19792129	49.685	20.440 #
2) SA Decachlor...	10.677	9.209	41290254	18290403	32.993m	16.169 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112024\
Data File : PP068625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 14:15
Operator : YP\AJ
Sample : P4918-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ROOF-1-2A-2B-2C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :Ankita Jodhani 11/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 02:45:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

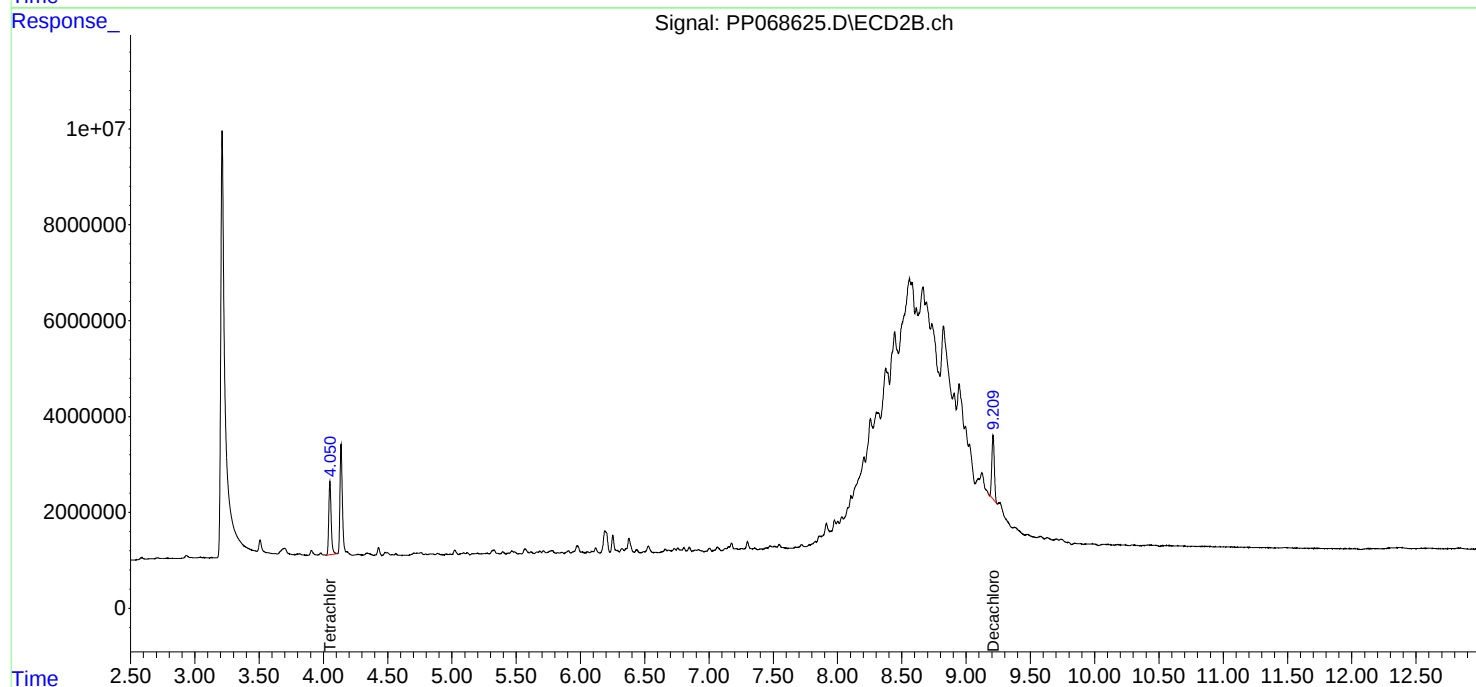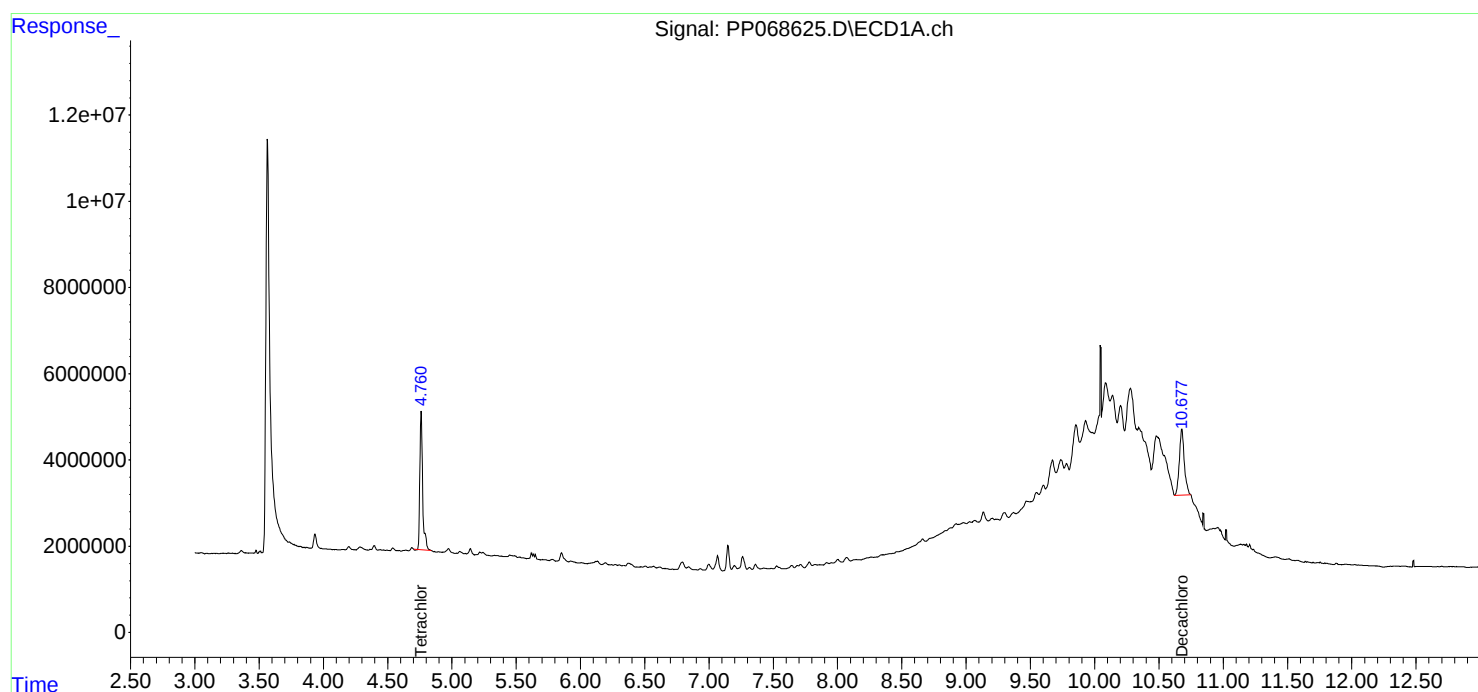

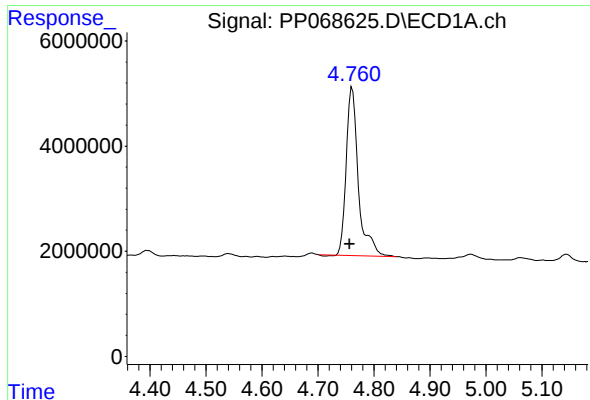


#1 Tetrachloro-m-xylene

R.T.: 4.761 min
Delta R.T.: 0.004 min
Response: 48225265
Conc: 49.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
ROOF-1-2A-2B-2C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :Ankita Jodhani 11/21/2024

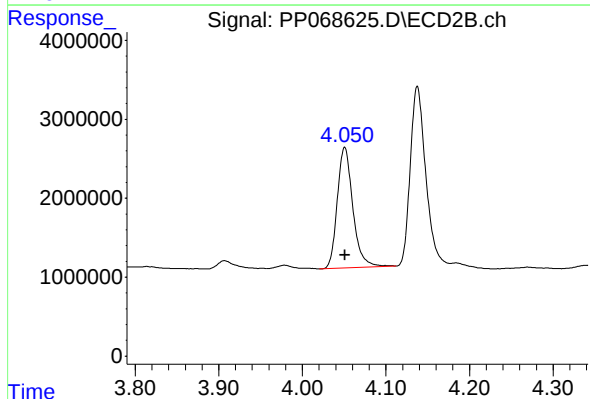


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 19792129
Conc: 20.44 ng/ml

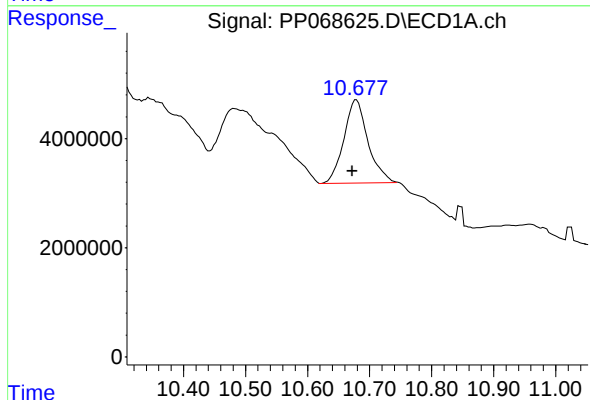

#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: 0.005 min
Response: 41290254
Conc: 32.99 ng/ml m

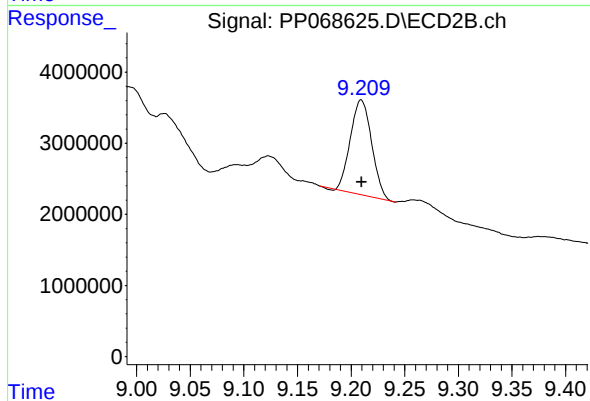

#2 Decachlorobiphenyl

R.T.: 9.209 min
Delta R.T.: 0.000 min
Response: 18290403
Conc: 16.17 ng/ml