

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112120\
 Data File : PP031500.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2020 9:38
 Operator : DD\AJ
 Sample : L4863-12RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S4-04-CRE

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:11:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 00:51:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.065	689849	658129	16.933m	15.742
2) SA Decachlor...	10.665	9.372	276673	302643	9.008	9.038

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112120\
Data File : PP031500.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2020 9:38
Operator : DD\AJ
Sample : L4863-12RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S4-04-CRE


Manual Integrations
APPROVED

mohammad
11/23/2020 12:11:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 00:51:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

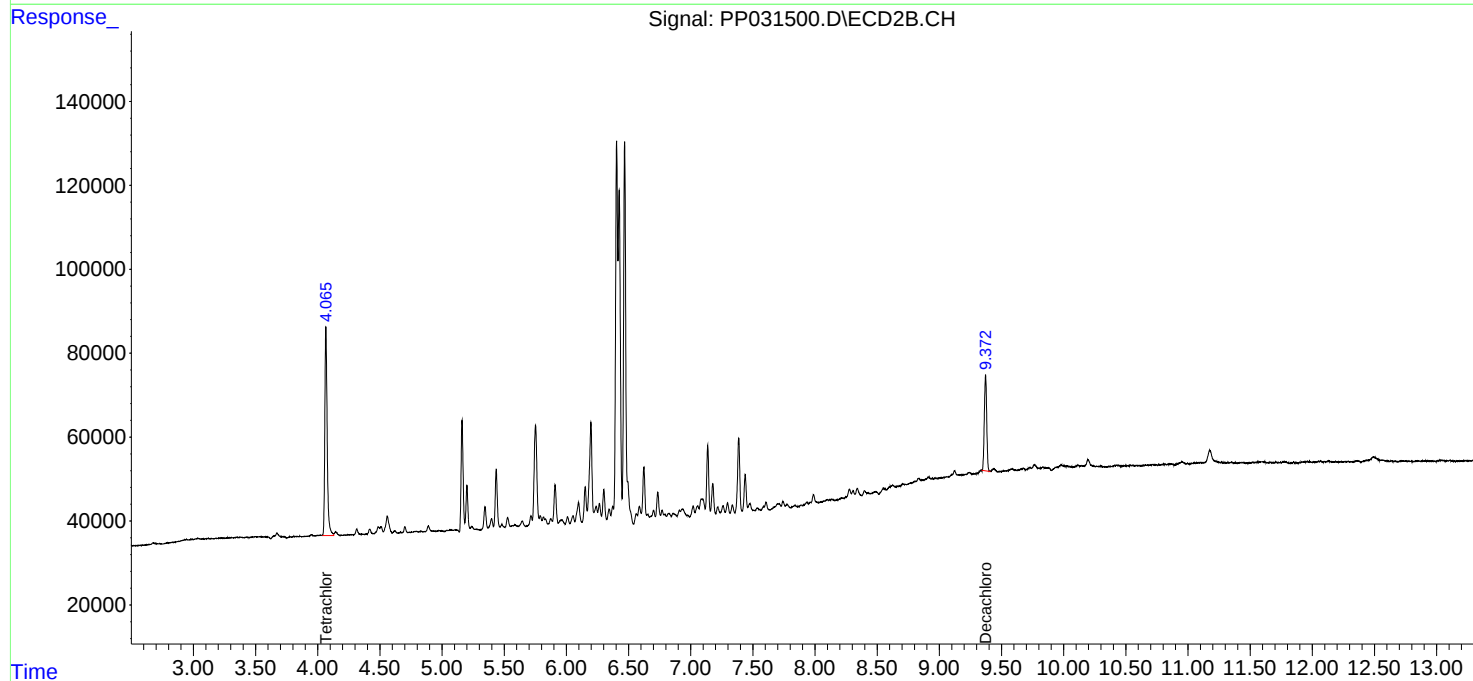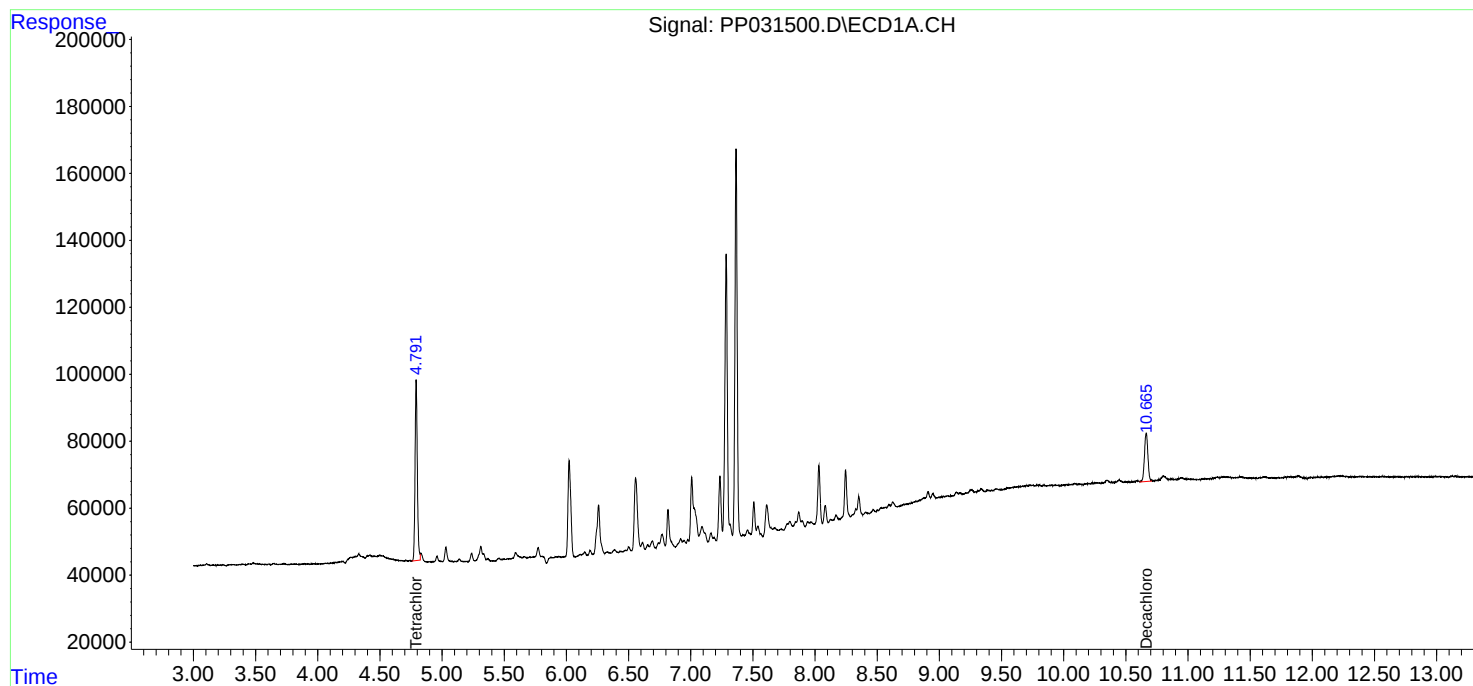

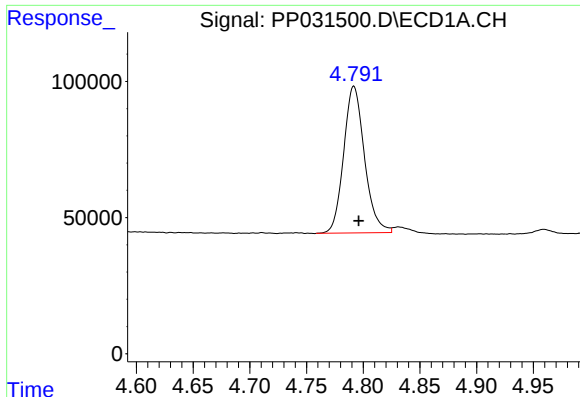


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: -0.005 min
Response: 689849
Conc: 16.93 ng/ml m

Instrument :
ECD_P
ClientSampleId :
S4-04-CRE


Manual Integrations
APPROVED

mohammad
11/23/2020 12:11:24 PM

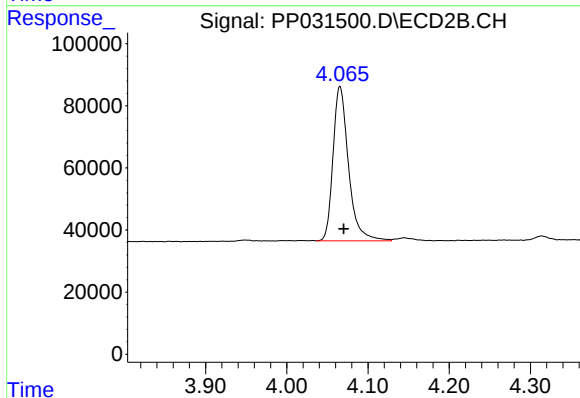


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.005 min
Response: 658129
Conc: 15.74 ng/ml

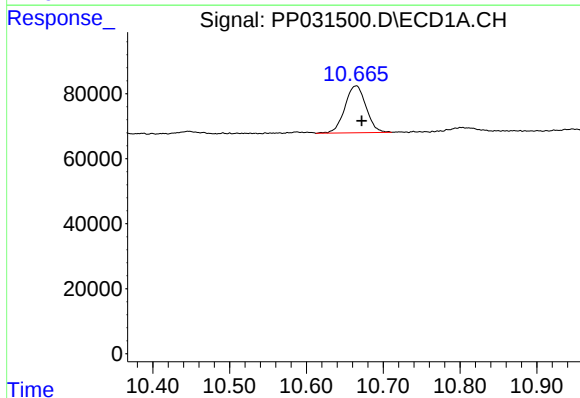

#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: -0.007 min
Response: 276673
Conc: 9.01 ng/ml

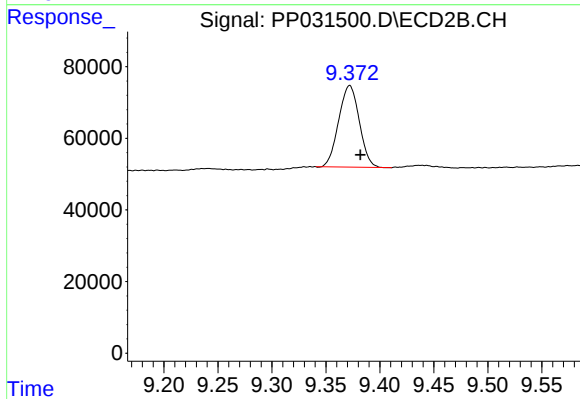

#2 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.010 min
Response: 302643
Conc: 9.04 ng/ml