

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112221\
 Data File : PP041202.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2021 14:59
 Operator : AJ\MA
 Sample : M4763-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FDA-683K-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 03:35:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	3.758	32495	51074	1.541	1.838
2) SA Decachlor...	10.659	9.019	50089	30954	2.293	2.159
Target Compounds						
30) L6 AR-1254-5	8.315	0.000	7814	0	7.352	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112221\
Data File : PP041202.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2021 14:59
Operator : AJ\MA
Sample : M4763-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FDA-683K-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 03:35:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

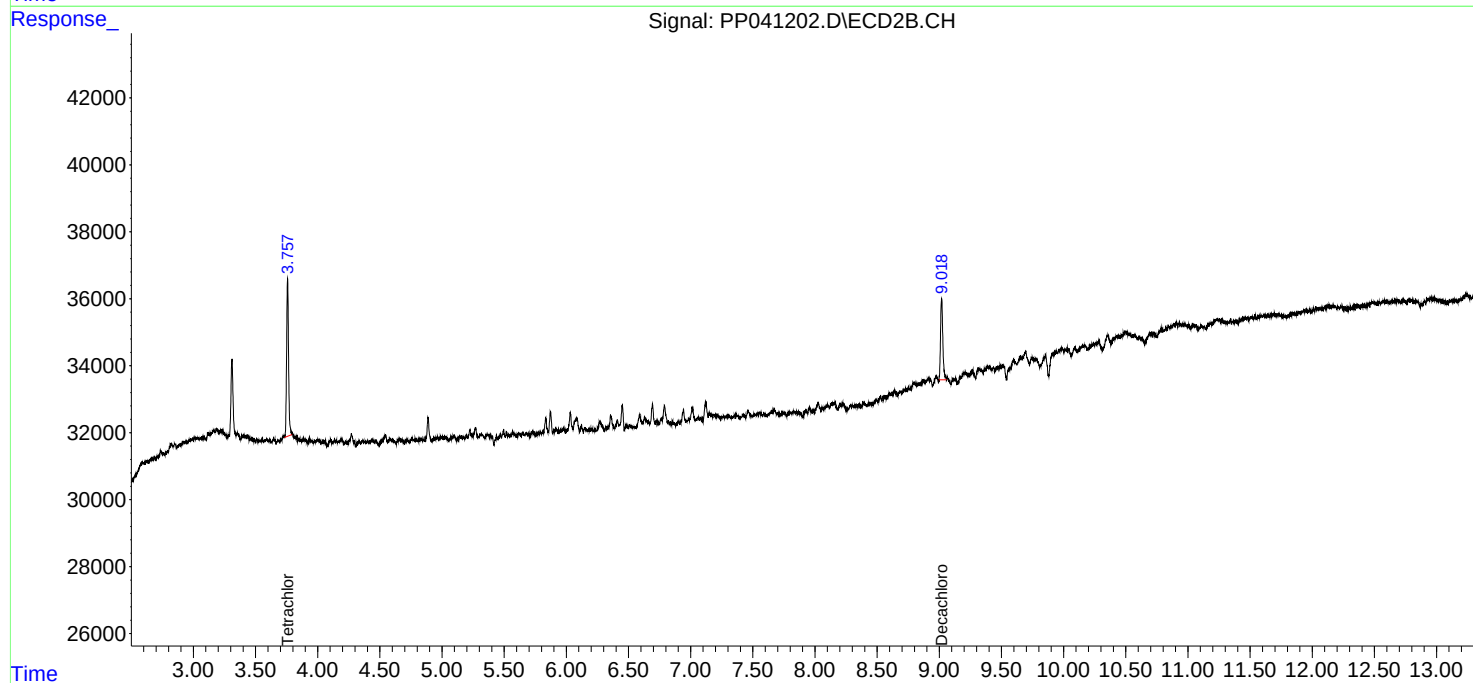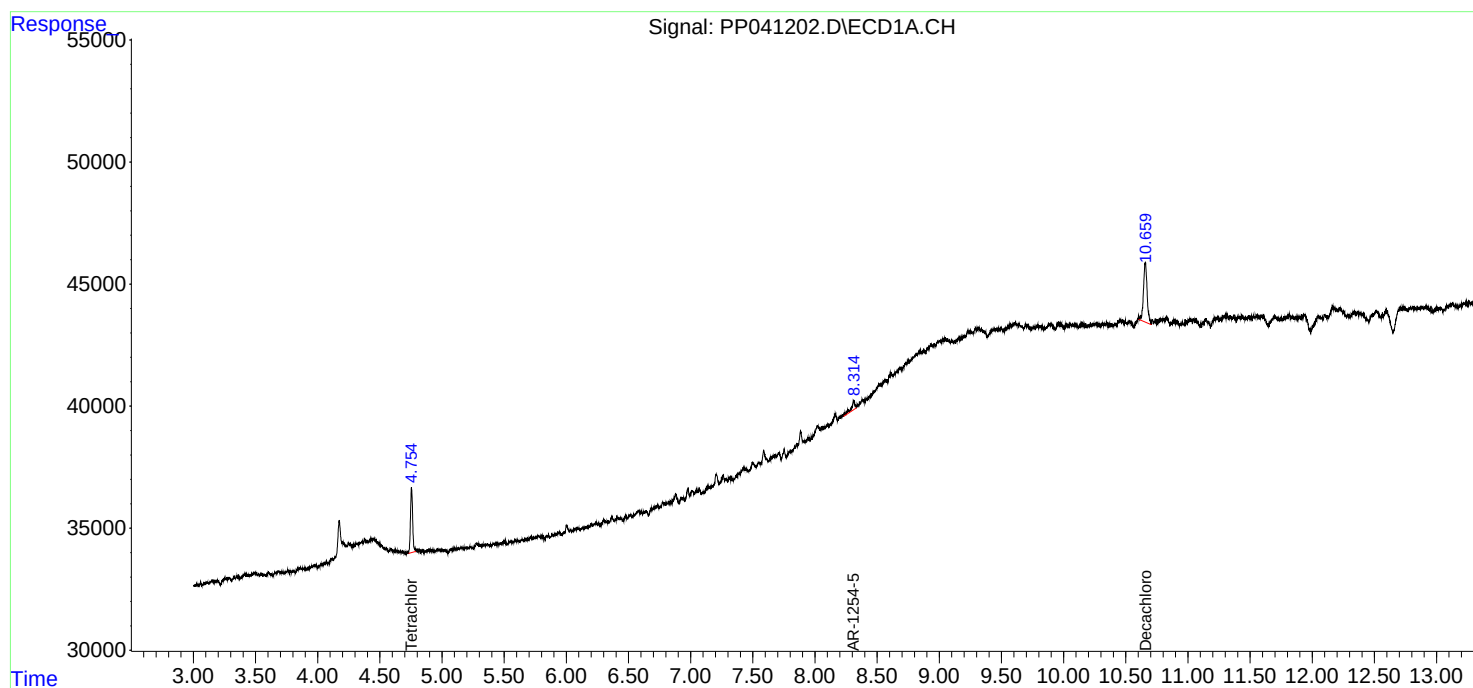


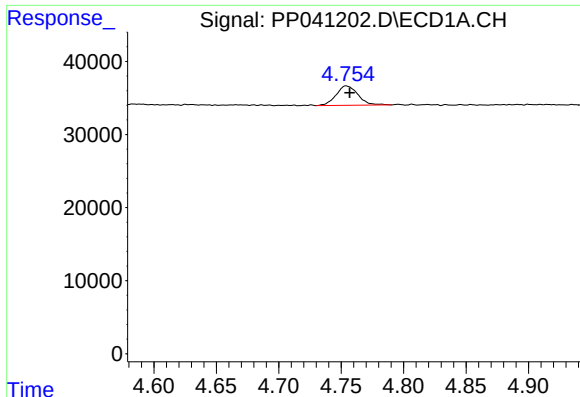

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 32495
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA-683K-1-1

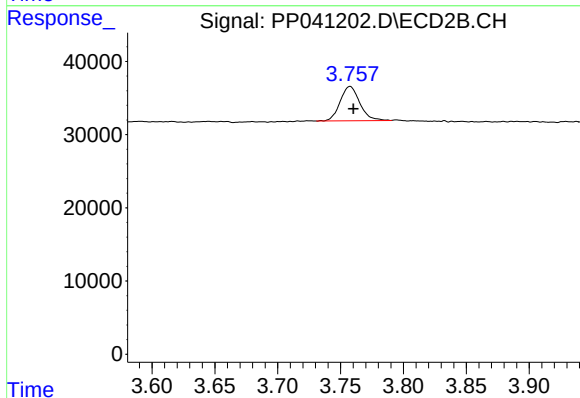


#1 Tetrachloro-m-xylene

R.T.: 3.758 min
Delta R.T.: -0.003 min
Response: 51074
Conc: 1.84 ng/ml

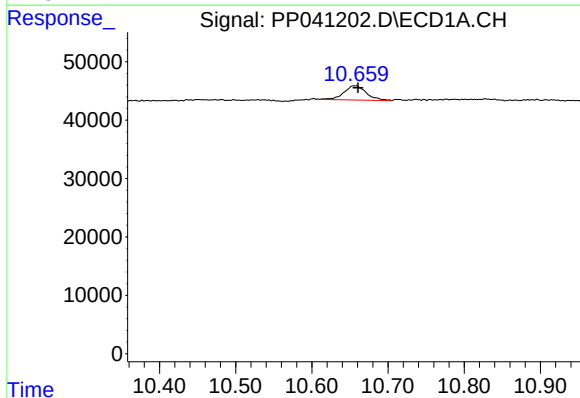


#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.002 min
Response: 50089
Conc: 2.29 ng/ml

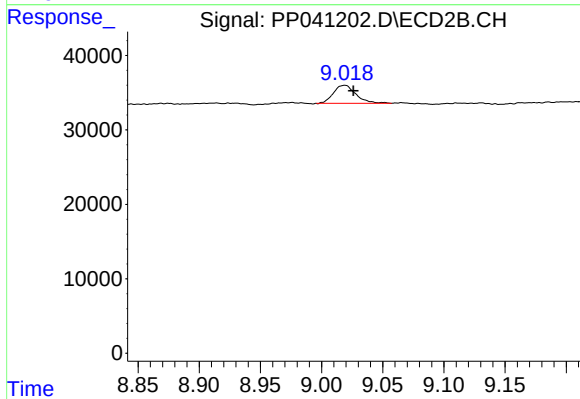

#2 Decachlorobiphenyl


R.T.: 9.019 min
Delta R.T.: -0.007 min
Response: 30954
Conc: 2.16 ng/ml

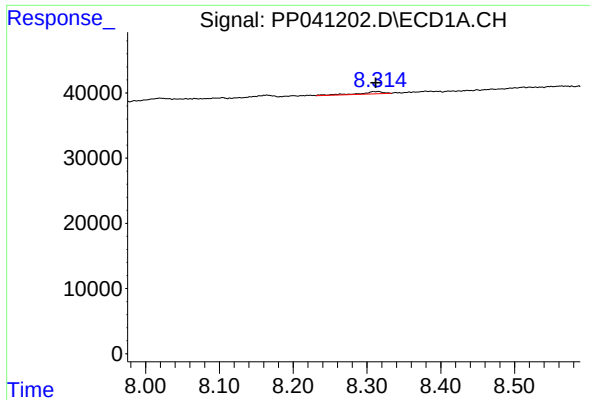

#30 AR-1254-5

R.T.: 8.315 min
Delta R.T.: 0.003 min
Response: 7814
Conc: 7.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA-683K-1-1

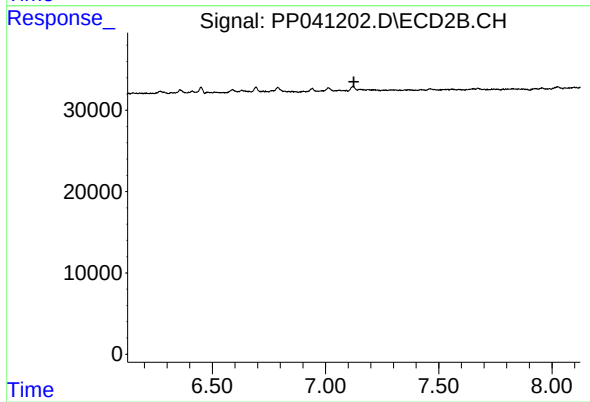

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.125 min
Response: 0
Conc: N.D.