

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112221\
 Data File : PP041218.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2021 19:54
 Operator : AJ\MA
 Sample : M4763-12 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IRV-2021-24B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 03:38:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.756	3.758	32543	54678	1.543	1.967 #
2)	SA Decachlor...	10.656	9.020	40175	34165	1.839	2.383 #
Target Compounds							
20)	L4 AR-1242-5	0.000	5.874	0	10758	N.D.	19.925 #
26)	L6 AR-1254-1	0.000	5.874	0	10758	N.D.	9.447 #
27)	L6 AR-1254-2	7.206	6.034	11335	12374	9.170	12.620 #
28)	L6 AR-1254-3	7.588	6.451	11496	16351	8.585	11.304 #
29)	L6 AR-1254-4	7.883	6.692	9751	9029	10.218	10.885
30)	L6 AR-1254-5	8.309	7.122	13614	13898	12.809	11.923
36)	L8 AR-1262-1	0.000	7.122	0	13898	N.D.	23.463 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112221\
Data File : PP041218.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2021 19:54
Operator : AJ\MA
Sample : M4763-12 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
IRV-2021-24B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 03:38:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

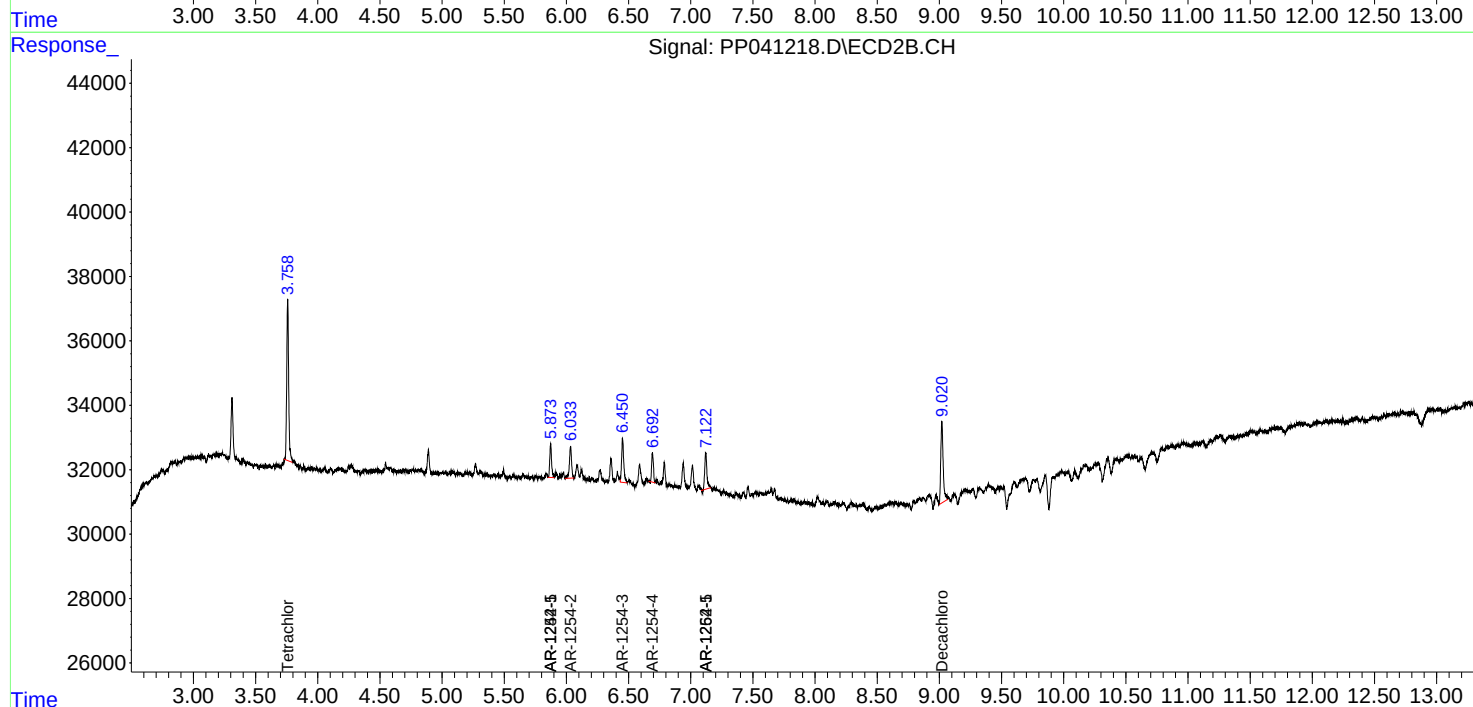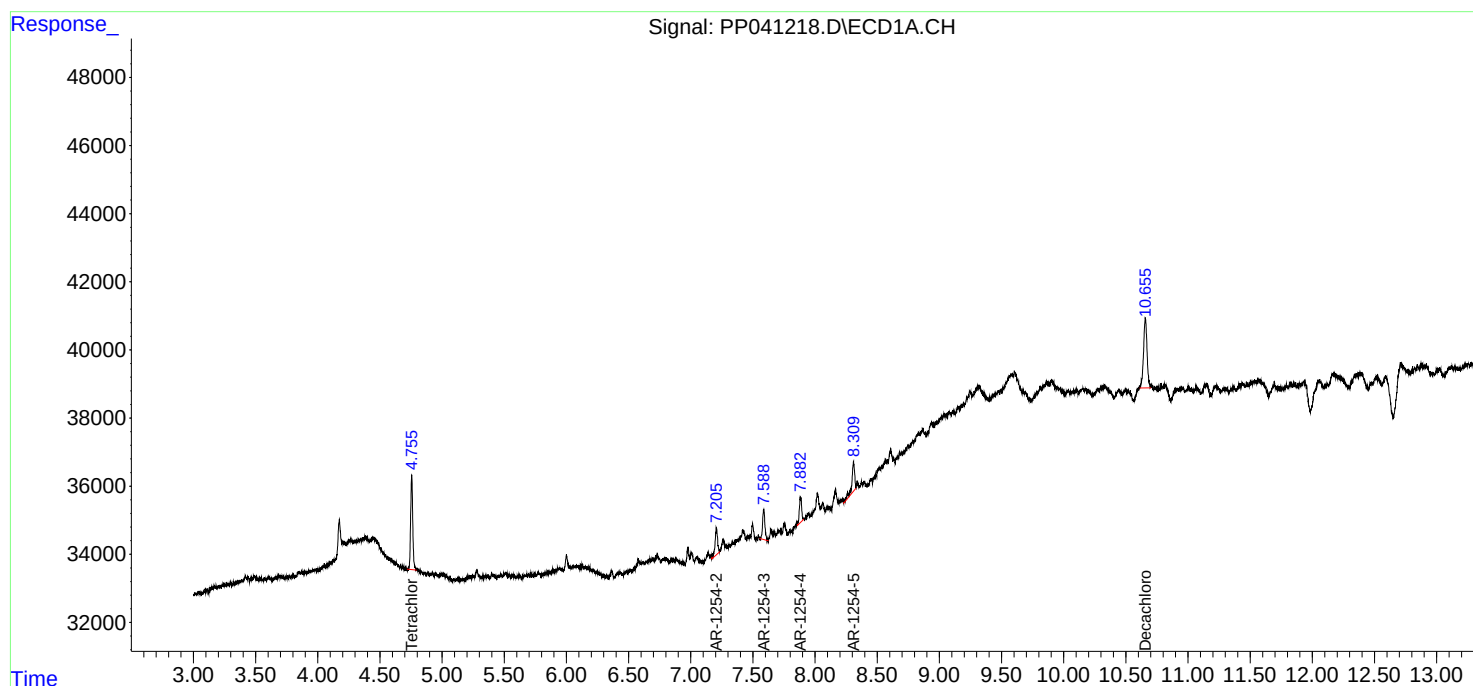


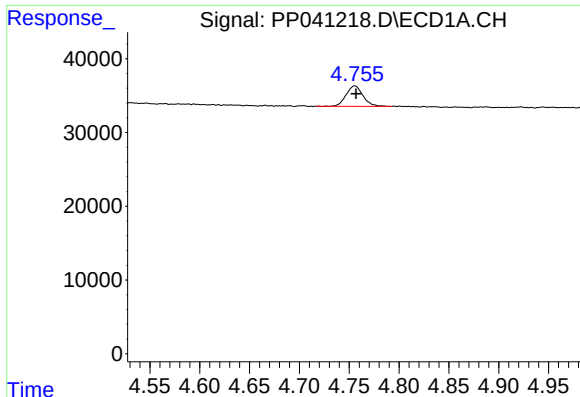

#1 Tetrachloro-m-xylene


R.T.: 4.756 min
Delta R.T.: -0.001 min
Response: 32543
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2021-24B

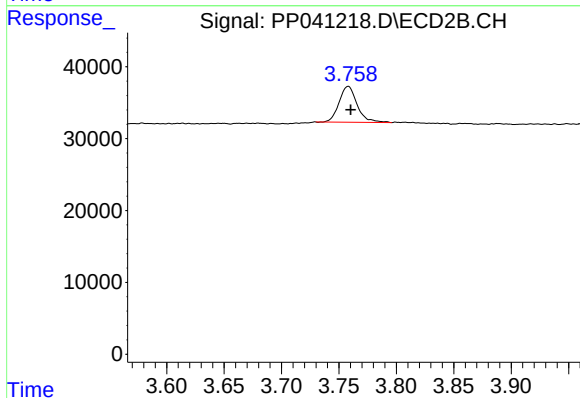


#1 Tetrachloro-m-xylene

R.T.: 3.758 min
Delta R.T.: -0.002 min
Response: 54678
Conc: 1.97 ng/ml

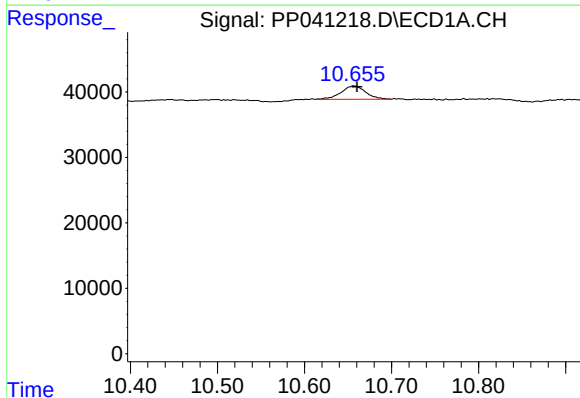


#2 Decachlorobiphenyl

R.T.: 10.656 min
Delta R.T.: -0.004 min
Response: 40175
Conc: 1.84 ng/ml

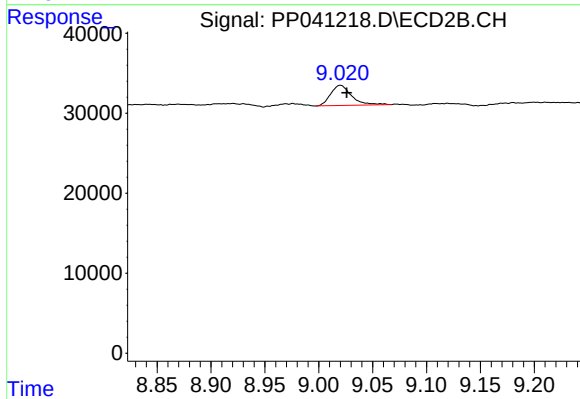

#2 Decachlorobiphenyl


R.T.: 9.020 min
Delta R.T.: -0.006 min
Response: 34165
Conc: 2.38 ng/ml

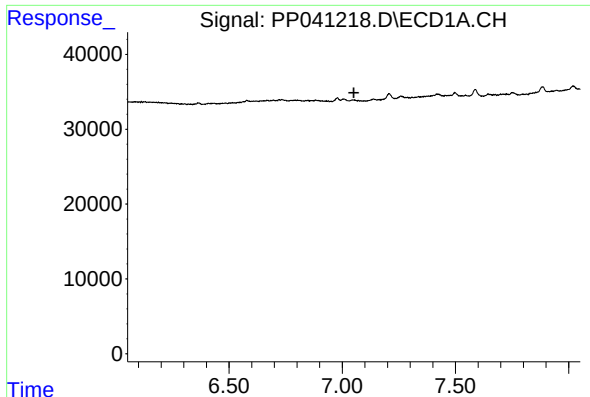

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
IRV-2021-24B

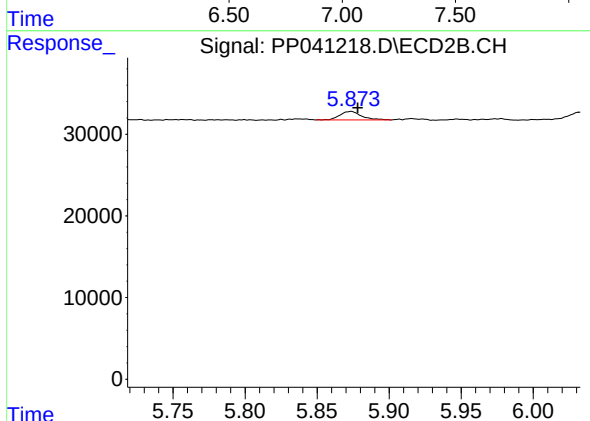


#20 AR-1242-5

R.T.: 5.874 min
Delta R.T.: -0.004 min
Response: 10758
Conc: 19.93 ng/ml

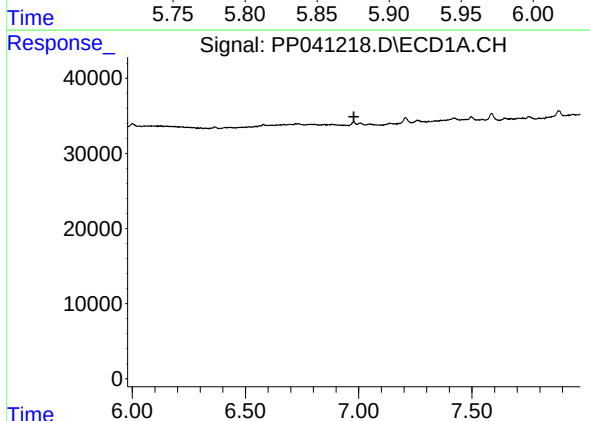


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.979 min
Response: 0
Conc: N.D.

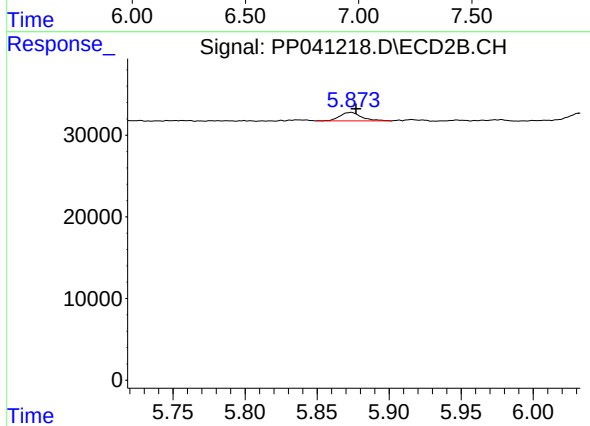

#26 AR-1254-1


R.T.: 5.874 min
Delta R.T.: -0.003 min
Response: 10758
Conc: 9.45 ng/ml

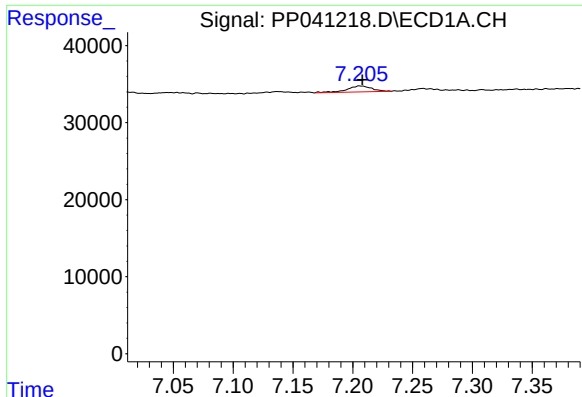

#27 AR-1254-2


R.T.: 7.206 min
Delta R.T.: -0.002 min
Response: 11335
Conc: 9.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2021-24B

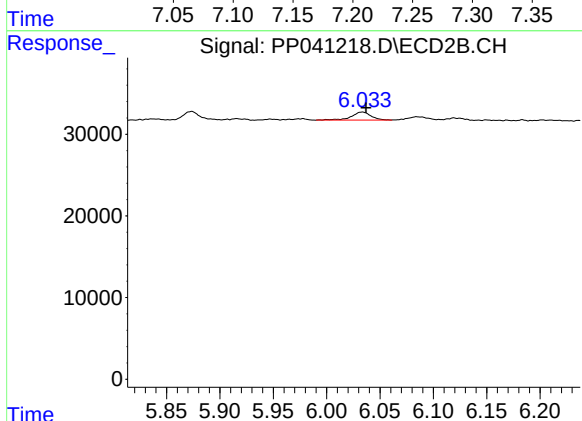


#27 AR-1254-2

R.T.: 6.034 min
Delta R.T.: -0.003 min
Response: 12374
Conc: 12.62 ng/ml

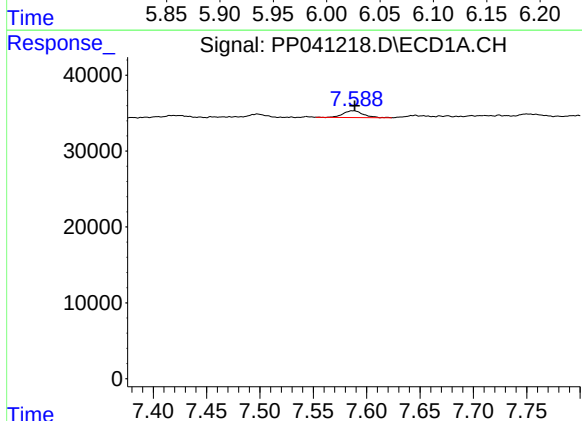


#28 AR-1254-3

R.T.: 7.588 min
Delta R.T.: 0.000 min
Response: 11496
Conc: 8.59 ng/ml

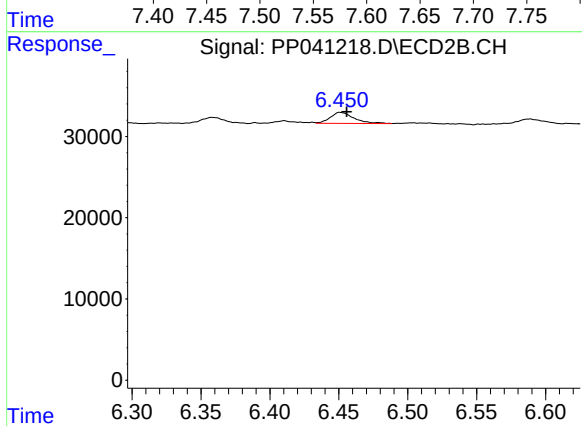

#28 AR-1254-3


R.T.: 6.451 min
Delta R.T.: -0.005 min
Response: 16351
Conc: 11.30 ng/ml

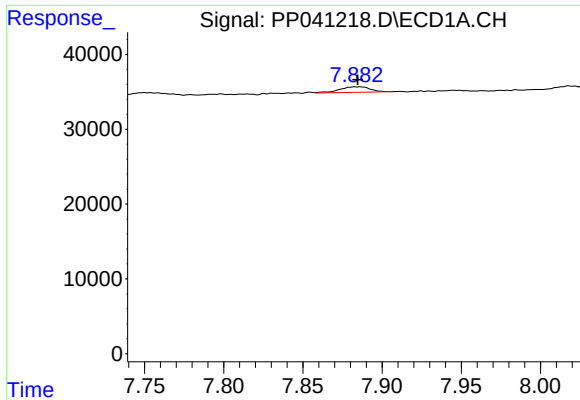

#29 AR-1254-4


R.T.: 7.883 min
Delta R.T.: -0.002 min
Response: 9751
Conc: 10.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2021-24B

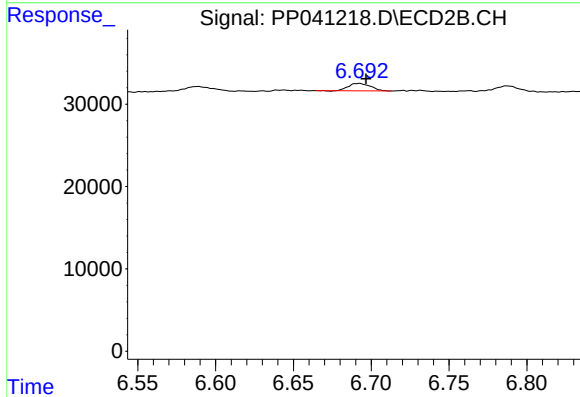


#29 AR-1254-4

R.T.: 6.692 min
Delta R.T.: -0.004 min
Response: 9029
Conc: 10.89 ng/ml

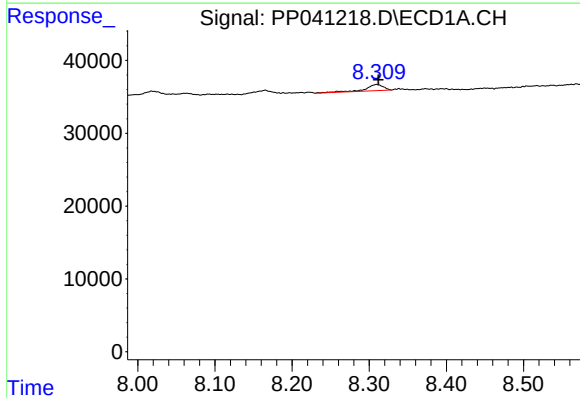


#30 AR-1254-5

R.T.: 8.309 min
Delta R.T.: -0.002 min
Response: 13614
Conc: 12.81 ng/ml

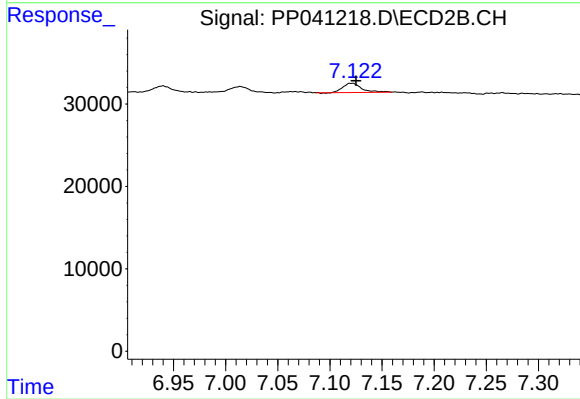

#30 AR-1254-5


R.T.: 7.122 min
Delta R.T.: -0.003 min
Response: 13898
Conc: 11.92 ng/ml

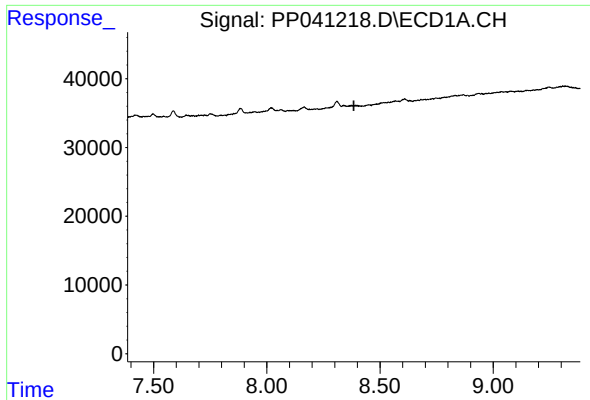

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.384 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
IRV-2021-24B

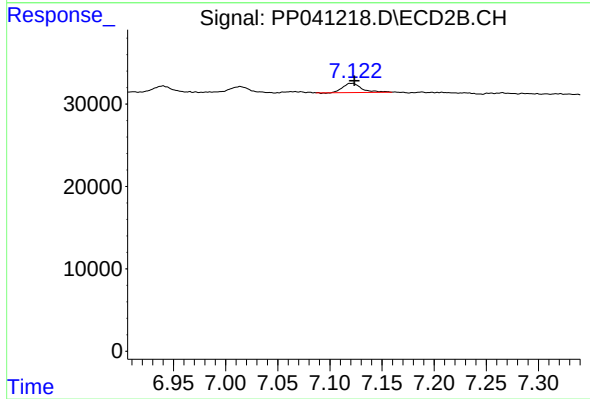

#36 AR-1262-1

R.T.: 7.122 min
Delta R.T.: -0.001 min
Response: 13898
Conc: 23.46 ng/ml