

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112222\
 Data File : PP053427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 15:33
 Operator : YP\AJ
 Sample : N5751-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 STOCK-PILE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2022
 Supervised By :Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:50:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 09 05:50:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.647	38703823	32663726	20.134	21.714
2) SA Decachlor...	10.205	8.725	34871472	52783307	25.717	28.161
Target Compounds						
31) L7 AR-1260-1	7.188	6.249	10008040	13149462	122.389	143.444
32) L7 AR-1260-2	7.443	6.441	18421578	16587537	198.920	144.149 #
33) L7 AR-1260-3	7.806	6.594	9409904	11807876	150.876	110.037 #
34) L7 AR-1260-4	8.031	7.071	13084820	9899588	174.666m	119.656 #
35) L7 AR-1260-5	8.356	7.315	18931940	20433349	149.581	107.911 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112222\
Data File : PP053427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 15:33
Operator : YP\AJ
Sample : N5751-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:50:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 09 05:50:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

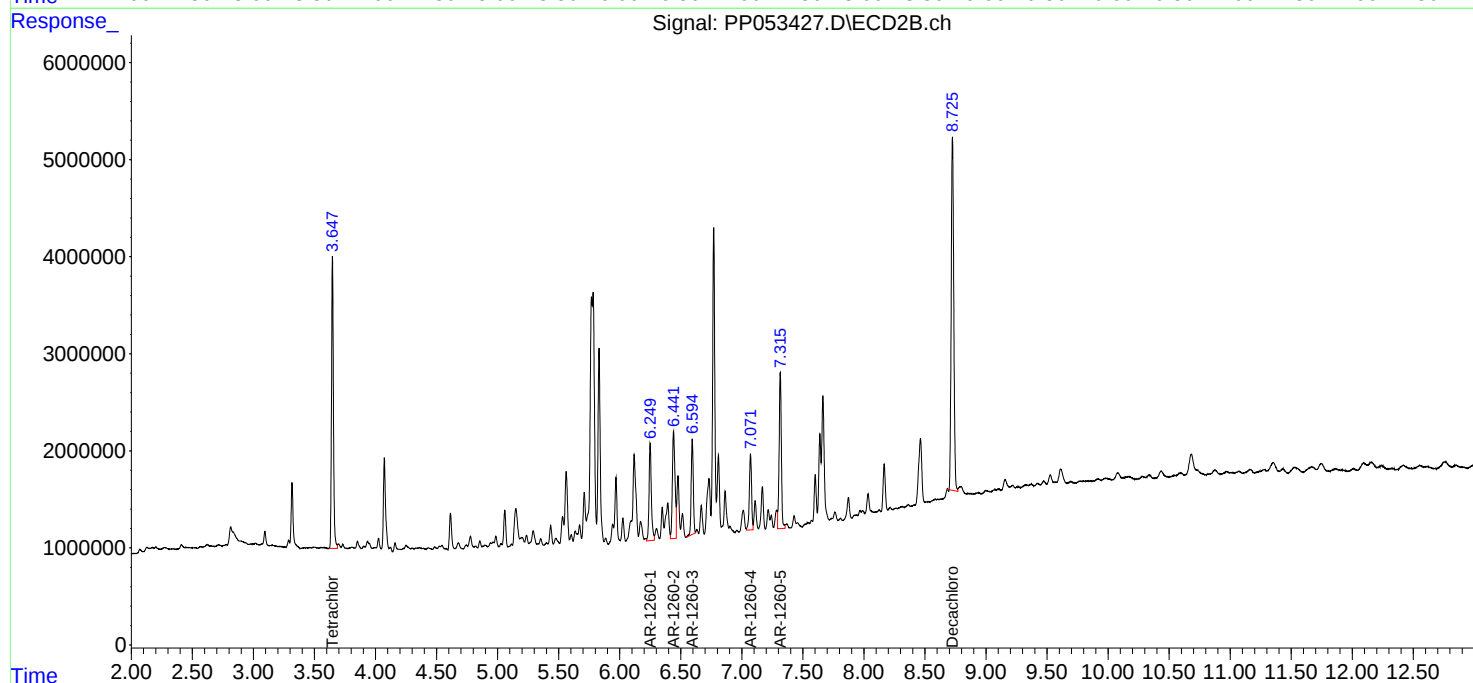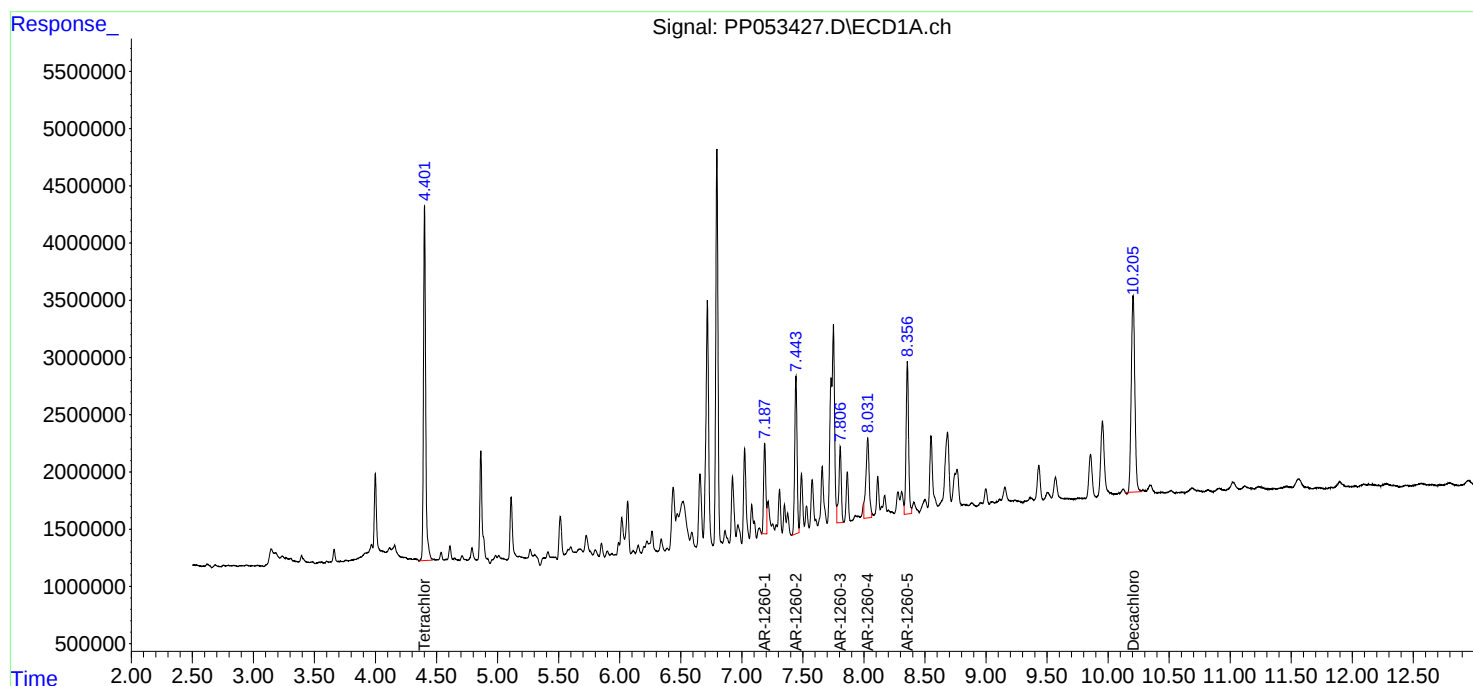

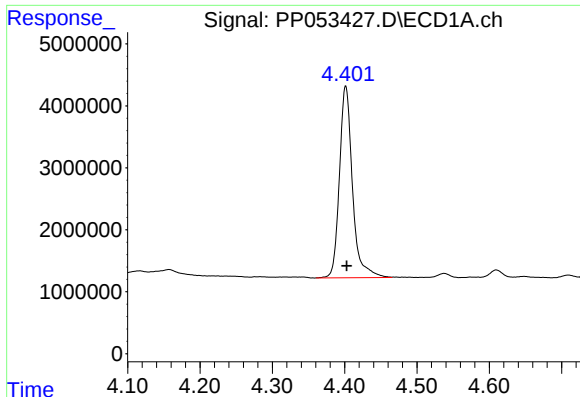


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: -0.001 min
Response: 38703823
Conc: 20.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

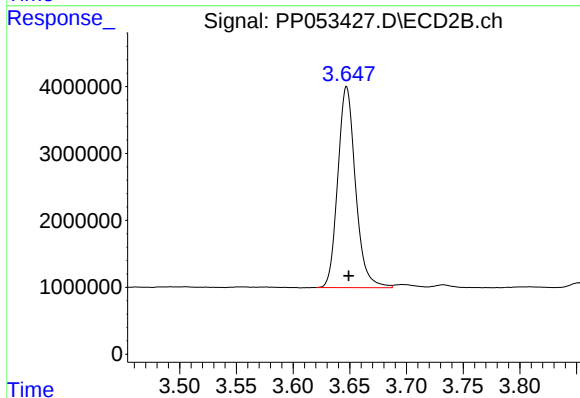


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 32663726
Conc: 21.71 ng/ml

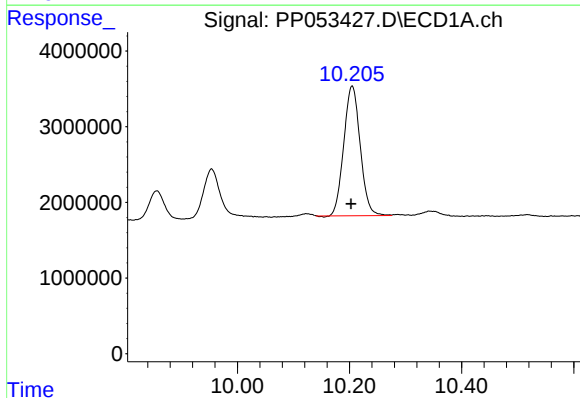


#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.002 min
Response: 34871472
Conc: 25.72 ng/ml

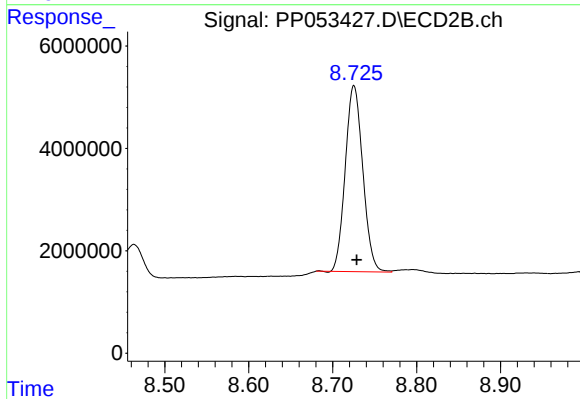

#2 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.003 min
Response: 52783307
Conc: 28.16 ng/ml

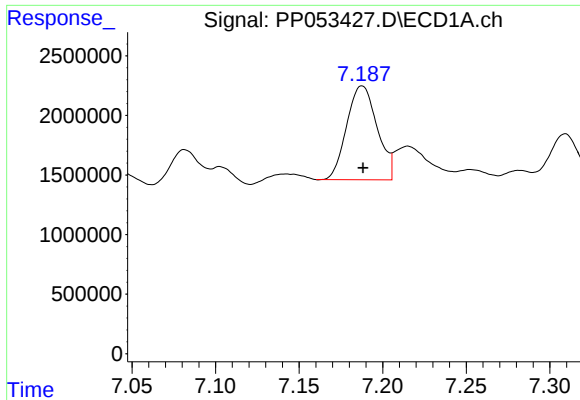


#31 AR-1260-1

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 10008040
Conc: 122.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

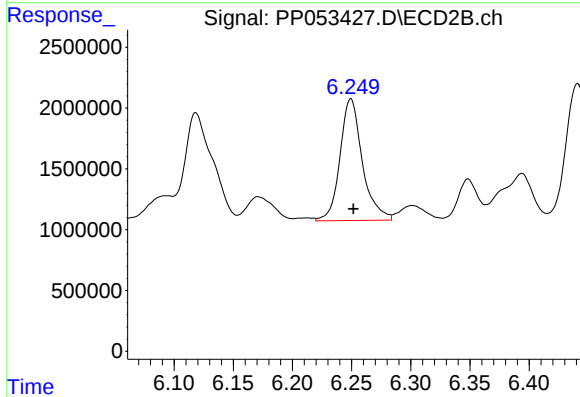


#31 AR-1260-1

R.T.: 6.249 min
Delta R.T.: -0.002 min
Response: 13149462
Conc: 143.44 ng/ml

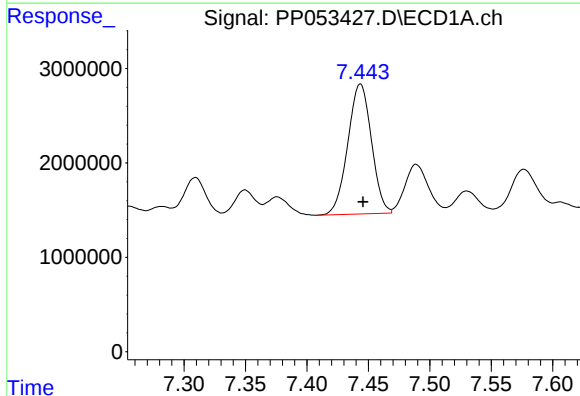


#32 AR-1260-2

R.T.: 7.443 min
Delta R.T.: -0.002 min
Response: 18421578
Conc: 198.92 ng/ml

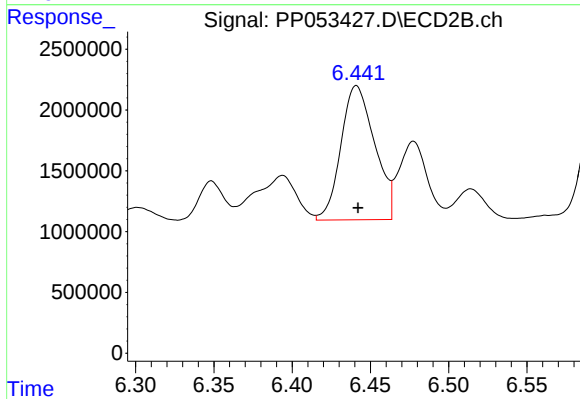

#32 AR-1260-2

R.T.: 6.441 min
Delta R.T.: -0.001 min
Response: 16587537
Conc: 144.15 ng/ml

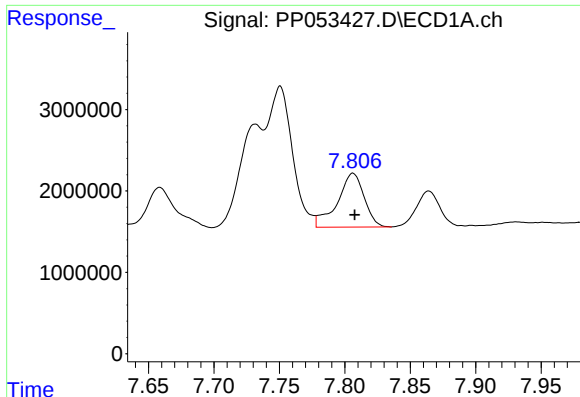


#33 AR-1260-3

R.T.: 7.806 min
Delta R.T.: -0.001 min
Response: 9409904
Conc: 150.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

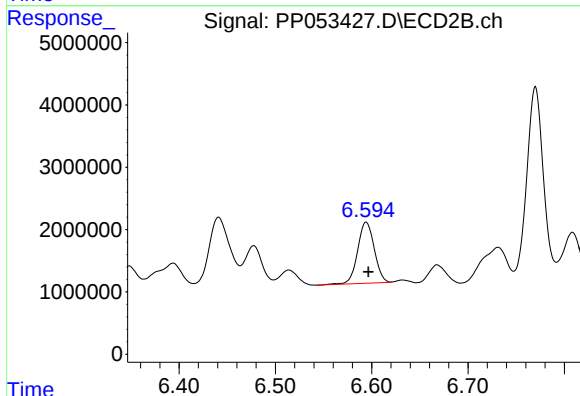


#33 AR-1260-3

R.T.: 6.594 min
Delta R.T.: -0.002 min
Response: 11807876
Conc: 110.04 ng/ml

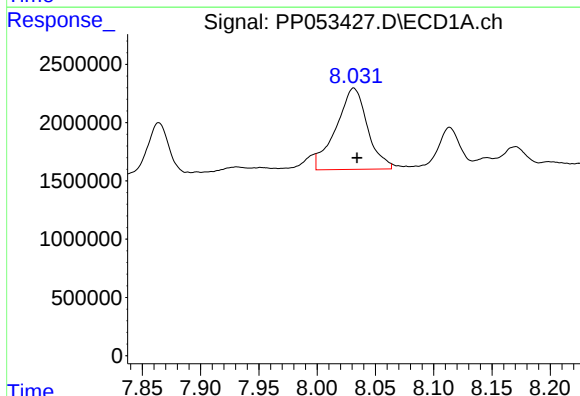


#34 AR-1260-4

R.T.: 8.031 min
Delta R.T.: -0.003 min
Response: 13084820
Conc: 174.67 ng/ml m

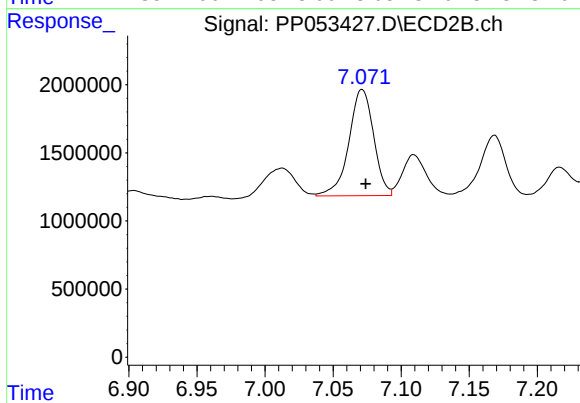

#34 AR-1260-4

R.T.: 7.071 min
Delta R.T.: -0.003 min
Response: 9899588
Conc: 119.66 ng/ml

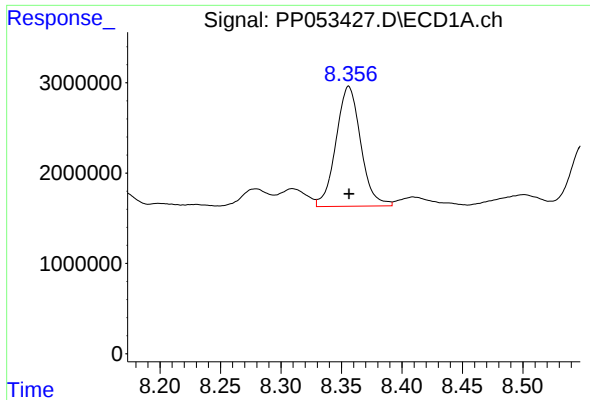


#35 AR-1260-5

R.T.: 8.356 min
Delta R.T.: 0.000 min
Response: 18931940
Conc: 149.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
STOCK-PILE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

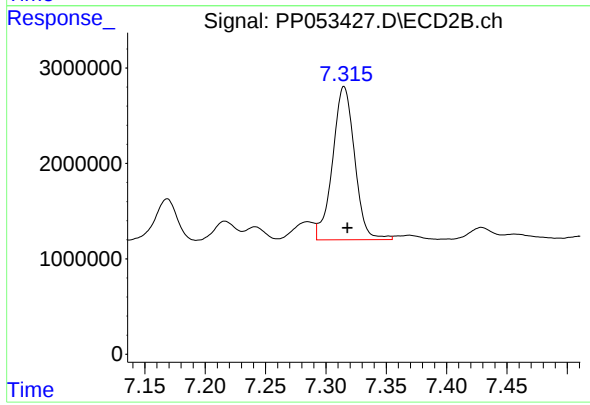

#35 AR-1260-5

R.T.: 7.315 min
Delta R.T.: -0.003 min
Response: 20433349
Conc: 107.91 ng/ml