

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031549.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 11:35
 Operator : DD\AJ
 Sample : L4809-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-CON-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 12:10:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.791	4.064	1136799	1050781	23.476	21.928
2)	SA Decachlor...	10.669	9.372	813721	806228	23.958	21.774
Target Compounds							
3)	L1 AR-1016-1	6.120f	5.322	92165	18107	60.803	12.253 #
4)	L1 AR-1016-2	6.120	5.341	92165	78134	40.816	35.935
5)	L1 AR-1016-3	0.000	5.533	0	54253	N.D.	46.419 #
6)	L1 AR-1016-4	6.290	5.584	51980	59278	44.733	67.911 #
7)	L1 AR-1016-5	6.605	5.812	103129	107252	93.562	94.296
9)	L2 AR-1221-2	0.000	4.418	0	17641	N.D.	45.731 #
10)	L2 AR-1221-3	0.000	4.510	0	6711	N.D.	5.564 #
11)	L3 AR-1232-1	0.000	4.510	0	6711	N.D.	6.459 #
12)	L3 AR-1232-2	0.000	5.341	0	78134	N.D.	80.234 #
13)	L3 AR-1232-3	6.120	5.533	92165	54253	91.261	102.872
14)	L3 AR-1232-4	6.290	5.628	51980	74250	98.034	175.812 #
15)	L3 AR-1232-5	6.391	5.812	60828	107252	189.357	370.108 #
16)	L4 AR-1242-1	6.120f	5.322	92165	18107	77.016	15.861 #
17)	L4 AR-1242-2	6.120	5.341	92165	78134	51.799	46.461
18)	L4 AR-1242-3	0.000	5.533	0	54253	N.D.	59.414 #
19)	L4 AR-1242-4	6.290	5.628	51980	74250	56.243	88.392 #
20)	L4 AR-1242-5	7.070	6.192	155686	156763	169.938	151.941
21)	L5 AR-1248-1	6.120f	5.322	92165	18107	99.808	21.022 #
22)	L5 AR-1248-2	6.391	5.584	60828	59278	51.425	49.646
23)	L5 AR-1248-3	6.605	5.628	103129	74250	70.495	58.662
24)	L5 AR-1248-4	7.031	5.812	127530	107252	81.323	70.005
25)	L5 AR-1248-5	7.070	6.235	155686	140284	98.071	96.150
26)	L6 AR-1254-1	7.000	6.192	107162	156763	70.323	72.468
27)	L6 AR-1254-2	7.233	6.351	177435	50805	76.401	27.271 #
28)	L6 AR-1254-3	7.609	6.771	110904	113685	43.899	36.776
29)	L6 AR-1254-4	7.905	7.010	78754	81573	46.413	48.015
30)	L6 AR-1254-5	0.000	7.439	0	38329	N.D.	14.198 #
31)	L7 AR-1260-1	0.000	6.920	0	58140	N.D.	29.422 #
32)	L7 AR-1260-2	0.000	7.105	0	14658	N.D.	6.019 #
33)	L7 AR-1260-3	0.000	7.259	0	22014	N.D.	9.640 #
34)	L7 AR-1260-4	0.000	7.745	0	10586	N.D.	5.571 #
35)	L7 AR-1260-5	0.000	7.989	0	37018	N.D.	8.157 #
36)	L8 AR-1262-1	0.000	7.477	0	14575	N.D.	5.670 #
37)	L8 AR-1262-2	0.000	7.989	0	37018	N.D.	8.216 #
38)	L8 AR-1262-3	0.000	8.275	0	21802	N.D.	12.754 #
39)	L8 AR-1262-4	0.000	8.338	0	30041	N.D.	8.723 #
40)	L8 AR-1262-5	0.000	8.837	0	19689	N.D.	12.346 #
41)	L9 AR-1268-1	0.000	8.275	0	21802	N.D.	3.940 #
42)	L9 AR-1268-2	0.000	8.338	0	30041	N.D.	5.556 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031549.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 11:35
 Operator : DD\AJ
 Sample : L4809-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-CON-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 12:10:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.548	0	3825	N.D.	0.834 #
44) L9	AR-1268-4	0.000	8.837	0	19689	N.D.	10.802 #
45) L9	AR-1268-5	0.000	9.123	0	12720	N.D.	0.919 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031549.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 11:35
Operator : DD\AJ
Sample : L4809-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
MS-CON-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 12:10:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

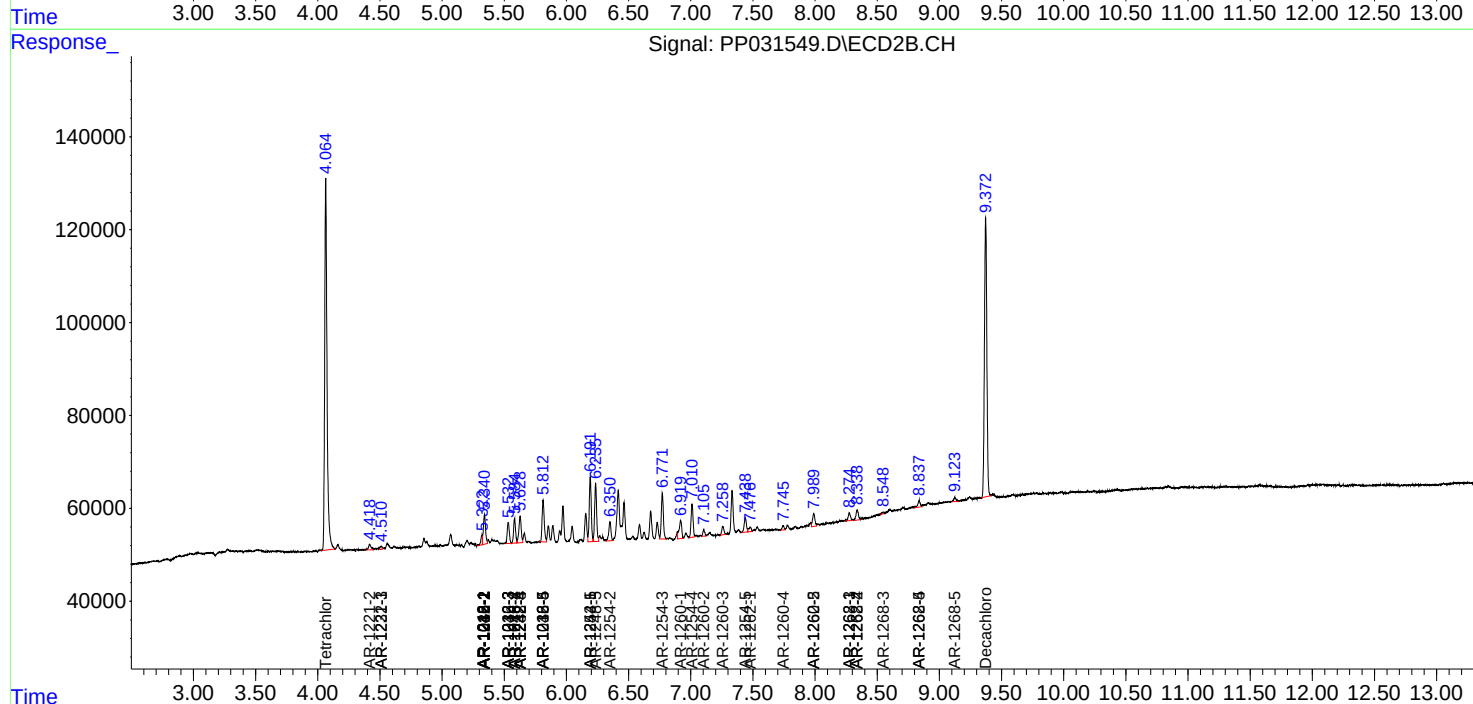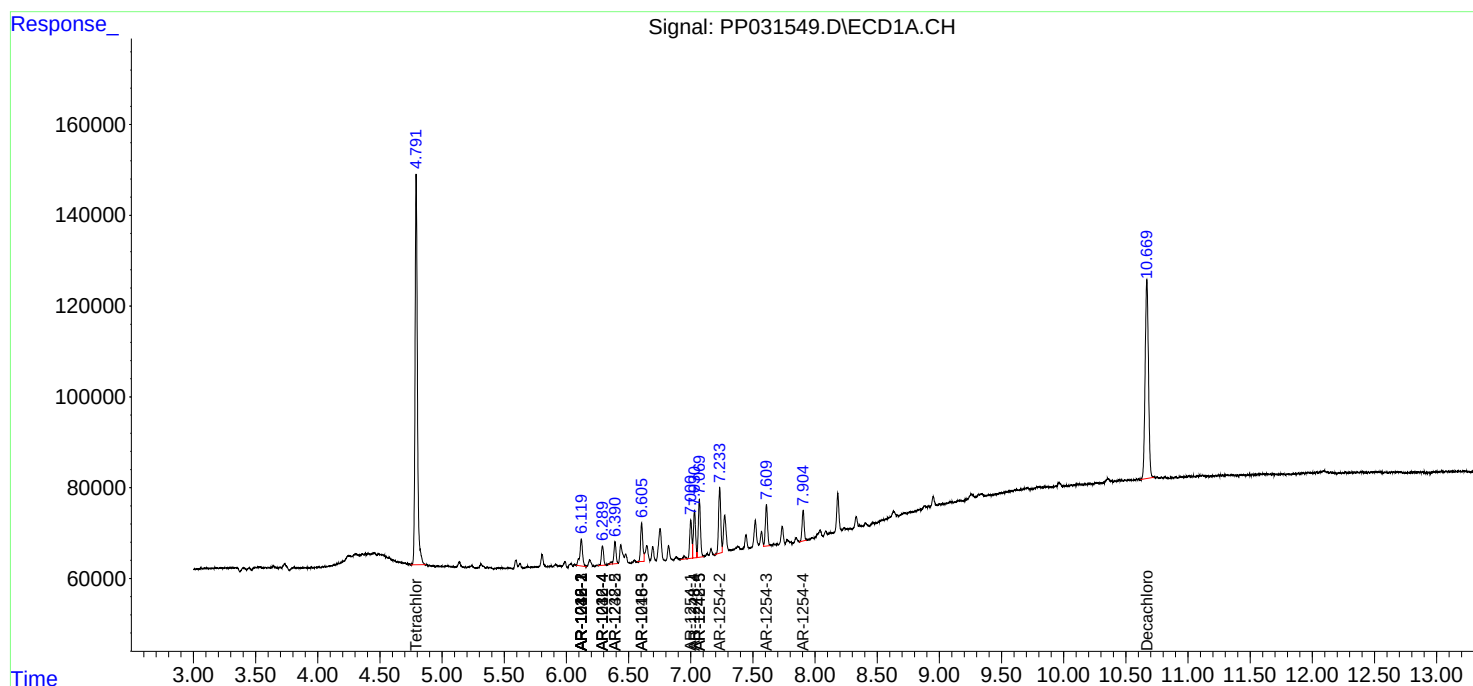


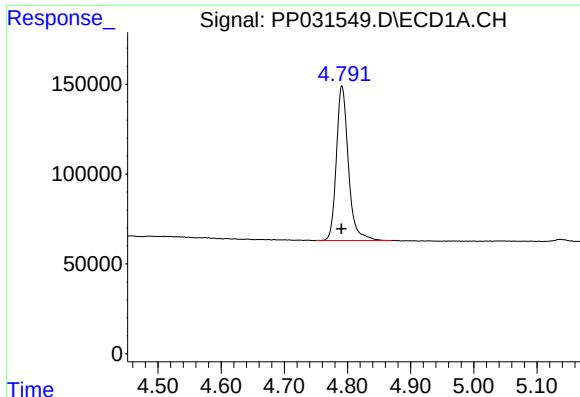

#1 Tetrachloro-m-xylene


R.T.: 4.791 min
Delta R.T.: 0.001 min
Response: 1136799
Conc: 23.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

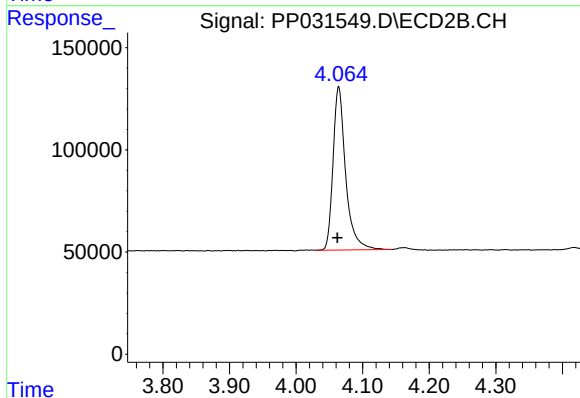


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.002 min
Response: 1050781
Conc: 21.93 ng/ml

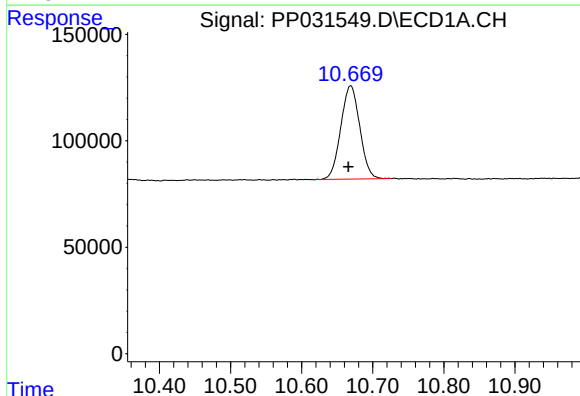


#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: 0.003 min
Response: 813721
Conc: 23.96 ng/ml

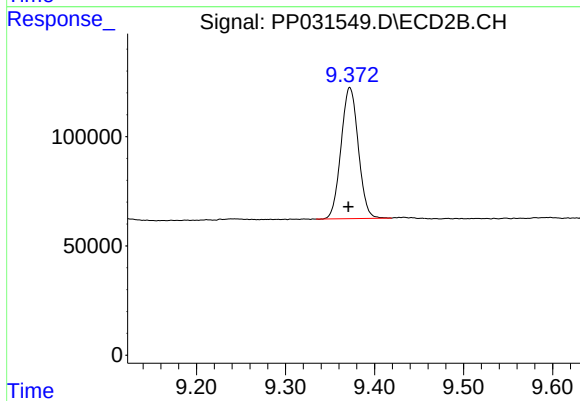

#2 Decachlorobiphenyl


R.T.: 9.372 min
Delta R.T.: 0.002 min
Response: 806228
Conc: 21.77 ng/ml

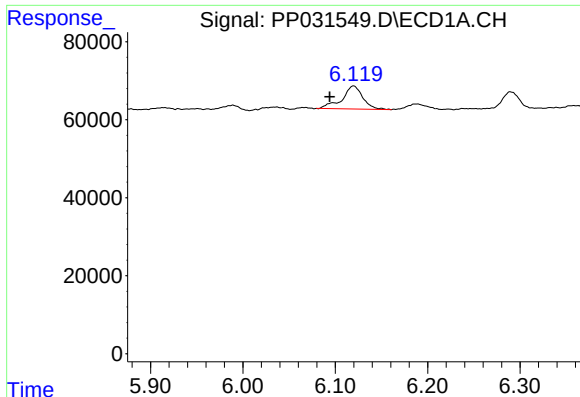

#3 AR-1016-1


R.T.: 6.120 min
Delta R.T.: 0.026 min
Response: 92165
Conc: 60.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

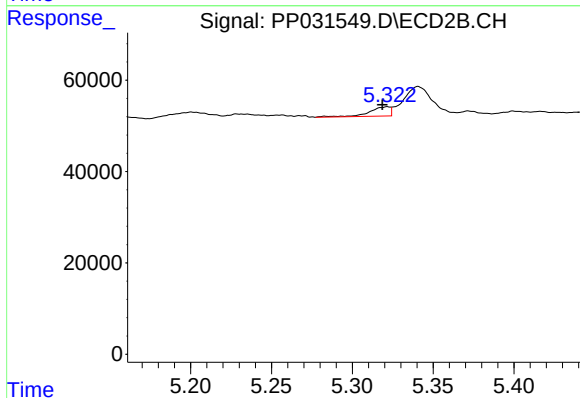


#3 AR-1016-1

R.T.: 5.322 min
Delta R.T.: 0.003 min
Response: 18107
Conc: 12.25 ng/ml

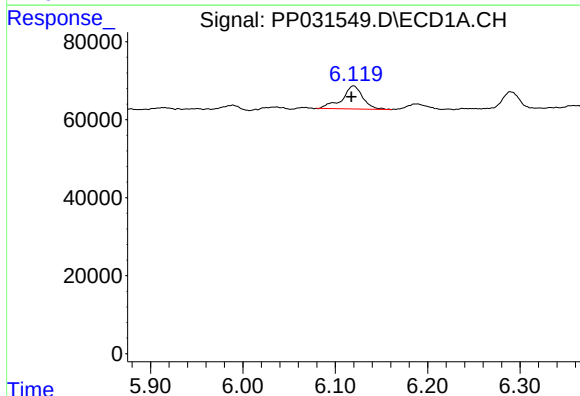


#4 AR-1016-2

R.T.: 6.120 min
Delta R.T.: 0.002 min
Response: 92165
Conc: 40.82 ng/ml

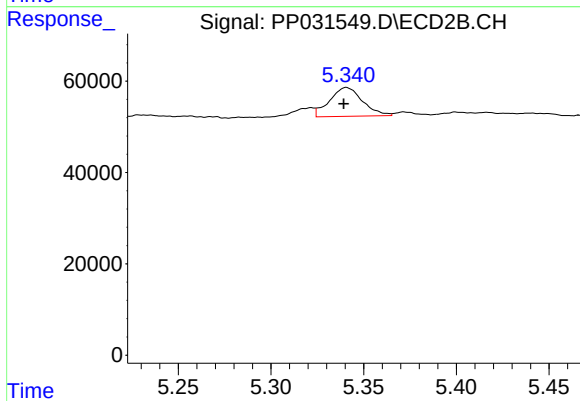

#4 AR-1016-2


R.T.: 5.341 min
Delta R.T.: 0.002 min
Response: 78134
Conc: 35.94 ng/ml

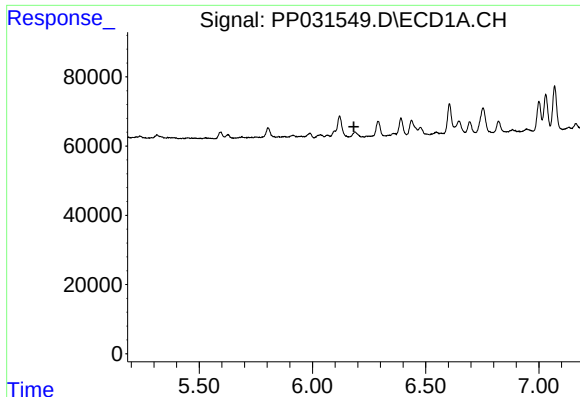

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

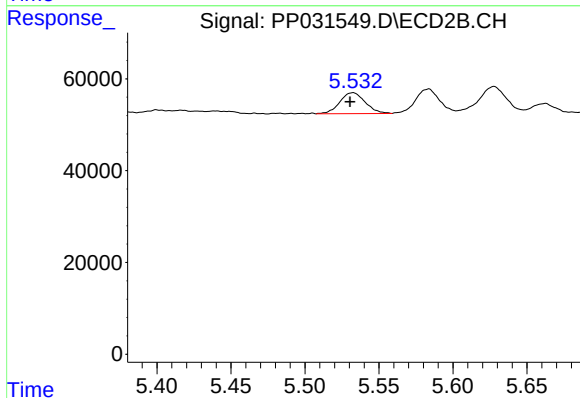


#5 AR-1016-3

R.T.: 5.533 min
Delta R.T.: 0.002 min
Response: 54253
Conc: 46.42 ng/ml

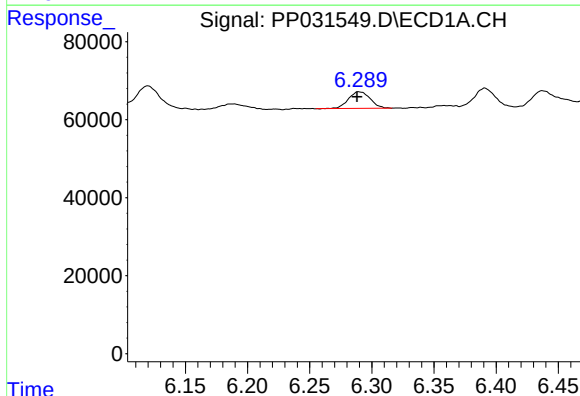


#6 AR-1016-4

R.T.: 6.290 min
Delta R.T.: 0.002 min
Response: 51980
Conc: 44.73 ng/ml

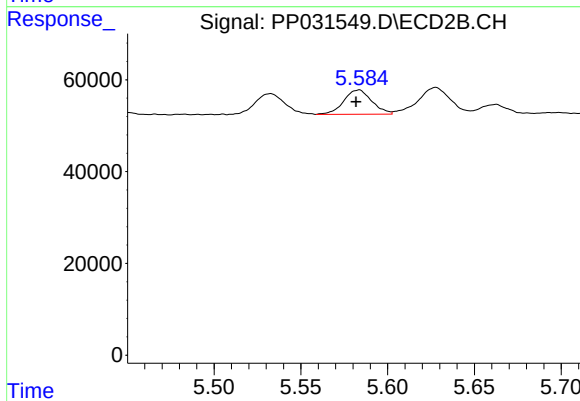

#6 AR-1016-4


R.T.: 5.584 min
Delta R.T.: 0.002 min
Response: 59278
Conc: 67.91 ng/ml

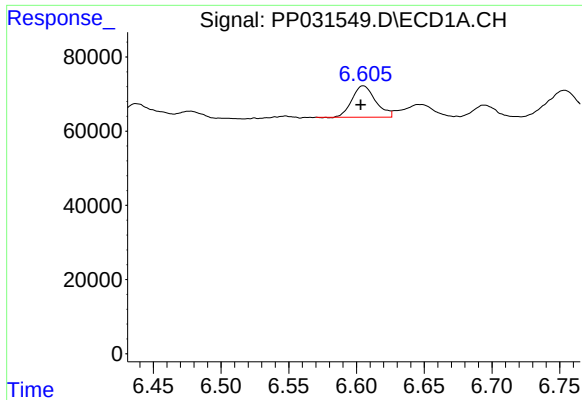

#7 AR-1016-5


R.T.: 6.605 min
Delta R.T.: 0.002 min
Response: 103129
Conc: 93.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

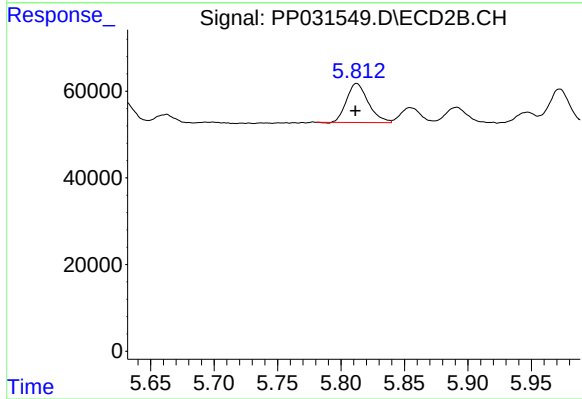


#7 AR-1016-5

R.T.: 5.812 min
Delta R.T.: 0.001 min
Response: 107252
Conc: 94.30 ng/ml

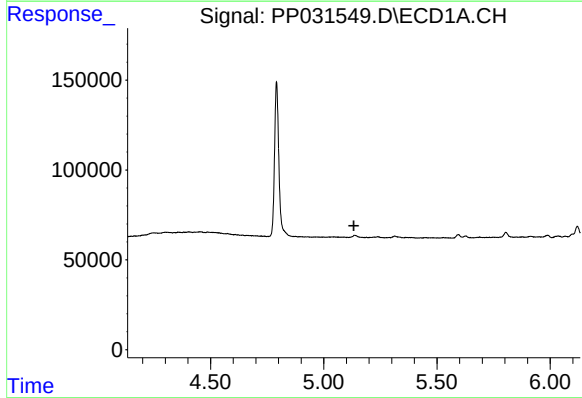


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

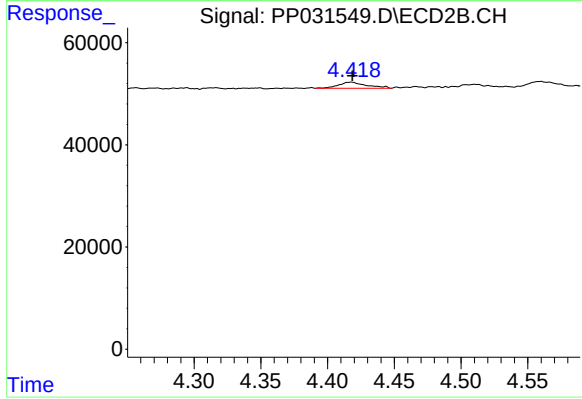

#9 AR-1221-2


R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 17641
Conc: 45.73 ng/ml

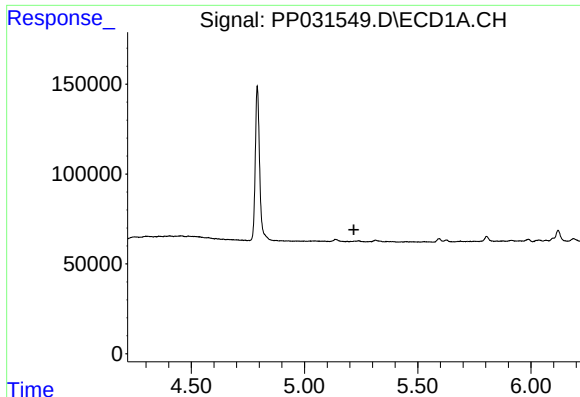

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

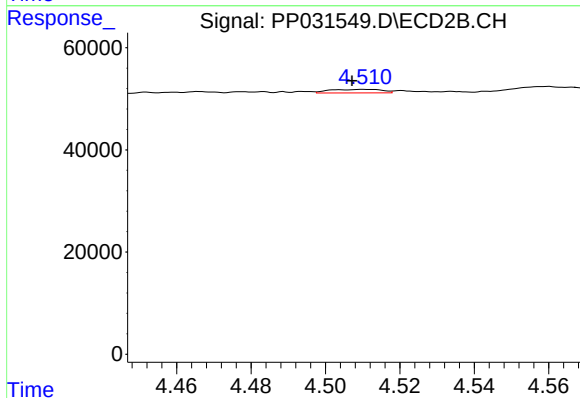


#10 AR-1221-3

R.T.: 4.510 min
Delta R.T.: 0.003 min
Response: 6711
Conc: 5.56 ng/ml

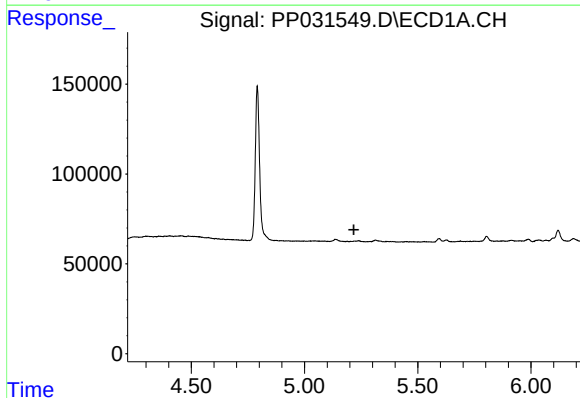


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

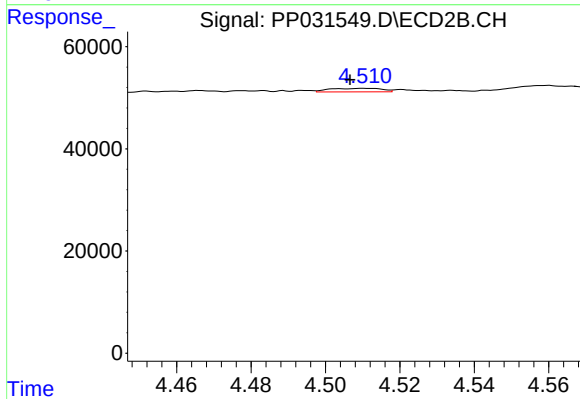

#11 AR-1232-1


R.T.: 4.510 min
Delta R.T.: 0.004 min
Response: 6711
Conc: 6.46 ng/ml

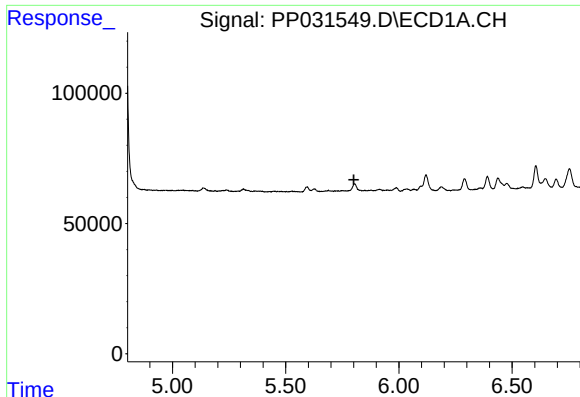

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

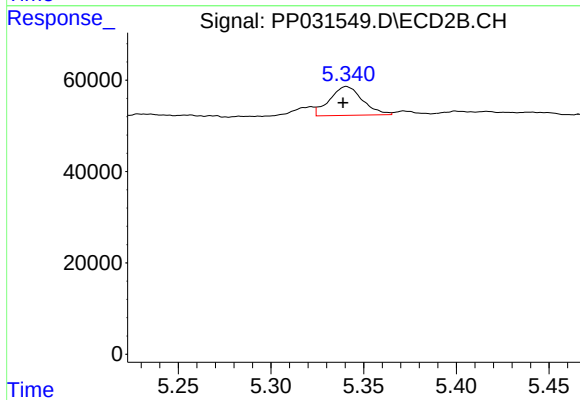


#12 AR-1232-2

R.T.: 5.341 min
Delta R.T.: 0.002 min
Response: 78134
Conc: 80.23 ng/ml

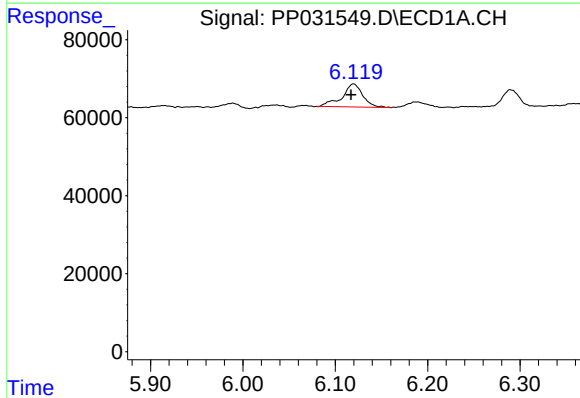


#13 AR-1232-3

R.T.: 6.120 min
Delta R.T.: 0.003 min
Response: 92165
Conc: 91.26 ng/ml

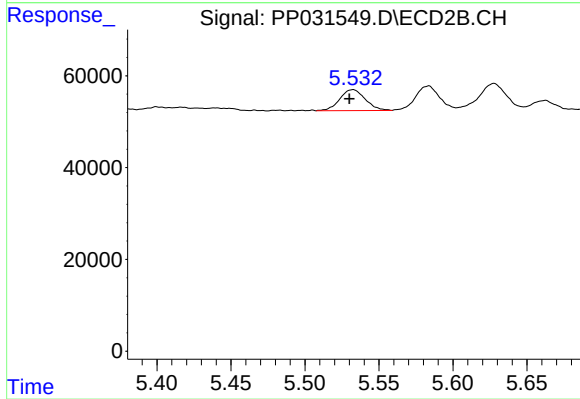

#13 AR-1232-3


R.T.: 5.533 min
Delta R.T.: 0.003 min
Response: 54253
Conc: 102.87 ng/ml

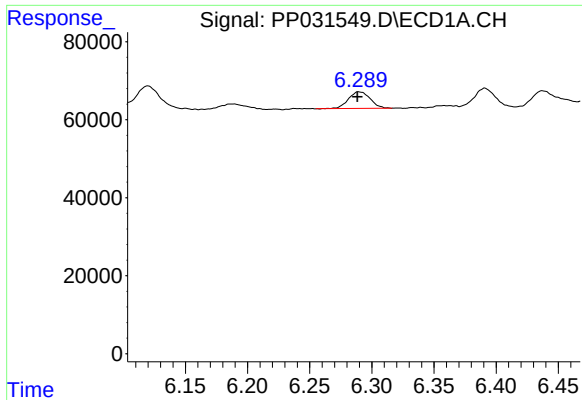

#14 AR-1232-4


R.T.: 6.290 min
Delta R.T.: 0.001 min
Response: 51980
Conc: 98.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

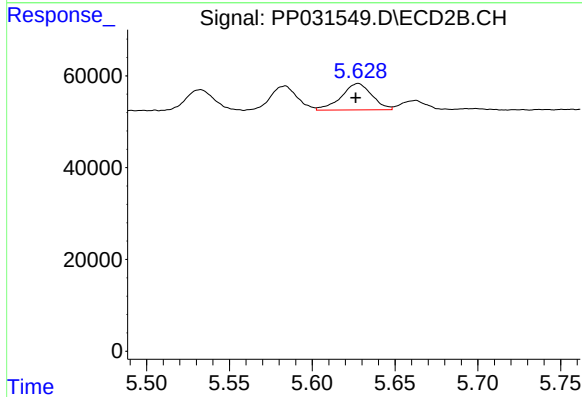


#14 AR-1232-4

R.T.: 5.628 min
Delta R.T.: 0.002 min
Response: 74250
Conc: 175.81 ng/ml

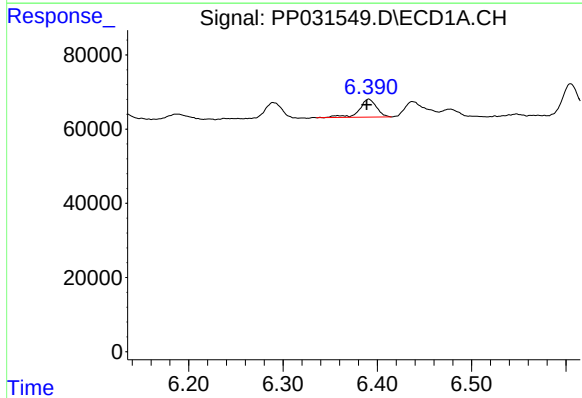


#15 AR-1232-5

R.T.: 6.391 min
Delta R.T.: 0.002 min
Response: 60828
Conc: 189.36 ng/ml

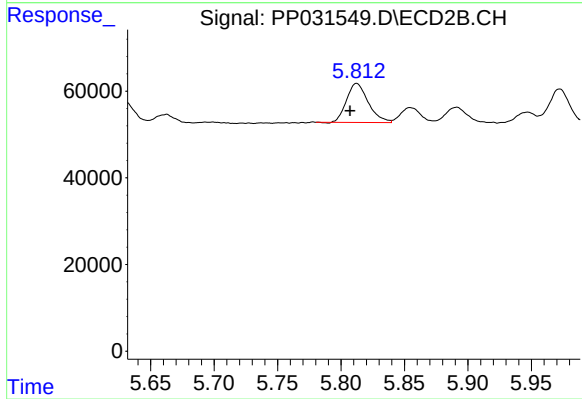

#15 AR-1232-5


R.T.: 5.812 min
Delta R.T.: 0.005 min
Response: 107252
Conc: 370.11 ng/ml

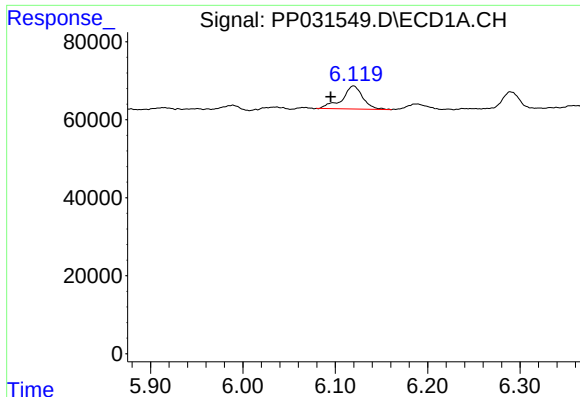

#16 AR-1242-1


R.T.: 6.120 min
Delta R.T.: 0.025 min
Response: 92165
Conc: 77.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

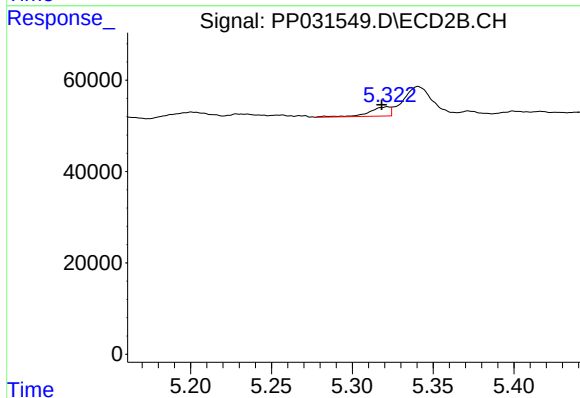


#16 AR-1242-1

R.T.: 5.322 min
Delta R.T.: 0.003 min
Response: 18107
Conc: 15.86 ng/ml

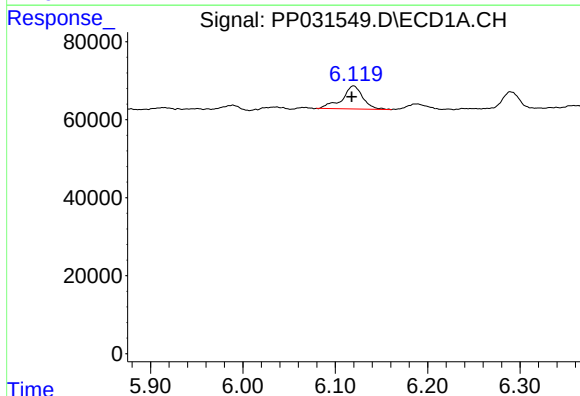


#17 AR-1242-2

R.T.: 6.120 min
Delta R.T.: 0.002 min
Response: 92165
Conc: 51.80 ng/ml

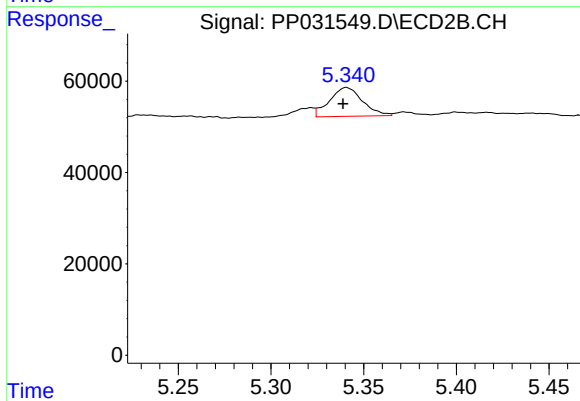

#17 AR-1242-2


R.T.: 5.341 min
Delta R.T.: 0.002 min
Response: 78134
Conc: 46.46 ng/ml

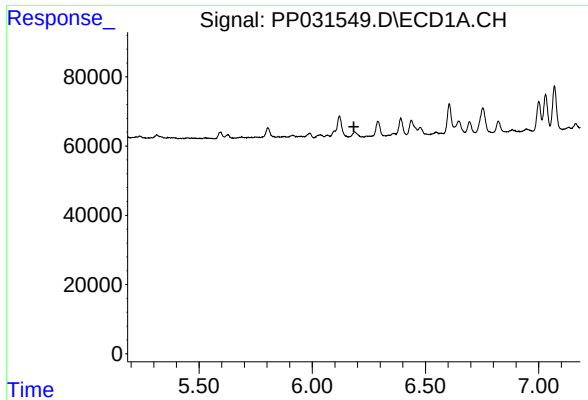

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

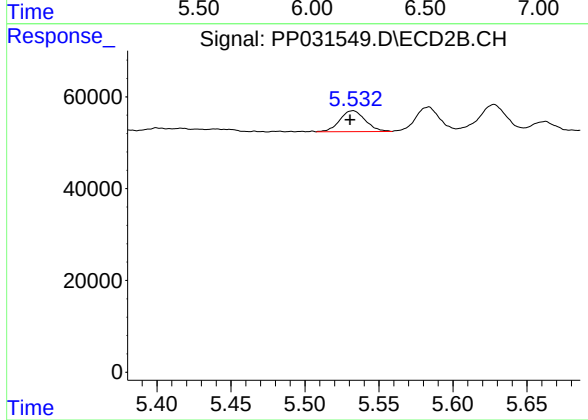


#18 AR-1242-3

R.T.: 5.533 min
Delta R.T.: 0.002 min
Response: 54253
Conc: 59.41 ng/ml

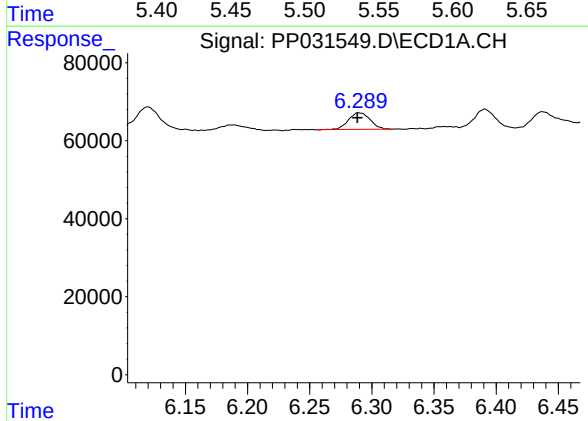


#19 AR-1242-4

R.T.: 6.290 min
Delta R.T.: 0.001 min
Response: 51980
Conc: 56.24 ng/ml

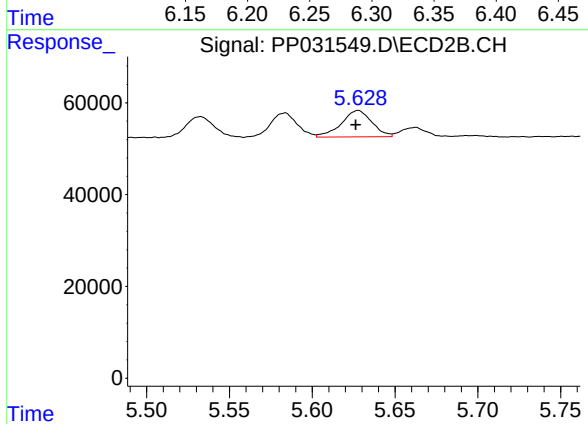

#19 AR-1242-4


R.T.: 5.628 min
Delta R.T.: 0.002 min
Response: 74250
Conc: 88.39 ng/ml

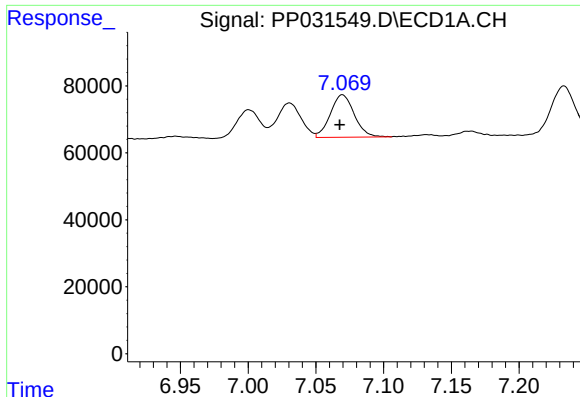

#20 AR-1242-5


R.T.: 7.070 min
Delta R.T.: 0.002 min
Response: 155686
Conc: 169.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

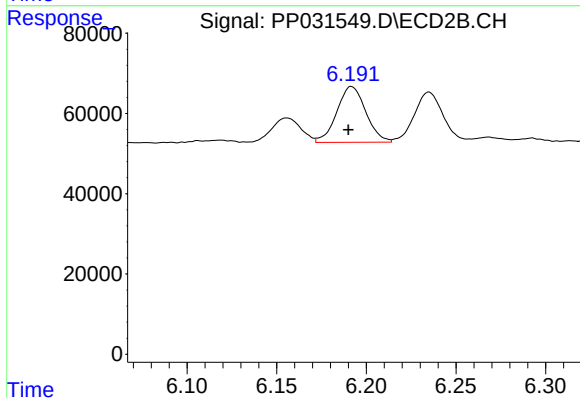


#20 AR-1242-5

R.T.: 6.192 min
Delta R.T.: 0.002 min
Response: 156763
Conc: 151.94 ng/ml

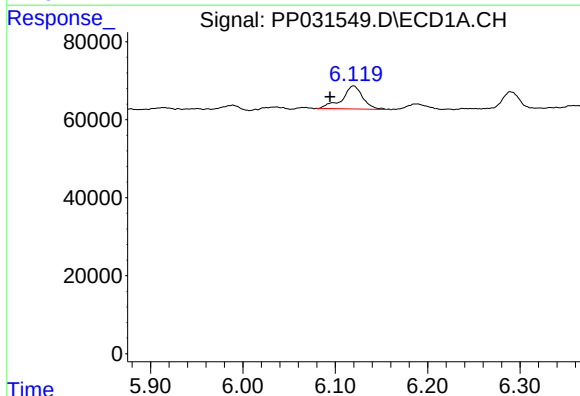


#21 AR-1248-1

R.T.: 6.120 min
Delta R.T.: 0.025 min
Response: 92165
Conc: 99.81 ng/ml

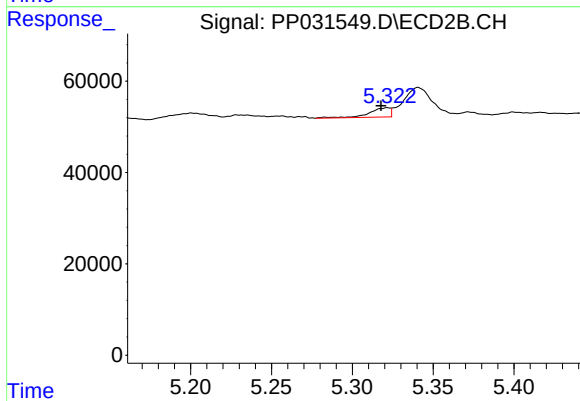

#21 AR-1248-1


R.T.: 5.322 min
Delta R.T.: 0.004 min
Response: 18107
Conc: 21.02 ng/ml

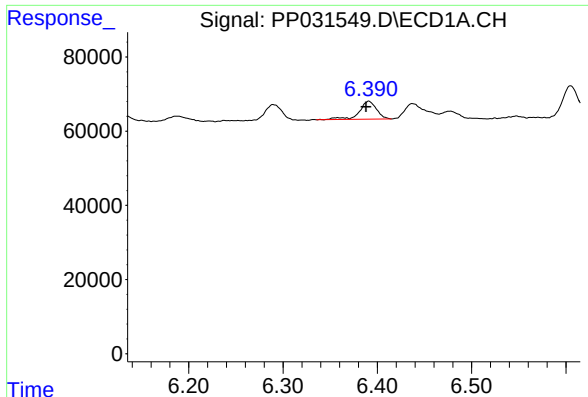

#22 AR-1248-2


R.T.: 6.391 min
Delta R.T.: 0.003 min
Response: 60828
Conc: 51.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

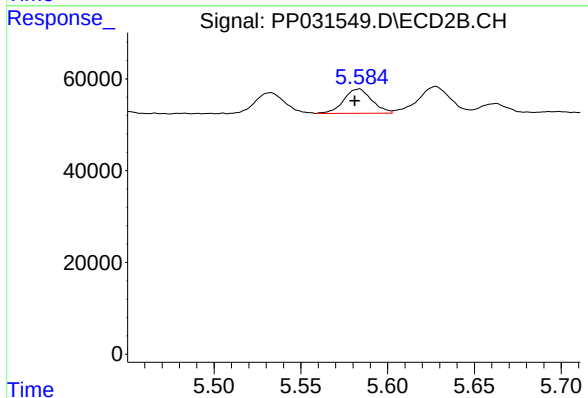


#22 AR-1248-2

R.T.: 5.584 min
Delta R.T.: 0.003 min
Response: 59278
Conc: 49.65 ng/ml

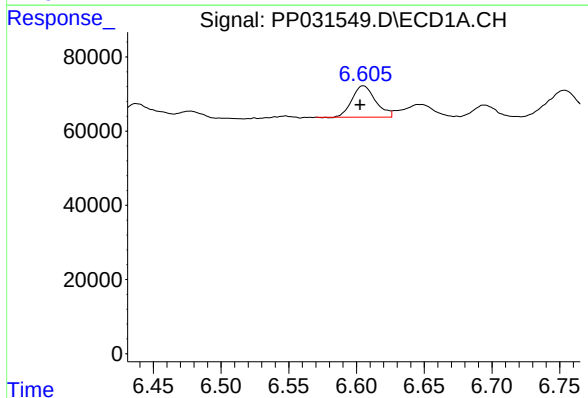


#23 AR-1248-3

R.T.: 6.605 min
Delta R.T.: 0.003 min
Response: 103129
Conc: 70.49 ng/ml

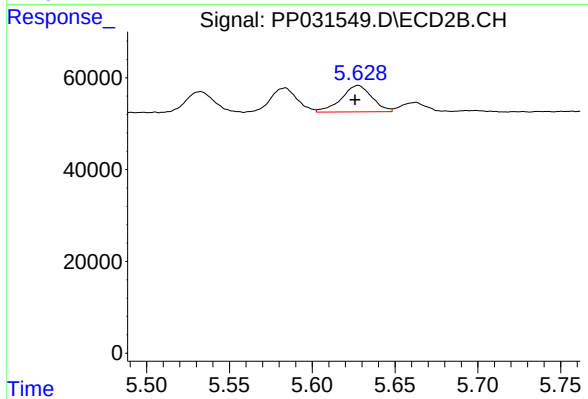

#23 AR-1248-3


R.T.: 5.628 min
Delta R.T.: 0.002 min
Response: 74250
Conc: 58.66 ng/ml

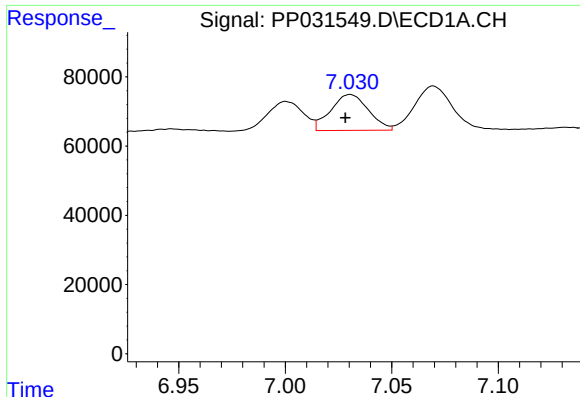

#24 AR-1248-4


R.T.: 7.031 min
Delta R.T.: 0.002 min
Response: 127530
Conc: 81.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

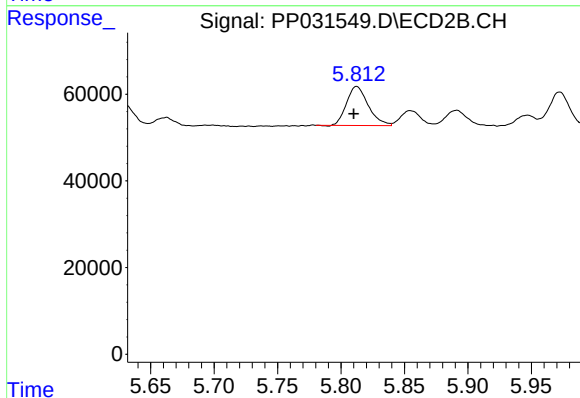


#24 AR-1248-4

R.T.: 5.812 min
Delta R.T.: 0.002 min
Response: 107252
Conc: 70.01 ng/ml

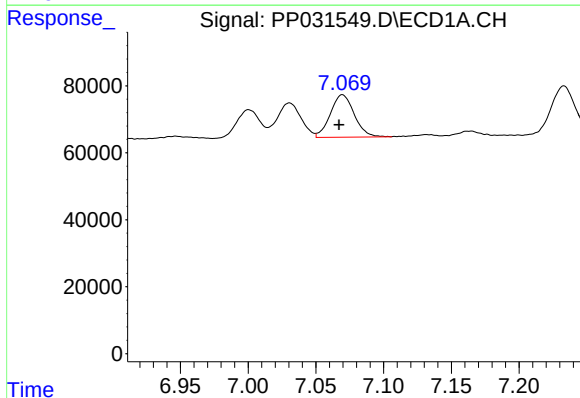


#25 AR-1248-5

R.T.: 7.070 min
Delta R.T.: 0.003 min
Response: 155686
Conc: 98.07 ng/ml

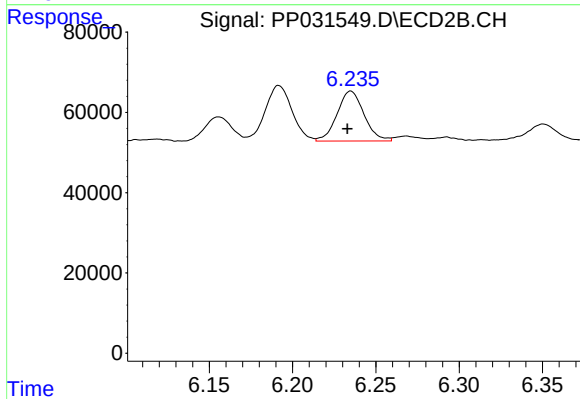

#25 AR-1248-5


R.T.: 6.235 min
Delta R.T.: 0.002 min
Response: 140284
Conc: 96.15 ng/ml

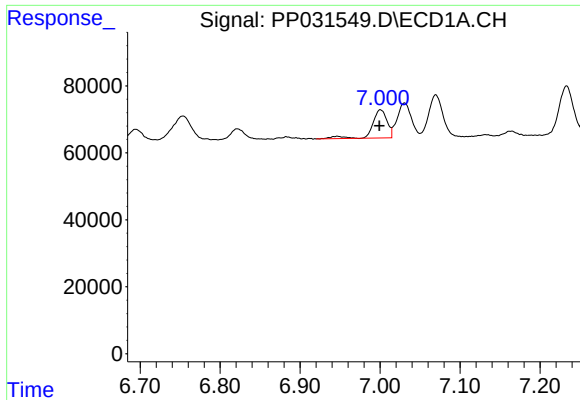

#26 AR-1254-1


R.T.: 7.000 min
Delta R.T.: 0.001 min
Response: 107162
Conc: 70.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

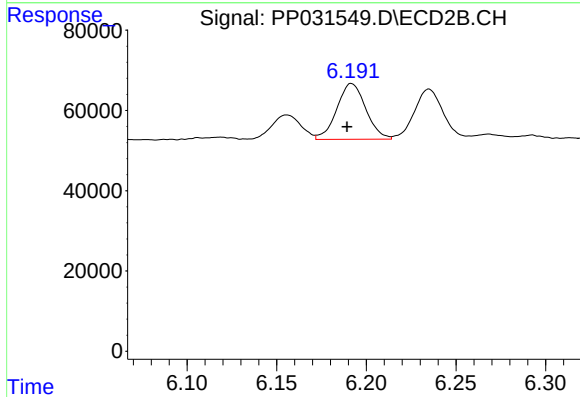


#26 AR-1254-1

R.T.: 6.192 min
Delta R.T.: 0.002 min
Response: 156763
Conc: 72.47 ng/ml

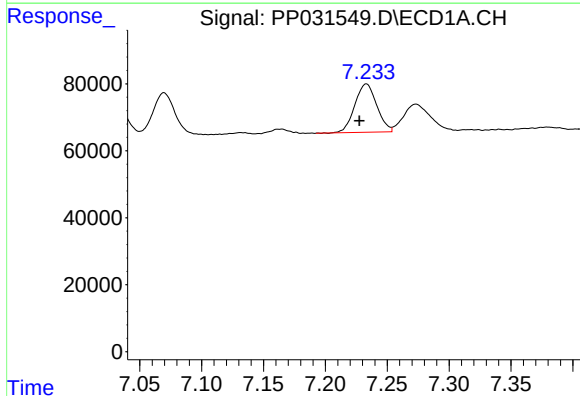


#27 AR-1254-2

R.T.: 7.233 min
Delta R.T.: 0.006 min
Response: 177435
Conc: 76.40 ng/ml

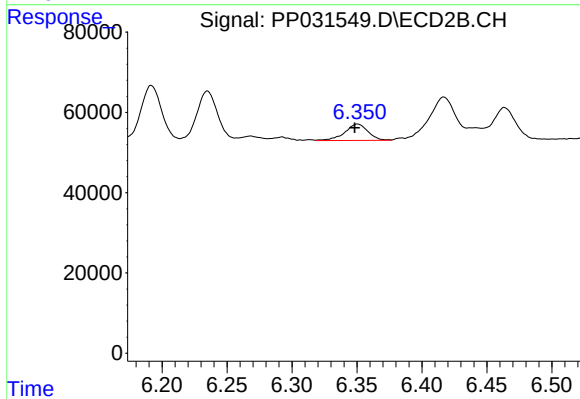

#27 AR-1254-2


R.T.: 6.351 min
Delta R.T.: 0.002 min
Response: 50805
Conc: 27.27 ng/ml

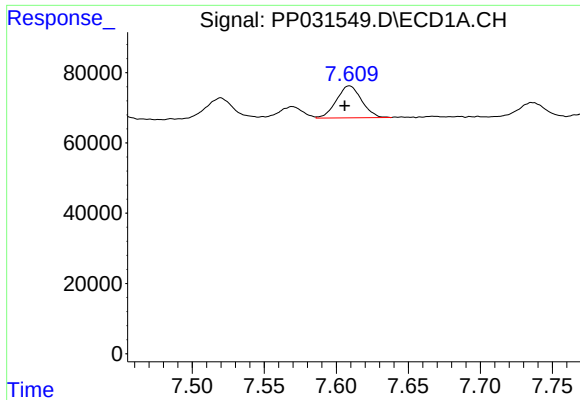

#28 AR-1254-3


R.T.: 7.609 min
Delta R.T.: 0.003 min
Response: 110904
Conc: 43.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

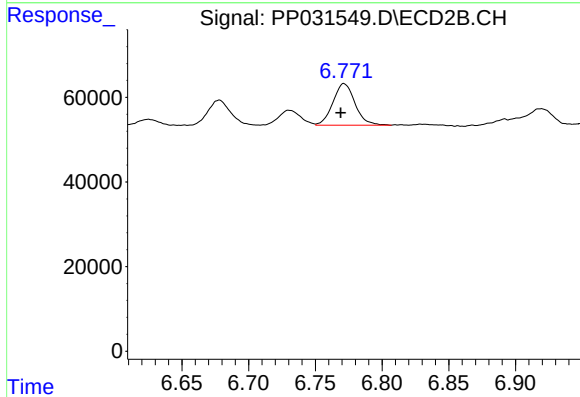


#28 AR-1254-3

R.T.: 6.771 min
Delta R.T.: 0.002 min
Response: 113685
Conc: 36.78 ng/ml

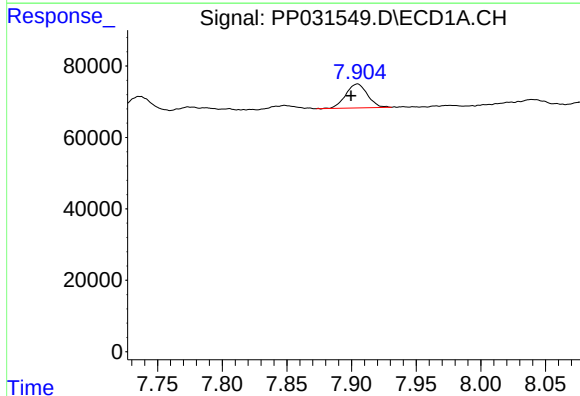


#29 AR-1254-4

R.T.: 7.905 min
Delta R.T.: 0.005 min
Response: 78754
Conc: 46.41 ng/ml

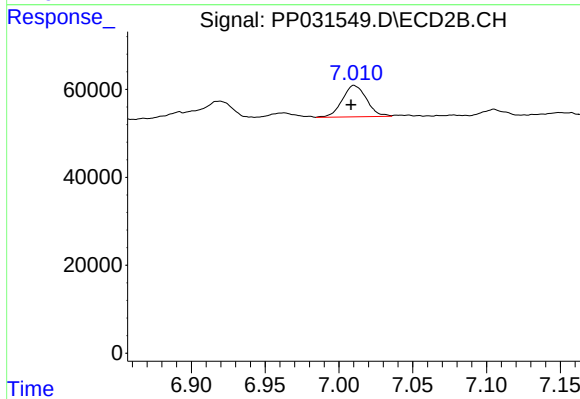

#29 AR-1254-4


R.T.: 7.010 min
Delta R.T.: 0.002 min
Response: 81573
Conc: 48.02 ng/ml

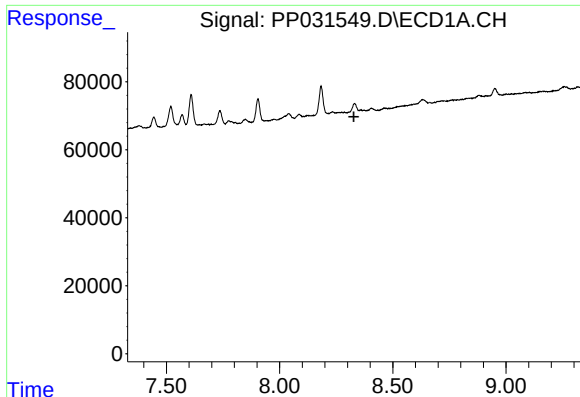

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 8.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

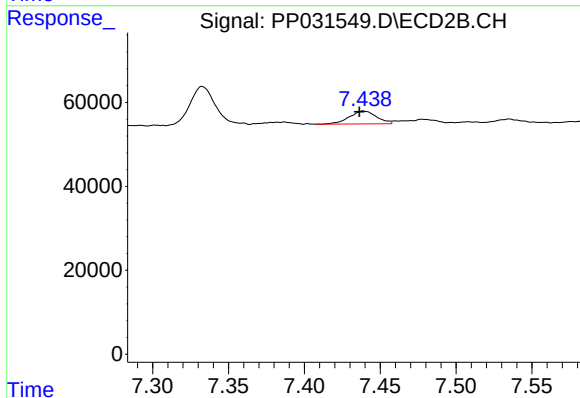


#30 AR-1254-5

R.T.: 7.439 min
Delta R.T.: 0.003 min
Response: 38329
Conc: 14.20 ng/ml

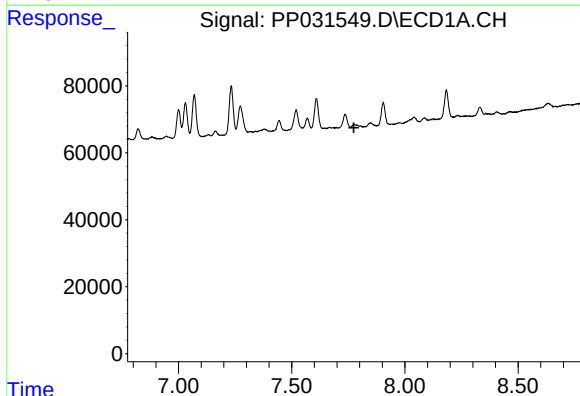


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.775 min
Response: 0
Conc: N.D.

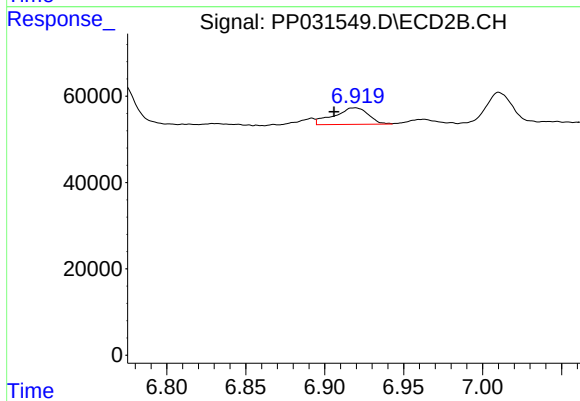

#31 AR-1260-1


R.T.: 6.920 min
Delta R.T.: 0.014 min
Response: 58140
Conc: 29.42 ng/ml

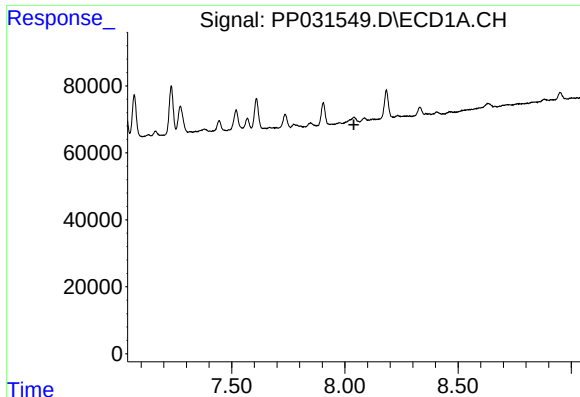

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

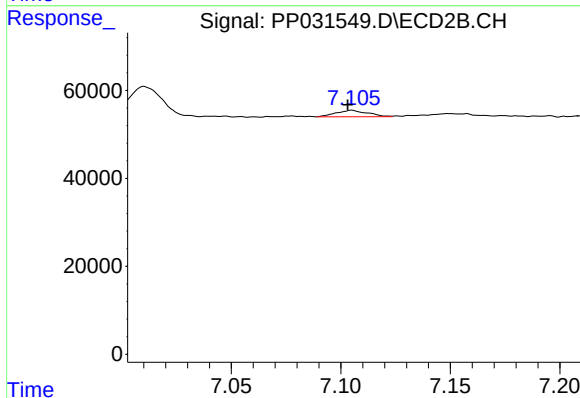


#32 AR-1260-2

R.T.: 7.105 min
Delta R.T.: 0.002 min
Response: 14658
Conc: 6.02 ng/ml

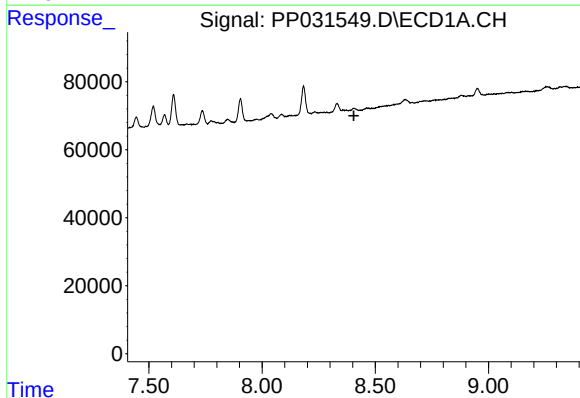


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

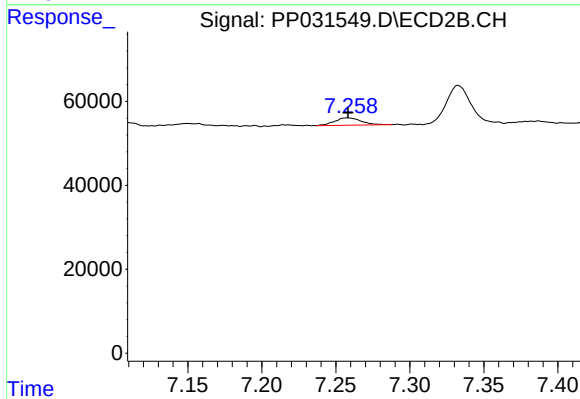

#33 AR-1260-3


R.T.: 7.259 min
Delta R.T.: 0.000 min
Response: 22014
Conc: 9.64 ng/ml

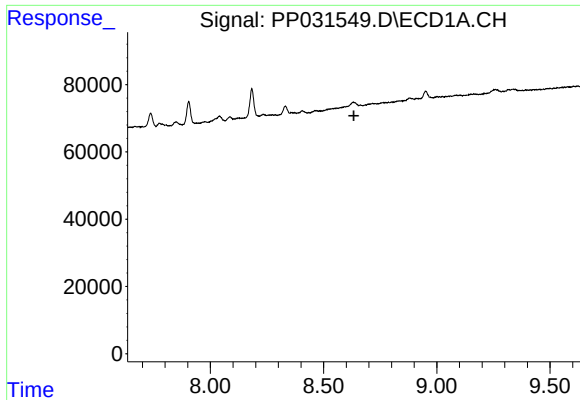

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

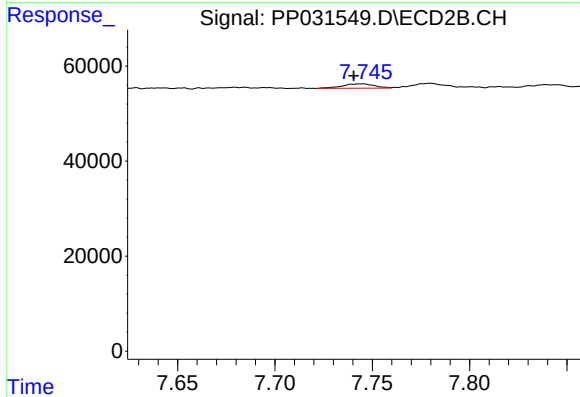


#34 AR-1260-4

R.T.: 7.745 min
Delta R.T.: 0.005 min
Response: 10586
Conc: 5.57 ng/ml

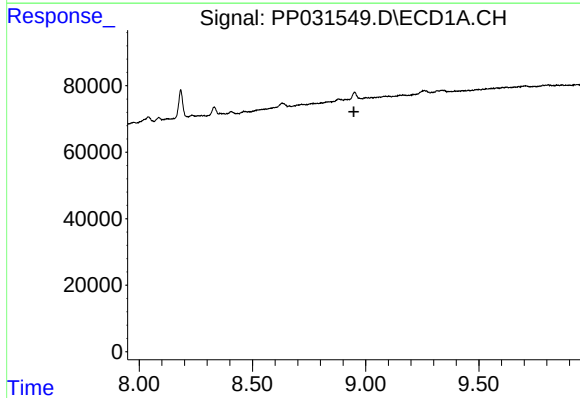


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.948 min
Response: 0
Conc: N.D.

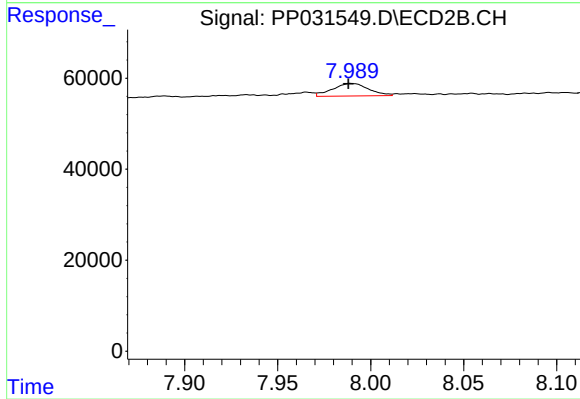

#35 AR-1260-5


R.T.: 7.989 min
Delta R.T.: 0.001 min
Response: 37018
Conc: 8.16 ng/ml

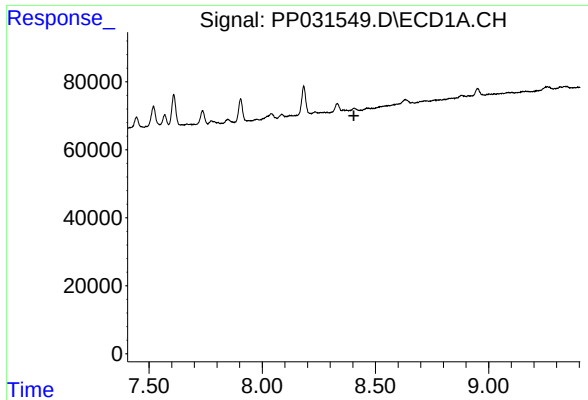

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

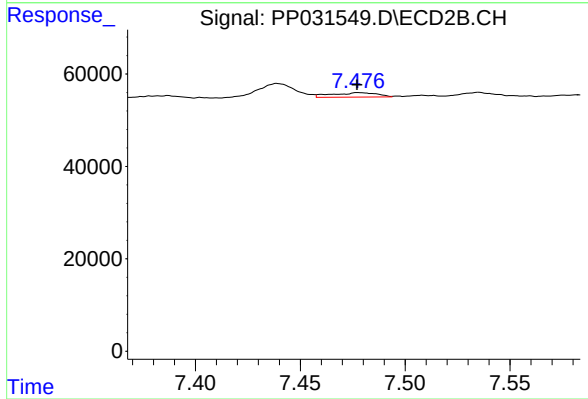


#36 AR-1262-1

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 14575
Conc: 5.67 ng/ml

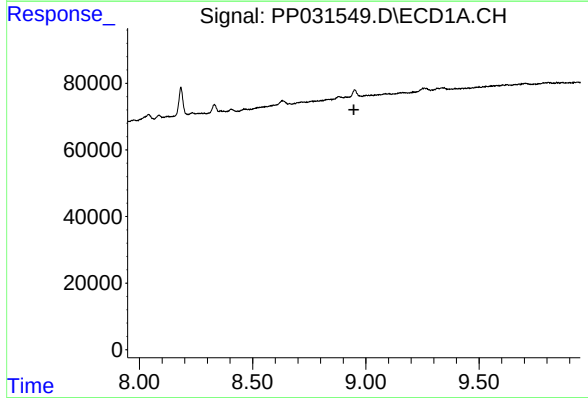


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.947 min
Response: 0
Conc: N.D.

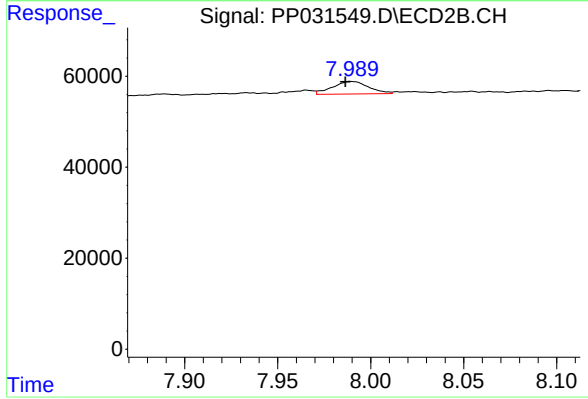

#37 AR-1262-2


R.T.: 7.989 min
Delta R.T.: 0.003 min
Response: 37018
Conc: 8.22 ng/ml

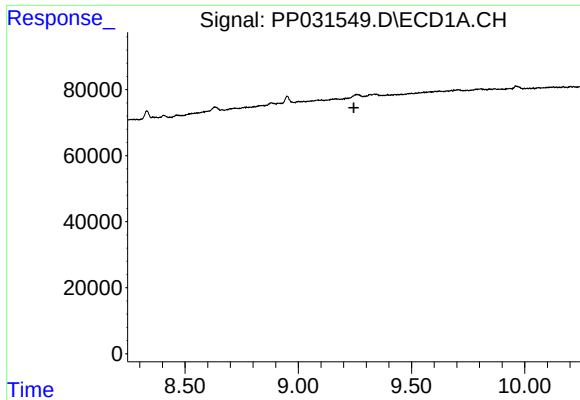

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

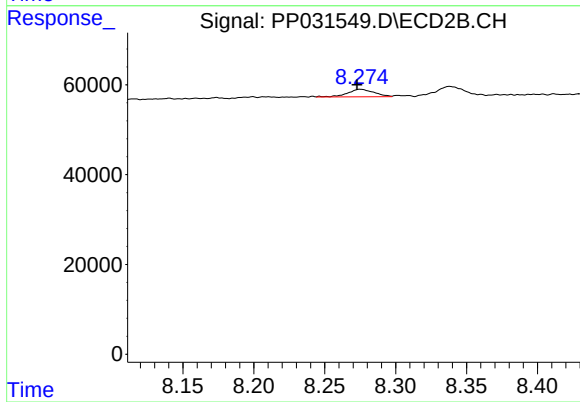


#38 AR-1262-3

R.T.: 8.275 min
Delta R.T.: 0.002 min
Response: 21802
Conc: 12.75 ng/ml

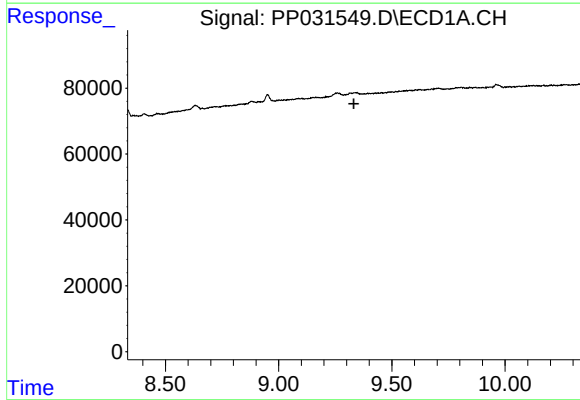


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.333 min
Response: 0
Conc: N.D.

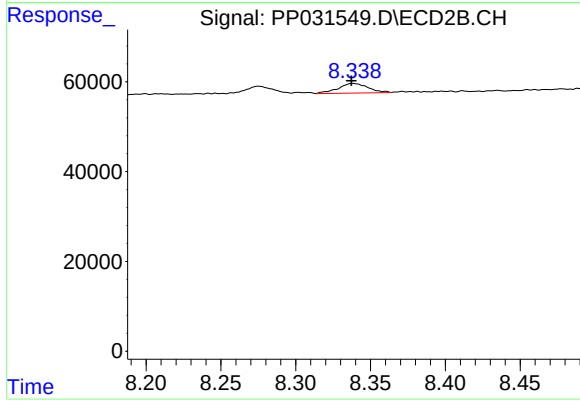

#39 AR-1262-4


R.T.: 8.338 min
Delta R.T.: 0.000 min
Response: 30041
Conc: 8.72 ng/ml

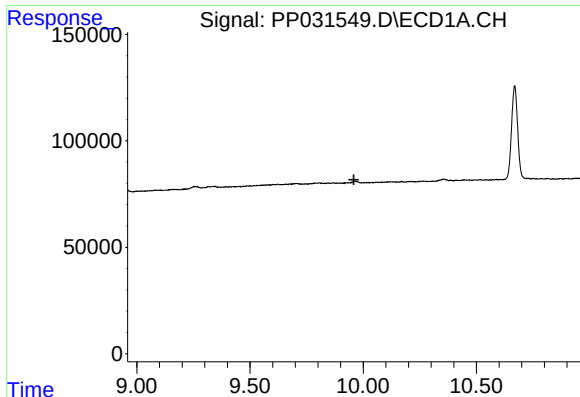

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

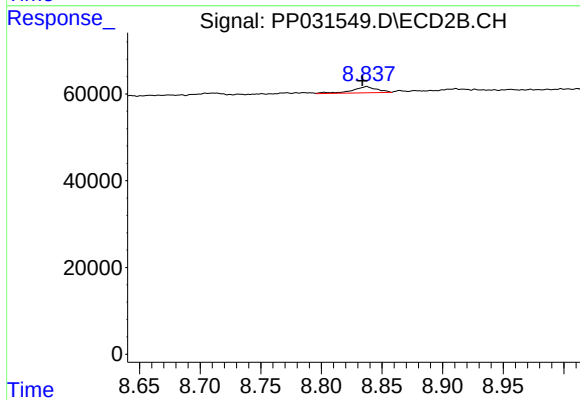


#40 AR-1262-5

R.T.: 8.837 min
Delta R.T.: 0.004 min
Response: 19689
Conc: 12.35 ng/ml

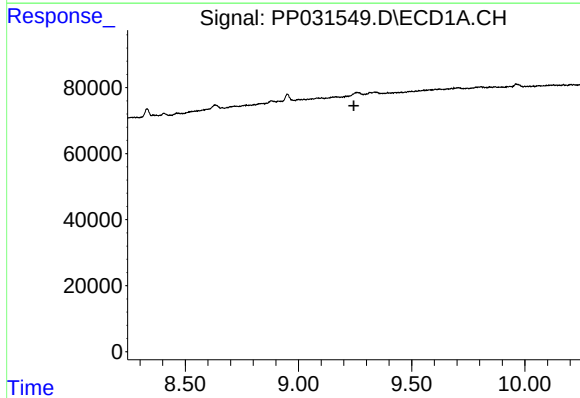


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.245 min
Response: 0
Conc: N.D.

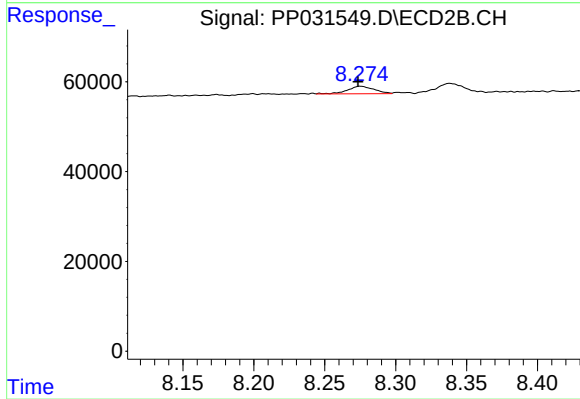

#41 AR-1268-1


R.T.: 8.275 min
Delta R.T.: 0.001 min
Response: 21802
Conc: 3.94 ng/ml

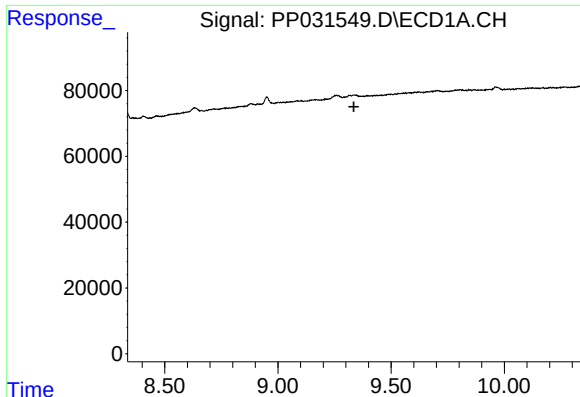

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

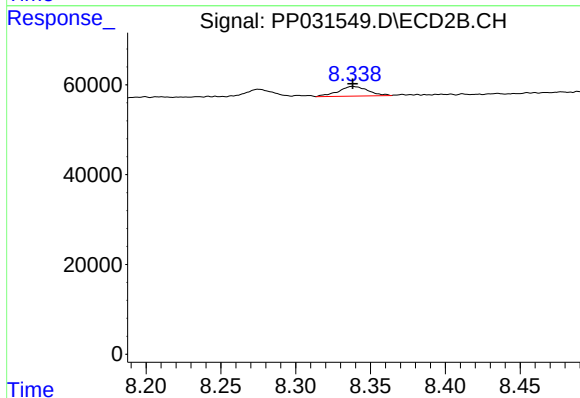


#42 AR-1268-2

R.T.: 8.338 min
Delta R.T.: 0.000 min
Response: 30041
Conc: 5.56 ng/ml

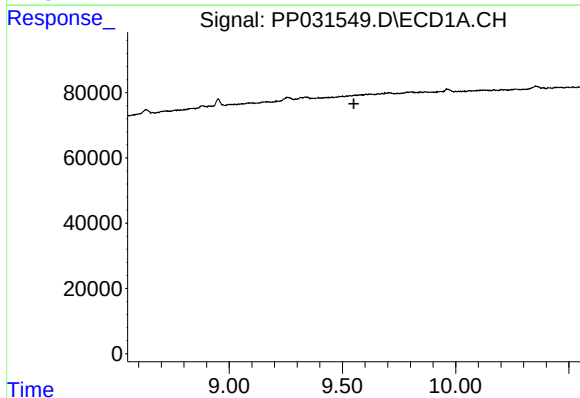


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.550 min
Response: 0
Conc: N.D.

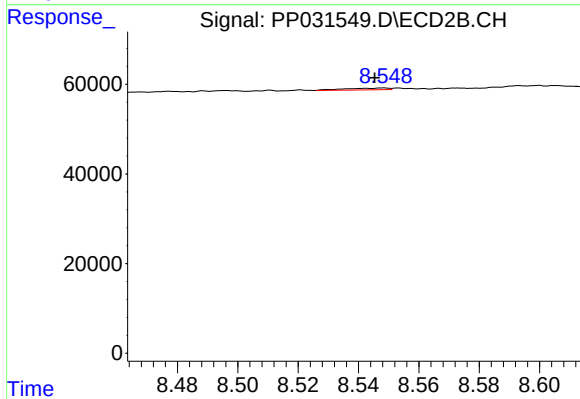

#43 AR-1268-3


R.T.: 8.548 min
Delta R.T.: 0.003 min
Response: 3825
Conc: 0.83 ng/ml

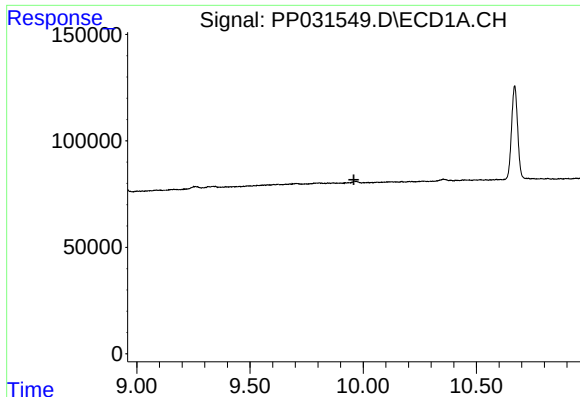

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-CON-E

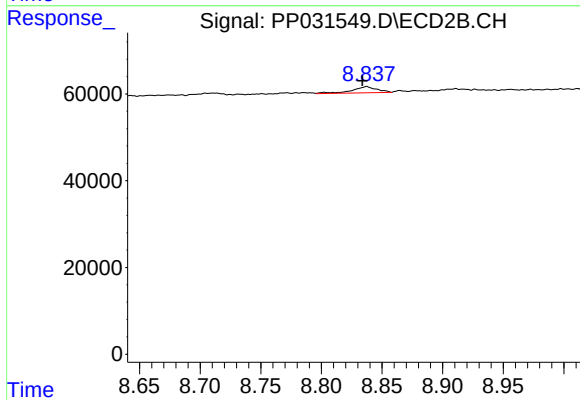


#44 AR-1268-4

R.T.: 8.837 min
Delta R.T.: 0.004 min
Response: 19689
Conc: 10.80 ng/ml

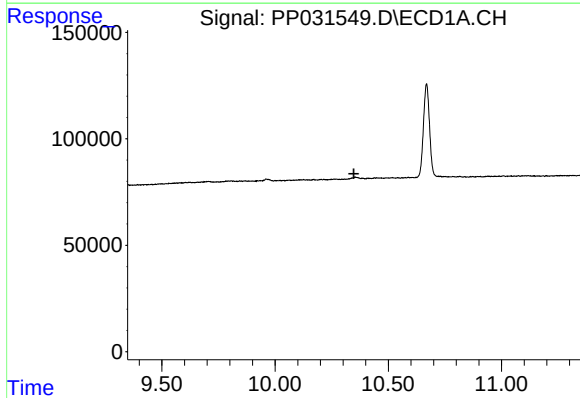

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.348 min
Response: 0
Conc: N.D.

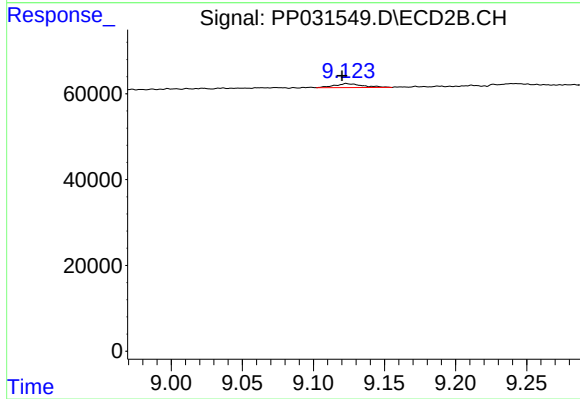

#45 AR-1268-5

R.T.: 9.123 min
Delta R.T.: 0.003 min
Response: 12720
Conc: 0.92 ng/ml