

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031592.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 00:06
 Operator : DD\AJ
 Sample : L4868-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-112020-BD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 01:35:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.789	4.062	1054719	996234	21.781	20.790
2)	SA Decachlor...	10.664	9.368	623472	678855	18.357	18.334
Target Compounds							
7)	L1 AR-1016-5	0.000	5.800	0	7413	N.D.	6.518 #
9)	L2 AR-1221-2	0.000	4.414	0	11598	N.D.	30.067 #
15)	L3 AR-1232-5	0.000	5.800	0	7413	N.D.	25.583 #
20)	L4 AR-1242-5	0.000	6.198	0	2611	N.D.	2.531 #
24)	L5 AR-1248-4	0.000	5.800	0	7413	N.D.	4.839 #
26)	L6 AR-1254-1	0.000	6.198	0	2611	N.D.	1.207 #
30)	L6 AR-1254-5	0.000	7.437	0	4244	N.D.	1.572 #
32)	L7 AR-1260-2	0.000	7.098	0	4414	N.D.	1.813 #
33)	L7 AR-1260-3	0.000	7.257	0	4736	N.D.	2.074 #
34)	L7 AR-1260-4	8.622	7.744	162751	8176	88.387	4.303 #
35)	L7 AR-1260-5	0.000	7.985	0	19195	N.D.	4.230 #
36)	L8 AR-1262-1	0.000	7.475	0	10966	N.D.	4.266 #
37)	L8 AR-1262-2	0.000	7.985	0	19195	N.D.	4.260 #
38)	L8 AR-1262-3	0.000	8.274	0	22872	N.D.	13.380 #
39)	L8 AR-1262-4	0.000	8.337	0	15365	N.D.	4.462 #
40)	L8 AR-1262-5	0.000	8.835	0	20501	N.D.	12.855 #
41)	L9 AR-1268-1	0.000	8.274	0	22872	N.D.	4.134 #
42)	L9 AR-1268-2	0.000	8.337	0	15365	N.D.	2.842 #
43)	L9 AR-1268-3	0.000	8.545	0	2320	N.D.	0.506 #
44)	L9 AR-1268-4	0.000	8.835	0	20501	N.D.	11.247 #
45)	L9 AR-1268-5	0.000	9.120	0	9004	N.D.	0.650 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031592.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 00:06
Operator : DD\AJ
Sample : L4868-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
KENS-112020-BD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 01:35:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

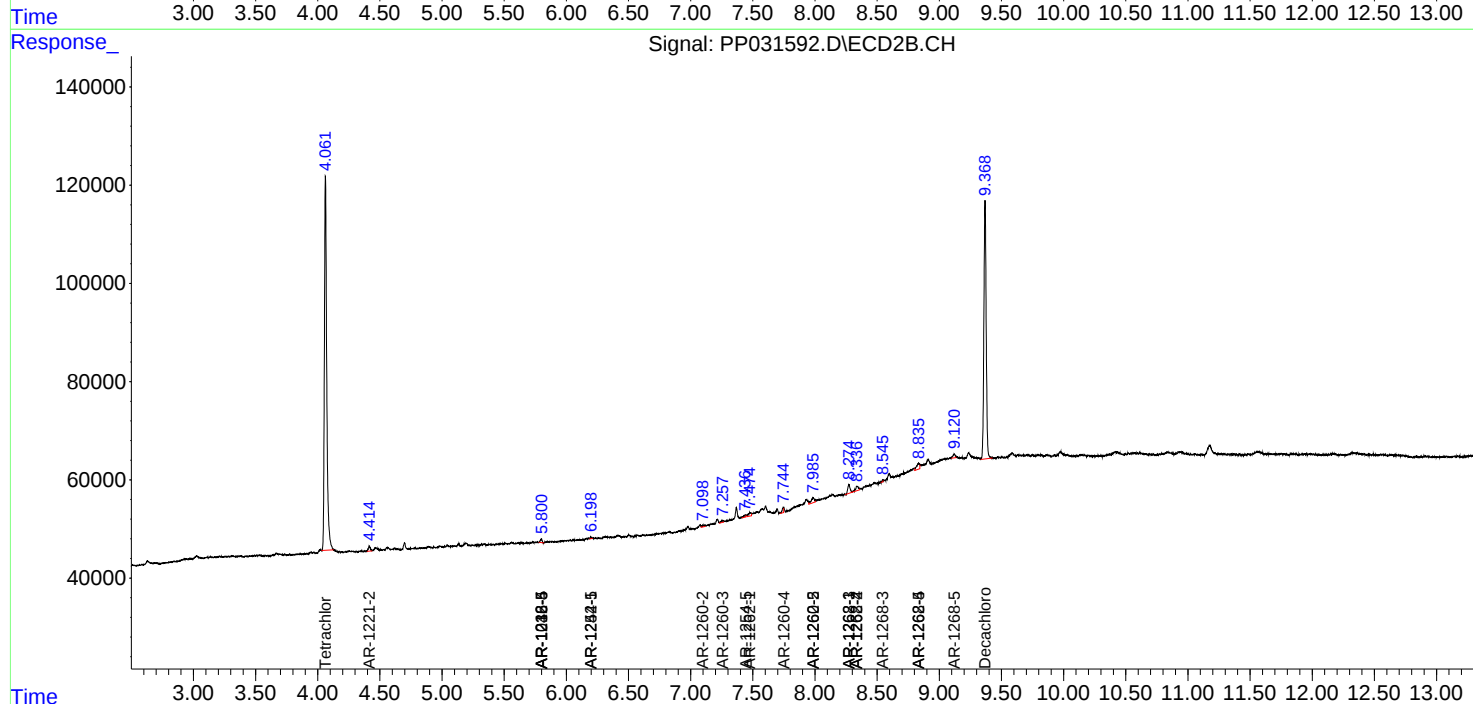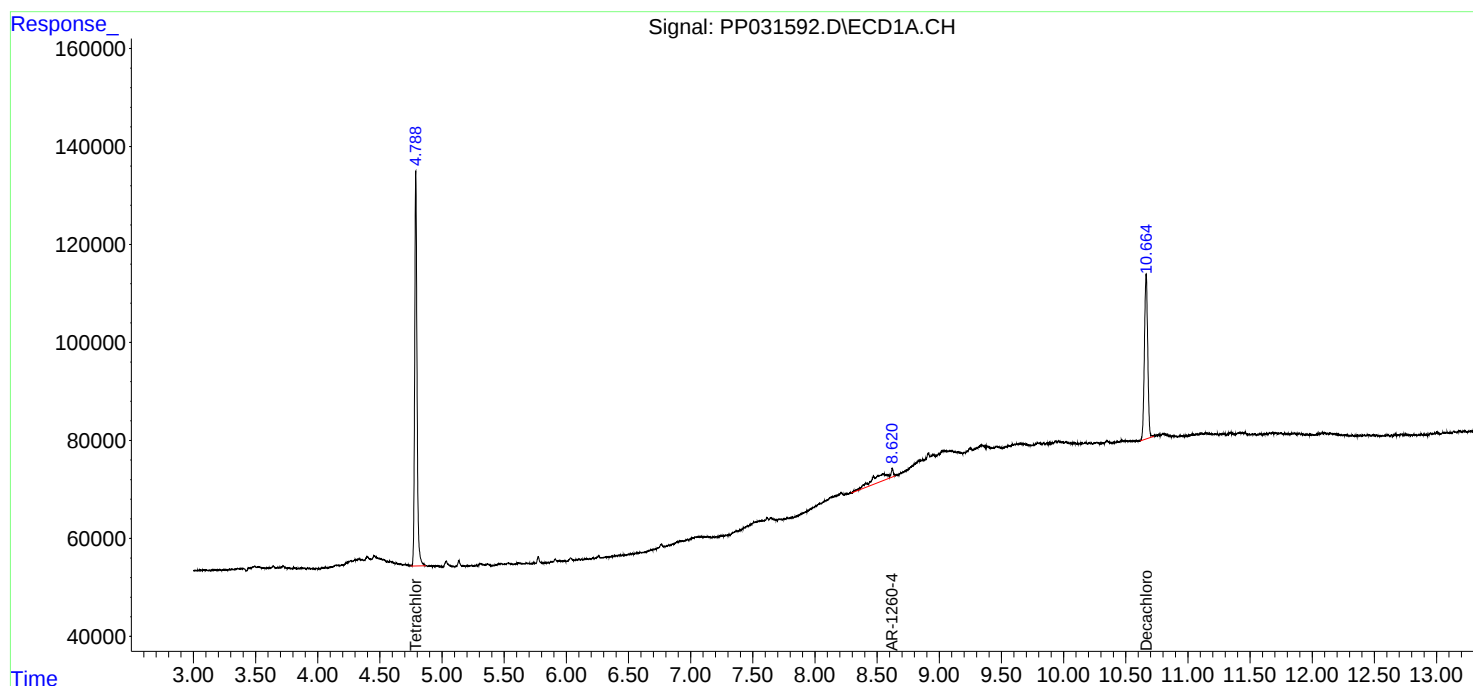


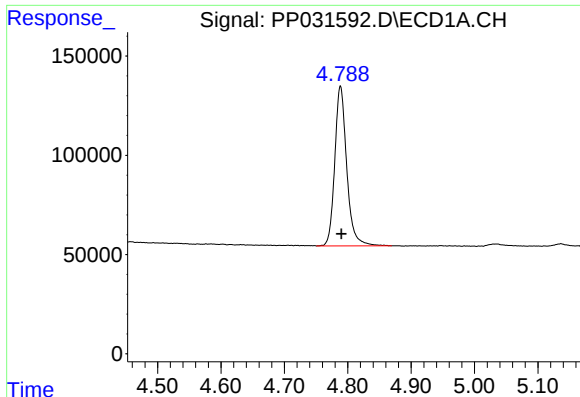

#1 Tetrachloro-m-xylene


R.T.: 4.789 min
Delta R.T.: -0.001 min
Response: 1054719
Conc: 21.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

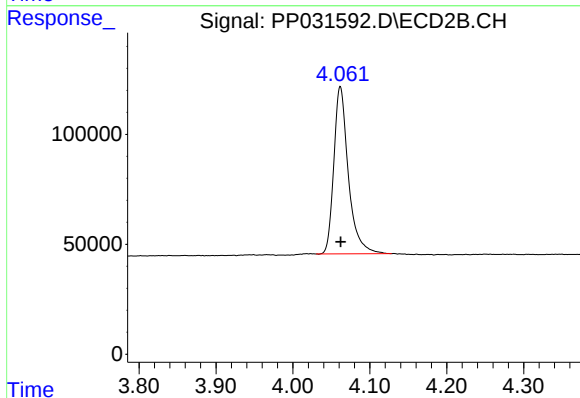


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: 0.000 min
Response: 996234
Conc: 20.79 ng/ml

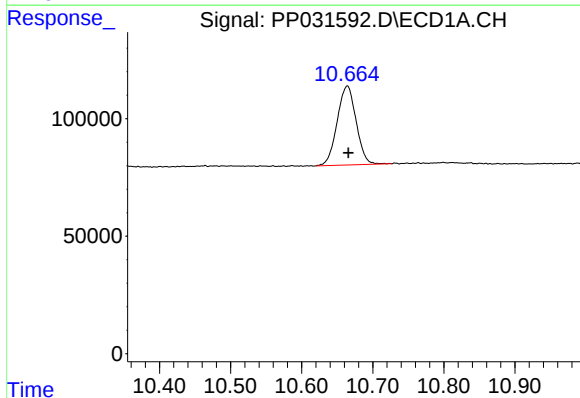


#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.001 min
Response: 623472
Conc: 18.36 ng/ml

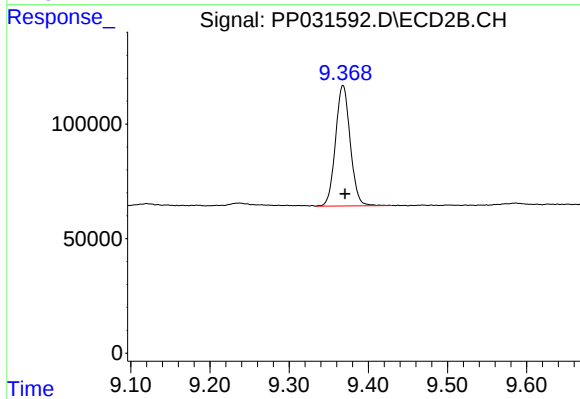

#2 Decachlorobiphenyl


R.T.: 9.368 min
Delta R.T.: -0.003 min
Response: 678855
Conc: 18.33 ng/ml

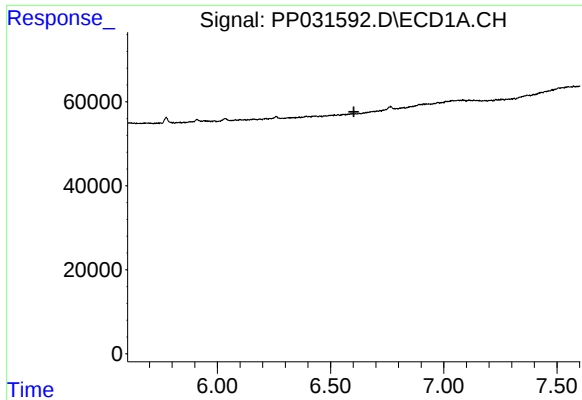

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

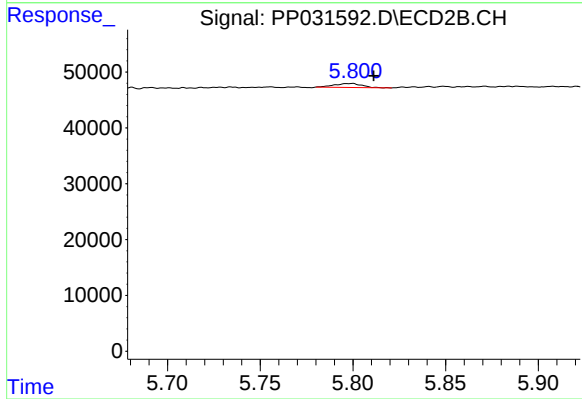


#7 AR-1016-5

R.T.: 5.800 min
Delta R.T.: -0.011 min
Response: 7413
Conc: 6.52 ng/ml

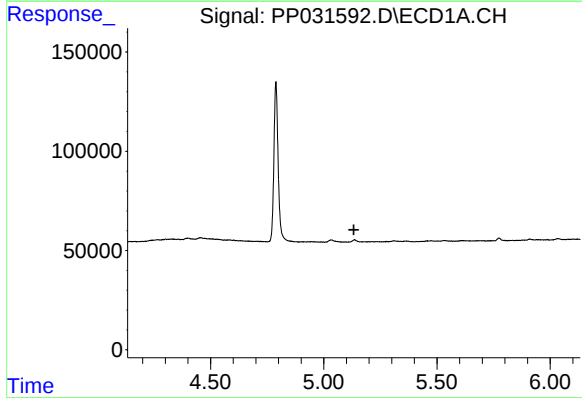


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

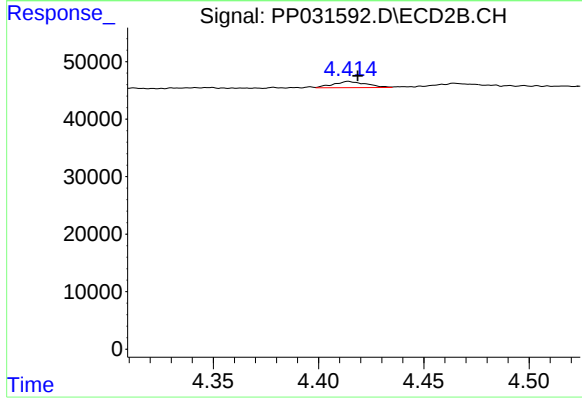

#9 AR-1221-2


R.T.: 4.414 min
Delta R.T.: -0.005 min
Response: 11598
Conc: 30.07 ng/ml

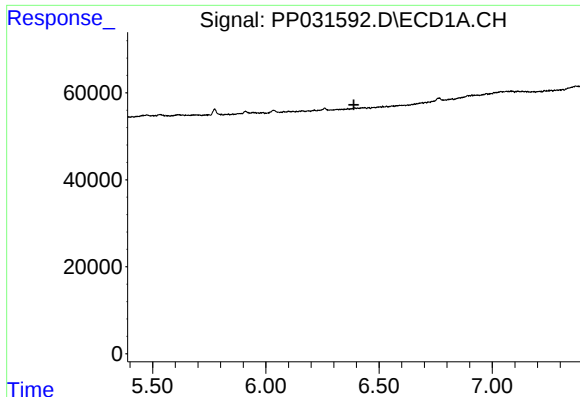

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

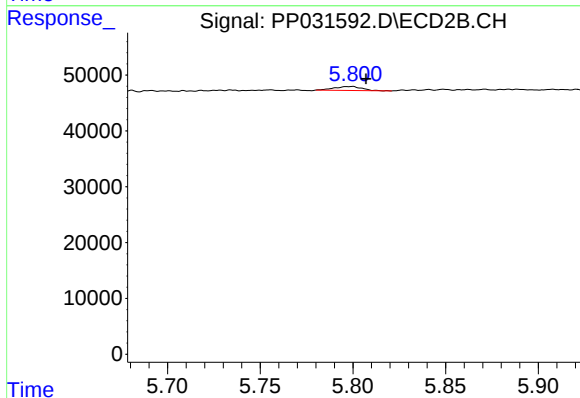


#15 AR-1232-5

R.T.: 5.800 min
Delta R.T.: -0.007 min
Response: 7413
Conc: 25.58 ng/ml

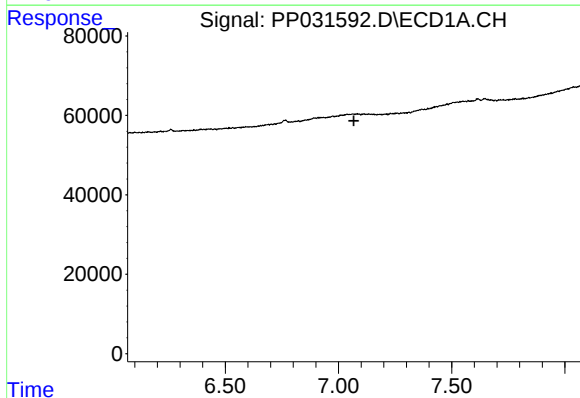


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.068 min
Response: 0
Conc: N.D.

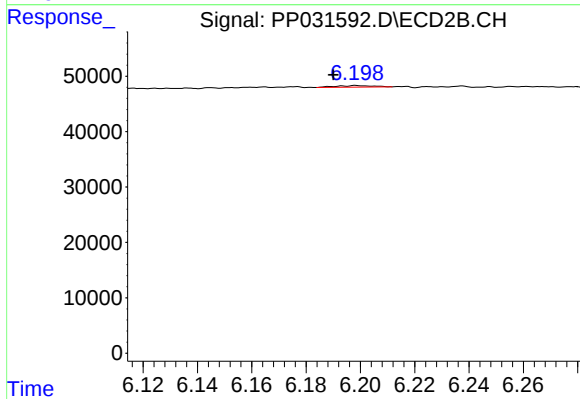

#20 AR-1242-5


R.T.: 6.198 min
Delta R.T.: 0.008 min
Response: 2611
Conc: 2.53 ng/ml

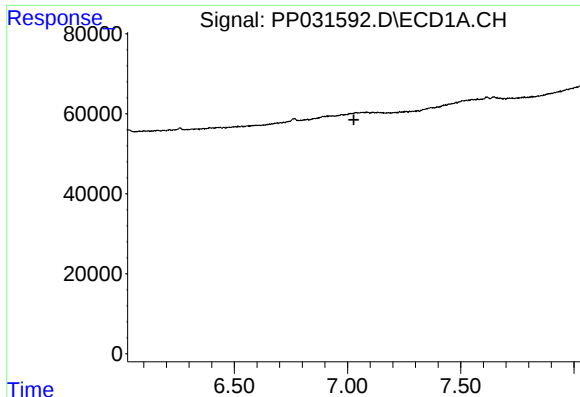

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 7.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

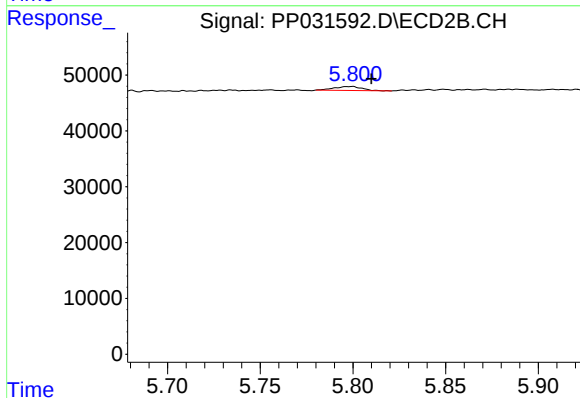


#24 AR-1248-4

R.T.: 5.800 min
Delta R.T.: -0.010 min
Response: 7413
Conc: 4.84 ng/ml

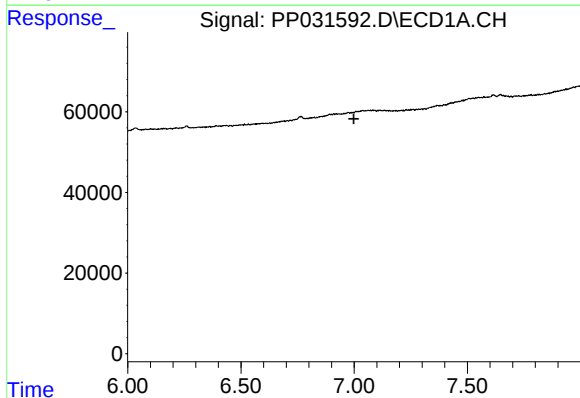


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.999 min
Response: 0
Conc: N.D.

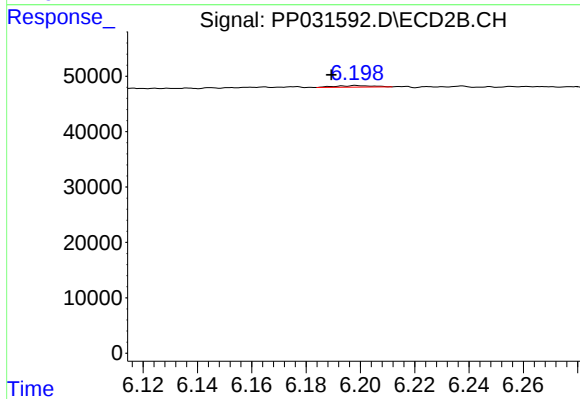

#26 AR-1254-1


R.T.: 6.198 min
Delta R.T.: 0.009 min
Response: 2611
Conc: 1.21 ng/ml

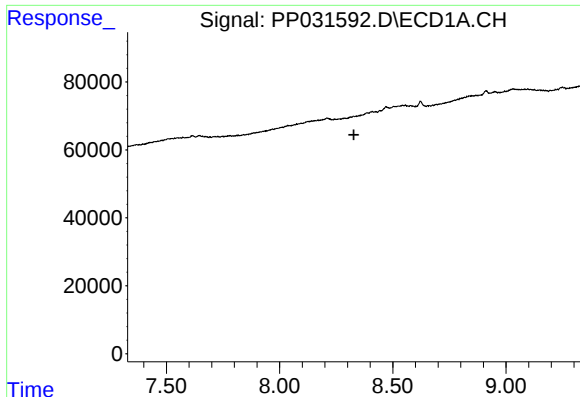

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 8.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

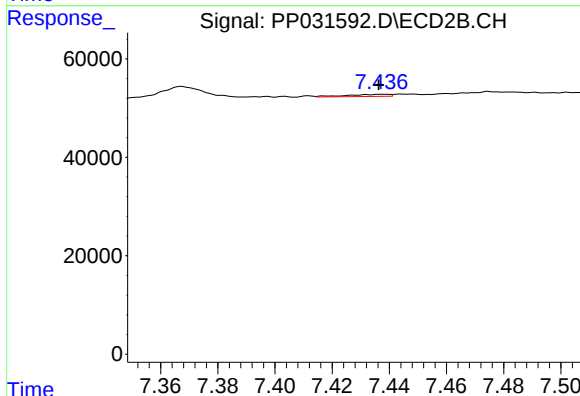


#30 AR-1254-5

R.T.: 7.437 min
Delta R.T.: 0.001 min
Response: 4244
Conc: 1.57 ng/ml

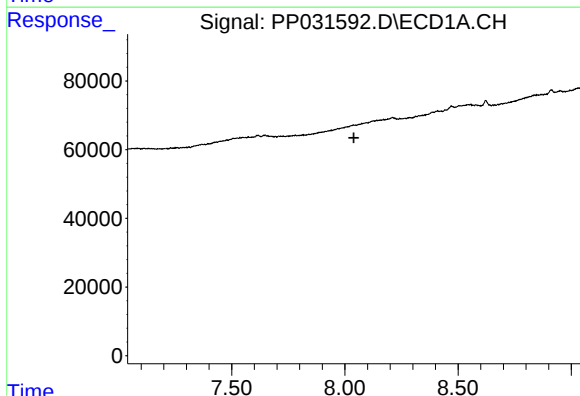


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.040 min
Response: 0
Conc: N.D.

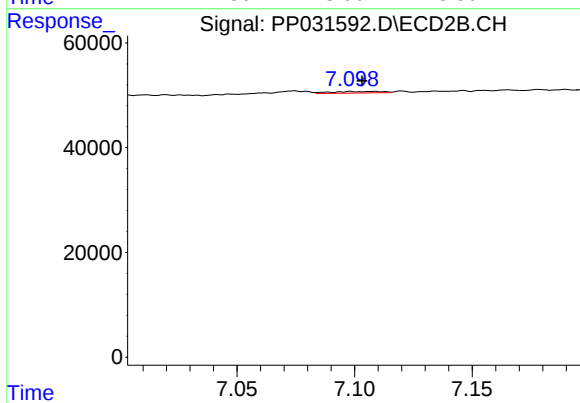

#32 AR-1260-2


R.T.: 7.098 min
Delta R.T.: -0.005 min
Response: 4414
Conc: 1.81 ng/ml

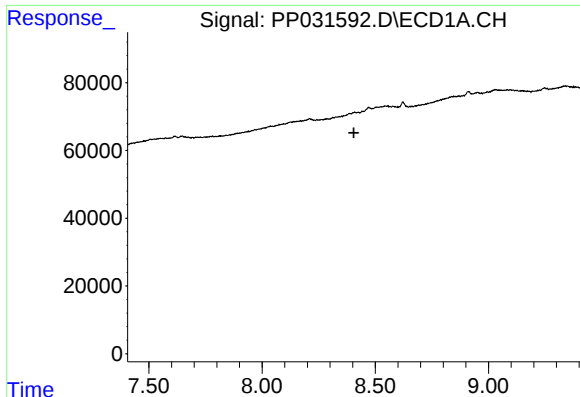

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

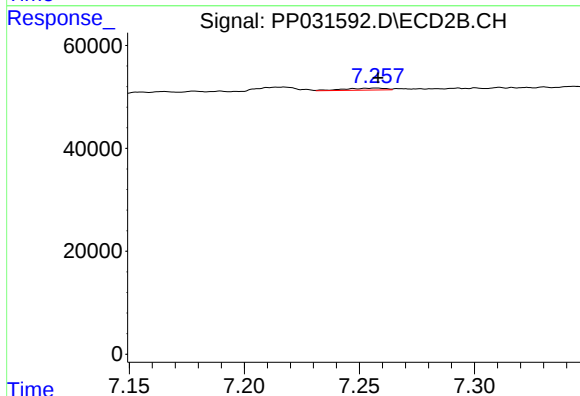


#33 AR-1260-3

R.T.: 7.257 min
Delta R.T.: 0.000 min
Response: 4736
Conc: 2.07 ng/ml

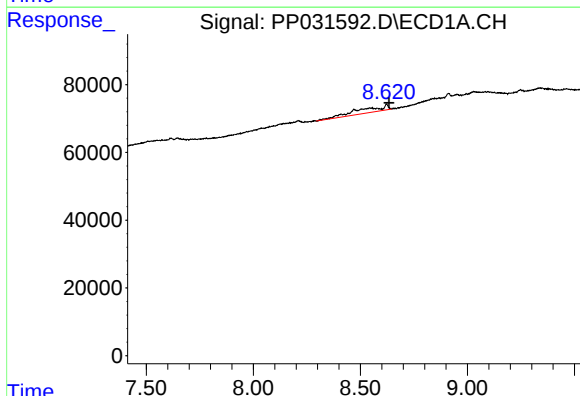


#34 AR-1260-4

R.T.: 8.622 min
Delta R.T.: -0.012 min
Response: 162751
Conc: 88.39 ng/ml

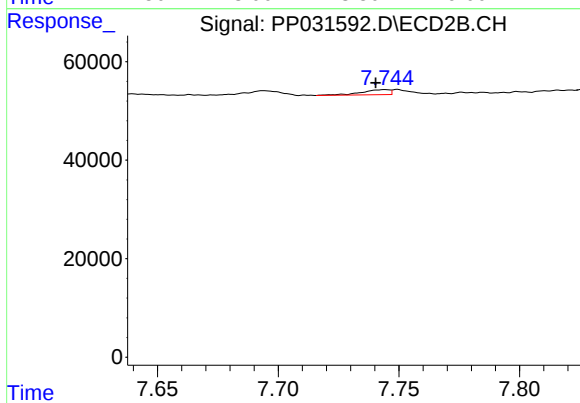

#34 AR-1260-4


R.T.: 7.744 min
Delta R.T.: 0.004 min
Response: 8176
Conc: 4.30 ng/ml

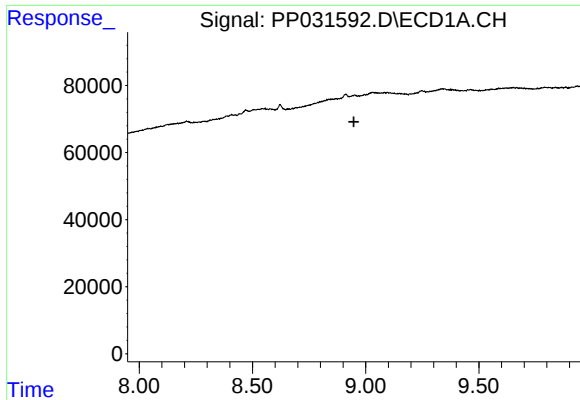

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

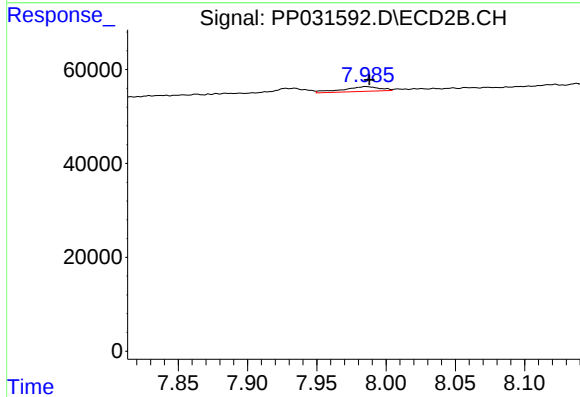


#35 AR-1260-5

R.T.: 7.985 min
Delta R.T.: -0.003 min
Response: 19195
Conc: 4.23 ng/ml

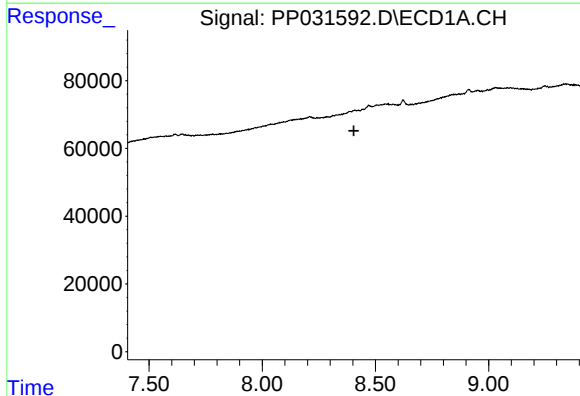


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.404 min
Response: 0
Conc: N.D.

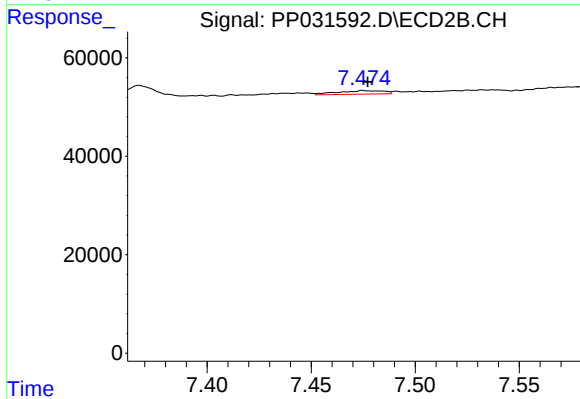

#36 AR-1262-1


R.T.: 7.475 min
Delta R.T.: -0.003 min
Response: 10966
Conc: 4.27 ng/ml

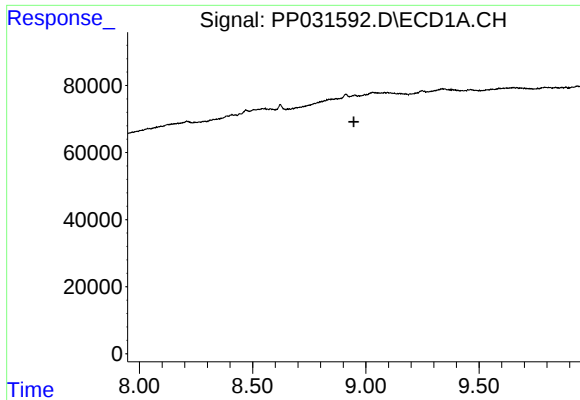

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.947 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

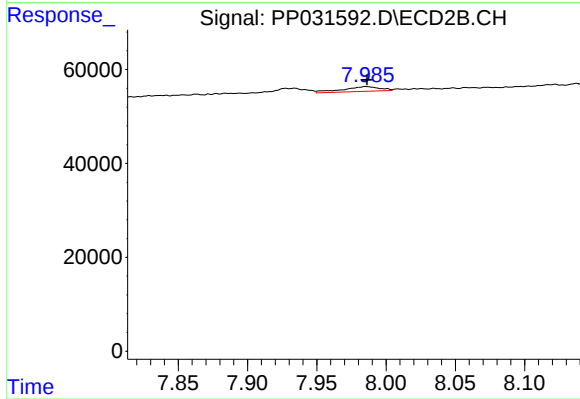


#37 AR-1262-2

R.T.: 7.985 min
Delta R.T.: -0.001 min
Response: 19195
Conc: 4.26 ng/ml

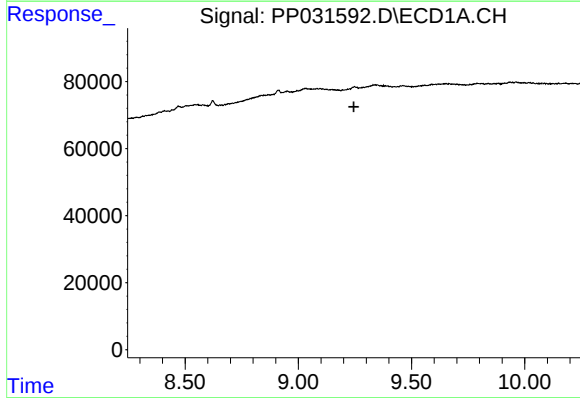


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.246 min
Response: 0
Conc: N.D.

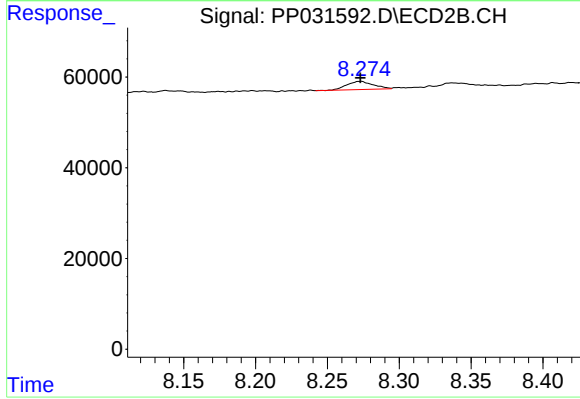

#38 AR-1262-3


R.T.: 8.274 min
Delta R.T.: 0.000 min
Response: 22872
Conc: 13.38 ng/ml

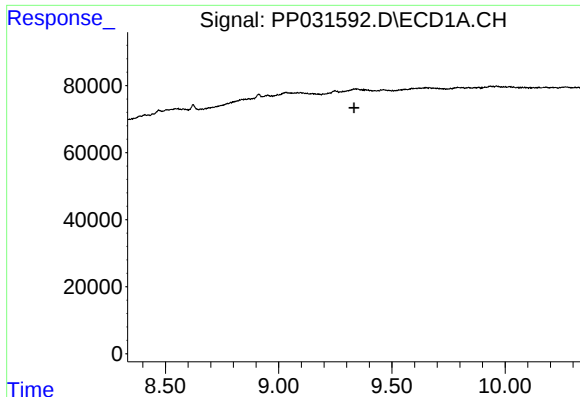

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

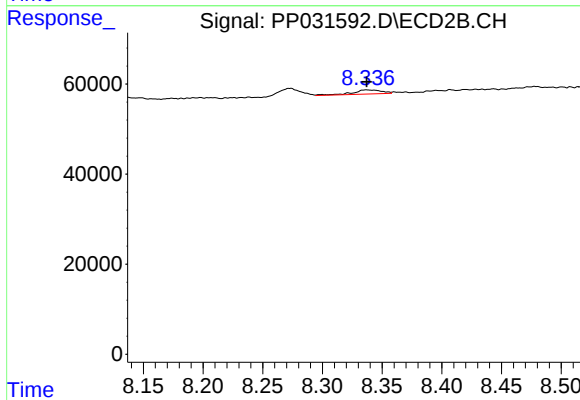


#39 AR-1262-4

R.T.: 8.337 min
Delta R.T.: 0.000 min
Response: 15365
Conc: 4.46 ng/ml

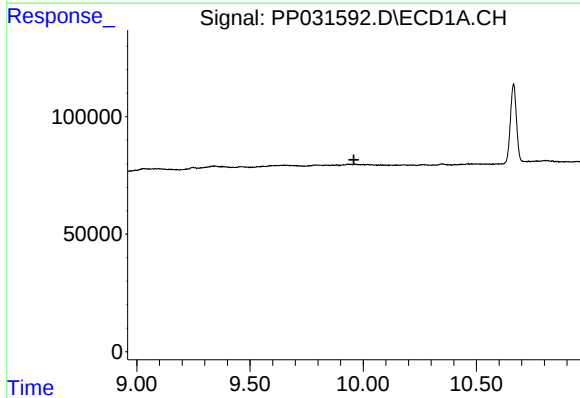


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.959 min
Response: 0
Conc: N.D.

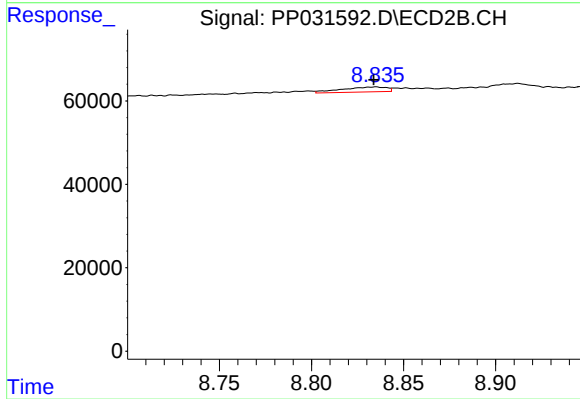

#40 AR-1262-5


R.T.: 8.835 min
Delta R.T.: 0.001 min
Response: 20501
Conc: 12.85 ng/ml

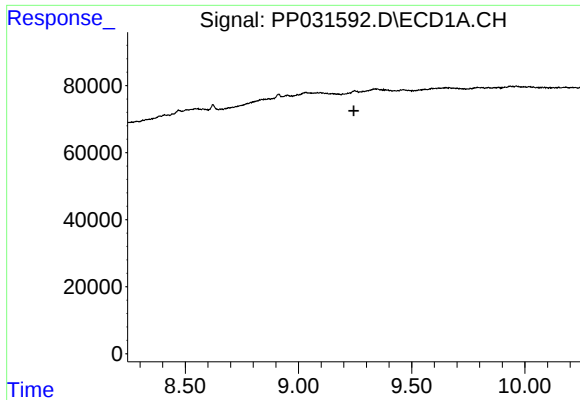

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.245 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

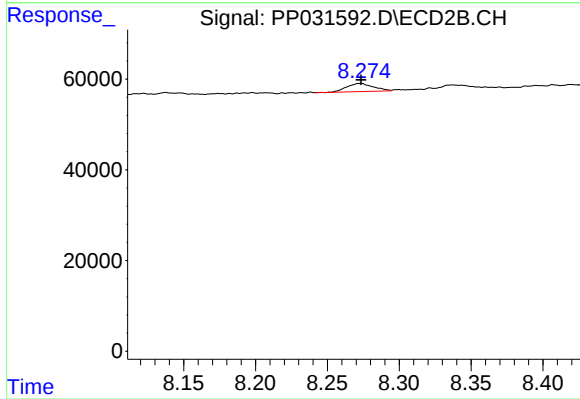


#41 AR-1268-1

R.T.: 8.274 min
Delta R.T.: 0.000 min
Response: 22872
Conc: 4.13 ng/ml

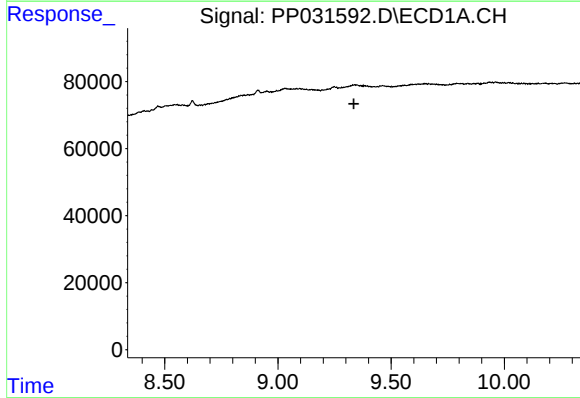


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.335 min
Response: 0
Conc: N.D.

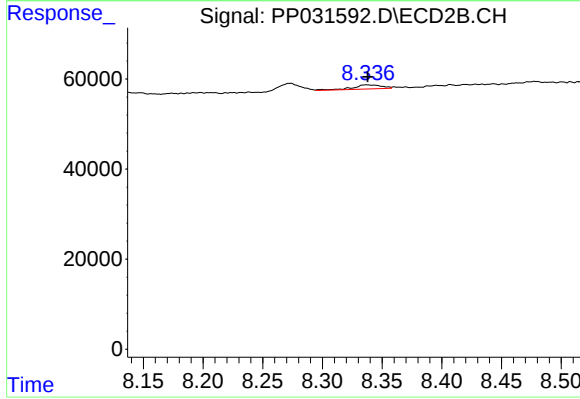

#42 AR-1268-2


R.T.: 8.337 min
Delta R.T.: -0.001 min
Response: 15365
Conc: 2.84 ng/ml

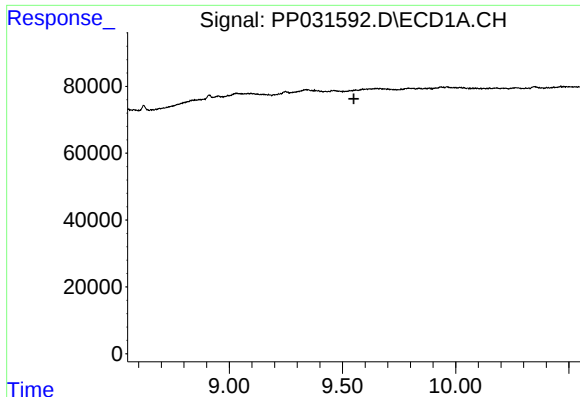

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

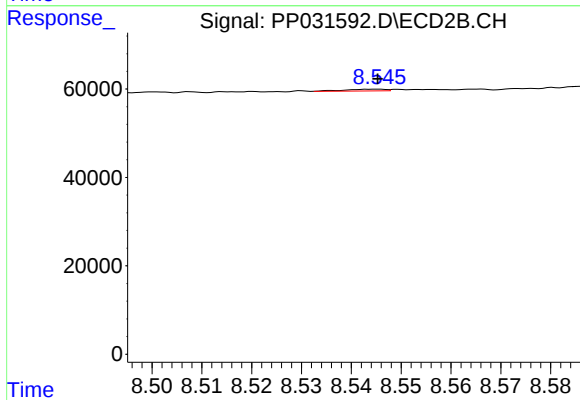


#43 AR-1268-3

R.T.: 8.545 min
Delta R.T.: 0.000 min
Response: 2320
Conc: 0.51 ng/ml

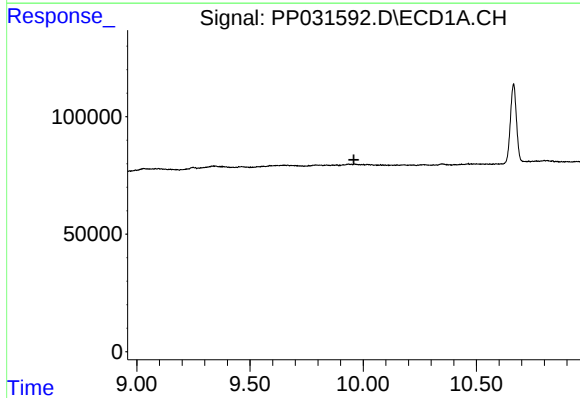


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.959 min
Response: 0
Conc: N.D.

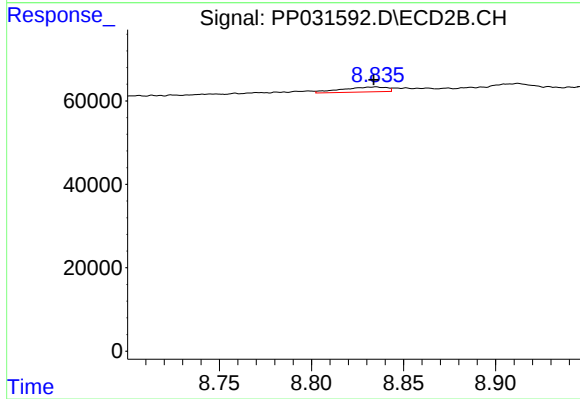

#44 AR-1268-4


R.T.: 8.835 min
Delta R.T.: 0.001 min
Response: 20501
Conc: 11.25 ng/ml

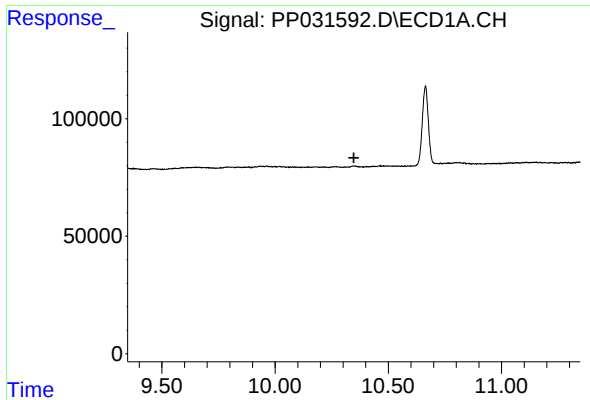

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.348 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-112020-BD

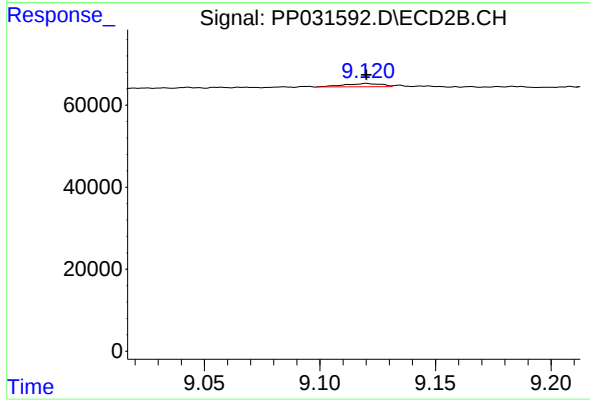

#45 AR-1268-5

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 9004
Conc: 0.65 ng/ml