

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 10:45
 Operator : DD\AJ
 Sample : L4809-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-CON-A

Manual Integrations
 APPROVED

Ankita
 11/25/2020 4:35:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 12:08:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.064	1070388	1004876	22.105	20.971
2) SA Decachlor...	10.668	9.374	769323	727985	22.651	19.661
Target Compounds						
26) L6 AR-1254-1	7.000	6.192	32195	56614	21.127m	26.171
27) L6 AR-1254-2	7.230	6.352	87031	66134	37.474m	35.499
28) L6 AR-1254-3	7.610	6.772	189278	199910	74.922	64.669
29) L6 AR-1254-4	7.904	7.012	206997	198281	121.992	116.711
30) L6 AR-1254-5	8.331	7.440	294169	508788	157.359	188.469

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 10:45
Operator : DD\AJ
Sample : L4809-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 12:08:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

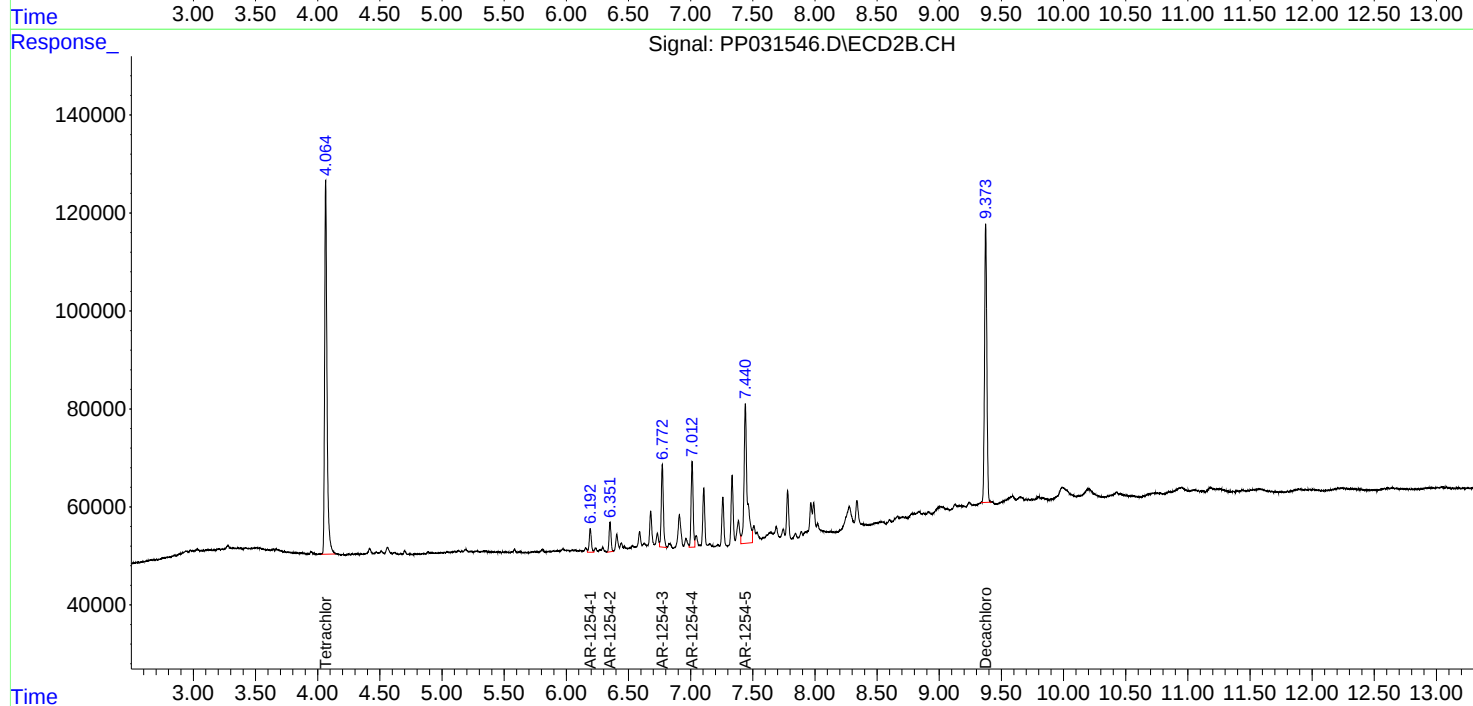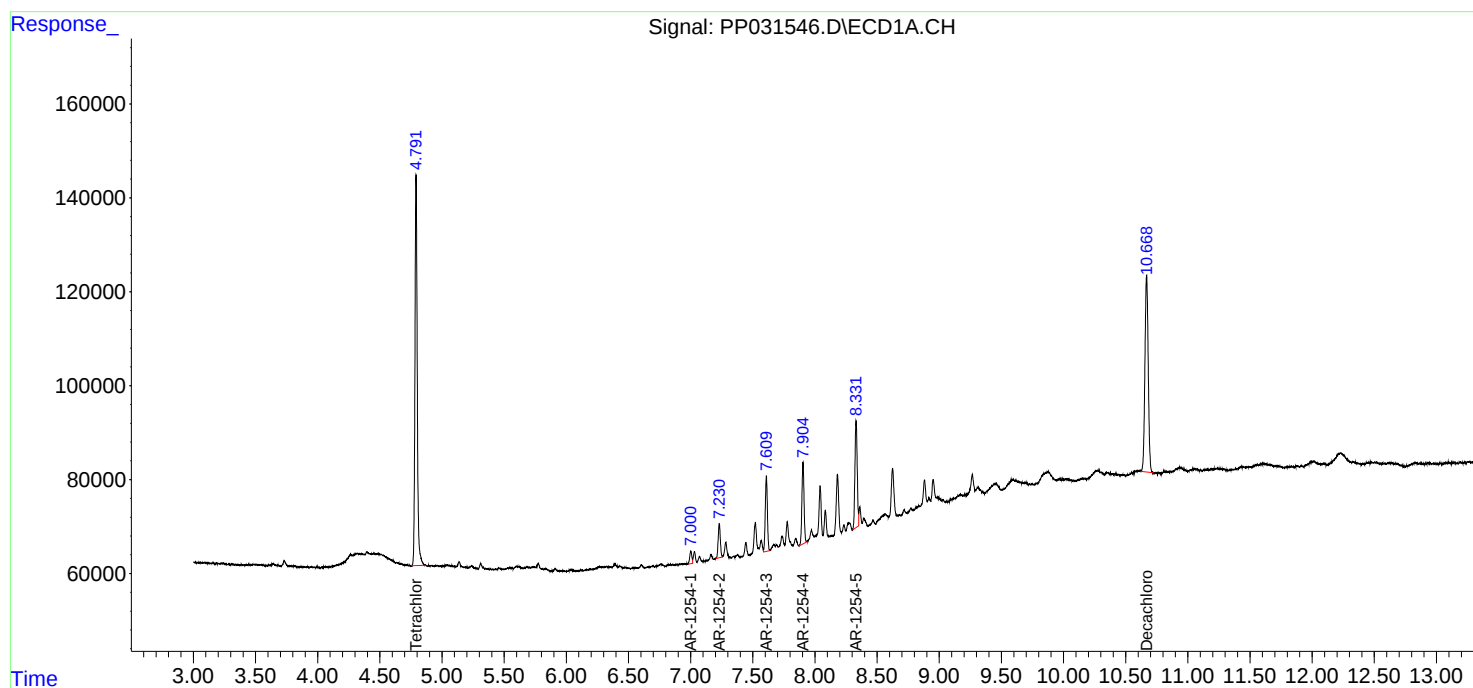

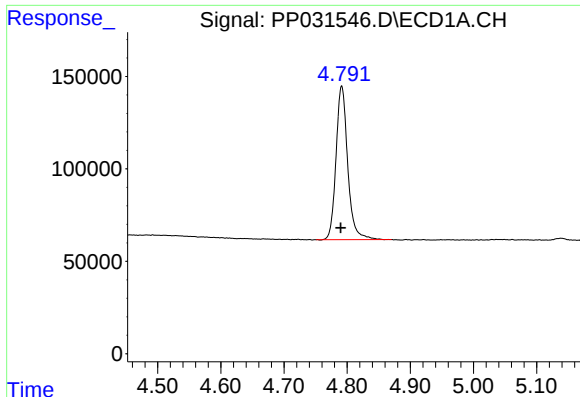


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: 0.001 min
Response: 1070388
Conc: 22.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:06 PM

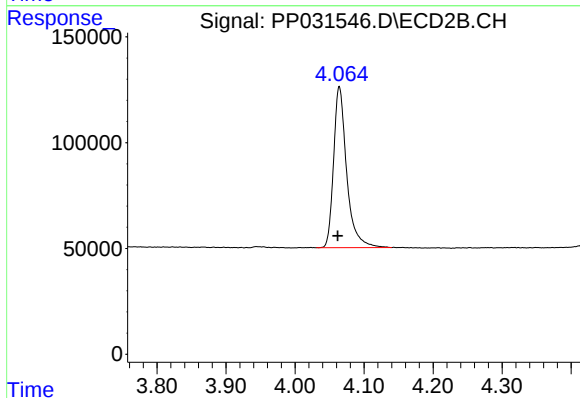


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.002 min
Response: 1004876
Conc: 20.97 ng/ml

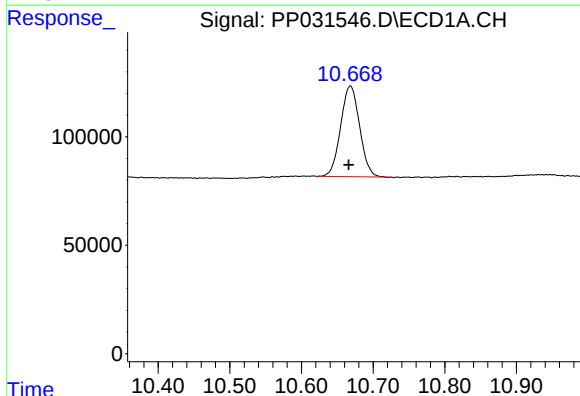


#2 Decachlorobiphenyl

R.T.: 10.668 min
Delta R.T.: 0.003 min
Response: 769323
Conc: 22.65 ng/ml

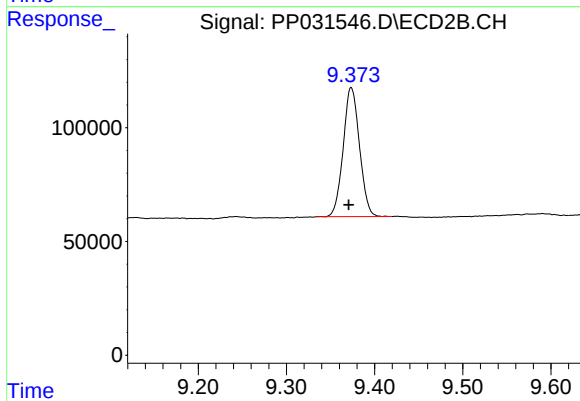

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.003 min
Response: 727985
Conc: 19.66 ng/ml

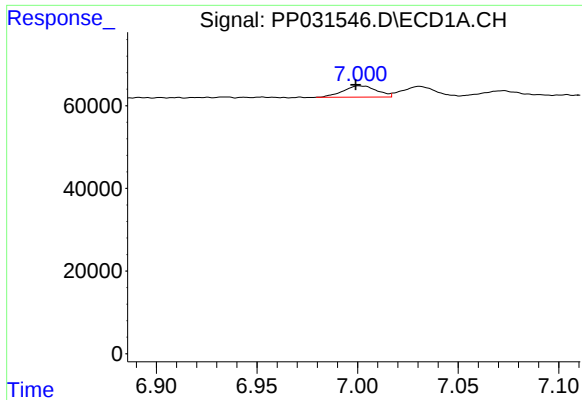


#26 AR-1254-1

R.T.: 7.000 min
Delta R.T.: 0.001 min
Response: 32195
Conc: 21.13 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:06 PM

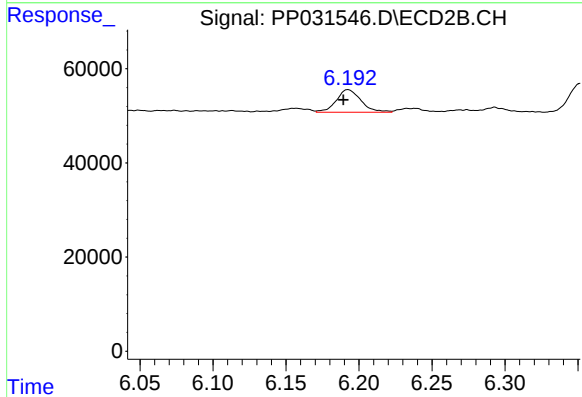


#26 AR-1254-1

R.T.: 6.192 min
Delta R.T.: 0.003 min
Response: 56614
Conc: 26.17 ng/ml

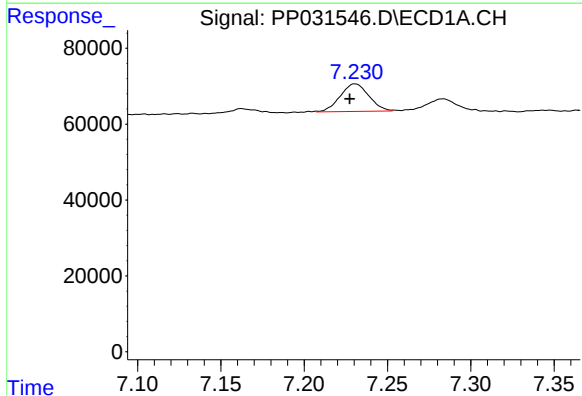


#27 AR-1254-2

R.T.: 7.230 min
Delta R.T.: 0.002 min
Response: 87031
Conc: 37.47 ng/ml m

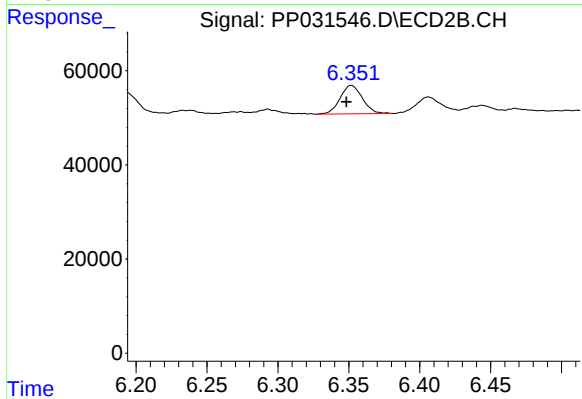

#27 AR-1254-2

R.T.: 6.352 min
Delta R.T.: 0.004 min
Response: 66134
Conc: 35.50 ng/ml

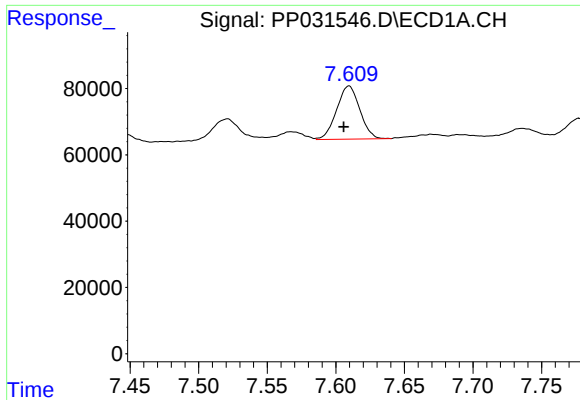


#28 AR-1254-3

R.T.: 7.610 min
Delta R.T.: 0.004 min
Response: 189278
Conc: 74.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-A


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:06 PM

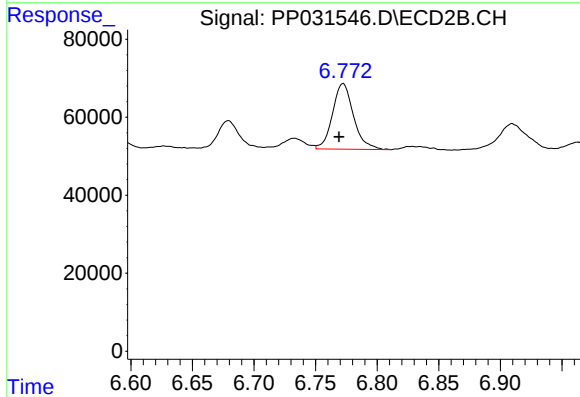


#28 AR-1254-3

R.T.: 6.772 min
Delta R.T.: 0.003 min
Response: 199910
Conc: 64.67 ng/ml

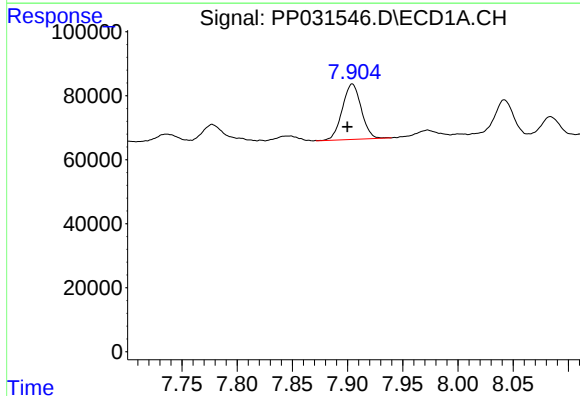


#29 AR-1254-4

R.T.: 7.904 min
Delta R.T.: 0.005 min
Response: 206997
Conc: 121.99 ng/ml

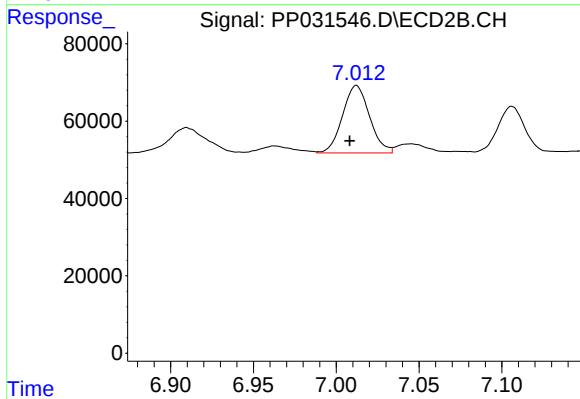

#29 AR-1254-4

R.T.: 7.012 min
Delta R.T.: 0.004 min
Response: 198281
Conc: 116.71 ng/ml

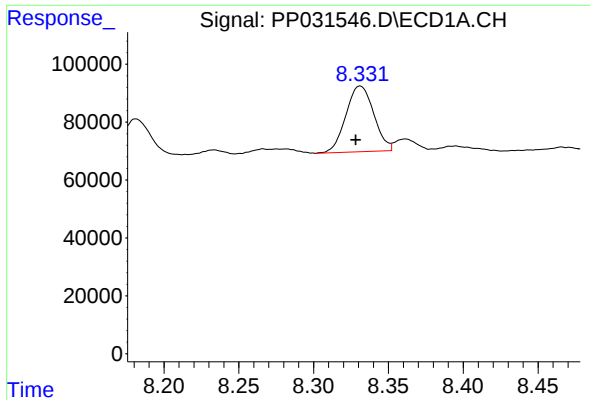


#30 AR-1254-5

R.T.: 8.331 min
Delta R.T.: 0.003 min
Response: 294169
Conc: 157.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-A

Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:06 PM

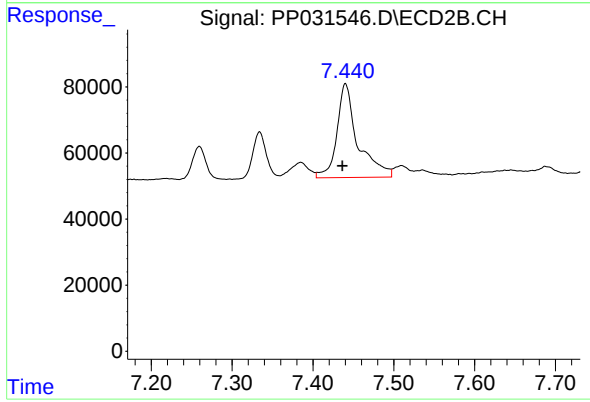

#30 AR-1254-5

R.T.: 7.440 min
Delta R.T.: 0.004 min
Response: 508788
Conc: 188.47 ng/ml