

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031547.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 11:02
 Operator : DD\AJ
 Sample : L4809-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-CON-B

Manual Integrations
 APPROVED

Ankita
 11/25/2020 4:35:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 12:09:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.791	4.065	1026483	955356	21.198	19.937
2)	SA Decachlor...	10.670	9.373	737052	705068	21.701	19.042
Target Compounds							
26)	L6 AR-1254-1	7.004	6.192	18085	20245	11.868m	9.359
27)	L6 AR-1254-2	7.232	6.351	23416	19294	10.083m	10.356
28)	L6 AR-1254-3	7.610	6.772	37660	38252	14.907	12.374
29)	L6 AR-1254-4	7.903	7.011	25692	25630	15.142m	15.086
30)	L6 AR-1254-5	8.332	7.440	33024	60761	17.665	22.508 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031547.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 11:02
Operator : DD\AJ
Sample : L4809-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
MS-CON-B


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 12:09:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

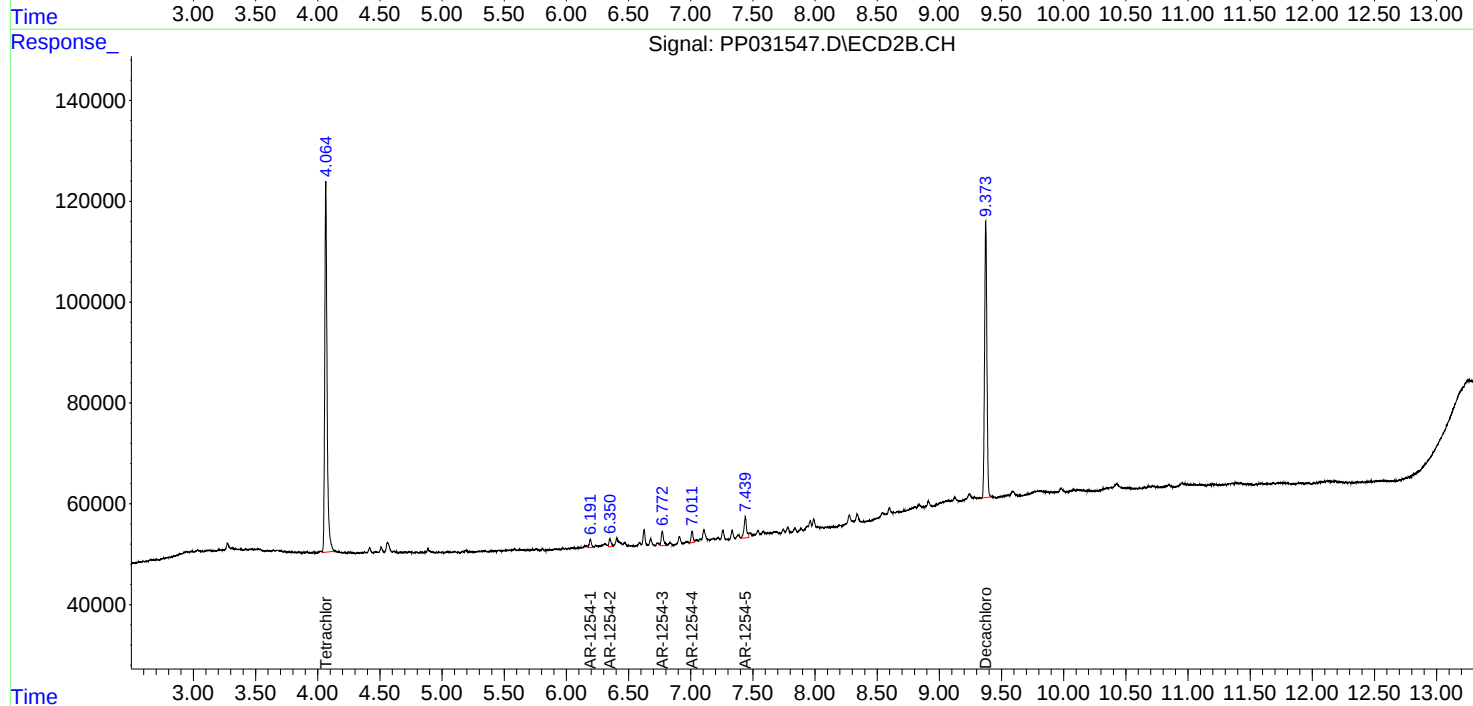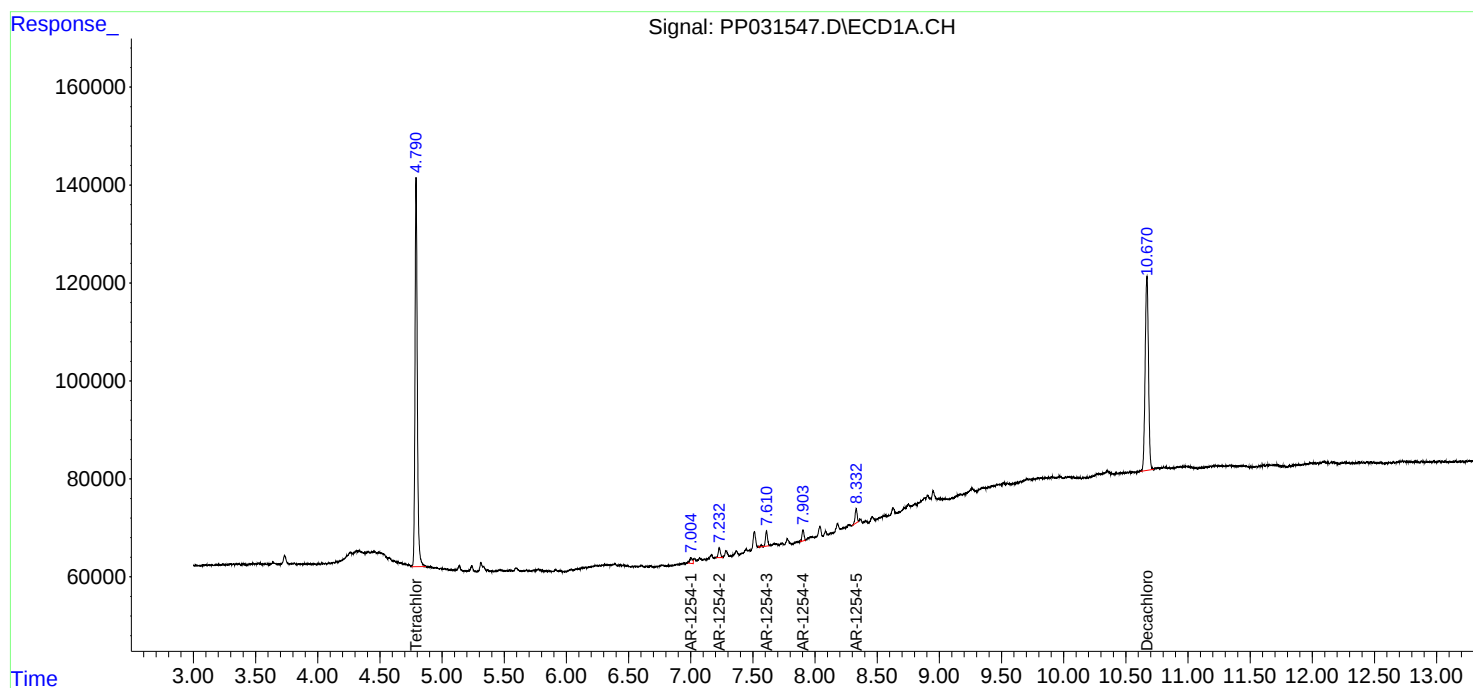

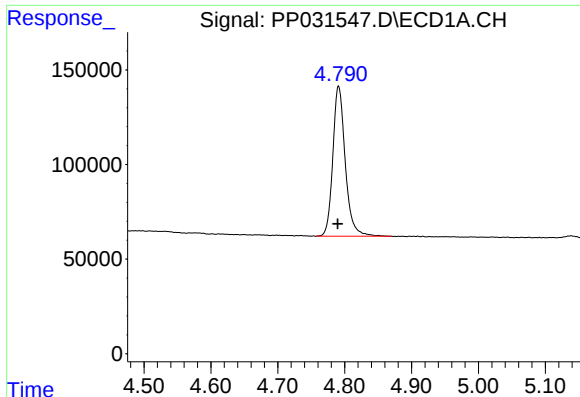


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 1026483
Conc: 21.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-B


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:08 PM

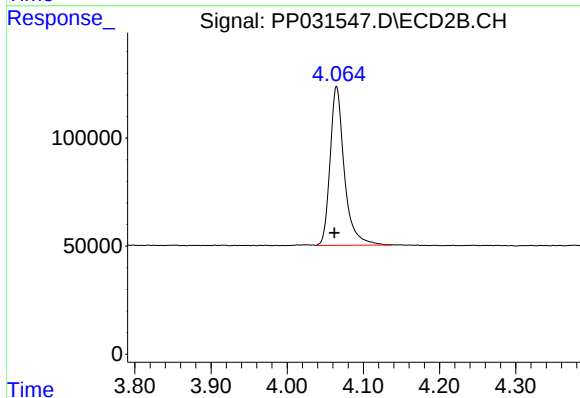


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.003 min
Response: 955356
Conc: 19.94 ng/ml

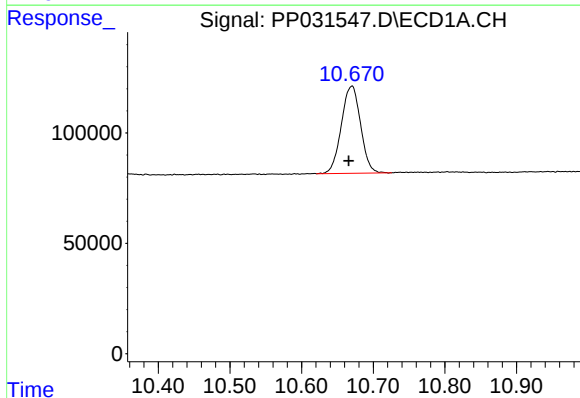


#2 Decachlorobiphenyl

R.T.: 10.670 min
Delta R.T.: 0.005 min
Response: 737052
Conc: 21.70 ng/ml

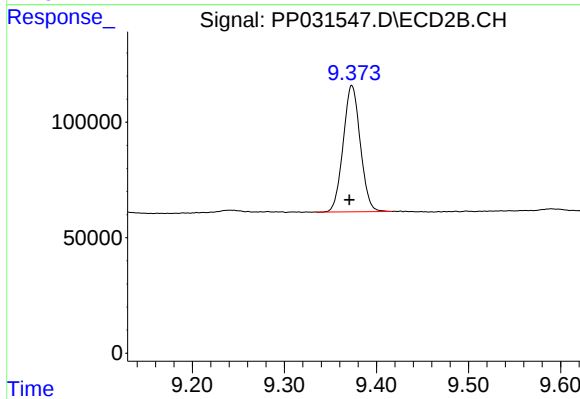

#2 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.002 min
Response: 705068
Conc: 19.04 ng/ml

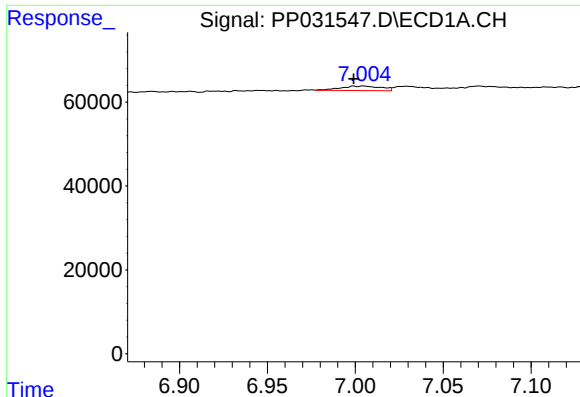


#26 AR-1254-1

R.T.: 7.004 min
Delta R.T.: 0.005 min
Response: 18085
Conc: 11.87 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MS-CON-B


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:08 PM

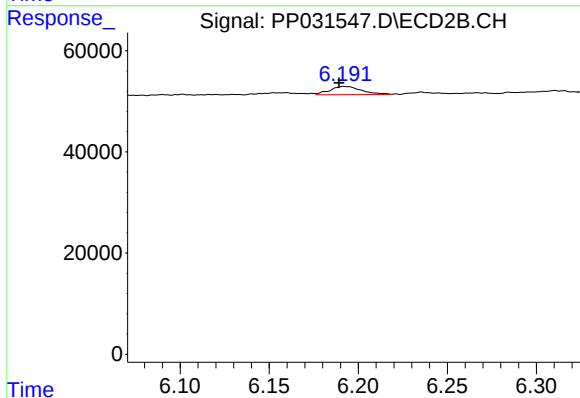


#26 AR-1254-1

R.T.: 6.192 min
Delta R.T.: 0.003 min
Response: 20245
Conc: 9.36 ng/ml

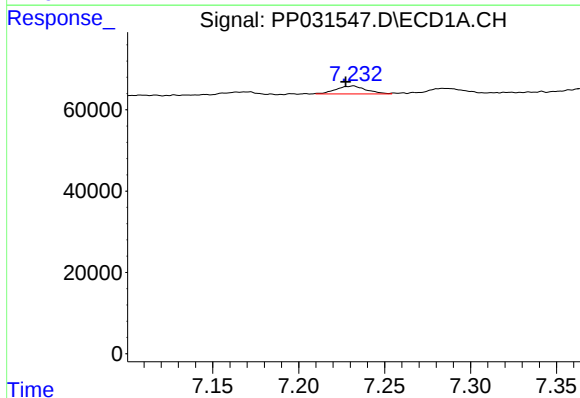


#27 AR-1254-2

R.T.: 7.232 min
Delta R.T.: 0.004 min
Response: 23416
Conc: 10.08 ng/ml m

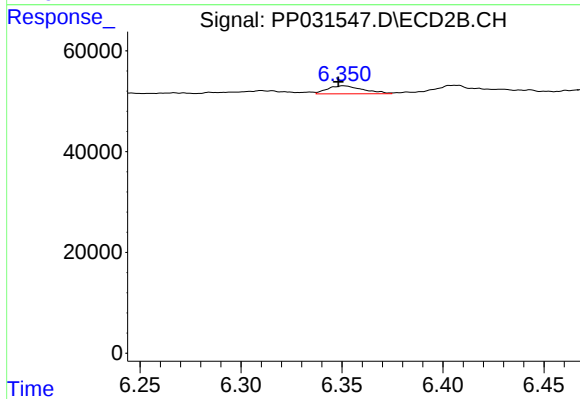

#27 AR-1254-2

R.T.: 6.351 min
Delta R.T.: 0.002 min
Response: 19294
Conc: 10.36 ng/ml

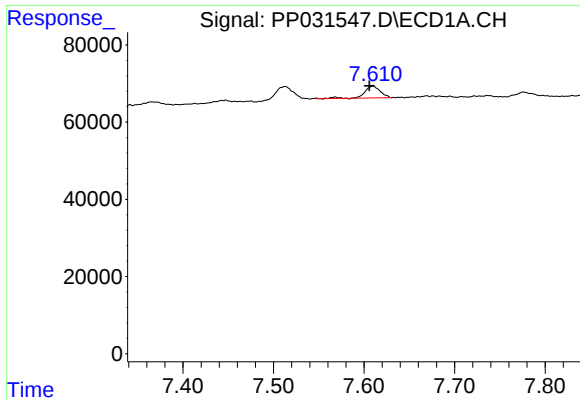


#28 AR-1254-3

R.T.: 7.610 min
Delta R.T.: 0.004 min
Response: 37660
Conc: 14.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-B


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:08 PM

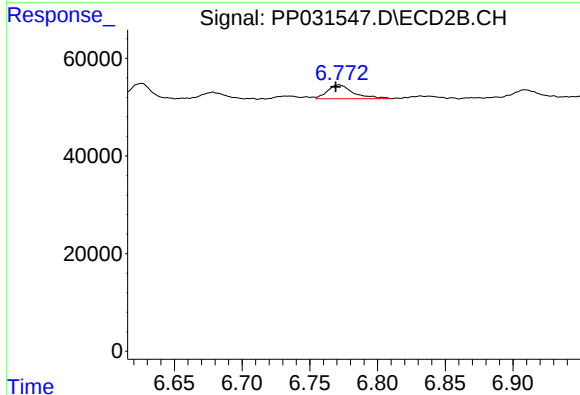


#28 AR-1254-3

R.T.: 6.772 min
Delta R.T.: 0.003 min
Response: 38252
Conc: 12.37 ng/ml

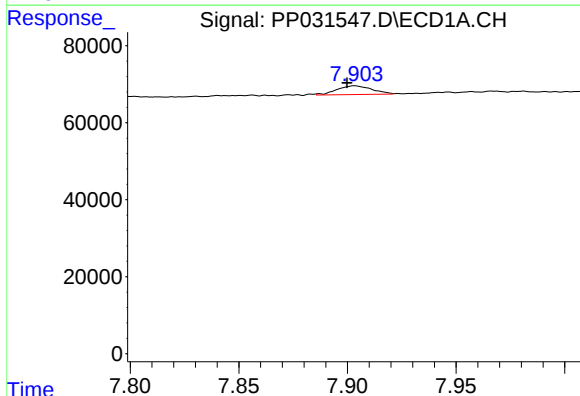


#29 AR-1254-4

R.T.: 7.903 min
Delta R.T.: 0.003 min
Response: 25692
Conc: 15.14 ng/ml m

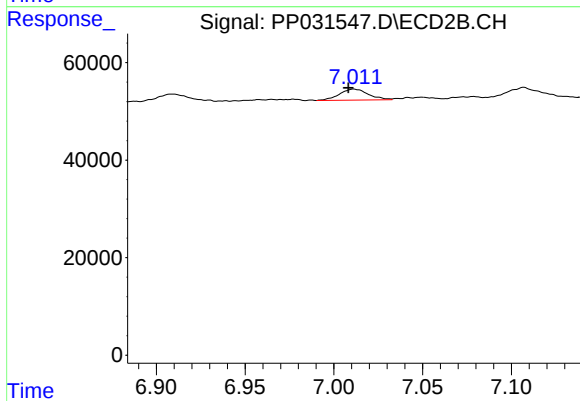

#29 AR-1254-4

R.T.: 7.011 min
Delta R.T.: 0.003 min
Response: 25630
Conc: 15.09 ng/ml

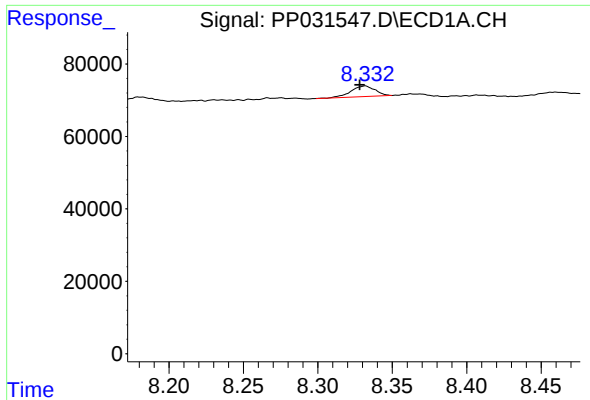


#30 AR-1254-5

R.T.: 8.332 min
Delta R.T.: 0.004 min
Response: 33024
Conc: 17.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-CON-B

Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:08 PM

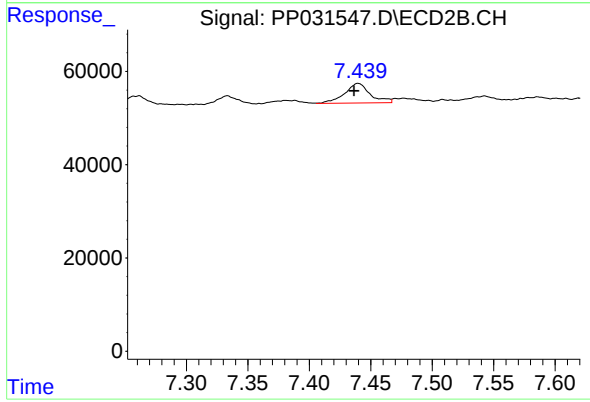

#30 AR-1254-5

R.T.: 7.440 min
Delta R.T.: 0.003 min
Response: 60761
Conc: 22.51 ng/ml