

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031553.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 12:42
 Operator : DD\AJ
 Sample : L4792-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 340EM-006-0002

Manual Integrations
 APPROVED

Ankita
 11/25/2020 4:35:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 14:18:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.065	996300	923530	20.575m	19.273
2) SA Decachlor...	10.669	9.372	872519	860116	25.689	23.229
Target Compounds						
41) L9 AR-1268-1	9.249	8.276	788291	777903	164.037	140.592
42) L9 AR-1268-2	9.339	8.341	806825	841373	173.318	155.617
43) L9 AR-1268-3	9.555	8.548	215504	225479	53.293	49.160
44) L9 AR-1268-4	9.964	8.837	511122	518285	329.059	284.349
45) L9 AR-1268-5	10.355	9.123	1147274	1158746	94.051	83.679

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031553.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 12:42
Operator : DD\AJ
Sample : L4792-09
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
340EM-006-0002


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 14:18:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

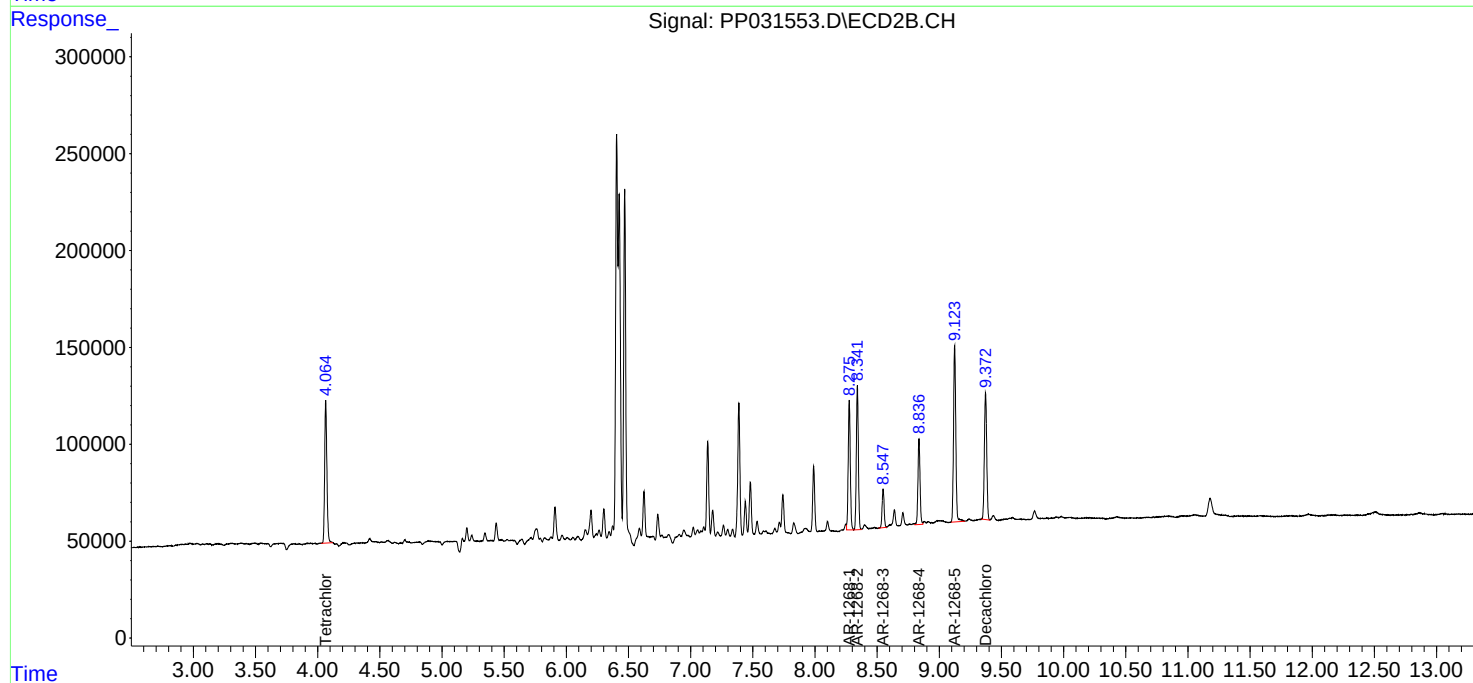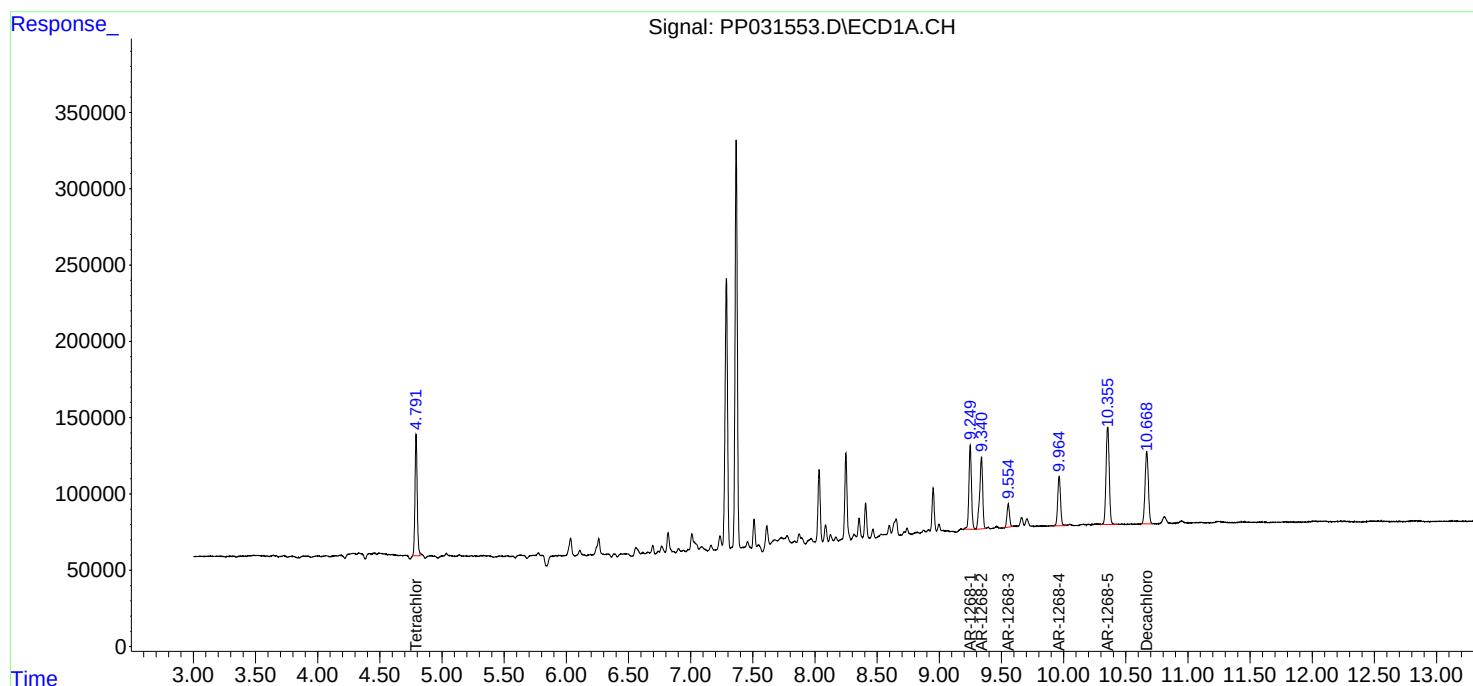

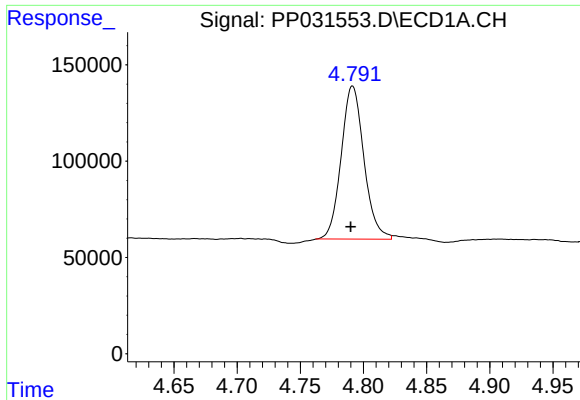


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 996300
Conc: 20.57 ng/ml m

Instrument :
ECD_P
ClientSampleId :
340EM-006-0002


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:15 PM

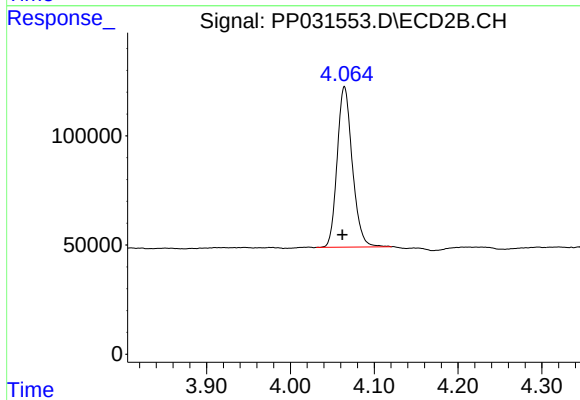


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.002 min
Response: 923530
Conc: 19.27 ng/ml

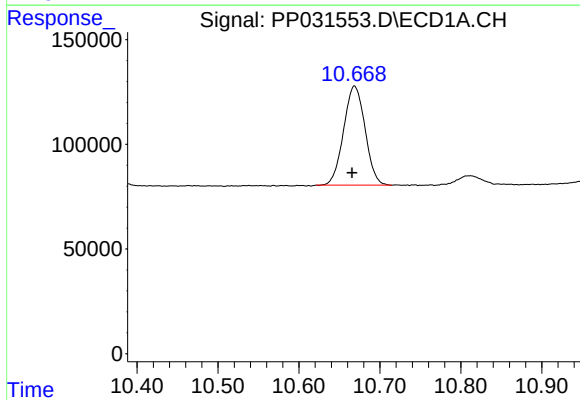


#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: 0.003 min
Response: 872519
Conc: 25.69 ng/ml

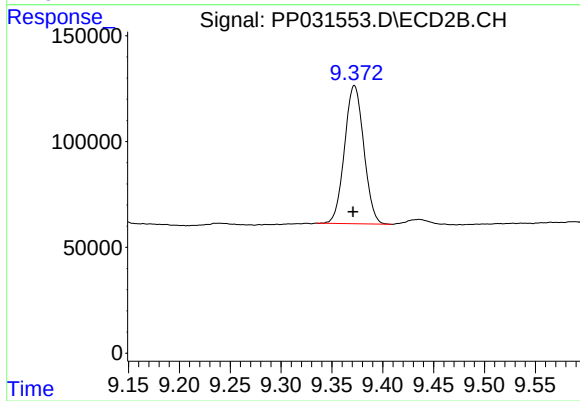

#2 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.001 min
Response: 860116
Conc: 23.23 ng/ml

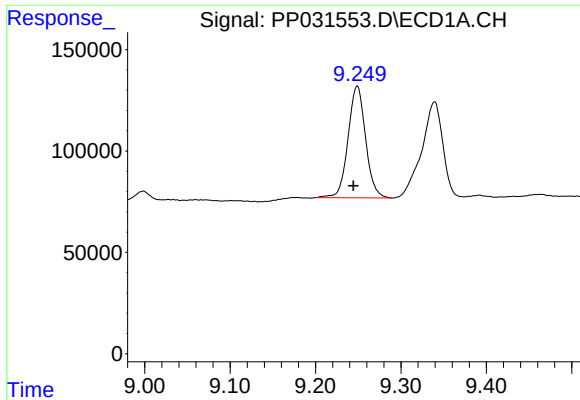


#41 AR-1268-1

R.T.: 9.249 min
Delta R.T.: 0.004 min
Response: 788291
Conc: 164.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
340EM-006-0002


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:15 PM

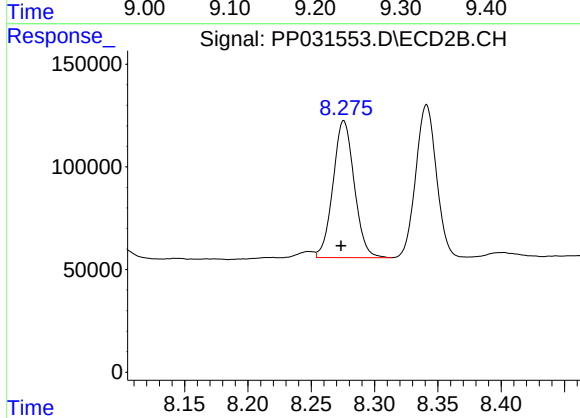


#41 AR-1268-1

R.T.: 8.276 min
Delta R.T.: 0.002 min
Response: 777903
Conc: 140.59 ng/ml

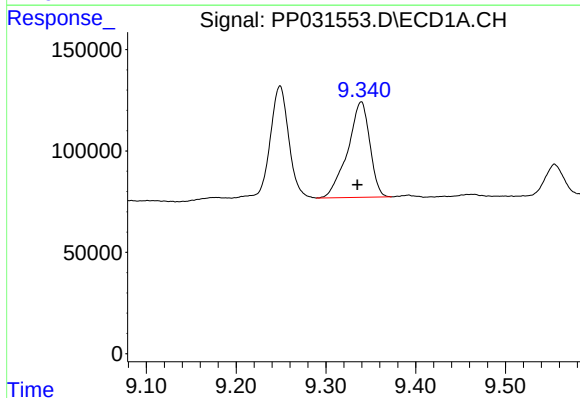


#42 AR-1268-2

R.T.: 9.339 min
Delta R.T.: 0.004 min
Response: 806825
Conc: 173.32 ng/ml

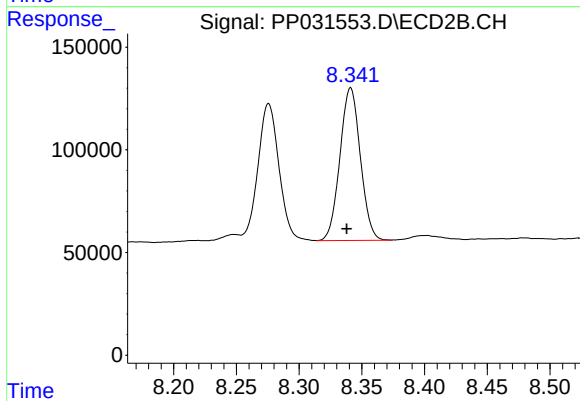

#42 AR-1268-2

R.T.: 8.341 min
Delta R.T.: 0.003 min
Response: 841373
Conc: 155.62 ng/ml

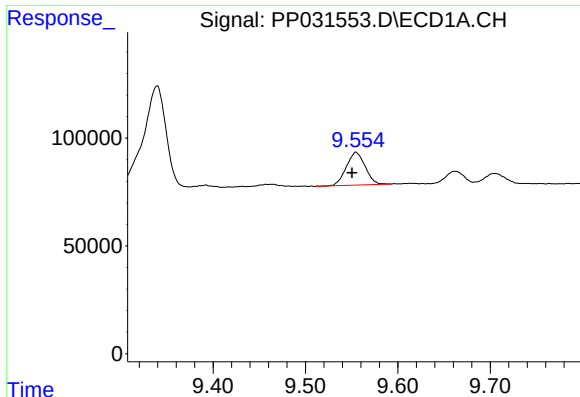


#43 AR-1268-3

R.T.: 9.555 min
Delta R.T.: 0.004 min
Response: 215504
Conc: 53.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
340EM-006-0002


Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:15 PM

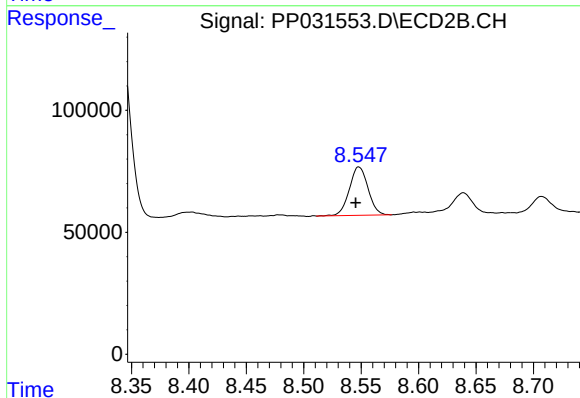


#43 AR-1268-3

R.T.: 8.548 min
Delta R.T.: 0.003 min
Response: 225479
Conc: 49.16 ng/ml

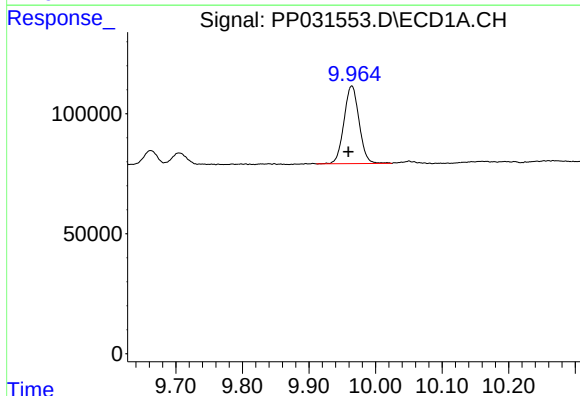


#44 AR-1268-4

R.T.: 9.964 min
Delta R.T.: 0.005 min
Response: 511122
Conc: 329.06 ng/ml

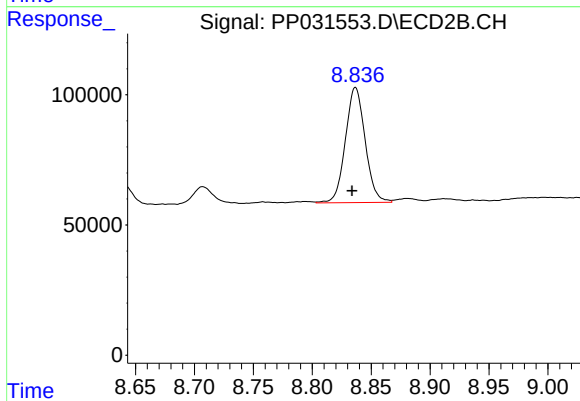

#44 AR-1268-4

R.T.: 8.837 min
Delta R.T.: 0.003 min
Response: 518285
Conc: 284.35 ng/ml

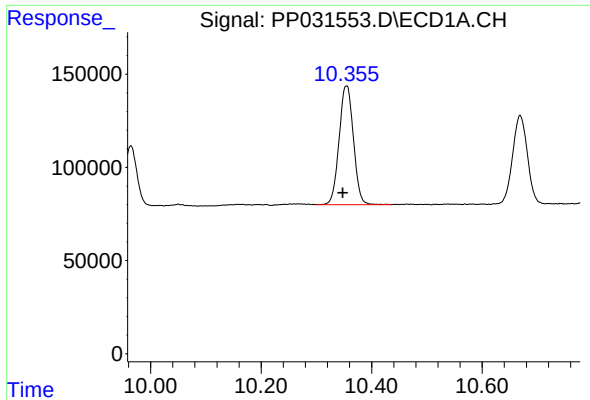


#45 AR-1268-5

R.T.: 10.355 min
Delta R.T.: 0.007 min
Response: 1147274
Conc: 94.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
340EM-006-0002

Manual Integrations
APPROVED

Ankita
11/25/2020 4:35:15 PM

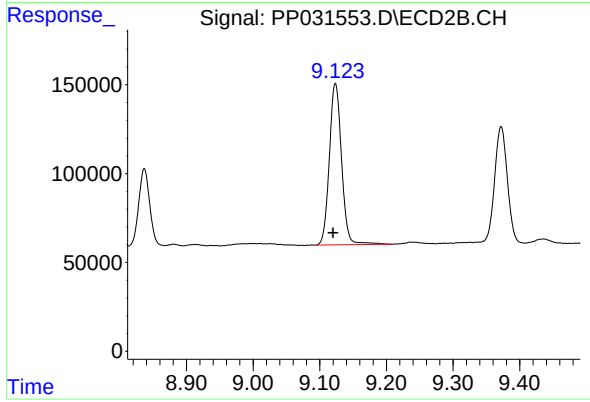

#45 AR-1268-5

R.T.: 9.123 min
Delta R.T.: 0.003 min
Response: 1158746
Conc: 83.68 ng/ml