

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031583.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 21:19
 Operator : DD\AJ
 Sample : L4868-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-B3-112020-0-2

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:28:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 01:33:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.789	4.061	1022767	895646	21.121	18.691
2) SA Decachlor...	10.665	9.369	610105	58143	17.963	1.570m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031583.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 21:19
Operator : DD\AJ
Sample : L4868-02
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KENS-B3-112020-0-2


Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 01:33:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

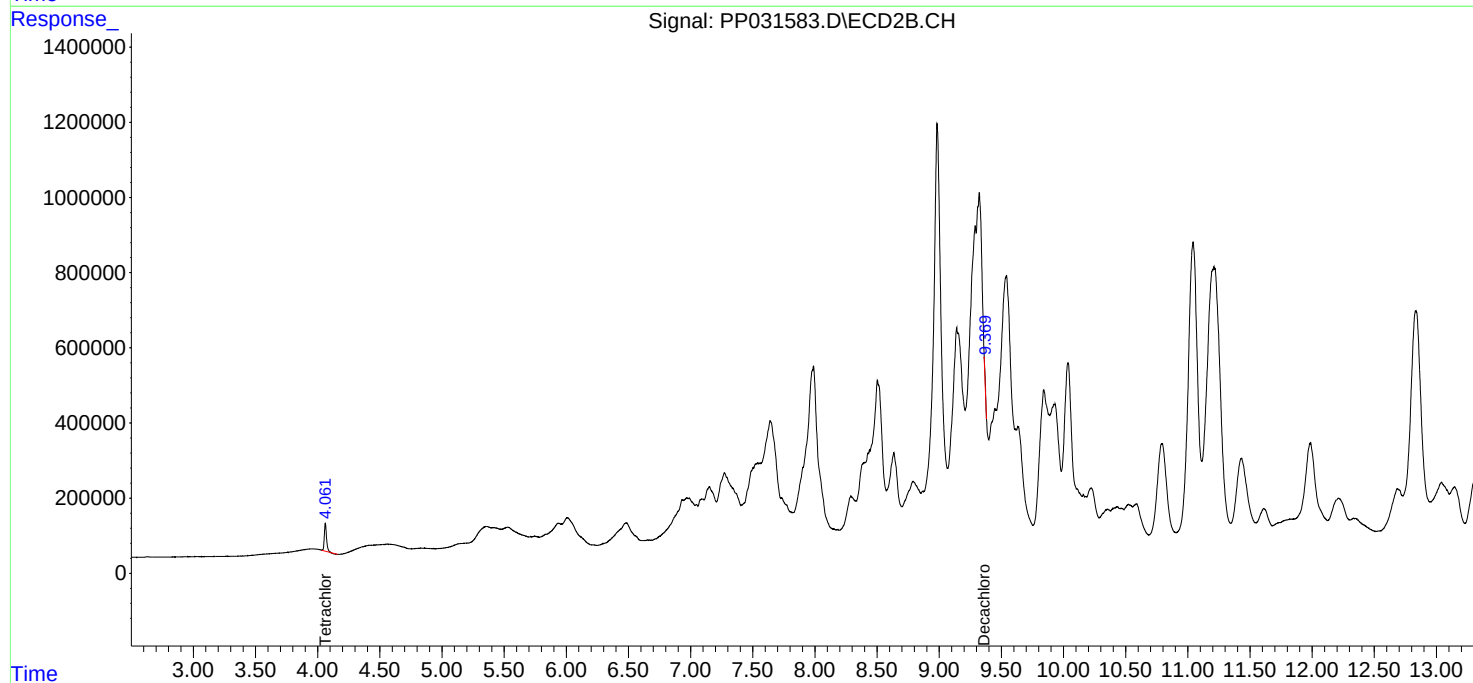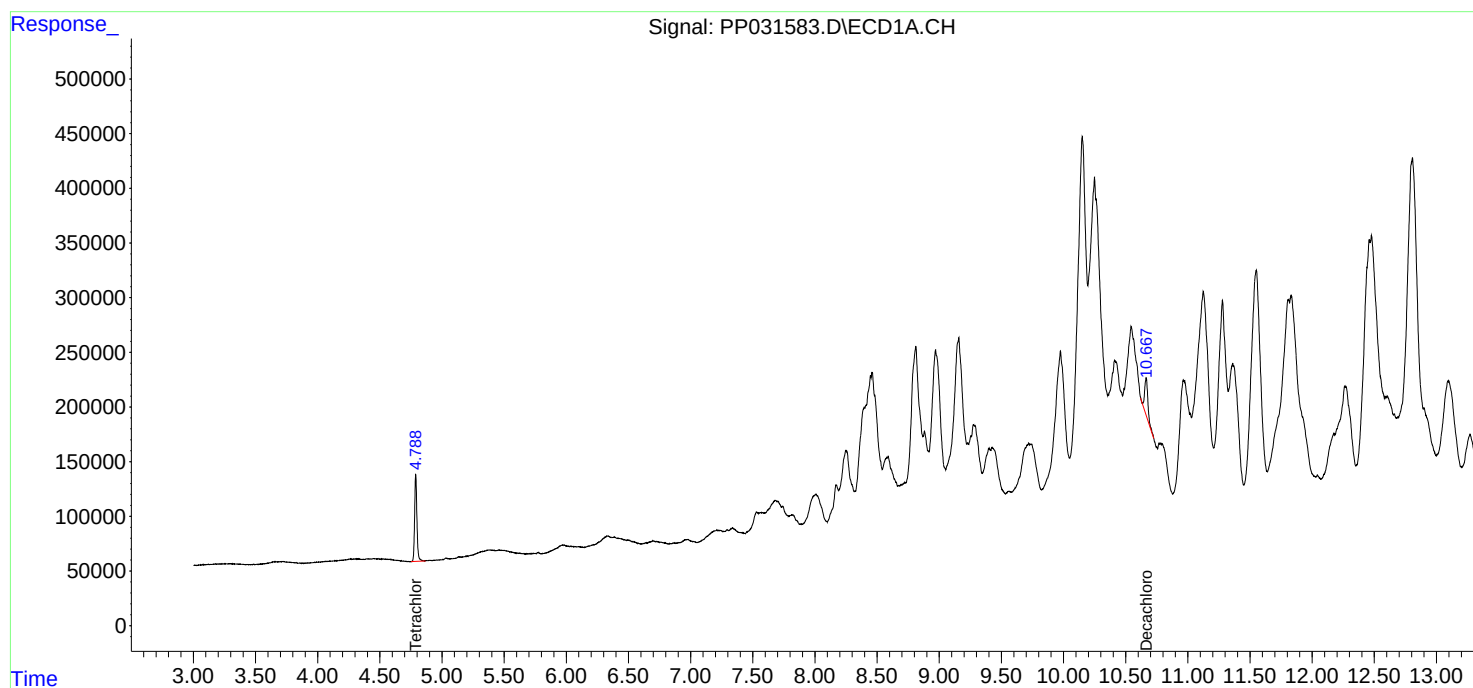

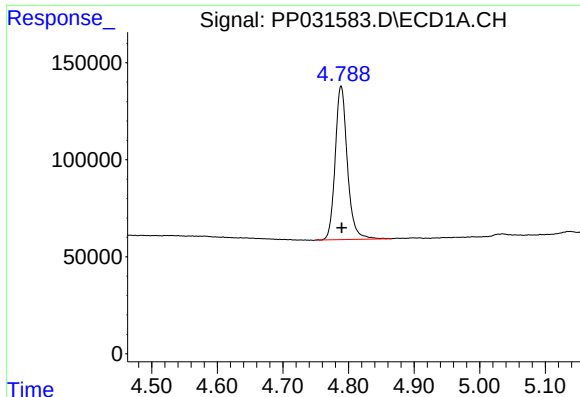


#1 Tetrachloro-m-xylene

R.T.: 4.789 min
Delta R.T.: -0.001 min
Response: 1022767
Conc: 21.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B3-112020-0-2


Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:46 PM

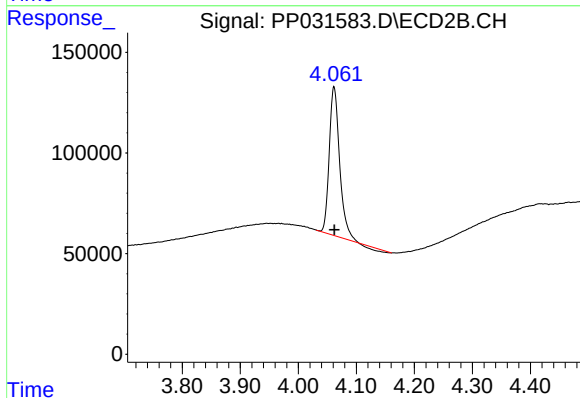


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 895646
Conc: 18.69 ng/ml

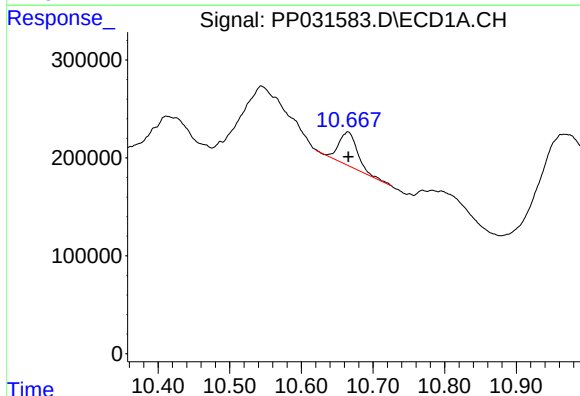

#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: 0.000 min
Response: 610105
Conc: 17.96 ng/ml

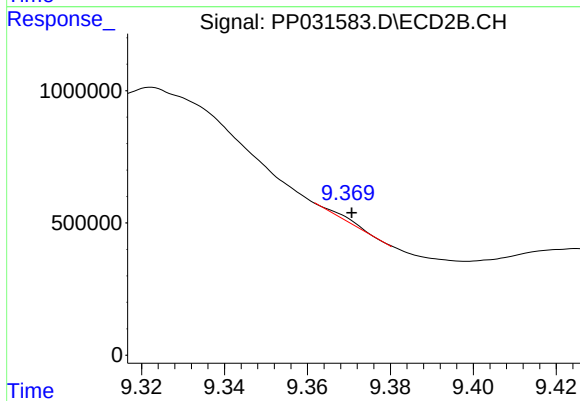

#2 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.002 min
Response: 58143
Conc: 1.57 ng/ml m