

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
 Data File : PP031601.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 3:38
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:28:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 03:40:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 23 04:59:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.062	2396356	2311678	49.488	48.242
2) SA Decachlor...	10.665	9.368	1699809	1878860	50.047	50.743
Target Compounds						
21) L5 AR-1248-1	6.095	5.317	417375	398095	451.989	462.196
22) L5 AR-1248-2	6.389	5.580	518489	538319	438.336	450.849
23) L5 AR-1248-3	6.603	5.625	653819	571698	446.924	451.678
24) L5 AR-1248-4	7.029	5.808	711769	620602	453.875	405.078m
25) L5 AR-1248-5	7.068	6.232	701126	681125	441.660	466.837

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112320\
Data File : PP031601.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 3:38
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 03:40:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 23 04:59:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

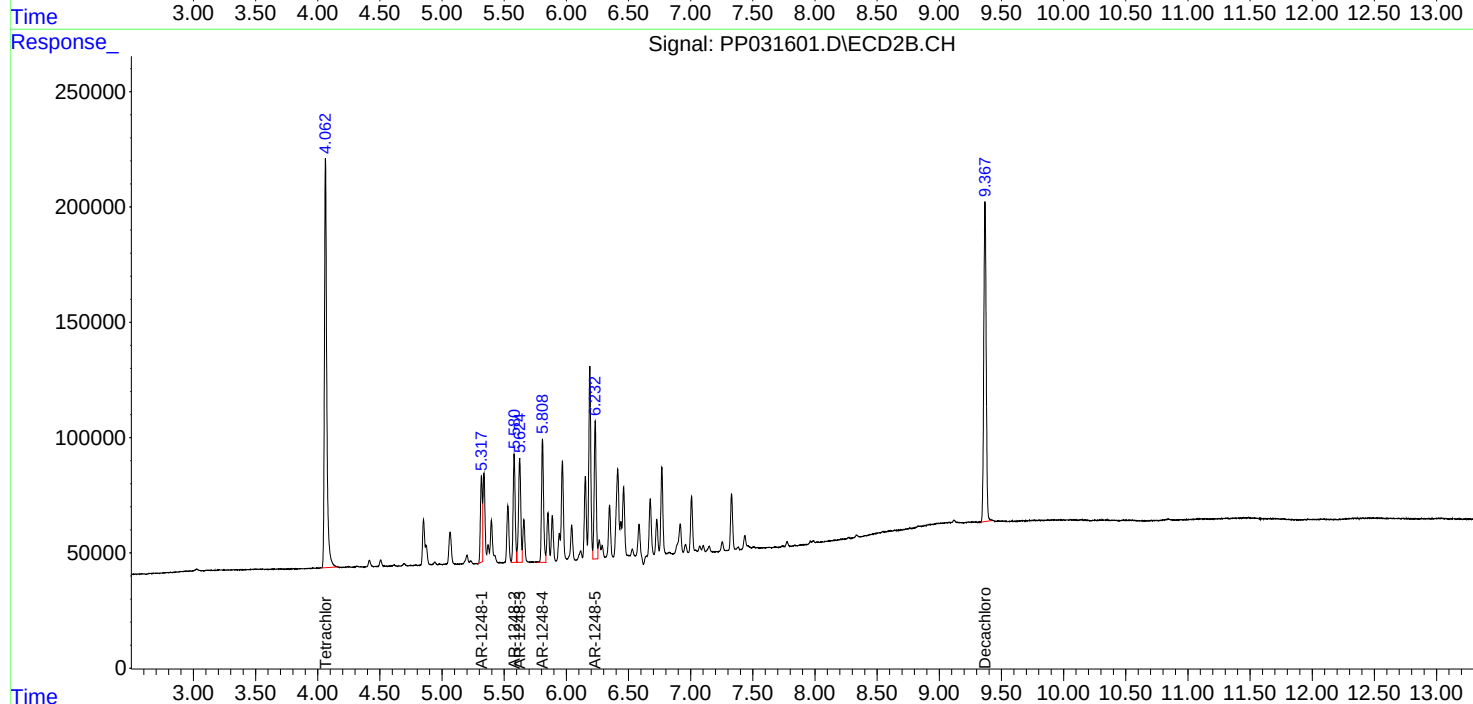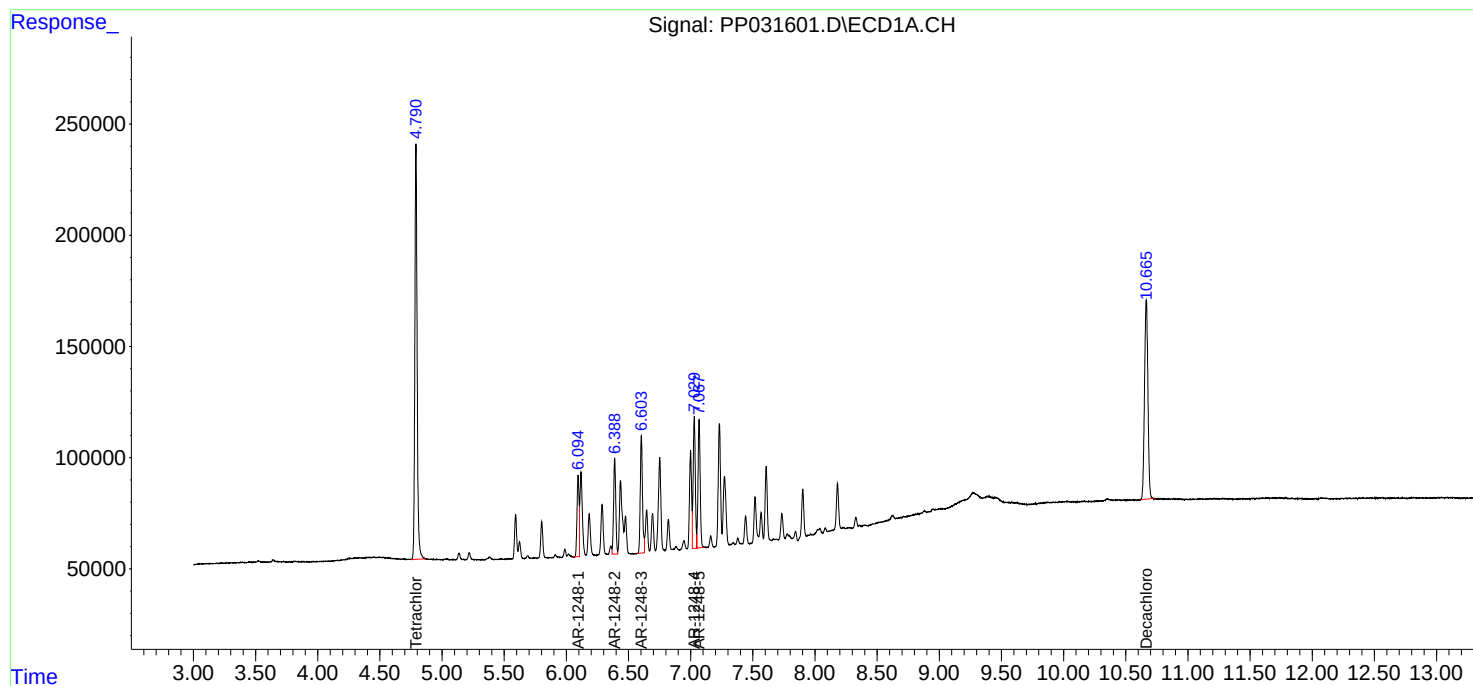

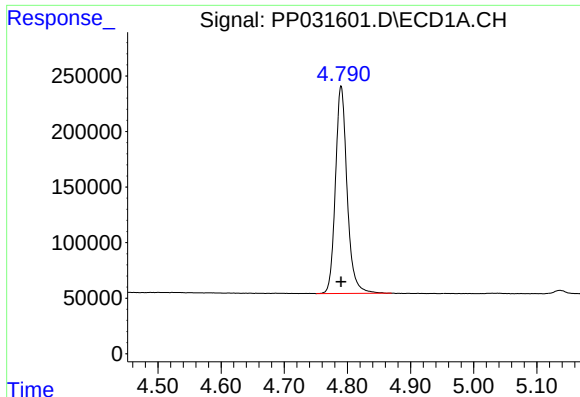


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 2396356
Conc: 49.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:59 PM

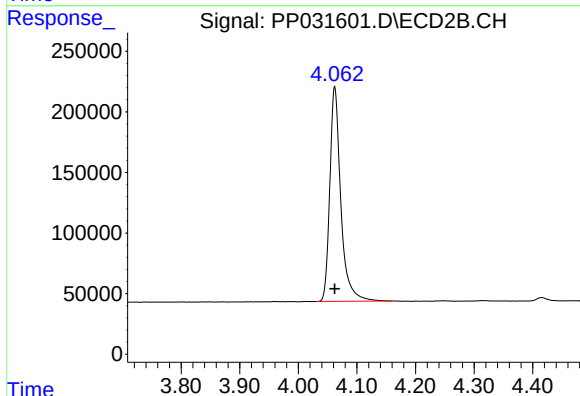


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: 0.000 min
Response: 2311678
Conc: 48.24 ng/ml

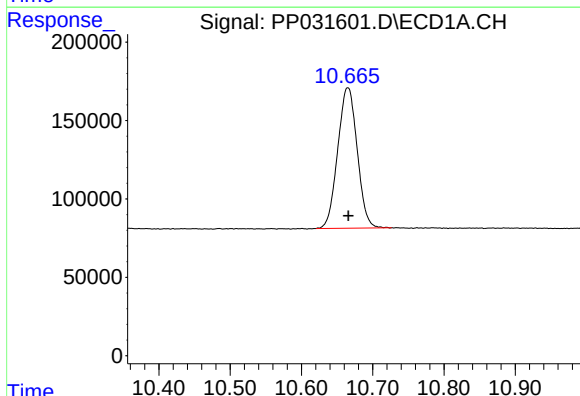


#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: 0.000 min
Response: 1699809
Conc: 50.05 ng/ml

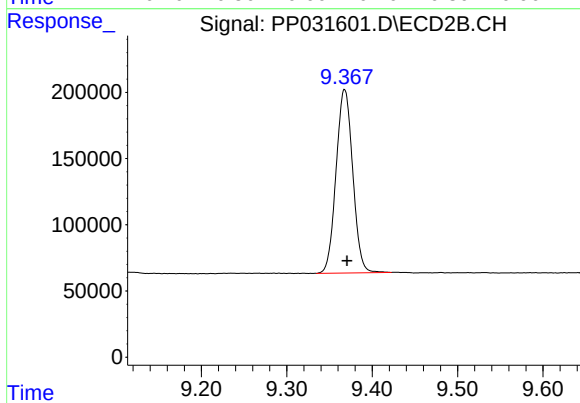

#2 Decachlorobiphenyl

R.T.: 9.368 min
Delta R.T.: -0.003 min
Response: 1878860
Conc: 50.74 ng/ml

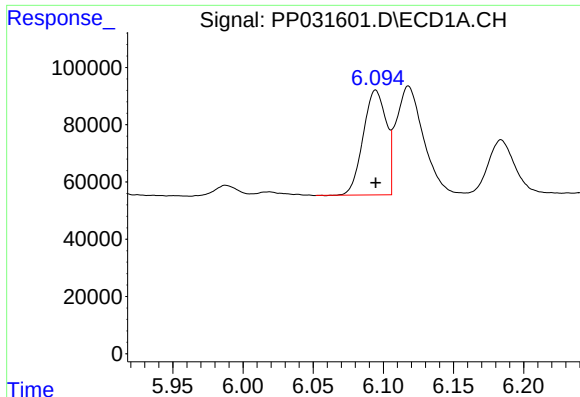


#21 AR-1248-1

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 417375
Conc: 451.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:59 PM

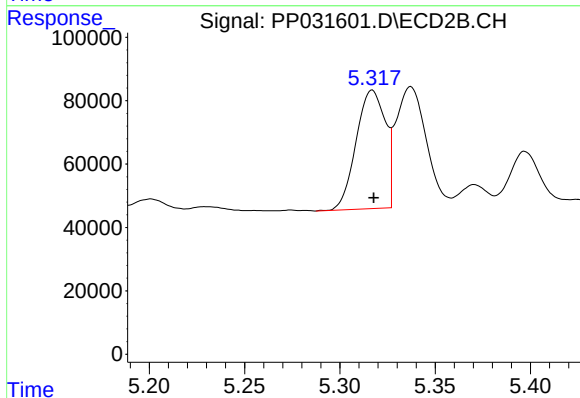


#21 AR-1248-1

R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 398095
Conc: 462.20 ng/ml

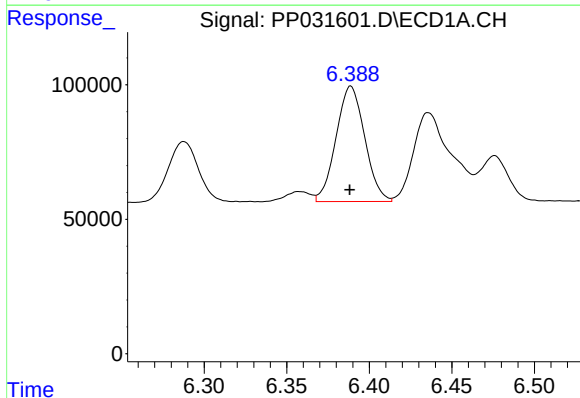


#22 AR-1248-2

R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 518489
Conc: 438.34 ng/ml

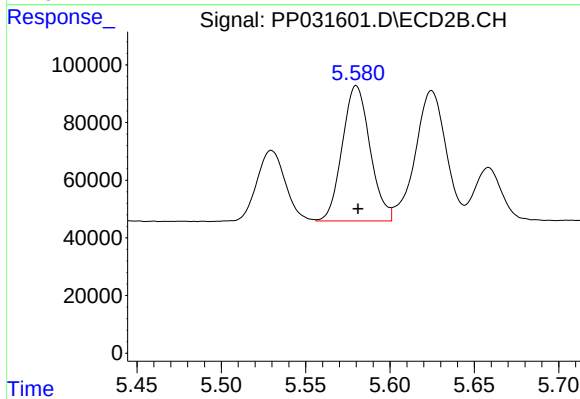

#22 AR-1248-2

R.T.: 5.580 min
Delta R.T.: -0.001 min
Response: 538319
Conc: 450.85 ng/ml

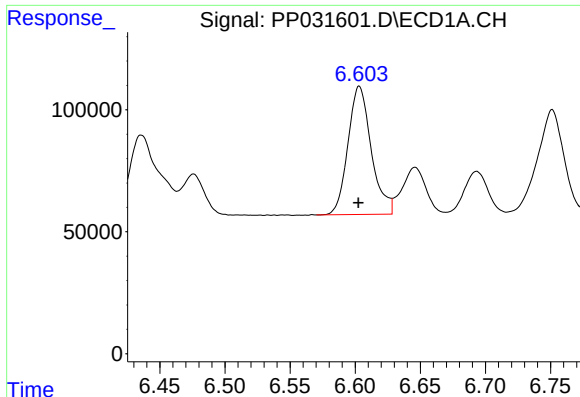


#23 AR-1248-3

R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 653819
Conc: 446.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:59 PM

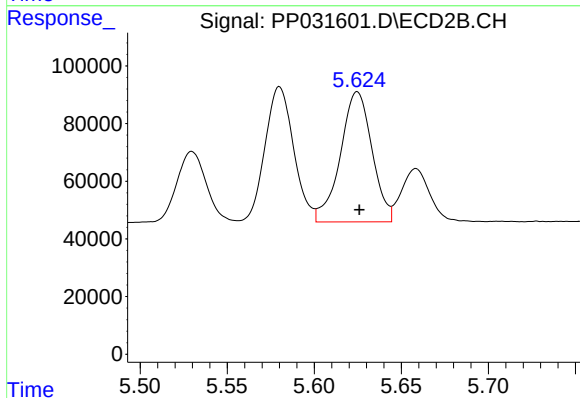


#23 AR-1248-3

R.T.: 5.625 min
Delta R.T.: -0.001 min
Response: 571698
Conc: 451.68 ng/ml

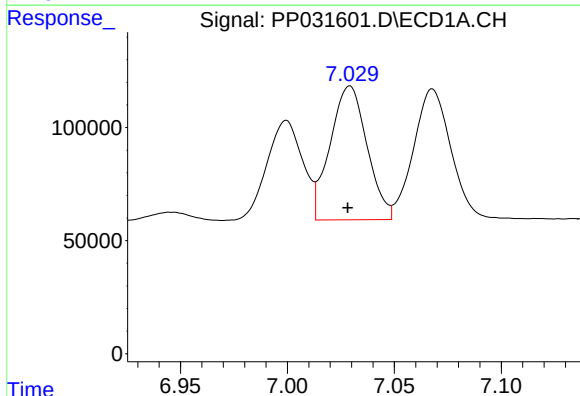


#24 AR-1248-4

R.T.: 7.029 min
Delta R.T.: 0.000 min
Response: 711769
Conc: 453.88 ng/ml

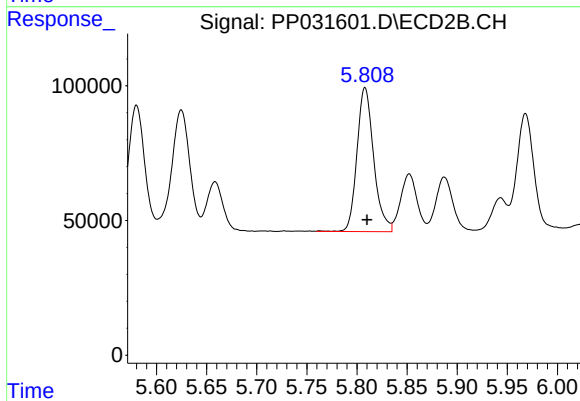

#24 AR-1248-4

R.T.: 5.808 min
Delta R.T.: -0.002 min
Response: 620602
Conc: 405.08 ng/ml m

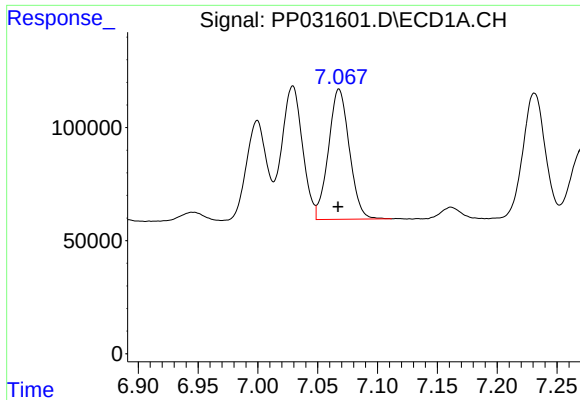


#25 AR-1248-5

R.T.: 7.068 min
Delta R.T.: 0.000 min
Response: 701126
Conc: 441.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
11/25/2020 5:28:59 PM

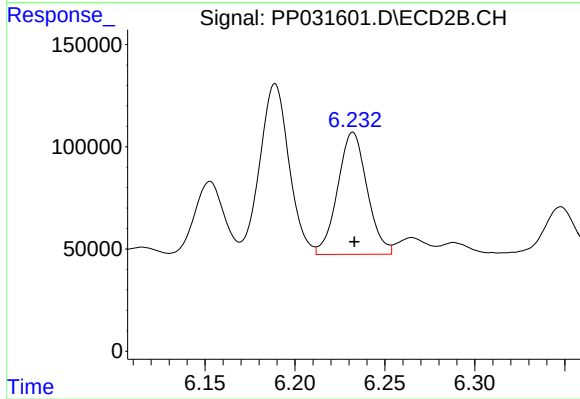

#25 AR-1248-5

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 681125
Conc: 466.84 ng/ml