

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112321\
 Data File : PP041252.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2021 15:02
 Operator : AJ\MA
 Sample : M4808-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-20001

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
 Supervised By :mohammad ahmed 11/24/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 17:24:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	3.757	366052	534088	17.358	19.218
2) SA Decachlor...	10.653	9.018	538971	360542	24.674	25.151
Target Compounds						
31) L7 AR-1260-1	7.751	6.587	42323	57364	42.939	59.921 #
32) L7 AR-1260-2	8.017	6.787	58657	61316	49.634	56.512
33) L7 AR-1260-3	8.381	6.939	40314	50095	44.408	49.926
34) L7 AR-1260-4	8.610	7.421	34719	37924	32.132m	46.238 #
35) L7 AR-1260-5	8.926	7.672	72690	76522	34.880	43.845 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112321\
Data File : PP041252.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2021 15:02
Operator : AJ\MA
Sample : M4808-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CHRT-20001


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 17:24:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

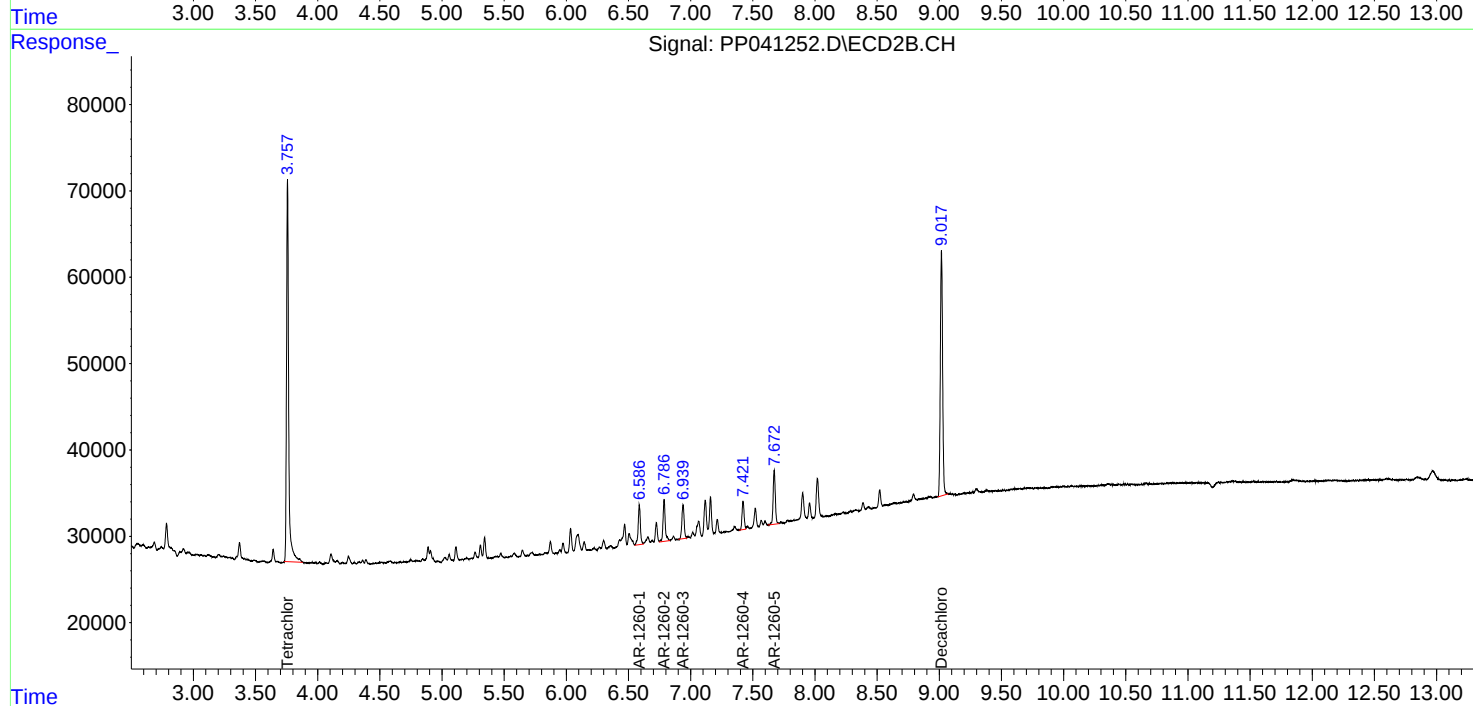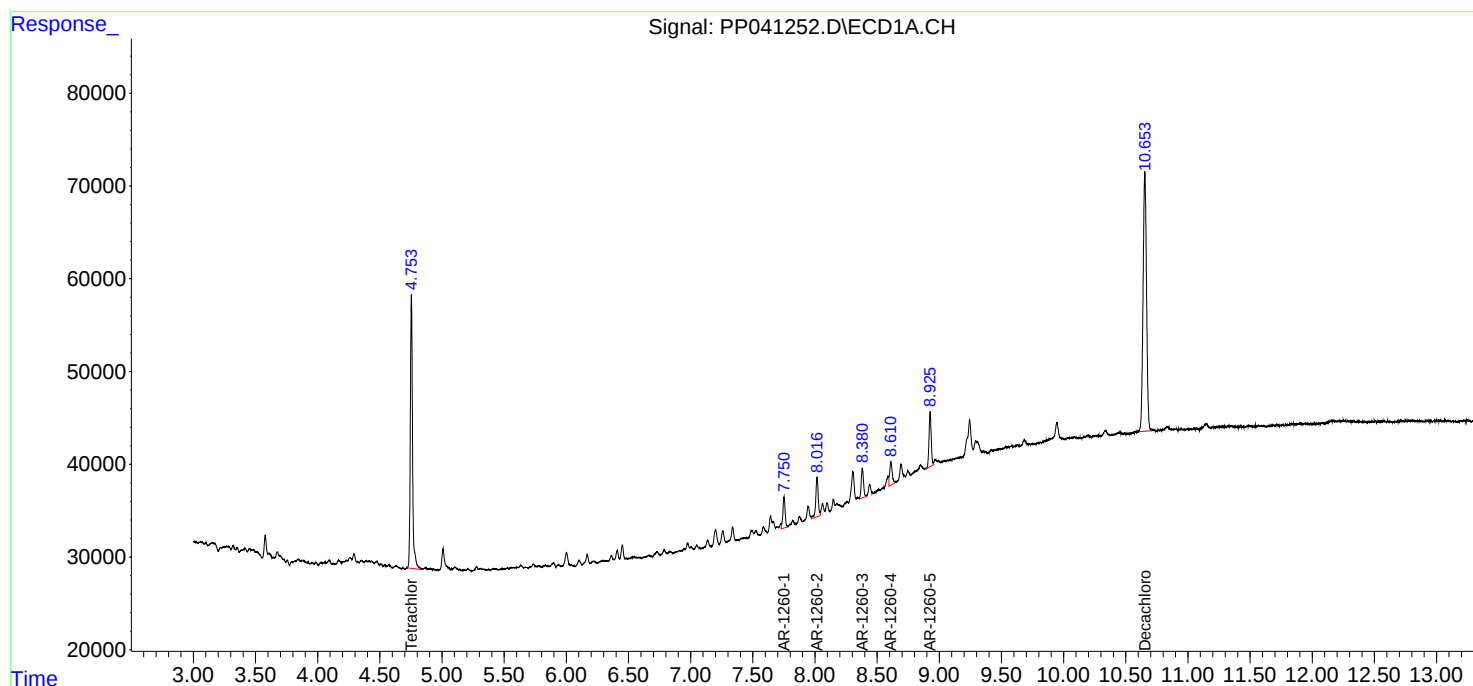

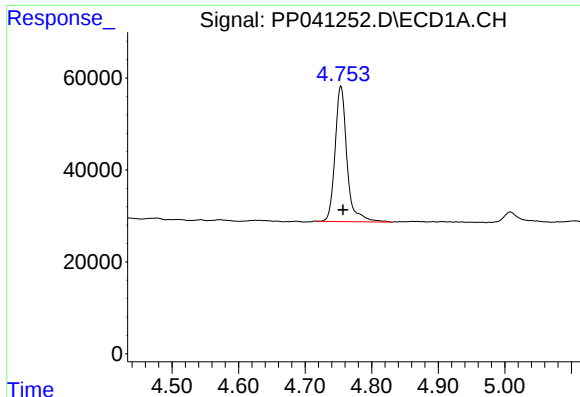


#1 Tetrachloro-m-xylene

R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 366052
Conc: 17.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-20001


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

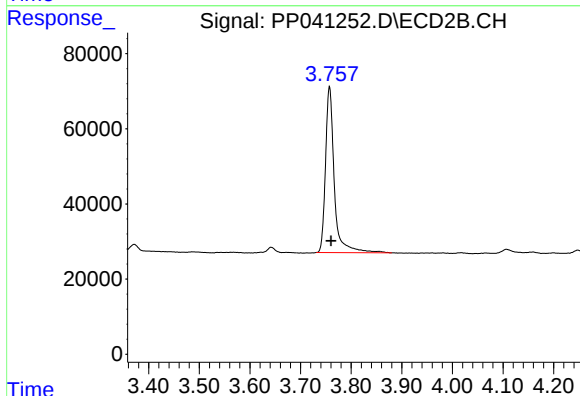


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 534088
Conc: 19.22 ng/ml

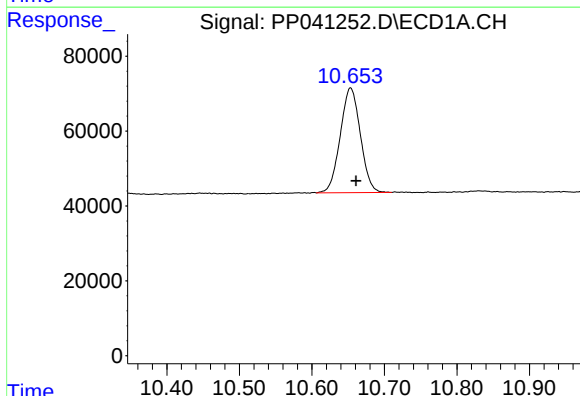


#2 Decachlorobiphenyl

R.T.: 10.653 min
Delta R.T.: -0.007 min
Response: 538971
Conc: 24.67 ng/ml

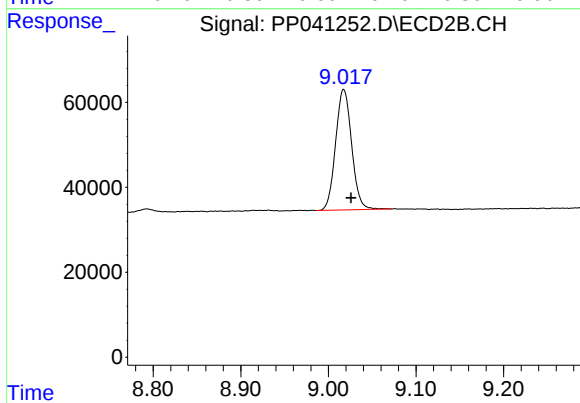

#2 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: -0.008 min
Response: 360542
Conc: 25.15 ng/ml

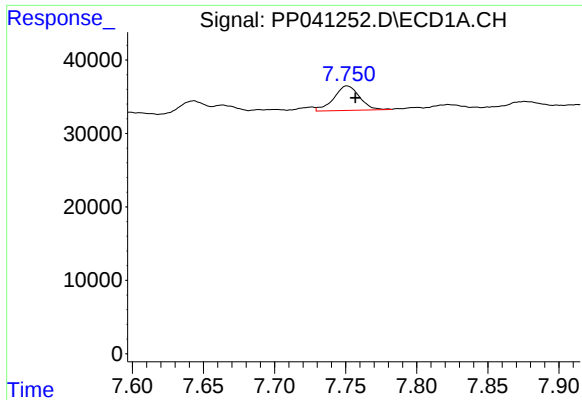


#31 AR-1260-1

R.T.: 7.751 min
Delta R.T.: -0.006 min
Response: 42323
Conc: 42.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-20001


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

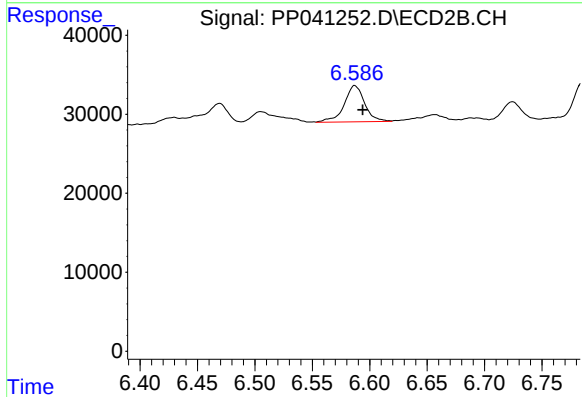


#31 AR-1260-1

R.T.: 6.587 min
Delta R.T.: -0.007 min
Response: 57364
Conc: 59.92 ng/ml

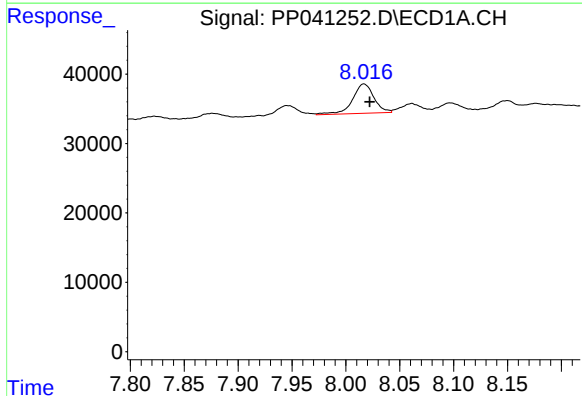


#32 AR-1260-2

R.T.: 8.017 min
Delta R.T.: -0.005 min
Response: 58657
Conc: 49.63 ng/ml

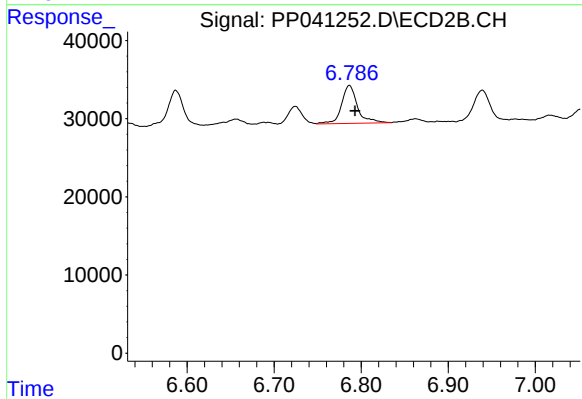

#32 AR-1260-2

R.T.: 6.787 min
Delta R.T.: -0.006 min
Response: 61316
Conc: 56.51 ng/ml

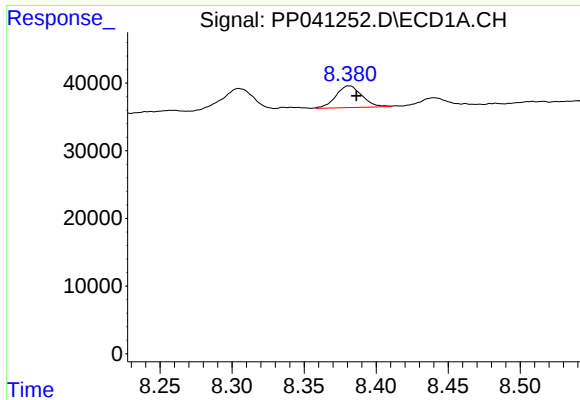


#33 AR-1260-3

R.T.: 8.381 min
Delta R.T.: -0.005 min
Response: 40314
Conc: 44.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-20001


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

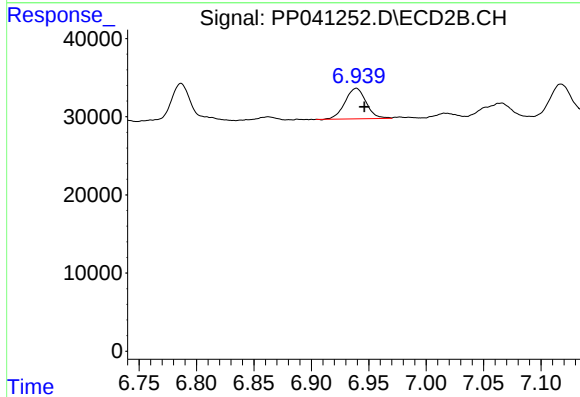


#33 AR-1260-3

R.T.: 6.939 min
Delta R.T.: -0.007 min
Response: 50095
Conc: 49.93 ng/ml

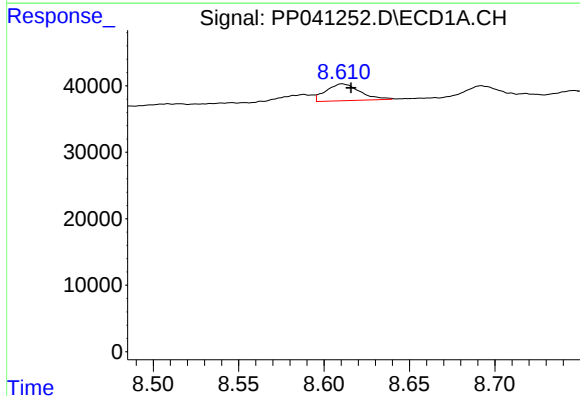


#34 AR-1260-4

R.T.: 8.610 min
Delta R.T.: -0.006 min
Response: 34719
Conc: 32.13 ng/ml m

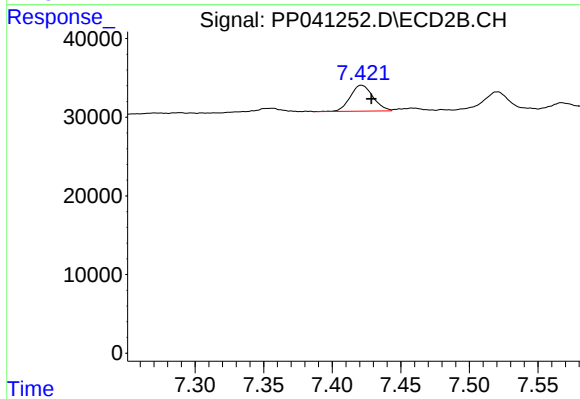

#34 AR-1260-4

R.T.: 7.421 min
Delta R.T.: -0.007 min
Response: 37924
Conc: 46.24 ng/ml

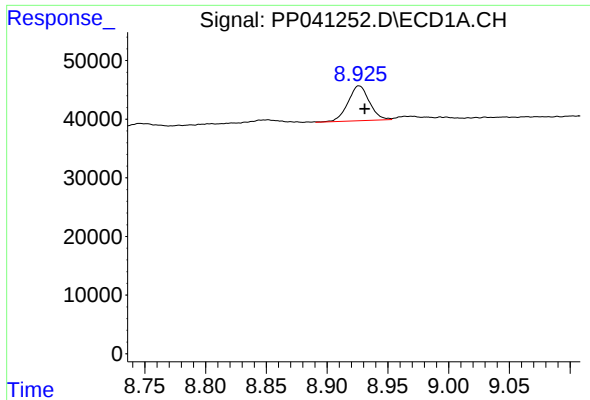


#35 AR-1260-5

R.T.: 8.926 min
Delta R.T.: -0.005 min
Response: 72690
Conc: 34.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-20001

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

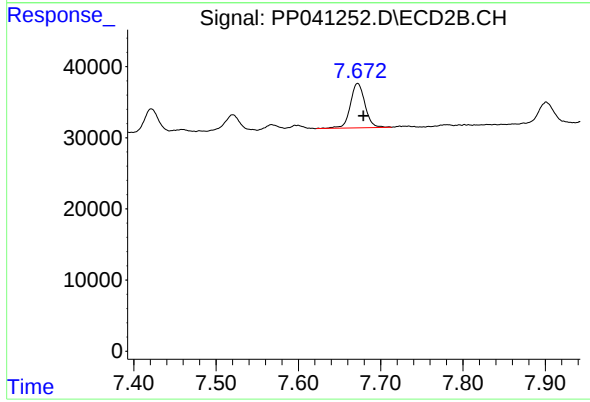

#35 AR-1260-5

R.T.: 7.672 min
Delta R.T.: -0.007 min
Response: 76522
Conc: 43.85 ng/ml