

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112322\
 Data File : PP053472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 18:20
 Operator : YP\AJ
 Sample : N5766-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CR-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/25/2022
 Supervised By :Ankita Jodhani 11/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 20:36:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 09 05:50:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.646	34062741	30630584	17.719	20.363
2) SA Decachlor...	10.199	8.723	28119196	23056995	20.738	12.301m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112322\
Data File : PP053472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 18:20
Operator : YP\AJ
Sample : N5766-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CR-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2022
Supervised By :Ankita Jodhani 11/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 20:36:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 09 05:50:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

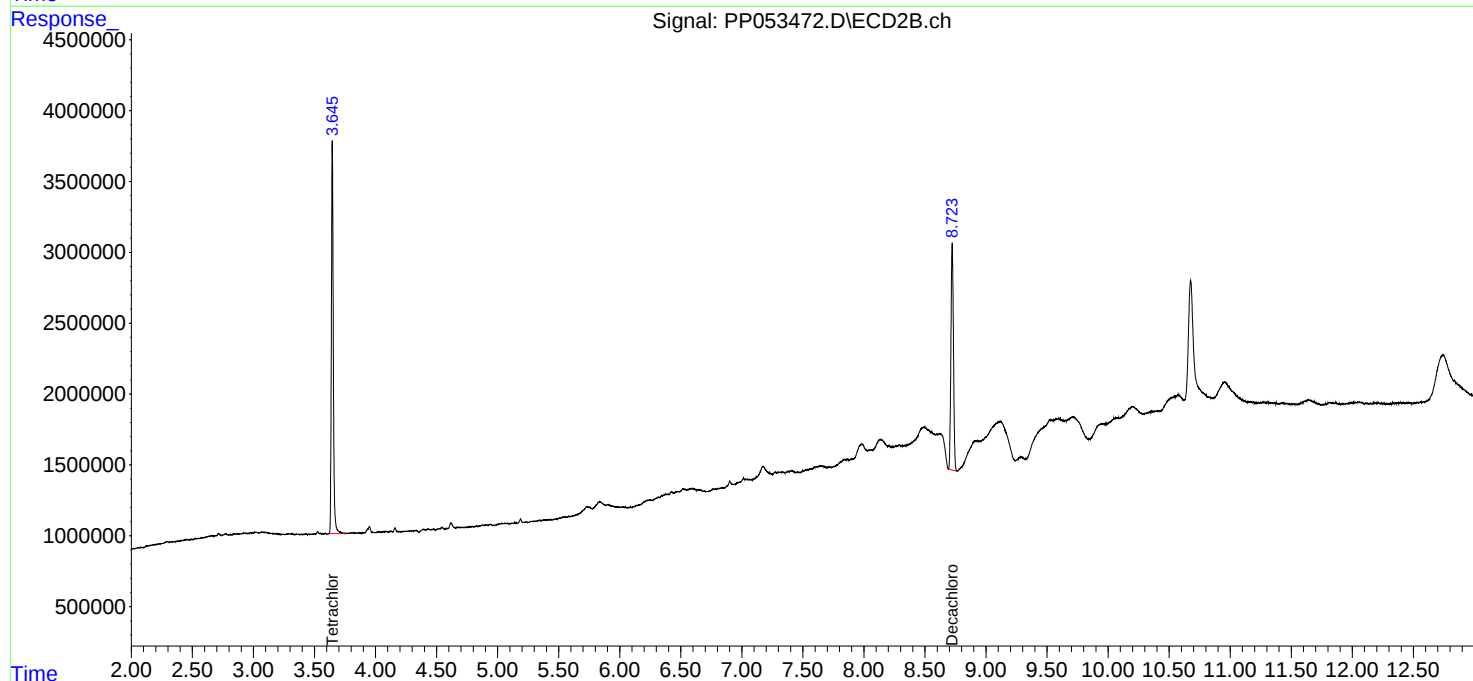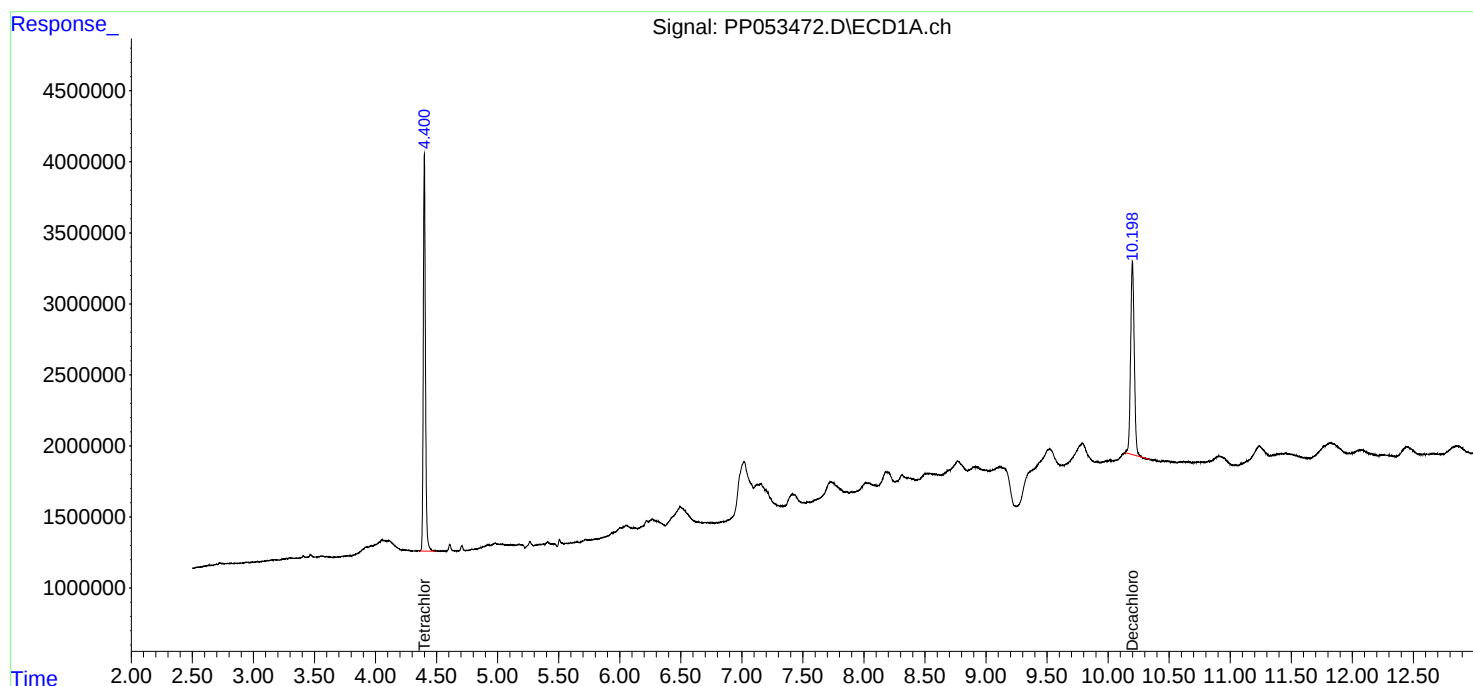

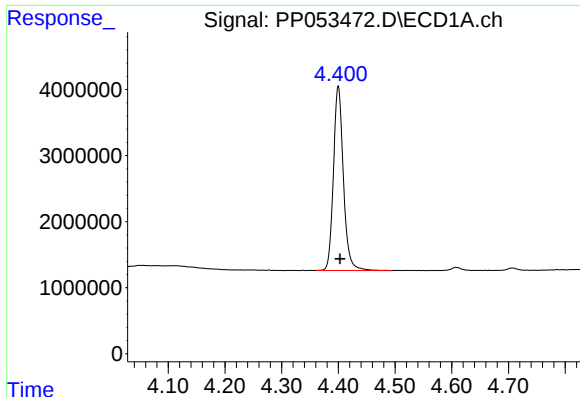


#1 Tetrachloro-m-xylene

R.T.: 4.400 min
Delta R.T.: -0.003 min
Response: 34062741
Conc: 17.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
CR-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2022
Supervised By :Ankita Jodhani 11/25/2022

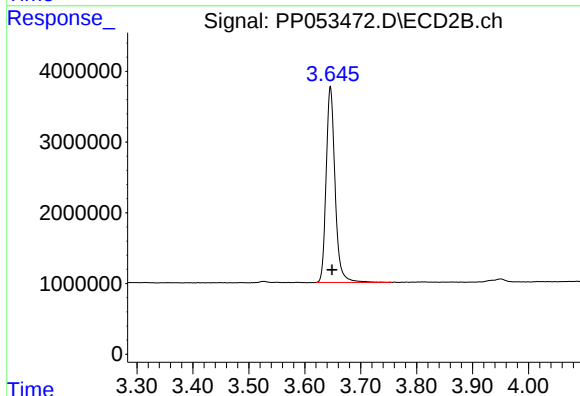


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.003 min
Response: 30630584
Conc: 20.36 ng/ml

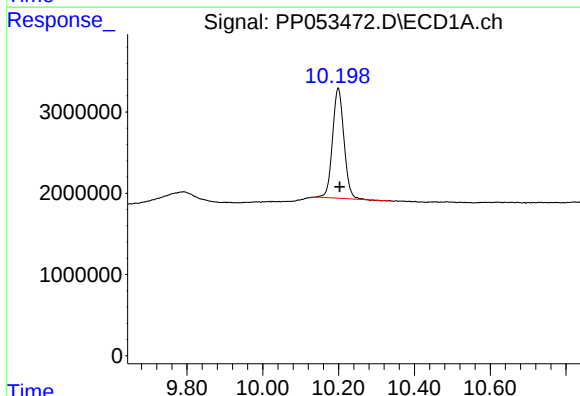

#2 Decachlorobiphenyl

R.T.: 10.199 min
Delta R.T.: -0.004 min
Response: 28119196
Conc: 20.74 ng/ml

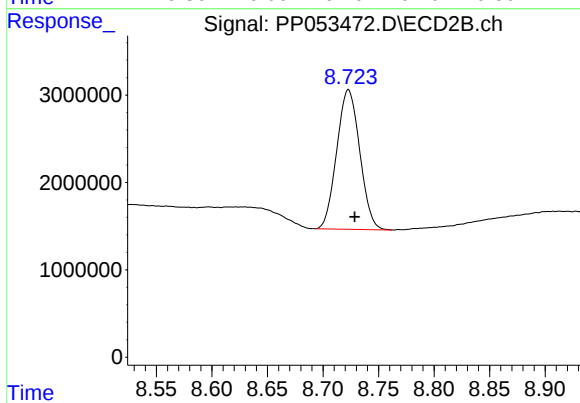

#2 Decachlorobiphenyl

R.T.: 8.723 min
Delta R.T.: -0.006 min
Response: 23056995
Conc: 12.30 ng/ml m