

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
 Data File : PP041336.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2021 00:51
 Operator : AJ\MA
 Sample : M4823-07 20X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 02:36:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.754	3.756	8950	14470	0.424	0.521
2)	SA Decachlor...	0.000	9.015	0	12073	N.D.	0.842 #
Target Compounds							
9)	L2 AR-1221-2	5.119	4.139f	28562	16053	184.508	63.310 #
28)	L6 AR-1254-3	7.604	6.458	55936	52475	41.773	36.278
31)	L7 AR-1260-1	0.000	6.611f	0	9987	N.D.	10.432 #
33)	L7 AR-1260-3	0.000	6.925f	0	12831	N.D.	12.788 #
35)	L7 AR-1260-5	0.000	7.682	0	16129	N.D.	9.242 #
37)	L8 AR-1262-2	0.000	7.682	0	16129	N.D.	9.744 #
39)	L8 AR-1262-4	0.000	8.010f	0	23064	N.D.	17.937 #
42)	L9 AR-1268-2	0.000	8.010f	0	23064	N.D.	12.104 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
Data File : PP041336.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2021 00:51
Operator : AJ\MA
Sample : M4823-07 20X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 02:36:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

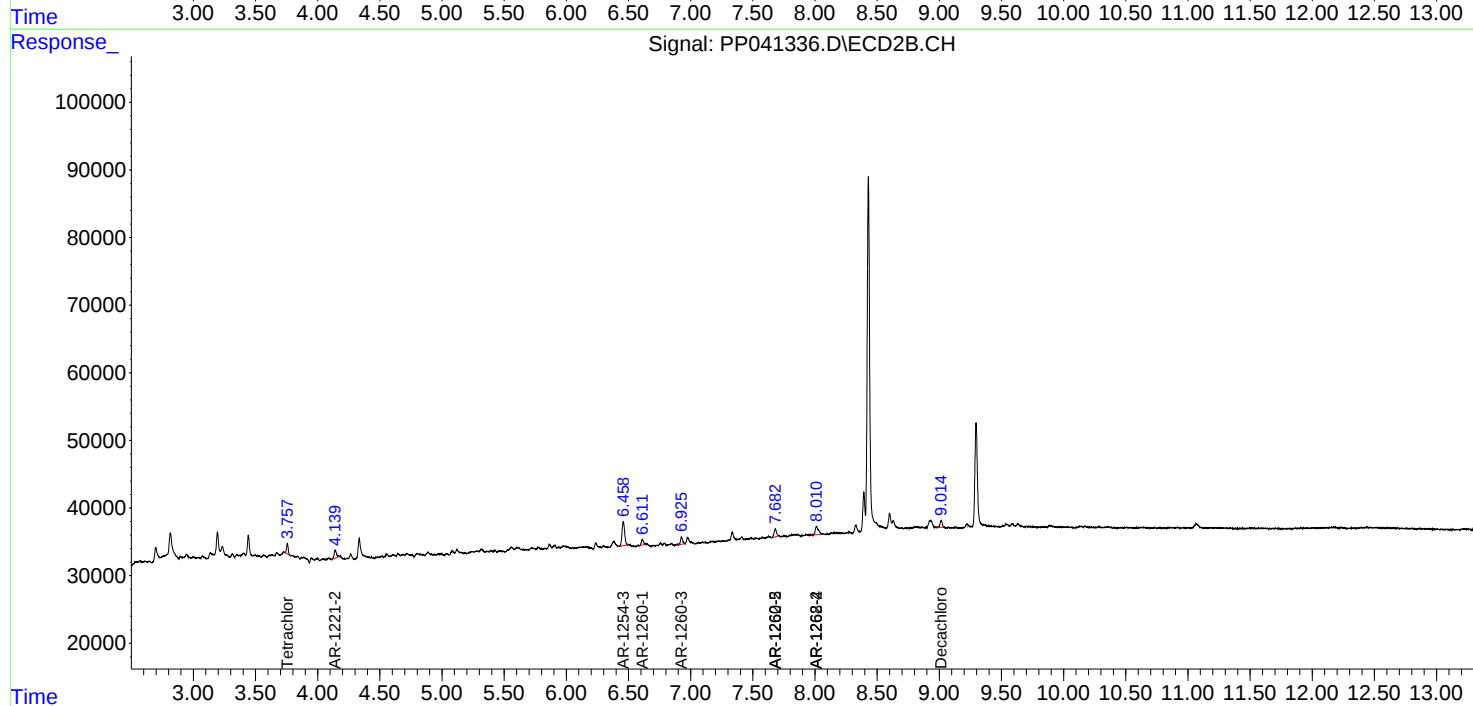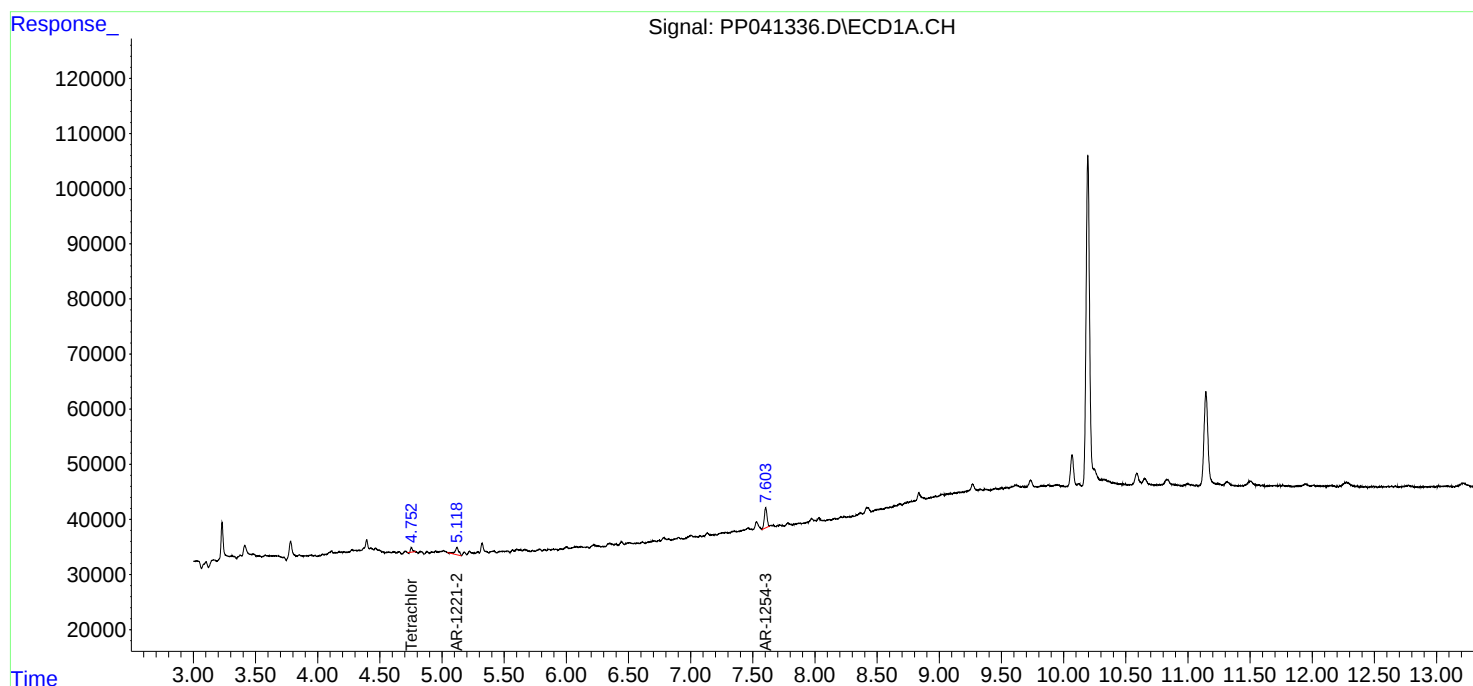


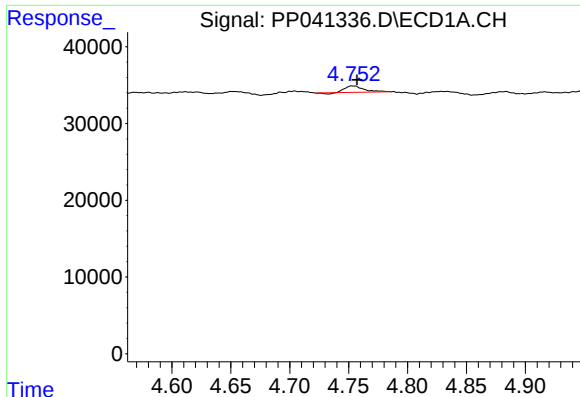

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 8950
Conc: 0.42 ng/ml

Instrument :
ECD_P
ClientSampleId :

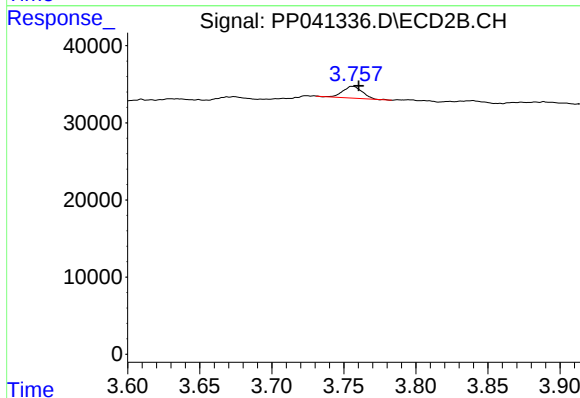


#1 Tetrachloro-m-xylene

R.T.: 3.756 min
Delta R.T.: -0.004 min
Response: 14470
Conc: 0.52 ng/ml

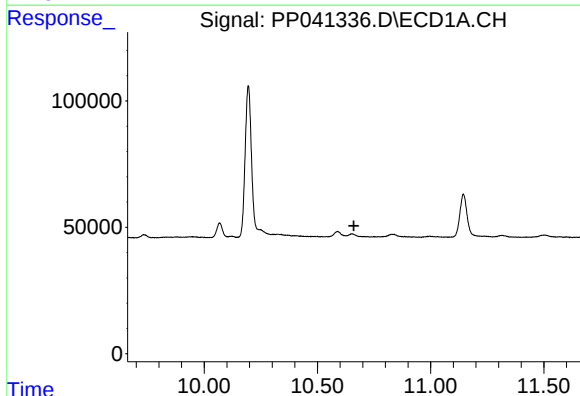


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.661 min
Response: 0
Conc: N.D.

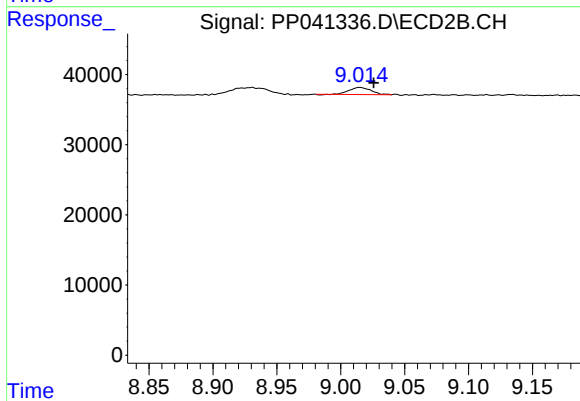

#2 Decachlorobiphenyl


R.T.: 9.015 min
Delta R.T.: -0.011 min
Response: 12073
Conc: 0.84 ng/ml

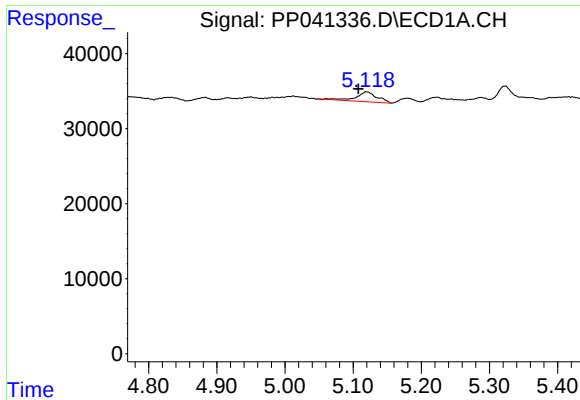

#9 AR-1221-2


R.T.: 5.119 min
Delta R.T.: 0.012 min
Response: 28562
Conc: 184.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

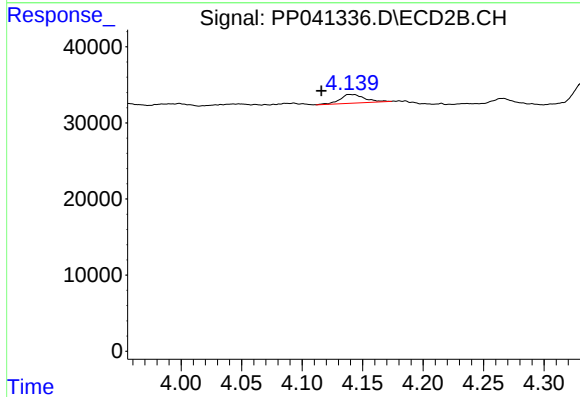


#9 AR-1221-2

R.T.: 4.139 min
Delta R.T.: 0.023 min
Response: 16053
Conc: 63.31 ng/ml

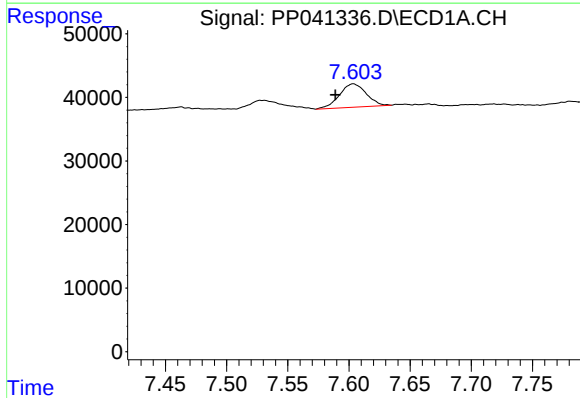


#28 AR-1254-3

R.T.: 7.604 min
Delta R.T.: 0.015 min
Response: 55936
Conc: 41.77 ng/ml

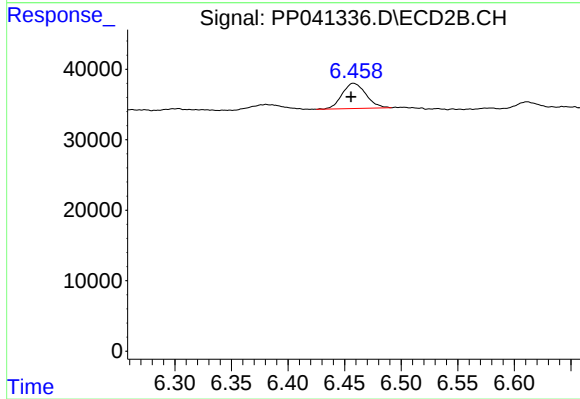

#28 AR-1254-3


R.T.: 6.458 min
Delta R.T.: 0.002 min
Response: 52475
Conc: 36.28 ng/ml

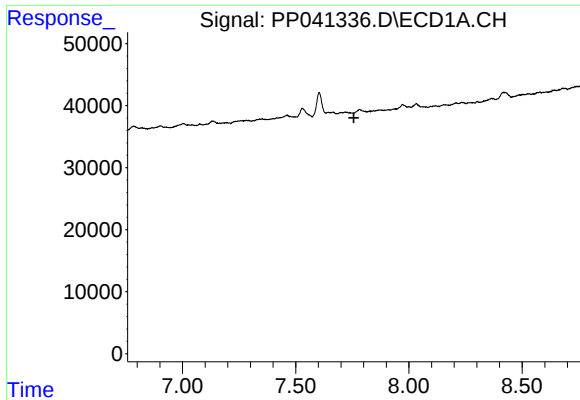

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

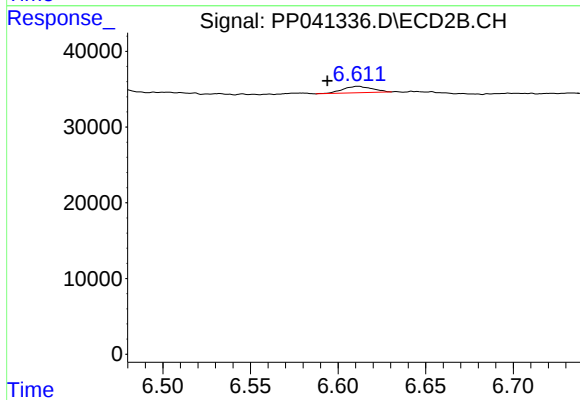


#31 AR-1260-1

R.T.: 6.611 min
Delta R.T.: 0.017 min
Response: 9987
Conc: 10.43 ng/ml

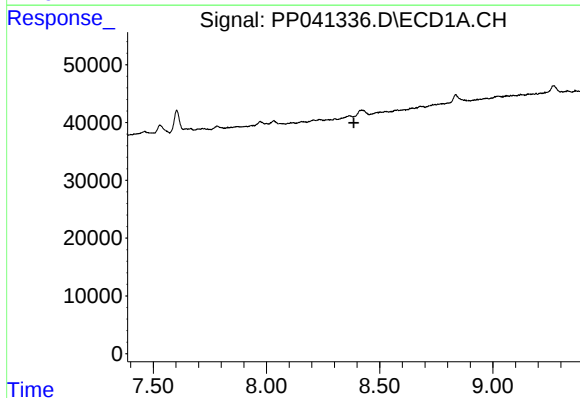


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.386 min
Response: 0
Conc: N.D.

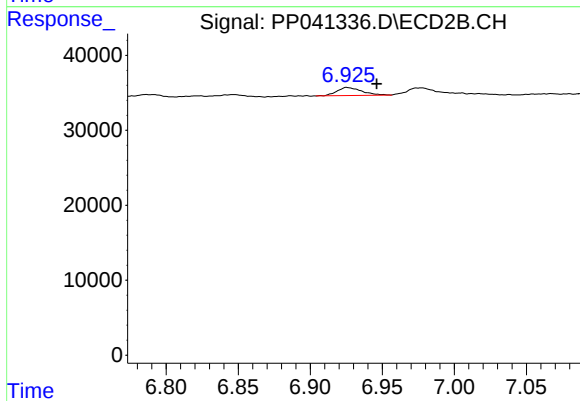

#33 AR-1260-3


R.T.: 6.925 min
Delta R.T.: -0.021 min
Response: 12831
Conc: 12.79 ng/ml

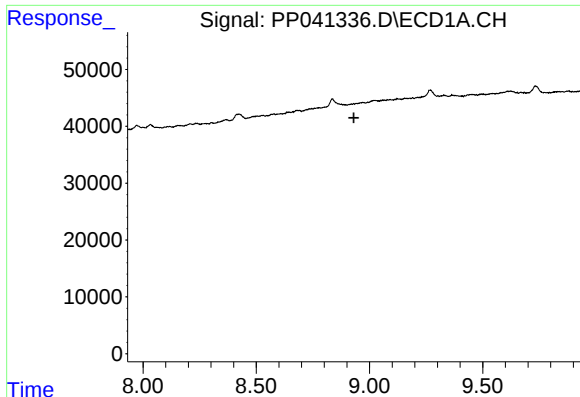

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

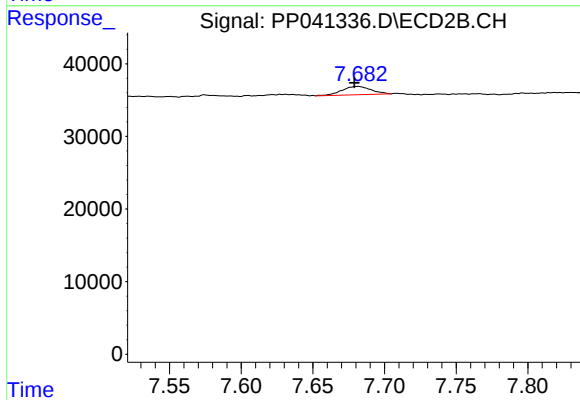


#35 AR-1260-5

R.T.: 7.682 min
Delta R.T.: 0.003 min
Response: 16129
Conc: 9.24 ng/ml

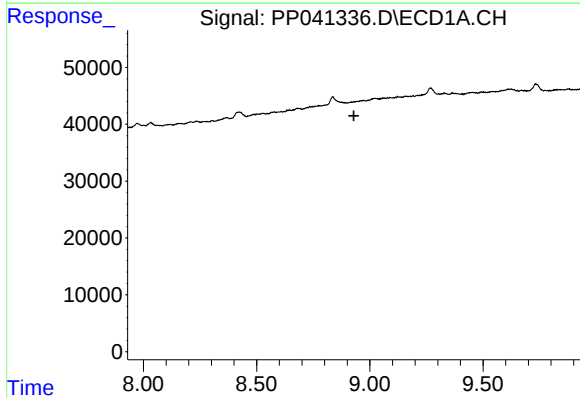


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.930 min
Response: 0
Conc: N.D.

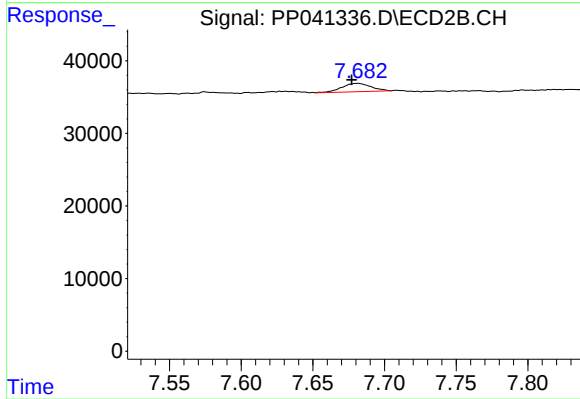

#37 AR-1262-2


R.T.: 7.682 min
Delta R.T.: 0.004 min
Response: 16129
Conc: 9.74 ng/ml

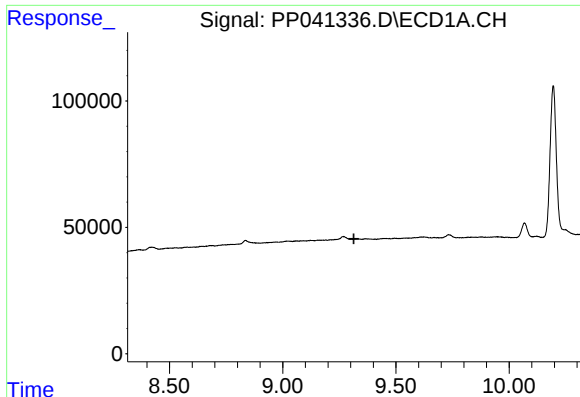

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.315 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

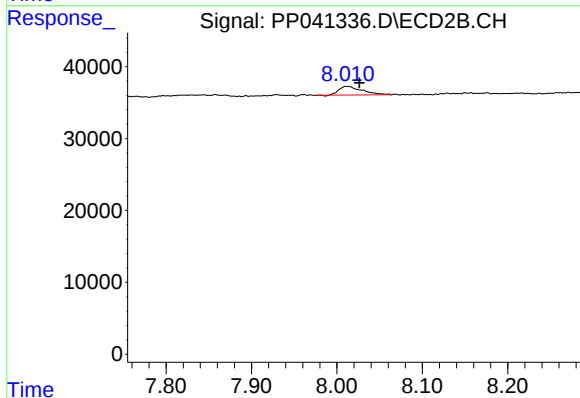


#39 AR-1262-4

R.T.: 8.010 min
Delta R.T.: -0.016 min
Response: 23064
Conc: 17.94 ng/ml

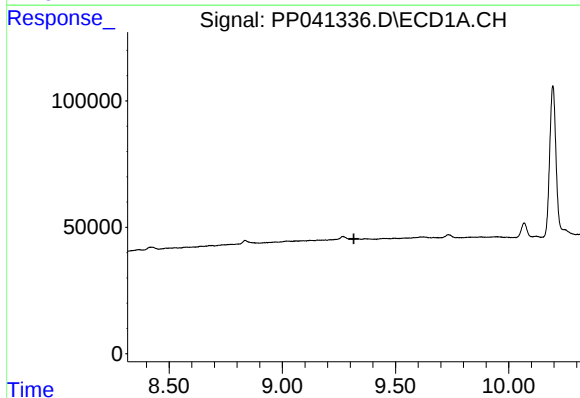

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.316 min
Response: 0
Conc: N.D.

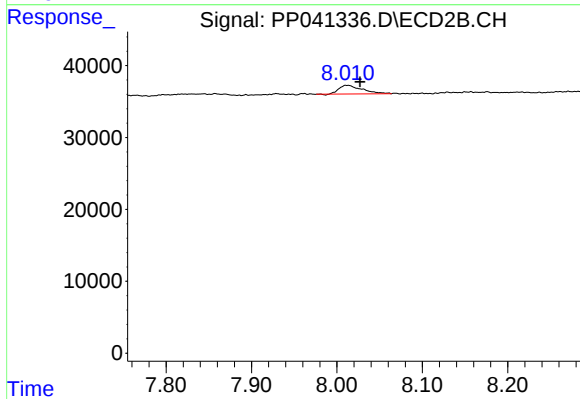

#42 AR-1268-2

R.T.: 8.010 min
Delta R.T.: -0.017 min
Response: 23064
Conc: 12.10 ng/ml