

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
 Data File : PP041338.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2021 1:25
 Operator : AJ\MA
 Sample : M4823-09 20X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 02:37:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.754	3.755	11181	18503	0.530	0.666 #
2)	SA Decachlor...	10.650	9.015	-1183	14181	N.D.	0.989
Target Compounds							
28)	L6 AR-1254-3	7.604	6.457	37184	40063	27.769	27.697
31)	L7 AR-1260-1	0.000	6.610f	0	11904	N.D.	12.435 #
32)	L7 AR-1260-2	8.031	0.000	7003	0	5.926	N.D. #
33)	L7 AR-1260-3	8.416f	6.975f	16235	12668	17.884	12.625 #
35)	L7 AR-1260-5	0.000	7.680	0	18205	N.D.	10.431 #
37)	L8 AR-1262-2	0.000	7.680	0	18205	N.D.	10.999 #
39)	L8 AR-1262-4	0.000	8.012	0	23852	N.D.	18.549 #
42)	L9 AR-1268-2	0.000	8.012	0	23852	N.D.	12.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
Data File : PP041338.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2021 1:25
Operator : AJ\MA
Sample : M4823-09 20X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 02:37:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

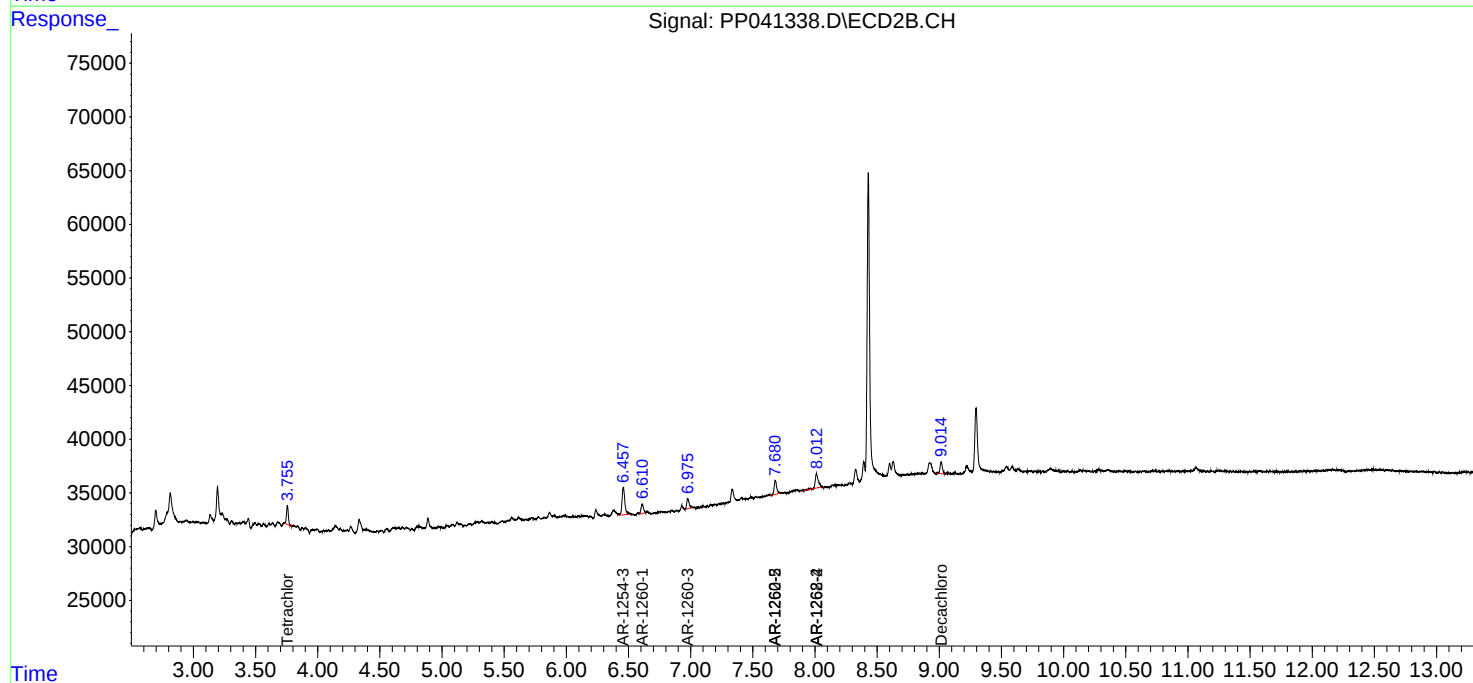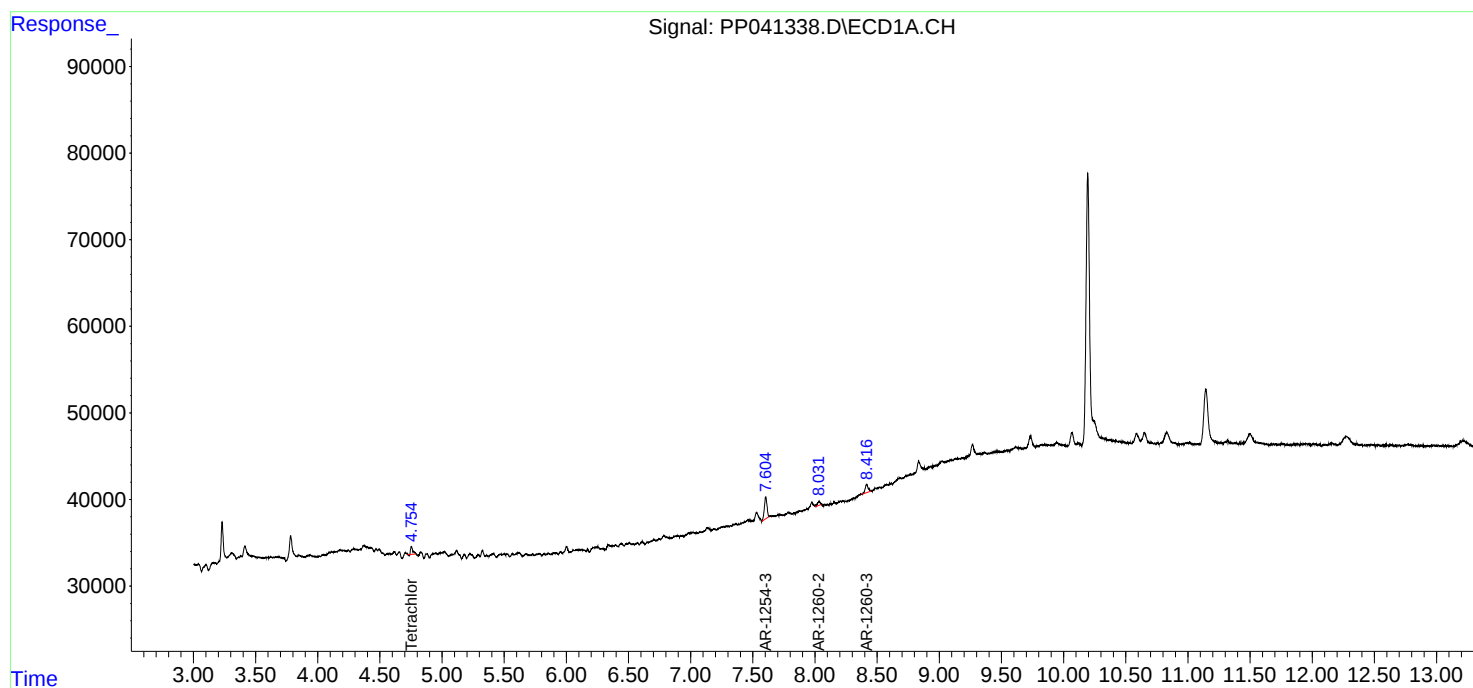


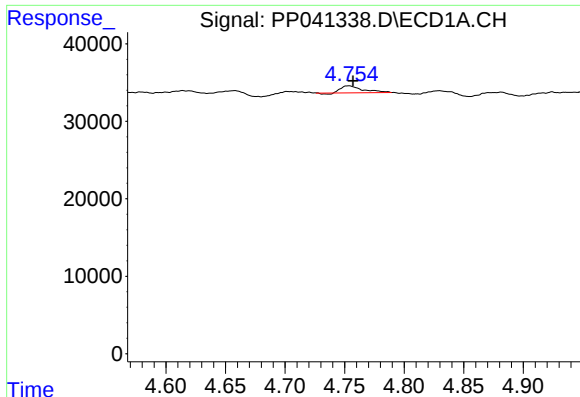

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 11181
Conc: 0.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

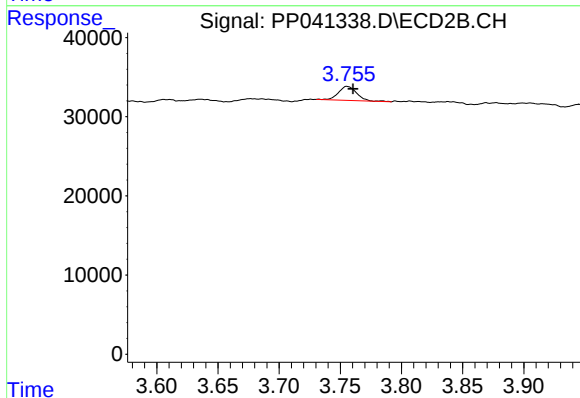


#1 Tetrachloro-m-xylene

R.T.: 3.755 min
Delta R.T.: -0.005 min
Response: 18503
Conc: 0.67 ng/ml

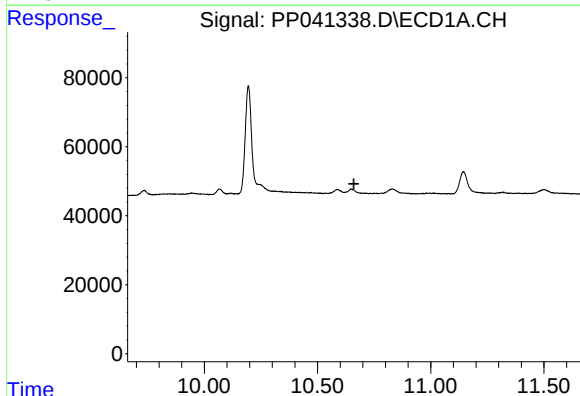


#2 Decachlorobiphenyl

R.T.: 10.650 min
Delta R.T.: -0.011 min
Response: -1183
Conc: N.D.

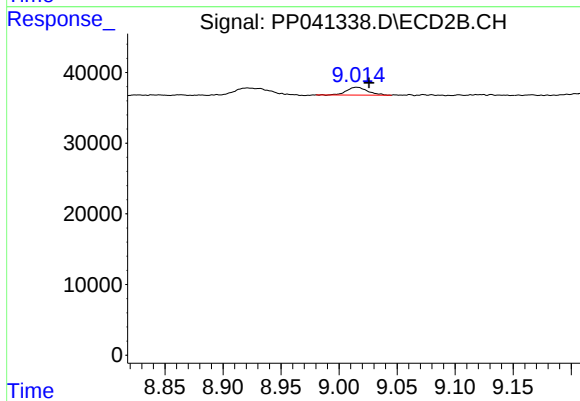

#2 Decachlorobiphenyl


R.T.: 9.015 min
Delta R.T.: -0.011 min
Response: 14181
Conc: 0.99 ng/ml

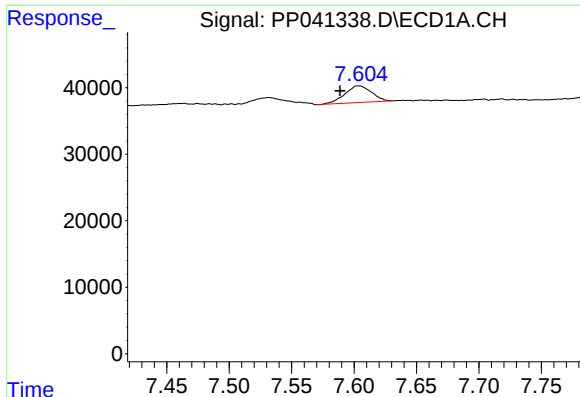

#28 AR-1254-3


R.T.: 7.604 min
Delta R.T.: 0.015 min
Response: 37184
Conc: 27.77 ng/ml

Instrument :
ECD_P
ClientSampleId :

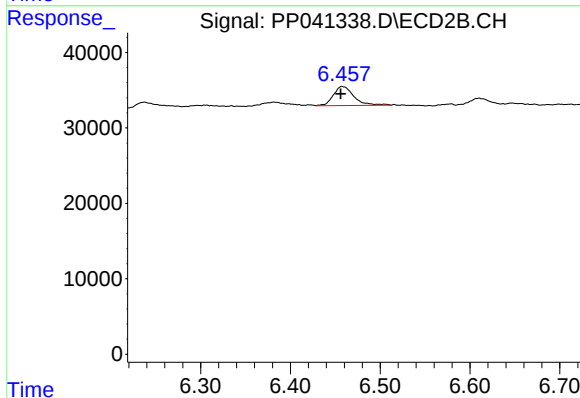


#28 AR-1254-3

R.T.: 6.457 min
Delta R.T.: 0.002 min
Response: 40063
Conc: 27.70 ng/ml

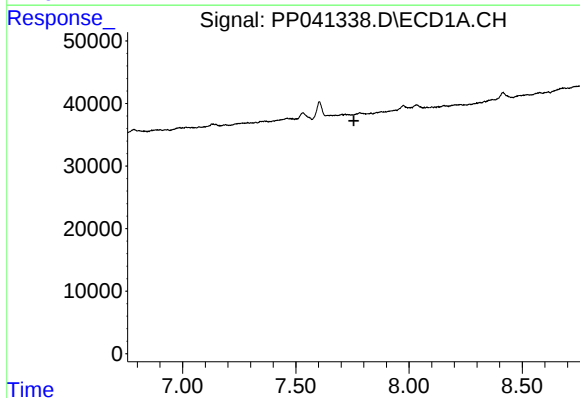


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.757 min
Response: 0
Conc: N.D.

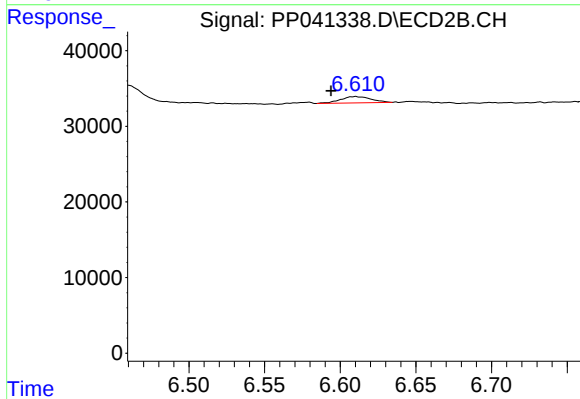

#31 AR-1260-1


R.T.: 6.610 min
Delta R.T.: 0.016 min
Response: 11904
Conc: 12.43 ng/ml

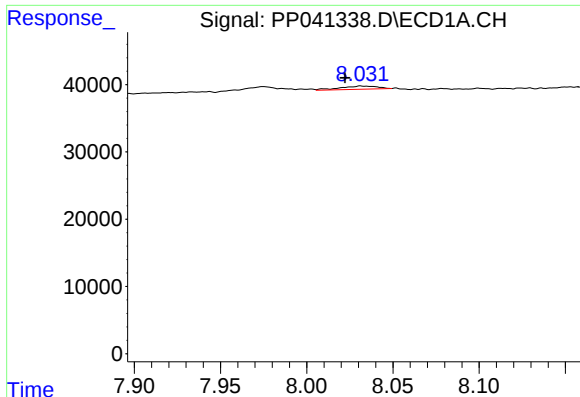

#32 AR-1260-2


R.T.: 8.031 min
Delta R.T.: 0.009 min
Response: 7003
Conc: 5.93 ng/ml

Instrument :
ECD_P
ClientSampleId :

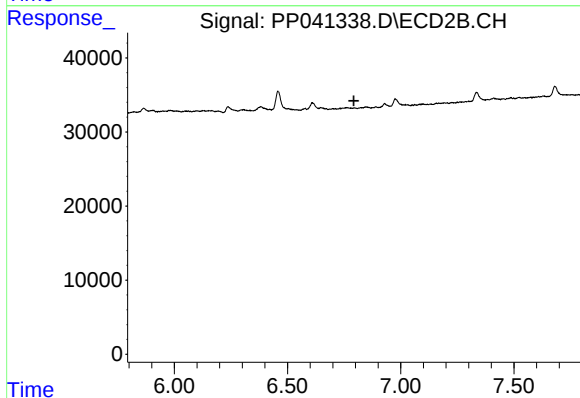


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.793 min
Response: 0
Conc: N.D.

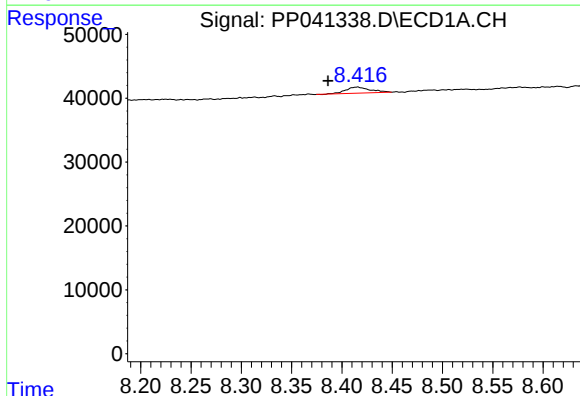


#33 AR-1260-3

R.T.: 8.416 min
Delta R.T.: 0.030 min
Response: 16235
Conc: 17.88 ng/ml

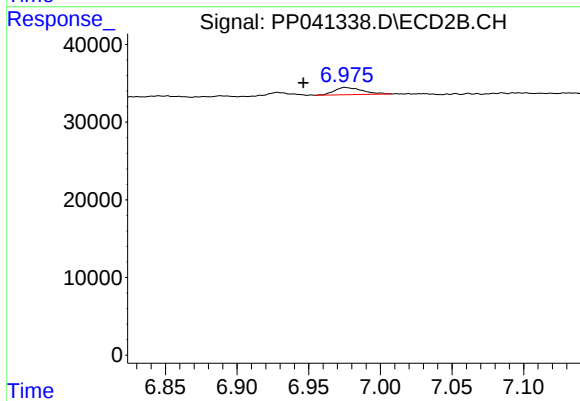

#33 AR-1260-3


R.T.: 6.975 min
Delta R.T.: 0.029 min
Response: 12668
Conc: 12.63 ng/ml

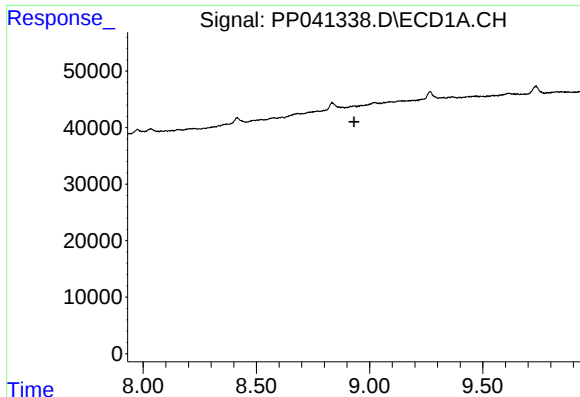

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

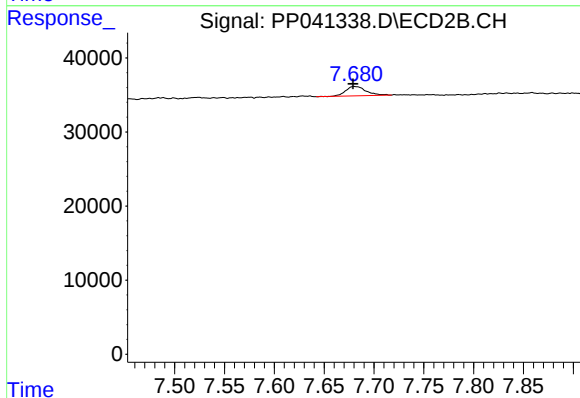


#35 AR-1260-5

R.T.: 7.680 min
Delta R.T.: 0.001 min
Response: 18205
Conc: 10.43 ng/ml

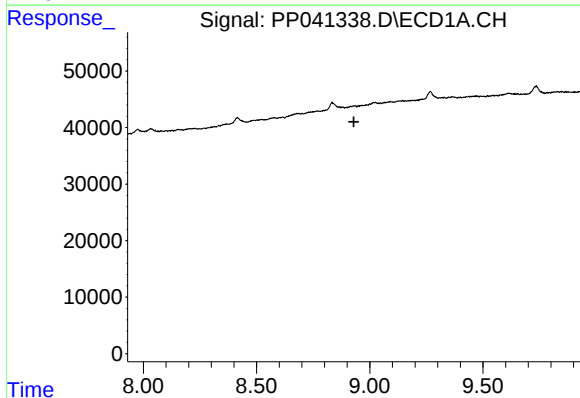


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.930 min
Response: 0
Conc: N.D.

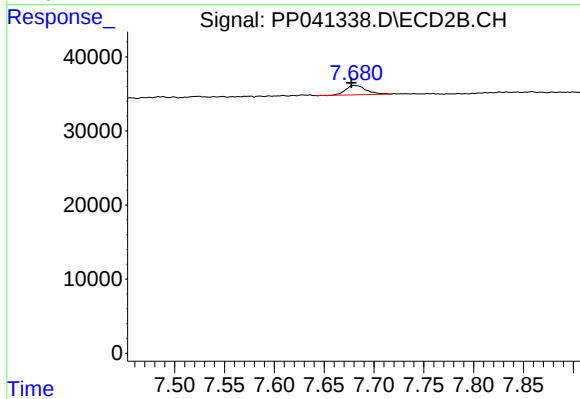

#37 AR-1262-2


R.T.: 7.680 min
Delta R.T.: 0.003 min
Response: 18205
Conc: 11.00 ng/ml

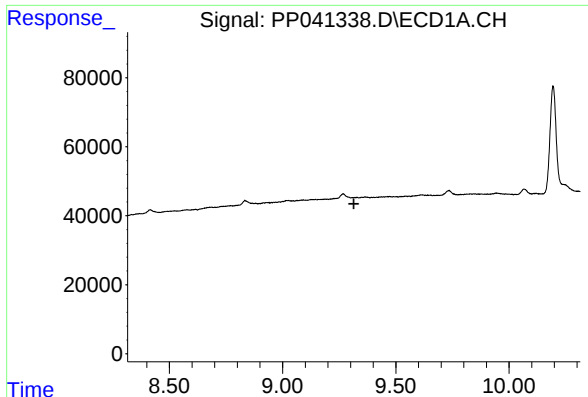

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.315 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

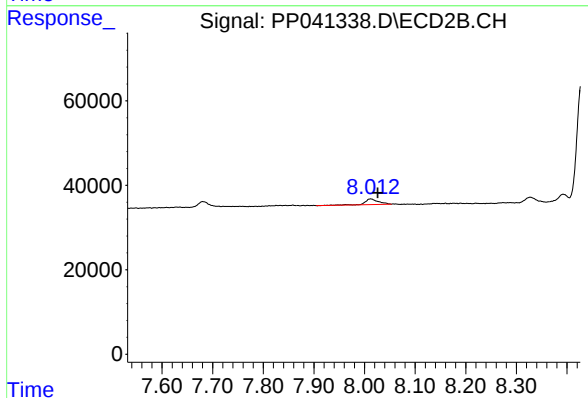


#39 AR-1262-4

R.T.: 8.012 min
Delta R.T.: -0.014 min
Response: 23852
Conc: 18.55 ng/ml

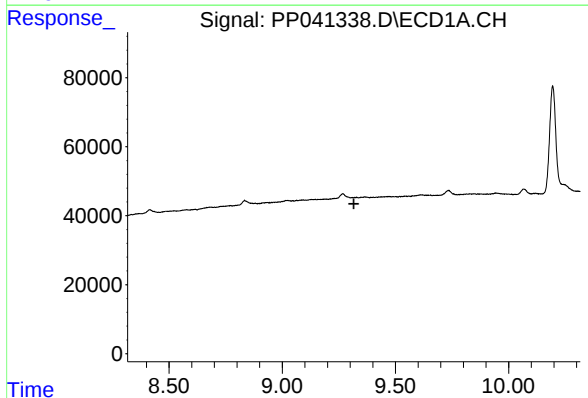

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.316 min
Response: 0
Conc: N.D.

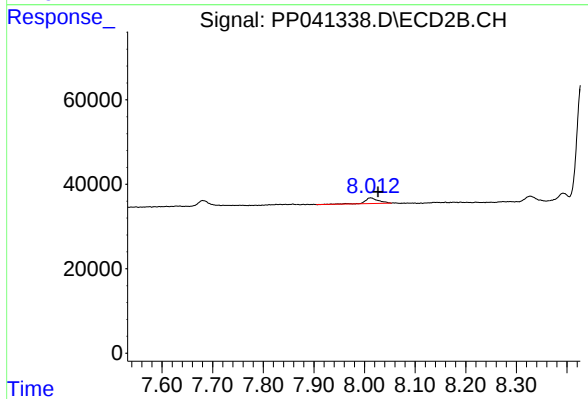

#42 AR-1268-2

R.T.: 8.012 min
Delta R.T.: -0.015 min
Response: 23852
Conc: 12.52 ng/ml