

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
 Data File : PP041317.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2021 18:54
 Operator : AJ\MA
 Sample : M4804-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 40444

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
 Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 02:31:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.753	3.757	444812	462667	21.092	16.648
2) SA Decachlor...	10.649	9.014	301555	199069	13.805m	13.887

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
Data File : PP041317.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2021 18:54
Operator : AJ\MA
Sample : M4804-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
40444


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 02:31:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

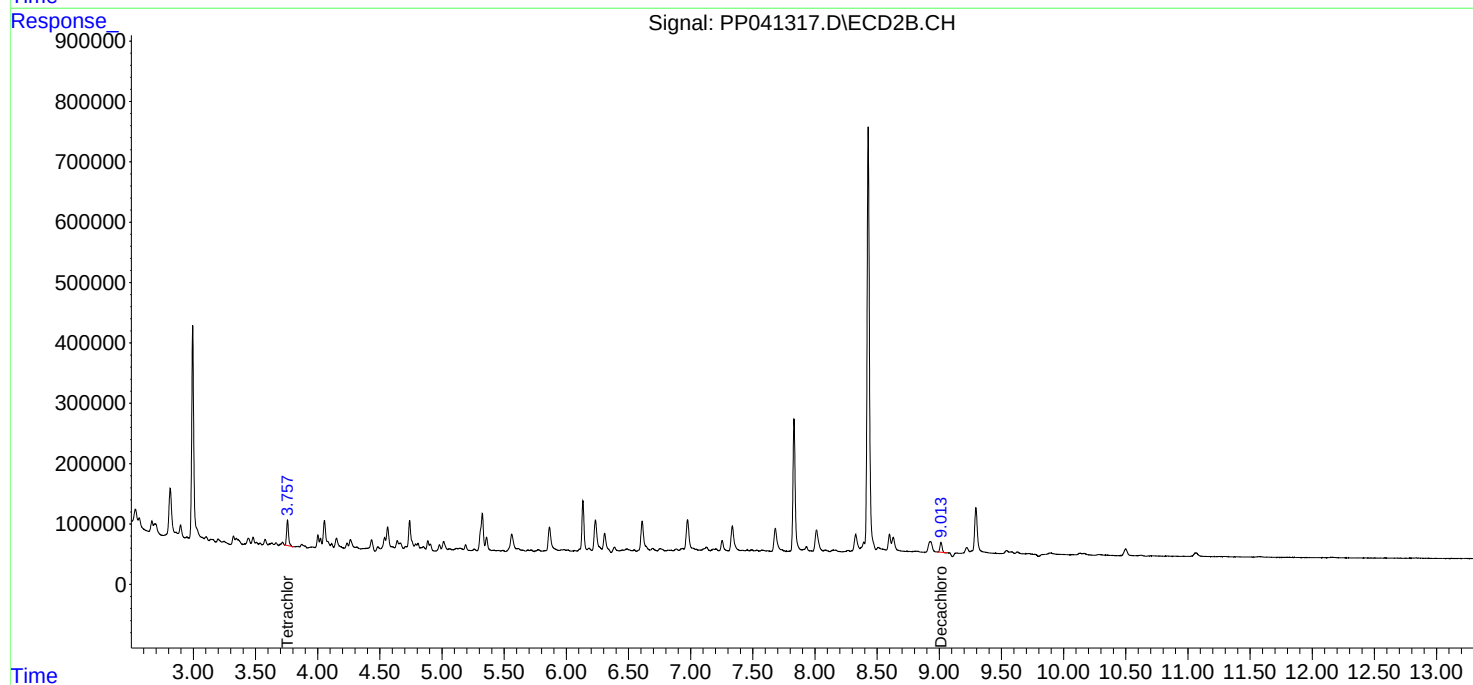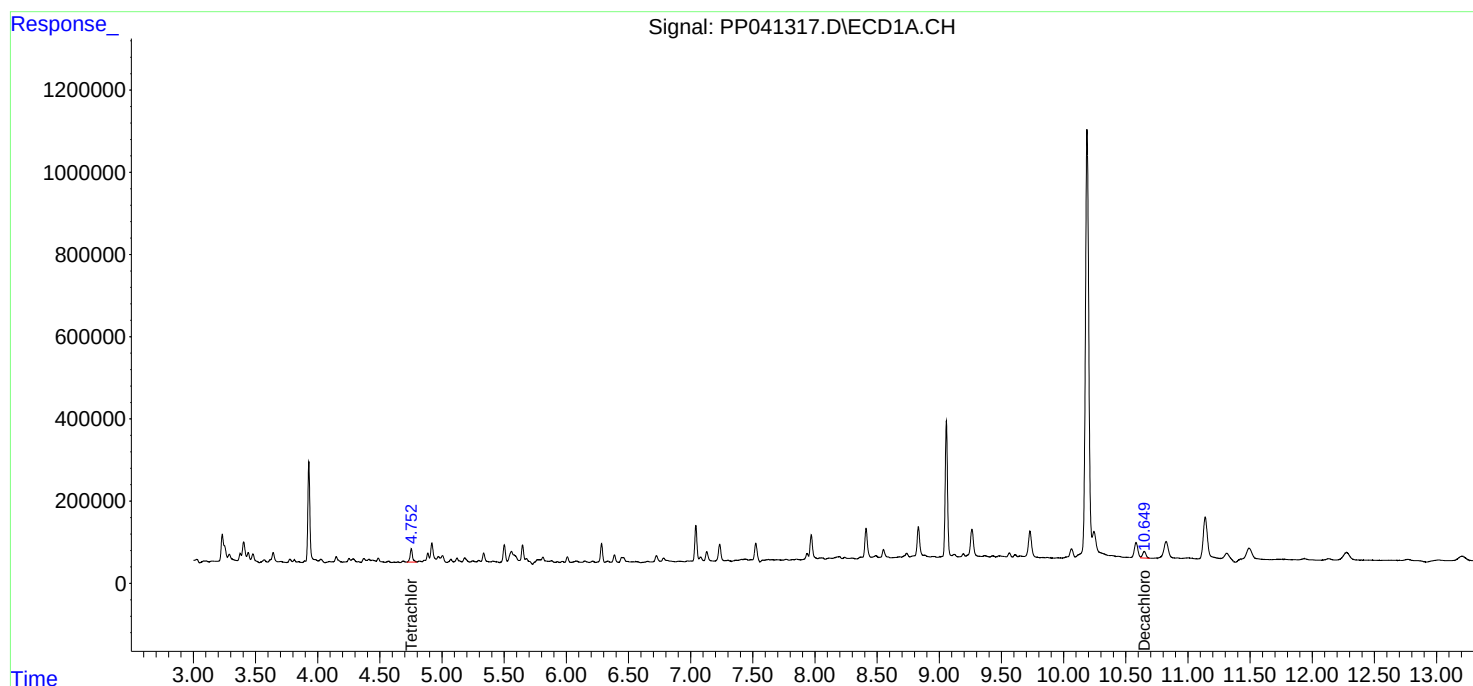

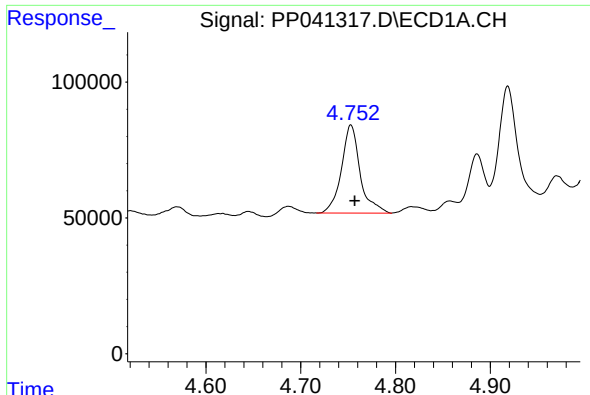


#1 Tetrachloro-m-xylene

R.T.: 4.753 min
Delta R.T.: -0.004 min
Response: 444812
Conc: 21.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
40444


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

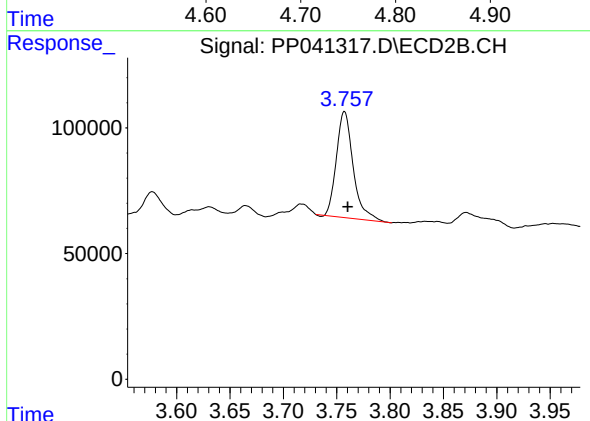


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 462667
Conc: 16.65 ng/ml

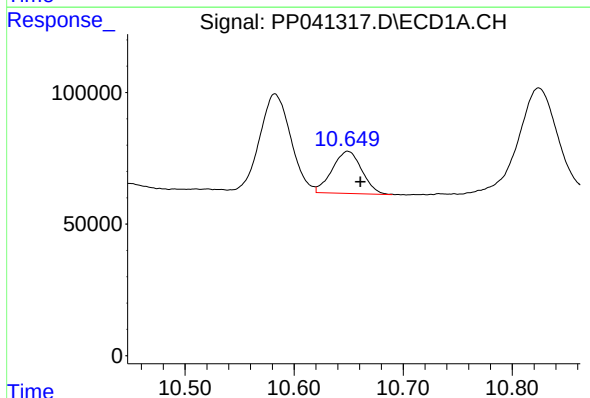

#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.012 min
Response: 301555
Conc: 13.80 ng/ml m

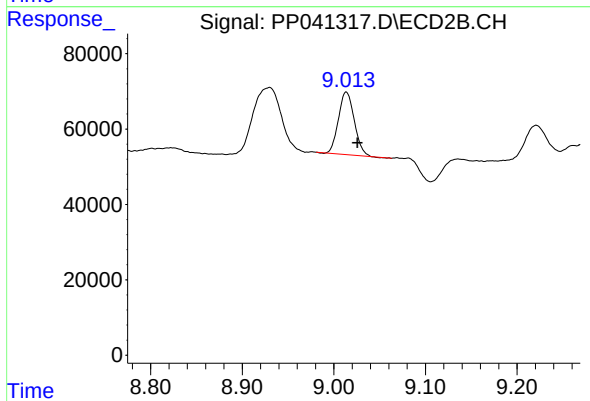

#2 Decachlorobiphenyl

R.T.: 9.014 min
Delta R.T.: -0.012 min
Response: 199069
Conc: 13.89 ng/ml