

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
 Data File : PP041321.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2021 20:01
 Operator : AJ\MA
 Sample : M4817-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 A6879

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 02:33:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.753	3.756	344014	547397	16.313	19.697
2) SA Decachlor...	10.649	9.013	306086	202153	14.012	14.102

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
Data File : PP041321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2021 20:01
Operator : AJ\MA
Sample : M4817-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
A6879

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 02:33:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

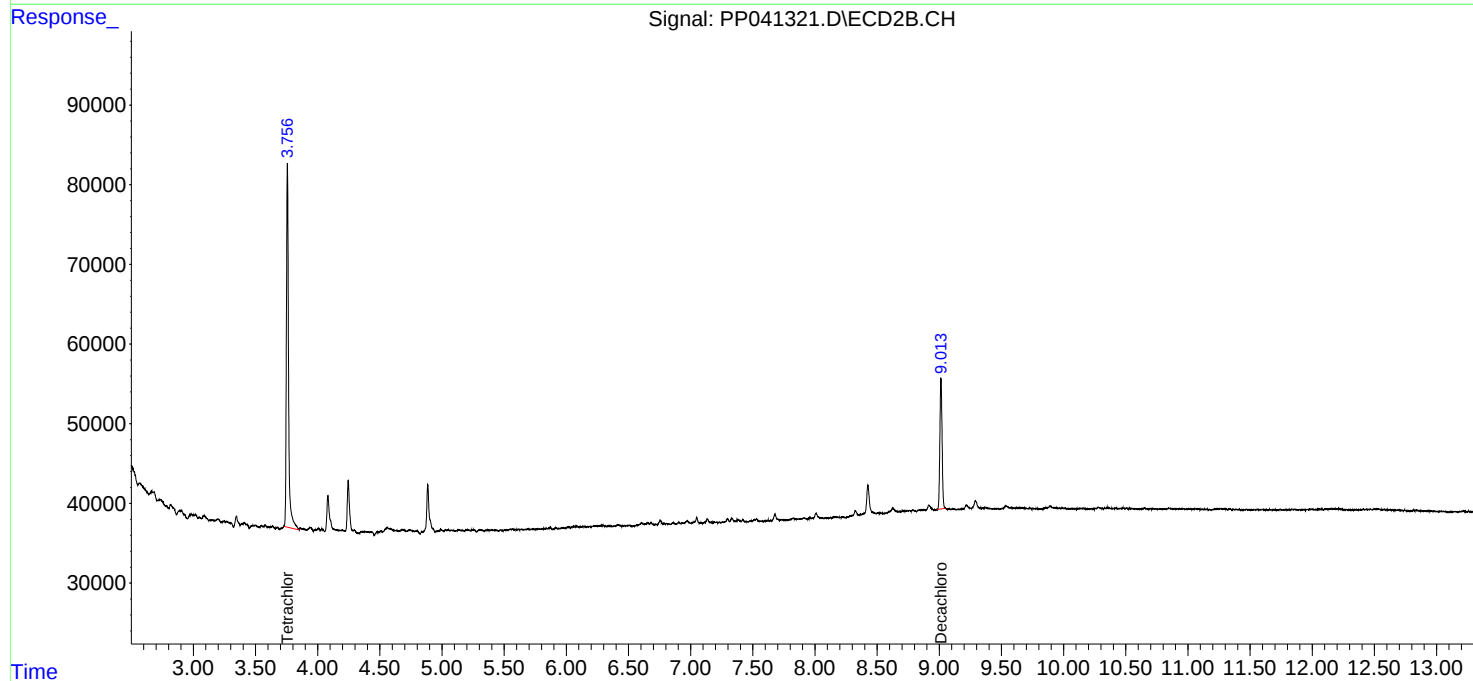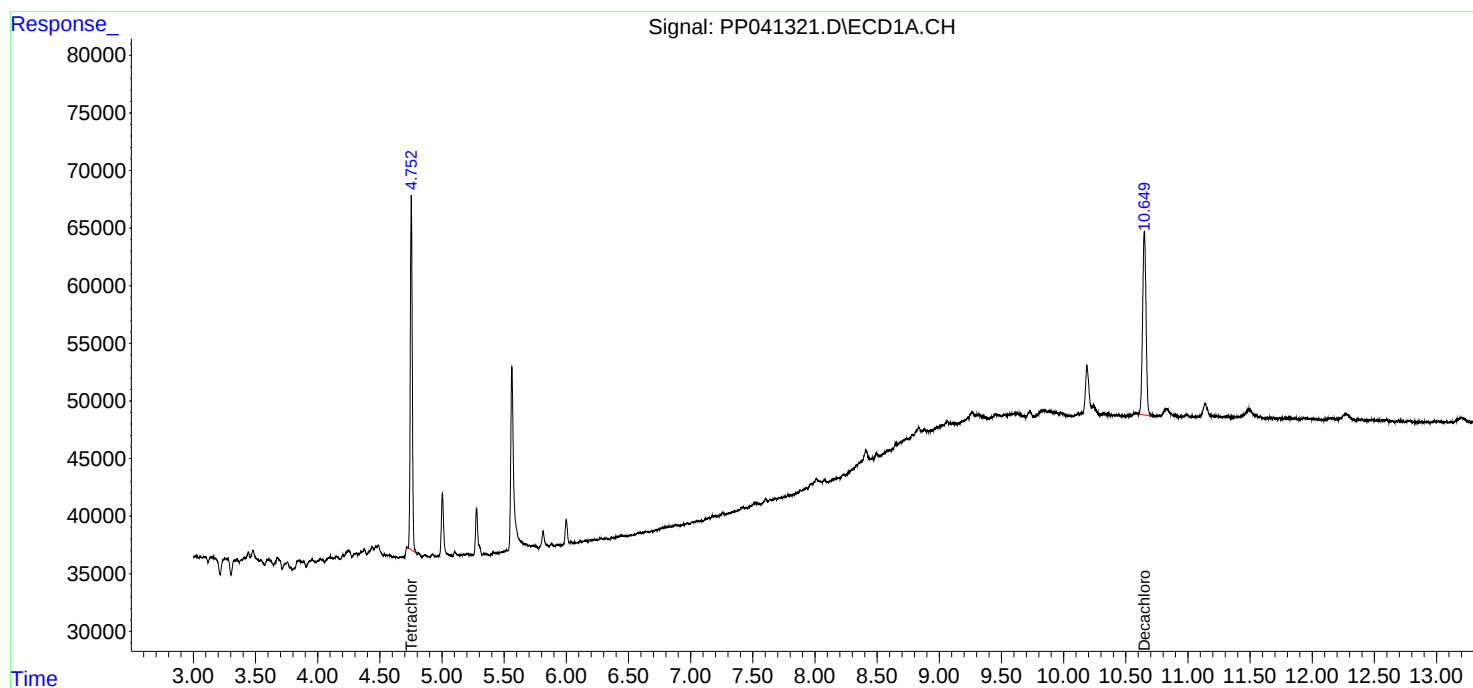


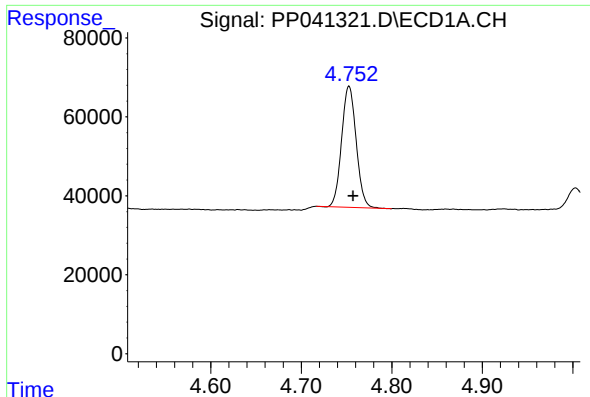

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.004 min
Response: 344014
Conc: 16.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
A6879

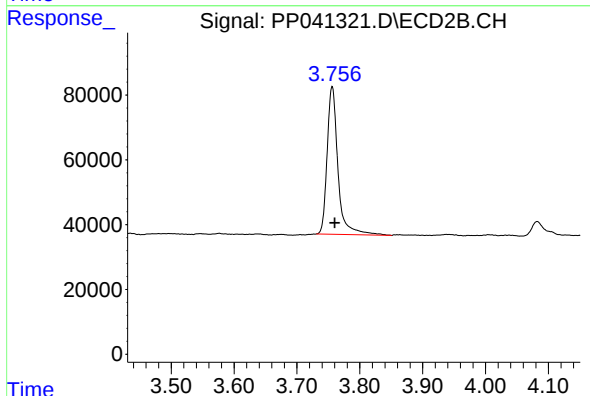


#1 Tetrachloro-m-xylene

R.T.: 3.756 min
Delta R.T.: -0.004 min
Response: 547397
Conc: 19.70 ng/ml

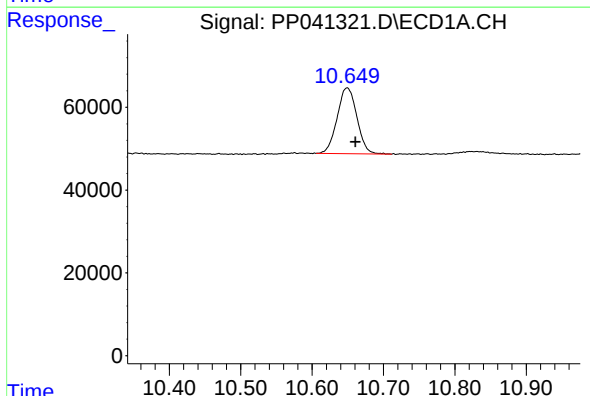

#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.011 min
Response: 306086
Conc: 14.01 ng/ml

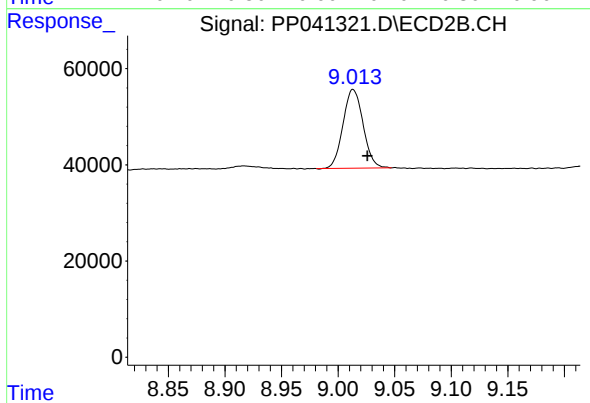

#2 Decachlorobiphenyl

R.T.: 9.013 min
Delta R.T.: -0.013 min
Response: 202153
Conc: 14.10 ng/ml