

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
 Data File : PP041333.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2021 00:01
 Operator : AJ\MA
 Sample : M4823-04 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2021-48B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
 Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 02:36:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.753	3.756	27652	47693	1.311	1.716 #
2) SA Decachlor...	10.651	9.014	34888	30090	1.597	2.099m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112421\
Data File : PP041333.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2021 00:01
Operator : AJ\MA
Sample : M4823-04 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SEC-2021-48B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 02:36:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

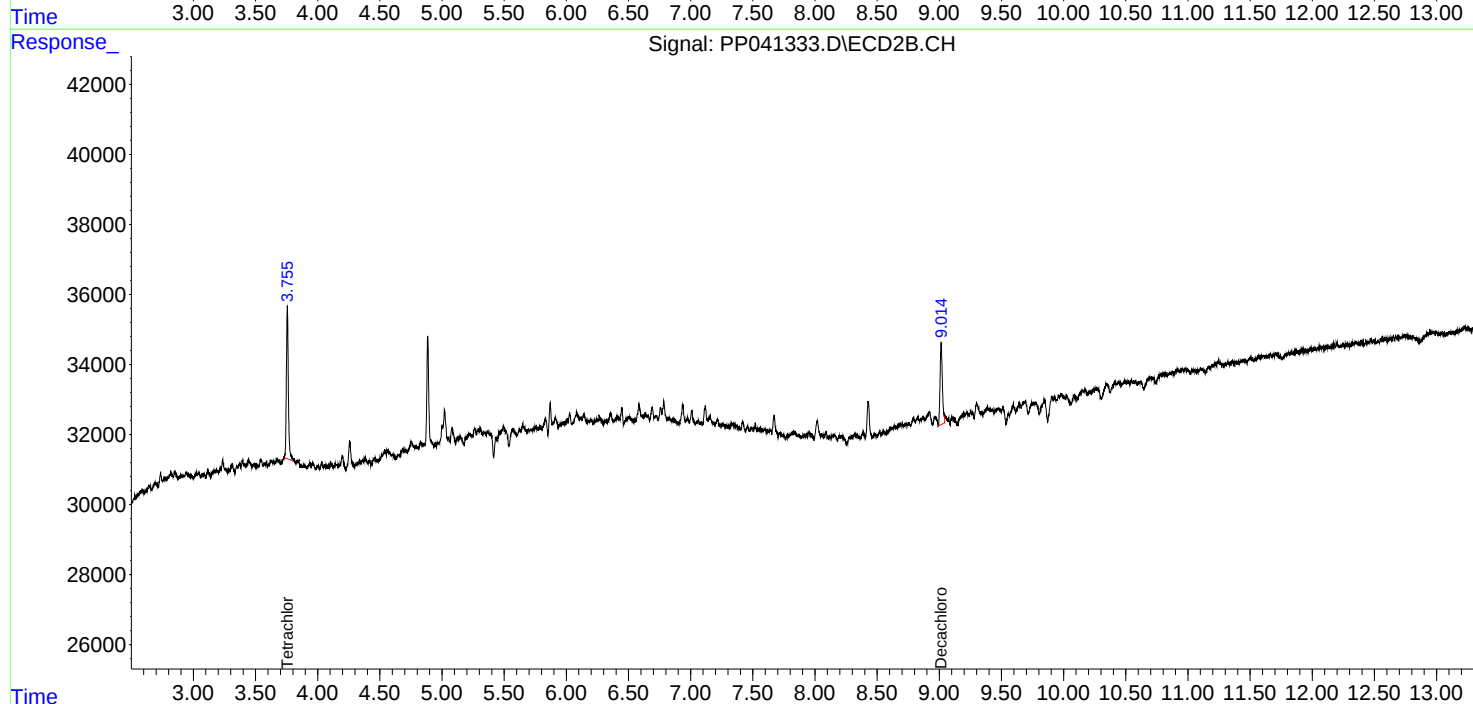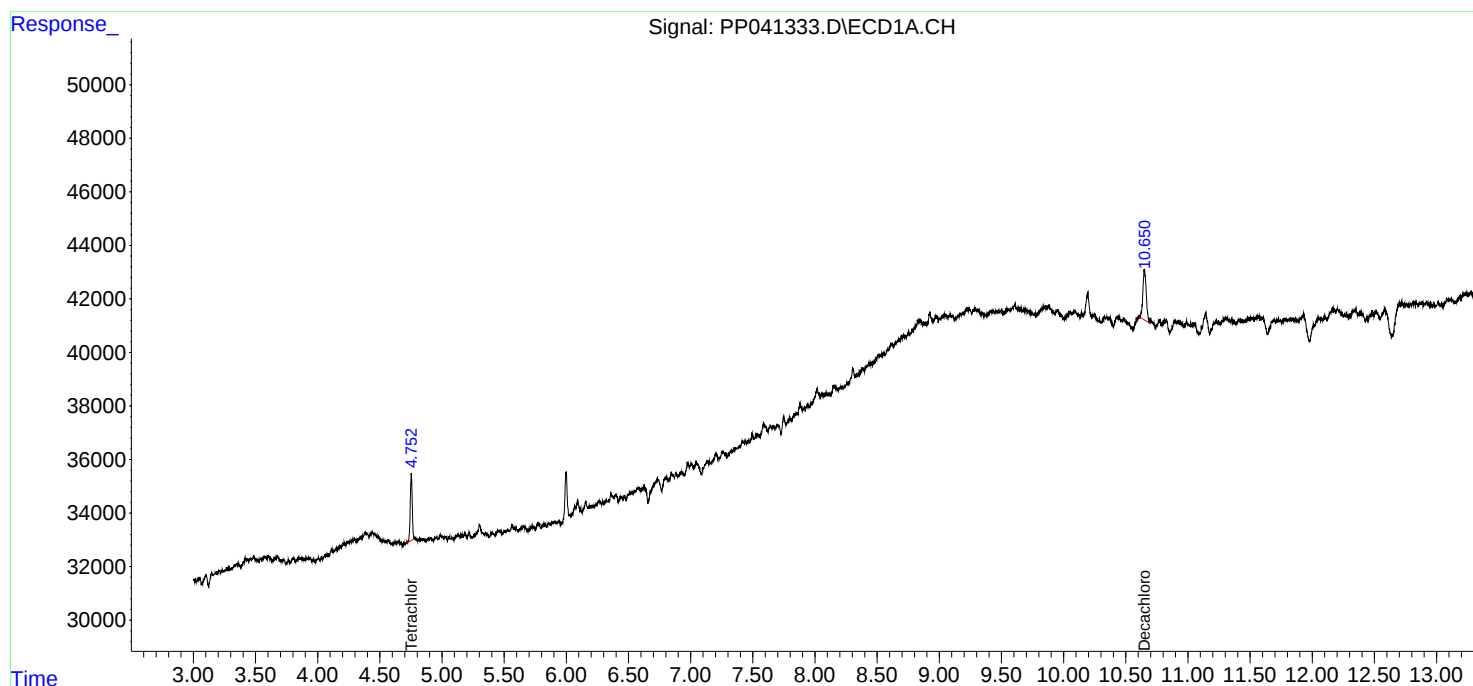

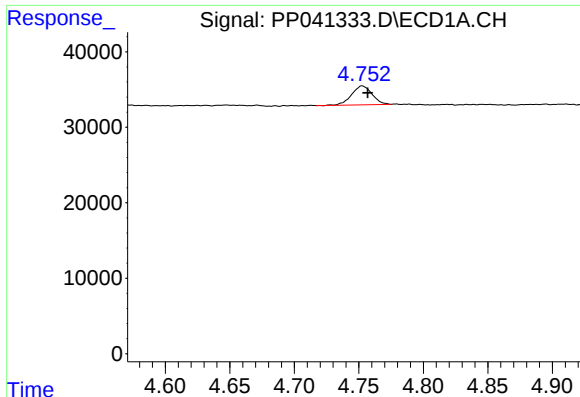

#1 Tetrachloro-m-xylene

R.T.: 4.753 min
Delta R.T.: -0.004 min
Response: 27652
Conc: 1.31 ng/ml

Instrument :

ECD_P


ClientSampleId :

SEC-2021-48B

Manual Integrations


APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

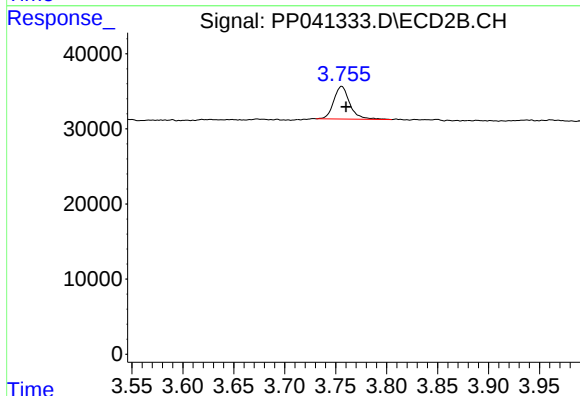


#1 Tetrachloro-m-xylene

R.T.: 3.756 min
Delta R.T.: -0.004 min
Response: 47693
Conc: 1.72 ng/ml

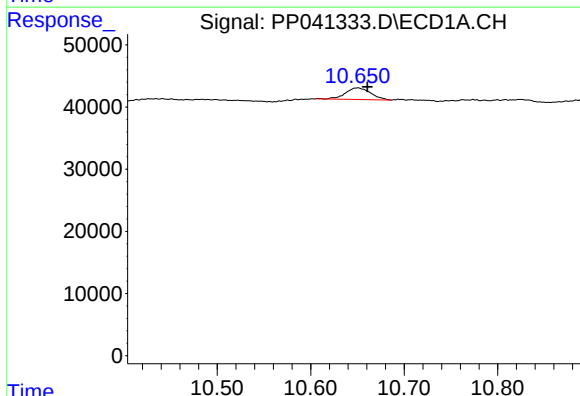

#2 Decachlorobiphenyl

R.T.: 10.651 min
Delta R.T.: -0.010 min
Response: 34888
Conc: 1.60 ng/ml

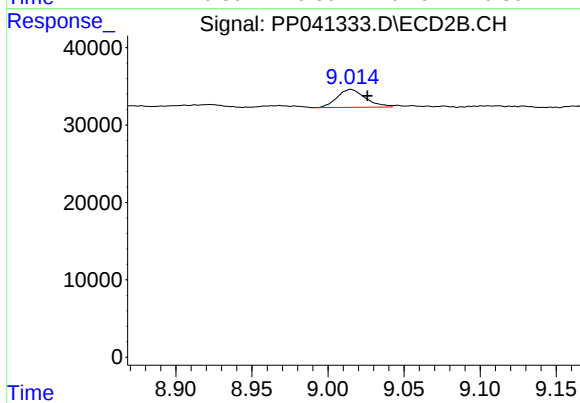

#2 Decachlorobiphenyl

R.T.: 9.014 min
Delta R.T.: -0.011 min
Response: 30090
Conc: 2.10 ng/ml m