

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
 Data File : PP031693.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 17:15
 Operator : DD\AJ
 Sample : L4880-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-B4-112320-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:44:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.789	4.062	1134630	1065055	23.431	22.226
2)	SA Decachlor...	10.661	9.363	687605	725341	20.245	19.589
Target Compounds							
7)	L1 AR-1016-5	0.000	5.794f	0	8790	N.D.	7.728 #
9)	L2 AR-1221-2	0.000	4.415	0	10220	N.D.	26.494 #
15)	L3 AR-1232-5	0.000	5.794	0	8790	N.D.	30.332 #
20)	L4 AR-1242-5	0.000	6.198	0	6436	N.D.	6.238 #
24)	L5 AR-1248-4	0.000	5.794f	0	8790	N.D.	5.737 #
26)	L6 AR-1254-1	0.000	6.198	0	6436	N.D.	2.975 #
30)	L6 AR-1254-5	0.000	7.436	0	12402	N.D.	4.594 #
31)	L7 AR-1260-1	0.000	6.921	0	1405	N.D.	0.711 #
32)	L7 AR-1260-2	0.000	7.097	0	6452	N.D.	2.649 #
33)	L7 AR-1260-3	0.000	7.255	0	1535	N.D.	0.672 #
34)	L7 AR-1260-4	0.000	7.741	0	14271	N.D.	7.511 #
35)	L7 AR-1260-5	0.000	7.977	0	63580	N.D.	14.011 #
36)	L8 AR-1262-1	0.000	7.474	0	7662	N.D.	2.757 #
37)	L8 AR-1262-2	0.000	7.977	0	63580	N.D.	13.089 #
38)	L8 AR-1262-3	0.000	8.267	0	8638	N.D.	4.392 #
39)	L8 AR-1262-4	0.000	8.343	0	13651	N.D.	3.766 #
40)	L8 AR-1262-5	0.000	8.834	0	1136	N.D.	0.700 #
41)	L9 AR-1268-1	0.000	8.267	0	8638	N.D.	1.561 #
42)	L9 AR-1268-2	0.000	8.343	0	13651	N.D.	2.525 #
44)	L9 AR-1268-4	0.000	8.834	0	1136	N.D.	0.623 #
45)	L9 AR-1268-5	0.000	9.122	0	2570	N.D.	0.186 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
Data File : PP031693.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 17:15
Operator : DD\AJ
Sample : L4880-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:44:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

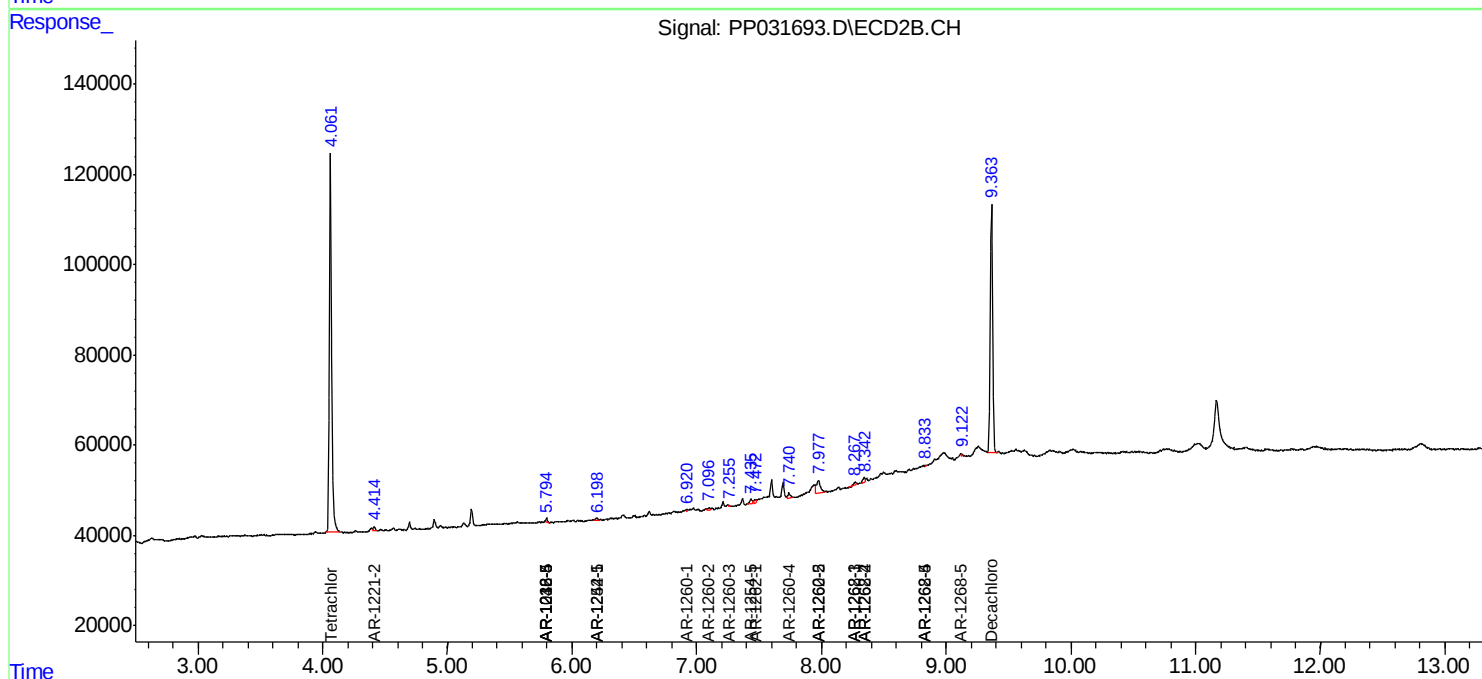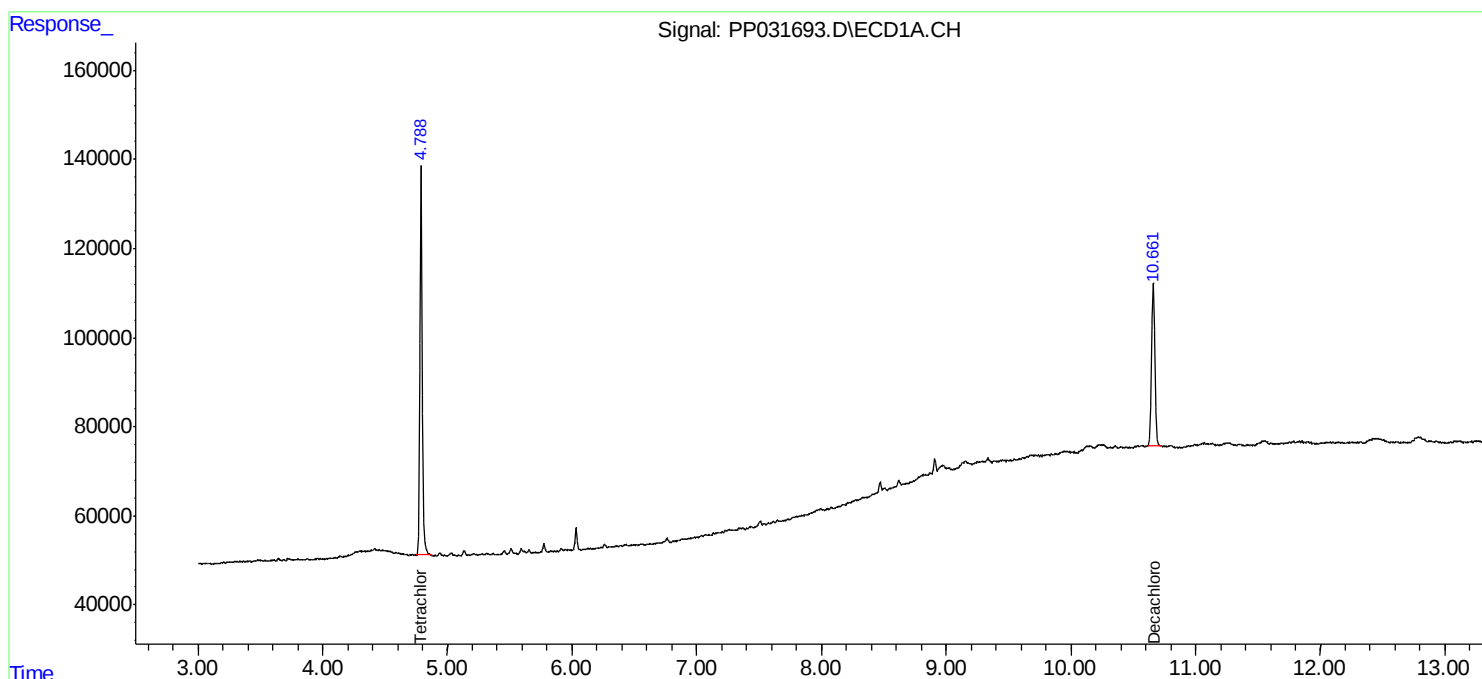


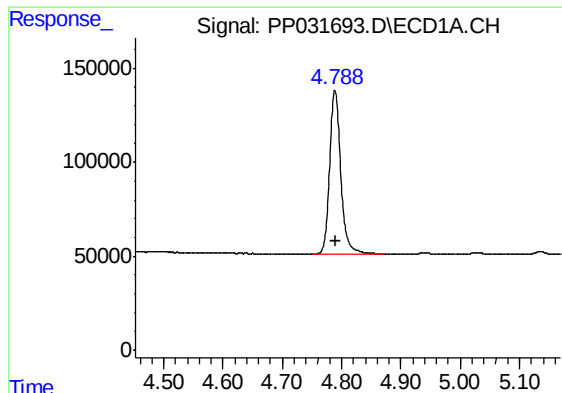

#1 Tetrachloro-m-xylene


R.T.: 4.789 min
Delta R.T.: -0.001 min
Response: 1134630
Conc: 23.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

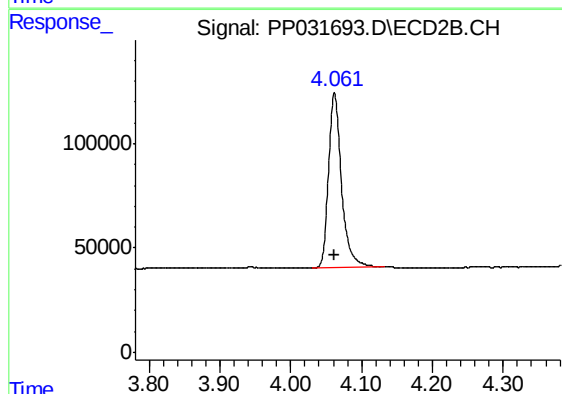


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: 0.000 min
Response: 1065055
Conc: 22.23 ng/ml

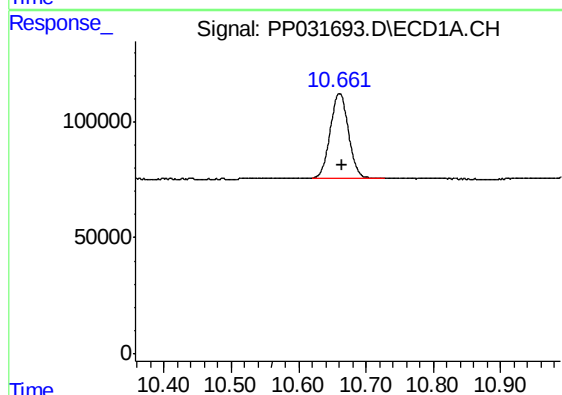


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.004 min
Response: 687605
Conc: 20.25 ng/ml

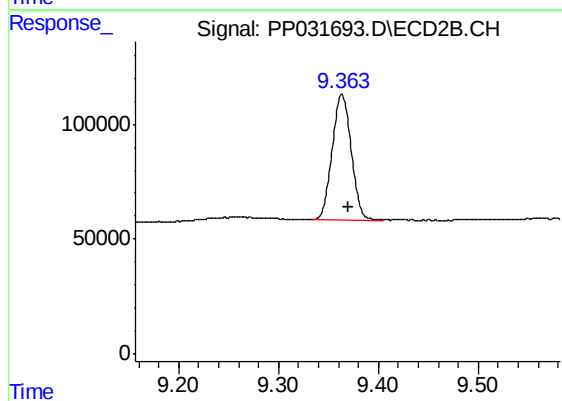

#2 Decachlorobiphenyl


R.T.: 9.363 min
Delta R.T.: -0.007 min
Response: 725341
Conc: 19.59 ng/ml

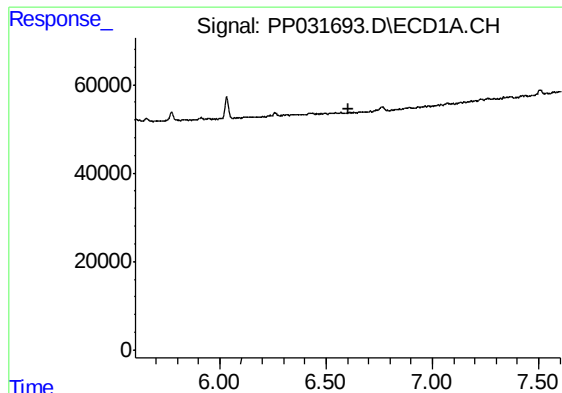

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

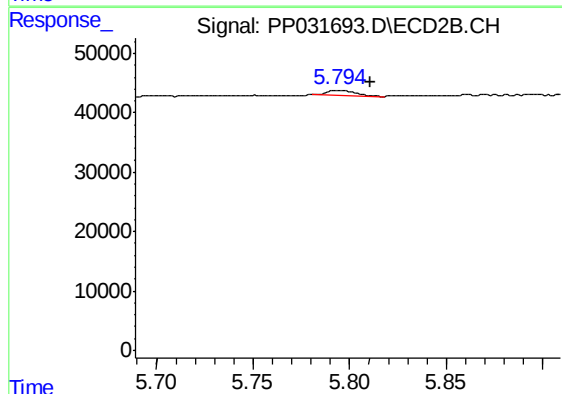


#7 AR-1016-5

R.T.: 5.794 min
Delta R.T.: -0.017 min
Response: 8790
Conc: 7.73 ng/ml




#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

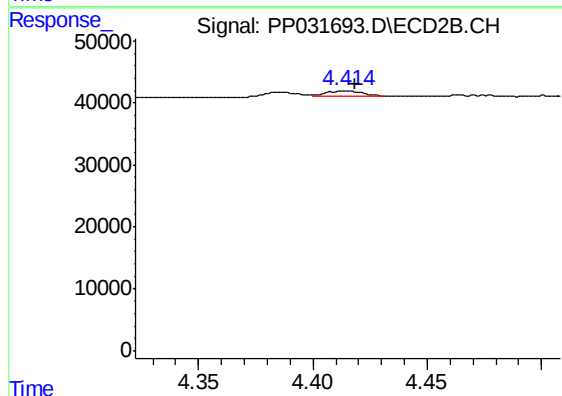

#9 AR-1221-2


R.T.: 4.415 min
Delta R.T.: -0.004 min
Response: 10220
Conc: 26.49 ng/ml

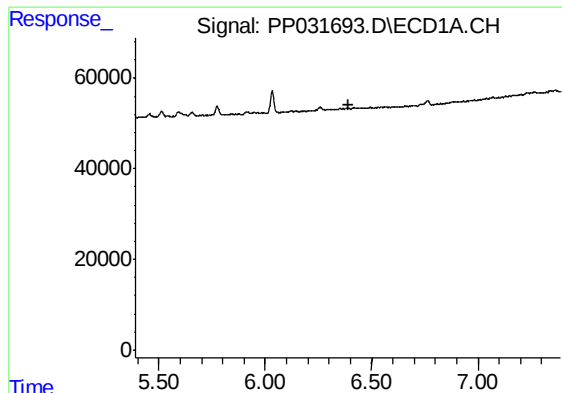

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

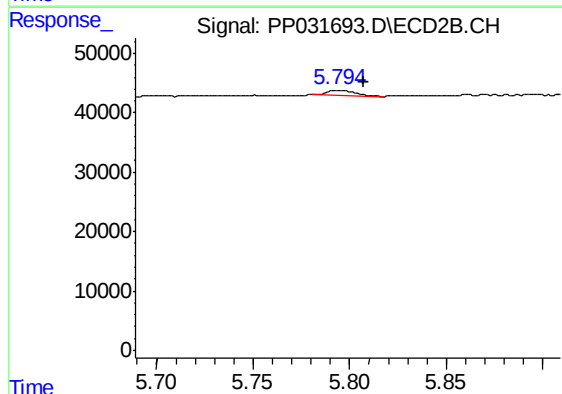


#15 AR-1232-5

R.T.: 5.794 min
Delta R.T.: -0.013 min
Response: 8790
Conc: 30.33 ng/ml

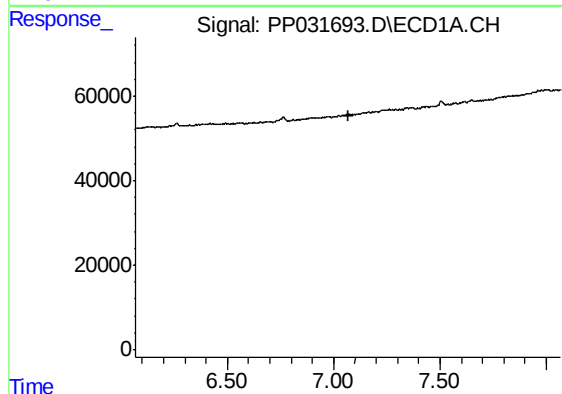


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

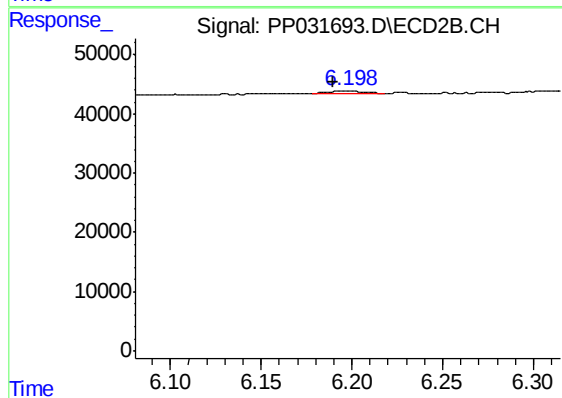

#20 AR-1242-5


R.T.: 6.198 min
Delta R.T.: 0.009 min
Response: 6436
Conc: 6.24 ng/ml



#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

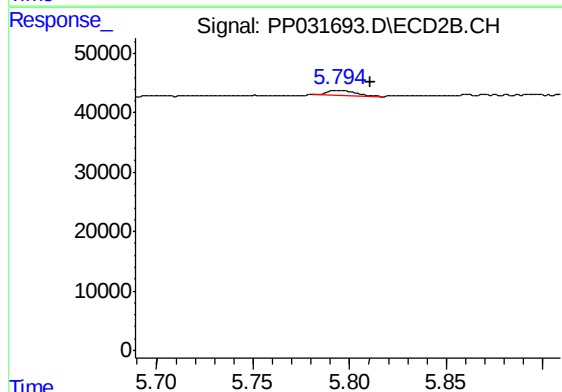


#24 AR-1248-4

R.T.: 5.794 min
Delta R.T.: -0.017 min
Response: 8790
Conc: 5.74 ng/ml




#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

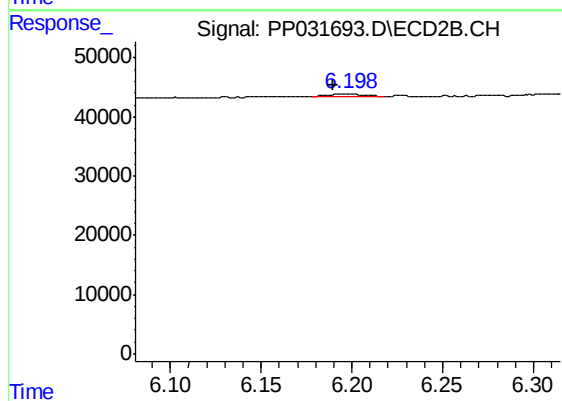

#26 AR-1254-1


R.T.: 6.198 min
Delta R.T.: 0.008 min
Response: 6436
Conc: 2.98 ng/ml

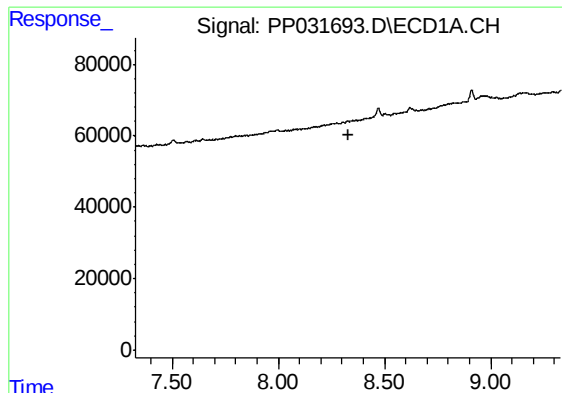

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 8.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

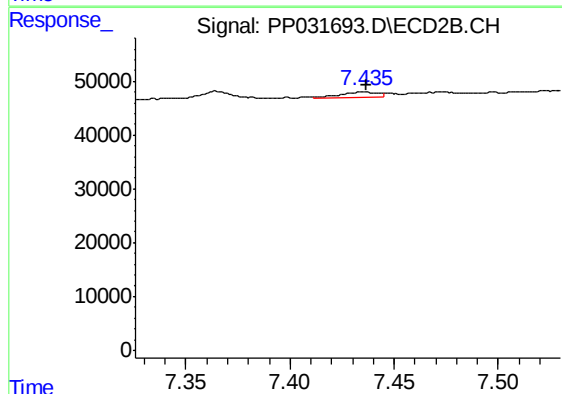


#30 AR-1254-5

R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 12402
Conc: 4.59 ng/ml




#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.775 min
Response: 0
Conc: N.D.

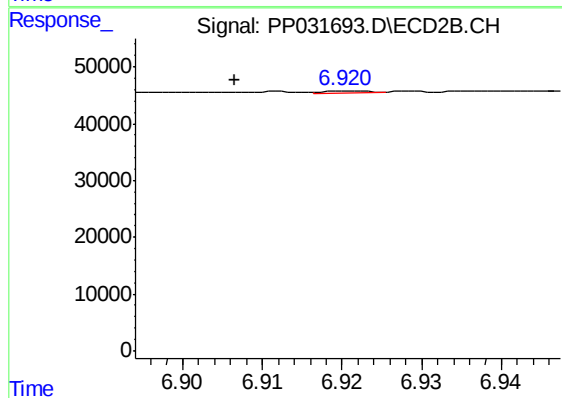

#31 AR-1260-1


R.T.: 6.921 min
Delta R.T.: 0.014 min
Response: 1405
Conc: 0.71 ng/ml



#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

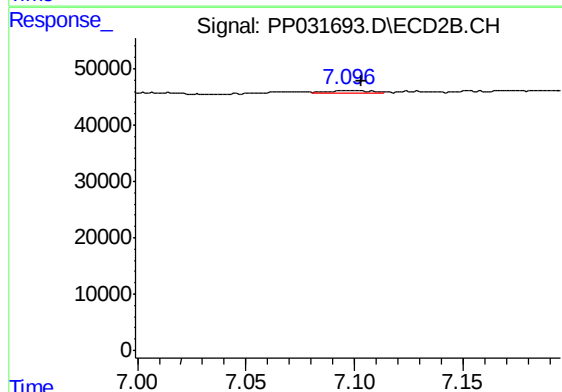


#32 AR-1260-2

R.T.: 7.097 min
Delta R.T.: -0.006 min
Response: 6452
Conc: 2.65 ng/ml




#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.406 min
Response: 0
Conc: N.D.

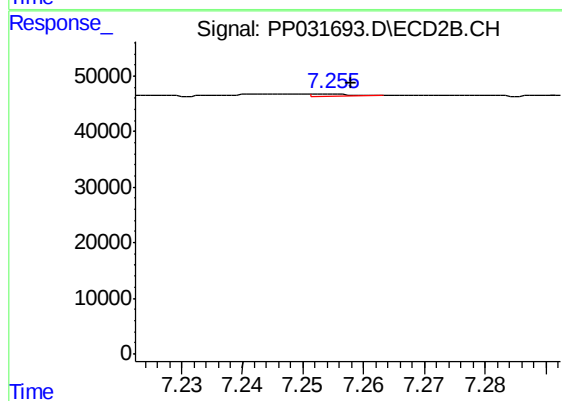

#33 AR-1260-3


R.T.: 7.255 min
Delta R.T.: -0.003 min
Response: 1535
Conc: 0.67 ng/ml



#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 8.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

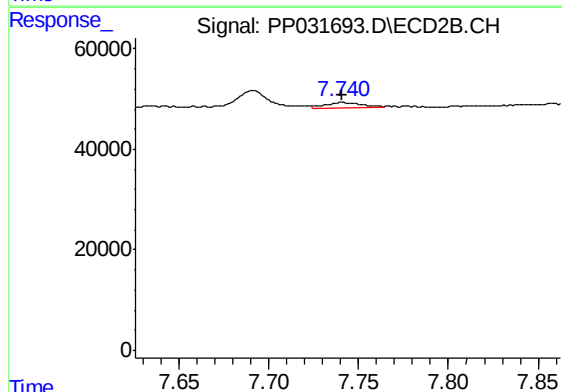


#34 AR-1260-4

R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 14271
Conc: 7.51 ng/ml




#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

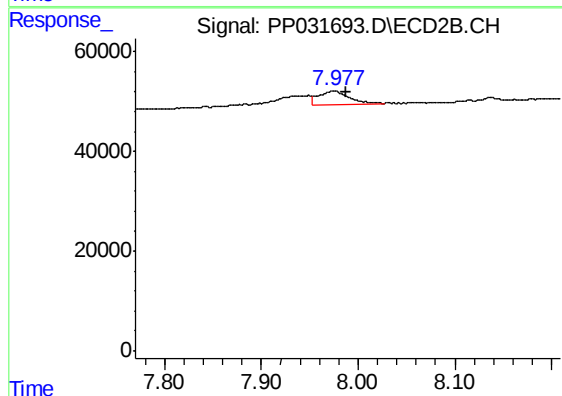

#35 AR-1260-5


R.T.: 7.977 min
Delta R.T.: -0.011 min
Response: 63580
Conc: 14.01 ng/ml



#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

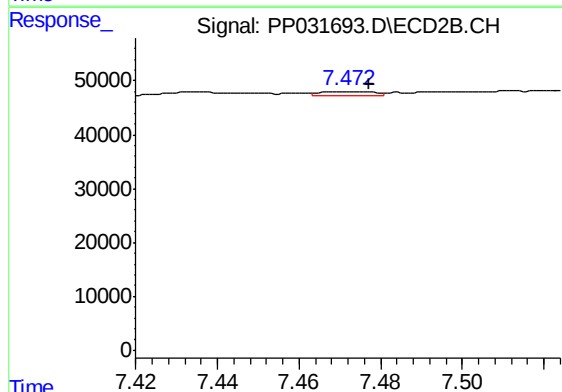


#36 AR-1262-1

R.T.: 7.474 min
Delta R.T.: -0.003 min
Response: 7662
Conc: 2.76 ng/ml




#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

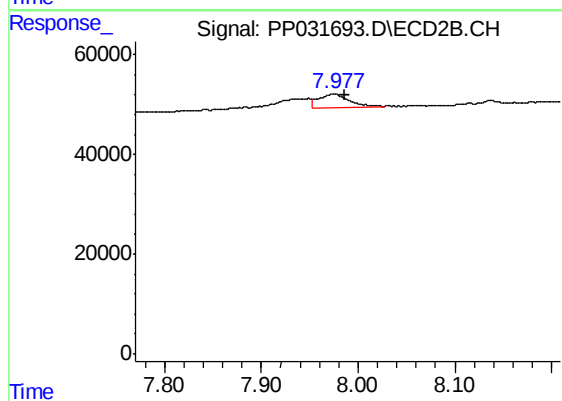

#37 AR-1262-2


R.T.: 7.977 min
Delta R.T.: -0.010 min
Response: 63580
Conc: 13.09 ng/ml



#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

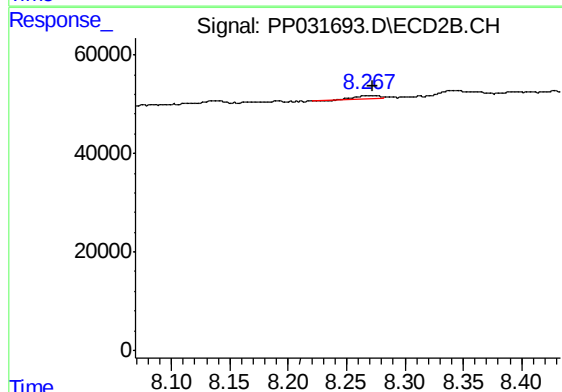


#38 AR-1262-3

R.T.: 8.267 min
Delta R.T.: -0.005 min
Response: 8638
Conc: 4.39 ng/ml




#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

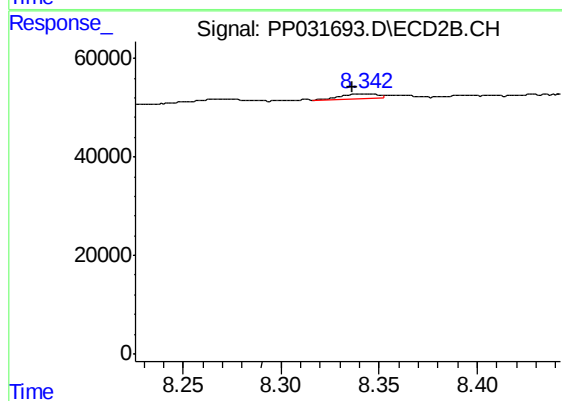

#39 AR-1262-4


R.T.: 8.343 min
Delta R.T.: 0.007 min
Response: 13651
Conc: 3.77 ng/ml

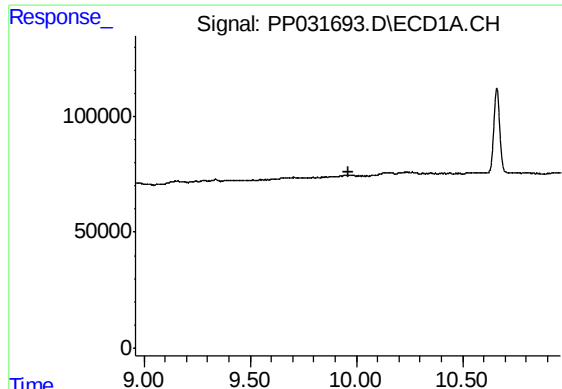

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

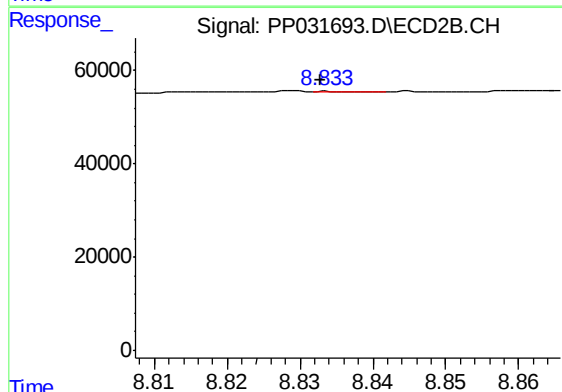


#40 AR-1262-5

R.T.: 8.834 min
Delta R.T.: 0.001 min
Response: 1136
Conc: 0.70 ng/ml




#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

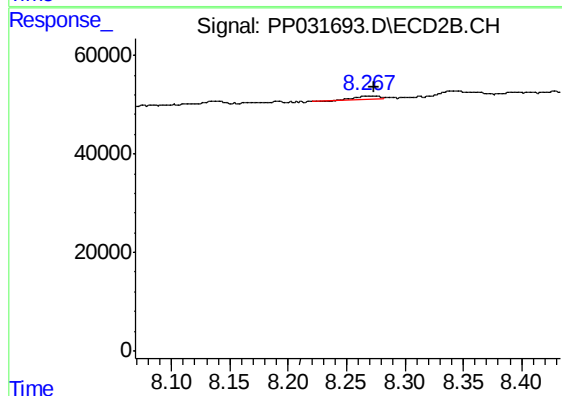

#41 AR-1268-1


R.T.: 8.267 min
Delta R.T.: -0.006 min
Response: 8638
Conc: 1.56 ng/ml



#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

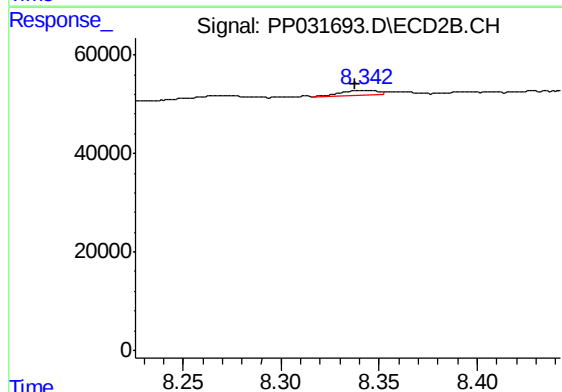


#42 AR-1268-2

R.T.: 8.343 min
Delta R.T.: 0.005 min
Response: 13651
Conc: 2.52 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

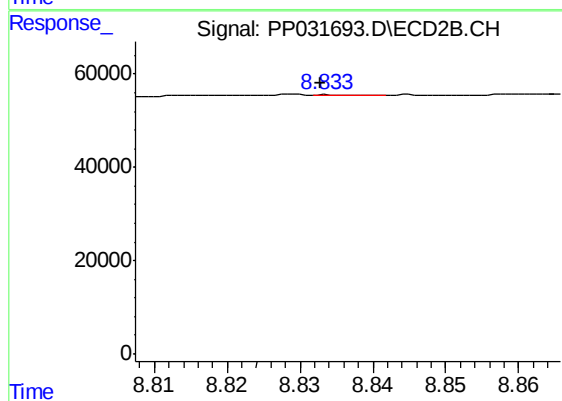

#44 AR-1268-4


R.T.: 8.834 min
Delta R.T.: 0.001 min
Response: 1136
Conc: 0.62 ng/ml

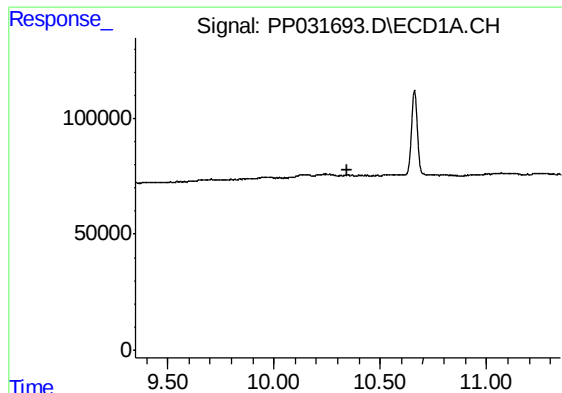

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2

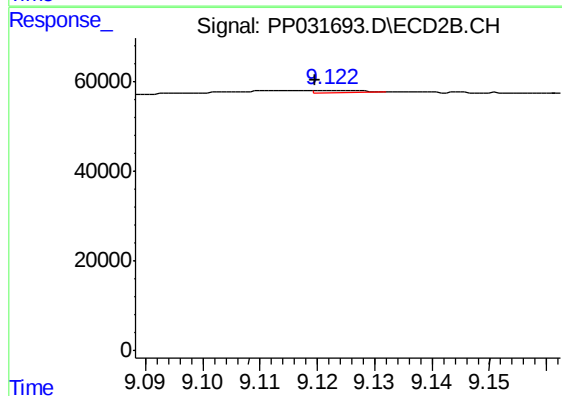

#45 AR-1268-5

R.T.: 9.122 min
Delta R.T.: 0.003 min
Response: 2570
Conc: 0.19 ng/ml