

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
 Data File : PP031695.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 17:48
 Operator : DD\AJ
 Sample : L4880-06MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-B4-112320-0-2MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:45:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.789	4.061	1294746	1178341	26.738	24.591
2)	SA Decachlor...	10.660	9.363	790976	866581	23.289	23.404
Target Compounds							
3)	L1 AR-1016-1	6.093	5.316	817521	783468	539.334	530.182
4)	L1 AR-1016-2	6.117	5.336	1210212	1151111	535.958	529.416
5)	L1 AR-1016-3	6.182	5.527	752563	628010	544.729	537.330
6)	L1 AR-1016-4	6.287	5.579	646645	457789	556.485	524.451
7)	L1 AR-1016-5	6.601	5.808	564630	604351	512.250	531.343
8)	L2 AR-1221-1	5.029	4.316	121388	76436	223.202	150.658 #
9)	L2 AR-1221-2	5.133	4.416	111722	111708	269.367	289.583
10)	L2 AR-1221-3	5.218	4.505	458452	446051	372.329	369.799
11)	L3 AR-1232-1	5.218	4.505	458452	446051	439.450	429.349
12)	L3 AR-1232-2	5.801	5.336	657292	1151111	1212.111	1182.049
13)	L3 AR-1232-3	6.117	5.527	1210212	628010	1198.348	1190.816
14)	L3 AR-1232-4	6.287	5.623	646645	566416	1219.560	1341.183
15)	L3 AR-1232-5	6.388	5.808	441518	604351	1374.443	2085.505 #
16)	L4 AR-1242-1	6.093	5.316	817521	783468	683.151	686.285
17)	L4 AR-1242-2	6.117	5.336	1210212	1151111	680.168	684.480
18)	L4 AR-1242-3	6.182	5.527	752563	628010	675.897	687.760
19)	L4 AR-1242-4	6.287	5.623	646645	566416	699.681	674.298
20)	L4 AR-1242-5	7.066	6.187	82601	466772	90.163	452.416 #
21)	L5 AR-1248-1	6.093	5.316	817521	783468	885.319	909.621
22)	L5 AR-1248-2	6.388	5.579	441518	457789	373.264	383.404
23)	L5 AR-1248-3	6.601	5.623	564630	566416	385.958	447.504
24)	L5 AR-1248-4	7.027	5.808	88423	604351	56.385	394.471 #
25)	L5 AR-1248-5	7.066	6.230	82601	76307	52.033	52.300
26)	L6 AR-1254-1	6.998	6.187	405054	466772	265.808	215.778
27)	L6 AR-1254-2	7.226	6.345	418190	442825	180.065	237.697 #
28)	L6 AR-1254-3	7.605	6.784	250930	784371	99.326	253.739 #
29)	L6 AR-1254-4	7.898	7.005	150782	86760	88.862	51.068 #
30)	L6 AR-1254-5	8.327	7.432	1386200	1541654	741.516	571.072
31)	L7 AR-1260-1	7.774	6.902	946369	1095216	540.769	554.234
32)	L7 AR-1260-2	8.038	7.098	1103250	1279312	536.929	525.332
33)	L7 AR-1260-3	8.403	7.253	731499	1249565	448.488	547.182
34)	L7 AR-1260-4	8.631	7.736	905890	908309	491.971	478.028
35)	L7 AR-1260-5	8.946	7.982	1732037	2207251	469.742	486.398
36)	L8 AR-1262-1	8.403	7.473	731499	965527	321.954	347.408
37)	L8 AR-1262-2	8.946	7.982	1732037	2207251	435.886	454.415
38)	L8 AR-1262-3	9.259	8.269	1138720	420738	409.425	213.909 #
39)	L8 AR-1262-4	9.332	8.332	273435	1585141	124.735	437.258 #
40)	L8 AR-1262-5	9.957	8.829	460880	524682	315.666	323.242
41)	L9 AR-1268-1	9.259f	8.269	1138720	420738	236.959	76.041 #
42)	L9 AR-1268-2	9.332	8.332	273435	1585141	58.738	293.181 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
 Data File : PP031695.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 17:48
 Operator : DD\AJ
 Sample : L4880-06MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-B4-112320-0-2MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:45:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.548	8.541	40431	42977	9.998	9.370
44) L9	AR-1268-4	9.957	8.829	460880	524682	296.713	287.859
45) L9	AR-1268-5	10.346	9.114	172837	183345	14.169	13.240



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
Data File : PP031695.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 17:48
Operator : DD\AJ
Sample : L4880-06MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:45:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

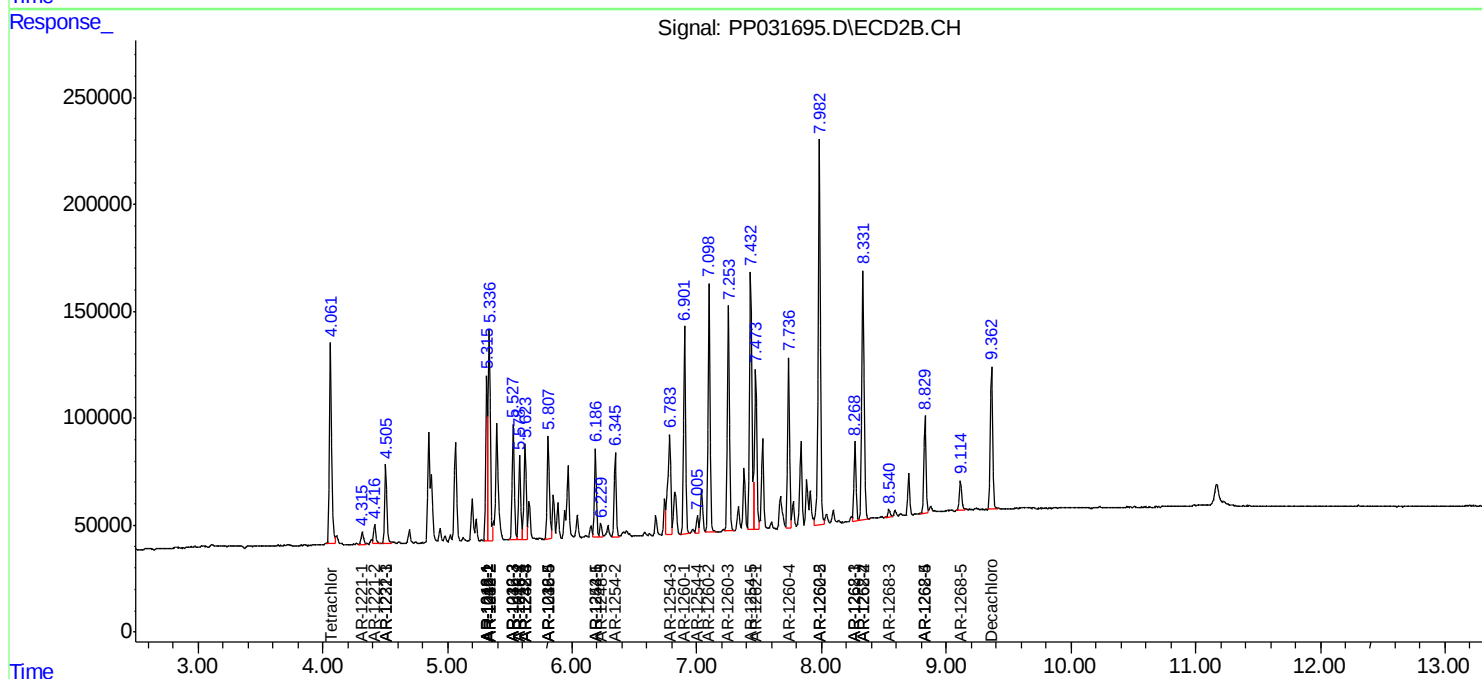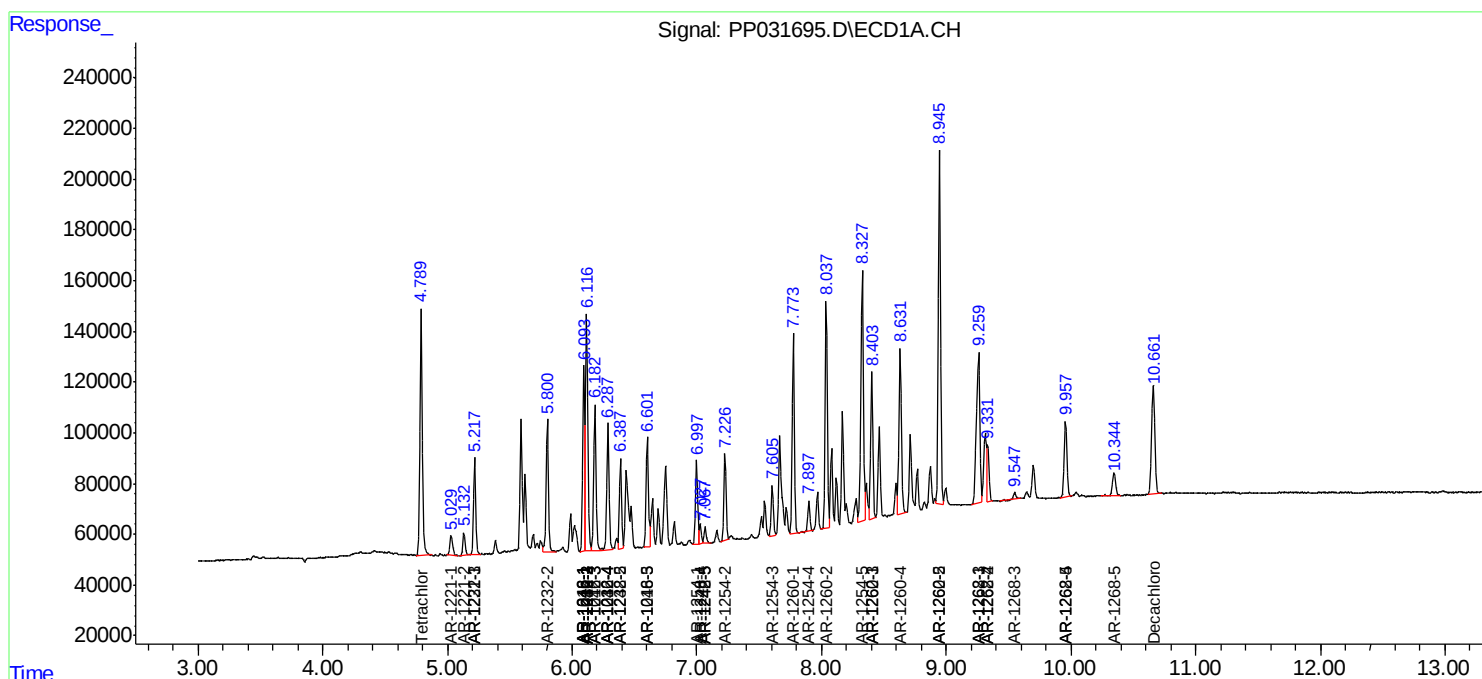


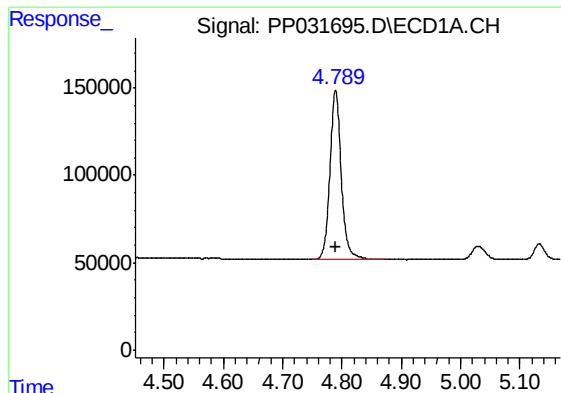

#1 Tetrachloro-m-xylene


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 1294746
Conc: 26.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

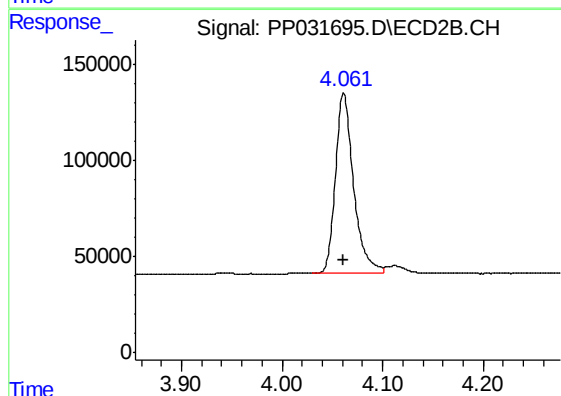


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1178341
Conc: 24.59 ng/ml

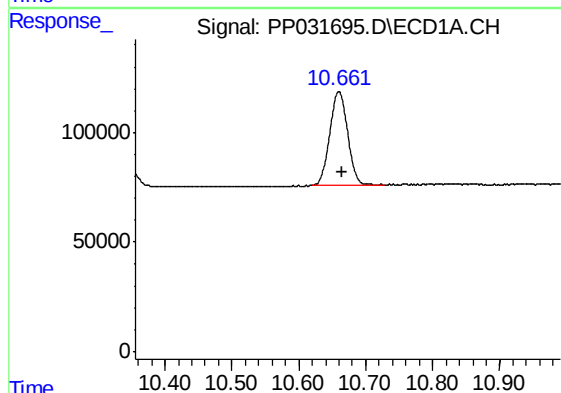


#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.005 min
Response: 790976
Conc: 23.29 ng/ml

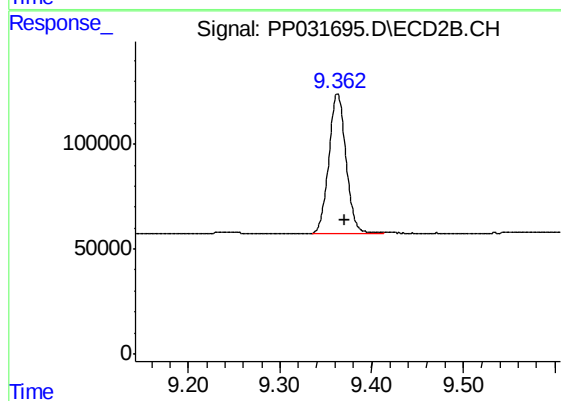

#2 Decachlorobiphenyl


R.T.: 9.363 min
Delta R.T.: -0.007 min
Response: 866581
Conc: 23.40 ng/ml

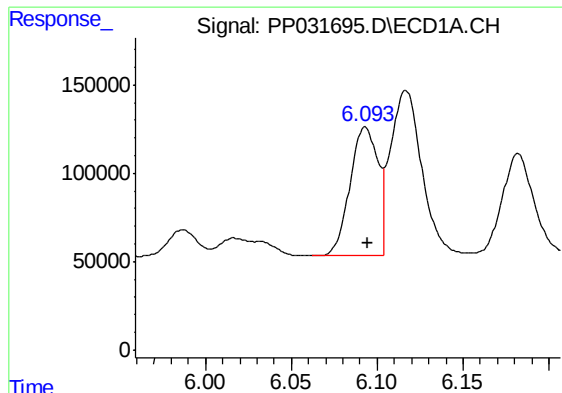

#3 AR-1016-1


R.T.: 6.093 min
Delta R.T.: -0.002 min
Response: 817521
Conc: 539.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

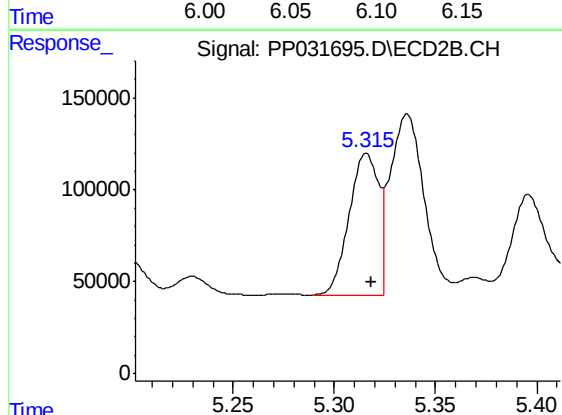


#3 AR-1016-1

R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 783468
Conc: 530.18 ng/ml

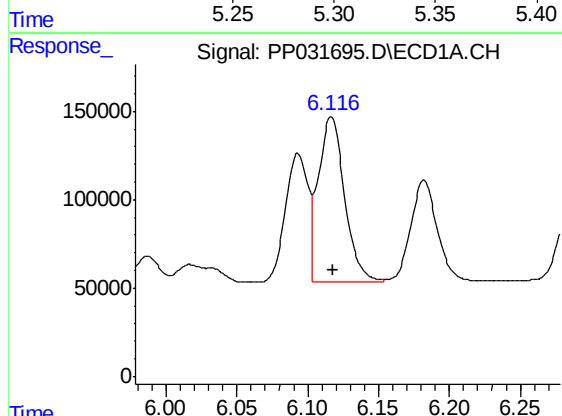


#4 AR-1016-2

R.T.: 6.117 min
Delta R.T.: -0.001 min
Response: 1210212
Conc: 535.96 ng/ml

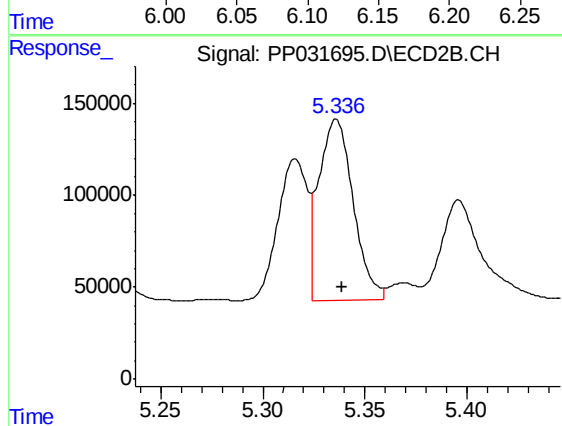

#4 AR-1016-2


R.T.: 5.336 min
Delta R.T.: -0.003 min
Response: 1151111
Conc: 529.42 ng/ml

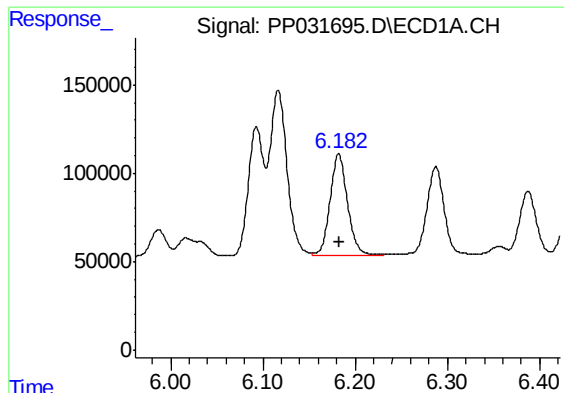

#5 AR-1016-3


R.T.: 6.182 min
Delta R.T.: -0.001 min
Response: 752563
Conc: 544.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

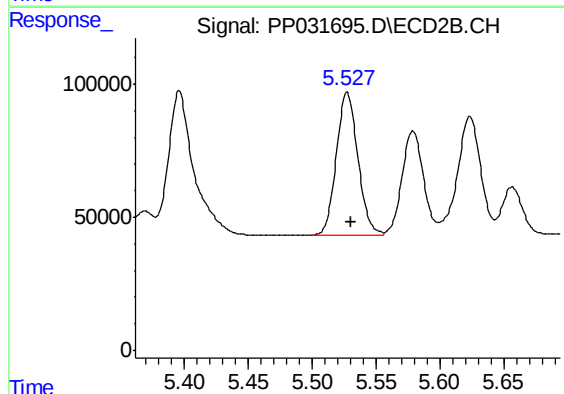


#5 AR-1016-3

R.T.: 5.527 min
Delta R.T.: -0.003 min
Response: 628010
Conc: 537.33 ng/ml

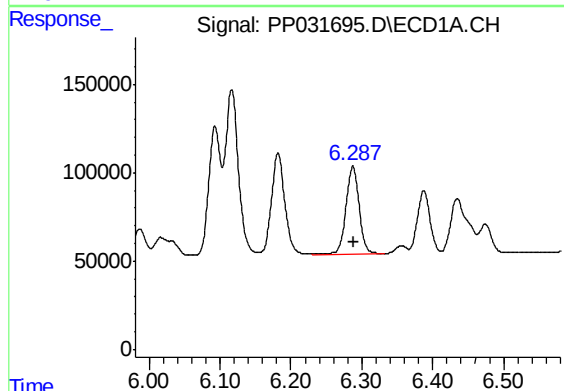


#6 AR-1016-4

R.T.: 6.287 min
Delta R.T.: -0.002 min
Response: 646645
Conc: 556.49 ng/ml

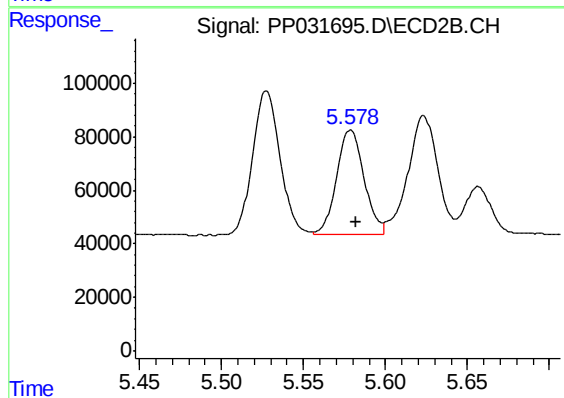

#6 AR-1016-4


R.T.: 5.579 min
Delta R.T.: -0.003 min
Response: 457789
Conc: 524.45 ng/ml



#7 AR-1016-5


R.T.: 6.601 min
Delta R.T.: -0.002 min
Response: 564630
Conc: 512.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#7 AR-1016-5

R.T.: 5.808 min
Delta R.T.: -0.003 min
Response: 604351
Conc: 531.34 ng/ml




#8 AR-1221-1

R.T.: 5.029 min
Delta R.T.: -0.006 min
Response: 121388
Conc: 223.20 ng/ml

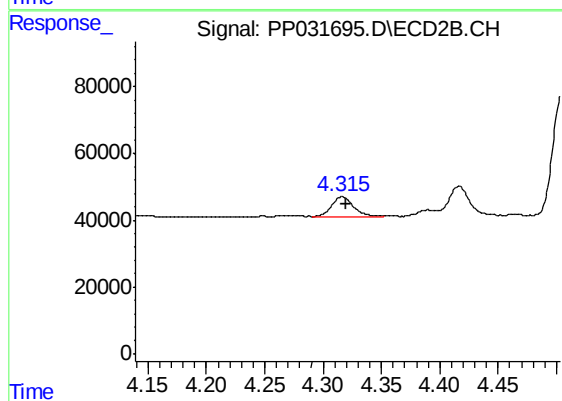

#8 AR-1221-1


R.T.: 4.316 min
Delta R.T.: -0.003 min
Response: 76436
Conc: 150.66 ng/ml

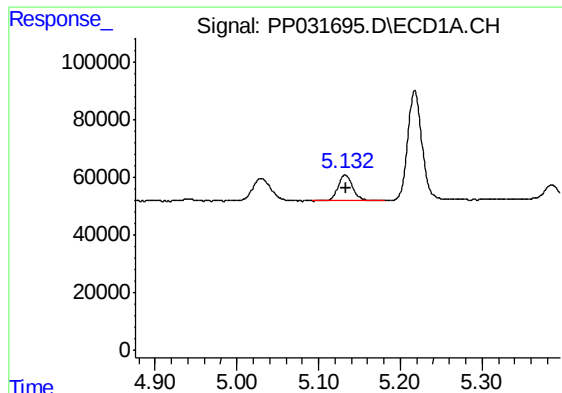

#9 AR-1221-2


R.T.: 5.133 min
Delta R.T.: 0.000 min
Response: 111722
Conc: 269.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

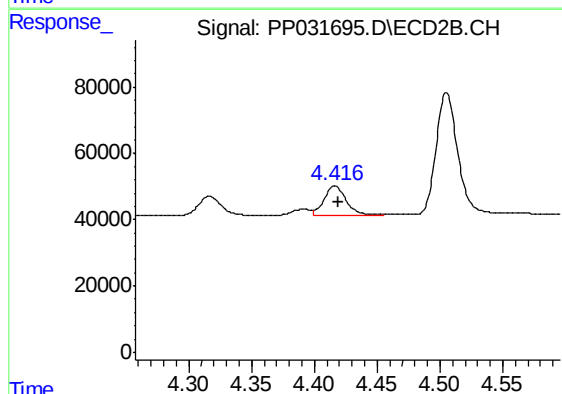


#9 AR-1221-2

R.T.: 4.416 min
Delta R.T.: -0.002 min
Response: 111708
Conc: 289.58 ng/ml

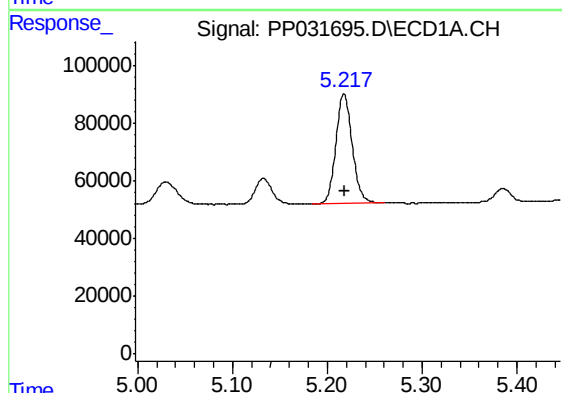


#10 AR-1221-3

R.T.: 5.218 min
Delta R.T.: 0.000 min
Response: 458452
Conc: 372.33 ng/ml

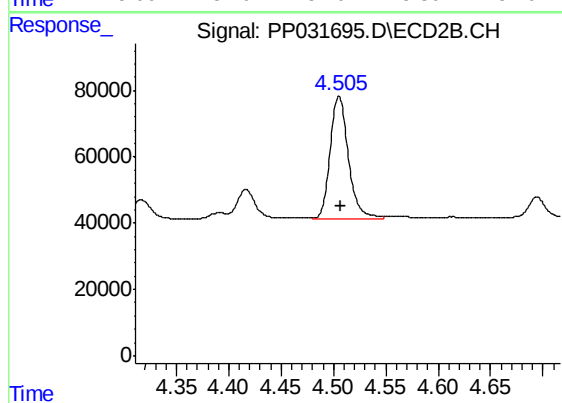

#10 AR-1221-3


R.T.: 4.505 min
Delta R.T.: -0.002 min
Response: 446051
Conc: 369.80 ng/ml



#11 AR-1232-1


R.T.: 5.218 min
Delta R.T.: 0.000 min
Response: 458452
Conc: 439.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#11 AR-1232-1

R.T.: 4.505 min
Delta R.T.: -0.002 min
Response: 446051
Conc: 429.35 ng/ml




#12 AR-1232-2

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 657292
Conc: 1212.11 ng/ml

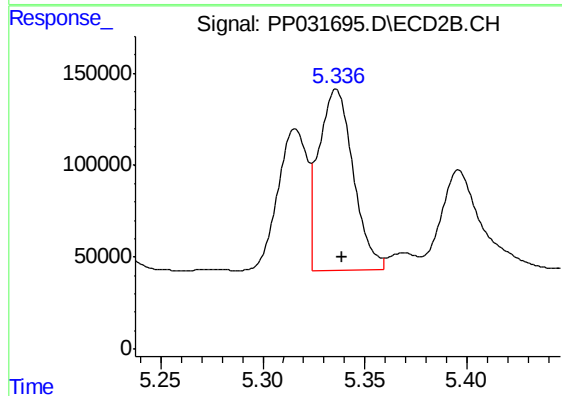

#12 AR-1232-2


R.T.: 5.336 min
Delta R.T.: -0.003 min
Response: 1151111
Conc: 1182.05 ng/ml



#13 AR-1232-3


R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 1210212
Conc: 1198.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

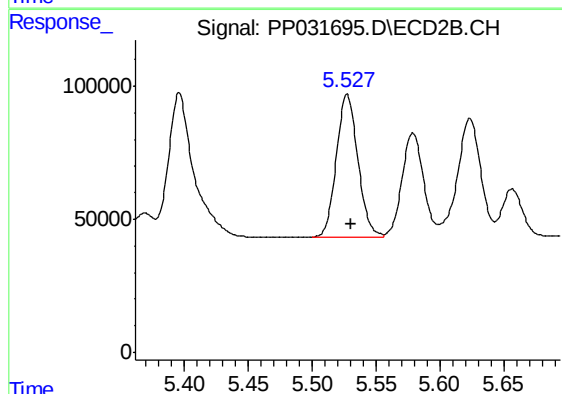


#13 AR-1232-3

R.T.: 5.527 min
Delta R.T.: -0.003 min
Response: 628010
Conc: 1190.82 ng/ml

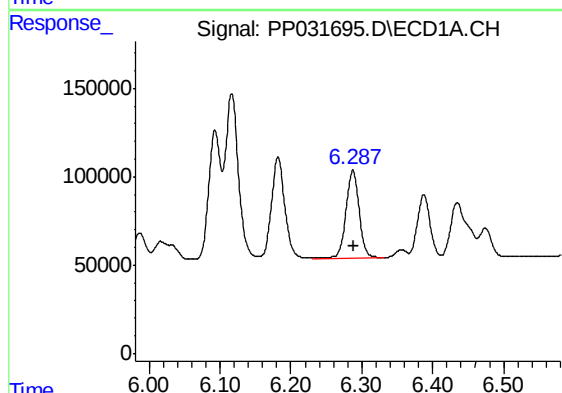


#14 AR-1232-4

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 646645
Conc: 1219.56 ng/ml

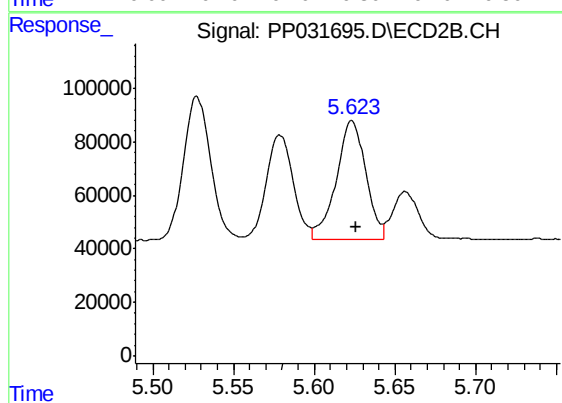

#14 AR-1232-4


R.T.: 5.623 min
Delta R.T.: -0.003 min
Response: 566416
Conc: 1341.18 ng/ml

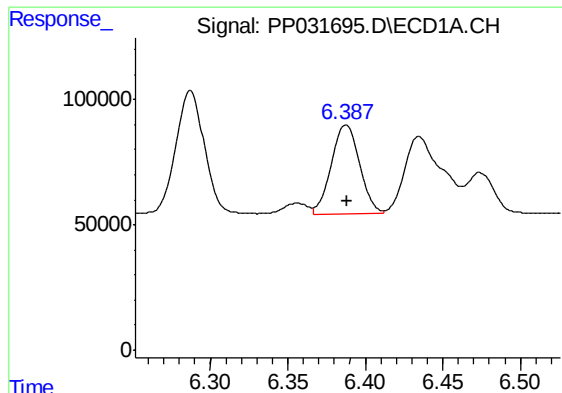

#15 AR-1232-5


R.T.: 6.388 min
Delta R.T.: -0.001 min
Response: 441518
Conc: 1374.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

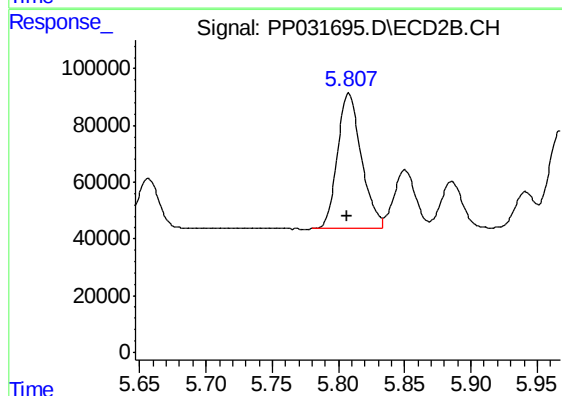


#15 AR-1232-5

R.T.: 5.808 min
Delta R.T.: 0.000 min
Response: 604351
Conc: 2085.51 ng/ml

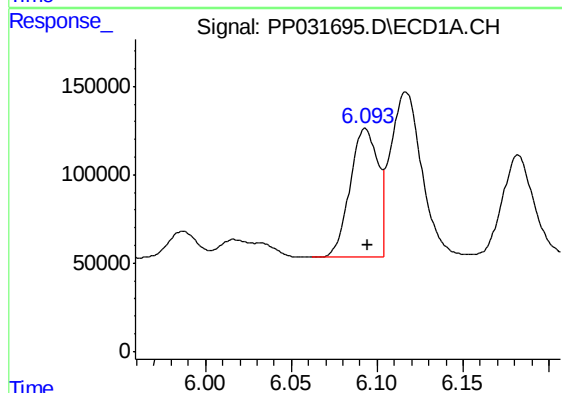


#16 AR-1242-1

R.T.: 6.093 min
Delta R.T.: -0.002 min
Response: 817521
Conc: 683.15 ng/ml

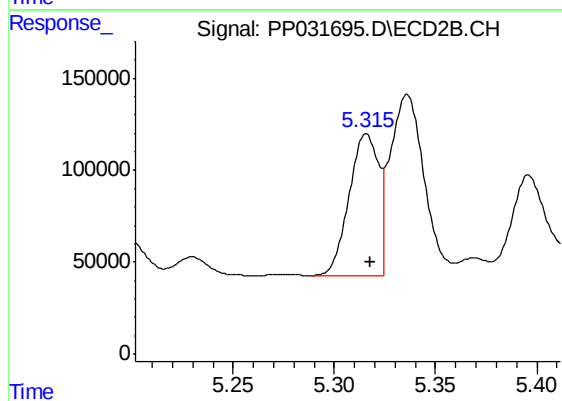

#16 AR-1242-1


R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 783468
Conc: 686.28 ng/ml



#17 AR-1242-2


R.T.: 6.117 min
Delta R.T.: -0.001 min
Response: 1210212
Conc: 680.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#17 AR-1242-2

R.T.: 5.336 min
Delta R.T.: -0.003 min
Response: 1151111
Conc: 684.48 ng/ml




#18 AR-1242-3

R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 752563
Conc: 675.90 ng/ml

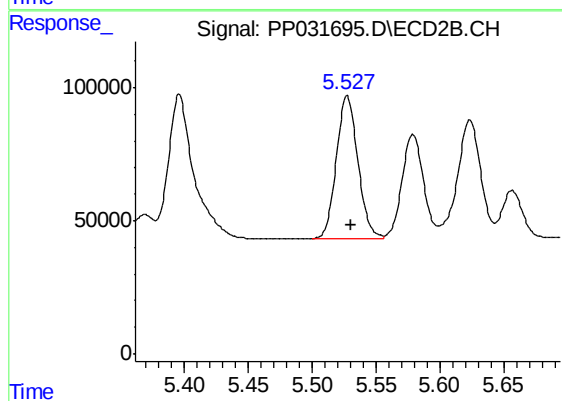

#18 AR-1242-3


R.T.: 5.527 min
Delta R.T.: -0.003 min
Response: 628010
Conc: 687.76 ng/ml

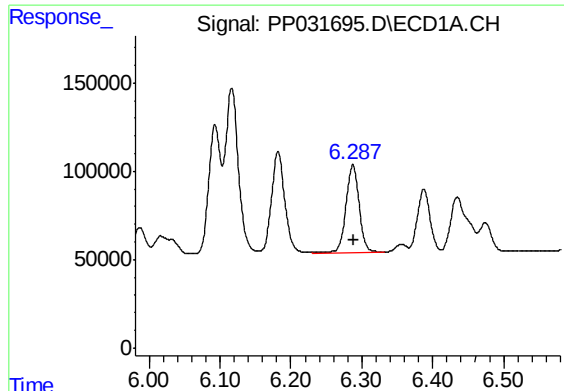

#19 AR-1242-4


R.T.: 6.287 min
Delta R.T.: -0.002 min
Response: 646645
Conc: 699.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

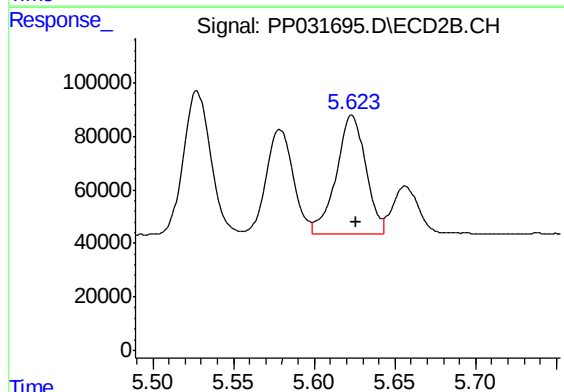


#19 AR-1242-4

R.T.: 5.623 min
Delta R.T.: -0.002 min
Response: 566416
Conc: 674.30 ng/ml

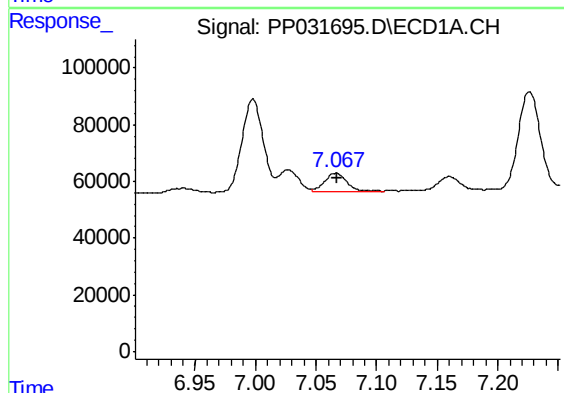


#20 AR-1242-5

R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 82601
Conc: 90.16 ng/ml

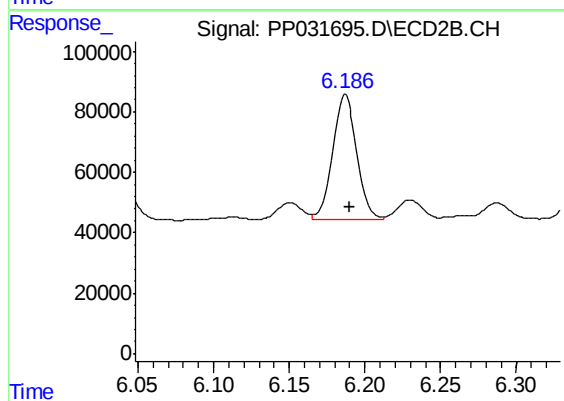

#20 AR-1242-5


R.T.: 6.187 min
Delta R.T.: -0.003 min
Response: 466772
Conc: 452.42 ng/ml



#21 AR-1248-1


R.T.: 6.093 min
Delta R.T.: -0.001 min
Response: 817521
Conc: 885.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

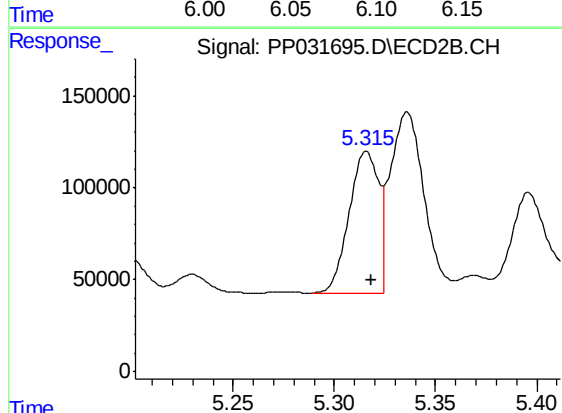


#21 AR-1248-1

R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 783468
Conc: 909.62 ng/ml

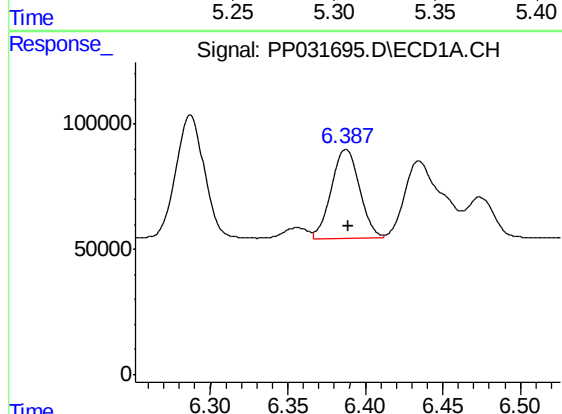


#22 AR-1248-2

R.T.: 6.388 min
Delta R.T.: -0.001 min
Response: 441518
Conc: 373.26 ng/ml

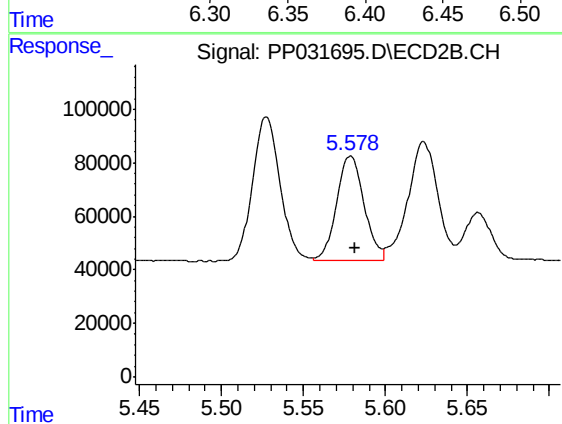

#22 AR-1248-2


R.T.: 5.579 min
Delta R.T.: -0.003 min
Response: 457789
Conc: 383.40 ng/ml



#23 AR-1248-3


R.T.: 6.601 min
Delta R.T.: -0.002 min
Response: 564630
Conc: 385.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#23 AR-1248-3

R.T.: 5.623 min
Delta R.T.: -0.003 min
Response: 566416
Conc: 447.50 ng/ml




#24 AR-1248-4

R.T.: 7.027 min
Delta R.T.: -0.002 min
Response: 88423
Conc: 56.38 ng/ml

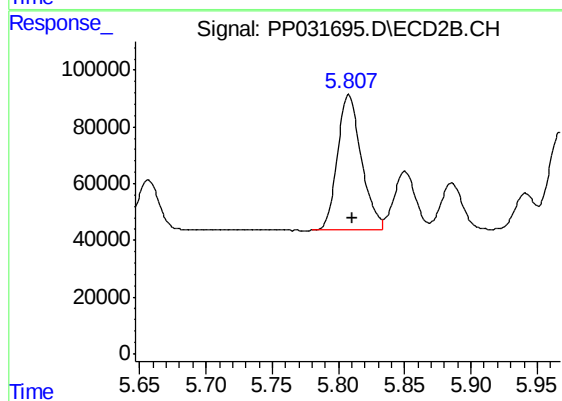

#24 AR-1248-4


R.T.: 5.808 min
Delta R.T.: -0.003 min
Response: 604351
Conc: 394.47 ng/ml



#25 AR-1248-5


R.T.: 7.066 min
Delta R.T.: -0.001 min
Response: 82601
Conc: 52.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#25 AR-1248-5

R.T.: 6.230 min
Delta R.T.: -0.004 min
Response: 76307
Conc: 52.30 ng/ml

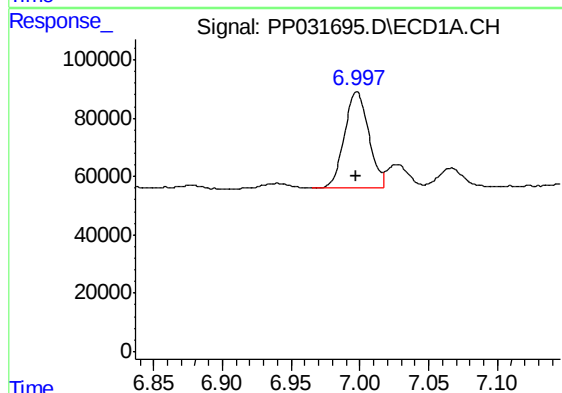


#26 AR-1254-1

R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 405054
Conc: 265.81 ng/ml

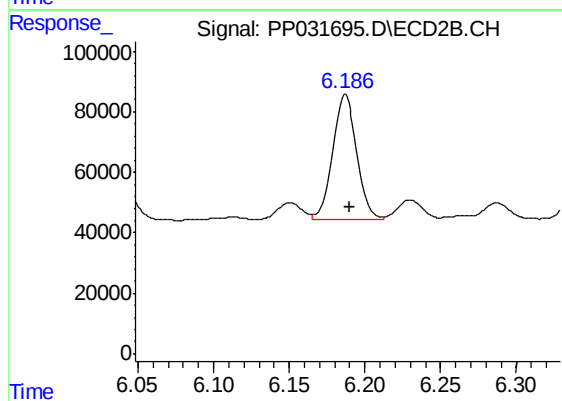

#26 AR-1254-1


R.T.: 6.187 min
Delta R.T.: -0.003 min
Response: 466772
Conc: 215.78 ng/ml



#27 AR-1254-2


R.T.: 7.226 min
Delta R.T.: -0.002 min
Response: 418190
Conc: 180.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#27 AR-1254-2

R.T.: 6.345 min
Delta R.T.: -0.004 min
Response: 442825
Conc: 237.70 ng/ml




#28 AR-1254-3

R.T.: 7.605 min
Delta R.T.: -0.001 min
Response: 250930
Conc: 99.33 ng/ml

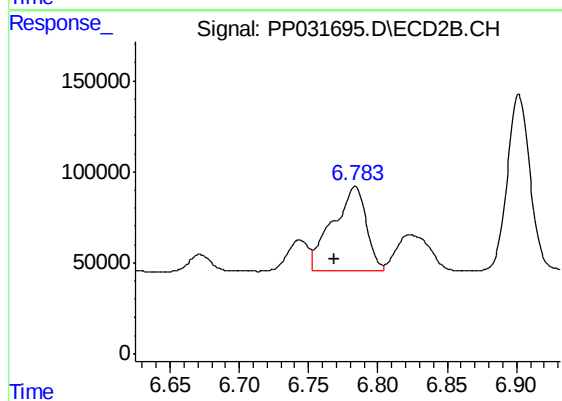

#28 AR-1254-3


R.T.: 6.784 min
Delta R.T.: 0.015 min
Response: 784371
Conc: 253.74 ng/ml

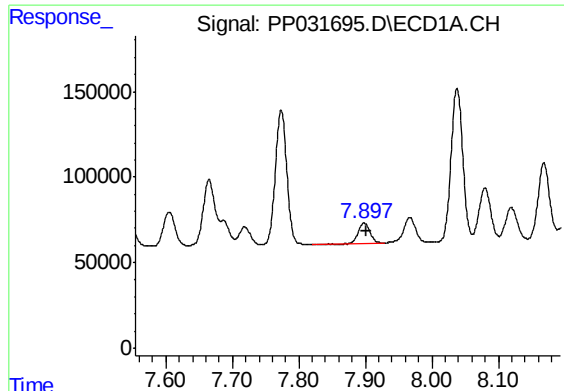

#29 AR-1254-4


R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 150782
Conc: 88.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

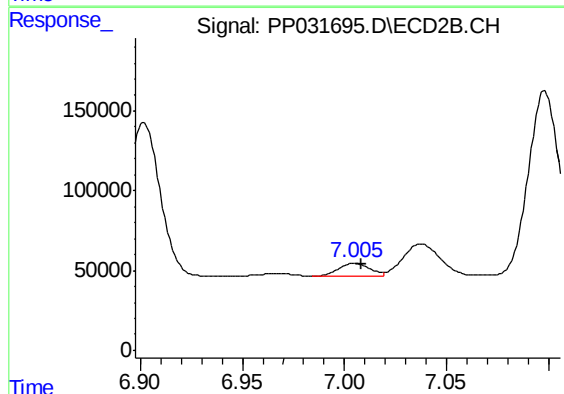


#29 AR-1254-4

R.T.: 7.005 min
Delta R.T.: -0.003 min
Response: 86760
Conc: 51.07 ng/ml

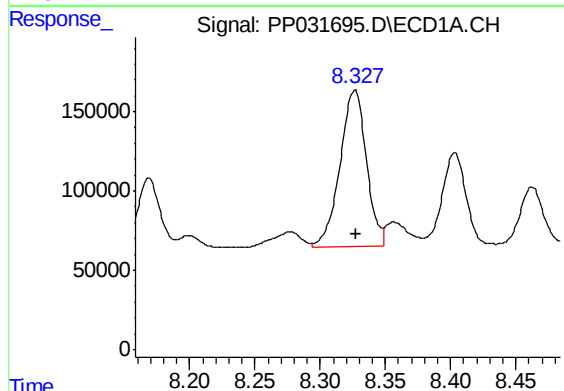


#30 AR-1254-5

R.T.: 8.327 min
Delta R.T.: -0.001 min
Response: 1386200
Conc: 741.52 ng/ml

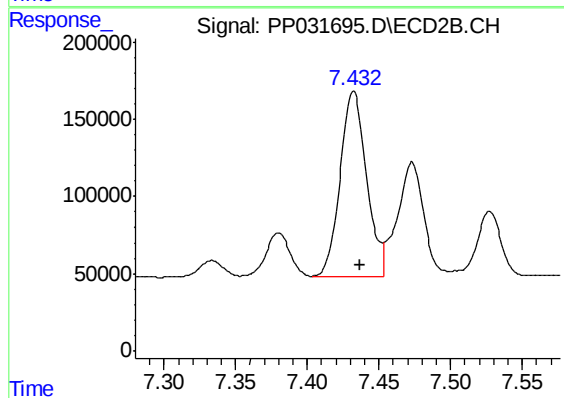

#30 AR-1254-5


R.T.: 7.432 min
Delta R.T.: -0.005 min
Response: 1541654
Conc: 571.07 ng/ml



#31 AR-1260-1


R.T.: 7.774 min
Delta R.T.: -0.002 min
Response: 946369
Conc: 540.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

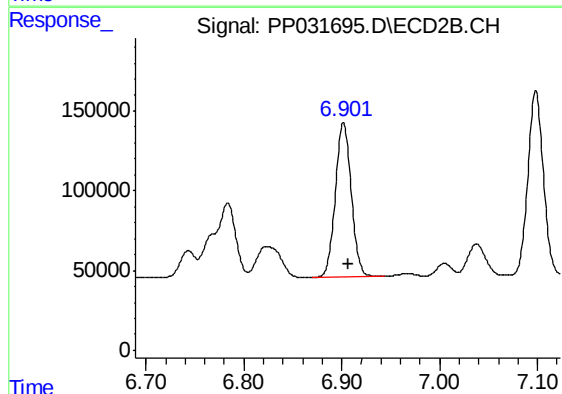


#31 AR-1260-1

R.T.: 6.902 min
Delta R.T.: -0.005 min
Response: 1095216
Conc: 554.23 ng/ml




#32 AR-1260-2

R.T.: 8.038 min
Delta R.T.: -0.002 min
Response: 1103250
Conc: 536.93 ng/ml

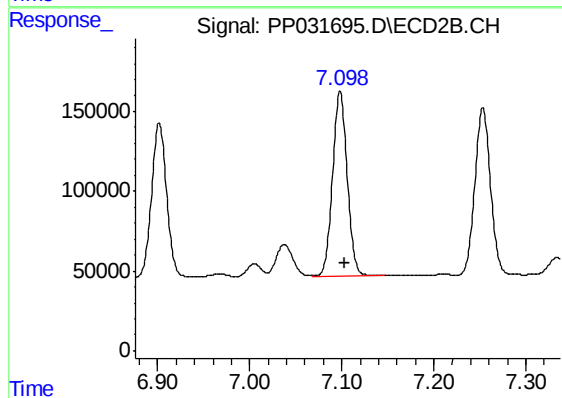

#32 AR-1260-2


R.T.: 7.098 min
Delta R.T.: -0.005 min
Response: 1279312
Conc: 525.33 ng/ml



#33 AR-1260-3


R.T.: 8.403 min
Delta R.T.: -0.003 min
Response: 731499
Conc: 448.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#33 AR-1260-3

R.T.: 7.253 min
Delta R.T.: -0.005 min
Response: 1249565
Conc: 547.18 ng/ml




#34 AR-1260-4

R.T.: 8.631 min
Delta R.T.: -0.002 min
Response: 905890
Conc: 491.97 ng/ml

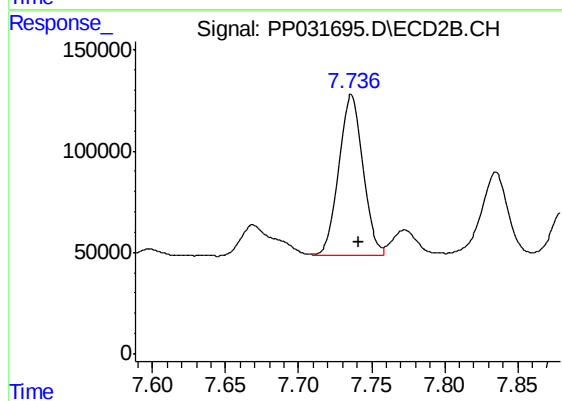

#34 AR-1260-4


R.T.: 7.736 min
Delta R.T.: -0.005 min
Response: 908309
Conc: 478.03 ng/ml



#35 AR-1260-5


R.T.: 8.946 min
Delta R.T.: -0.002 min
Response: 1732037
Conc: 469.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#35 AR-1260-5

R.T.: 7.982 min
Delta R.T.: -0.005 min
Response: 2207251
Conc: 486.40 ng/ml

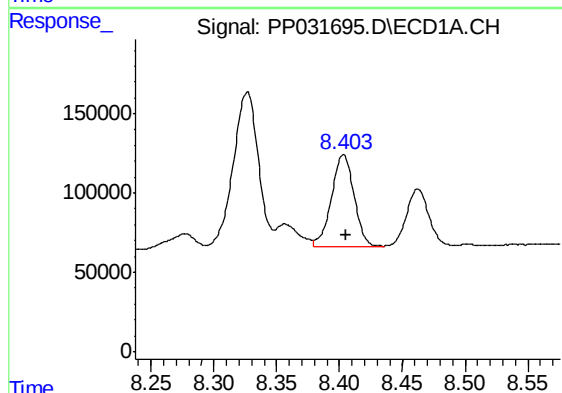


#36 AR-1262-1

R.T.: 8.403 min
Delta R.T.: -0.002 min
Response: 731499
Conc: 321.95 ng/ml

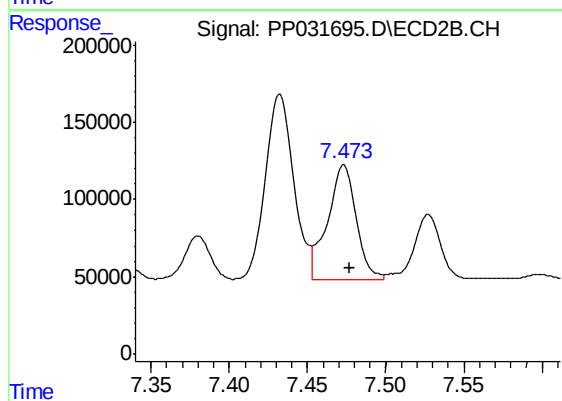

#36 AR-1262-1


R.T.: 7.473 min
Delta R.T.: -0.004 min
Response: 965527
Conc: 347.41 ng/ml



#37 AR-1262-2


R.T.: 8.946 min
Delta R.T.: -0.002 min
Response: 1732037
Conc: 435.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

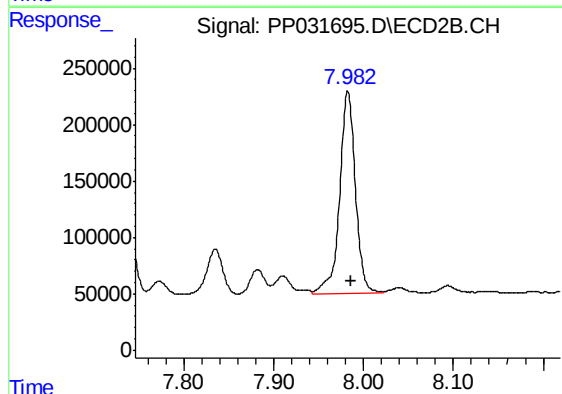


#37 AR-1262-2

R.T.: 7.982 min
Delta R.T.: -0.004 min
Response: 2207251
Conc: 454.41 ng/ml




#38 AR-1262-3

R.T.: 9.259 min
Delta R.T.: 0.013 min
Response: 1138720
Conc: 409.43 ng/ml

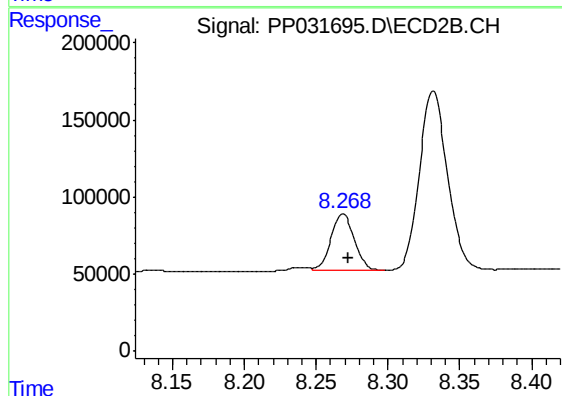

#38 AR-1262-3


R.T.: 8.269 min
Delta R.T.: -0.004 min
Response: 420738
Conc: 213.91 ng/ml



#39 AR-1262-4


R.T.: 9.332 min
Delta R.T.: -0.002 min
Response: 273435
Conc: 124.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#39 AR-1262-4

R.T.: 8.332 min
Delta R.T.: -0.005 min
Response: 1585141
Conc: 437.26 ng/ml




#40 AR-1262-5

R.T.: 9.957 min
Delta R.T.: -0.003 min
Response: 460880
Conc: 315.67 ng/ml

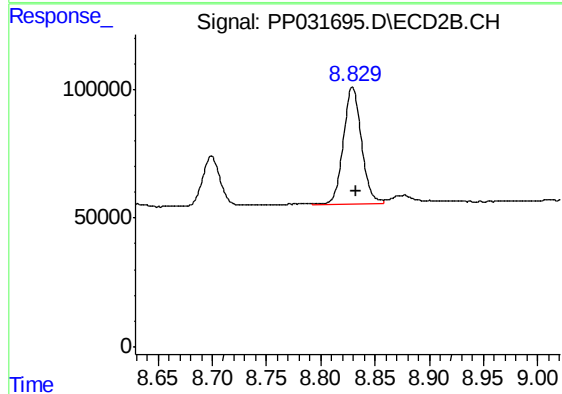

#40 AR-1262-5


R.T.: 8.829 min
Delta R.T.: -0.004 min
Response: 524682
Conc: 323.24 ng/ml

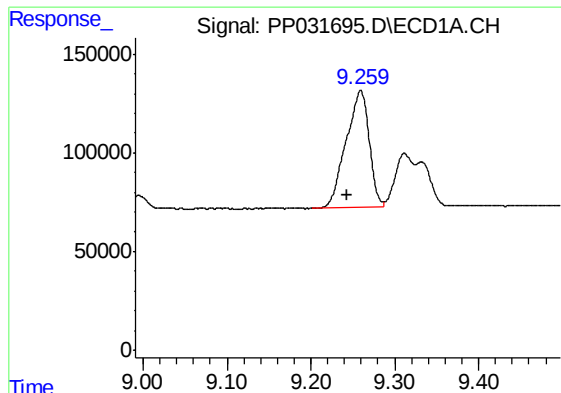

#41 AR-1268-1


R.T.: 9.259 min
Delta R.T.: 0.015 min
Response: 1138720
Conc: 236.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

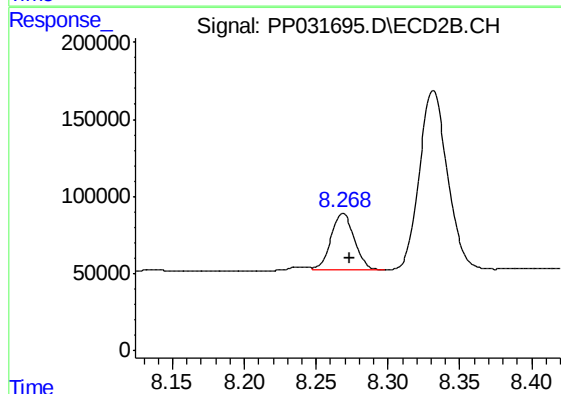


#41 AR-1268-1

R.T.: 8.269 min
Delta R.T.: -0.005 min
Response: 420738
Conc: 76.04 ng/ml

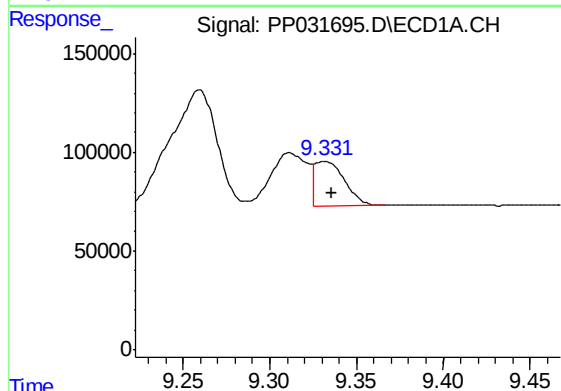


#42 AR-1268-2

R.T.: 9.332 min
Delta R.T.: -0.004 min
Response: 273435
Conc: 58.74 ng/ml

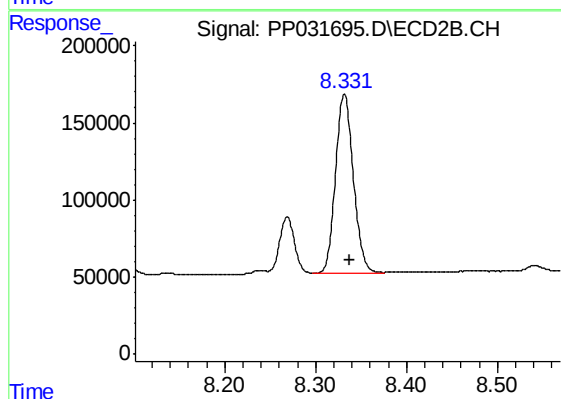

#42 AR-1268-2


R.T.: 8.332 min
Delta R.T.: -0.006 min
Response: 1585141
Conc: 293.18 ng/ml



#43 AR-1268-3


R.T.: 9.548 min
Delta R.T.: -0.002 min
Response: 40431
Conc: 10.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD




#43 AR-1268-3

R.T.: 8.541 min
Delta R.T.: -0.004 min
Response: 42977
Conc: 9.37 ng/ml




#44 AR-1268-4

R.T.: 9.957 min
Delta R.T.: -0.002 min
Response: 460880
Conc: 296.71 ng/ml

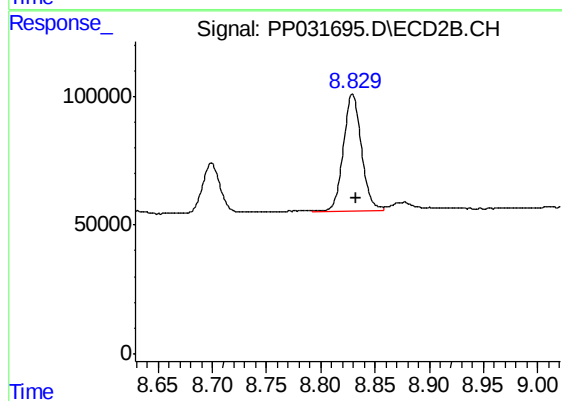

#44 AR-1268-4


R.T.: 8.829 min
Delta R.T.: -0.003 min
Response: 524682
Conc: 287.86 ng/ml

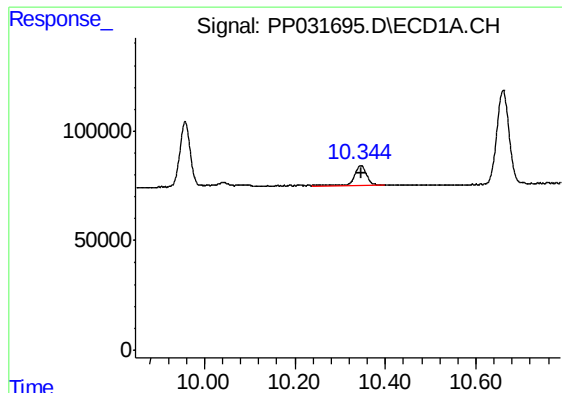

#45 AR-1268-5

R.T.: 10.346 min
Delta R.T.: -0.002 min
Response: 172837
Conc: 14.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-0-2MSD

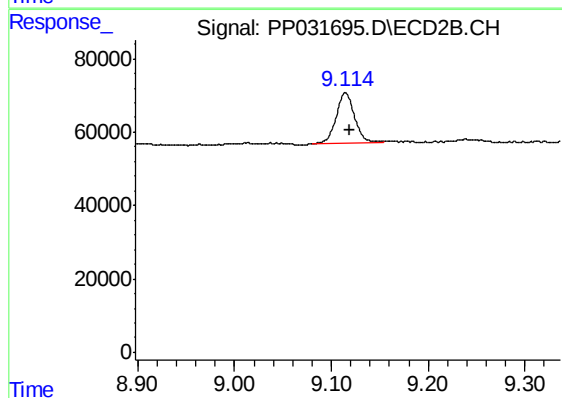

#45 AR-1268-5

R.T.: 9.114 min
Delta R.T.: -0.005 min
Response: 183345
Conc: 13.24 ng/ml