

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
 Data File : PP031696.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 18:05
 Operator : DD\AJ
 Sample : L4880-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-B4-112320-6-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:46:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.789	4.061	1162638	1103812	24.010	23.035
2)	SA Decachlor...	10.661	9.364	719598	790957	21.187	21.361
Target Compounds							
7)	L1 AR-1016-5	0.000	5.795f	0	9177	N.D.	8.068 #
9)	L2 AR-1221-2	0.000	4.414	0	13218	N.D.	34.266 #
15)	L3 AR-1232-5	0.000	5.795	0	9177	N.D.	31.667 #
20)	L4 AR-1242-5	0.000	6.203	0	1965	N.D.	1.905 #
24)	L5 AR-1248-4	0.000	5.795f	0	9177	N.D.	5.990 #
26)	L6 AR-1254-1	0.000	6.203	0	1965	N.D.	0.909 #
30)	L6 AR-1254-5	0.000	7.434	0	6254	N.D.	2.317 #
32)	L7 AR-1260-2	0.000	7.074f	0	2431	N.D.	0.998 #
33)	L7 AR-1260-3	0.000	7.260	0	3329	N.D.	1.458 #
34)	L7 AR-1260-4	0.000	7.743	0	13720	N.D.	7.220 #
35)	L7 AR-1260-5	0.000	7.977	0	22631	N.D.	4.987 #
36)	L8 AR-1262-1	0.000	7.475	0	5278	N.D.	1.899 #
37)	L8 AR-1262-2	0.000	7.977	0	22631	N.D.	4.659 #
38)	L8 AR-1262-3	0.000	8.275	0	6254	N.D.	3.179 #
39)	L8 AR-1262-4	0.000	8.338	0	10301	N.D.	2.842 #
40)	L8 AR-1262-5	0.000	8.831	0	7818	N.D.	4.817 #
41)	L9 AR-1268-1	0.000	8.275	0	6254	N.D.	1.130 #
42)	L9 AR-1268-2	0.000	8.338	0	10301	N.D.	1.905 #
43)	L9 AR-1268-3	0.000	8.535	0	2195	N.D.	0.479 #
44)	L9 AR-1268-4	0.000	8.831	0	7818	N.D.	4.289 #
45)	L9 AR-1268-5	0.000	9.118	0	6384	N.D.	0.461 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112520\
Data File : PP031696.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 18:05
Operator : DD\AJ
Sample : L4880-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:46:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

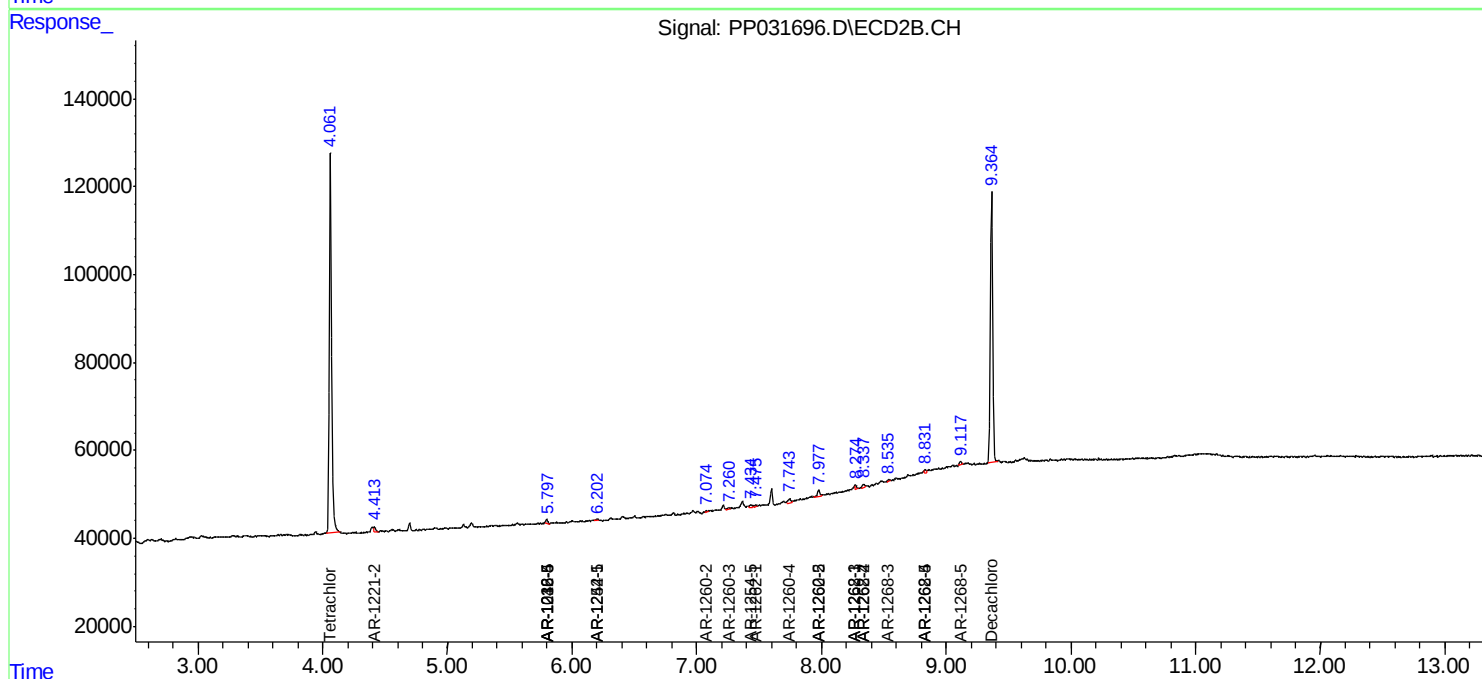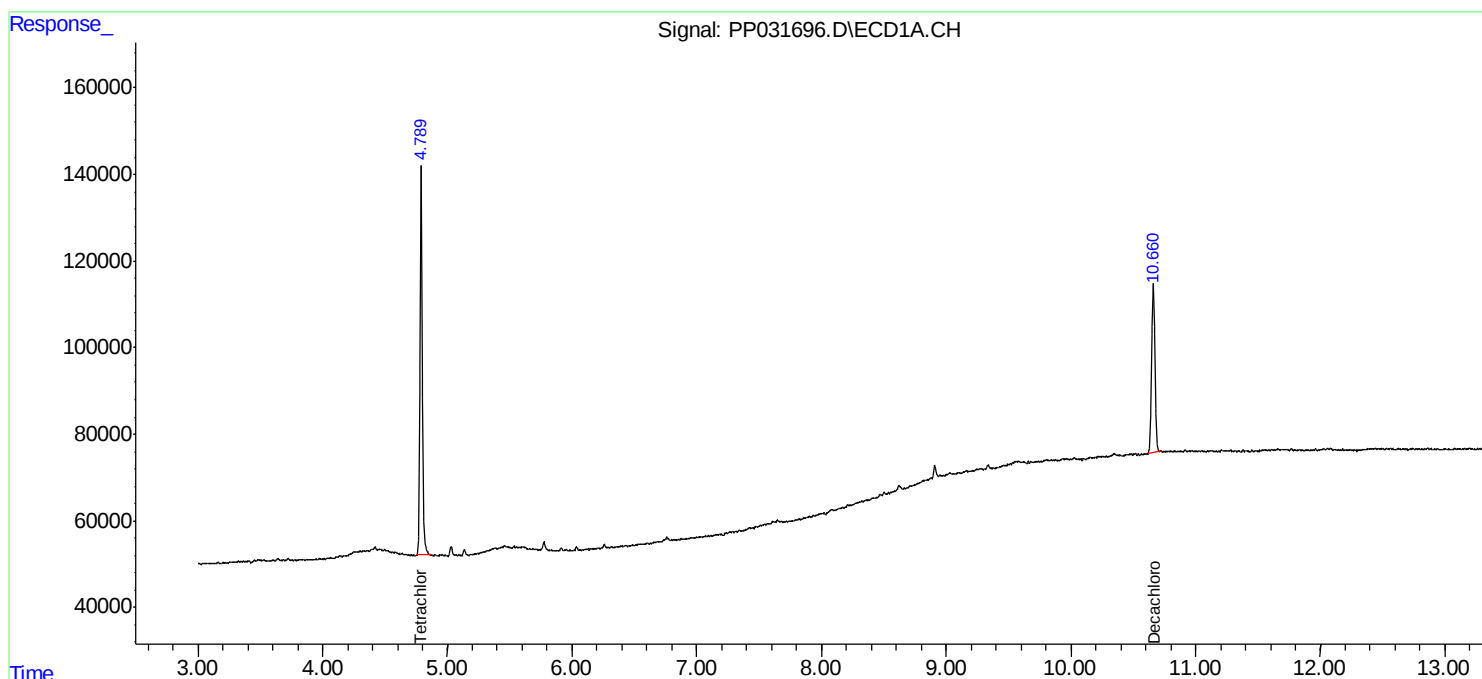


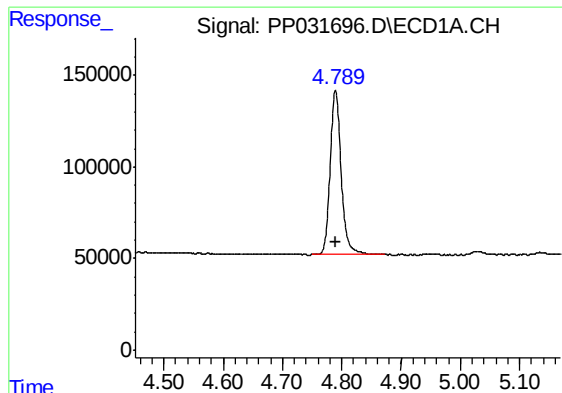

#1 Tetrachloro-m-xylene


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 1162638
Conc: 24.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

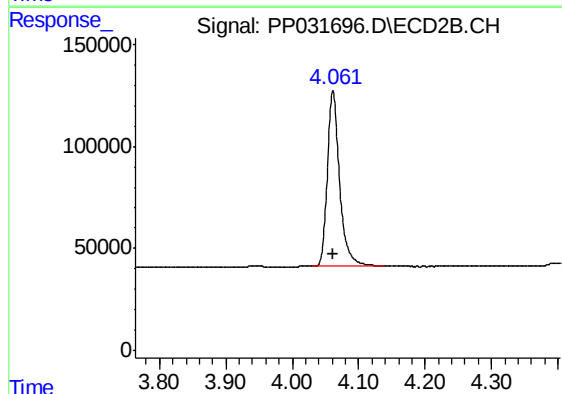


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1103812
Conc: 23.04 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.004 min
Response: 719598
Conc: 21.19 ng/ml

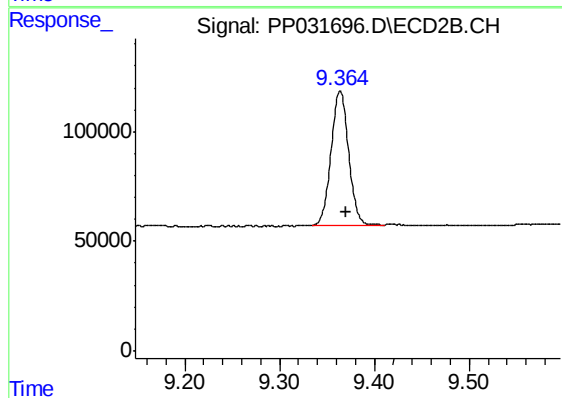

#2 Decachlorobiphenyl


R.T.: 9.364 min
Delta R.T.: -0.006 min
Response: 790957
Conc: 21.36 ng/ml

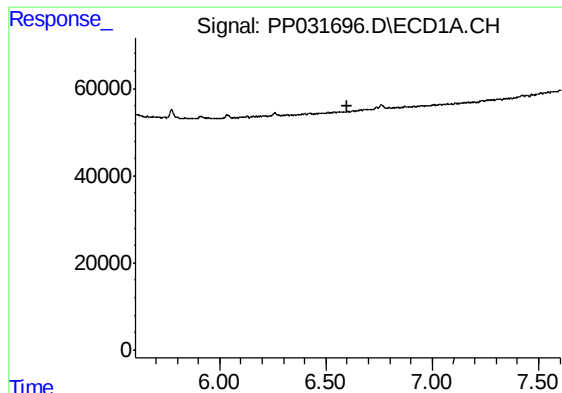

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

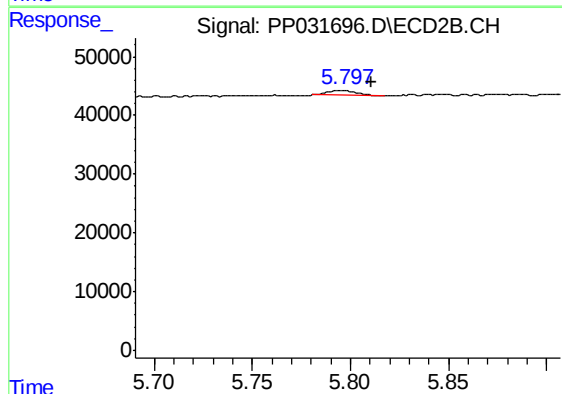


#7 AR-1016-5

R.T.: 5.795 min
Delta R.T.: -0.016 min
Response: 9177
Conc: 8.07 ng/ml

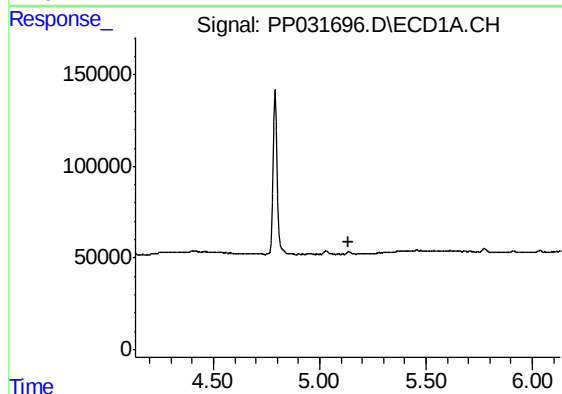


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

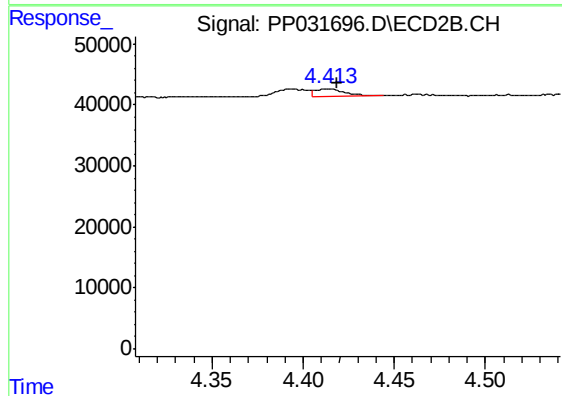

#9 AR-1221-2


R.T.: 4.414 min
Delta R.T.: -0.005 min
Response: 13218
Conc: 34.27 ng/ml

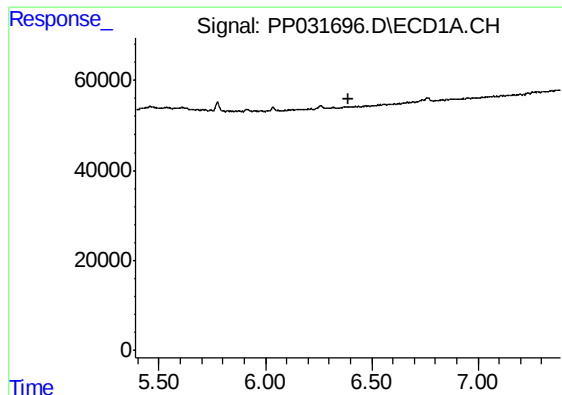

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

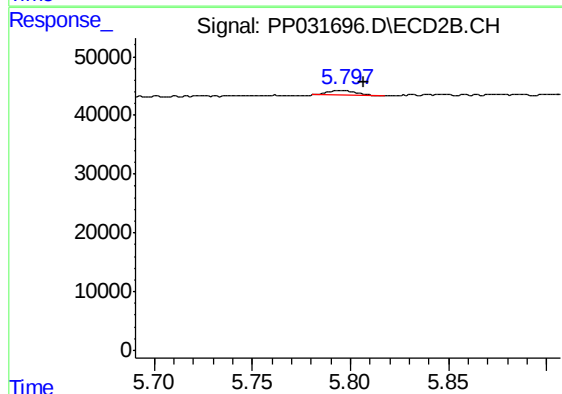


#15 AR-1232-5

R.T.: 5.795 min
Delta R.T.: -0.013 min
Response: 9177
Conc: 31.67 ng/ml

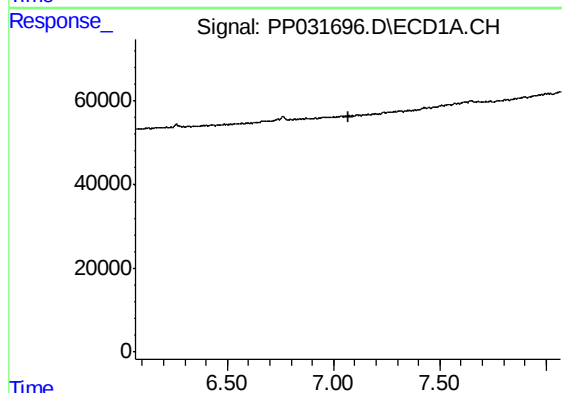


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

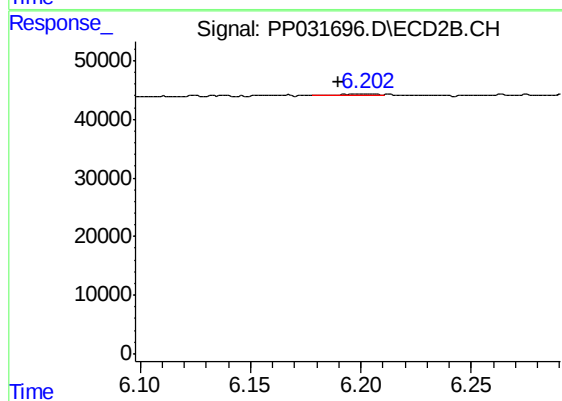

#20 AR-1242-5


R.T.: 6.203 min
Delta R.T.: 0.013 min
Response: 1965
Conc: 1.90 ng/ml

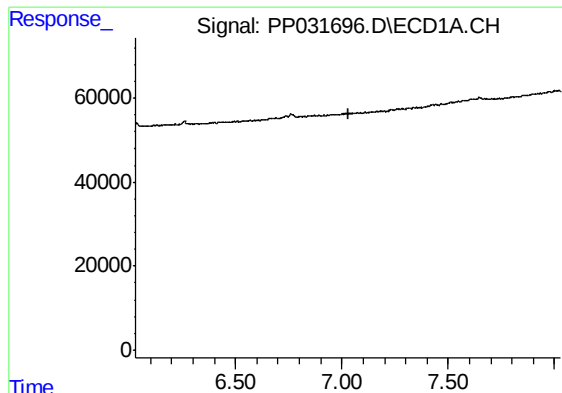

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

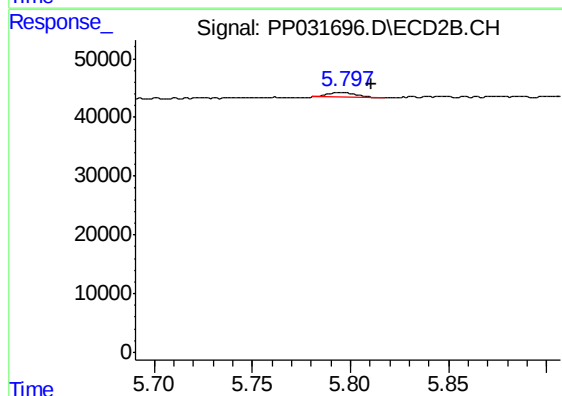


#24 AR-1248-4

R.T.: 5.795 min
Delta R.T.: -0.016 min
Response: 9177
Conc: 5.99 ng/ml

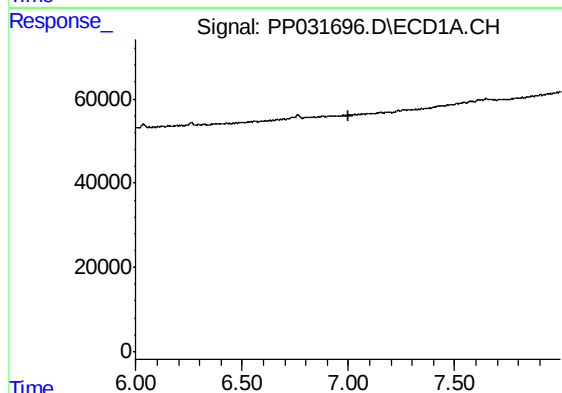


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

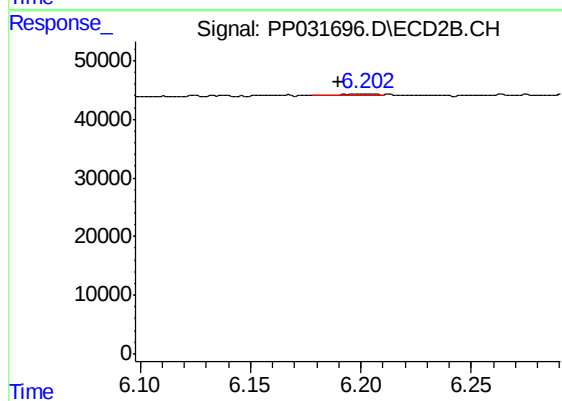

#26 AR-1254-1


R.T.: 6.203 min
Delta R.T.: 0.012 min
Response: 1965
Conc: 0.91 ng/ml

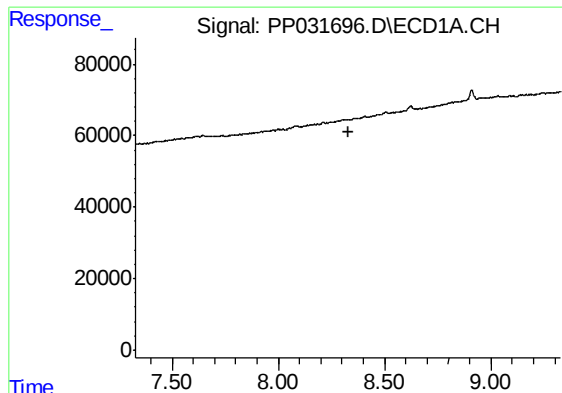

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 8.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

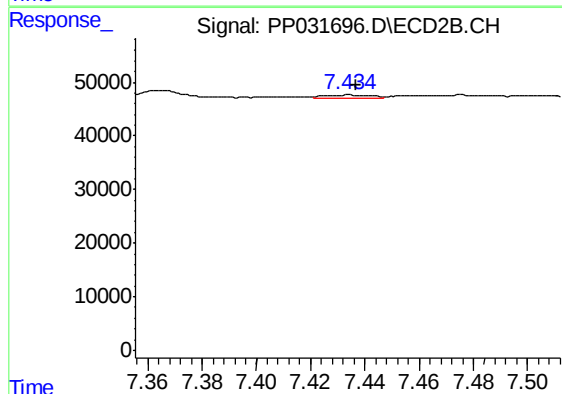


#30 AR-1254-5

R.T.: 7.434 min
Delta R.T.: -0.003 min
Response: 6254
Conc: 2.32 ng/ml




#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

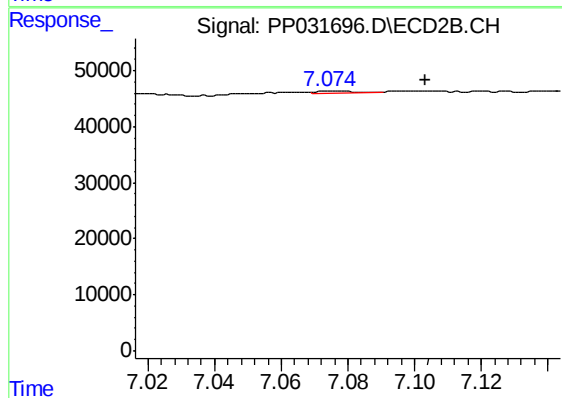

#32 AR-1260-2


R.T.: 7.074 min
Delta R.T.: -0.029 min
Response: 2431
Conc: 1.00 ng/ml



#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 8.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

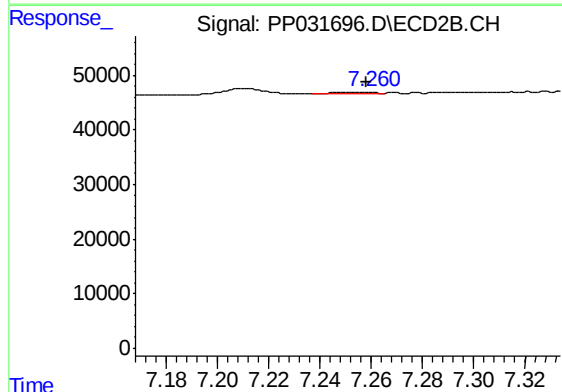


#33 AR-1260-3

R.T.: 7.260 min
Delta R.T.: 0.002 min
Response: 3329
Conc: 1.46 ng/ml

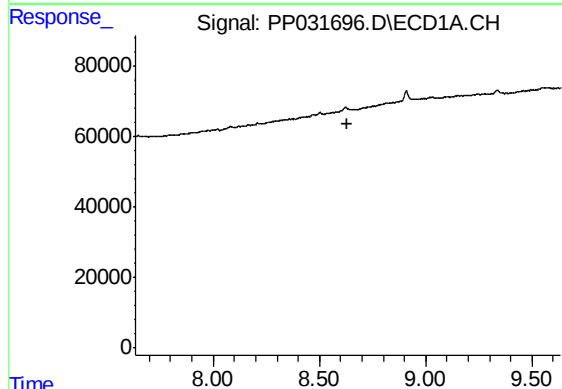


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.634 min
Response: 0
Conc: N.D.

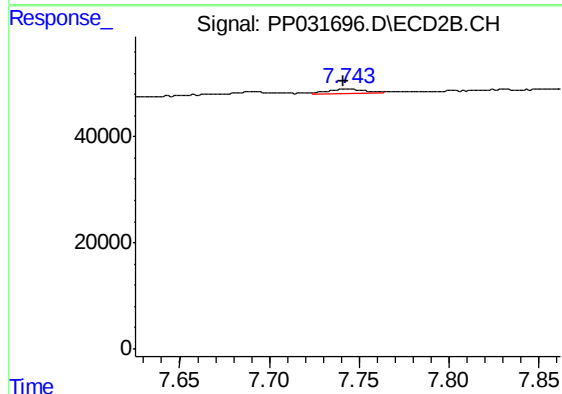

#34 AR-1260-4


R.T.: 7.743 min
Delta R.T.: 0.002 min
Response: 13720
Conc: 7.22 ng/ml

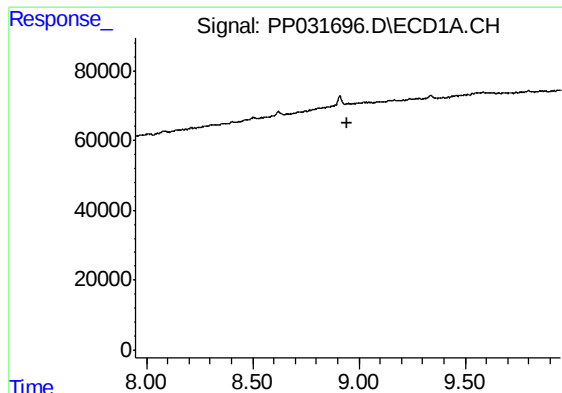

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

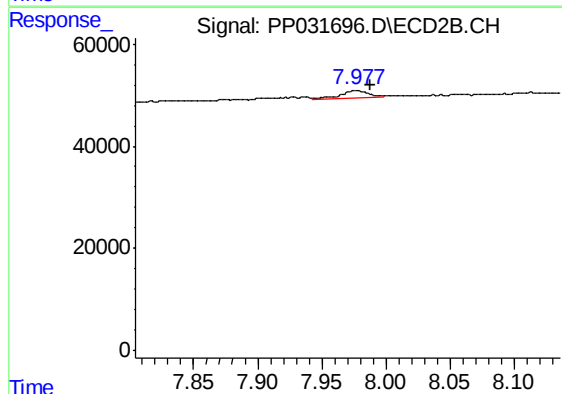


#35 AR-1260-5

R.T.: 7.977 min
Delta R.T.: -0.010 min
Response: 22631
Conc: 4.99 ng/ml




#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

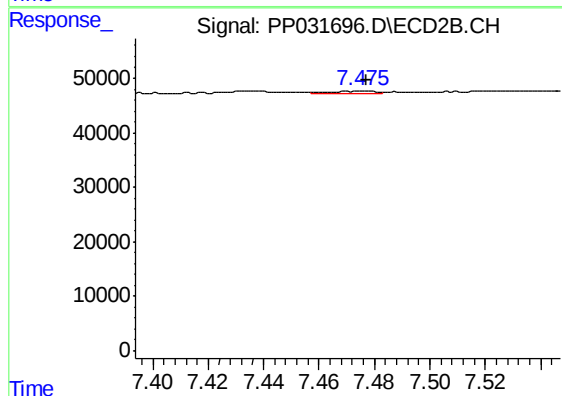

#36 AR-1262-1


R.T.: 7.475 min
Delta R.T.: -0.002 min
Response: 5278
Conc: 1.90 ng/ml



#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

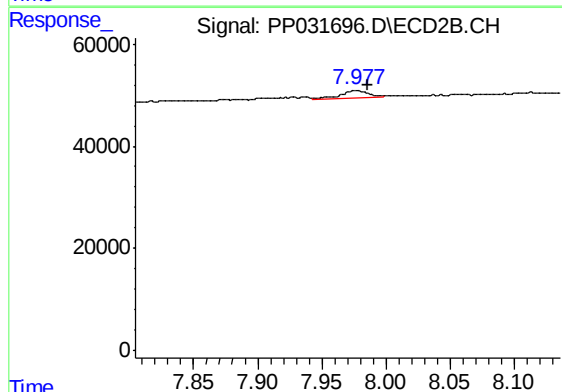


#37 AR-1262-2

R.T.: 7.977 min
Delta R.T.: -0.009 min
Response: 22631
Conc: 4.66 ng/ml




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

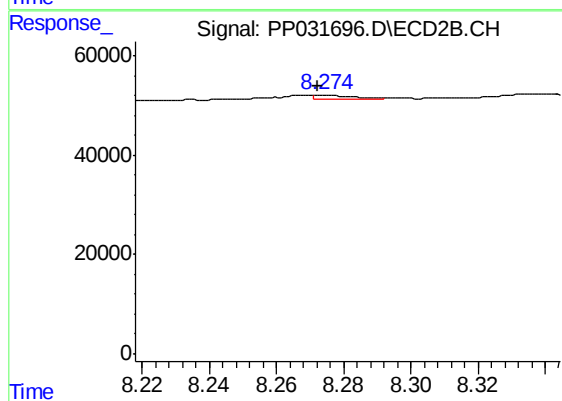

#38 AR-1262-3


R.T.: 8.275 min
Delta R.T.: 0.002 min
Response: 6254
Conc: 3.18 ng/ml



#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

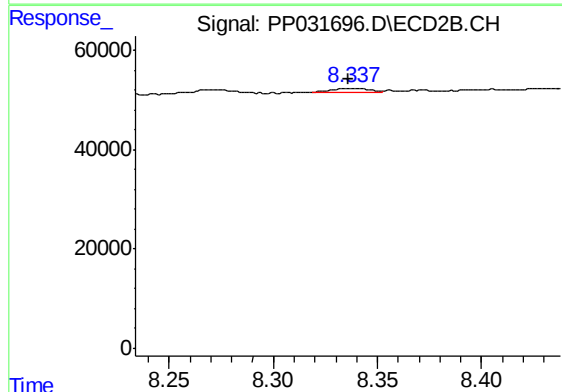


#39 AR-1262-4

R.T.: 8.338 min
Delta R.T.: 0.002 min
Response: 10301
Conc: 2.84 ng/ml

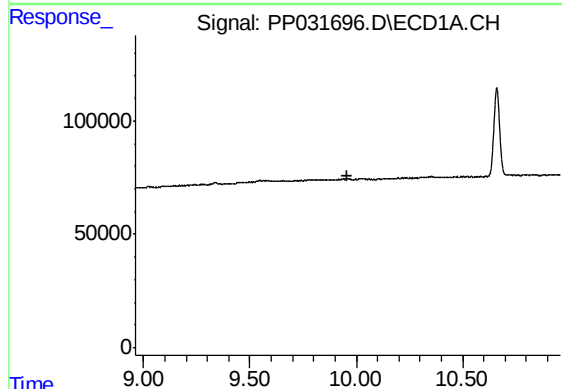


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

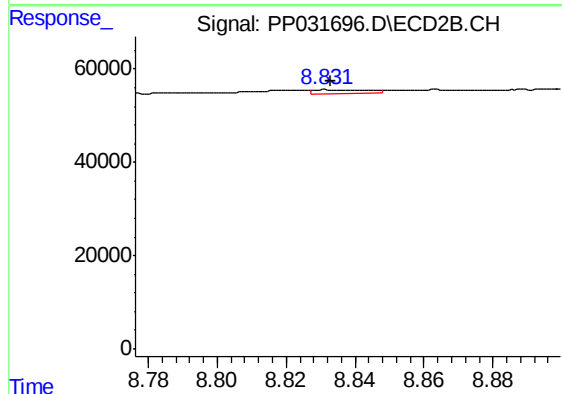

#40 AR-1262-5


R.T.: 8.831 min
Delta R.T.: -0.002 min
Response: 7818
Conc: 4.82 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

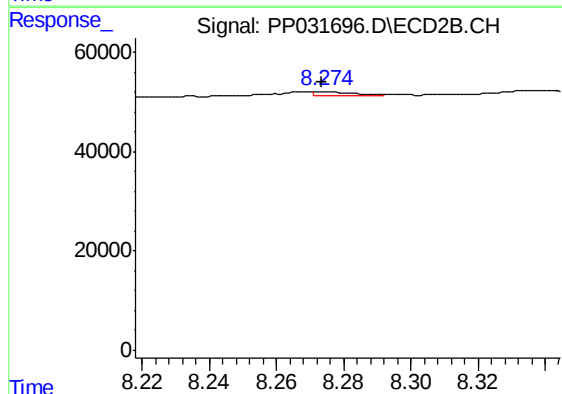


#41 AR-1268-1

R.T.: 8.275 min
Delta R.T.: 0.001 min
Response: 6254
Conc: 1.13 ng/ml




#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

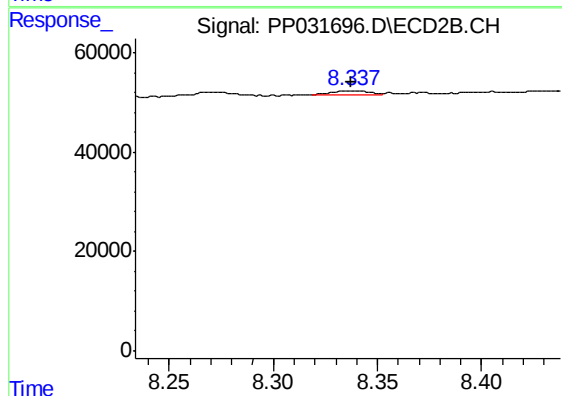

#42 AR-1268-2


R.T.: 8.338 min
Delta R.T.: 0.000 min
Response: 10301
Conc: 1.91 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 9.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

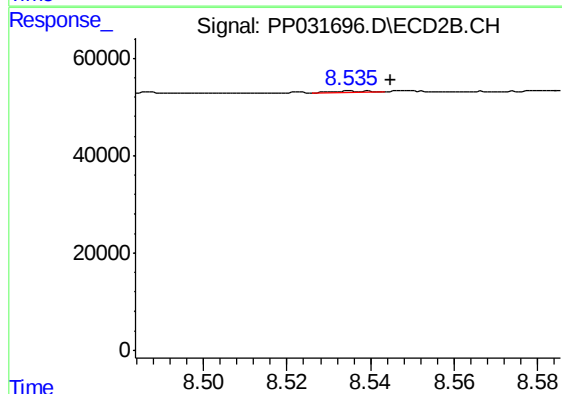


#43 AR-1268-3

R.T.: 8.535 min
Delta R.T.: -0.010 min
Response: 2195
Conc: 0.48 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

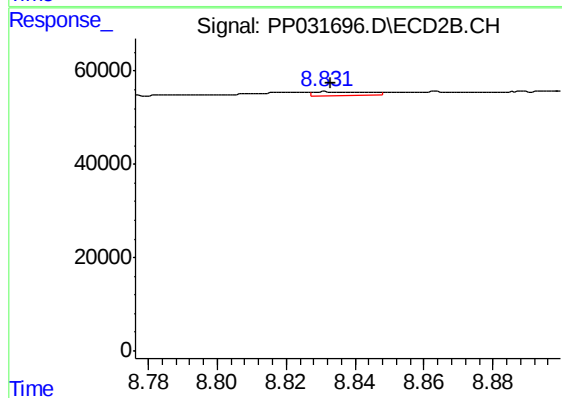

#44 AR-1268-4


R.T.: 8.831 min
Delta R.T.: -0.002 min
Response: 7818
Conc: 4.29 ng/ml

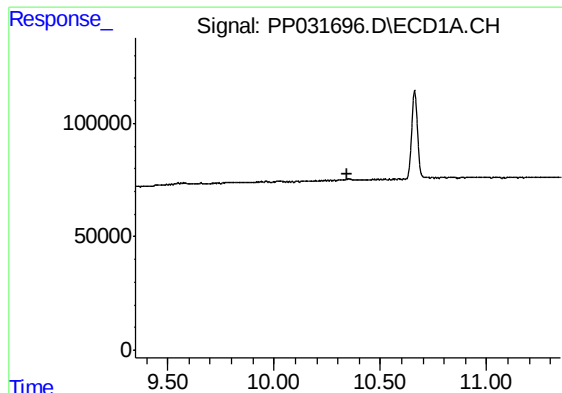

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-B4-112320-6-8

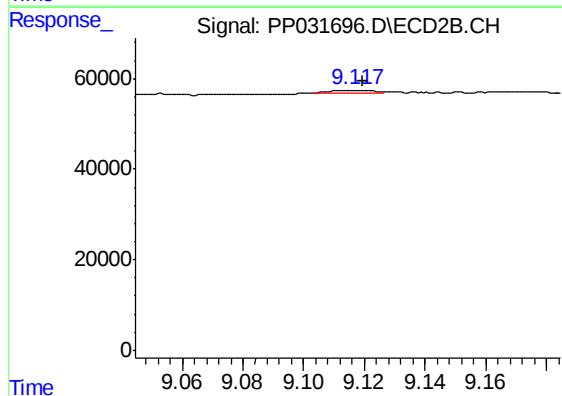

#45 AR-1268-5

R.T.: 9.118 min
Delta R.T.: -0.002 min
Response: 6384
Conc: 0.46 ng/ml