

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112524\
 Data File : PP068681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 12:23
 Operator : YP\AJ
 Sample : PB165225BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB165225BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/26/2024
 Supervised By :Ankita Jodhani 11/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:14:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	4.049	18796469	18916873	19.366	19.536
2) SA Decachlor...	10.669	9.202	26856092	24950560	21.459	22.057m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112524\
Data File : PP068681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 12:23
Operator : YP\AJ
Sample : PB165225BL
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB165225BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/26/2024
Supervised By :Ankita Jodhani 11/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:14:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

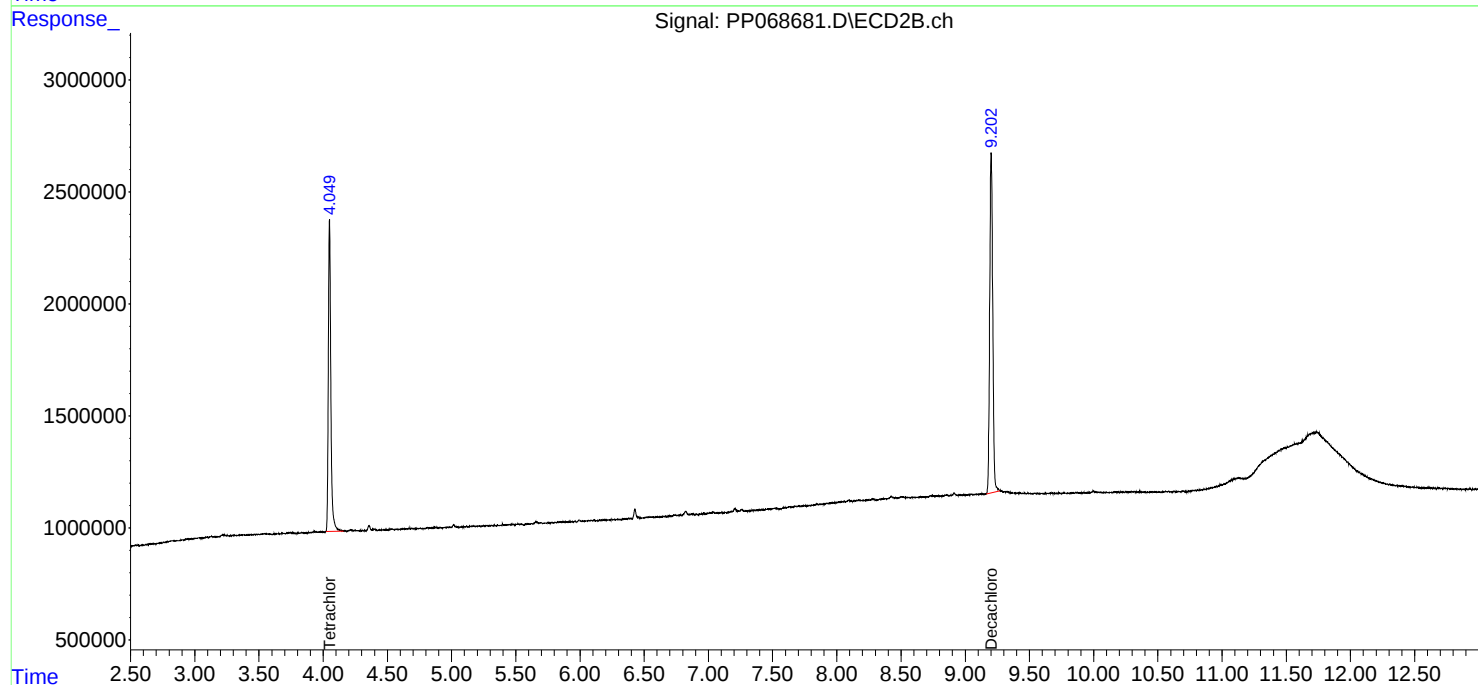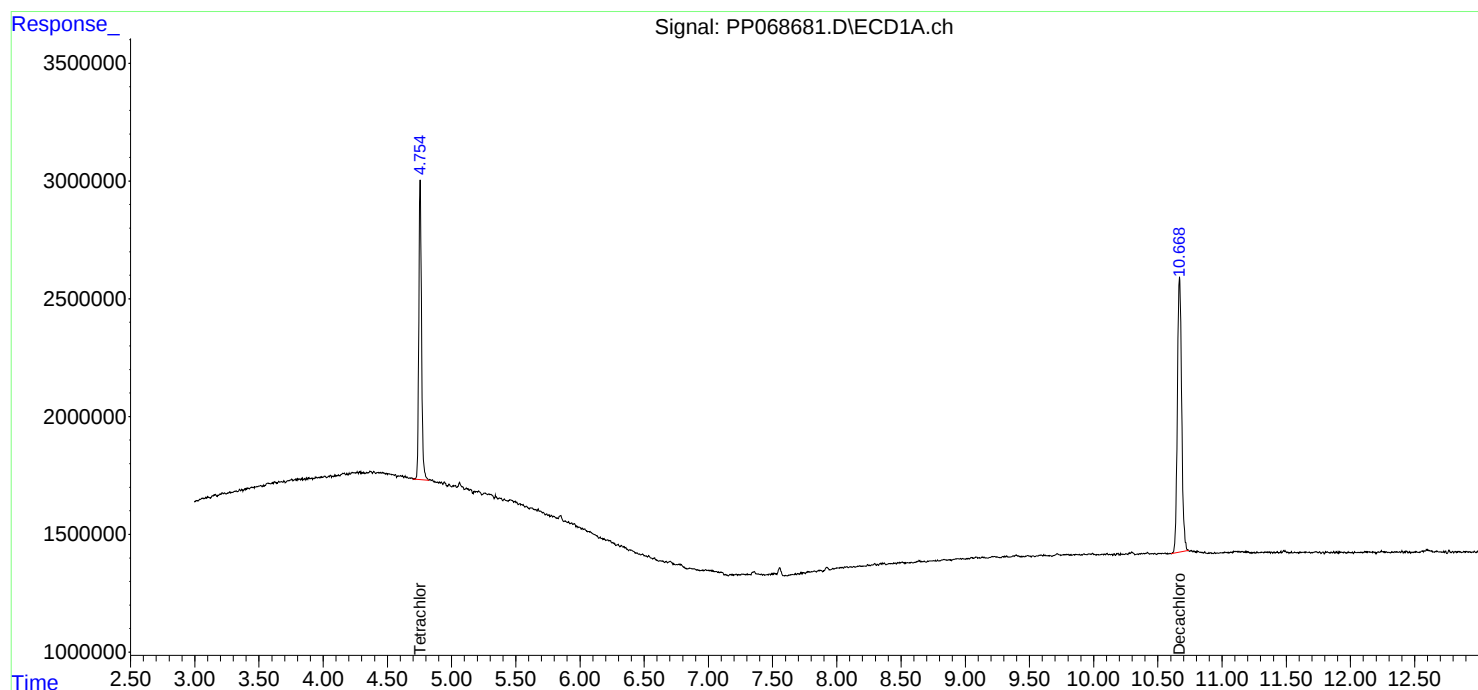

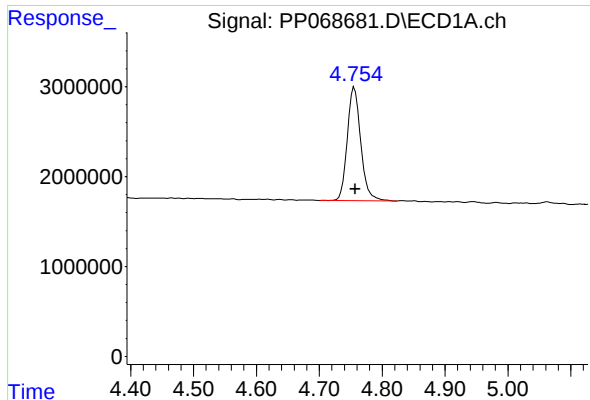


#1 Tetrachloro-m-xylene

R.T.: 4.756 min
Delta R.T.: -0.001 min
Response: 18796469
Conc: 19.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB165225BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/26/2024
Supervised By :Ankita Jodhani 11/26/2024

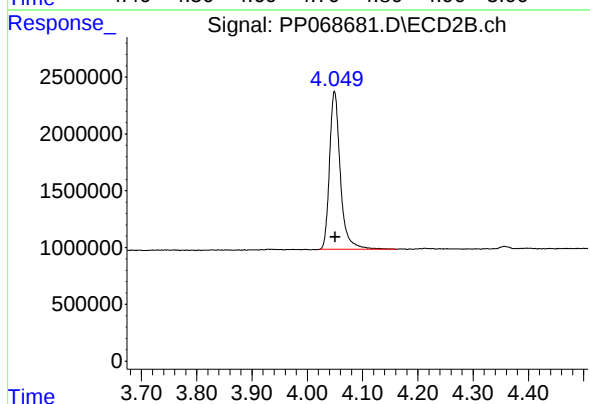


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.002 min
Response: 18916873
Conc: 19.54 ng/ml

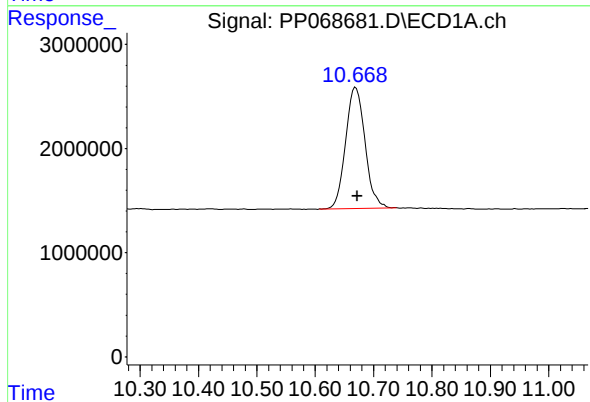

#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.003 min
Response: 26856092
Conc: 21.46 ng/ml

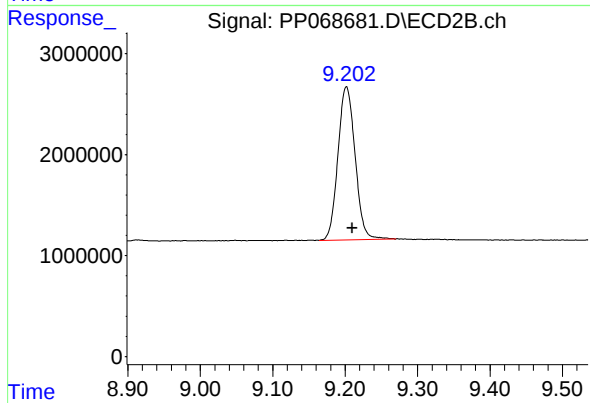

#2 Decachlorobiphenyl

R.T.: 9.202 min
Delta R.T.: -0.008 min
Response: 24950560
Conc: 22.06 ng/ml m