

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112524\
 Data File : PP068697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 21:30
 Operator : YP\AJ
 Sample : P4975-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01A-01B-01C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/26/2024
 Supervised By :Ankita Jodhani 11/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 23:08:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.758	4.047	18046973	17818040	18.593	18.402
2) SA Decachlor...	10.672	9.201	23918699	24848993	19.112	21.967m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112524\
Data File : PP068697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 21:30
Operator : YP\AJ
Sample : P4975-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

01A-01B-01C

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 11/26/2024

Supervised By :Ankita Jodhani 11/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 23:08:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

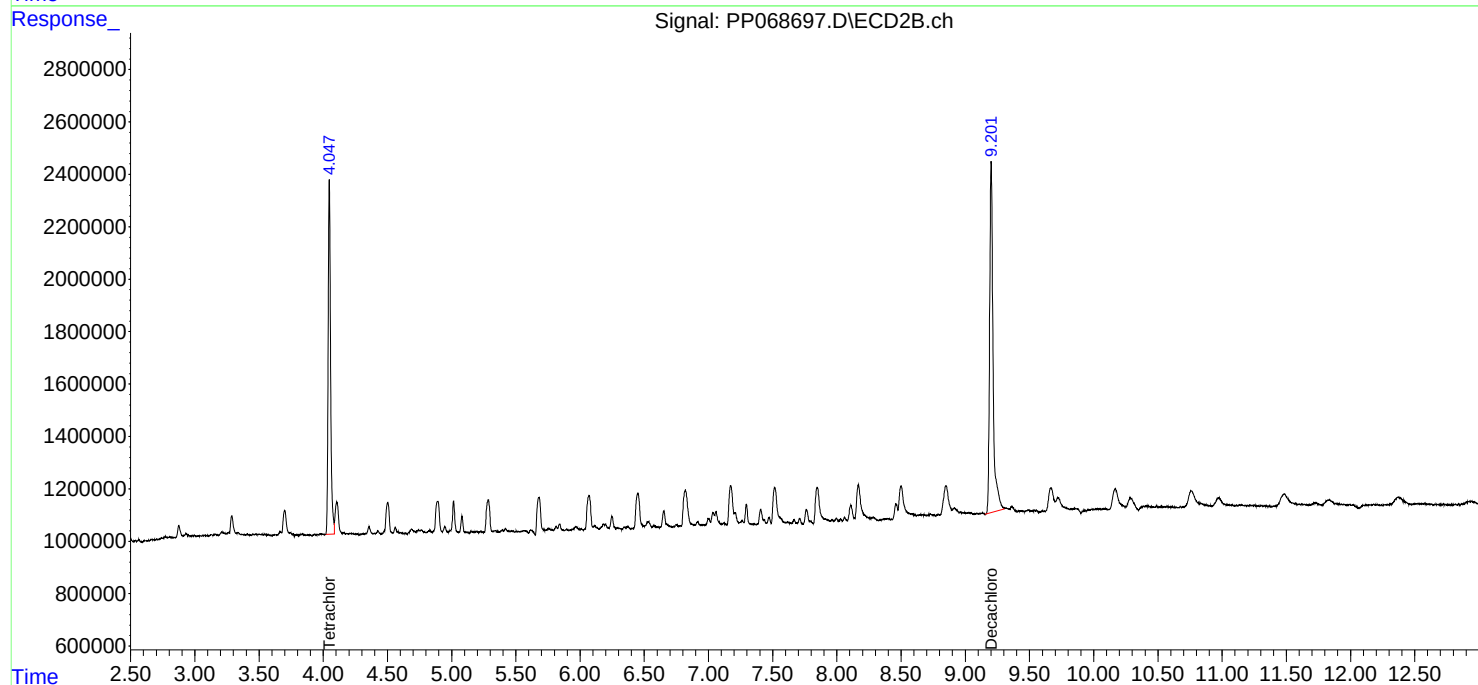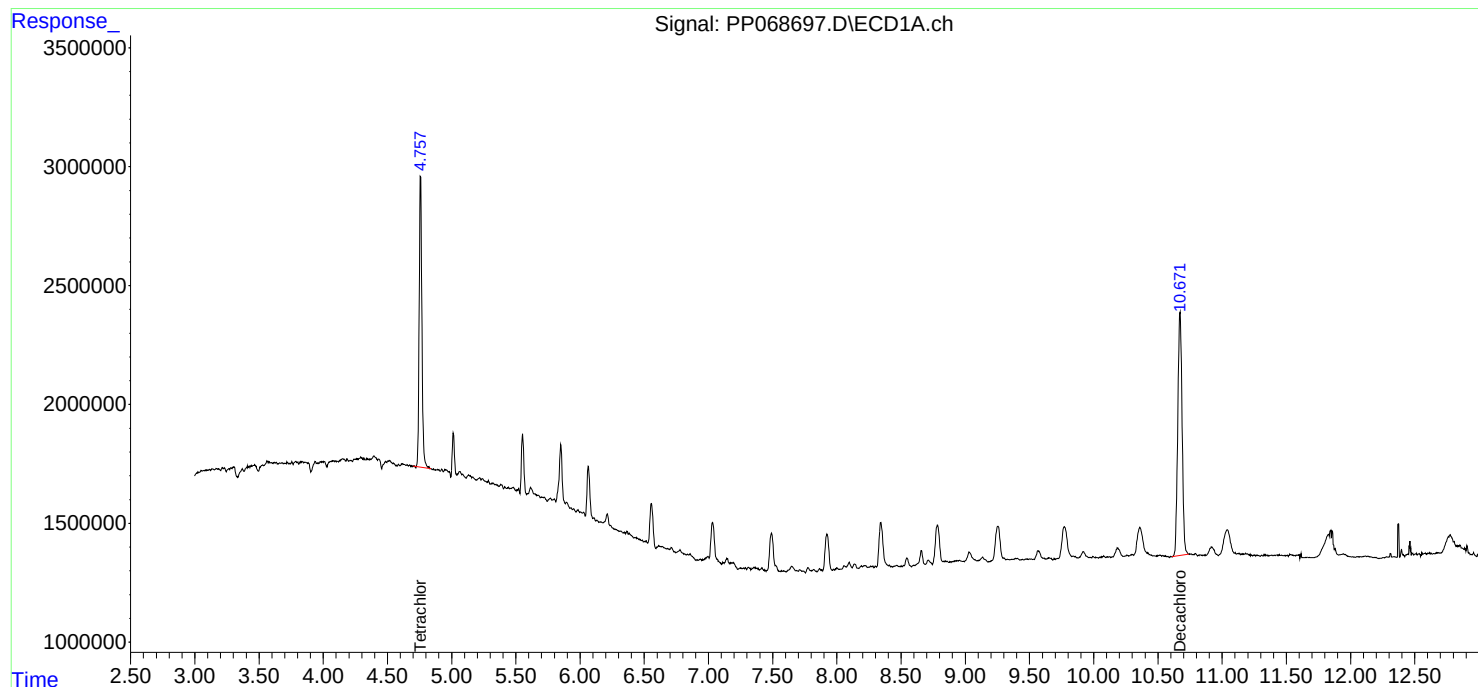

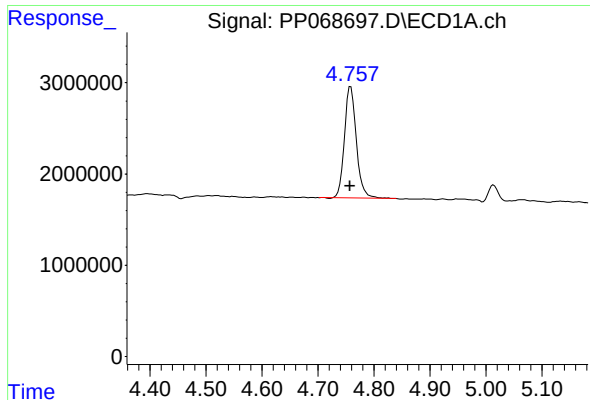


#1 Tetrachloro-m-xylene

R.T.: 4.758 min
Delta R.T.: 0.001 min
Response: 18046973
Conc: 18.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
01A-01B-01C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/26/2024
Supervised By :Ankita Jodhani 11/26/2024

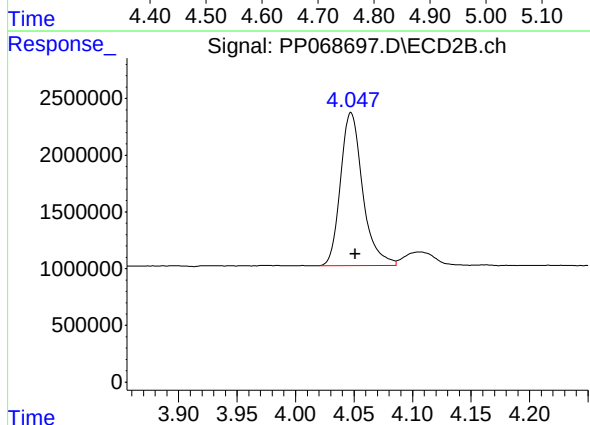


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: -0.004 min
Response: 17818040
Conc: 18.40 ng/ml

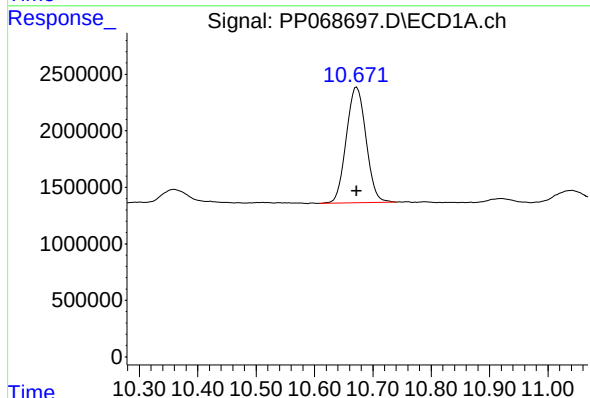

#2 Decachlorobiphenyl

R.T.: 10.672 min
Delta R.T.: 0.000 min
Response: 23918699
Conc: 19.11 ng/ml

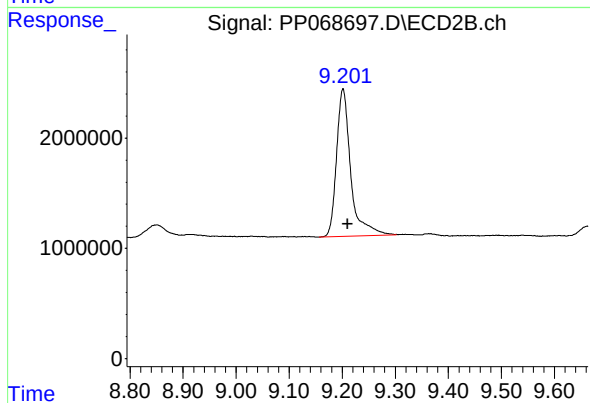

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.009 min
Response: 24848993
Conc: 21.97 ng/ml m