

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112621\
 Data File : PP041361.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Nov 2021 11:51
 Operator : AJ\MA
 Sample : M4841-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 16991

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 23:14:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	3.757	501564	741265	23.784	26.673
2) SA Decachlor...	10.660	9.020	511568	361280	23.419	25.202

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112621\
Data File : PP041361.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Nov 2021 11:51
Operator : AJ\MA
Sample : M4841-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
16991

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 23:14:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

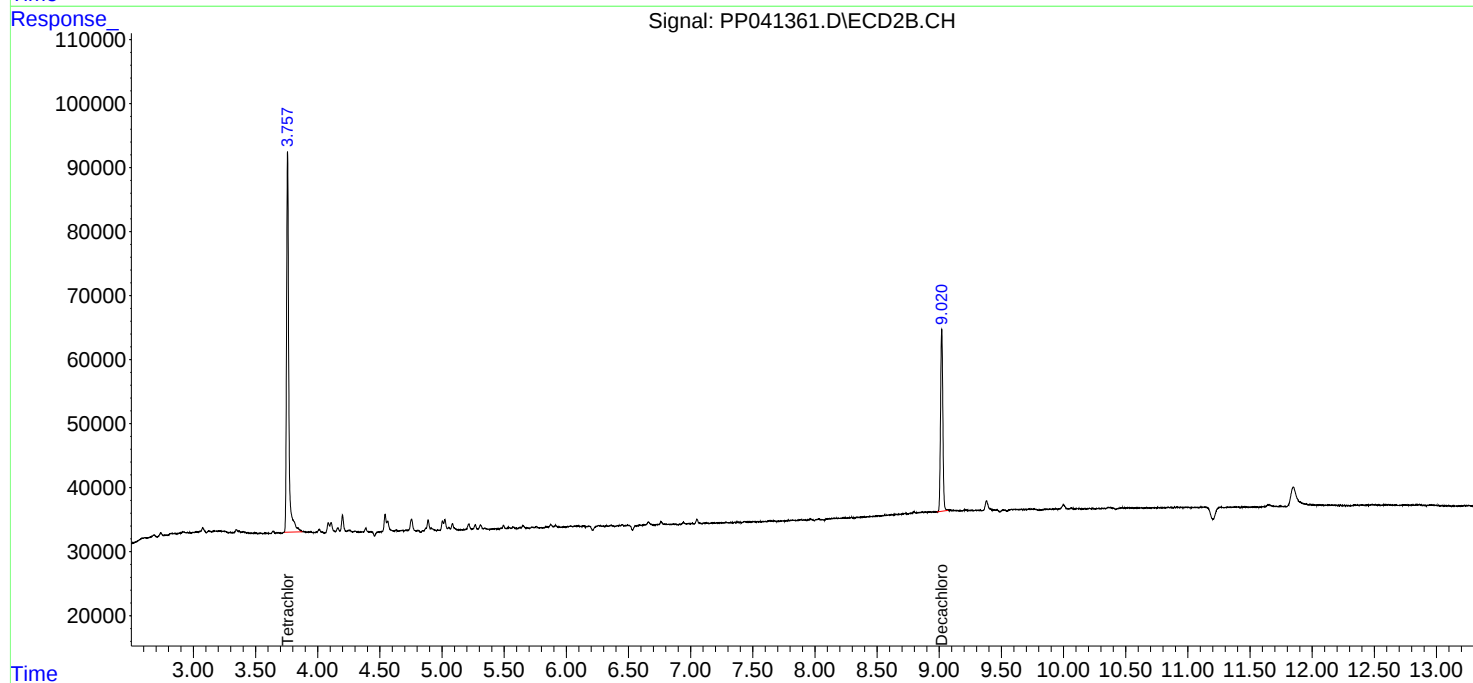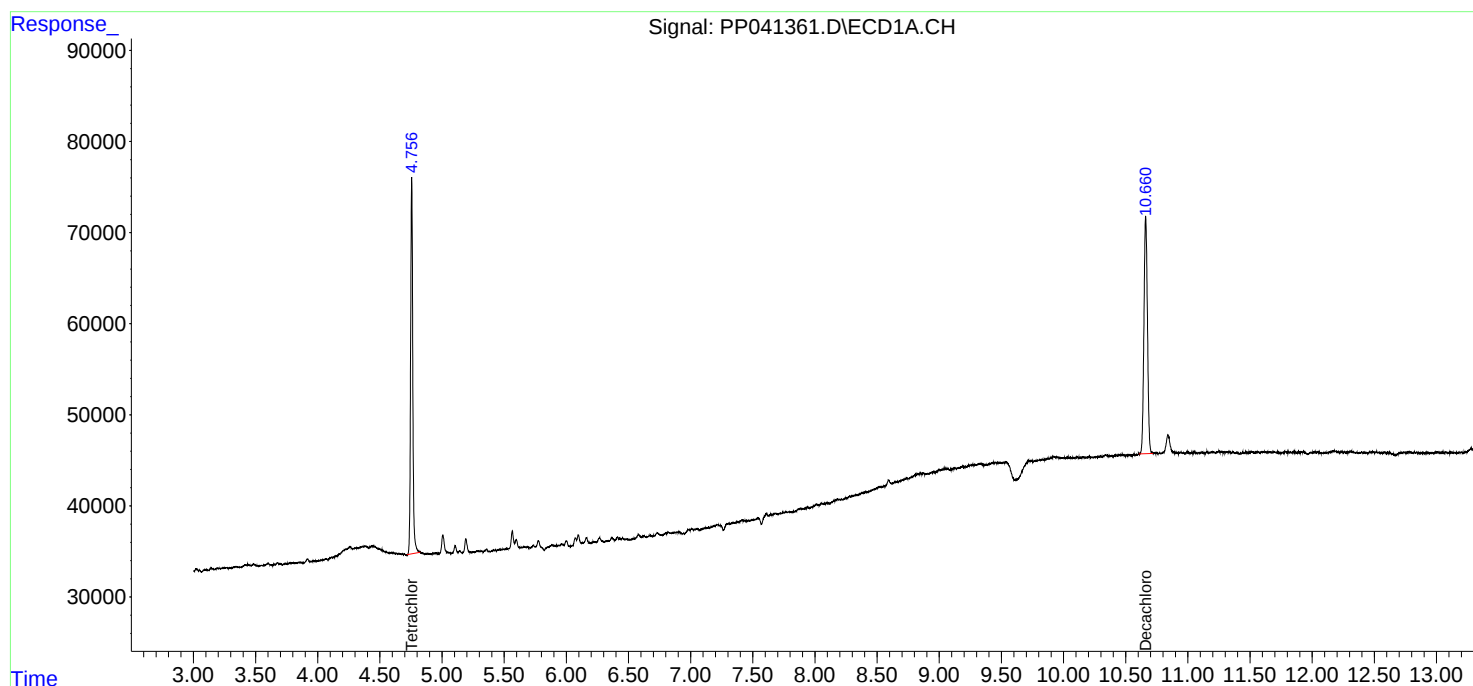


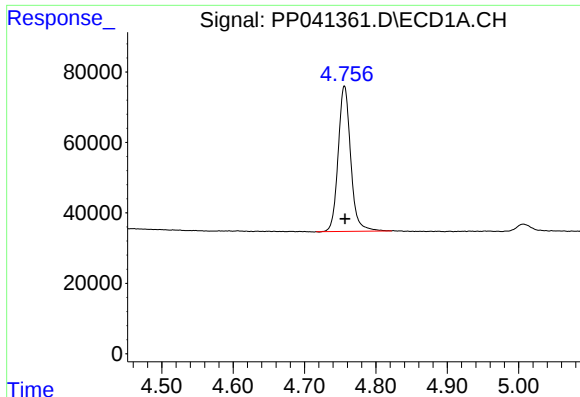

#1 Tetrachloro-m-xylene


R.T.: 4.756 min
Delta R.T.: -0.001 min
Response: 501564
Conc: 23.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
16991

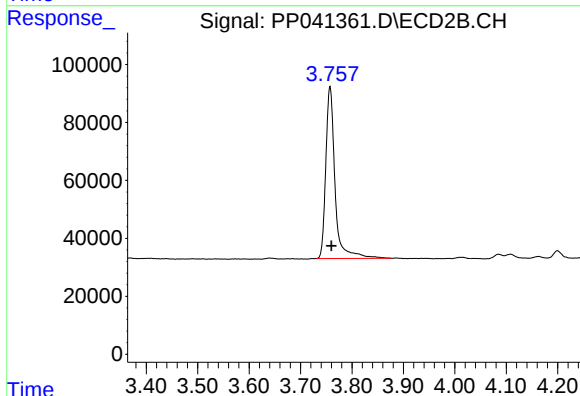


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.003 min
Response: 741265
Conc: 26.67 ng/ml

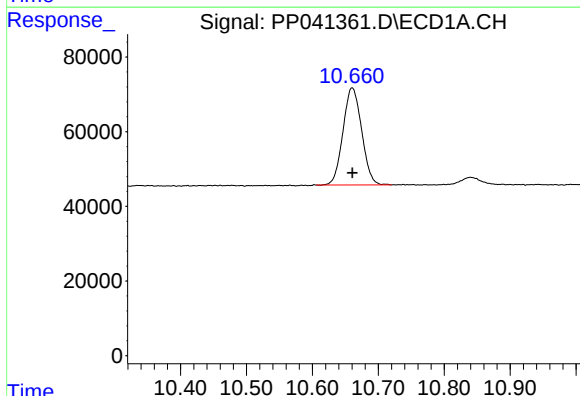

#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: 0.000 min
Response: 511568
Conc: 23.42 ng/ml

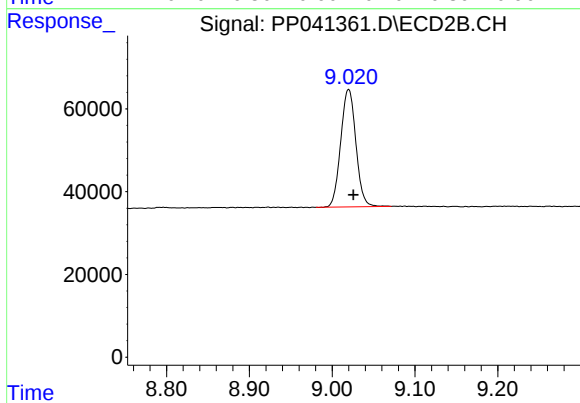

#2 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: -0.006 min
Response: 361280
Conc: 25.20 ng/ml