

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112923\
 Data File : PP061960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 10:22
 Operator : YP\AJ
 Sample : PB157428BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 12:25:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.452	3.724	26797181	36490772	20.356	20.280
2)	SA Decachlor...	10.241	8.848	23892095	45543023	23.151	22.066
Target Compounds							
7)	L1 AR-1016-5	0.000	5.297	0	20945	N.D.	0.362 #
9)	L2 AR-1221-2	4.759	4.032	378743	569076	28.399	29.918
15)	L3 AR-1232-5	0.000	5.297	0	20945	N.D.	0.823 #
20)	L4 AR-1242-5	0.000	5.681f	0	300906	N.D.	5.750 #
24)	L5 AR-1248-4	6.506	5.297	235454	20945	4.645	0.272 #
25)	L5 AR-1248-5	0.000	5.681f	0	300906	N.D.	3.011 #
26)	L6 AR-1254-1	6.506f	5.681f	235454	300906	4.197	2.764 #
32)	L7 AR-1260-2	0.000	6.521f	0	471370	N.D.	3.460 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP112923\
Data File : PP061960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 10:22
Operator : YP\AJ
Sample : PB157428BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 12:25:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

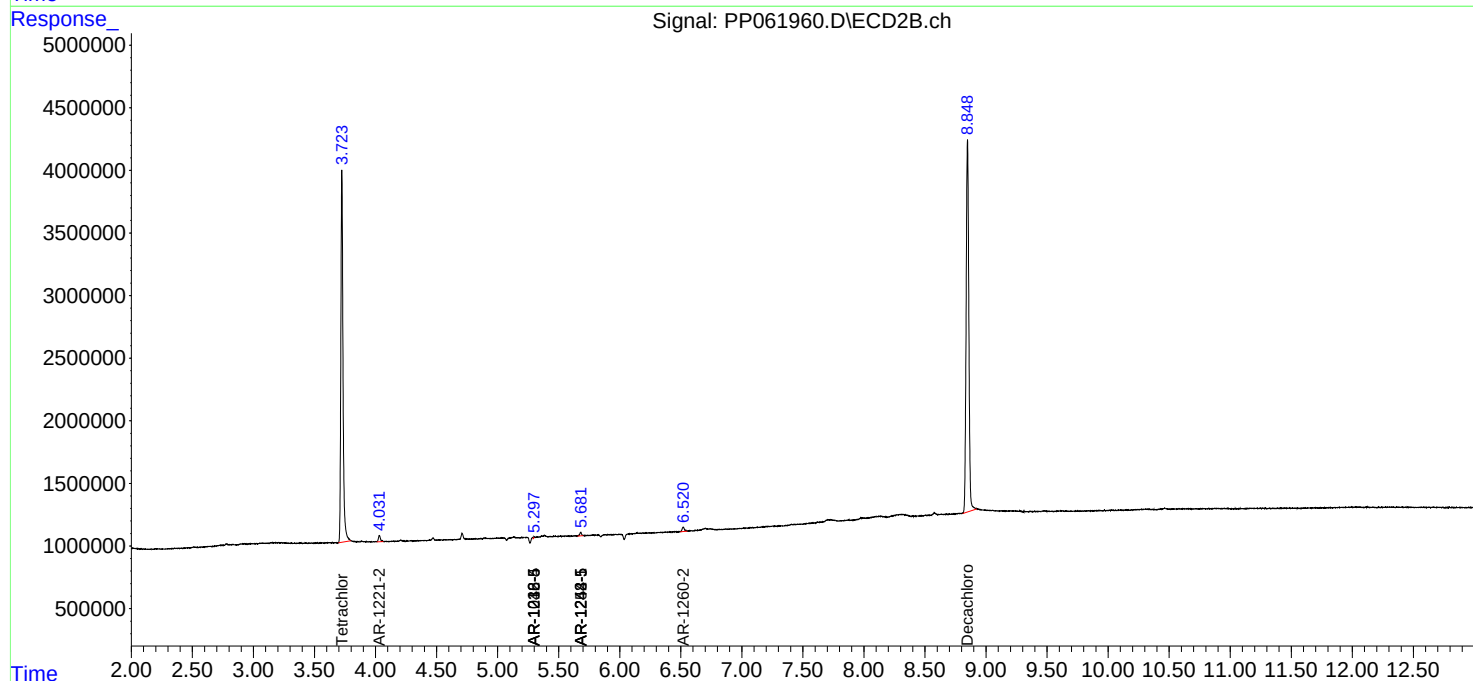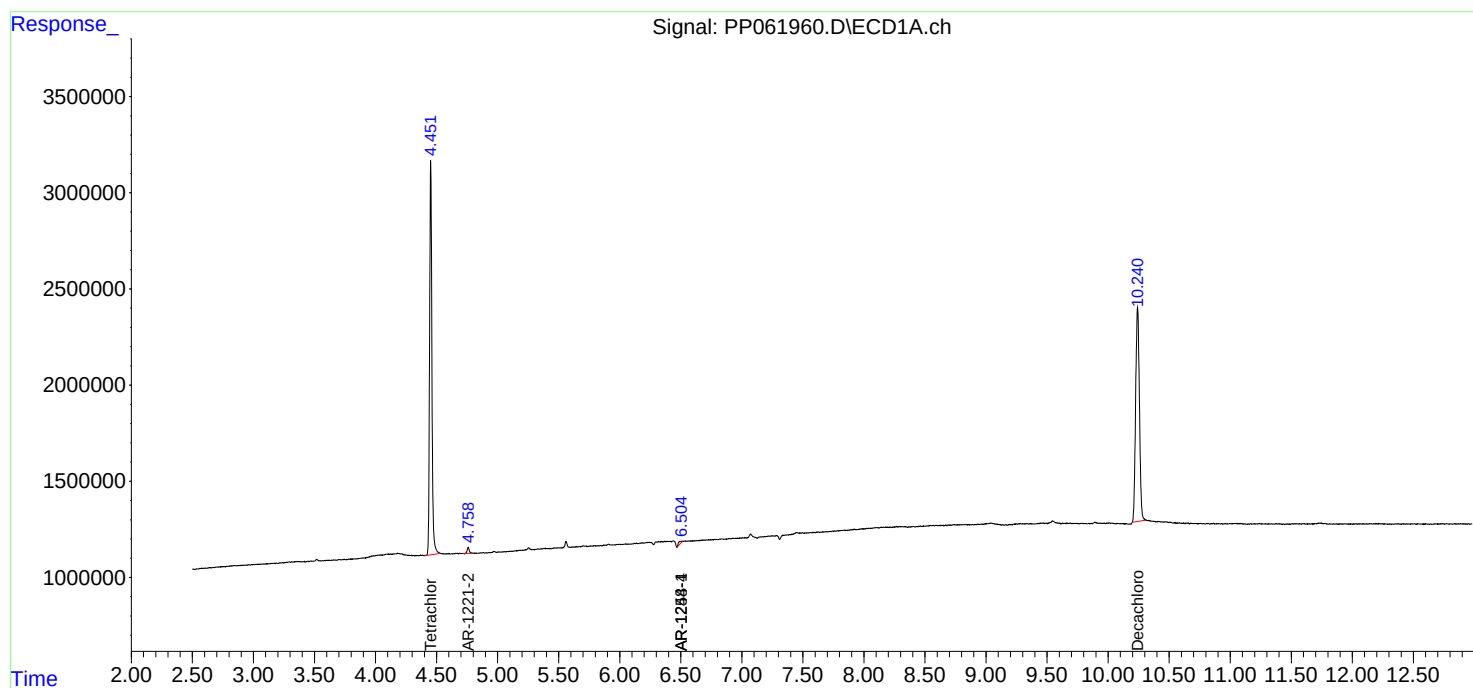


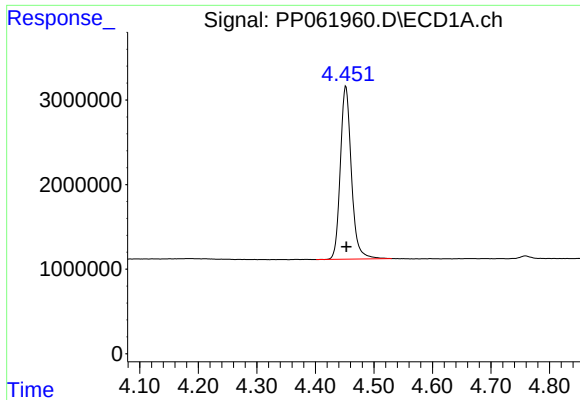

#1 Tetrachloro-m-xylene


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 26797181
Conc: 20.36 ng/ml

Instrument :
ECD_P
ClientSampleId :

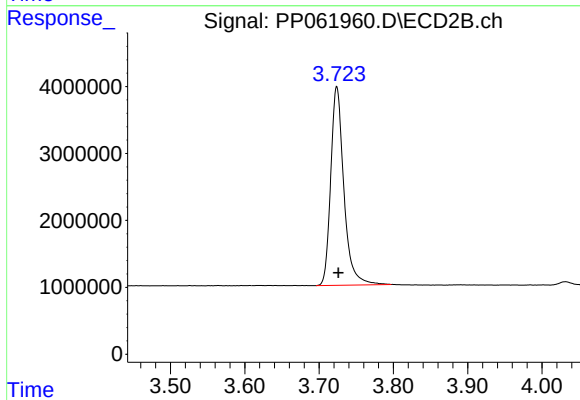


#1 Tetrachloro-m-xylene

R.T.: 3.724 min
Delta R.T.: -0.002 min
Response: 36490772
Conc: 20.28 ng/ml

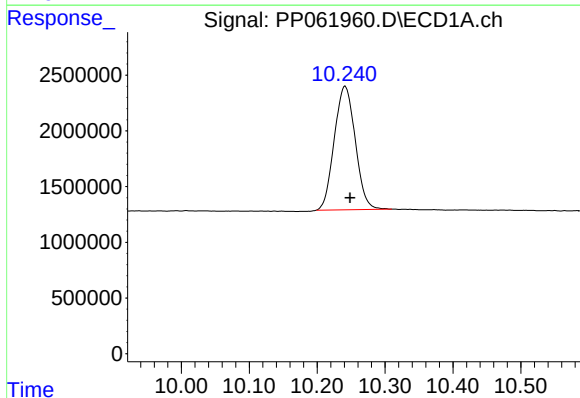


#2 Decachlorobiphenyl

R.T.: 10.241 min
Delta R.T.: -0.007 min
Response: 23892095
Conc: 23.15 ng/ml

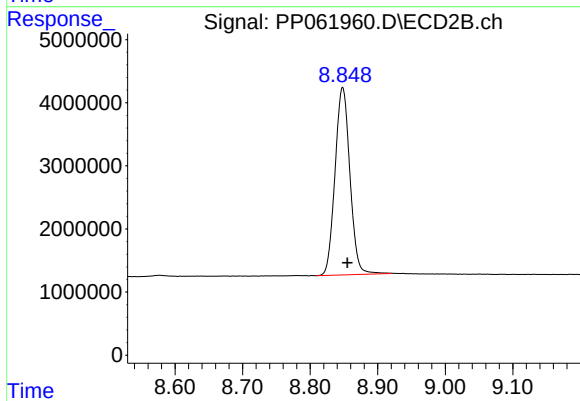

#2 Decachlorobiphenyl


R.T.: 8.848 min
Delta R.T.: -0.007 min
Response: 45543023
Conc: 22.07 ng/ml

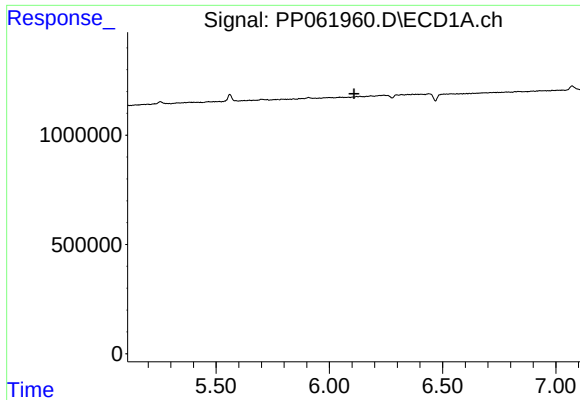

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

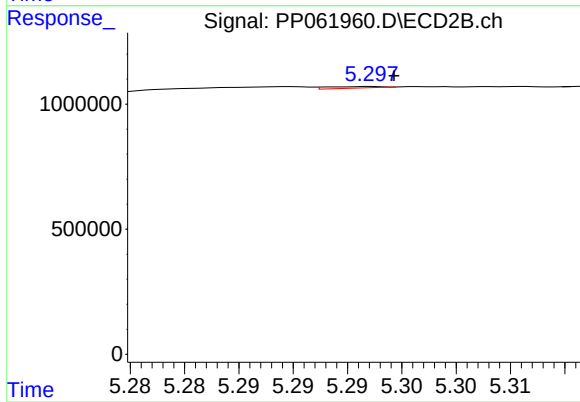


#7 AR-1016-5

R.T.: 5.297 min
Delta R.T.: -0.002 min
Response: 20945
Conc: 0.36 ng/ml

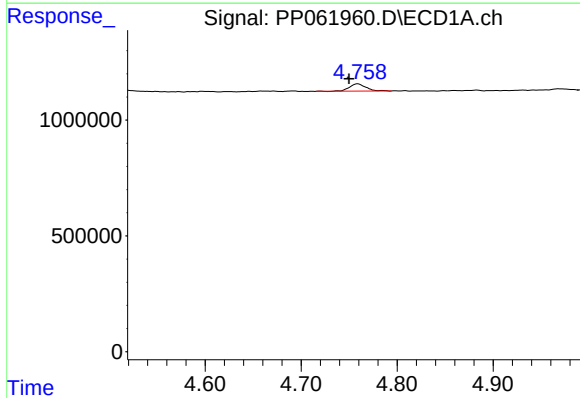


#9 AR-1221-2

R.T.: 4.759 min
Delta R.T.: 0.009 min
Response: 378743
Conc: 28.40 ng/ml

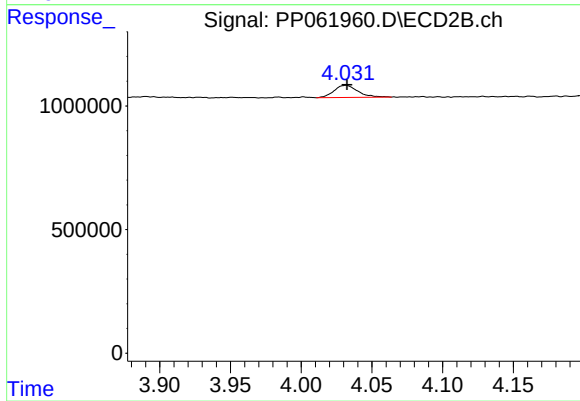

#9 AR-1221-2


R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 569076
Conc: 29.92 ng/ml

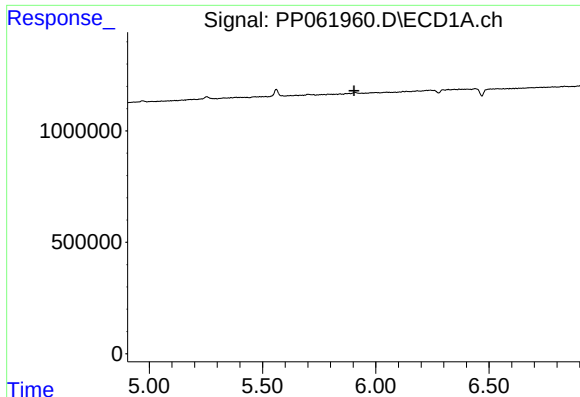

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

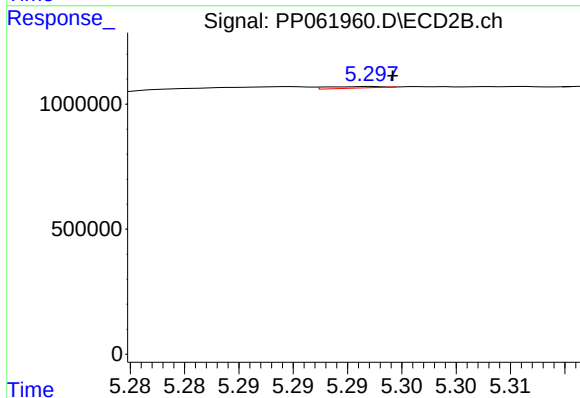


#15 AR-1232-5

R.T.: 5.297 min
Delta R.T.: -0.002 min
Response: 20945
Conc: 0.82 ng/ml

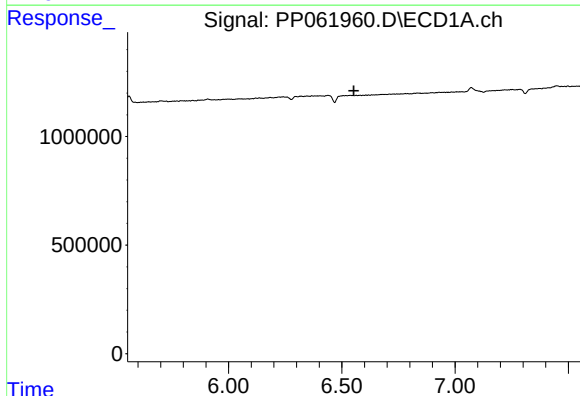


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.553 min
Response: 0
Conc: N.D.

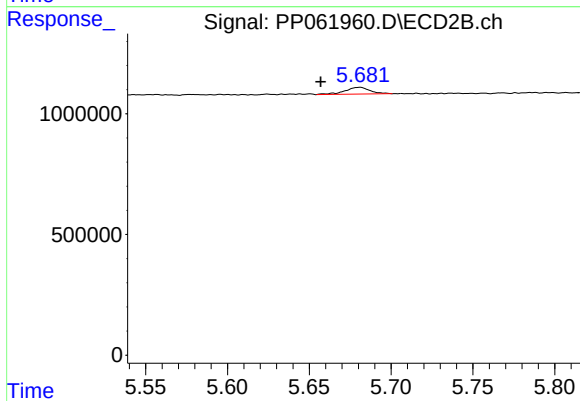

#20 AR-1242-5


R.T.: 5.681 min
Delta R.T.: 0.024 min
Response: 300906
Conc: 5.75 ng/ml

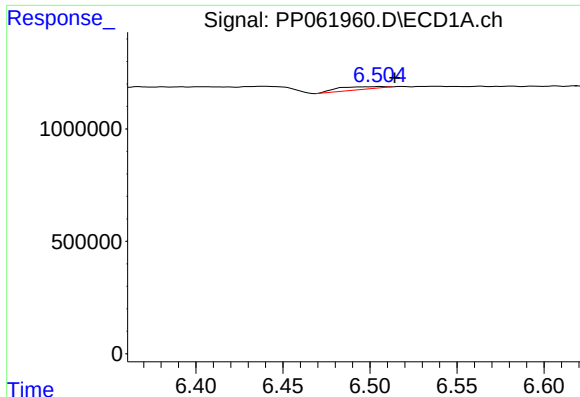

#24 AR-1248-4


R.T.: 6.506 min
Delta R.T.: -0.008 min
Response: 235454
Conc: 4.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

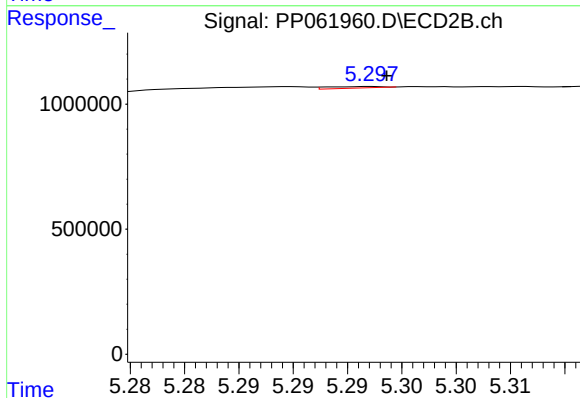


#24 AR-1248-4

R.T.: 5.297 min
Delta R.T.: -0.001 min
Response: 20945
Conc: 0.27 ng/ml

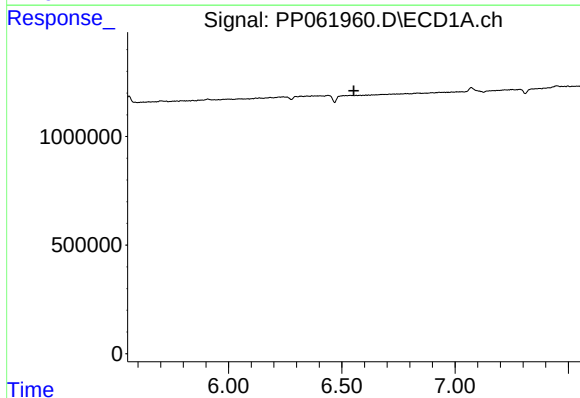


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.553 min
Response: 0
Conc: N.D.

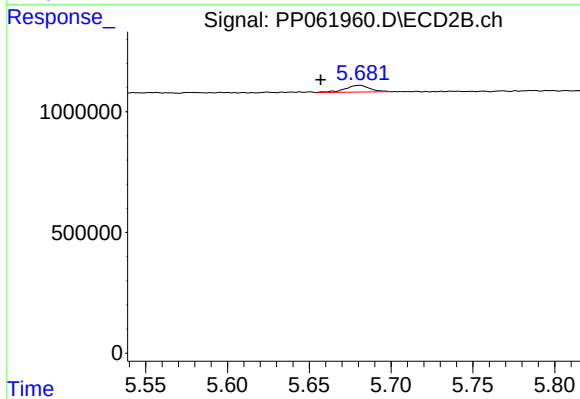

#25 AR-1248-5


R.T.: 5.681 min
Delta R.T.: 0.024 min
Response: 300906
Conc: 3.01 ng/ml

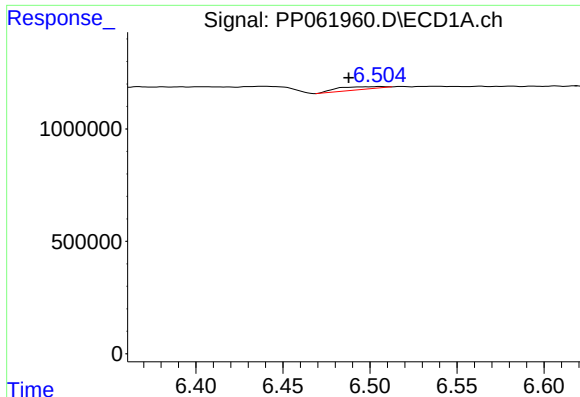

#26 AR-1254-1


R.T.: 6.506 min
Delta R.T.: 0.018 min
Response: 235454
Conc: 4.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

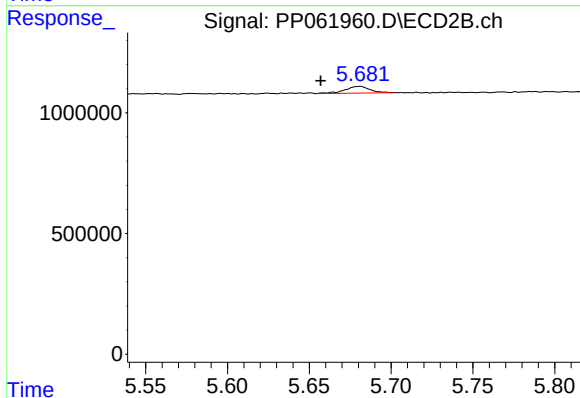


#26 AR-1254-1

R.T.: 5.681 min
Delta R.T.: 0.024 min
Response: 300906
Conc: 2.76 ng/ml

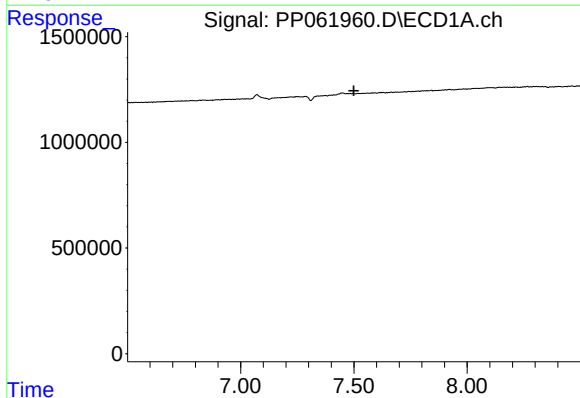

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.499 min
Response: 0
Conc: N.D.

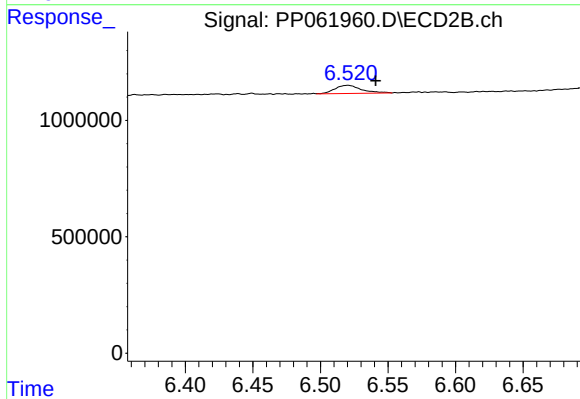

#32 AR-1260-2

R.T.: 6.521 min
Delta R.T.: -0.020 min
Response: 471370
Conc: 3.46 ng/ml