

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
 Data File : PP031728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Nov 2020 13:10
 Operator : DD\AJ
 Sample : L4899-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 14:34:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.792	4.065	1202389	1047486	24.831	21.860
2)	SA Decachlor...	10.671	9.371	822226	808316	24.209	21.830
Target Compounds							
6)	L1 AR-1016-4	0.000	5.566f	0	4348	N.D.	4.981 #
7)	L1 AR-1016-5	0.000	5.800	0	12191	N.D.	10.718 #
8)	L2 AR-1221-1	5.031	0.000	131422	0	241.652	N.D. #
9)	L2 AR-1221-2	0.000	4.435f	0	577	N.D.	1.496 #
15)	L3 AR-1232-5	0.000	5.800	0	12191	N.D.	42.070 #
20)	L4 AR-1242-5	0.000	6.197	0	9645	N.D.	9.349 #
22)	L5 AR-1248-2	0.000	5.566f	0	4348	N.D.	3.641 #
24)	L5 AR-1248-4	0.000	5.800	0	12191	N.D.	7.957 #
26)	L6 AR-1254-1	0.000	6.197	0	9645	N.D.	4.459 #
30)	L6 AR-1254-5	0.000	7.436	0	6106	N.D.	2.262 #
32)	L7 AR-1260-2	0.000	7.074f	0	3171	N.D.	1.302 #
33)	L7 AR-1260-3	0.000	7.255	0	3025	N.D.	1.325 #
34)	L7 AR-1260-4	0.000	7.744	0	5464	N.D.	2.876 #
35)	L7 AR-1260-5	0.000	7.980	0	20275	N.D.	4.468 #
37)	L8 AR-1262-2	0.000	7.980	0	20275	N.D.	4.174 #
38)	L8 AR-1262-3	0.000	8.279	0	6547	N.D.	3.329 #
39)	L8 AR-1262-4	0.000	8.344	0	15146	N.D.	4.178 #
40)	L8 AR-1262-5	0.000	8.836	0	6523	N.D.	4.019 #
41)	L9 AR-1268-1	0.000	8.279	0	6547	N.D.	1.183 #
42)	L9 AR-1268-2	0.000	8.344	0	15146	N.D.	2.801 #
43)	L9 AR-1268-3	0.000	8.567f	0	5699	N.D.	1.243 #
44)	L9 AR-1268-4	0.000	8.836	0	6523	N.D.	3.579 #
45)	L9 AR-1268-5	0.000	9.130	0	7749	N.D.	0.560 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
Data File : PP031728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2020 13:10
Operator : DD\AJ
Sample : L4899-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 14:34:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

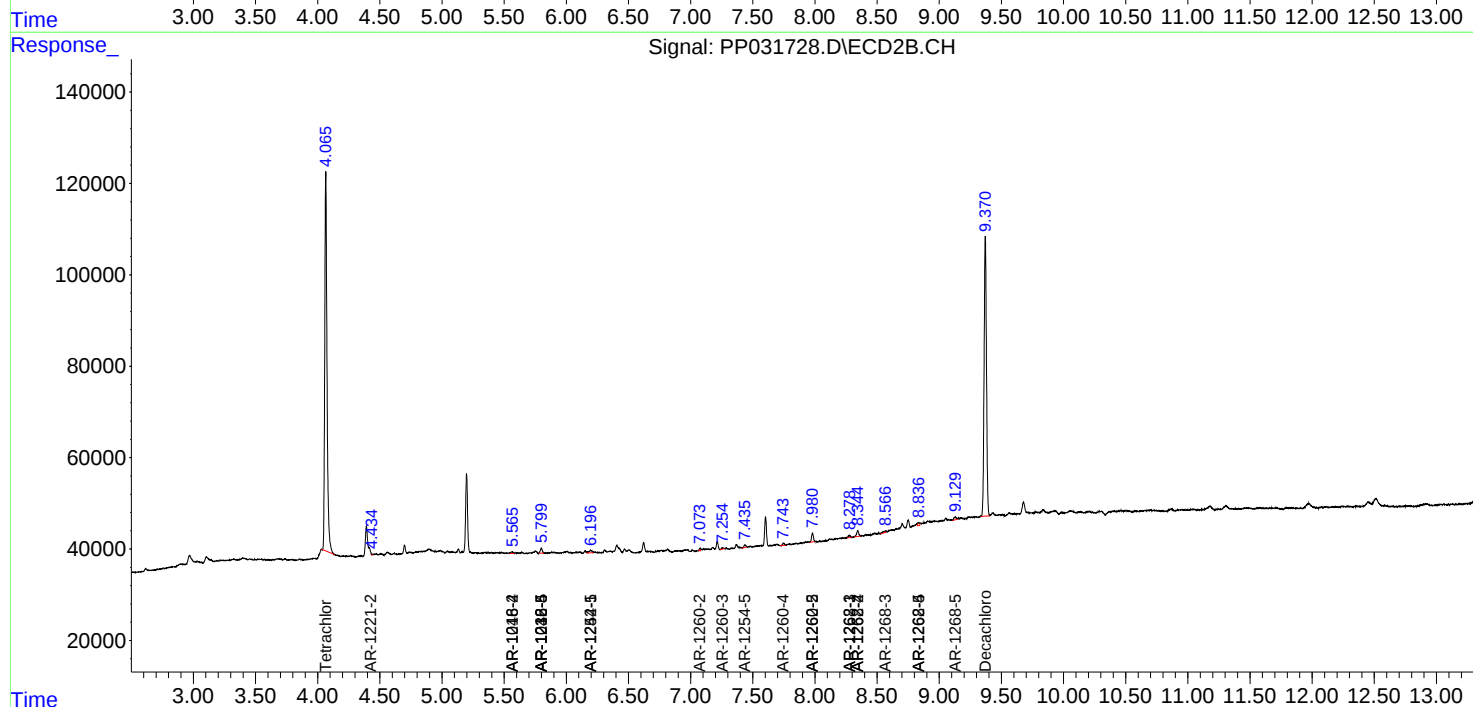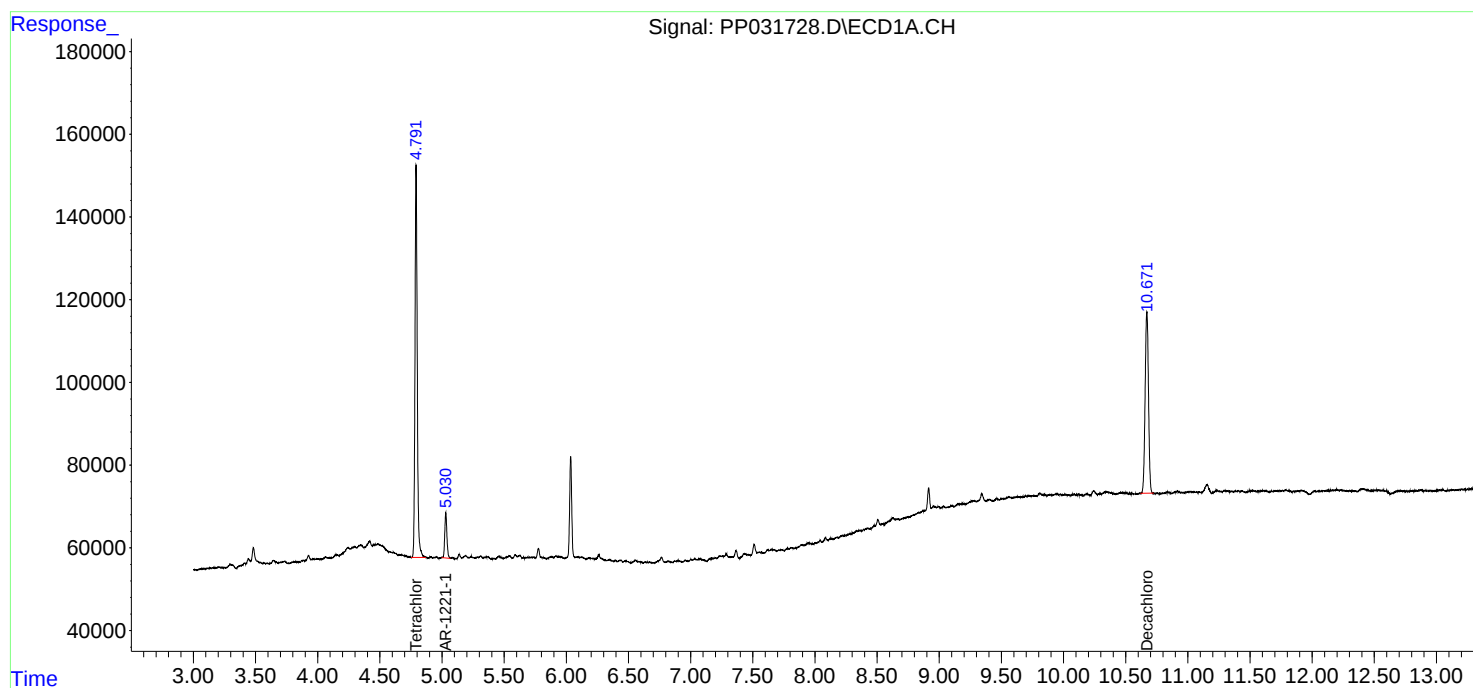


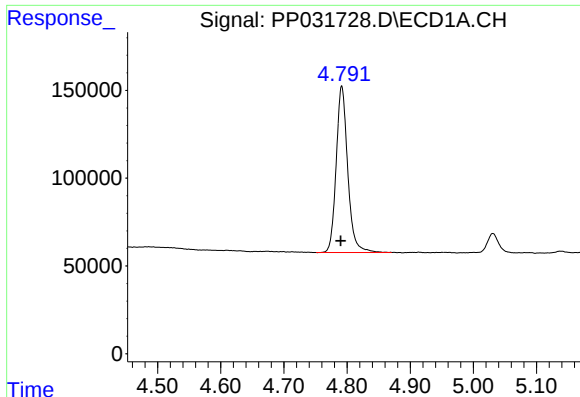

#1 Tetrachloro-m-xylene


R.T.: 4.792 min
Delta R.T.: 0.002 min
Response: 1202389
Conc: 24.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

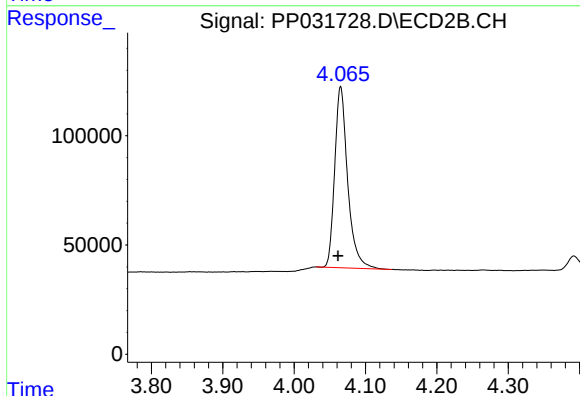


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.004 min
Response: 1047486
Conc: 21.86 ng/ml

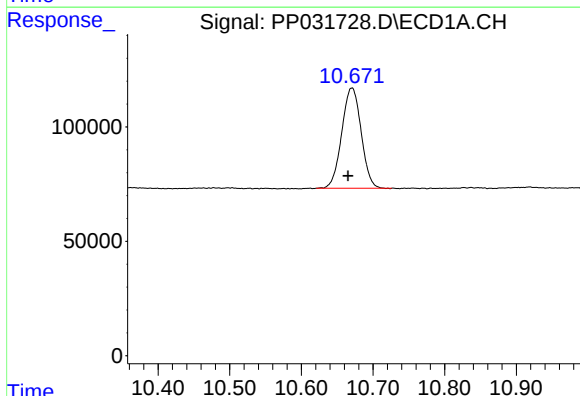


#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: 0.005 min
Response: 822226
Conc: 24.21 ng/ml

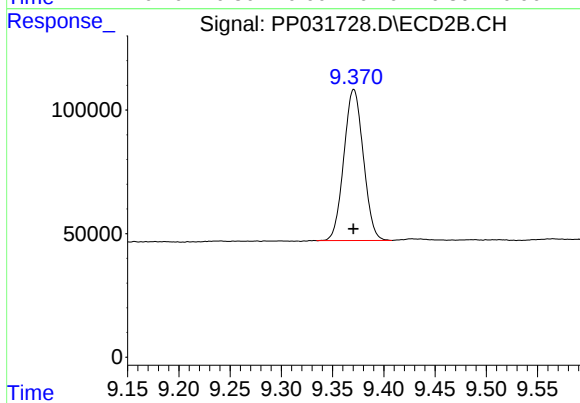

#2 Decachlorobiphenyl


R.T.: 9.371 min
Delta R.T.: 0.000 min
Response: 808316
Conc: 21.83 ng/ml

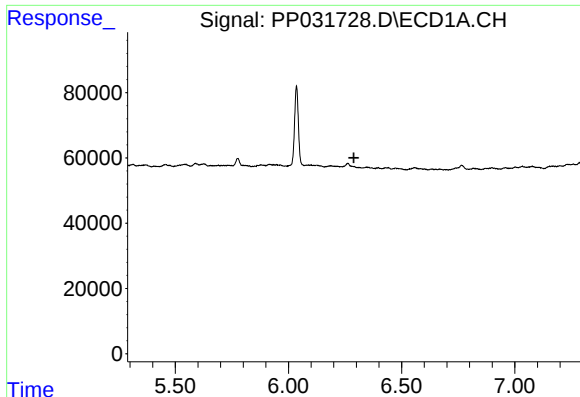

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 6.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

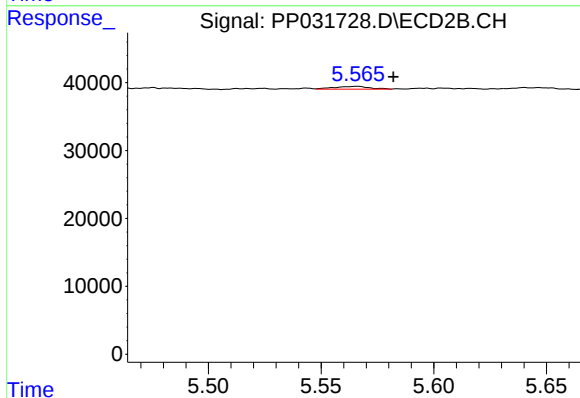


#6 AR-1016-4

R.T.: 5.566 min
Delta R.T.: -0.016 min
Response: 4348
Conc: 4.98 ng/ml

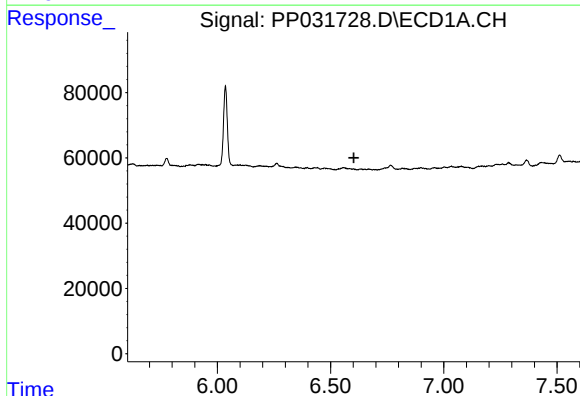


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T.: 6.603 min
Response: 0
Conc: N.D.

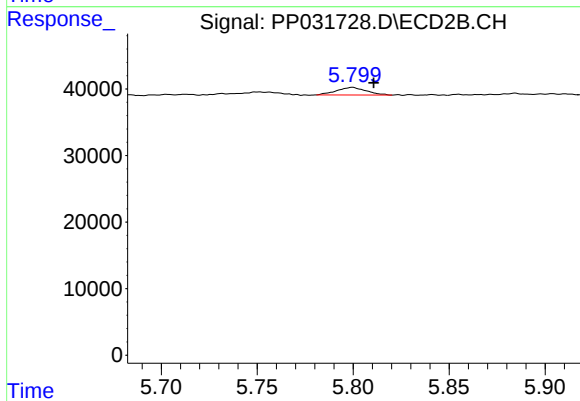

#7 AR-1016-5


R.T.: 5.800 min
Delta R.T.: -0.011 min
Response: 12191
Conc: 10.72 ng/ml

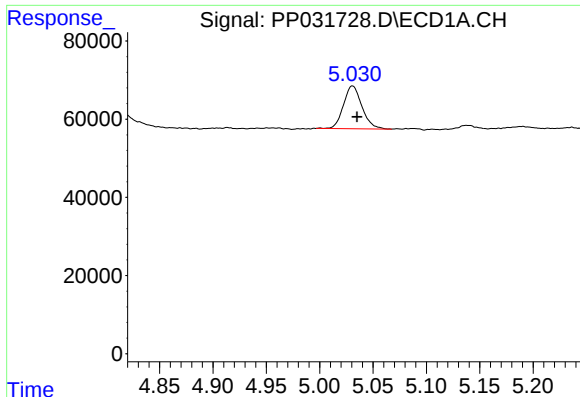

#8 AR-1221-1


R.T.: 5.031 min
Delta R.T.: -0.004 min
Response: 131422
Conc: 241.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

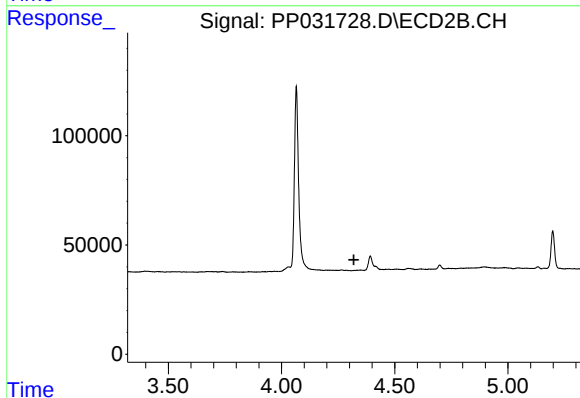


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

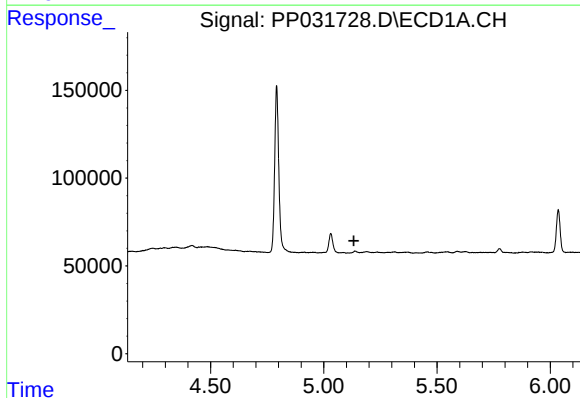


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

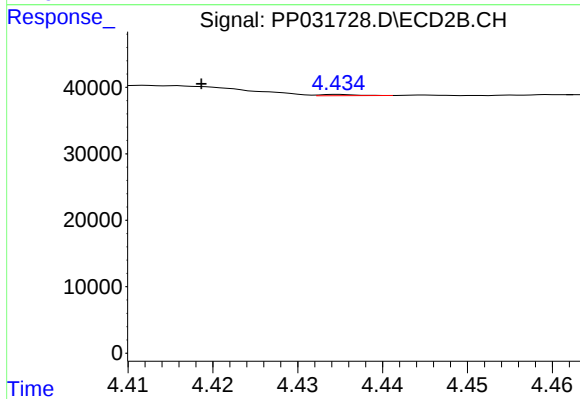

#9 AR-1221-2


R.T.: 4.435 min
Delta R.T.: 0.016 min
Response: 577
Conc: 1.50 ng/ml

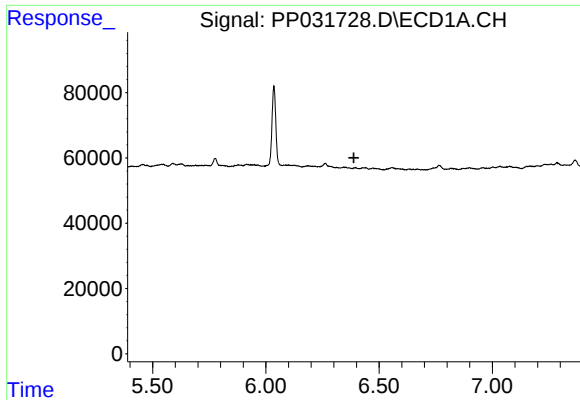

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

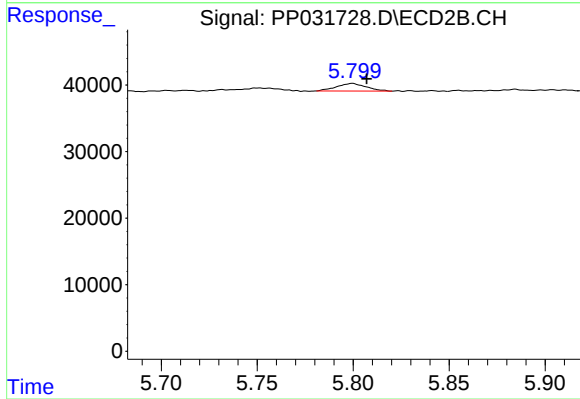


#15 AR-1232-5

R.T.: 5.800 min
Delta R.T.: -0.007 min
Response: 12191
Conc: 42.07 ng/ml

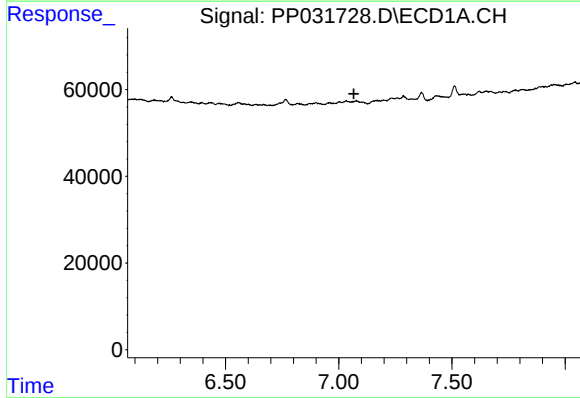


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.067 min
Response: 0
Conc: N.D.

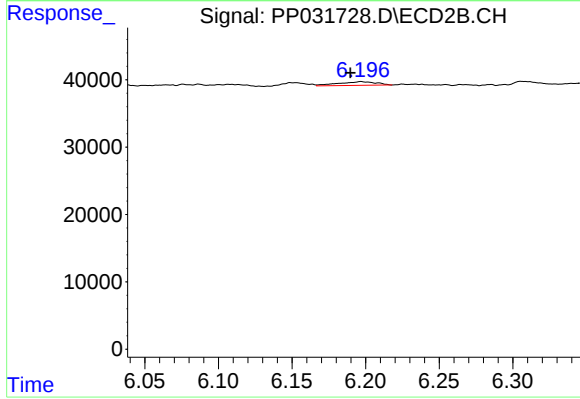

#20 AR-1242-5


R.T.: 6.197 min
Delta R.T.: 0.007 min
Response: 9645
Conc: 9.35 ng/ml

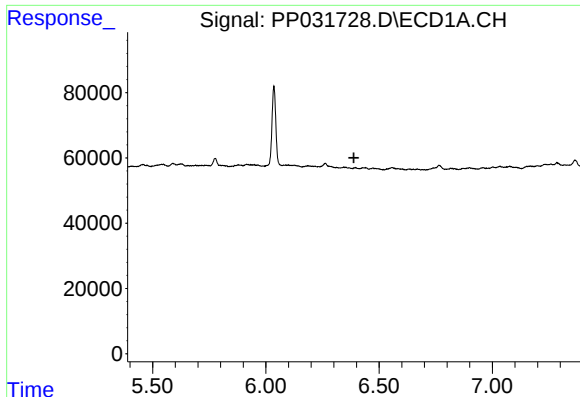

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

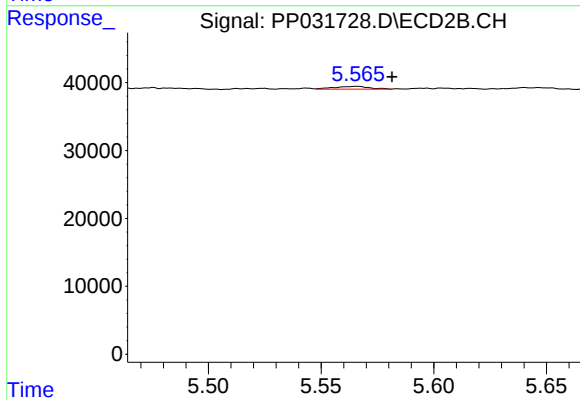


#22 AR-1248-2

R.T.: 5.566 min
Delta R.T.: -0.015 min
Response: 4348
Conc: 3.64 ng/ml

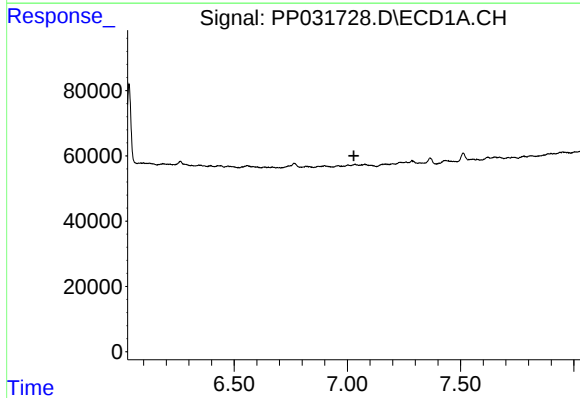


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

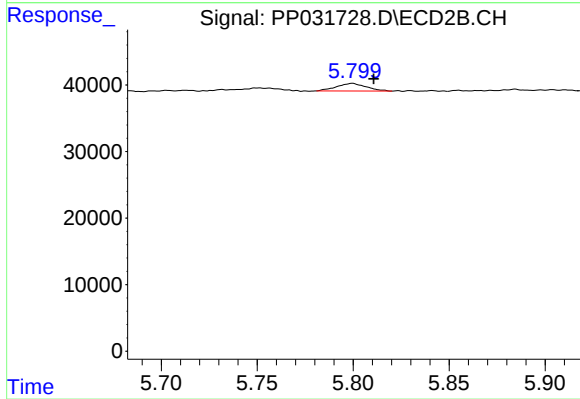

#24 AR-1248-4


R.T.: 5.800 min
Delta R.T.: -0.011 min
Response: 12191
Conc: 7.96 ng/ml

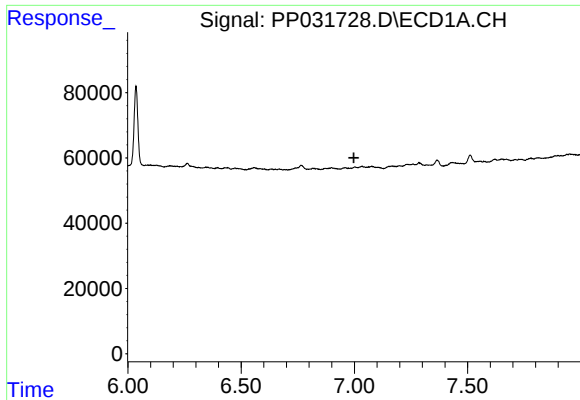

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

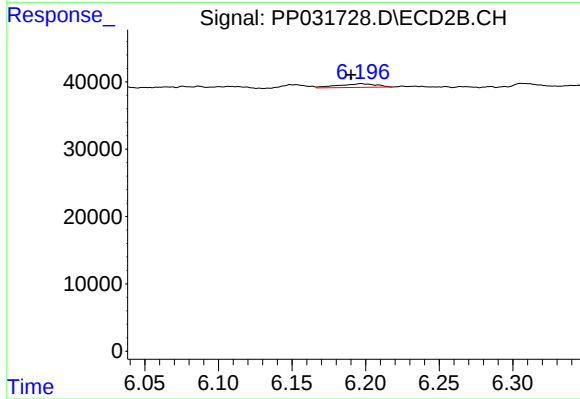


#26 AR-1254-1

R.T.: 6.197 min
Delta R.T.: 0.007 min
Response: 9645
Conc: 4.46 ng/ml

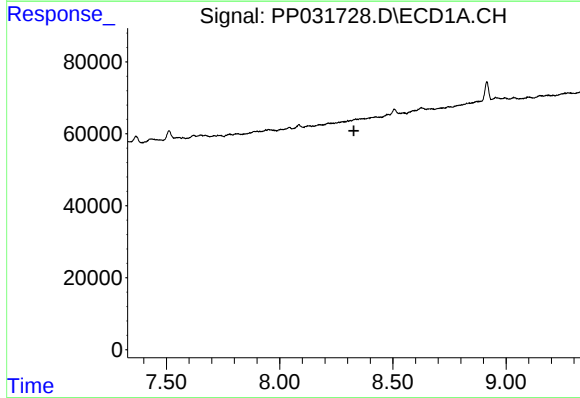


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.328 min
Response: 0
Conc: N.D.

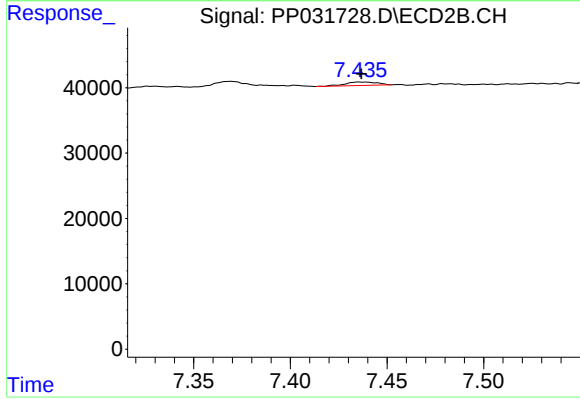

#30 AR-1254-5


R.T.: 7.436 min
Delta R.T.: -0.001 min
Response: 6106
Conc: 2.26 ng/ml

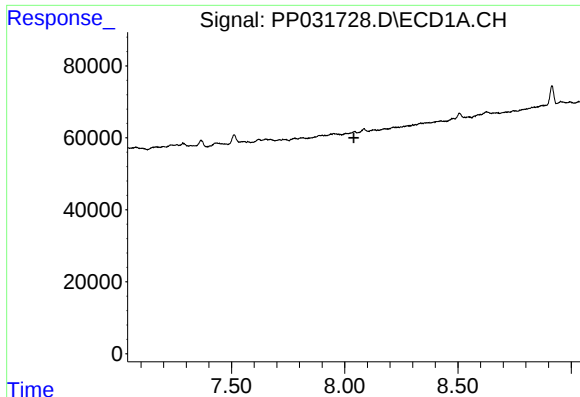

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

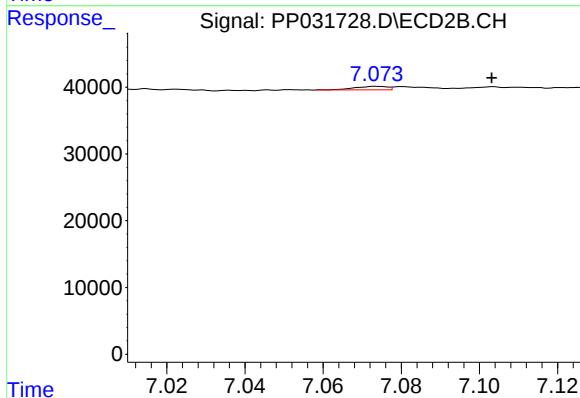


#32 AR-1260-2

R.T.: 7.074 min
Delta R.T.: -0.029 min
Response: 3171
Conc: 1.30 ng/ml

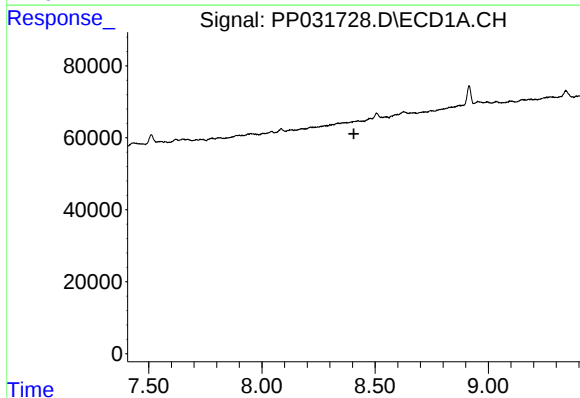


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

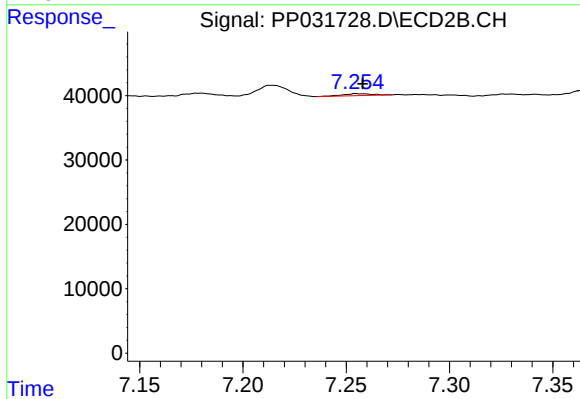

#33 AR-1260-3


R.T.: 7.255 min
Delta R.T.: -0.003 min
Response: 3025
Conc: 1.32 ng/ml

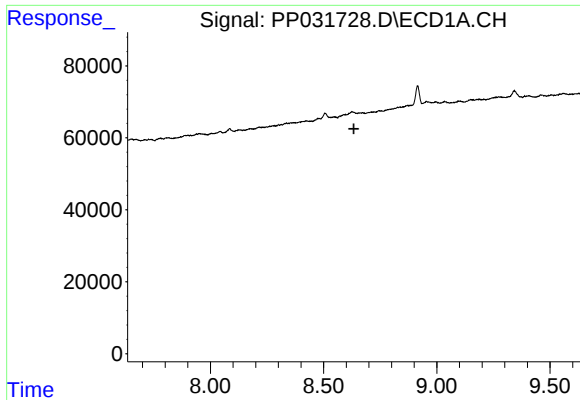

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 8.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

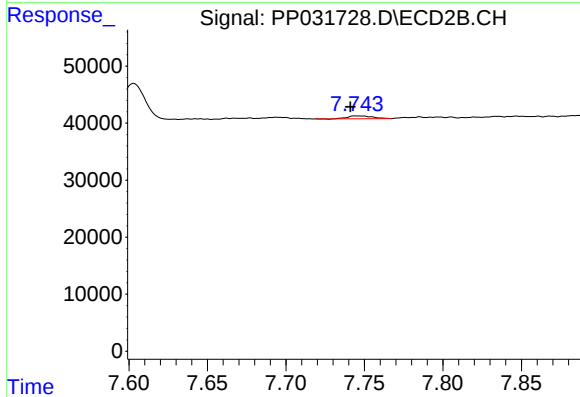


#34 AR-1260-4

R.T.: 7.744 min
Delta R.T.: 0.003 min
Response: 5464
Conc: 2.88 ng/ml

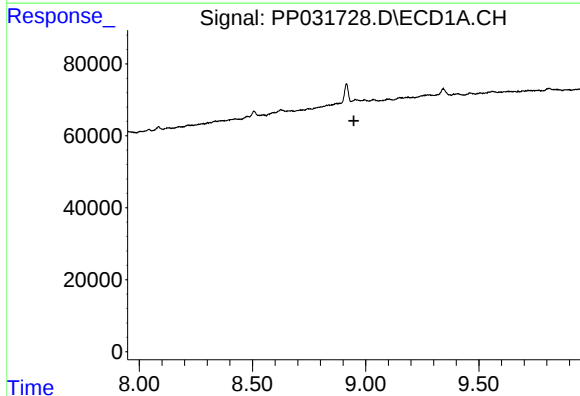


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

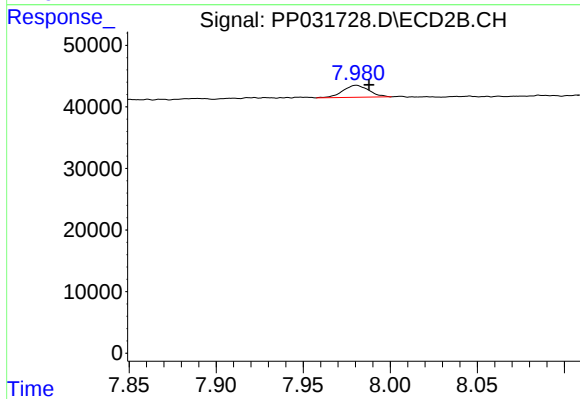

#35 AR-1260-5


R.T.: 7.980 min
Delta R.T.: -0.007 min
Response: 20275
Conc: 4.47 ng/ml

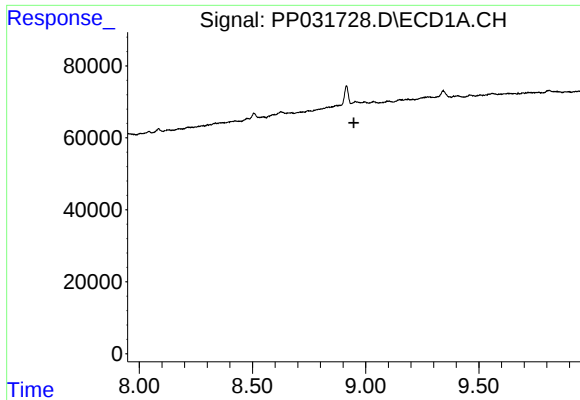

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

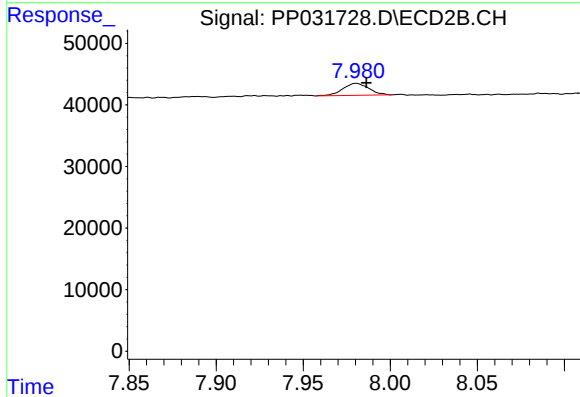


#37 AR-1262-2

R.T.: 7.980 min
Delta R.T.: -0.006 min
Response: 20275
Conc: 4.17 ng/ml

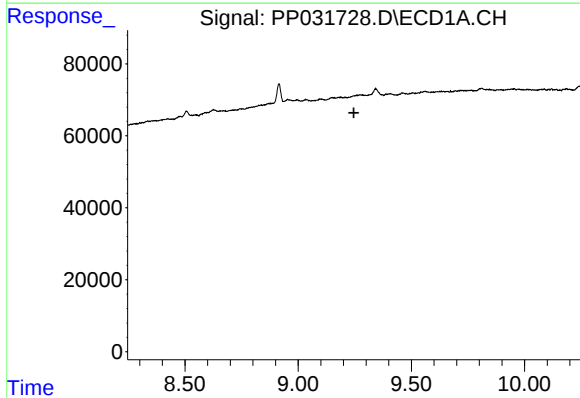


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

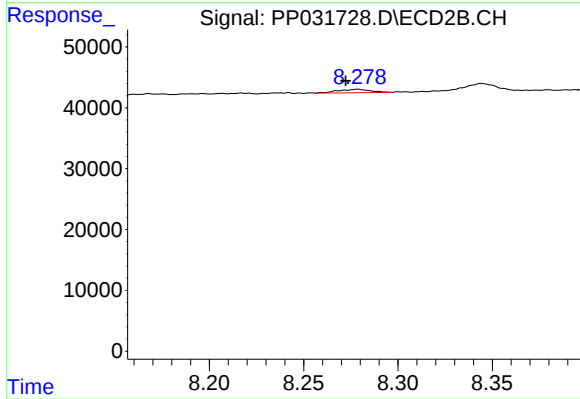

#38 AR-1262-3


R.T.: 8.279 min
Delta R.T.: 0.006 min
Response: 6547
Conc: 3.33 ng/ml

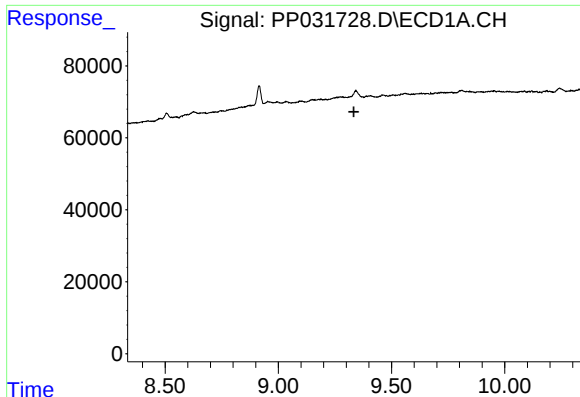

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

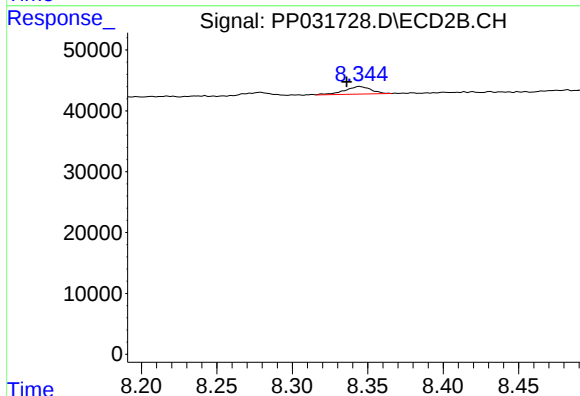


#39 AR-1262-4

R.T.: 8.344 min
Delta R.T.: 0.008 min
Response: 15146
Conc: 4.18 ng/ml

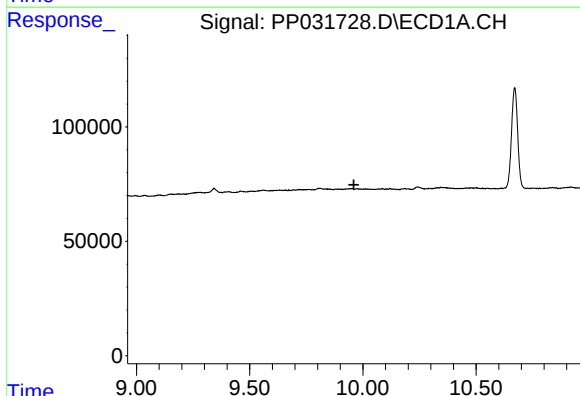


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

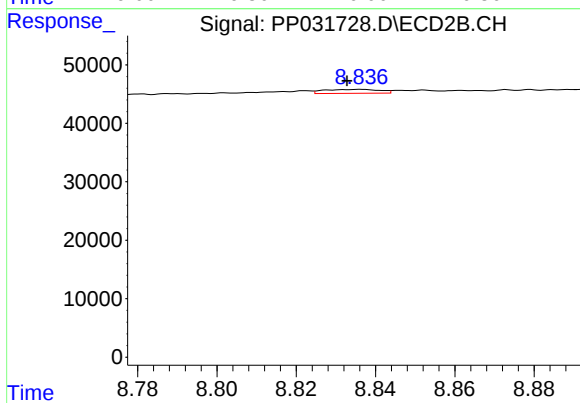

#40 AR-1262-5


R.T.: 8.836 min
Delta R.T.: 0.004 min
Response: 6523
Conc: 4.02 ng/ml

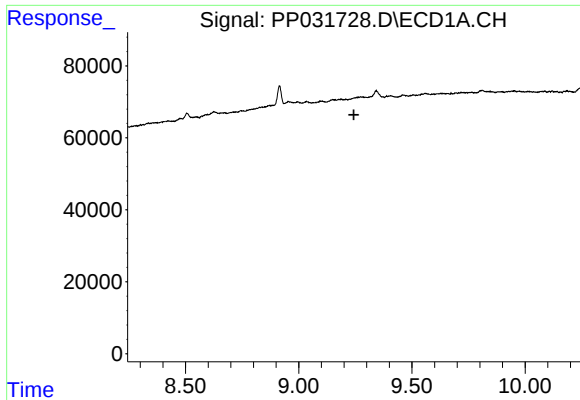

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

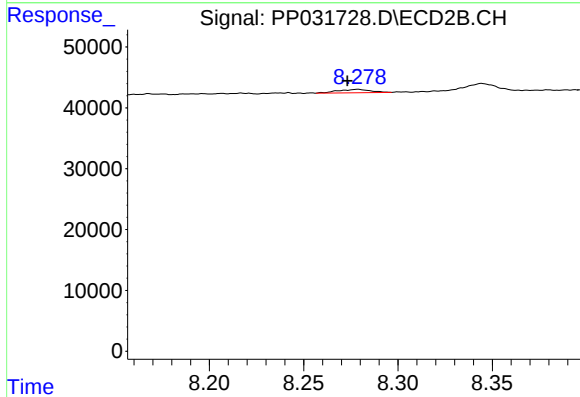


#41 AR-1268-1

R.T.: 8.279 min
Delta R.T.: 0.006 min
Response: 6547
Conc: 1.18 ng/ml

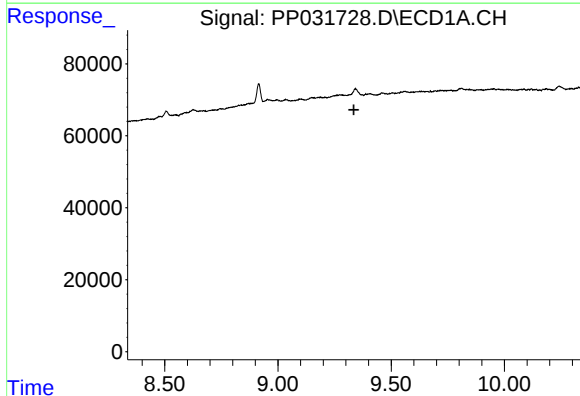


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

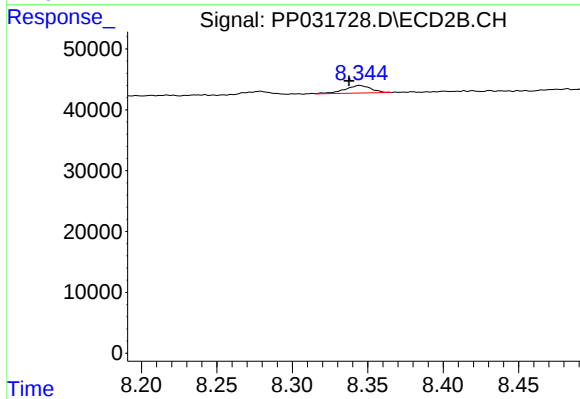

#42 AR-1268-2


R.T.: 8.344 min
Delta R.T.: 0.007 min
Response: 15146
Conc: 2.80 ng/ml

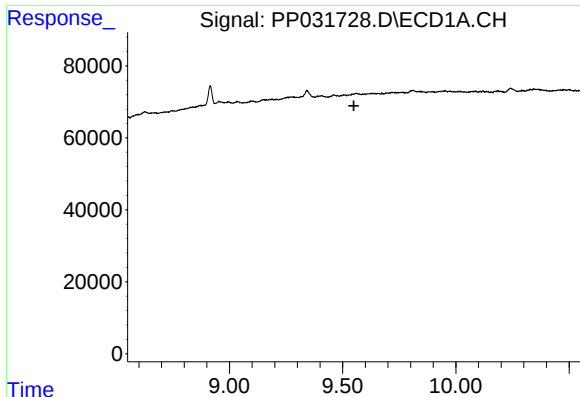

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

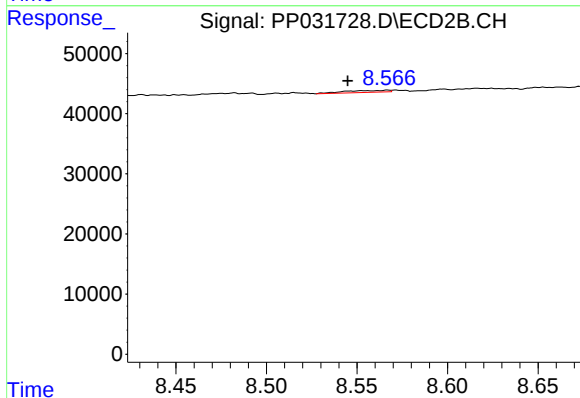


#43 AR-1268-3

R.T.: 8.567 min
Delta R.T.: 0.022 min
Response: 5699
Conc: 1.24 ng/ml

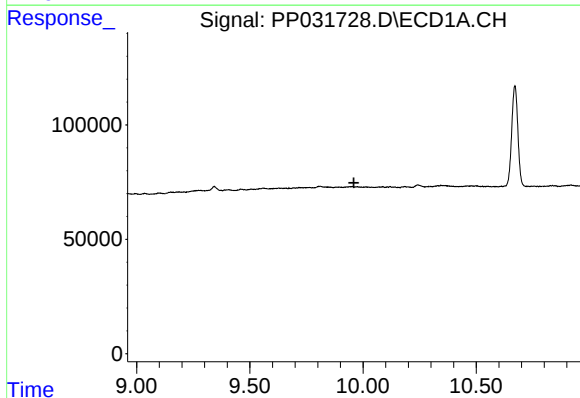


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.960 min
Response: 0
Conc: N.D.

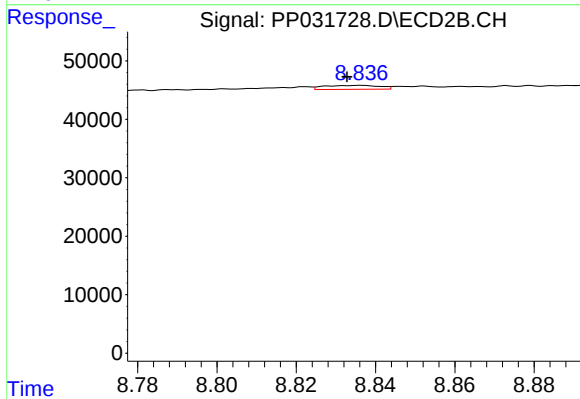

#44 AR-1268-4


R.T.: 8.836 min
Delta R.T.: 0.004 min
Response: 6523
Conc: 3.58 ng/ml

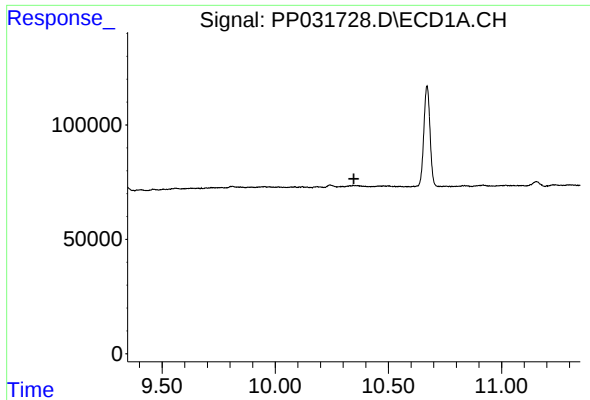

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

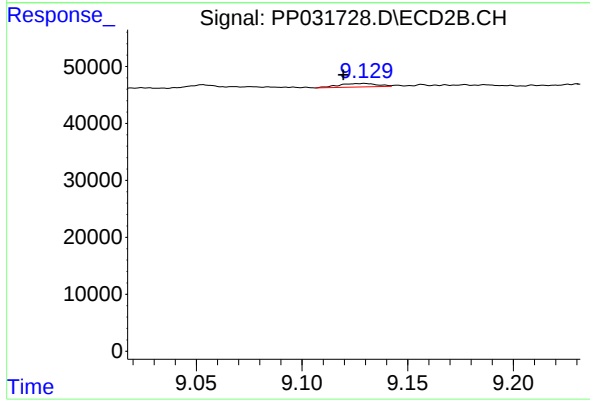

#45 AR-1268-5

R.T.: 9.130 min
Delta R.T.: 0.010 min
Response: 7749
Conc: 0.56 ng/ml