

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
 Data File : PP031735.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Nov 2020 15:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 15:41:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.792	4.066	1186620	1109427	24.505	23.152
2)	SA Decachlor...	10.671	9.372	781549	818617	23.011	22.109
Target Compounds							
9)	L2 AR-1221-2	0.000	4.418	0	12511	N.D.	32.433 #
20)	L4 AR-1242-5	0.000	6.213f	0	500	N.D.	0.485 #
25)	L5 AR-1248-5	0.000	6.213f	0	500	N.D.	0.343 #
26)	L6 AR-1254-1	0.000	6.213f	0	500	N.D.	0.231 #
32)	L7 AR-1260-2	0.000	7.076f	0	12418	N.D.	5.099 #
35)	L7 AR-1260-5	0.000	7.990	0	3465	N.D.	0.764 #
37)	L8 AR-1262-2	0.000	7.990	0	3465	N.D.	0.713 #
38)	L8 AR-1262-3	0.000	8.272	0	374	N.D.	0.190 #
39)	L8 AR-1262-4	0.000	8.341	0	3748	N.D.	1.034 #
40)	L8 AR-1262-5	0.000	8.835	0	6101	N.D.	3.759 #
41)	L9 AR-1268-1	0.000	8.272	0	374	N.D.	0.068 #
42)	L9 AR-1268-2	0.000	8.341	0	3748	N.D.	0.693 #
43)	L9 AR-1268-3	0.000	8.550	0	1536	N.D.	0.335 #
44)	L9 AR-1268-4	0.000	8.835	0	6101	N.D.	3.347 #
45)	L9 AR-1268-5	0.000	9.113	0	1903	N.D.	0.137 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
Data File : PP031735.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2020 15:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 15:41:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

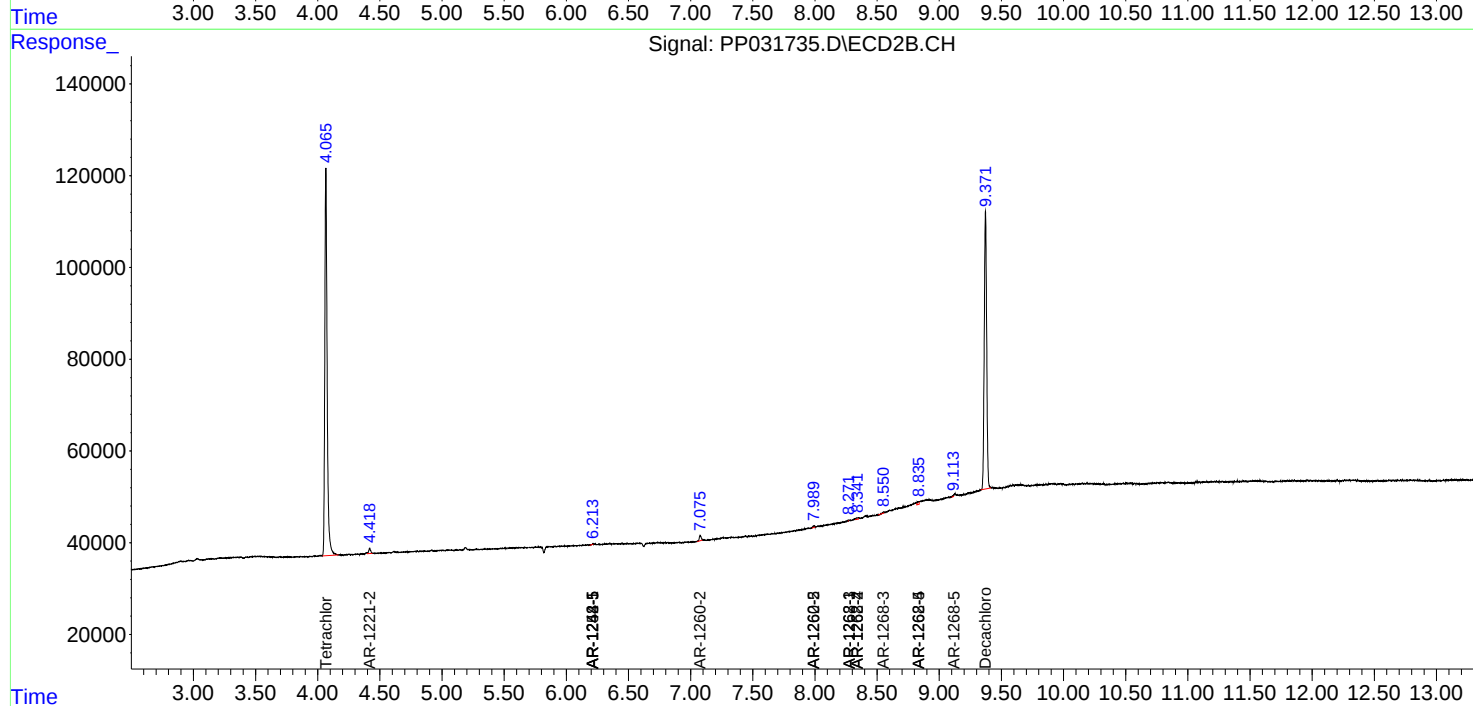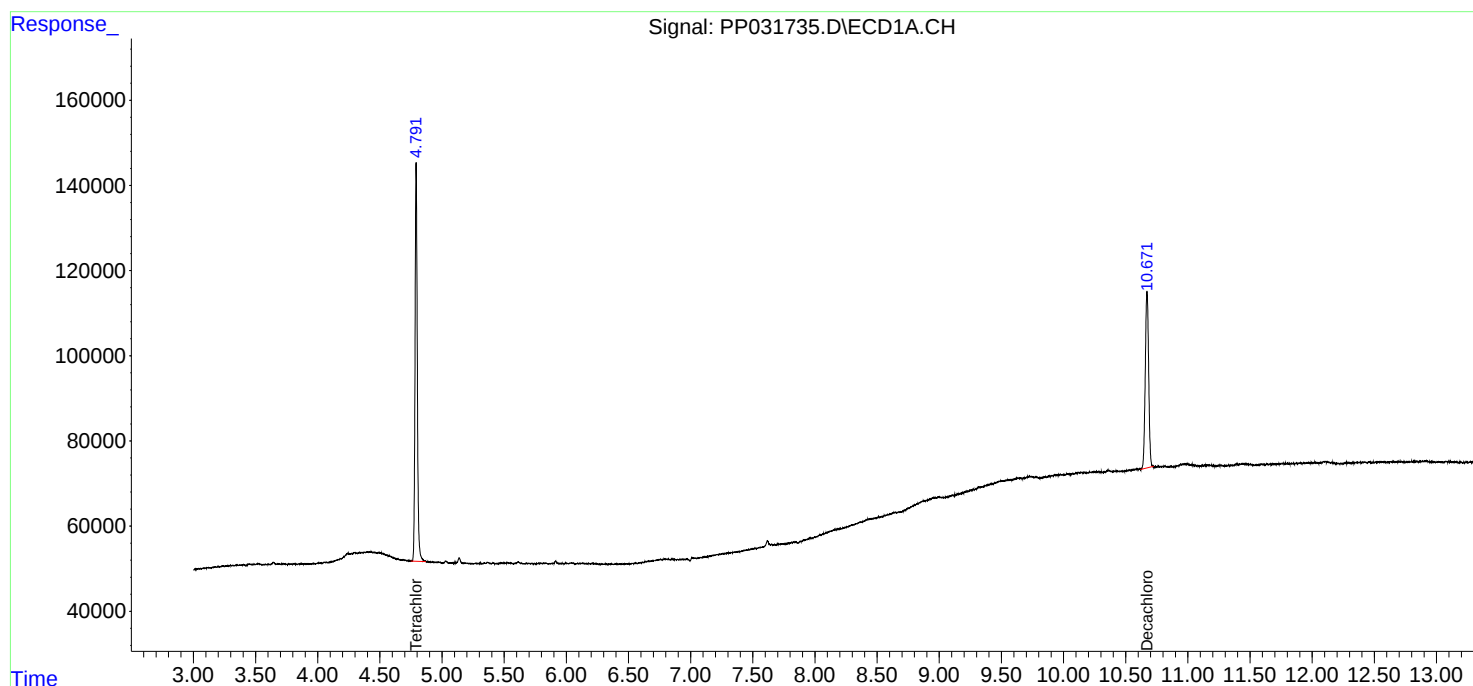


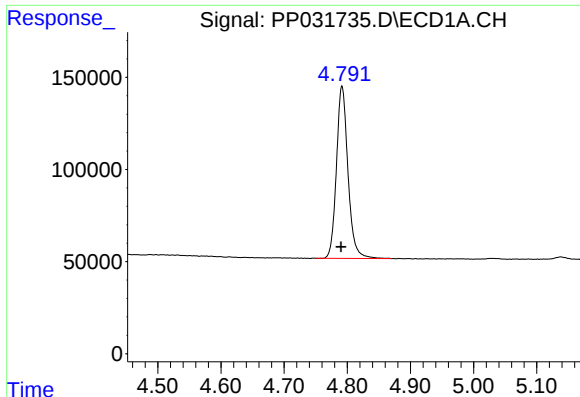

#1 Tetrachloro-m-xylene


R.T.: 4.792 min
Delta R.T.: 0.002 min
Response: 1186620
Conc: 24.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

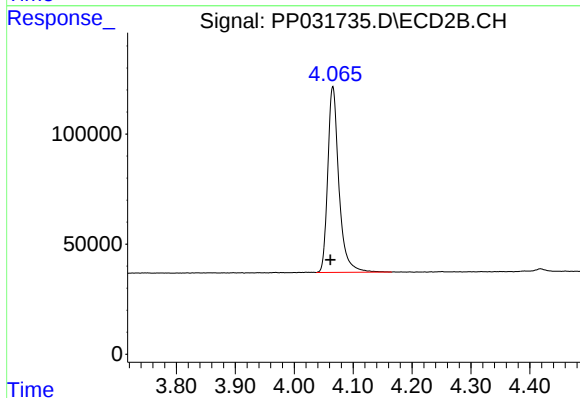


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: 0.004 min
Response: 1109427
Conc: 23.15 ng/ml

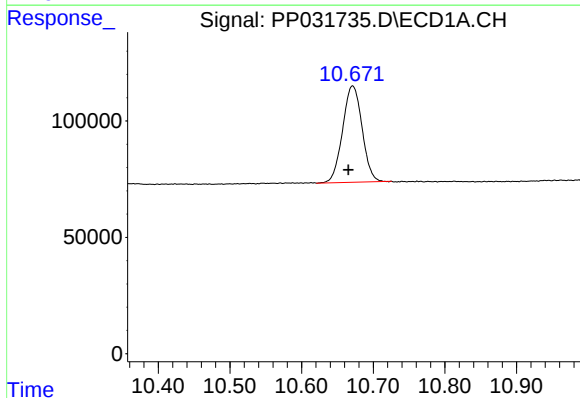


#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: 0.006 min
Response: 781549
Conc: 23.01 ng/ml

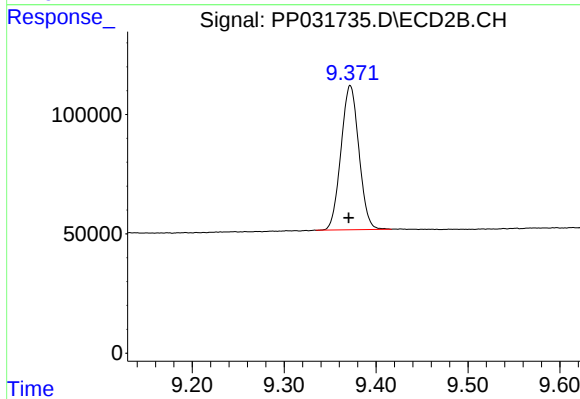

#2 Decachlorobiphenyl


R.T.: 9.372 min
Delta R.T.: 0.002 min
Response: 818617
Conc: 22.11 ng/ml

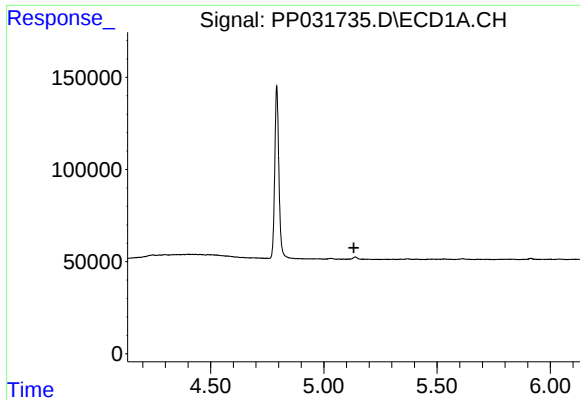

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

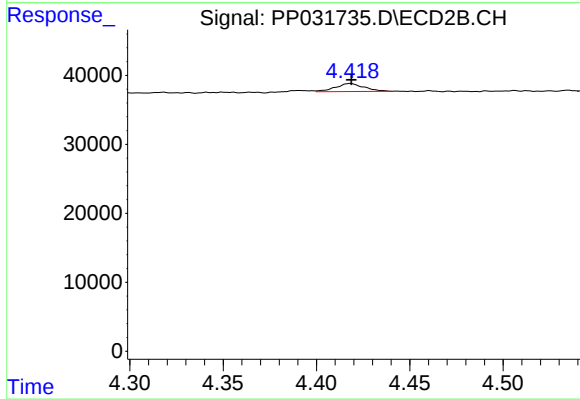


#9 AR-1221-2

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 12511
Conc: 32.43 ng/ml

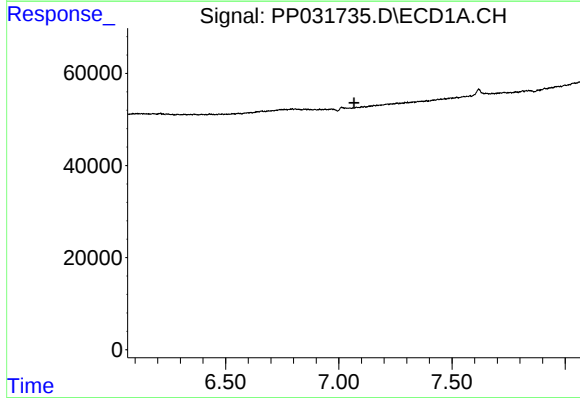


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

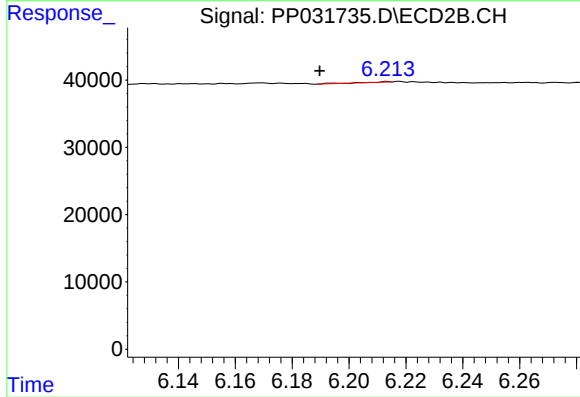

#20 AR-1242-5


R.T.: 6.213 min
Delta R.T.: 0.023 min
Response: 500
Conc: 0.48 ng/ml

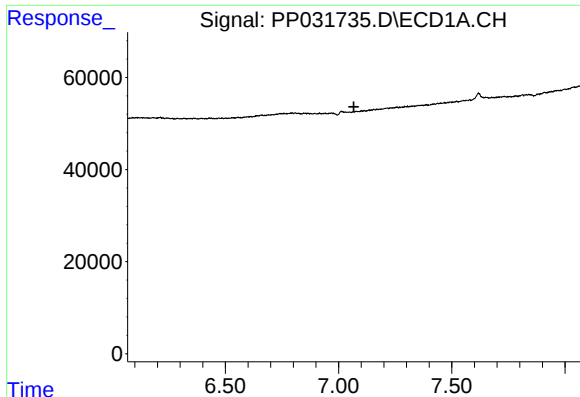

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 7.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

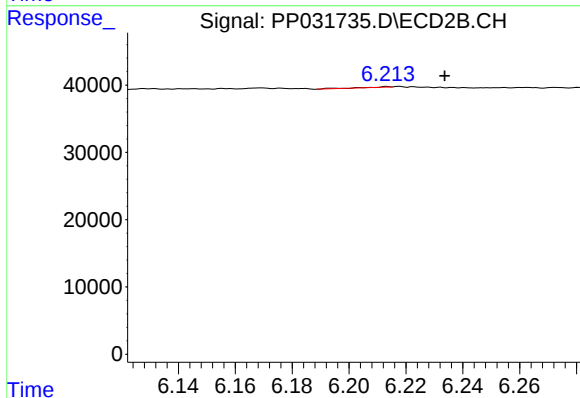


#25 AR-1248-5

R.T.: 6.213 min
Delta R.T.: -0.020 min
Response: 500
Conc: 0.34 ng/ml

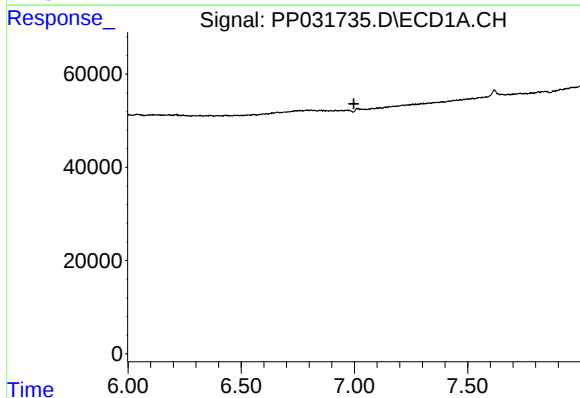


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

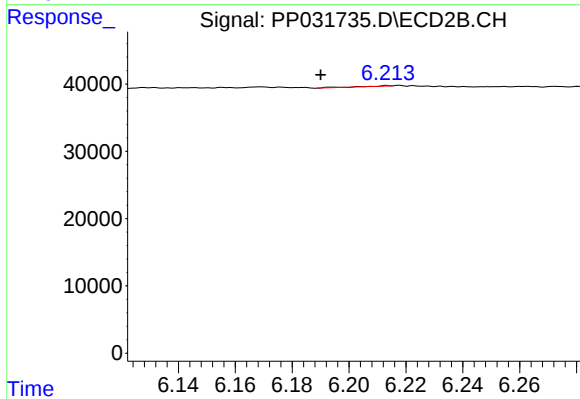

#26 AR-1254-1


R.T.: 6.213 min
Delta R.T.: 0.023 min
Response: 500
Conc: 0.23 ng/ml

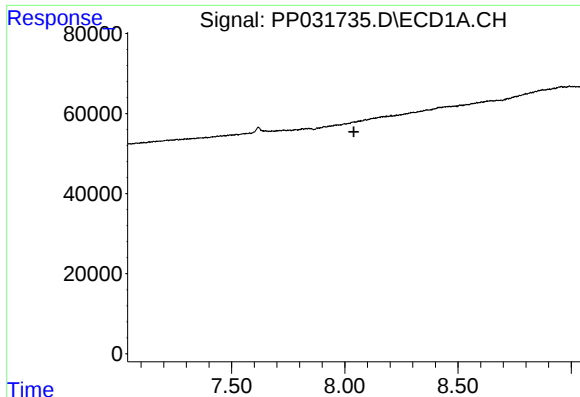

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

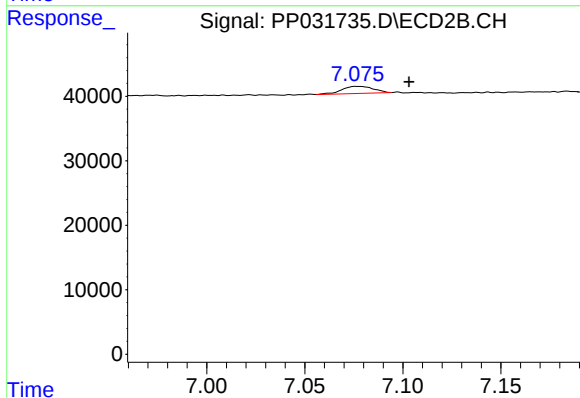


#32 AR-1260-2

R.T.: 7.076 min
Delta R.T.: -0.027 min
Response: 12418
Conc: 5.10 ng/ml

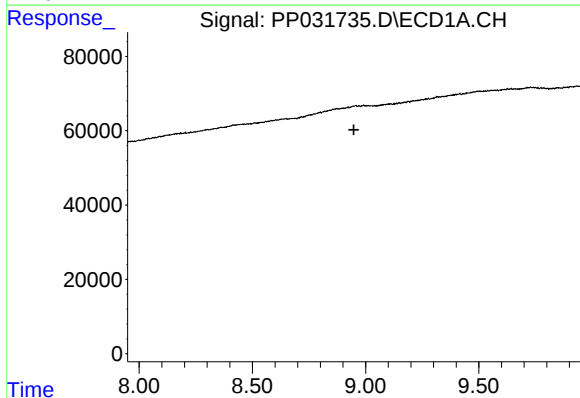


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.948 min
Response: 0
Conc: N.D.

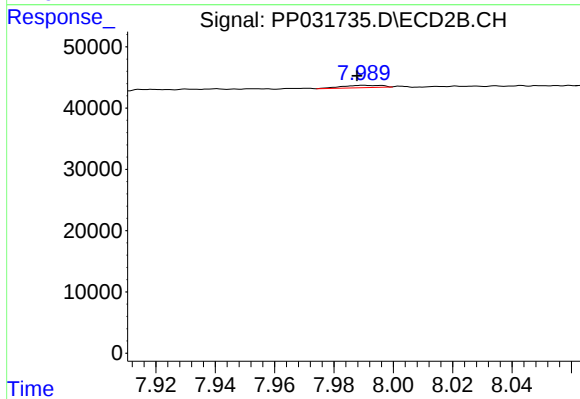

#35 AR-1260-5


R.T.: 7.990 min
Delta R.T.: 0.002 min
Response: 3465
Conc: 0.76 ng/ml

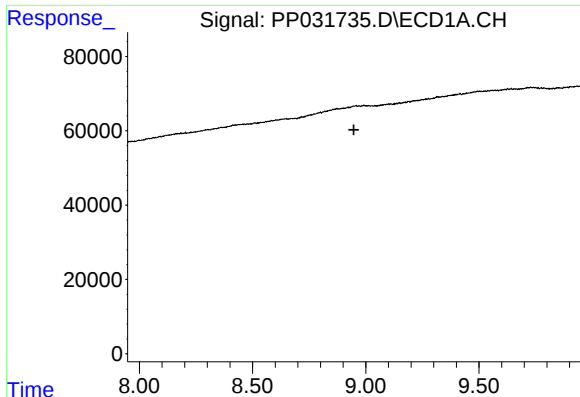

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

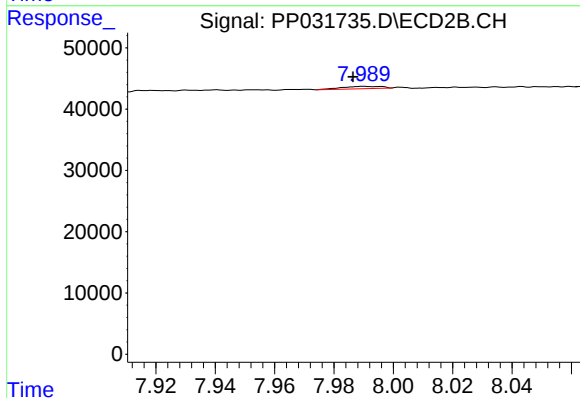


#37 AR-1262-2

R.T.: 7.990 min
Delta R.T.: 0.004 min
Response: 3465
Conc: 0.71 ng/ml

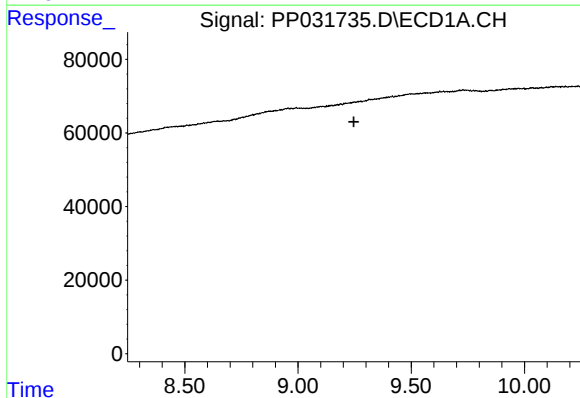


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

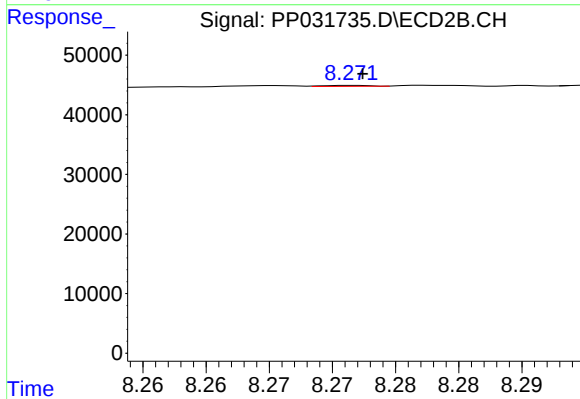

#38 AR-1262-3


R.T.: 8.272 min
Delta R.T.: 0.000 min
Response: 374
Conc: 0.19 ng/ml

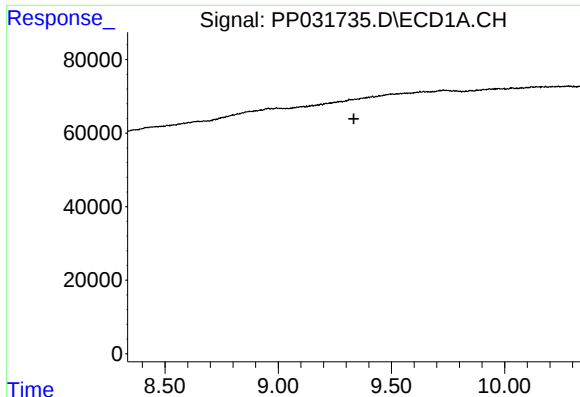

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

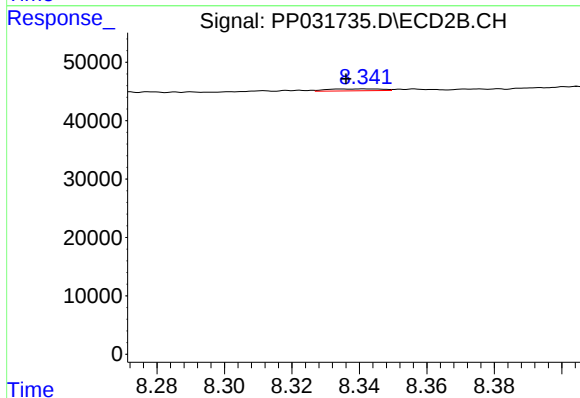


#39 AR-1262-4

R.T.: 8.341 min
Delta R.T.: 0.005 min
Response: 3748
Conc: 1.03 ng/ml

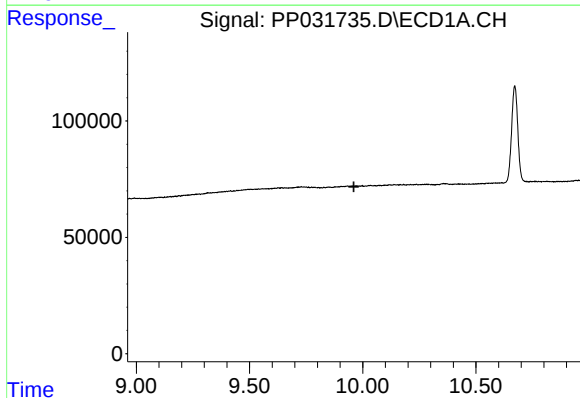


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.961 min
Response: 0
Conc: N.D.

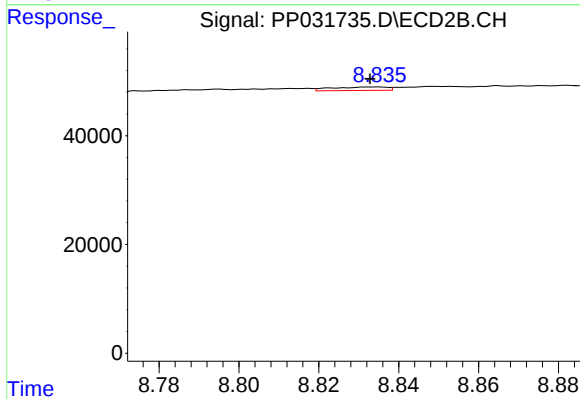

#40 AR-1262-5


R.T.: 8.835 min
Delta R.T.: 0.002 min
Response: 6101
Conc: 3.76 ng/ml

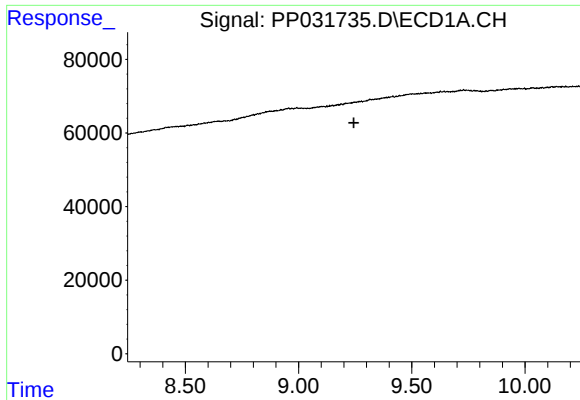

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

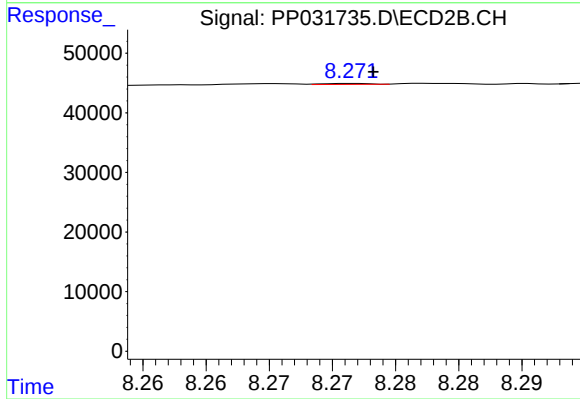


#41 AR-1268-1

R.T.: 8.272 min
Delta R.T.: -0.001 min
Response: 374
Conc: 0.07 ng/ml

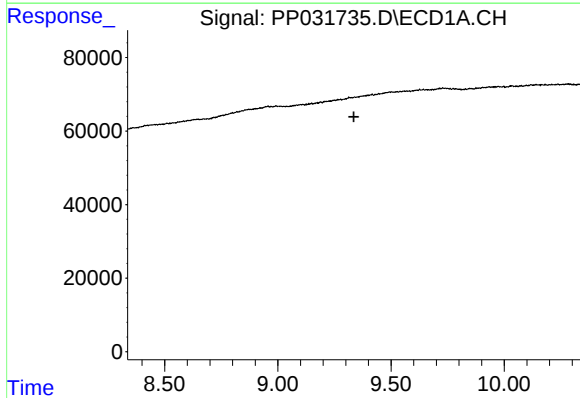


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.336 min
Response: 0
Conc: N.D.

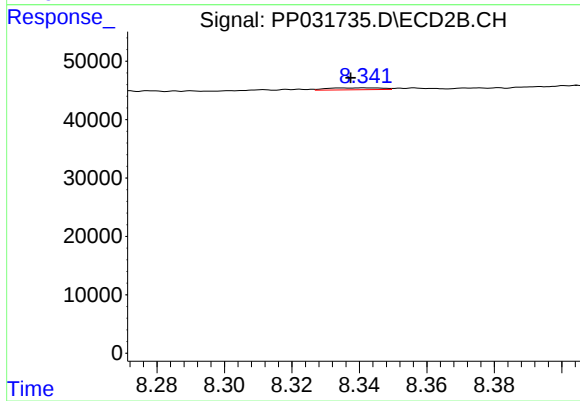

#42 AR-1268-2


R.T.: 8.341 min
Delta R.T.: 0.004 min
Response: 3748
Conc: 0.69 ng/ml

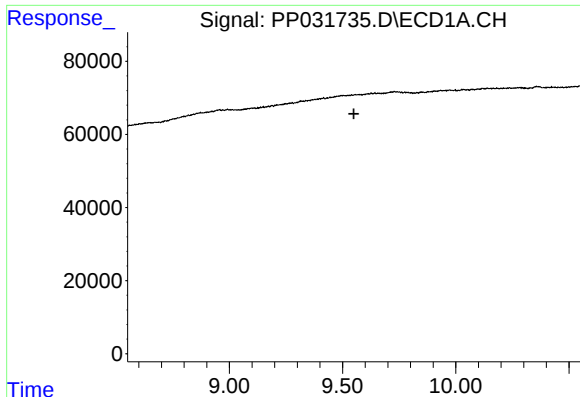

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

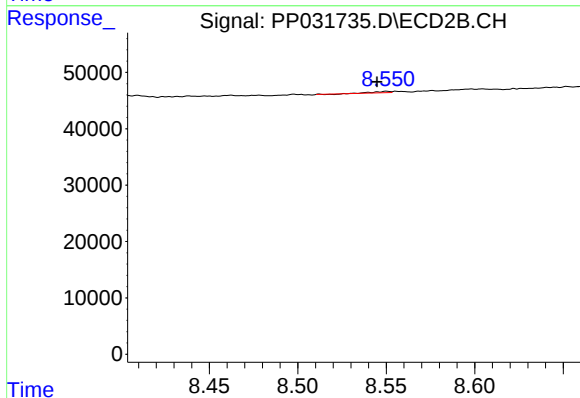


#43 AR-1268-3

R.T.: 8.550 min
Delta R.T.: 0.005 min
Response: 1536
Conc: 0.33 ng/ml

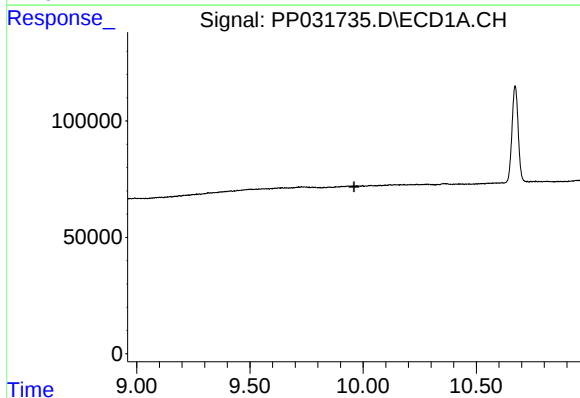


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.960 min
Response: 0
Conc: N.D.

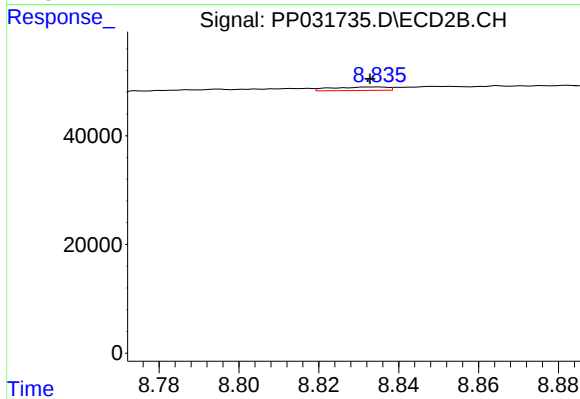

#44 AR-1268-4


R.T.: 8.835 min
Delta R.T.: 0.002 min
Response: 6101
Conc: 3.35 ng/ml

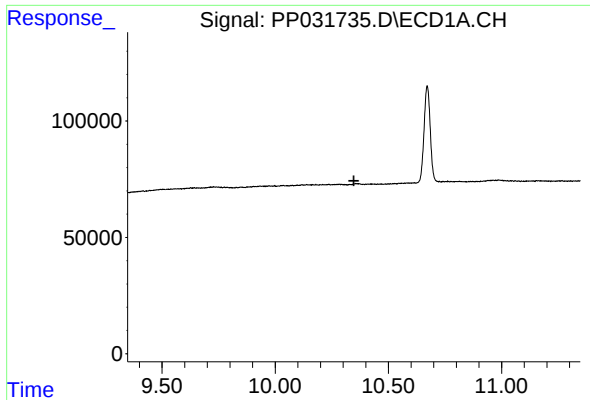

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

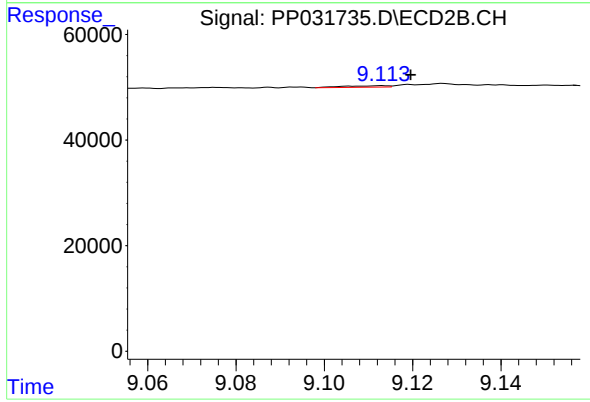

#45 AR-1268-5

R.T.: 9.113 min
Delta R.T.: -0.006 min
Response: 1903
Conc: 0.14 ng/ml