

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
 Data File : PP031726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Nov 2020 12:36
 Operator : DD\AJ
 Sample : L4897-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 88-CHOPIN

Manual Integrations
 APPROVED

Ankita
 12/1/2020 12:07:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 14:33:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.806f	4.087f	921020	856828	19.020m	17.881m
2) SA Decachlor...	10.669	9.371	899972	919078	26.498	24.822

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
Data File : PP031726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2020 12:36
Operator : DD\AJ
Sample : L4897-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
88-CHOPIN


Manual Integrations
APPROVED

Ankita
12/1/2020 12:07:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 14:33:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

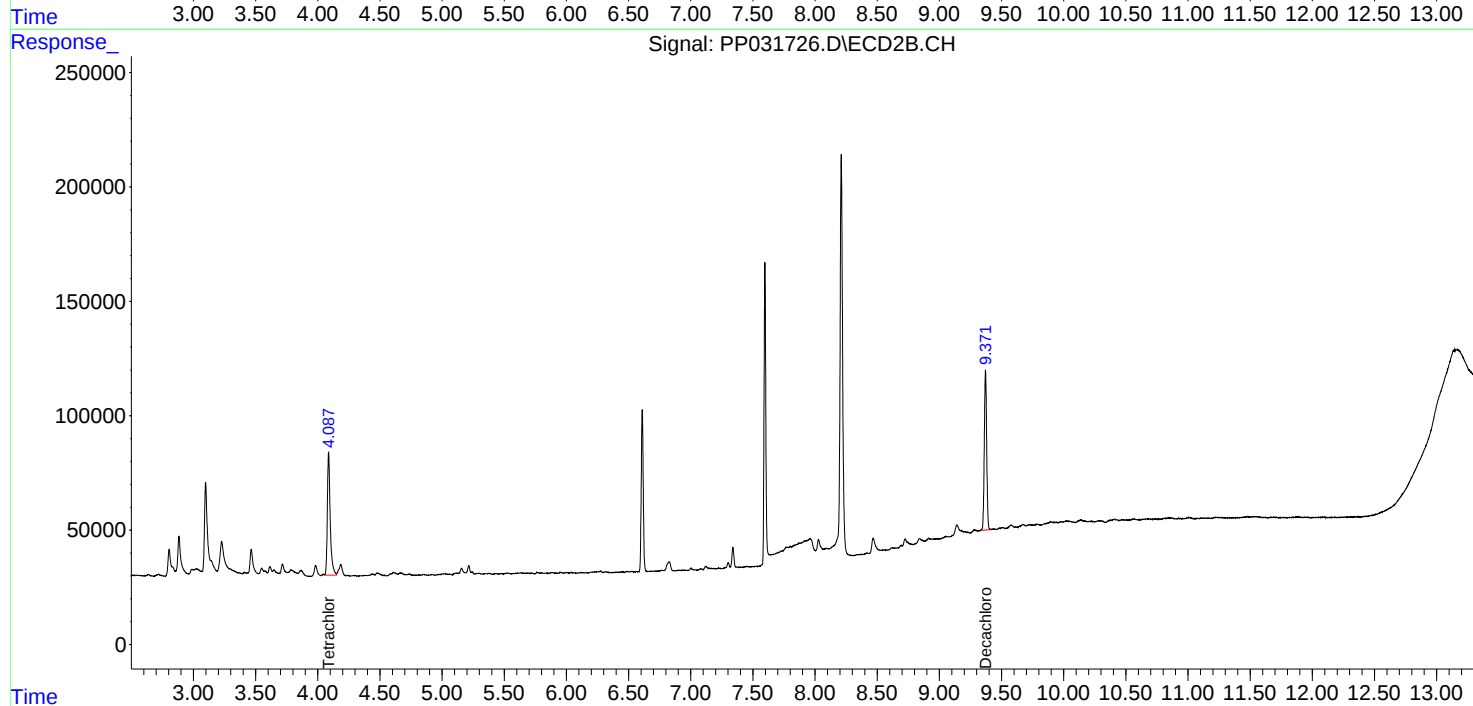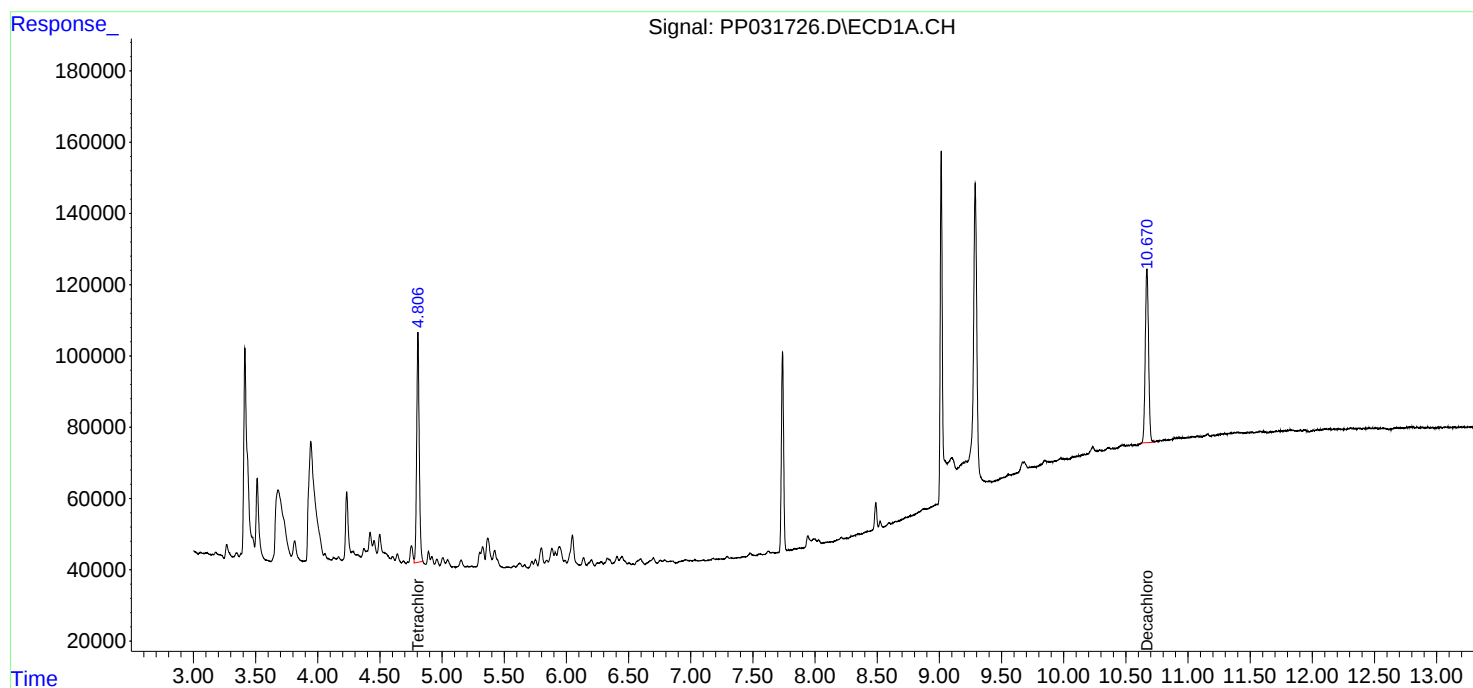

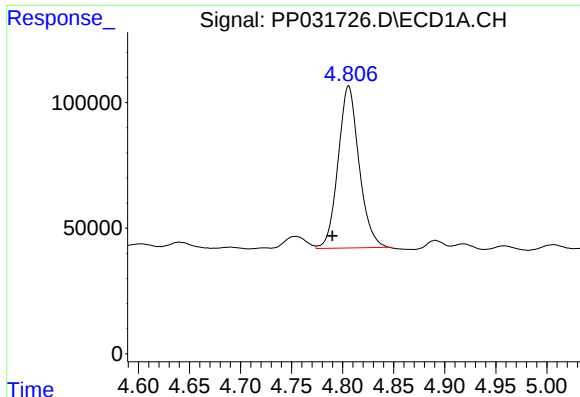


#1 Tetrachloro-m-xylene

R.T.: 4.806 min
Delta R.T.: 0.016 min
Response: 921020
Conc: 19.02 ng/ml m

Instrument :
ECD_P
ClientSampleId :
88-CHOPIN


Manual Integrations
APPROVED

Ankita
12/1/2020 12:07:07 PM

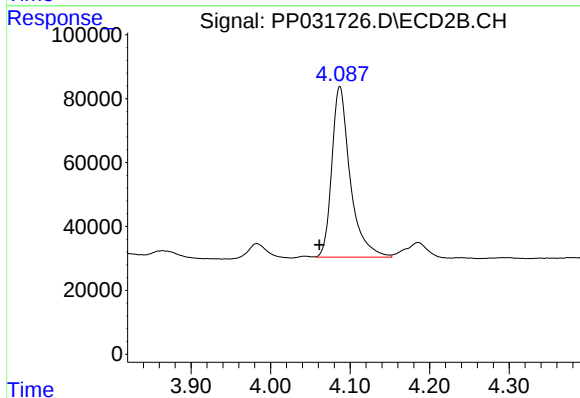


#1 Tetrachloro-m-xylene

R.T.: 4.087 min
Delta R.T.: 0.025 min
Response: 856828
Conc: 17.88 ng/ml m

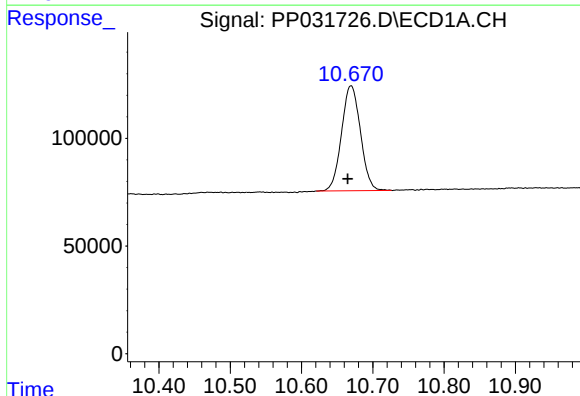

#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: 0.004 min
Response: 899972
Conc: 26.50 ng/ml

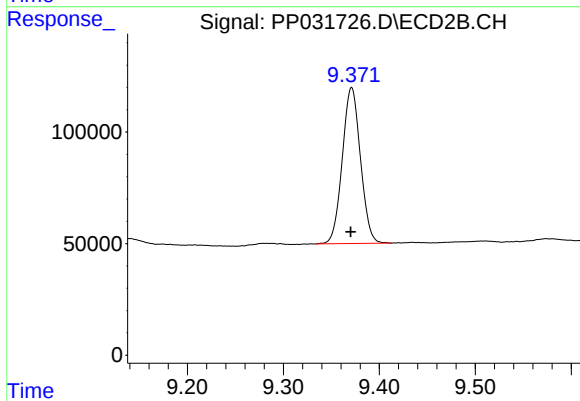

#2 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: 0.000 min
Response: 919078
Conc: 24.82 ng/ml