

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
 Data File : PP031730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Nov 2020 13:43
 Operator : DD\AJ
 Sample : L4900-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAV-B2-112520-10-12.75

Manual Integrations
 APPROVED

Ankita
 12/1/2020 12:07:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 14:35:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.065	1138115	1128574	23.503m	23.552
2) SA Decachlor...	10.671	9.371	769652	764500	22.661	20.647

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113020\
Data File : PP031730.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2020 13:43
Operator : DD\AJ
Sample : L4900-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAV-B2-112520-10-12.75


Manual Integrations
APPROVED

Ankita
12/1/2020 12:07:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 14:35:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

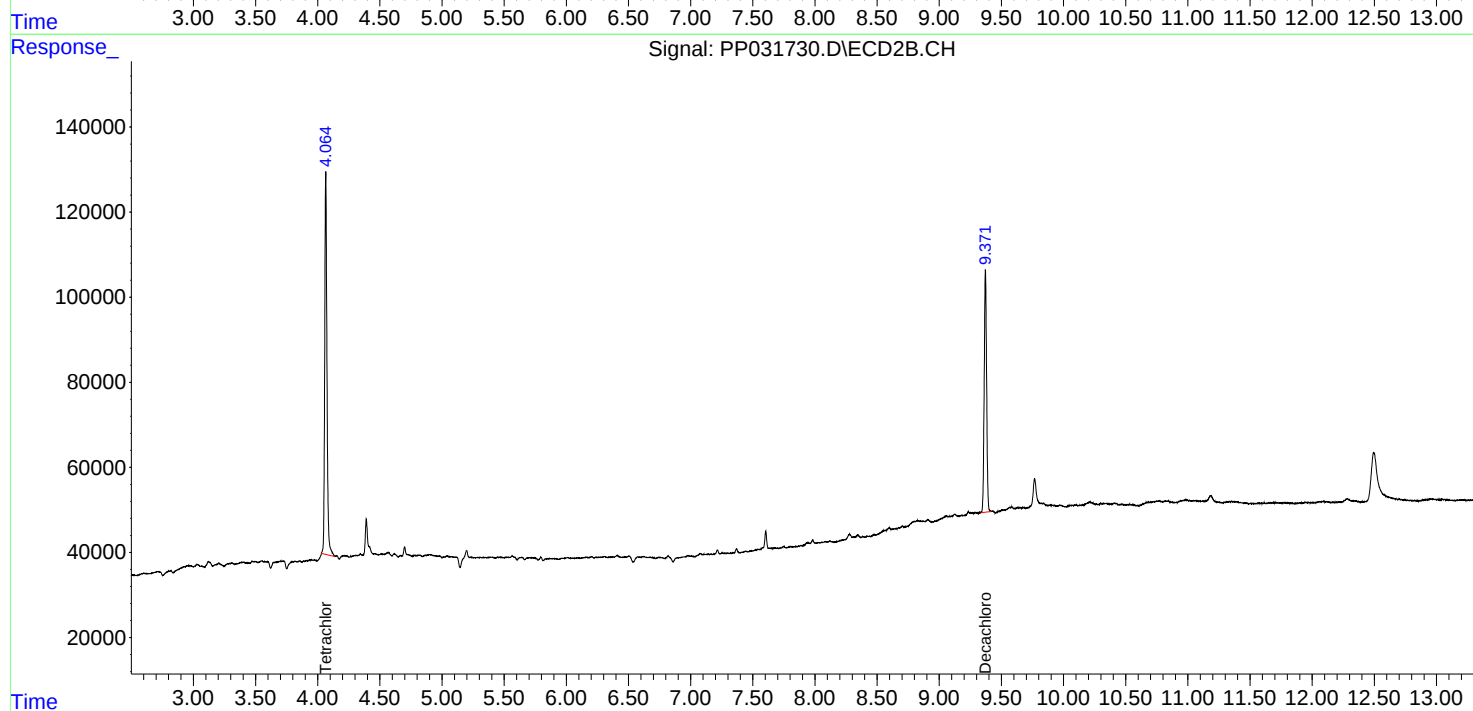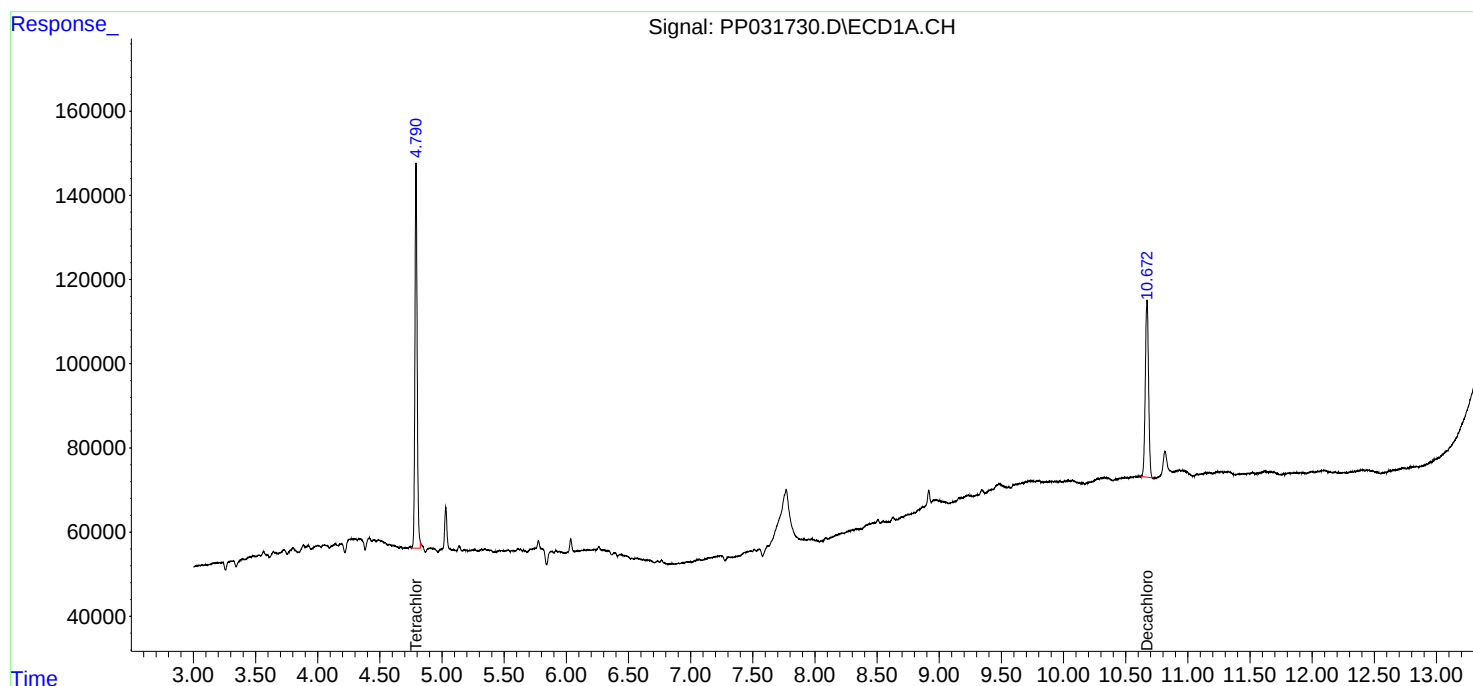

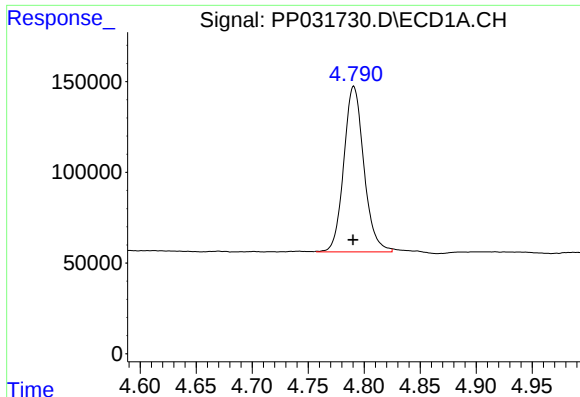


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 1138115
Conc: 23.50 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PAV-B2-112520-10-12.75


Manual Integrations
APPROVED

Ankita
12/1/2020 12:07:09 PM

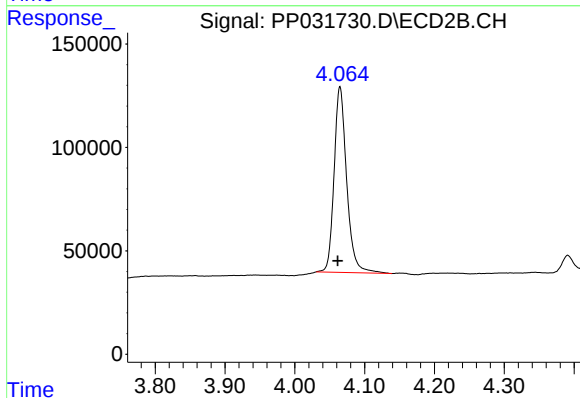


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.003 min
Response: 1128574
Conc: 23.55 ng/ml

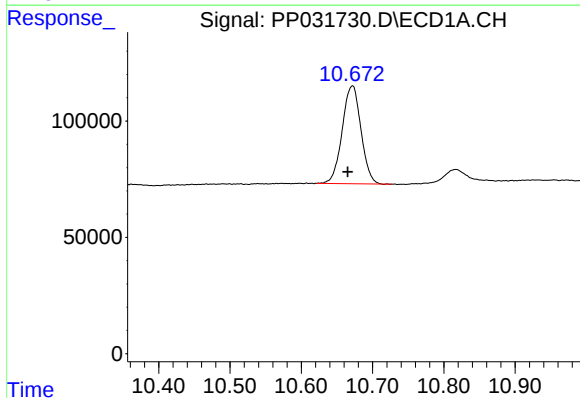

#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: 0.006 min
Response: 769652
Conc: 22.66 ng/ml

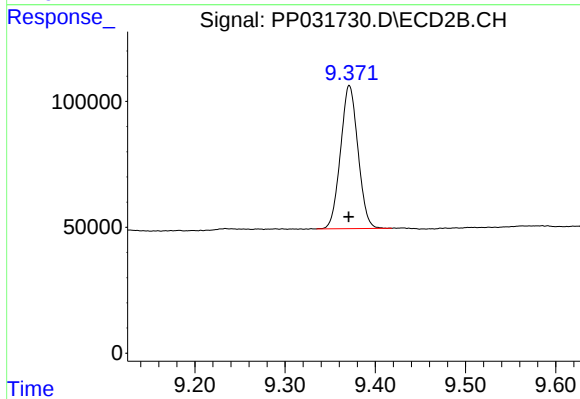

#2 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: 0.000 min
Response: 764500
Conc: 20.65 ng/ml